

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081320\
 Data File : PL060685.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2020 12:01
 Operator : DD\AJ
 Sample : L3504-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 13:40:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 11 01:39:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	4.011	27174002	33510469	14.495	12.602
28)	SA Decachlor...	8.219	9.098	20345774	22624901	11.147	12.059
Target Compounds							
8)	B Heptachlo...	0.000	5.885	0	8624736	N.D.	3.380 #
9)	A Endosulfan I	0.000	6.244	0	1903009	N.D.	0.672 #
10)	B gamma-Chl...	0.000	6.125	0	11279249	N.D.	3.731 #
11)	B alpha-Chl...	0.000	6.199	0	18867246	N.D.	6.137 #
12)	B 4,4'-DDE	0.000	6.350	0	5469927	N.D.	1.922 #
23)	Chlordane-1	4.332	5.008	898126	2995366	16.507	28.495 #
25)	Chlordane-3	0.000	6.125	0	11279249	N.D.	31.149 #
26)	Chlordane-4	0.000	6.199	0	18867246	N.D.	43.523 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081320\
Data File : PL060685.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2020 12:01
Operator : DD\AJ
Sample : L3504-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 13:40:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
Quant Title : GC Extractables
QLast Update : Tue Aug 11 01:39:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

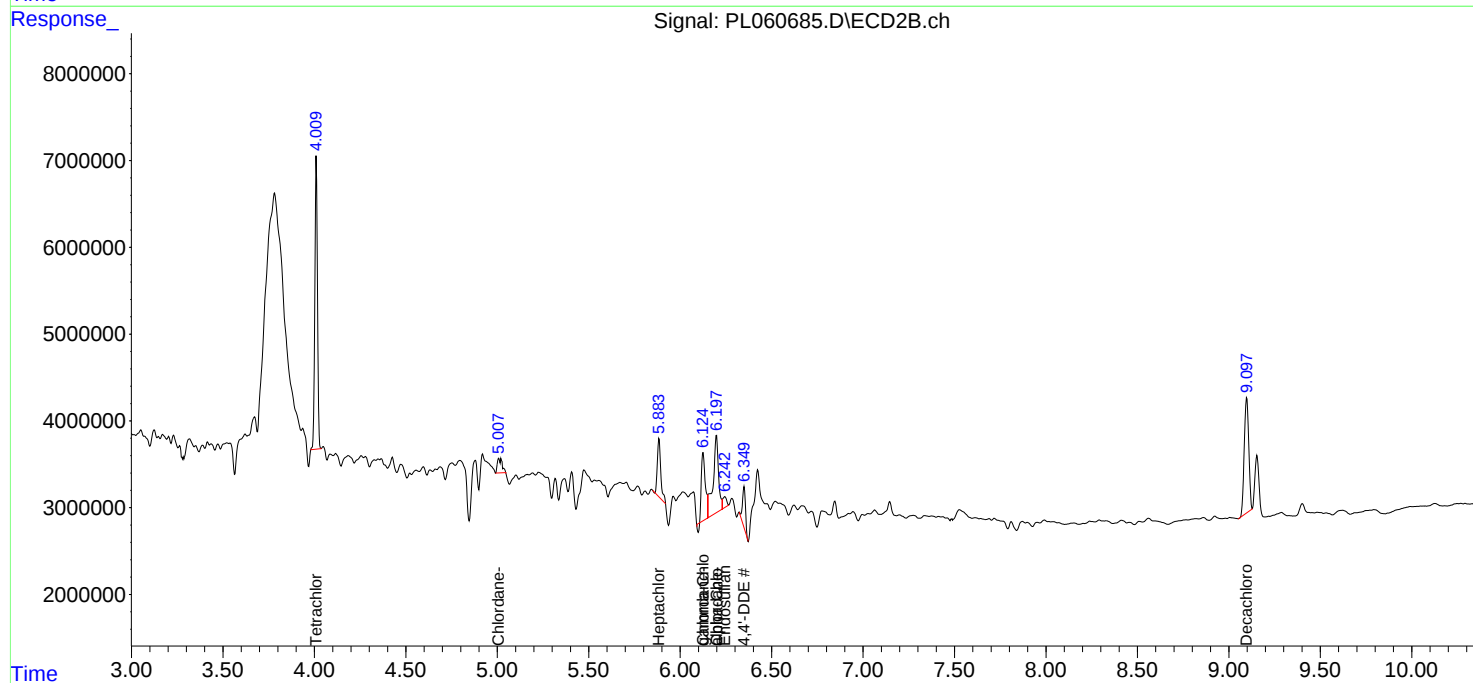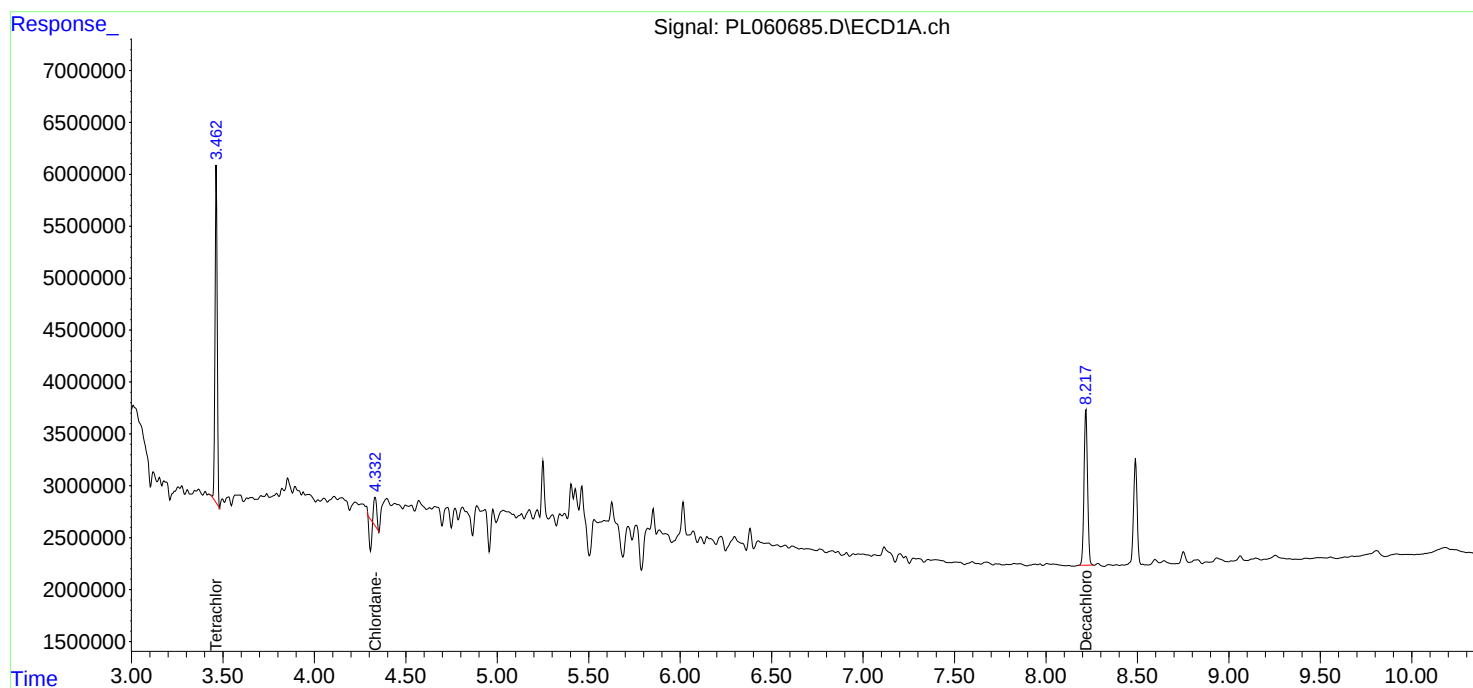


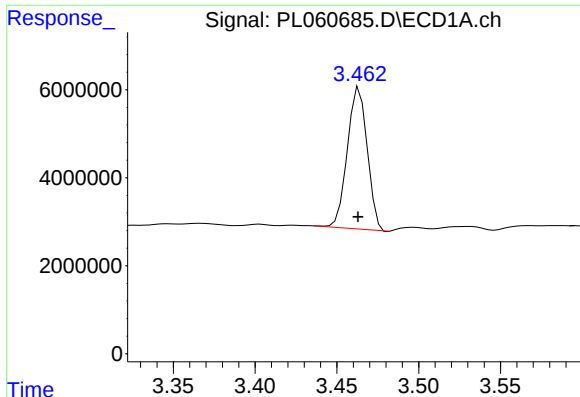

#1 Tetrachloro-m-xylene


R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 27174002
Conc: 14.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

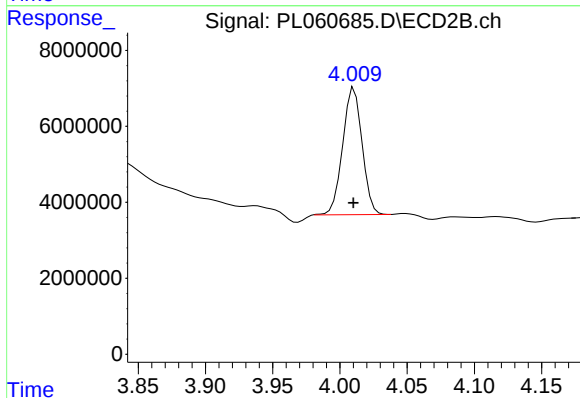


#1 Tetrachloro-m-xylene

R.T.: 4.011 min
Delta R.T.: 0.000 min
Response: 33510469
Conc: 12.60 ng/ml

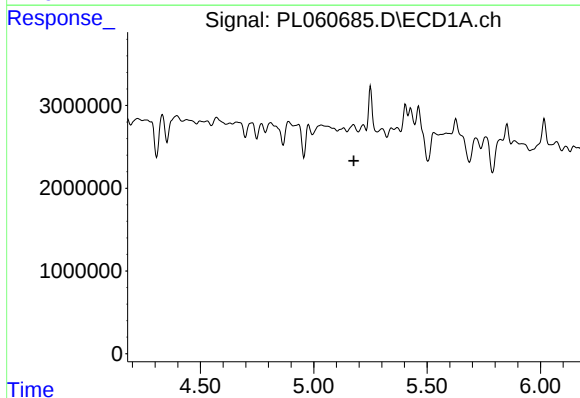


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.177 min
Response: 0
Conc: N.D.

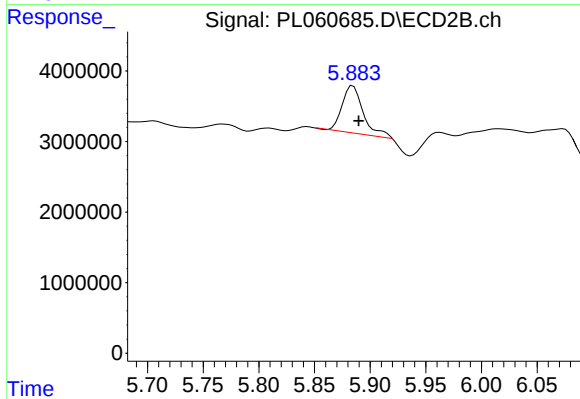

#8 Heptachlor epoxide


R.T.: 5.885 min
Delta R.T.: -0.005 min
Response: 8624736
Conc: 3.38 ng/ml

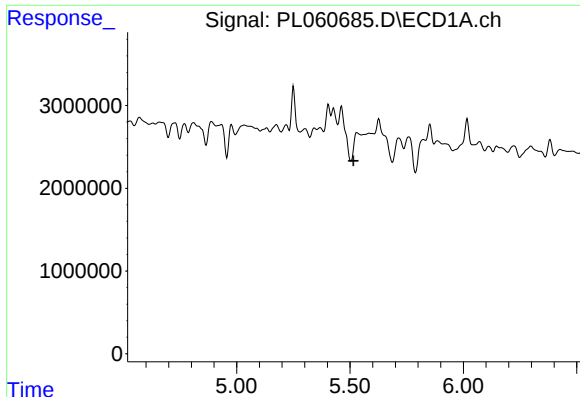

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.516 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

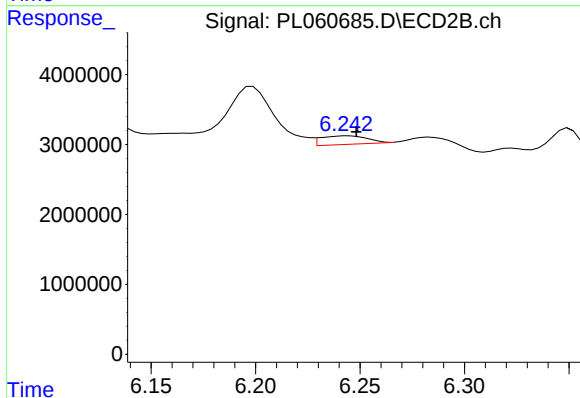


#9 Endosulfan I

R.T.: 6.244 min
Delta R.T.: -0.004 min
Response: 1903009
Conc: 0.67 ng/ml

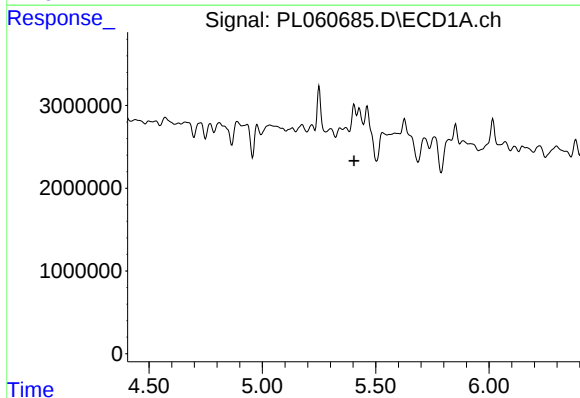


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.405 min
Response: 0
Conc: N.D.

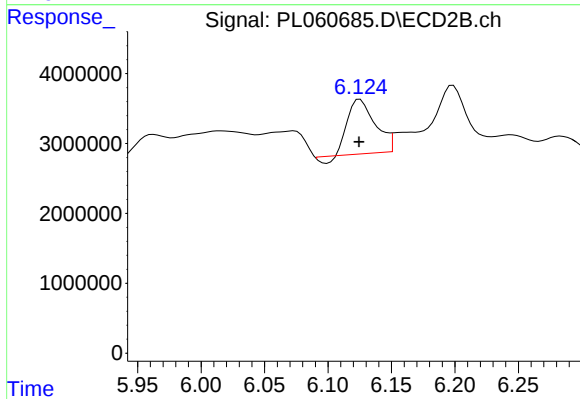

#10 gamma-Chlordane


R.T.: 6.125 min
Delta R.T.: 0.000 min
Response: 11279249
Conc: 3.73 ng/ml

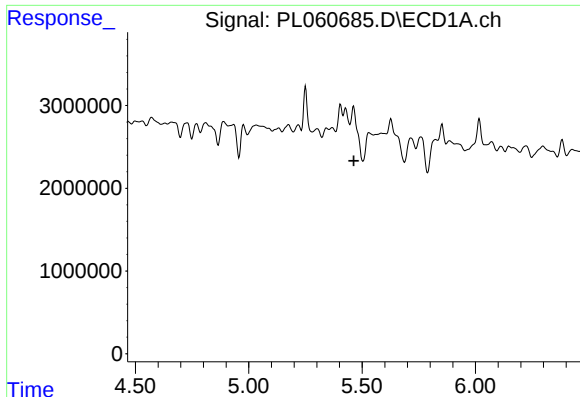

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.463 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

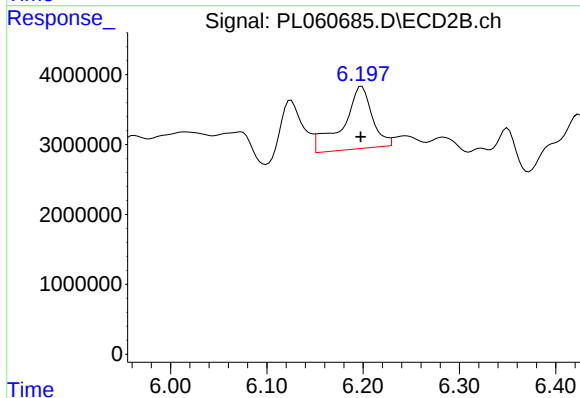


#11 alpha-Chlordane

R.T.: 6.199 min
Delta R.T.: 0.001 min
Response: 18867246
Conc: 6.14 ng/ml

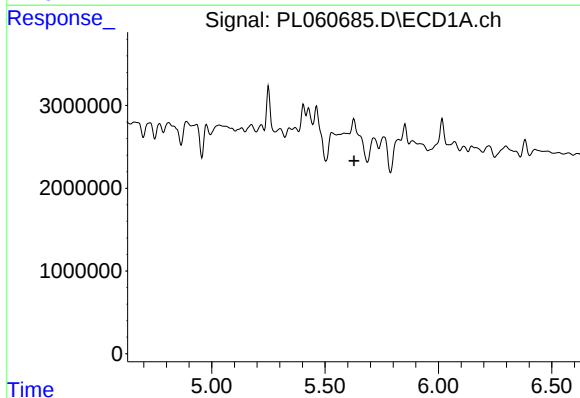


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.628 min
Response: 0
Conc: N.D.

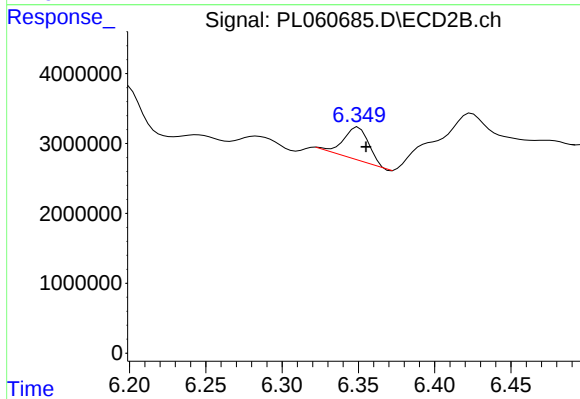

#12 4,4'-DDE


R.T.: 6.350 min
Delta R.T.: -0.005 min
Response: 5469927
Conc: 1.92 ng/ml

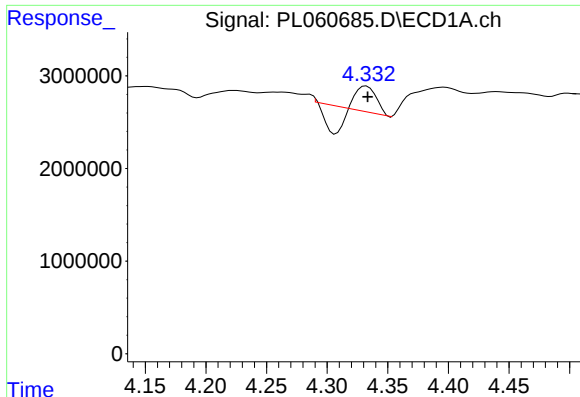

#23 Chlordane-1


R.T.: 4.332 min
Delta R.T.: -0.001 min
Response: 898126
Conc: 16.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

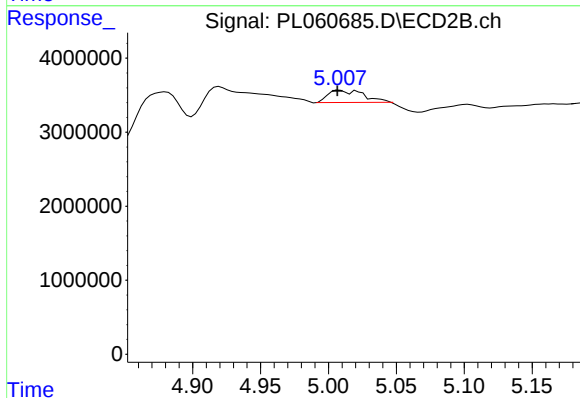


#23 Chlordane-1

R.T.: 5.008 min
Delta R.T.: 0.001 min
Response: 2995366
Conc: 28.50 ng/ml

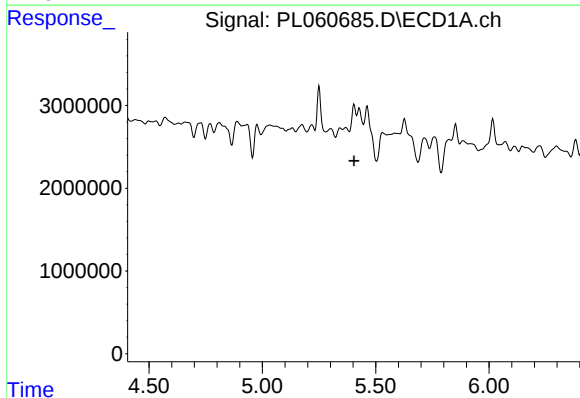


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.404 min
Response: 0
Conc: N.D.

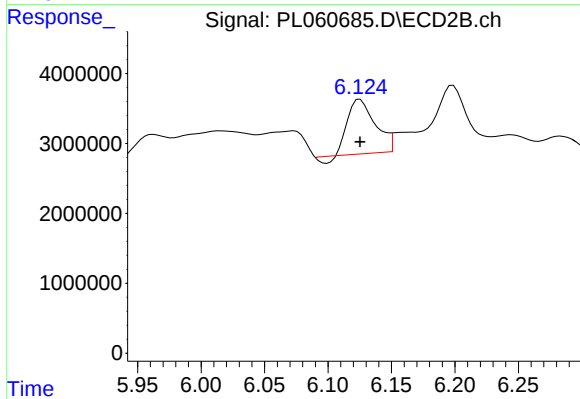

#25 Chlordane-3


R.T.: 6.125 min
Delta R.T.: 0.000 min
Response: 11279249
Conc: 31.15 ng/ml

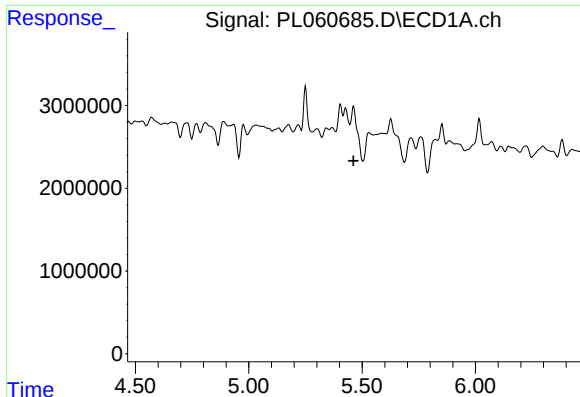

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.463 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

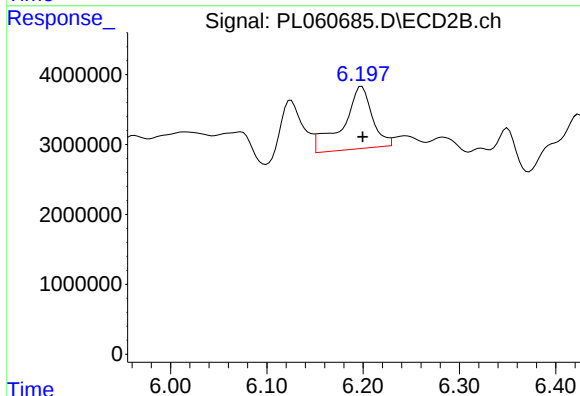


#26 Chlordane-4

R.T.: 6.199 min
Delta R.T.: -0.001 min
Response: 18867246
Conc: 43.52 ng/ml

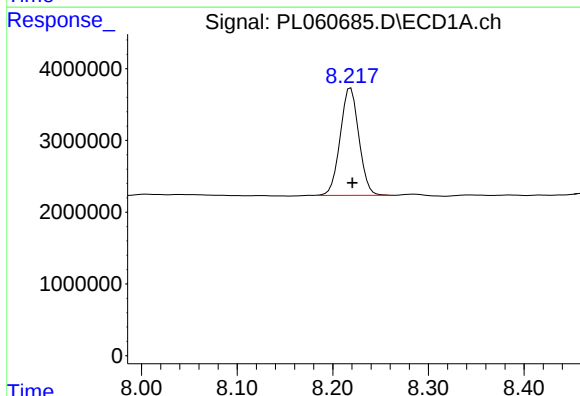

#28 Decachlorobiphenyl

R.T.: 8.219 min
Delta R.T.: -0.002 min
Response: 20345774
Conc: 11.15 ng/ml

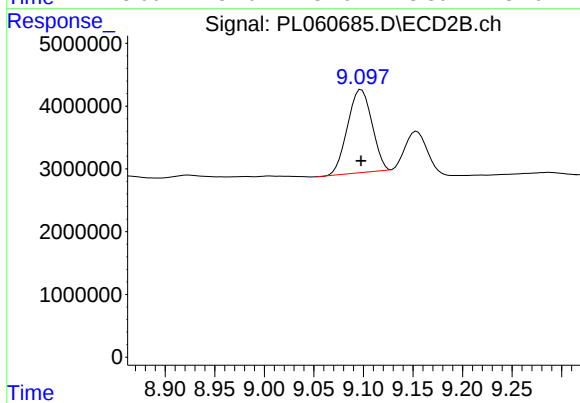

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: 0.000 min
Response: 22624901
Conc: 12.06 ng/ml