

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081320\
 Data File : PL060700.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2020 16:07
 Operator : DD\AJ
 Sample : L3501-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 01:58:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 11 01:39:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.462	4.010	24200377	29922715	12.909	11.253
28)	SA Decachlor...	8.219	9.097	17580408	20929403	9.632	11.155
Target Compounds							
6)	B beta-BHC	0.000	4.869	0	3108956	N.D.	1.941 #
8)	B Heptachlo...	0.000	5.881	0	3103313	N.D.	1.216 #
10)	B gamma-Chl...	0.000	6.126	0	852378	N.D.	0.282 #
11)	B alpha-Chl...	0.000	6.198	0	4559821	N.D.	1.483 #
12)	B 4,4'-DDE	0.000	6.351	0	5817387	N.D.	2.044 #
13)	MA Dieldrin	5.752	6.504	10724912	4579432	5.187	1.571 #
16)	A 4,4'-DDD	0.000	6.851	0	7676474	N.D.	3.345 #
17)	MA 4,4'-DDT	6.379	7.119f	9501989	13268208	5.748	6.070
23)	Chlordane-1	0.000	5.008	0	3078632	N.D.	29.287 #
25)	Chlordane-3	0.000	6.126	0	852378	N.D.	2.354 #
26)	Chlordane-4	0.000	6.198	0	4559821	N.D.	10.519 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081320\
Data File : PL060700.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2020 16:07
Operator : DD\AJ
Sample : L3501-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 01:58:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
Quant Title : GC Extractables
QLast Update : Tue Aug 11 01:39:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

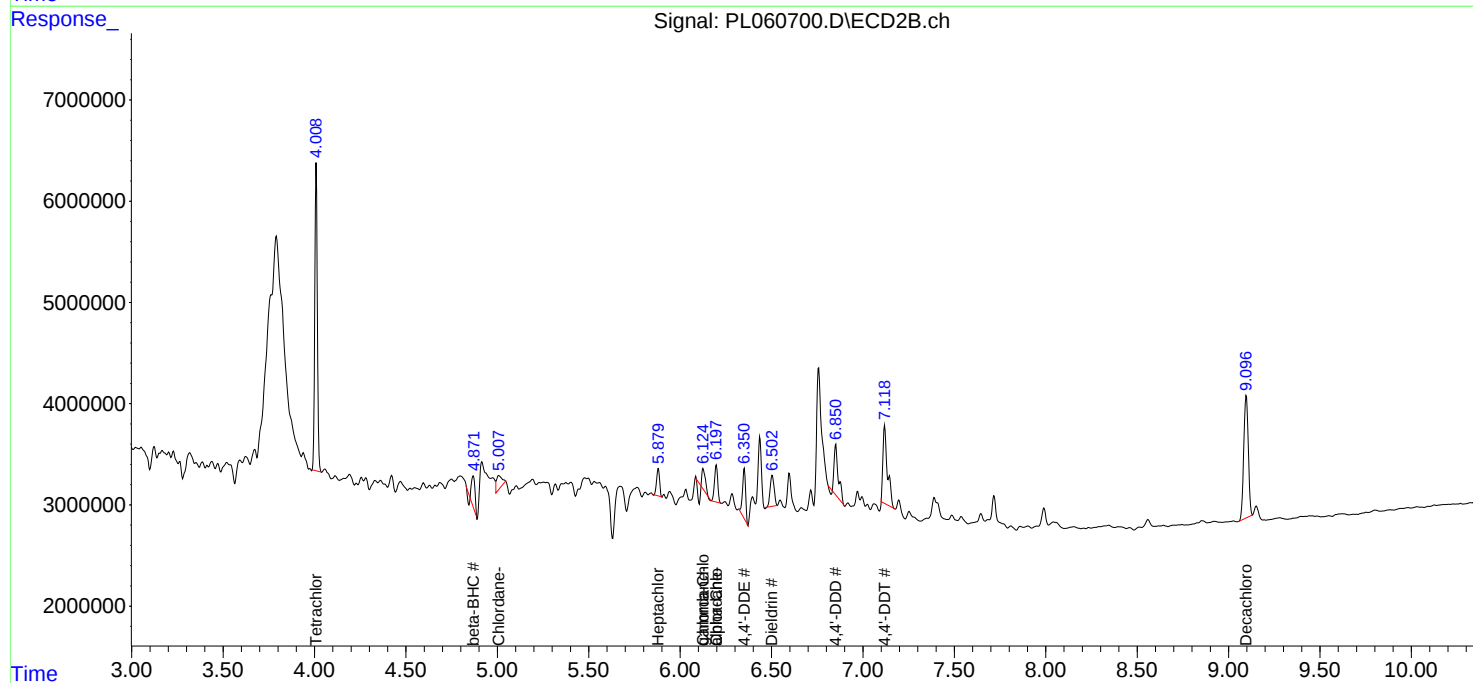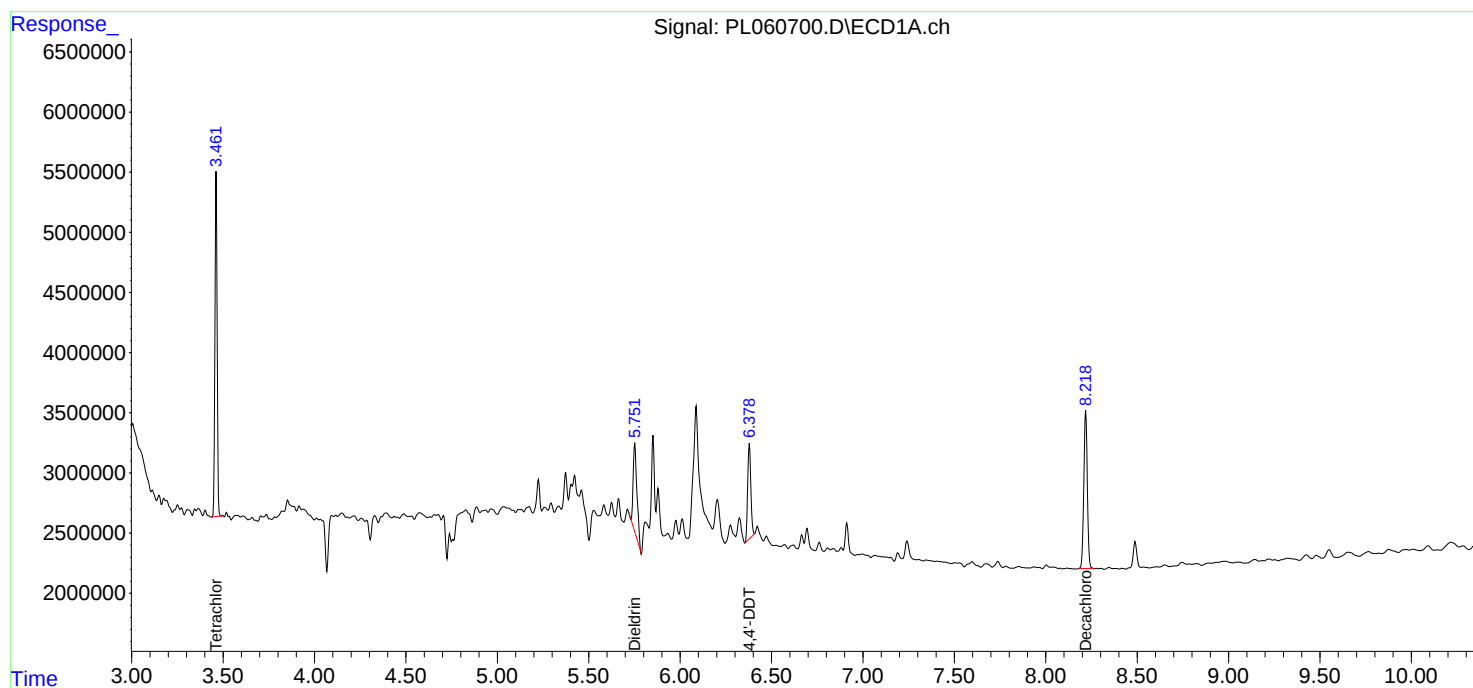


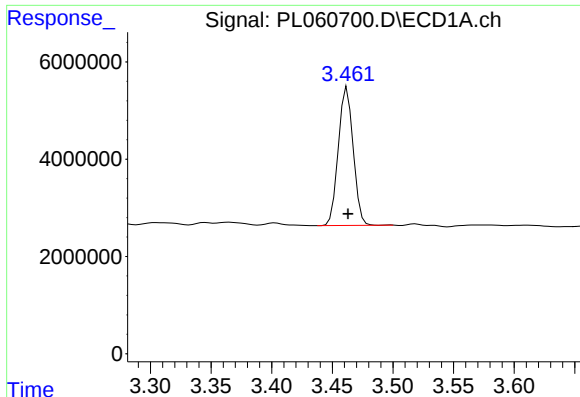

#1 Tetrachloro-m-xylene


R.T.: 3.462 min
Delta R.T.: 0.000 min
Response: 24200377
Conc: 12.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

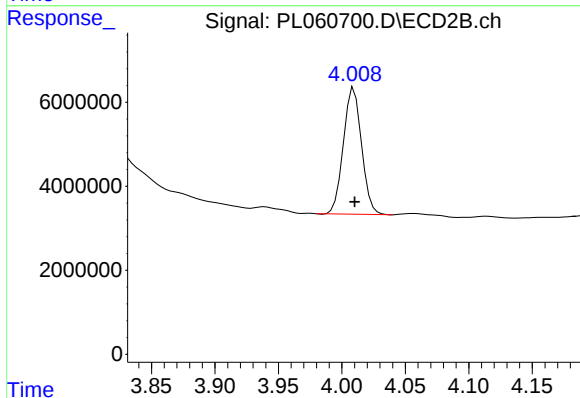


#1 Tetrachloro-m-xylene

R.T.: 4.010 min
Delta R.T.: 0.000 min
Response: 29922715
Conc: 11.25 ng/ml

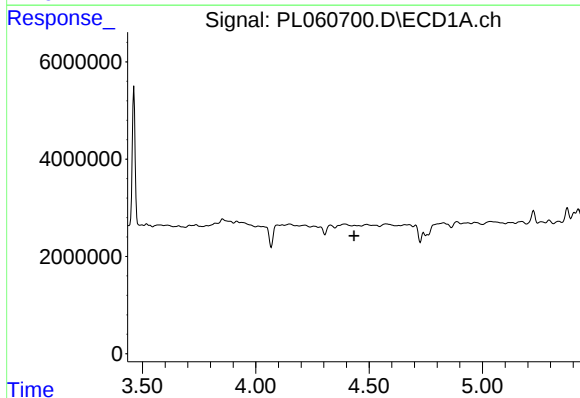


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.434 min
Response: 0
Conc: N.D.

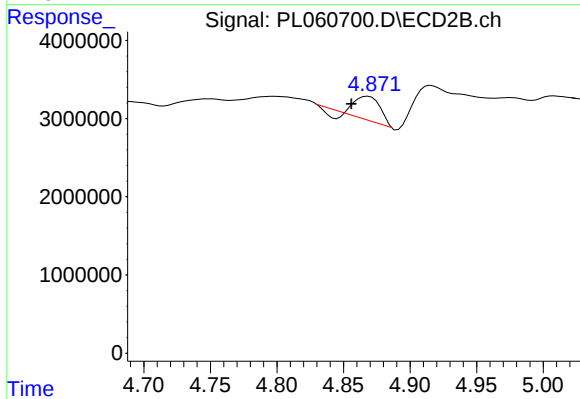

#6 beta-BHC


R.T.: 4.869 min
Delta R.T.: 0.013 min
Response: 3108956
Conc: 1.94 ng/ml

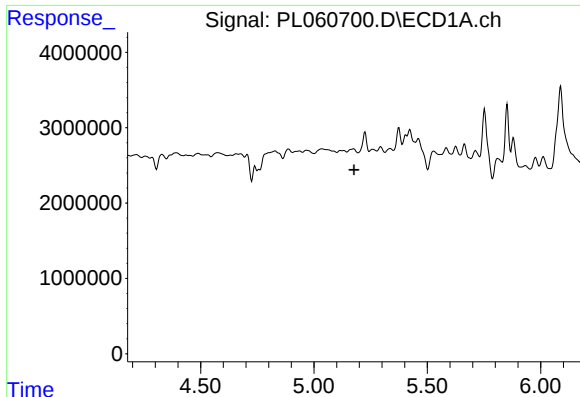

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.177 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

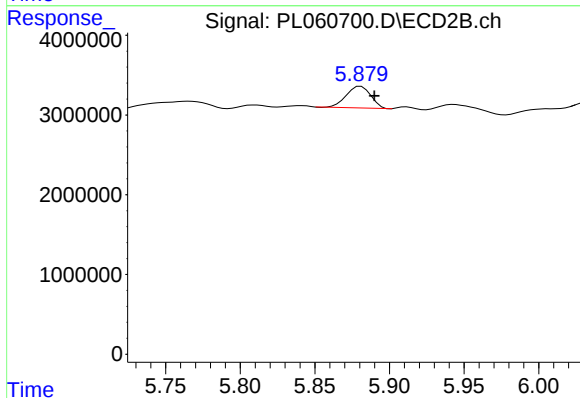


#8 Heptachlor epoxide

R.T.: 5.881 min
Delta R.T.: -0.009 min
Response: 3103313
Conc: 1.22 ng/ml

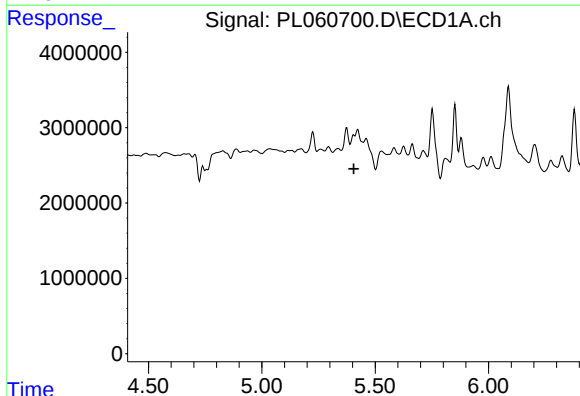


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.405 min
Response: 0
Conc: N.D.

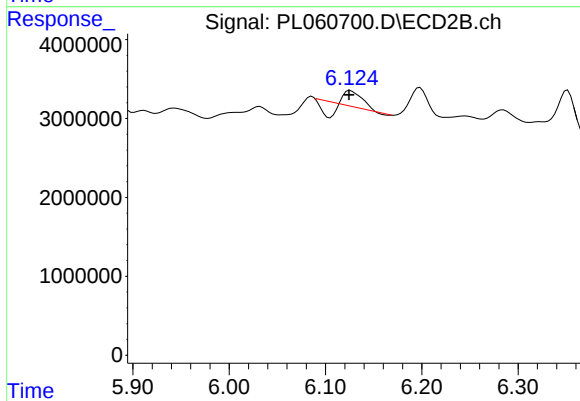

#10 gamma-Chlordane


R.T.: 6.126 min
Delta R.T.: 0.002 min
Response: 852378
Conc: 0.28 ng/ml

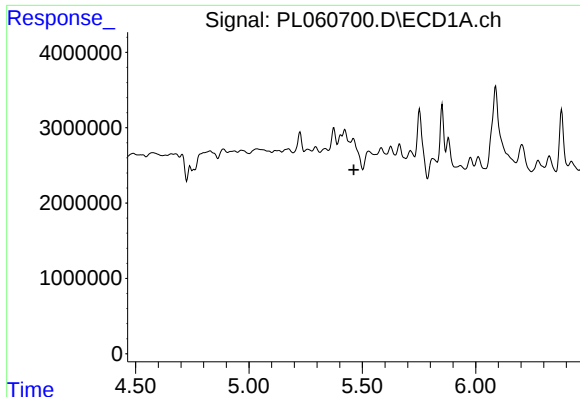

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.463 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

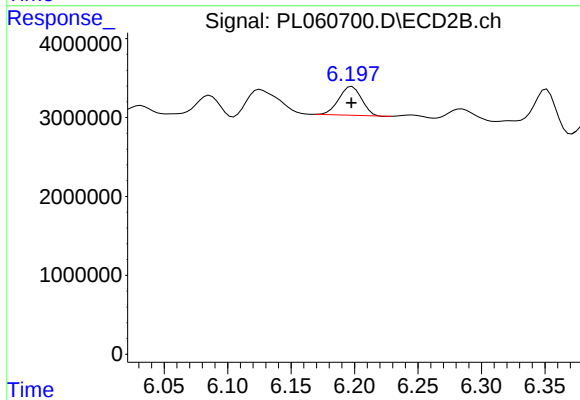


#11 alpha-Chlordane

R.T.: 6.198 min
Delta R.T.: 0.000 min
Response: 4559821
Conc: 1.48 ng/ml

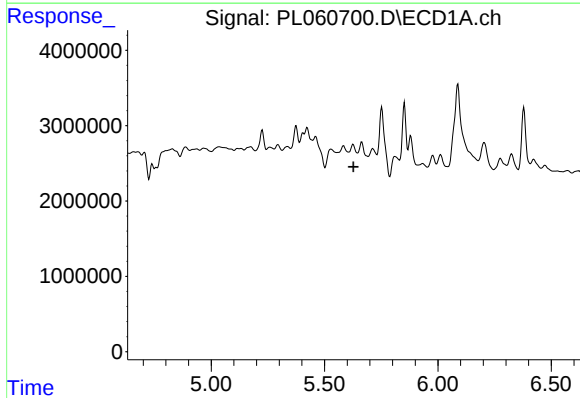


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.628 min
Response: 0
Conc: N.D.

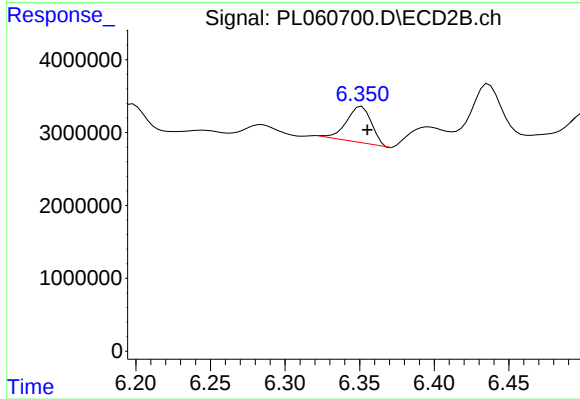

#12 4,4'-DDE


R.T.: 6.351 min
Delta R.T.: -0.004 min
Response: 5817387
Conc: 2.04 ng/ml

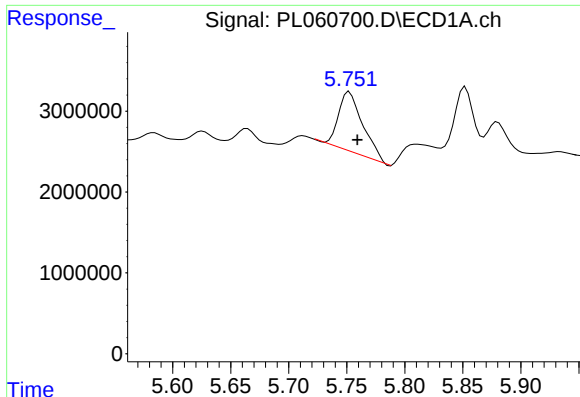

#13 Dieldrin


R.T.: 5.752 min
Delta R.T.: -0.007 min
Response: 10724912
Conc: 5.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

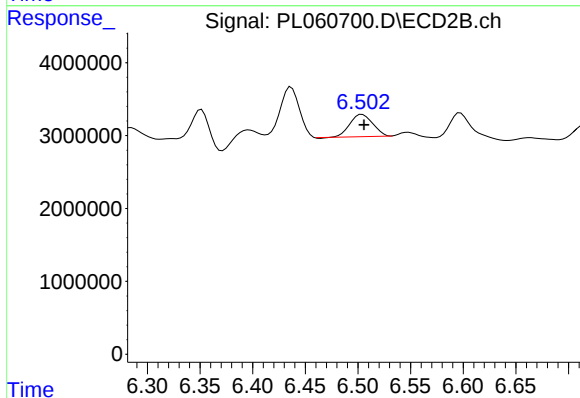


#13 Dieldrin

R.T.: 6.504 min
Delta R.T.: -0.002 min
Response: 4579432
Conc: 1.57 ng/ml

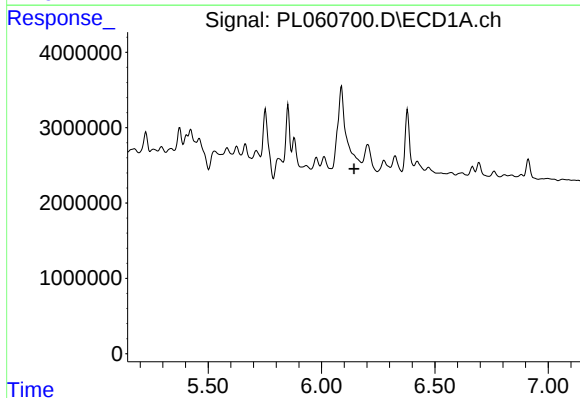


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.144 min
Response: 0
Conc: N.D.

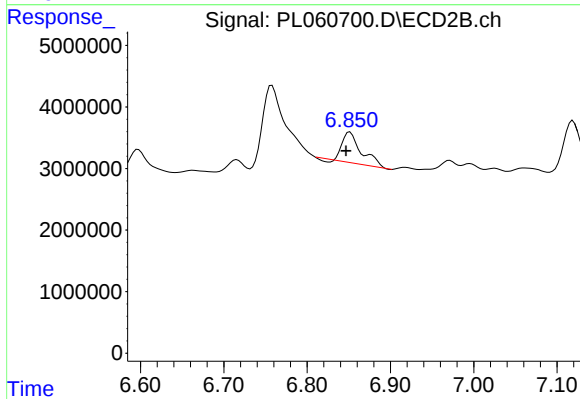

#16 4,4'-DDD


R.T.: 6.851 min
Delta R.T.: 0.005 min
Response: 7676474
Conc: 3.35 ng/ml

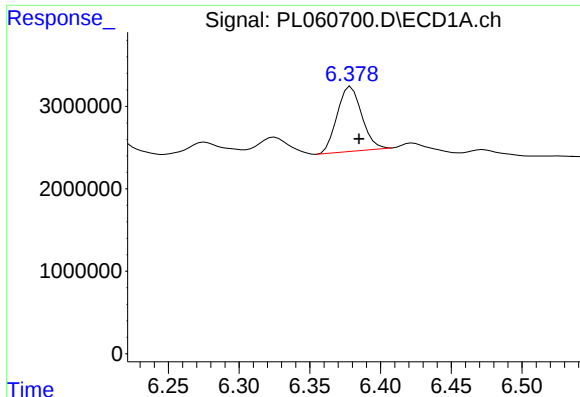

#17 4,4'-DDT


R.T.: 6.379 min
Delta R.T.: -0.006 min
Response: 9501989
Conc: 5.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

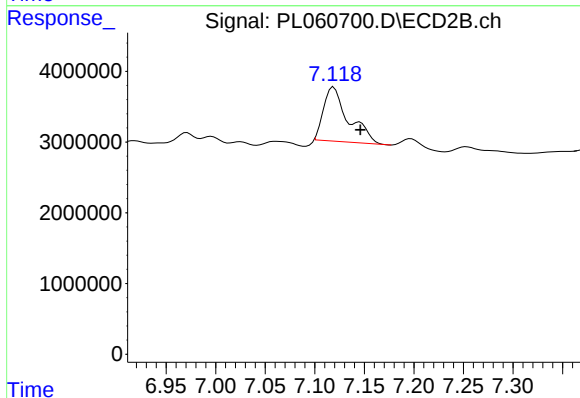


#17 4,4'-DDT

R.T.: 7.119 min
Delta R.T.: -0.027 min
Response: 13268208
Conc: 6.07 ng/ml

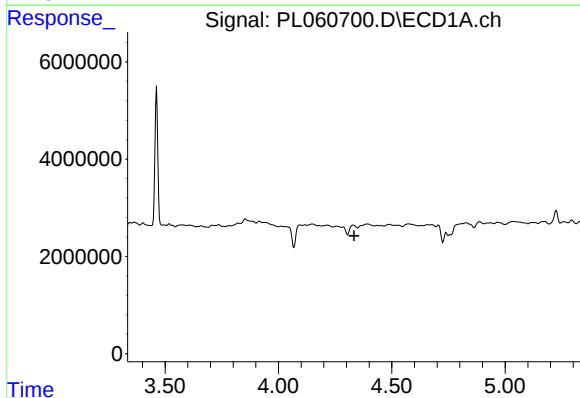


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.333 min
Response: 0
Conc: N.D.

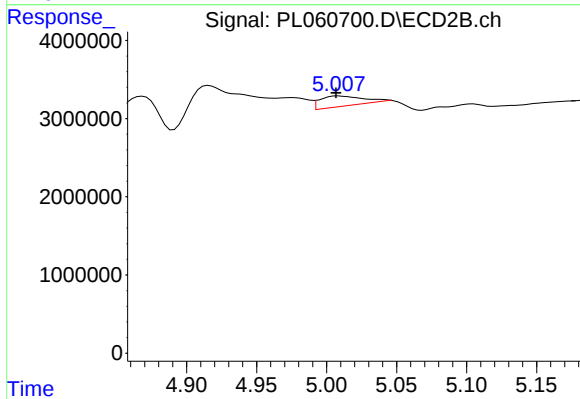

#23 Chlordane-1


R.T.: 5.008 min
Delta R.T.: 0.001 min
Response: 3078632
Conc: 29.29 ng/ml

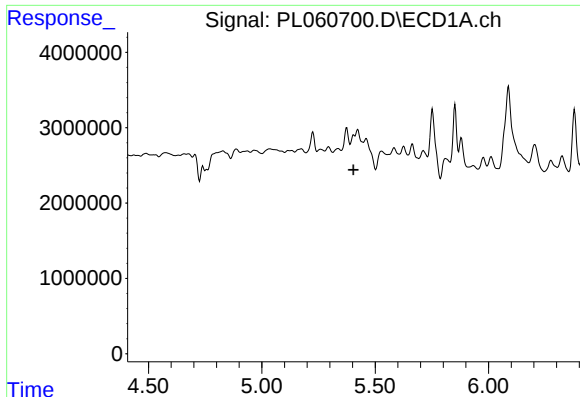

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.404 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

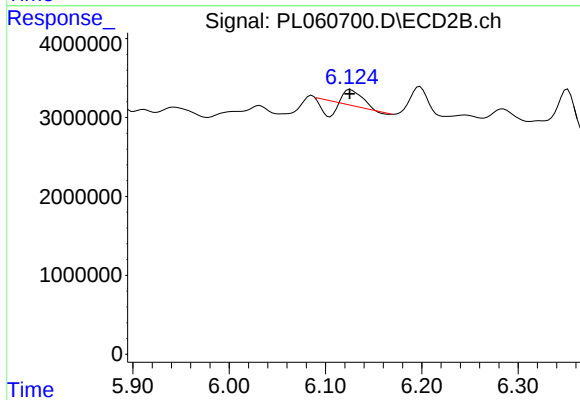


#25 Chlordane-3

R.T.: 6.126 min
Delta R.T.: 0.001 min
Response: 852378
Conc: 2.35 ng/ml

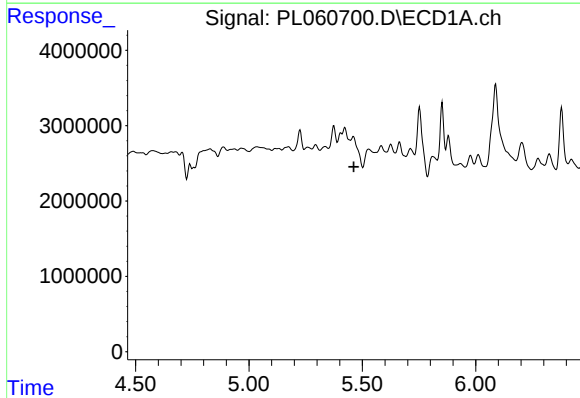


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.463 min
Response: 0
Conc: N.D.

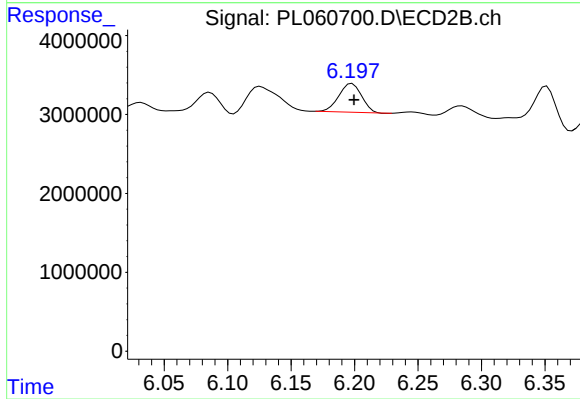

#26 Chlordane-4


R.T.: 6.198 min
Delta R.T.: -0.002 min
Response: 4559821
Conc: 10.52 ng/ml

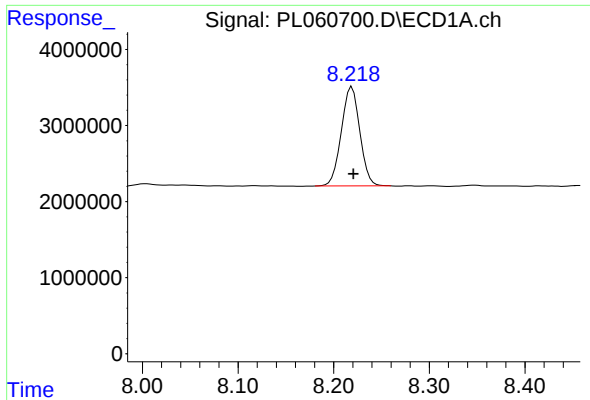

#28 Decachlorobiphenyl

R.T.: 8.219 min
Delta R.T.: -0.001 min
Response: 17580408
Conc: 9.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

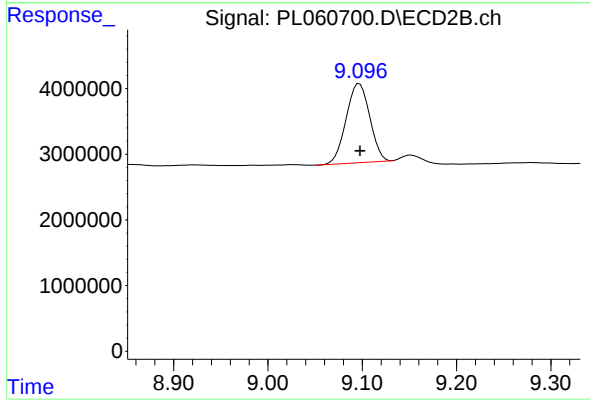

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: 0.000 min
Response: 20929403
Conc: 11.16 ng/ml