

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081321\
 Data File : PL068971.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2021 18:49
 Operator : AR\AJ
 Sample : M3394-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SWCS-01-1015

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 05:49:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.636	5.567	9768667	27611396	23.616	27.194
28)	SA Decachlor...	10.405	11.487	13798011	24233807	24.009	24.977
Target Compounds							
9)	A Endosulfan I	0.000	8.459f	0	328642	N.D.	0.312 #
14)	MA Endrin	0.000	8.966	0	162003	N.D.	0.178 #
15)	B Endosulfa...	0.000	9.216	0	1834204	N.D.	2.000 #
22)	Mirex	0.000	10.537	0	69220	N.D.	0.088 #
23)	Chlordane-1	0.000	6.975f	0	602411	N.D.	14.286 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081321\
Data File : PL068971.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2021 18:49
Operator : AR\AJ
Sample : M3394-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SWCS-01-1015

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 05:49:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

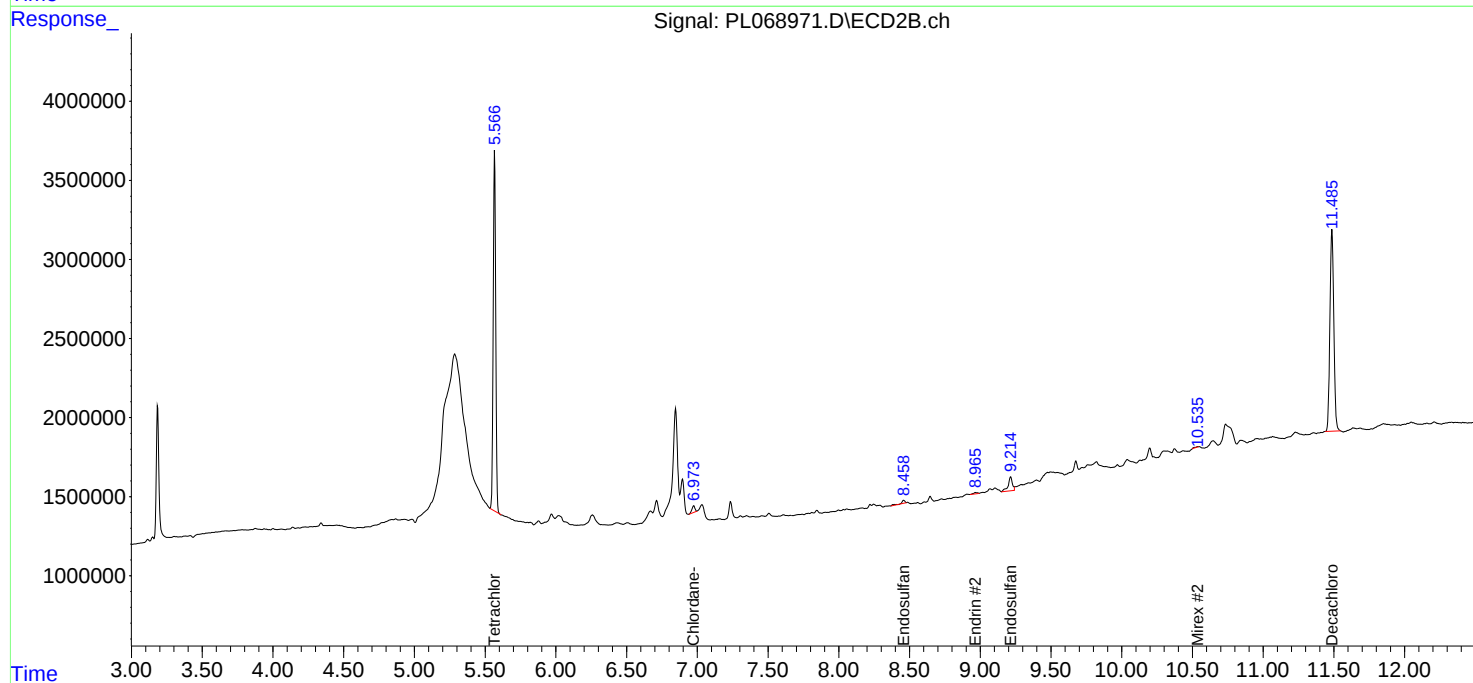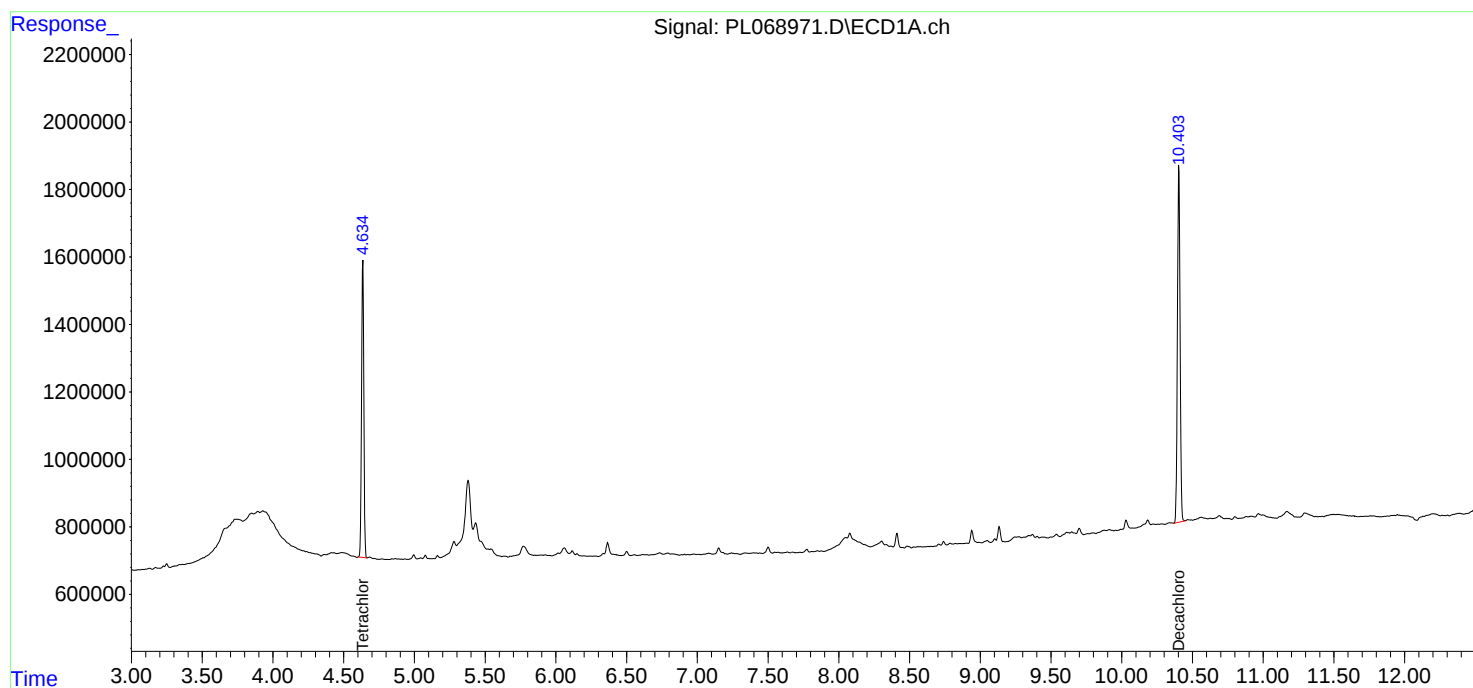


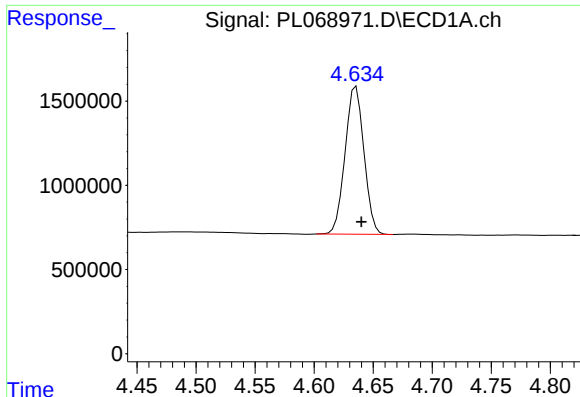

#1 Tetrachloro-m-xylene


R.T.: 4.636 min
Delta R.T.: -0.004 min
Response: 9768667
Conc: 23.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
SWCS-01-1015

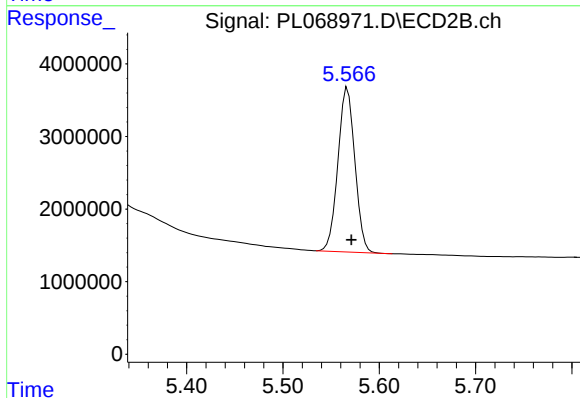


#1 Tetrachloro-m-xylene

R.T.: 5.567 min
Delta R.T.: -0.004 min
Response: 27611396
Conc: 27.19 ng/ml

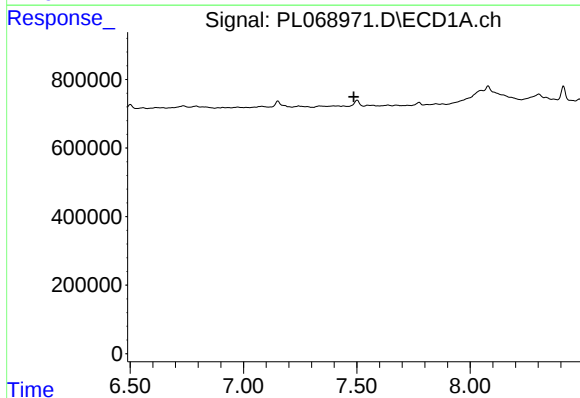


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.487 min
Response: 0
Conc: N.D.

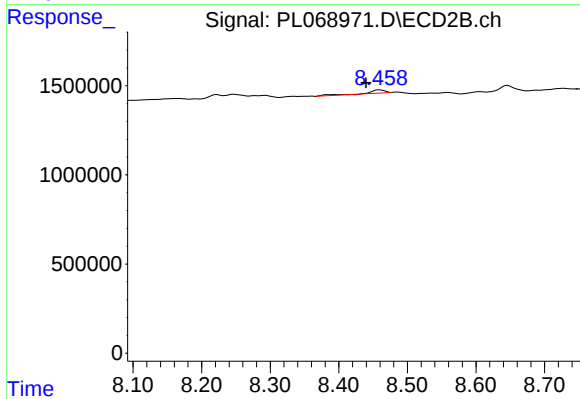

#9 Endosulfan I


R.T.: 8.459 min
Delta R.T.: 0.019 min
Response: 328642
Conc: 0.31 ng/ml

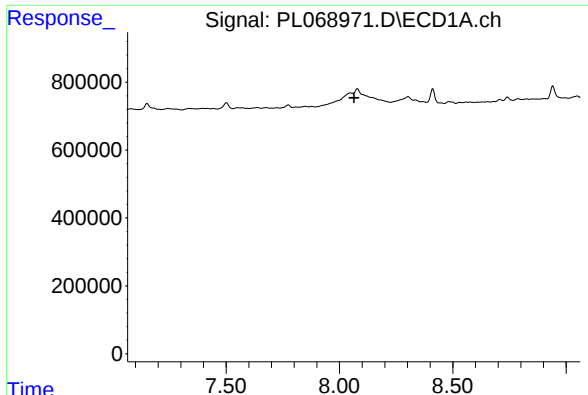

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SWCS-01-1015

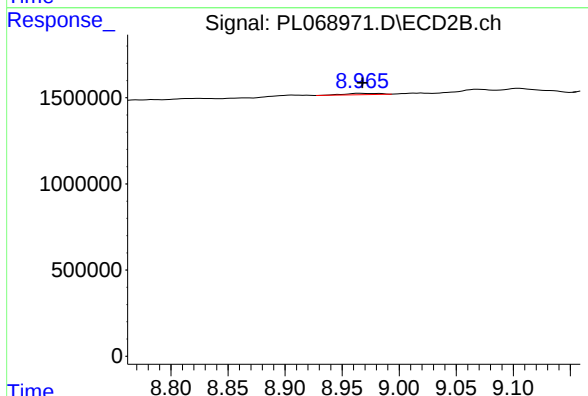


#14 Endrin

R.T.: 8.966 min
Delta R.T.: -0.001 min
Response: 162003
Conc: 0.18 ng/ml

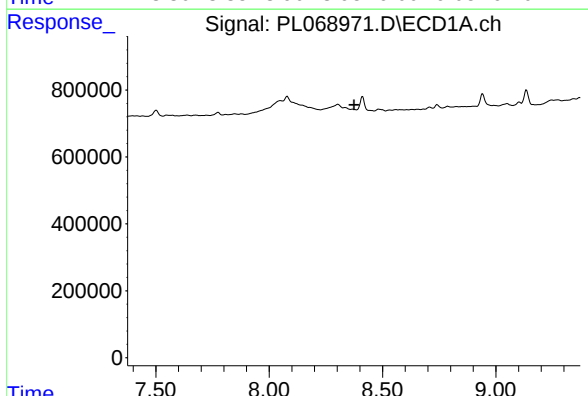


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

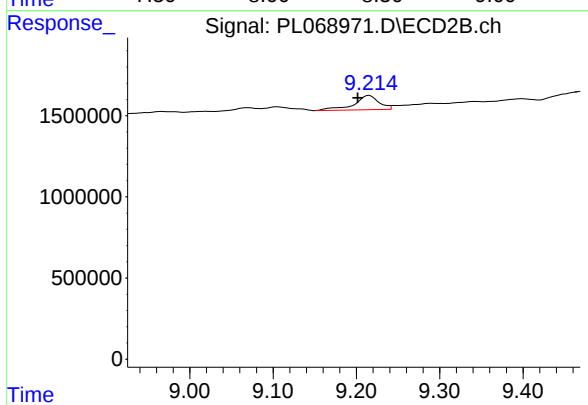

#15 Endosulfan II


R.T.: 9.216 min
Delta R.T.: 0.014 min
Response: 1834204
Conc: 2.00 ng/ml

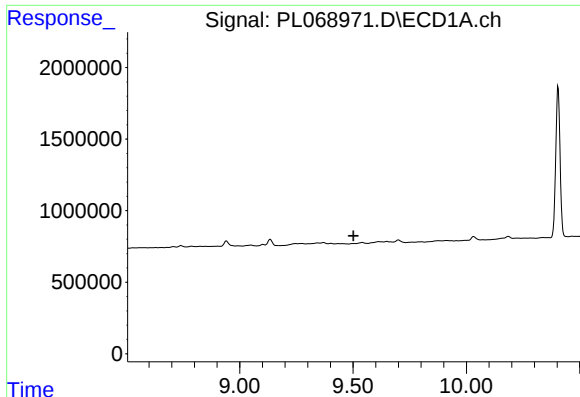

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.502 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SWCS-01-1015

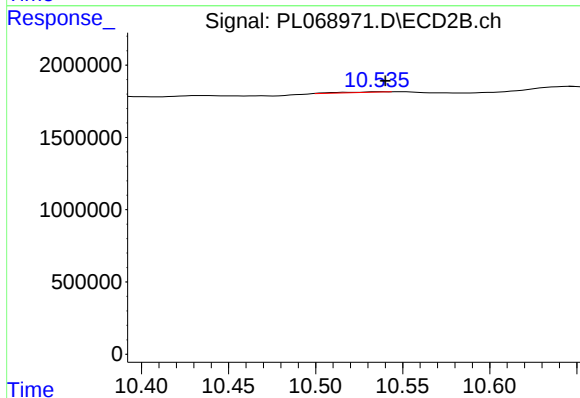


#22 Mirex

R.T.: 10.537 min
Delta R.T.: -0.003 min
Response: 69220
Conc: 0.09 ng/ml

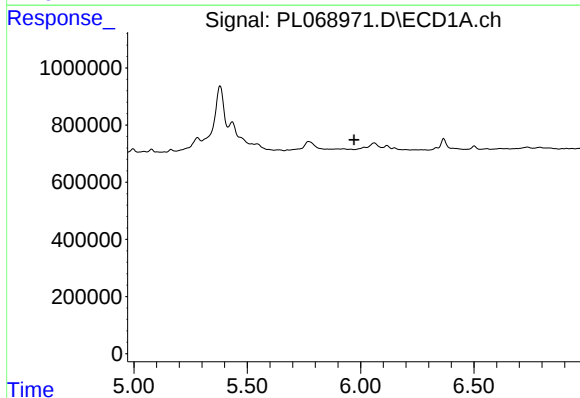


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.971 min
Response: 0
Conc: N.D.

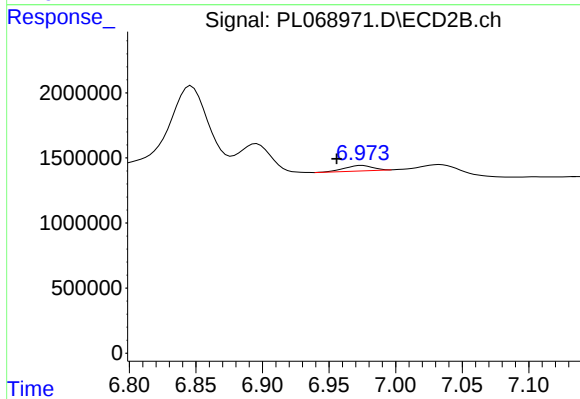

#23 Chlordane-1


R.T.: 6.975 min
Delta R.T.: 0.019 min
Response: 602411
Conc: 14.29 ng/ml

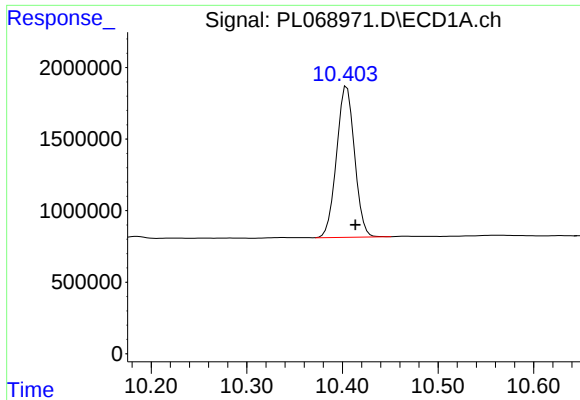

#28 Decachlorobiphenyl

R.T.: 10.405 min
Delta R.T.: -0.009 min
Response: 13798011
Conc: 24.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
SWCS-01-1015

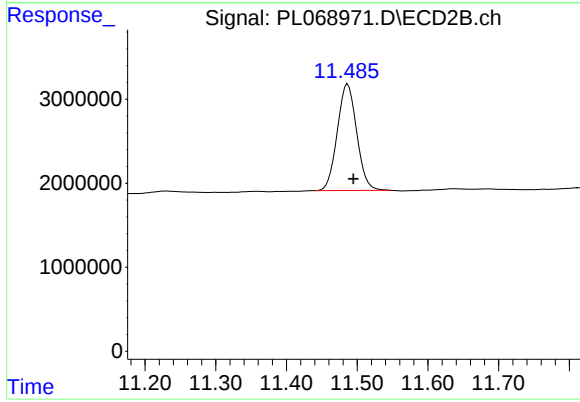

#28 Decachlorobiphenyl

R.T.: 11.487 min
Delta R.T.: -0.008 min
Response: 24233807
Conc: 24.98 ng/ml