

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081321\
 Data File : PL068988.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2021 01:29
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 05:53:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.636	5.568	9077509	25603414	21.945	25.217
28)	SA Decachlor...	10.404	11.488	12953661	22526933	22.540	23.218
Target Compounds							
4)	MA Heptachlor	6.152f	0.000	420981	0	0.717	N.D. #
6)	B beta-BHC	6.152	0.000	420981	0	1.493	N.D. #
8)	B Heptachlo...	0.000	8.036	0	460198	N.D.	0.398 #
14)	MA Endrin	8.079	0.000	464359	0	0.964	N.D. #
15)	B Endosulfa...	0.000	9.212	0	405904	N.D.	0.443 #
17)	MA 4,4'-DDT	0.000	9.445f	0	113239	N.D.	0.120 #
21)	B Endrin ke...	0.000	10.099f	0	143859	N.D.	0.141 #
22)	Mirex	0.000	10.565f	0	91672	N.D.	0.116 #
23)	Chlordane-1	0.000	6.975f	0	290282	N.D.	6.884 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081321\
Data File : PL068988.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2021 01:29
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 05:53:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

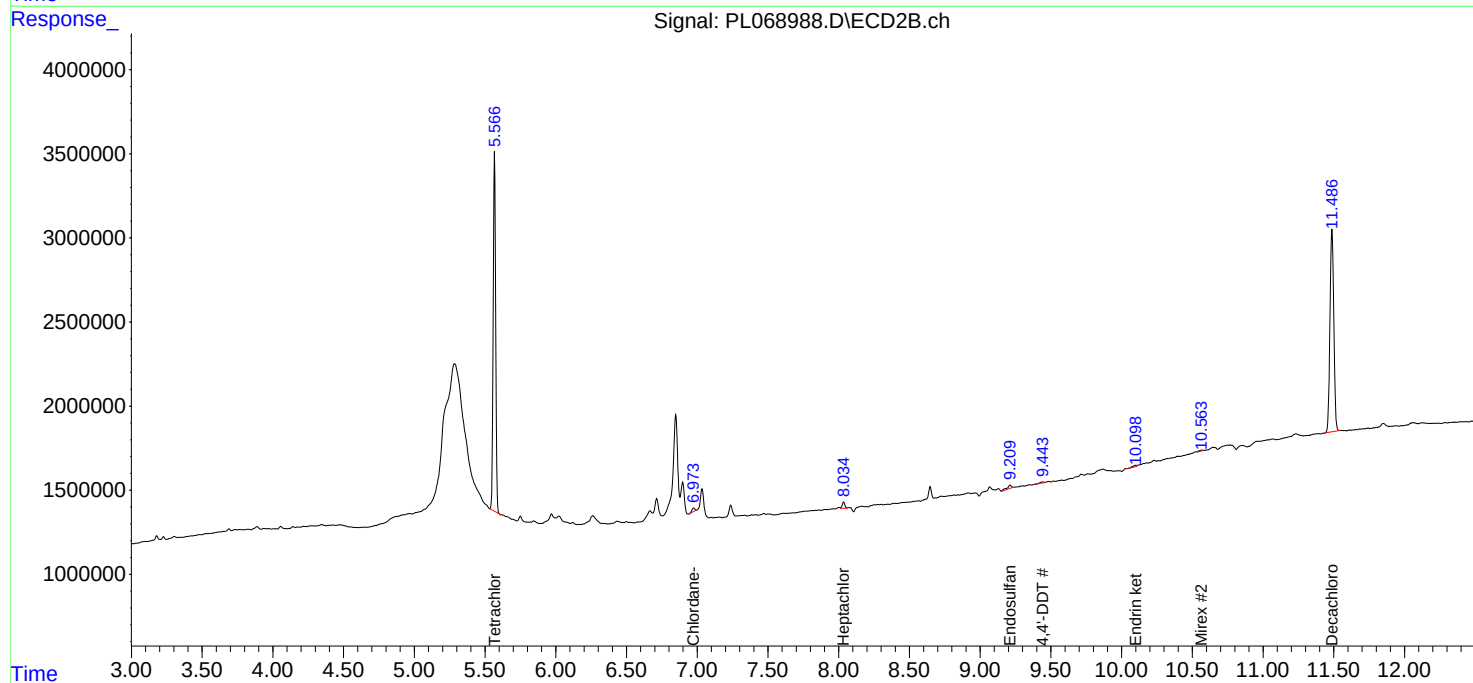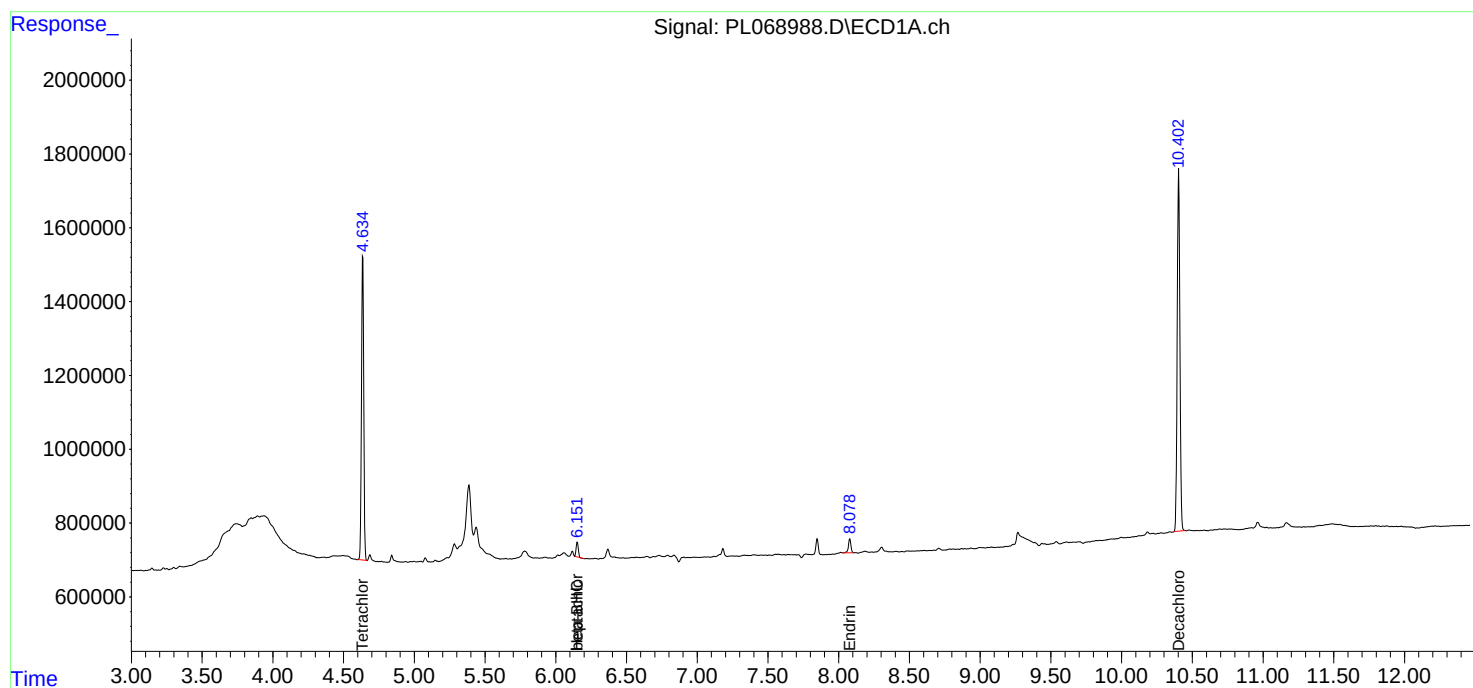


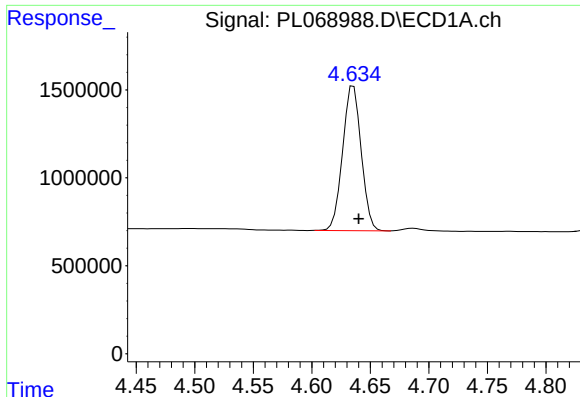

#1 Tetrachloro-m-xylene


R.T.: 4.636 min
Delta R.T.: -0.004 min
Response: 9077509
Conc: 21.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

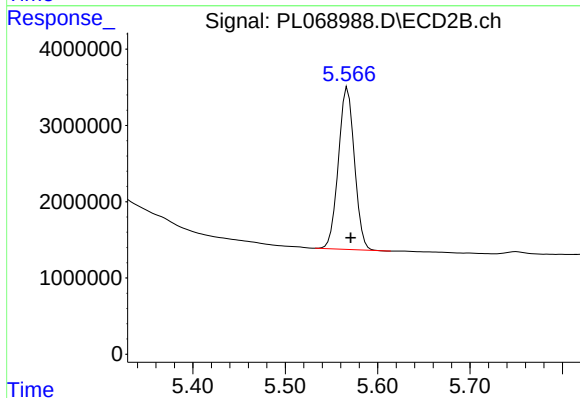


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 25603414
Conc: 25.22 ng/ml

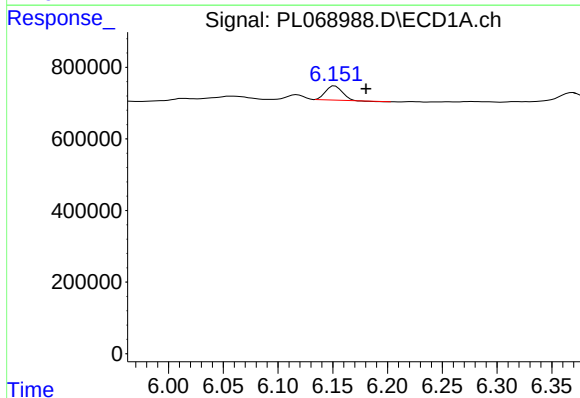


#4 Heptachlor

R.T.: 6.152 min
Delta R.T.: -0.028 min
Response: 420981
Conc: 0.72 ng/ml

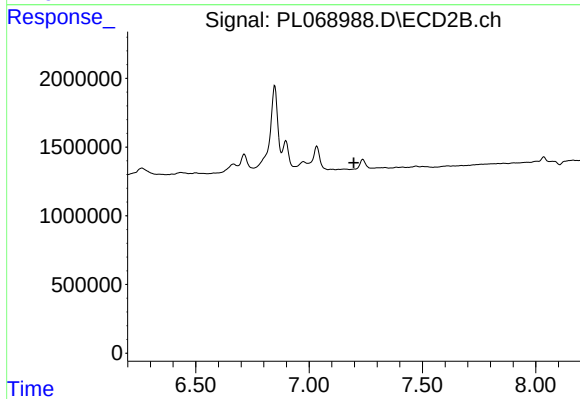

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 7.197 min
Response: 0
Conc: N.D.

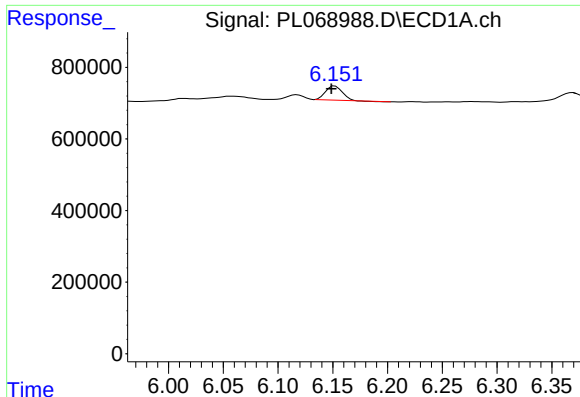

#6 beta-BHC


R.T.: 6.152 min
Delta R.T.: 0.003 min
Response: 420981
Conc: 1.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

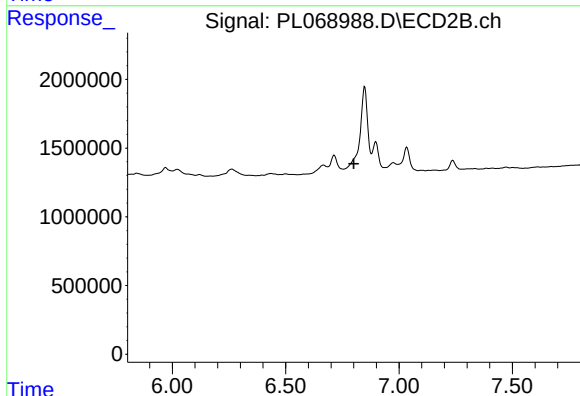


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.800 min
Response: 0
Conc: N.D.

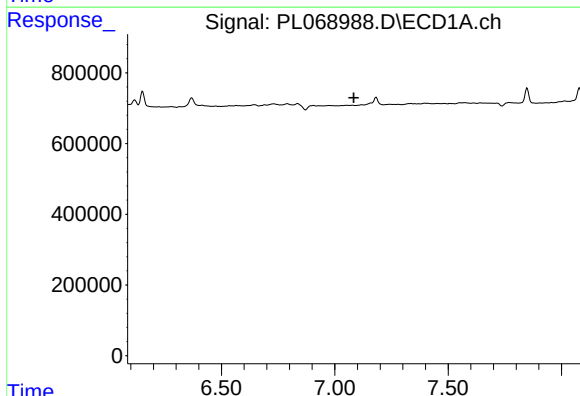


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.084 min
Response: 0
Conc: N.D.

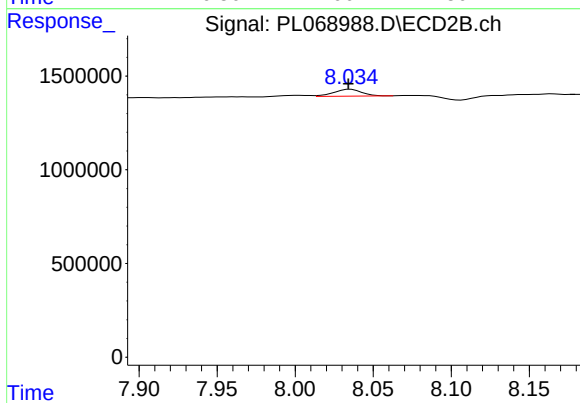

#8 Heptachlor epoxide


R.T.: 8.036 min
Delta R.T.: 0.002 min
Response: 460198
Conc: 0.40 ng/ml

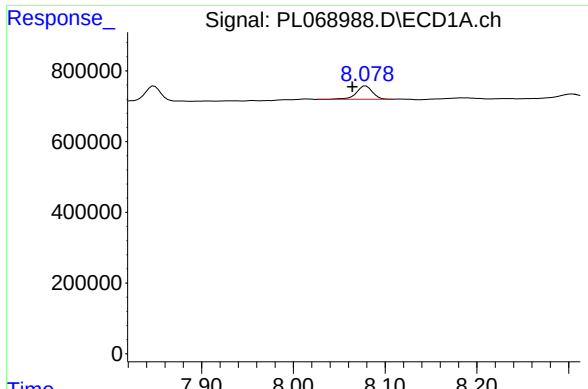

#14 Endrin


R.T.: 8.079 min
Delta R.T.: 0.015 min
Response: 464359
Conc: 0.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

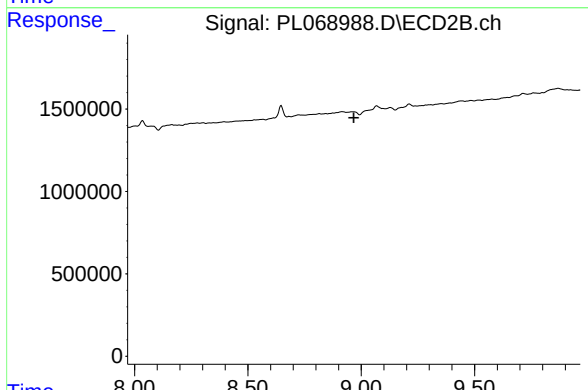


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.968 min
Response: 0
Conc: N.D.

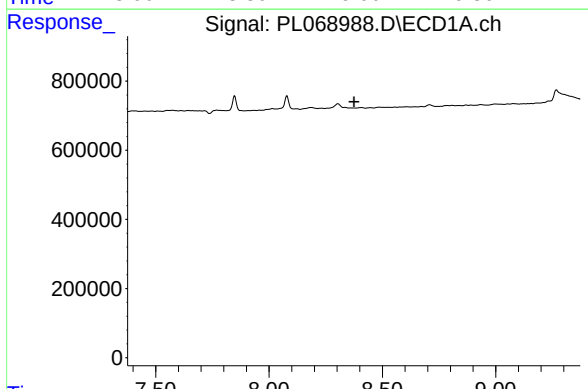


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

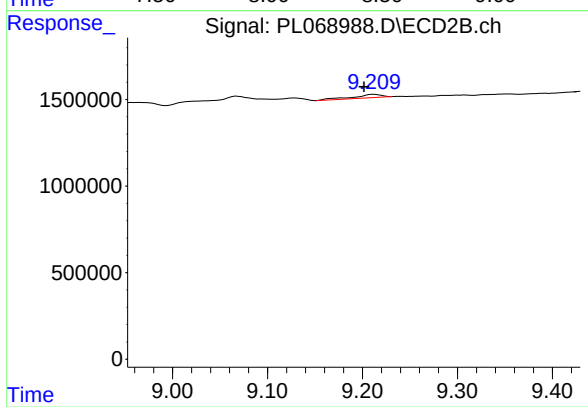

#15 Endosulfan II


R.T.: 9.212 min
Delta R.T.: 0.010 min
Response: 405904
Conc: 0.44 ng/ml

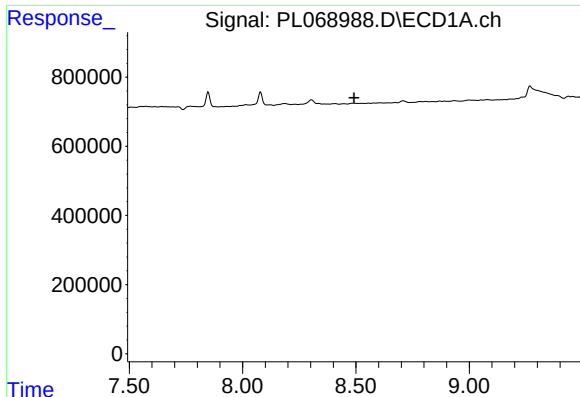

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.492 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

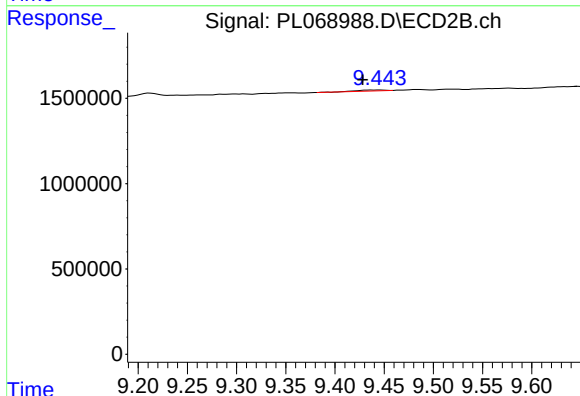


#17 4,4'-DDT

R.T.: 9.445 min
Delta R.T.: 0.017 min
Response: 113239
Conc: 0.12 ng/ml

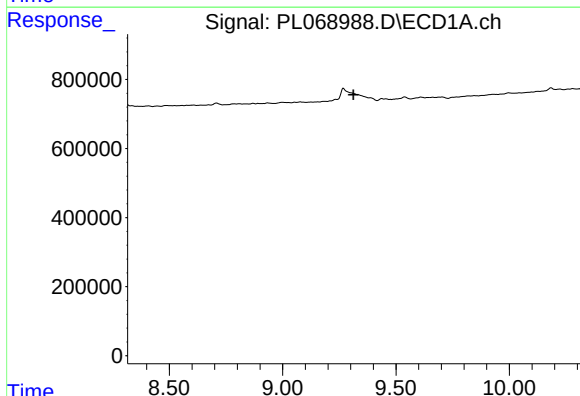


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.313 min
Response: 0
Conc: N.D.

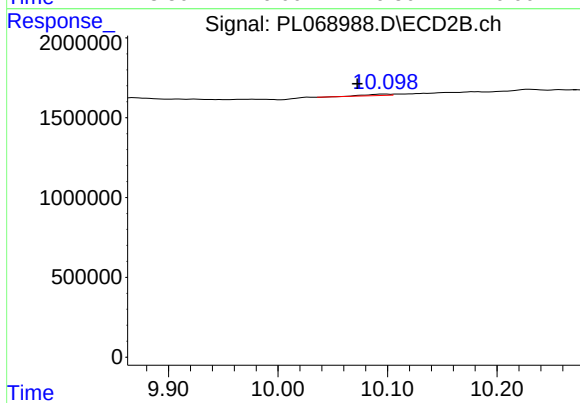

#21 Endrin ketone


R.T.: 10.099 min
Delta R.T.: 0.026 min
Response: 143859
Conc: 0.14 ng/ml

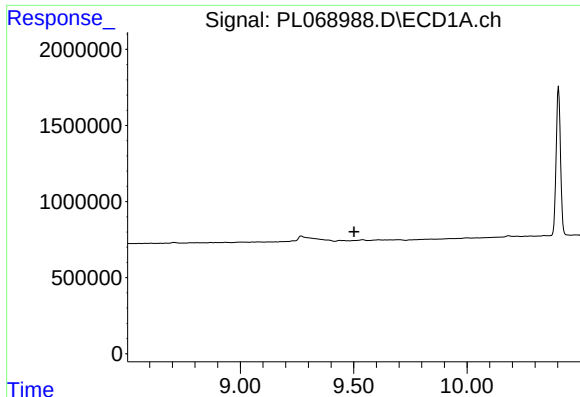

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 9.502 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

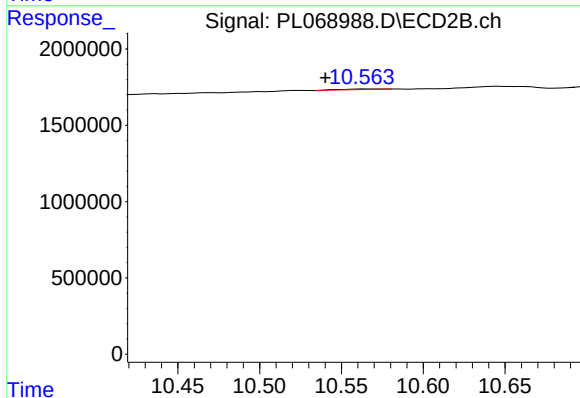


#22 Mirex

R.T.: 10.565 min
Delta R.T.: 0.024 min
Response: 91672
Conc: 0.12 ng/ml

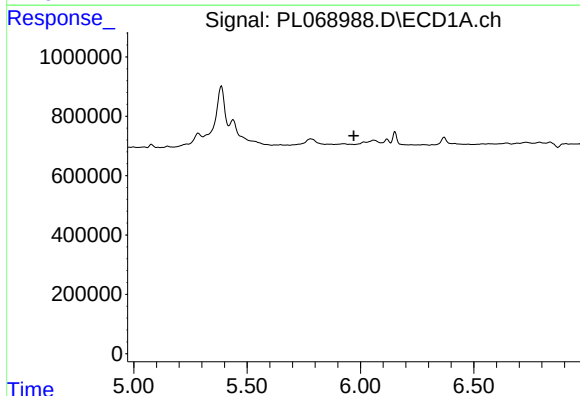


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.971 min
Response: 0
Conc: N.D.

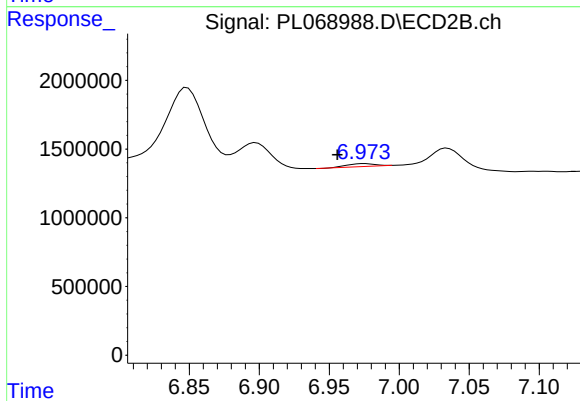

#23 Chlordane-1


R.T.: 6.975 min
Delta R.T.: 0.019 min
Response: 290282
Conc: 6.88 ng/ml

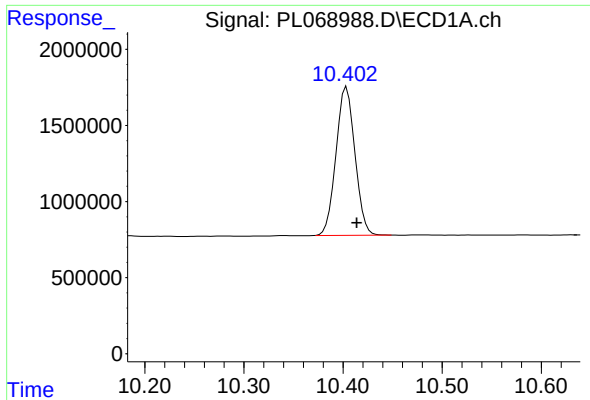

#28 Decachlorobiphenyl

R.T.: 10.404 min
Delta R.T.: -0.010 min
Response: 12953661
Conc: 22.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

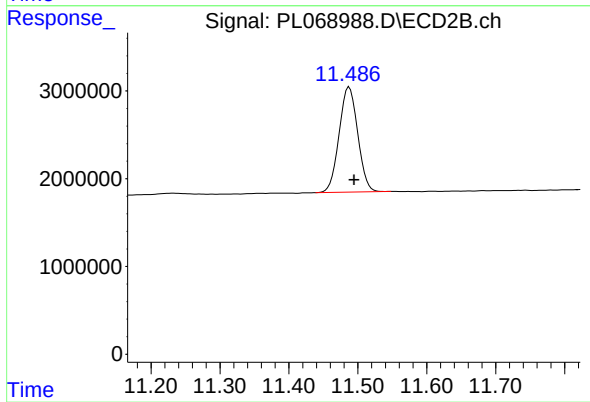

#28 Decachlorobiphenyl

R.T.: 11.488 min
Delta R.T.: -0.007 min
Response: 22526933
Conc: 23.22 ng/ml