

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081321\
 Data File : PL068956.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2021 13:23
 Operator : AR\AJ
 Sample : M3389-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CRT-21

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 05:45:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.637	5.568	9079376	24303454	21.950	23.936
28)	SA Decachlor...	10.407	11.489	13204833	22421362	22.977	23.109
Target Compounds							
12)	B 4,4'-DDE	7.640	8.565	410243	654893	0.849	0.620 #
17)	MA 4,4'-DDT	8.484	9.425	1241296	1162944	2.556	1.229 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081321\
Data File : PL068956.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2021 13:23
Operator : AR\AJ
Sample : M3389-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
CRT-21

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 05:45:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

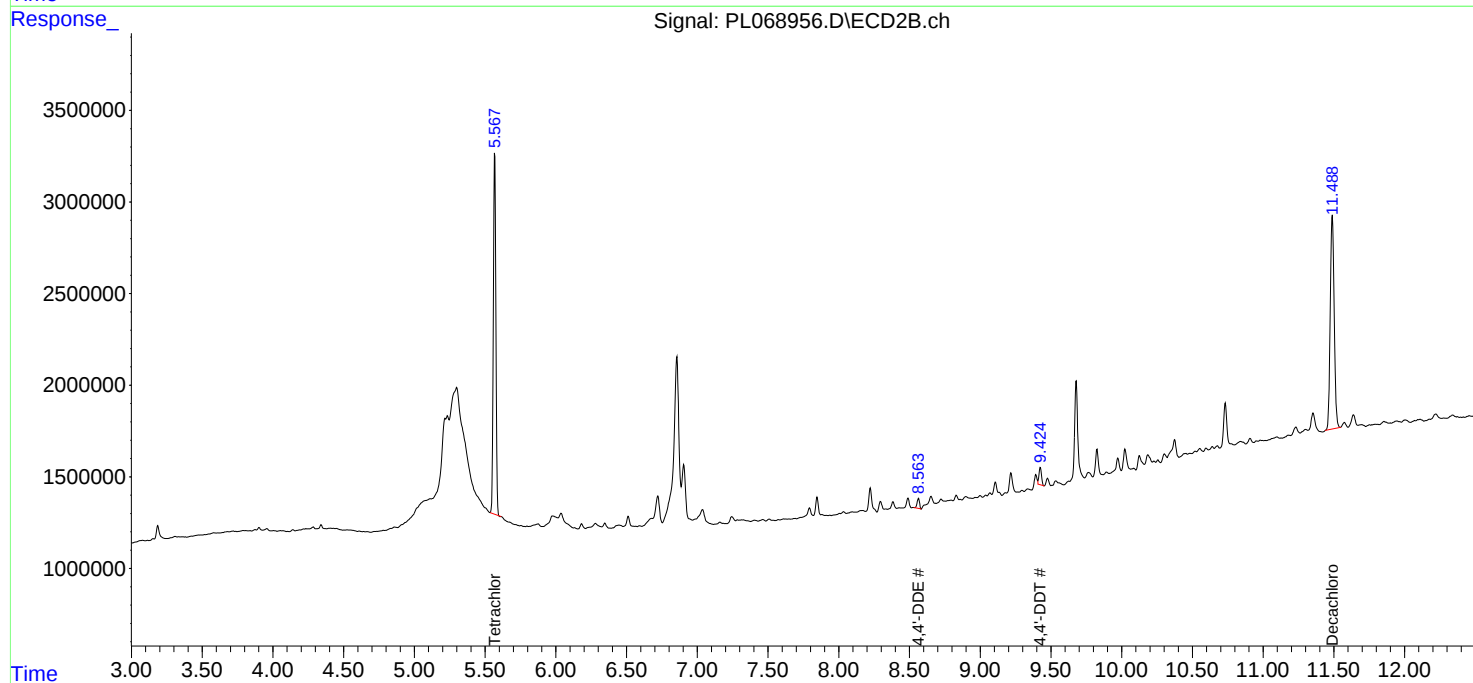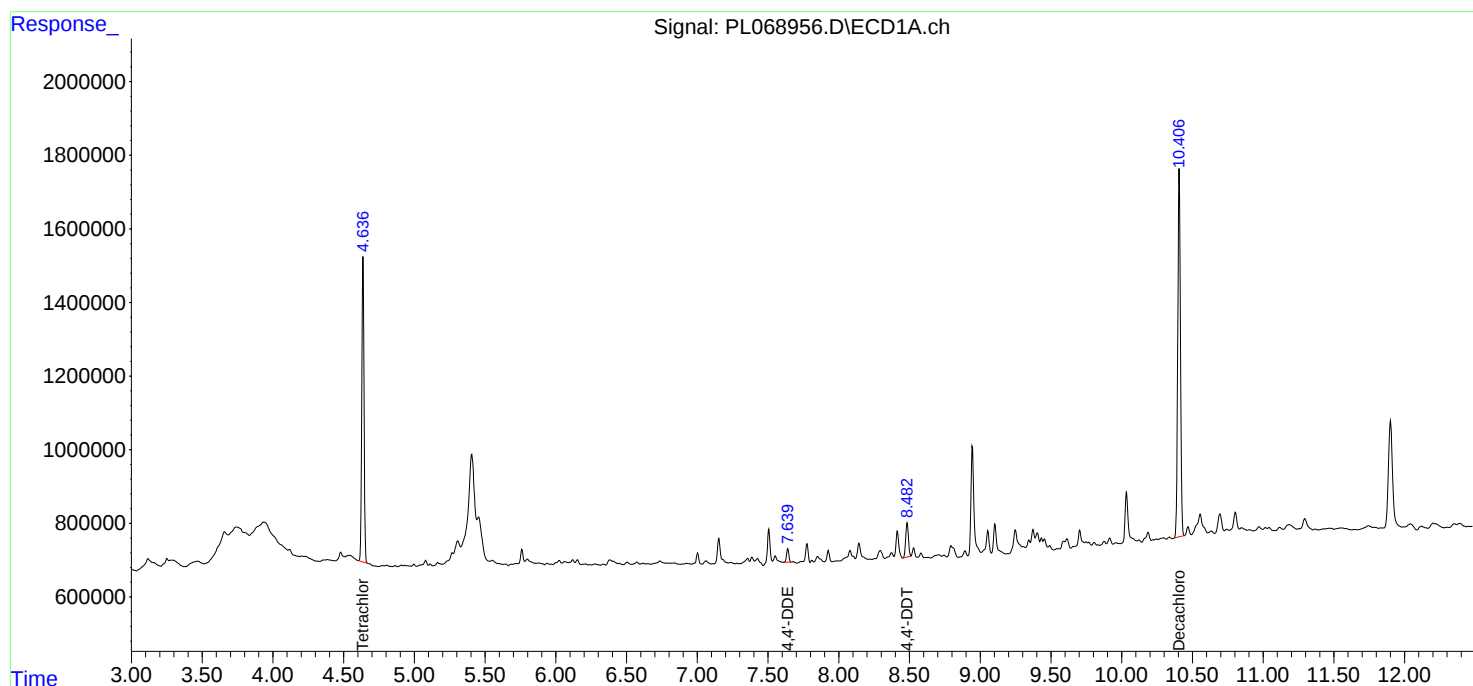


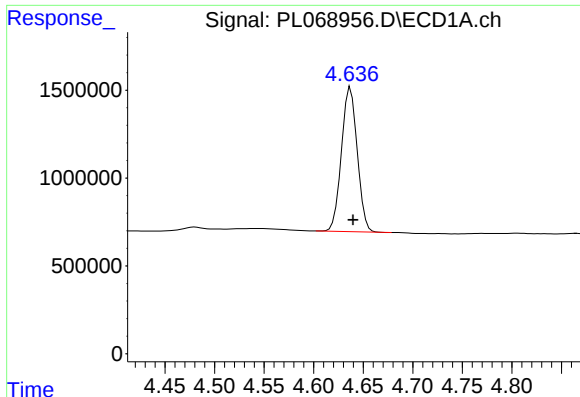

#1 Tetrachloro-m-xylene


R.T.: 4.637 min
Delta R.T.: -0.003 min
Response: 9079376
Conc: 21.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
CRT-21

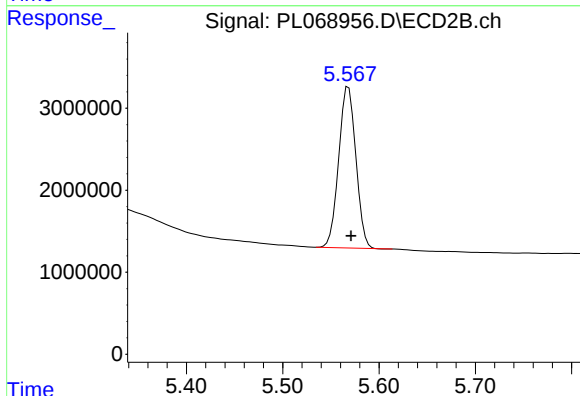


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 24303454
Conc: 23.94 ng/ml

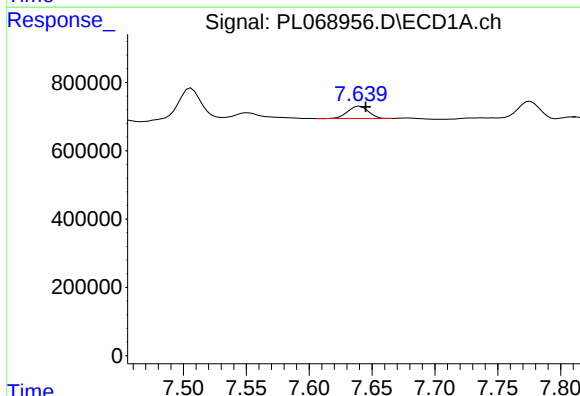


#12 4,4'-DDE

R.T.: 7.640 min
Delta R.T.: -0.005 min
Response: 410243
Conc: 0.85 ng/ml

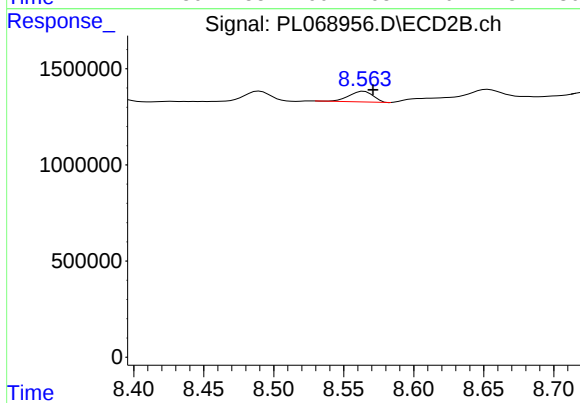

#12 4,4'-DDE


R.T.: 8.565 min
Delta R.T.: -0.006 min
Response: 654893
Conc: 0.62 ng/ml

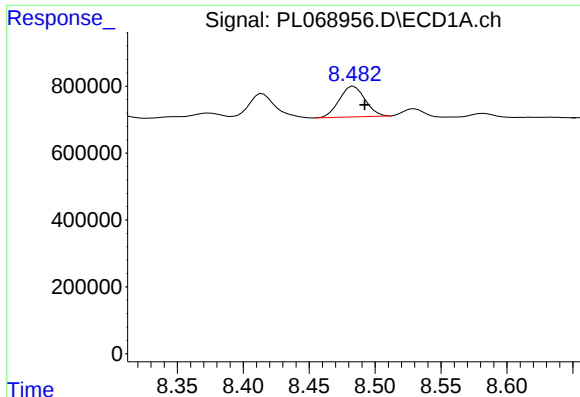

#17 4,4'-DDT


R.T.: 8.484 min
Delta R.T.: -0.008 min
Response: 1241296
Conc: 2.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
CRT-21

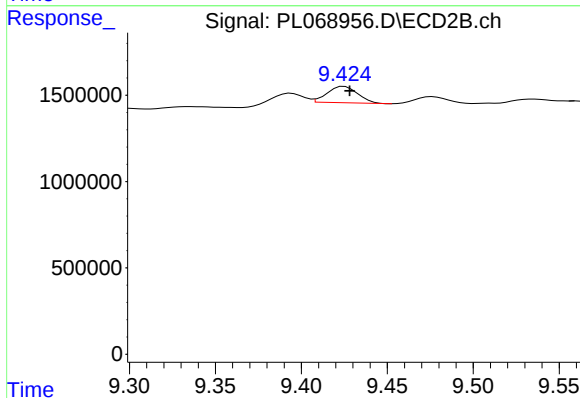


#17 4,4'-DDT

R.T.: 9.425 min
Delta R.T.: -0.003 min
Response: 1162944
Conc: 1.23 ng/ml

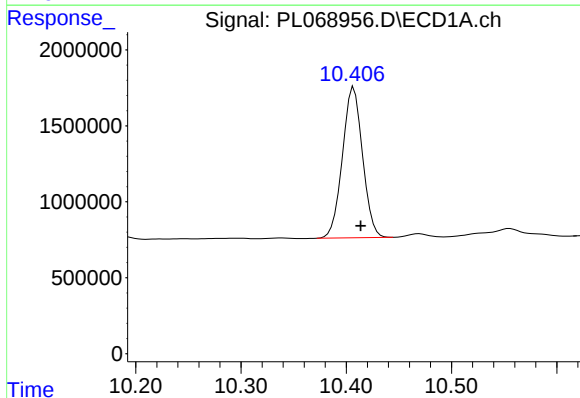

#28 Decachlorobiphenyl

R.T.: 10.407 min
Delta R.T.: -0.006 min
Response: 13204833
Conc: 22.98 ng/ml

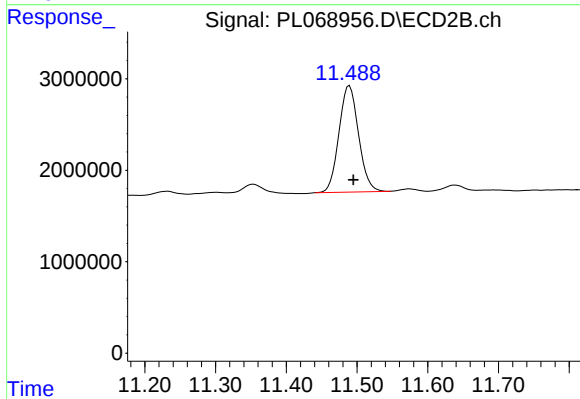

#28 Decachlorobiphenyl

R.T.: 11.489 min
Delta R.T.: -0.005 min
Response: 22421362
Conc: 23.11 ng/ml