

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081321\
 Data File : PL068987.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2021 01:12
 Operator : AR\AJ
 Sample : M3397-21
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SWCS-06-1015

Manual Integrations
 APPROVED

mohammad
 8/16/2021 9:36:05 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 05:53:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.636	5.568	8988141	25401384	21.729	25.018
28)	SA Decachlor...	10.404	11.487	10825301	19068688	18.837	19.654
Target Compounds							
12)	B 4,4'-DDE	7.636	8.564	181542	347264	0.376m	0.329

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081321\
Data File : PL068987.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2021 01:12
Operator : AR\AJ
Sample : M3397-21
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SWCS-06-1015


Manual Integrations
APPROVED

mohammad
8/16/2021 9:36:05 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 05:53:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

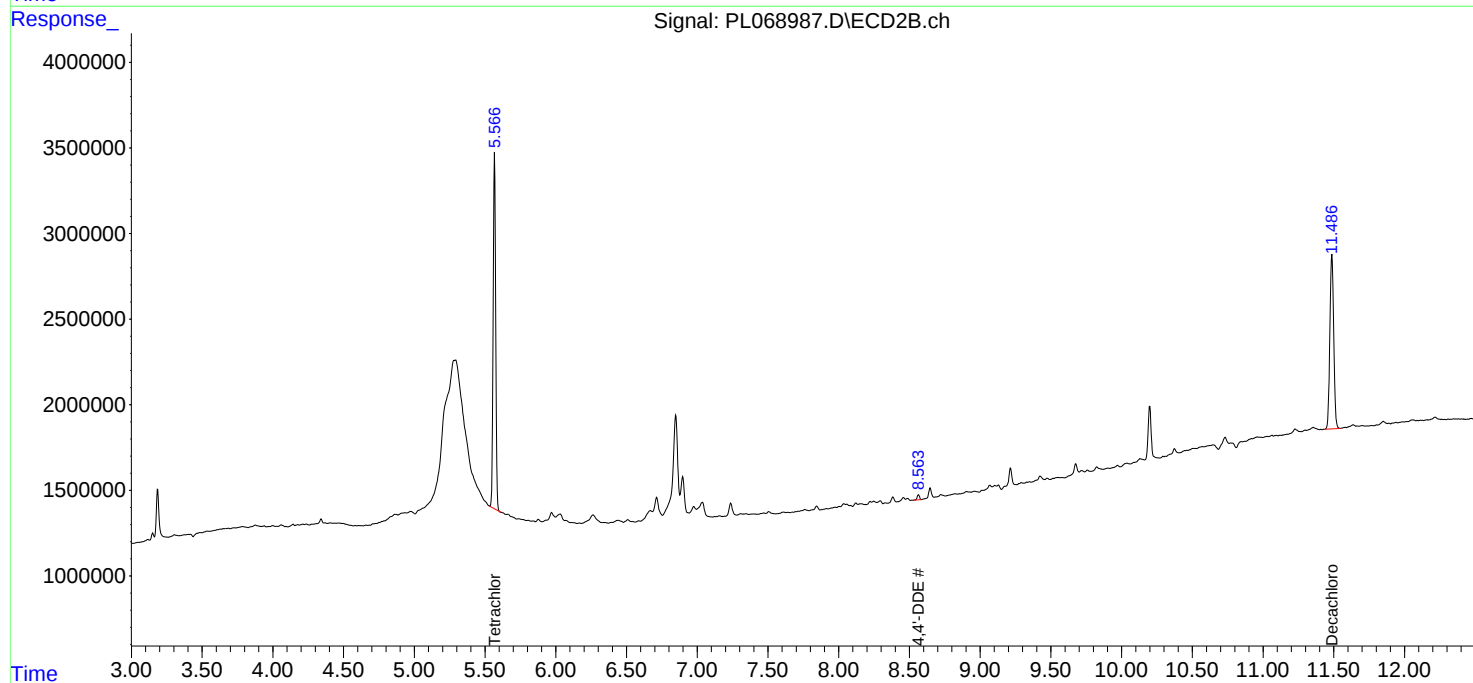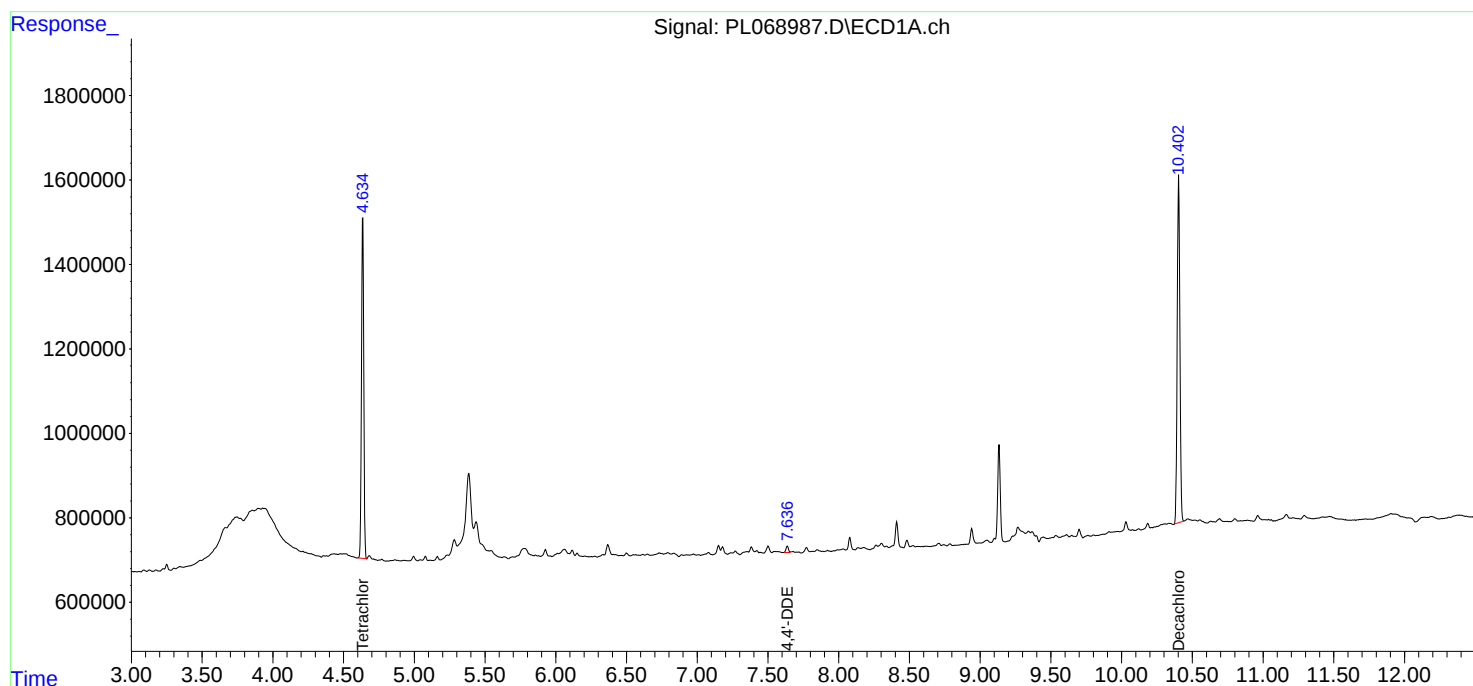

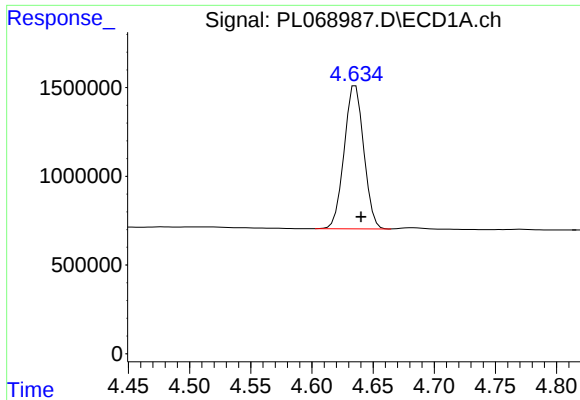


#1 Tetrachloro-m-xylene

R.T.: 4.636 min
Delta R.T.: -0.004 min
Response: 8988141
Conc: 21.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
SWCS-06-1015


Manual Integrations
APPROVED

mohammad
8/16/2021 9:36:05 AM

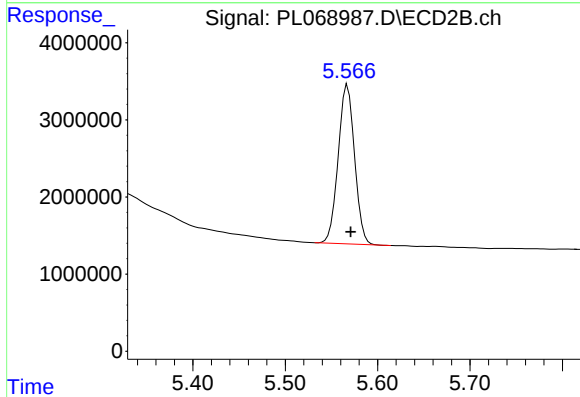


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 25401384
Conc: 25.02 ng/ml

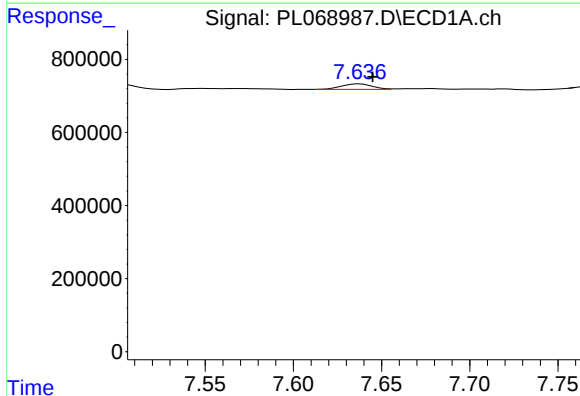


#12 4,4'-DDE

R.T.: 7.636 min
Delta R.T.: -0.009 min
Response: 181542
Conc: 0.38 ng/ml m

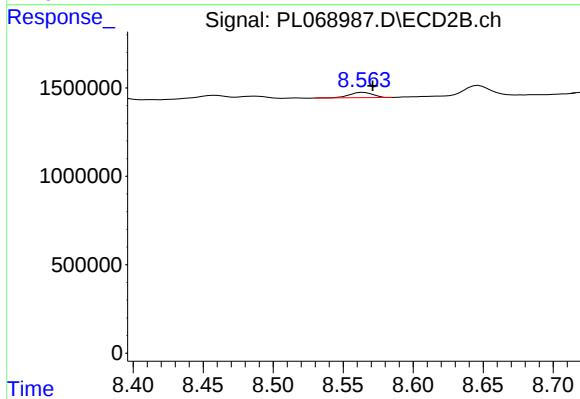

#12 4,4'-DDE

R.T.: 8.564 min
Delta R.T.: -0.007 min
Response: 347264
Conc: 0.33 ng/ml

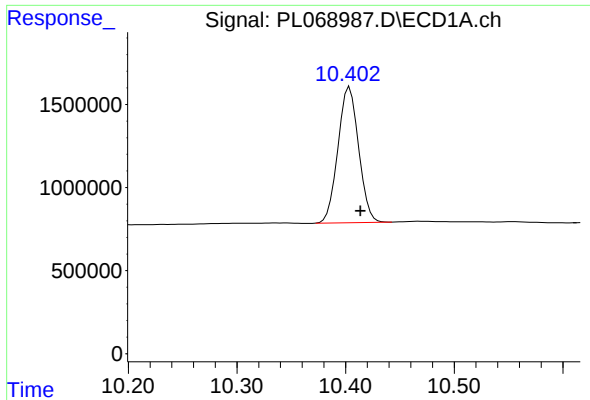


#28 Decachlorobiphenyl

R.T.: 10.404 min
Delta R.T.: -0.010 min
Response: 10825301
Conc: 18.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
SWCS-06-1015

Manual Integrations
APPROVED

mohammad
8/16/2021 9:36:05 AM

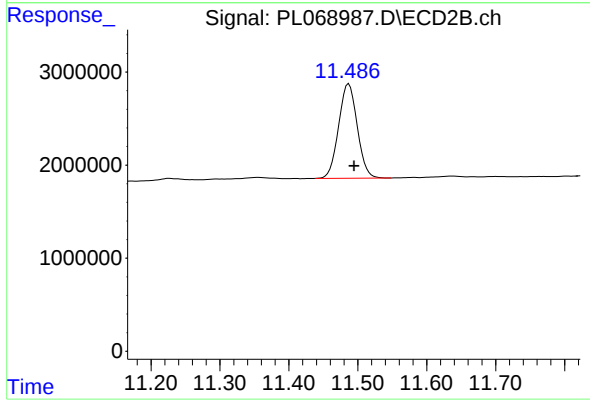

#28 Decachlorobiphenyl

R.T.: 11.487 min
Delta R.T.: -0.008 min
Response: 19068688
Conc: 19.65 ng/ml