

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081324\
 Data File : PL091012.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2024 23:36
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 03:41:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081324.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 14 03:38:39 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.784	202.3E6	242.8E6	102.256	106.944
28)	SA Decachlor...	9.056	7.926	137.8E6	182.7E6	95.984	99.539
Target Compounds							
23)	Chlordane-1	4.706	3.784	90392101	74598504	986.809	1053.532
24)	Chlordane-2	5.235	4.361	93394814	86028950	965.656	989.079
25)	Chlordane-3	5.944	4.991	333.4E6	254.4E6	1021.228	1055.528
26)	Chlordane-4	6.026	5.054	404.1E6	239.8E6	1013.519	1037.591
27)	Chlordane-5	6.875	5.719	71144423	68235196	970.062	1006.982



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081324\
Data File : PL091012.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2024 23:36
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 03:41:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081324.M
Quant Title : GC Extractables
QLast Update : Wed Aug 14 03:38:39 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

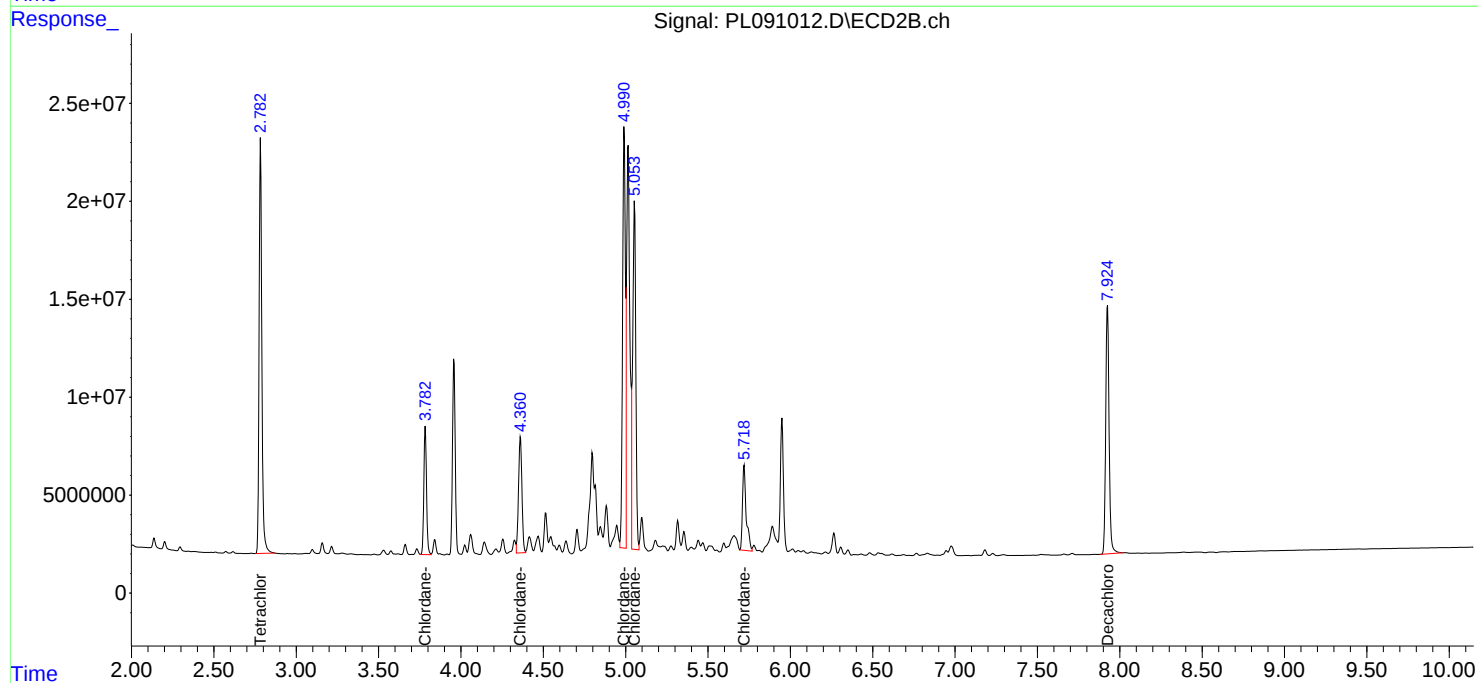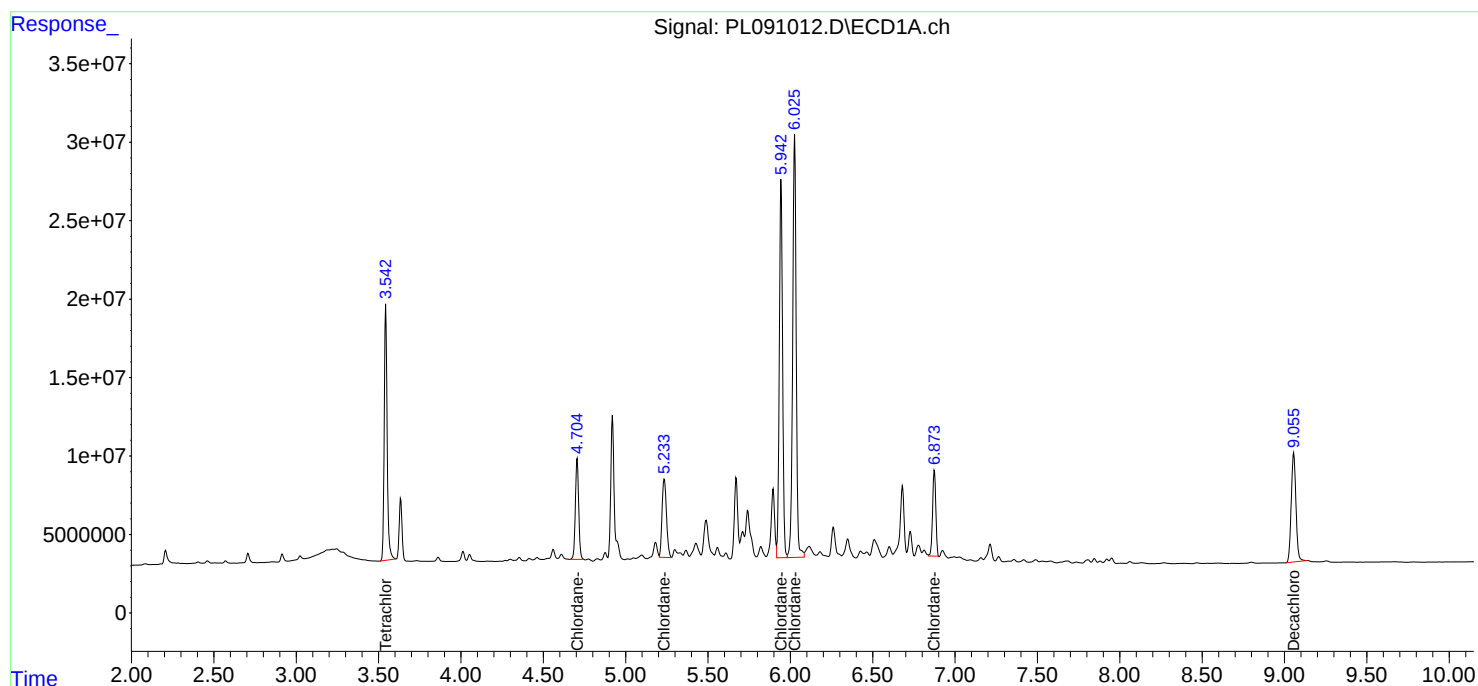


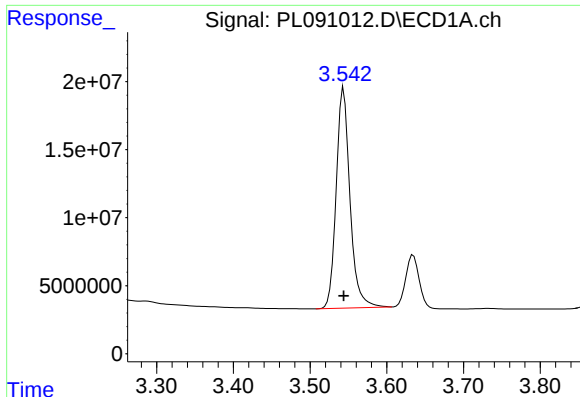

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 202272574
Conc: 102.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

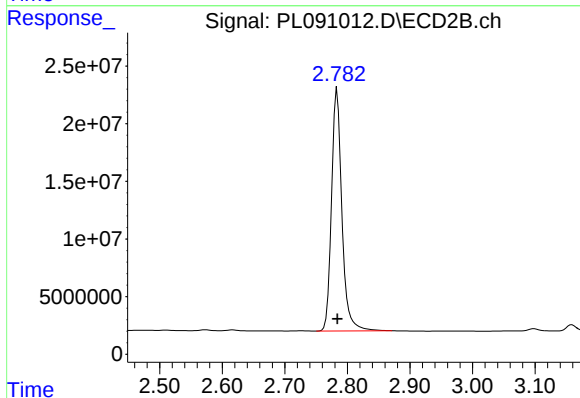


#1 Tetrachloro-m-xylene

R.T.: 2.784 min
Delta R.T.: 0.000 min
Response: 242828855
Conc: 106.94 ng/ml

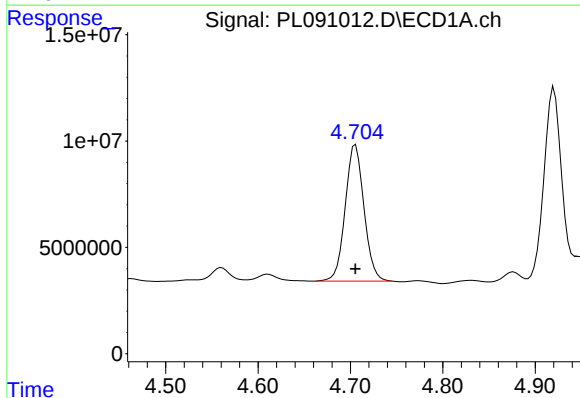


#23 Chlordane-1

R.T.: 4.706 min
Delta R.T.: 0.000 min
Response: 90392101
Conc: 986.81 ng/ml

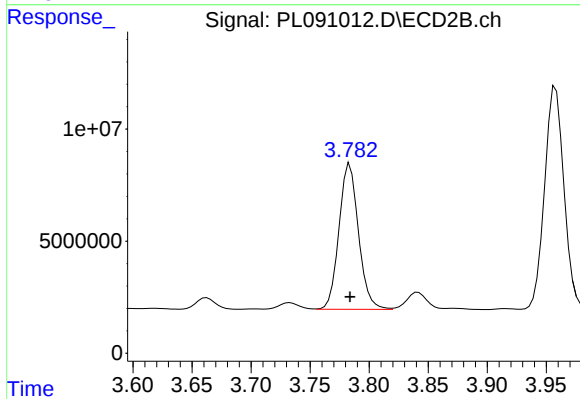

#23 Chlordane-1


R.T.: 3.784 min
Delta R.T.: 0.000 min
Response: 74598504
Conc: 1053.53 ng/ml

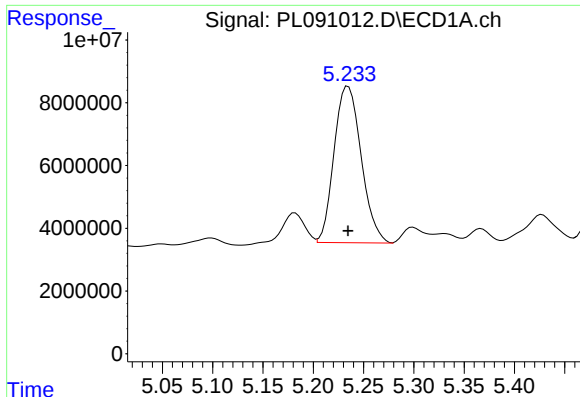

#24 Chlordane-2


R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 93394814
Conc: 965.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

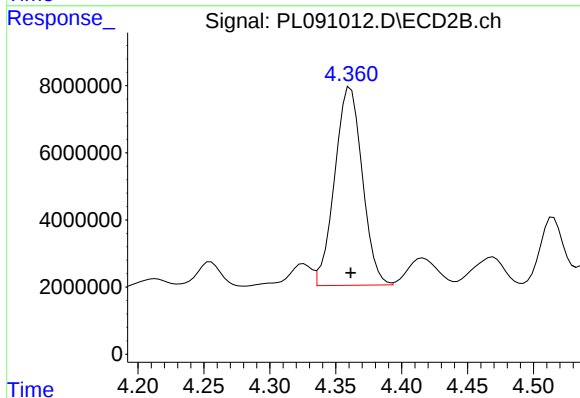


#24 Chlordane-2

R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 86028950
Conc: 989.08 ng/ml

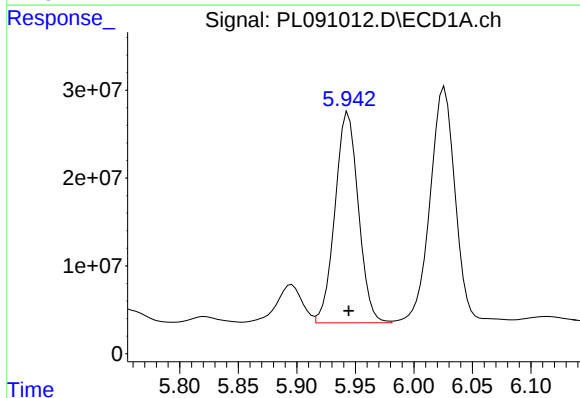


#25 Chlordane-3

R.T.: 5.944 min
Delta R.T.: 0.000 min
Response: 333447074
Conc: 1021.23 ng/ml

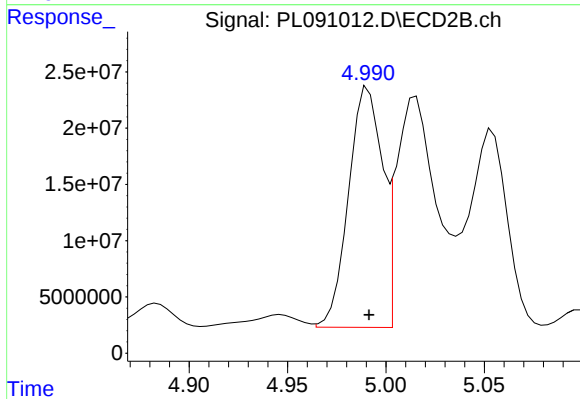

#25 Chlordane-3


R.T.: 4.991 min
Delta R.T.: 0.000 min
Response: 254373987
Conc: 1055.53 ng/ml

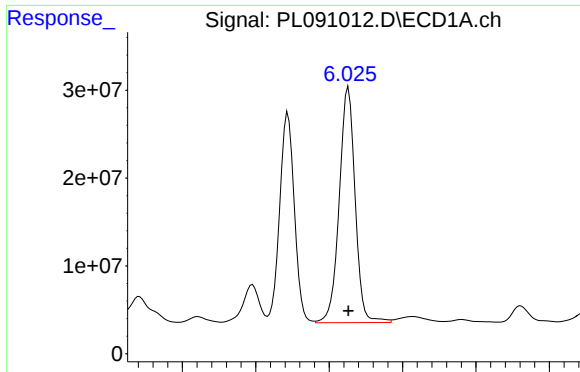

#26 Chlordane-4


R.T.: 6.026 min
Delta R.T.: 0.000 min
Response: 404139799
Conc: 1013.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

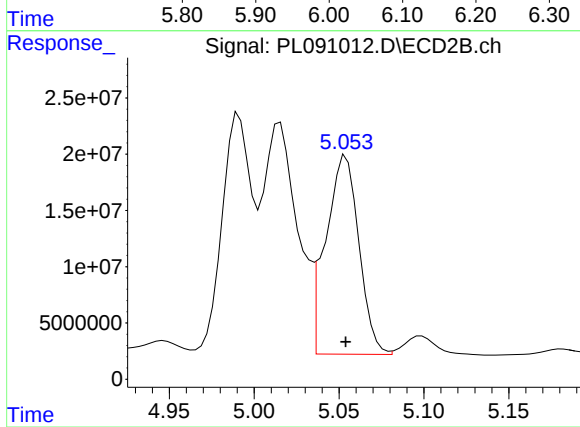


#26 Chlordane-4

R.T.: 5.054 min
Delta R.T.: 0.000 min
Response: 239796760
Conc: 1037.59 ng/ml

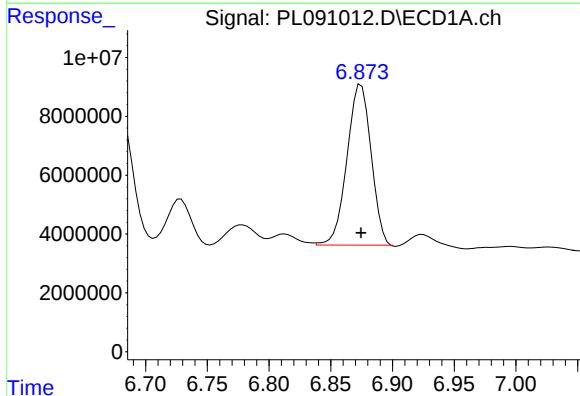


#27 Chlordane-5

R.T.: 6.875 min
Delta R.T.: 0.000 min
Response: 71144423
Conc: 970.06 ng/ml

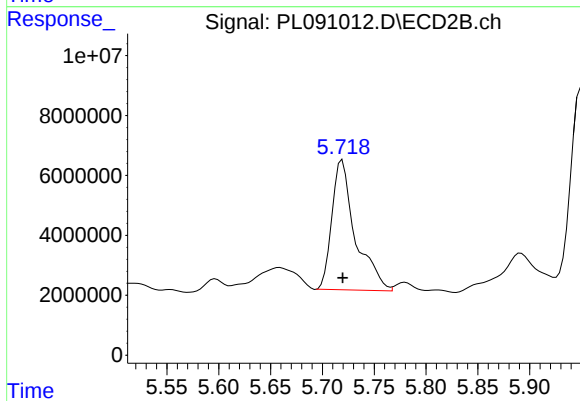

#27 Chlordane-5


R.T.: 5.719 min
Delta R.T.: 0.000 min
Response: 68235196
Conc: 1006.98 ng/ml

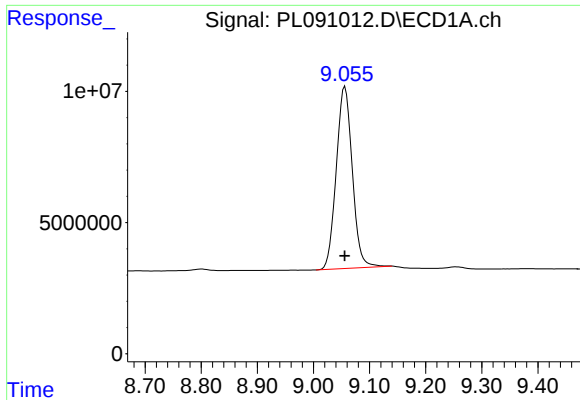

#28 Decachlorobiphenyl

R.T.: 9.056 min
Delta R.T.: 0.000 min
Response: 137825395
Conc: 95.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

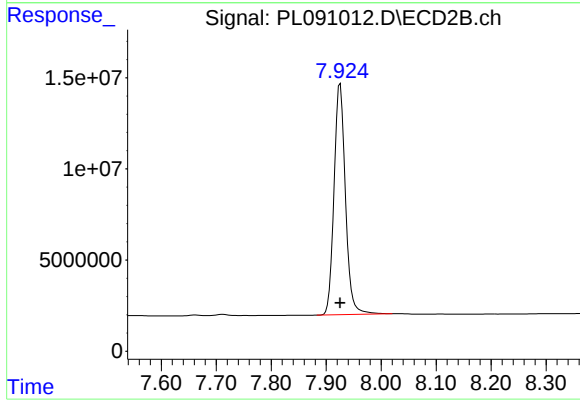

#28 Decachlorobiphenyl

R.T.: 7.926 min
Delta R.T.: 0.000 min
Response: 182683569
Conc: 99.54 ng/ml