

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081324\
 Data File : PL091013.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2024 23:50
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 03:41:42 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081324.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 14 03:38:39 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.784	142.7E6	167.2E6	72.148	73.623
28)	SA Decachlor...	9.055	7.926	101.1E6	130.5E6	70.410	71.087
Target Compounds							
23)	Chlordane-1	4.706	3.784	64733006	51656356	706.689	729.527
24)	Chlordane-2	5.234	4.362	67502476	69910540	697.942	803.765
25)	Chlordane-3	5.944	4.992	234.7E6	178.3E6	718.939	739.804
26)	Chlordane-4	6.026	5.054	285.7E6	167.7E6	716.399	725.778
27)	Chlordane-5	6.875	5.720	51633681	48048892	704.031	709.083



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081324\
Data File : PL091013.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2024 23:50
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 03:41:42 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081324.M
Quant Title : GC Extractables
QLast Update : Wed Aug 14 03:38:39 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

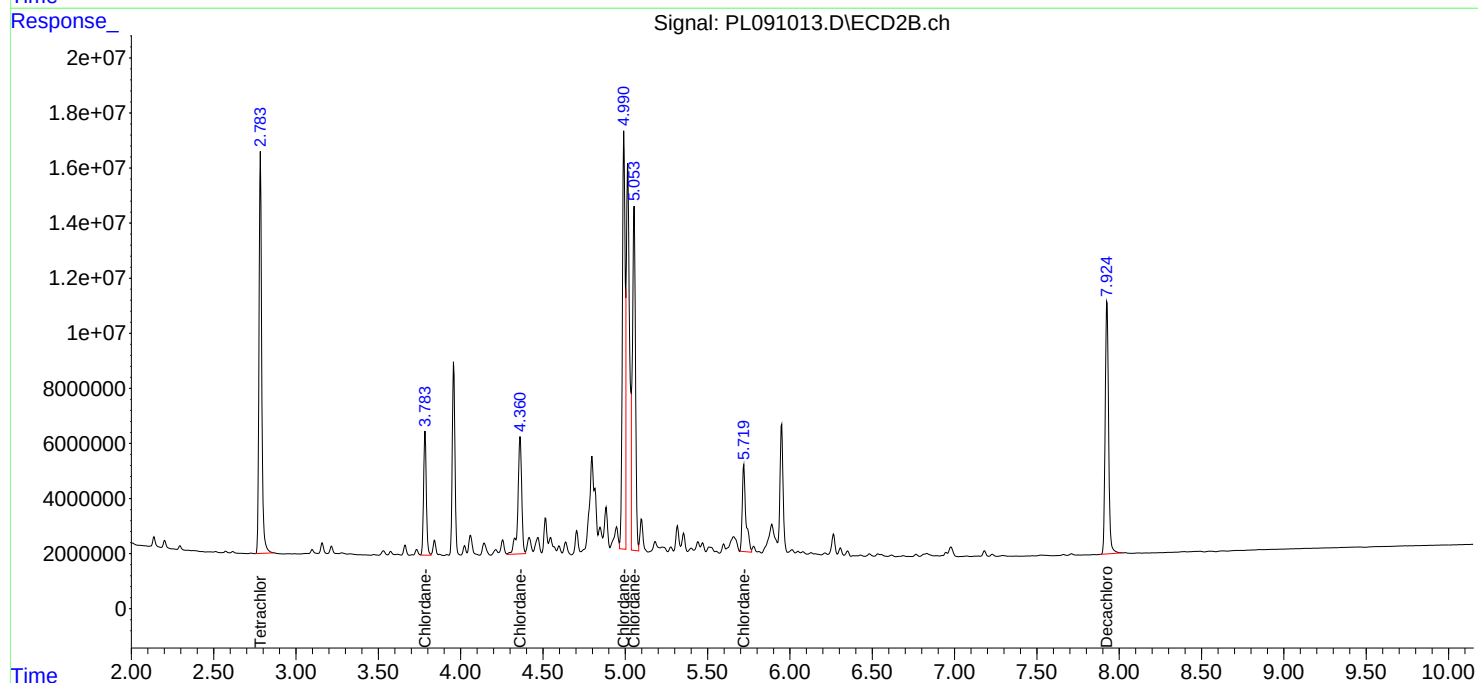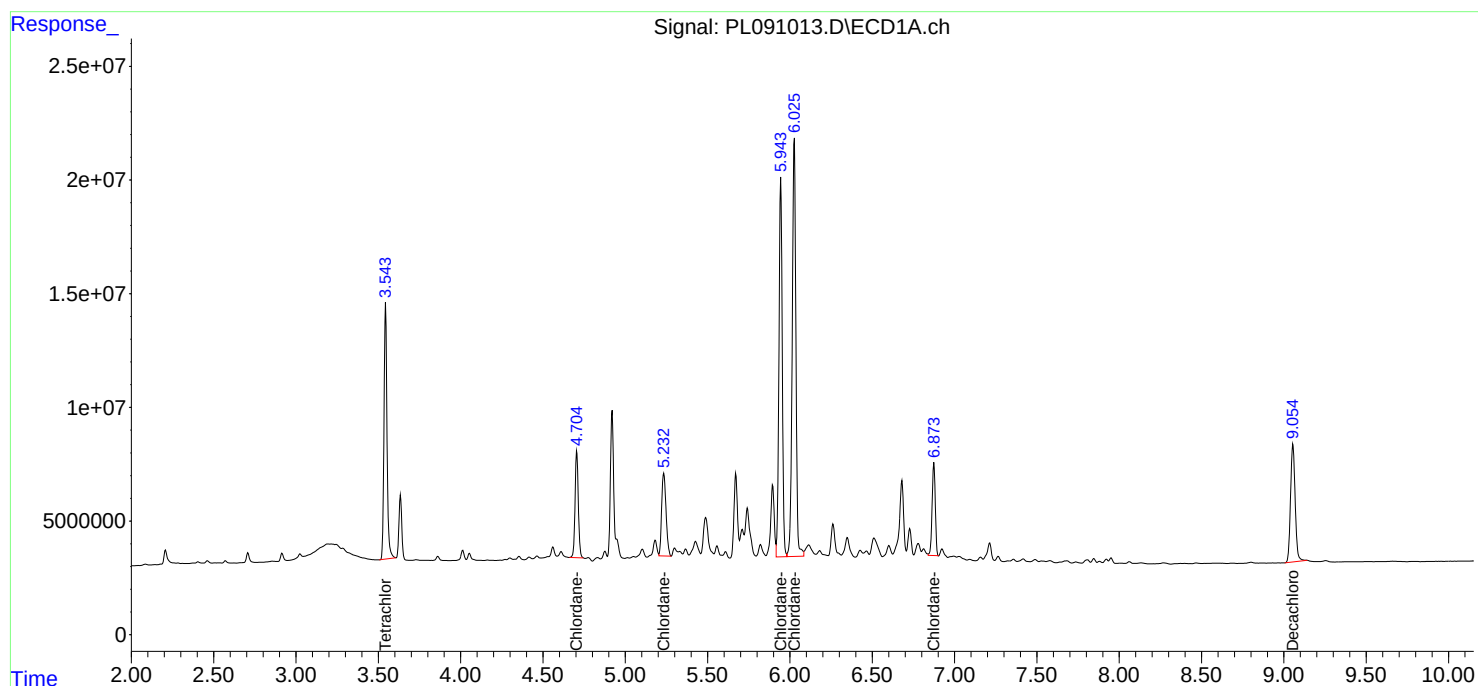


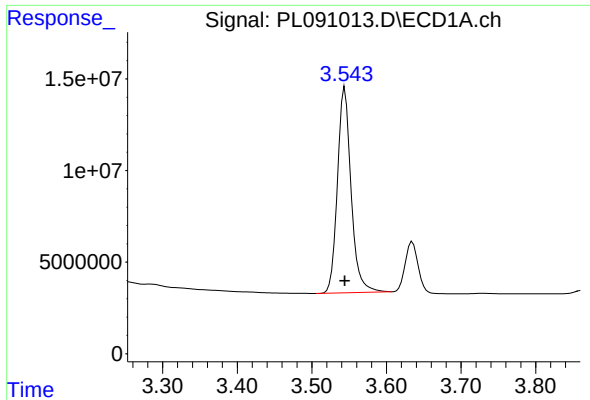

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 142715824
Conc: 72.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

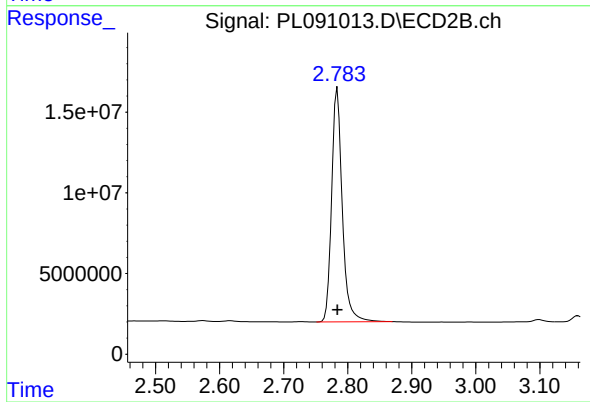


#1 Tetrachloro-m-xylene

R.T.: 2.784 min
Delta R.T.: 0.000 min
Response: 167170588
Conc: 73.62 ng/ml

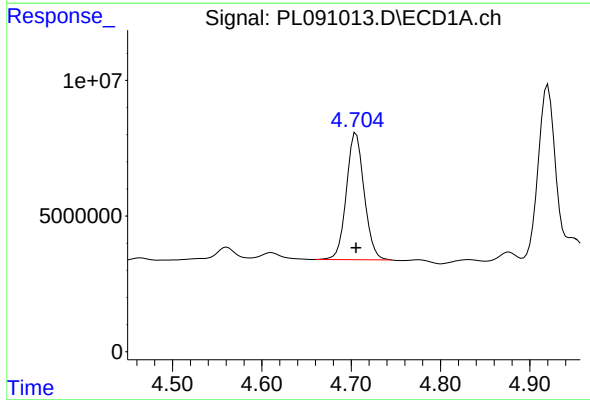


#23 Chlordane-1

R.T.: 4.706 min
Delta R.T.: 0.000 min
Response: 64733006
Conc: 706.69 ng/ml

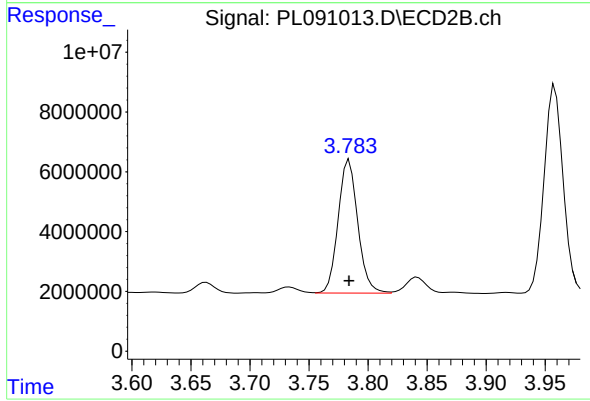

#23 Chlordane-1


R.T.: 3.784 min
Delta R.T.: 0.000 min
Response: 51656356
Conc: 729.53 ng/ml

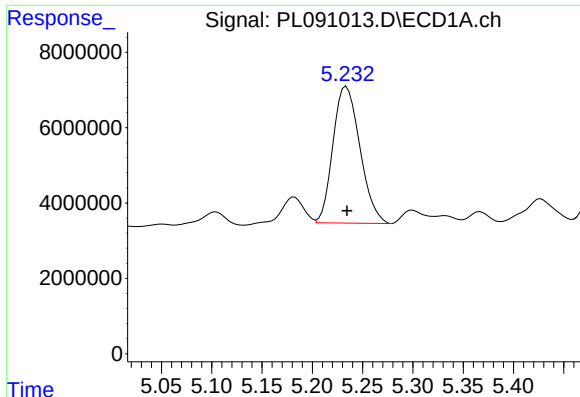

#24 Chlordane-2


R.T.: 5.234 min
Delta R.T.: 0.000 min
Response: 67502476
Conc: 697.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

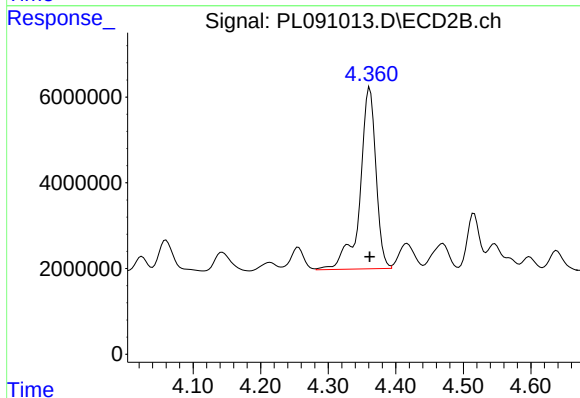


#24 Chlordane-2

R.T.: 4.362 min
Delta R.T.: 0.000 min
Response: 69910540
Conc: 803.77 ng/ml

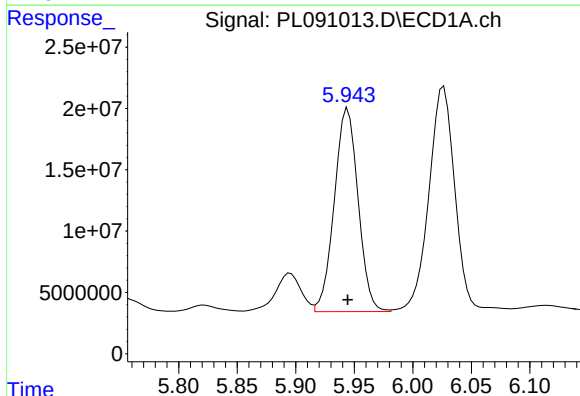


#25 Chlordane-3

R.T.: 5.944 min
Delta R.T.: 0.000 min
Response: 234744807
Conc: 718.94 ng/ml

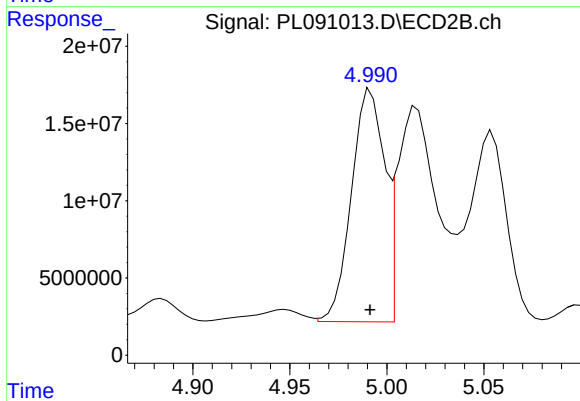

#25 Chlordane-3


R.T.: 4.992 min
Delta R.T.: 0.000 min
Response: 178286909
Conc: 739.80 ng/ml

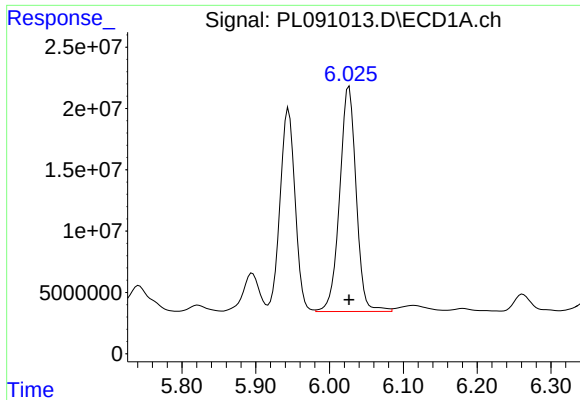

#26 Chlordane-4


R.T.: 6.026 min
Delta R.T.: 0.000 min
Response: 285663417
Conc: 716.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

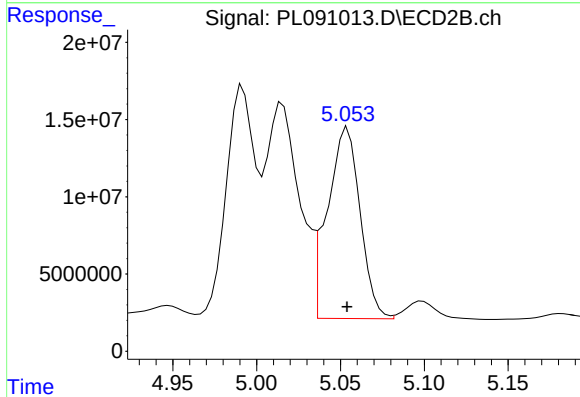


#26 Chlordane-4

R.T.: 5.054 min
Delta R.T.: 0.000 min
Response: 167733916
Conc: 725.78 ng/ml

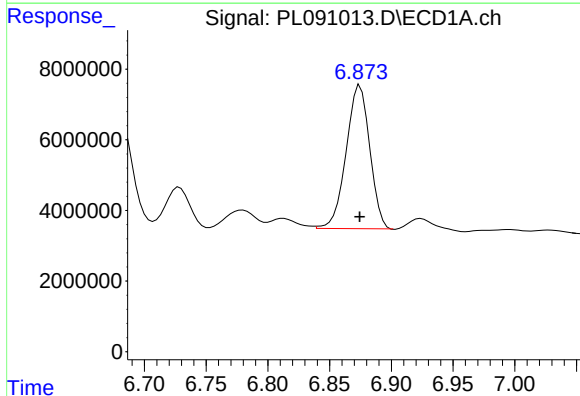


#27 Chlordane-5

R.T.: 6.875 min
Delta R.T.: 0.000 min
Response: 51633681
Conc: 704.03 ng/ml

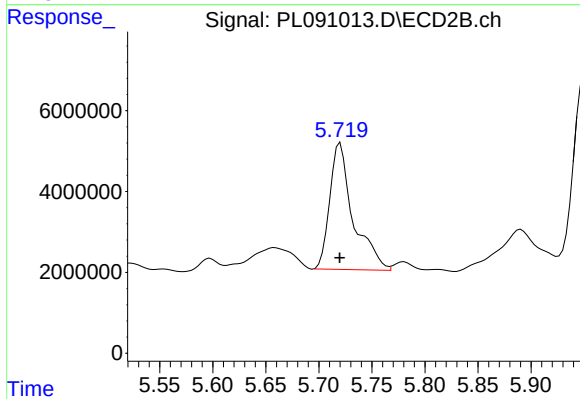

#27 Chlordane-5

R.T.: 5.720 min
Delta R.T.: 0.000 min
Response: 48048892
Conc: 709.08 ng/ml

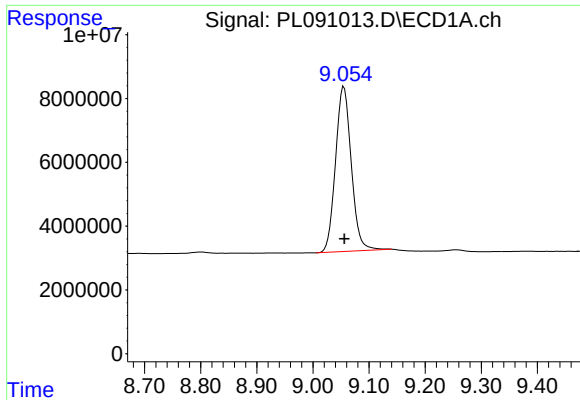

#28 Decachlorobiphenyl


R.T.: 9.055 min

Delta R.T.: 0.000 min

Response: 101103008

Conc: 70.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

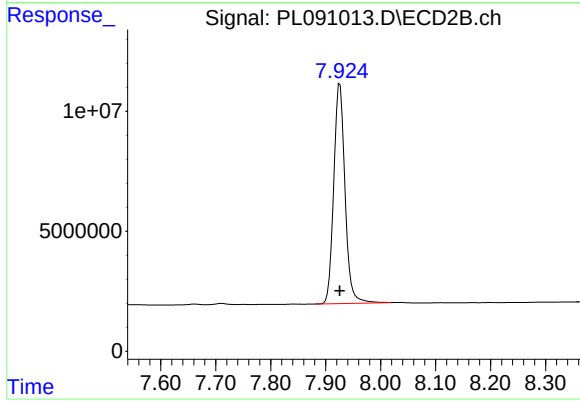

#28 Decachlorobiphenyl

R.T.: 7.926 min

Delta R.T.: 0.000 min

Response: 130466560

Conc: 71.09 ng/ml