

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081324\
 Data File : PL091014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2024 00:03
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 03:42:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081324.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 14 03:38:39 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.784	98905033	113.5E6	50.000	50.000
28)	SA Decachlor...	9.056	7.925	71795838	91765031	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.705	3.784	45800209	35404003	500.000	500.000
24)	Chlordane-2	5.235	4.361	48358226	43489414	500.000	500.000
25)	Chlordane-3	5.944	4.991	163.3E6	120.5E6	500.000	500.000
26)	Chlordane-4	6.026	5.054	199.4E6	115.6E6	500.000	500.000
27)	Chlordane-5	6.874	5.720	36670029	33881030	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081324\
Data File : PL091014.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2024 00:03
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 03:42:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081324.M
Quant Title : GC Extractables
QLast Update : Wed Aug 14 03:38:39 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

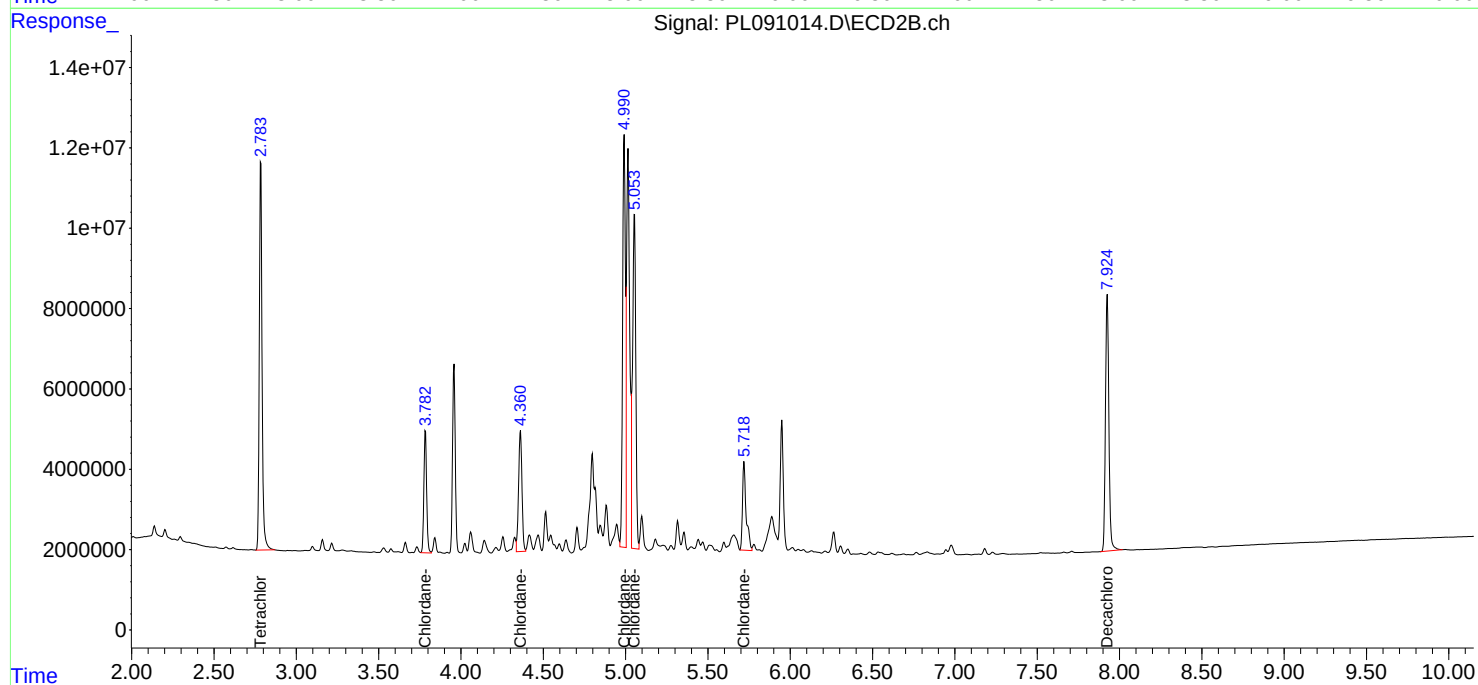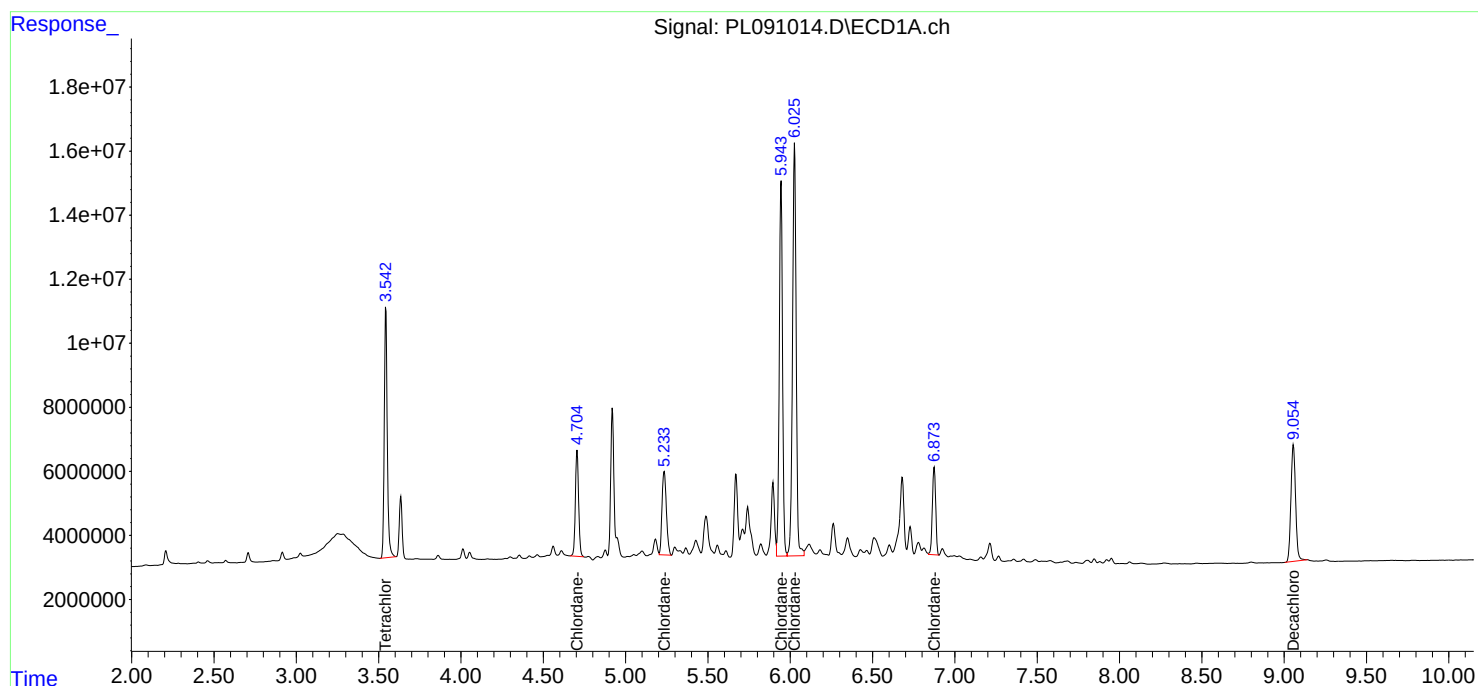


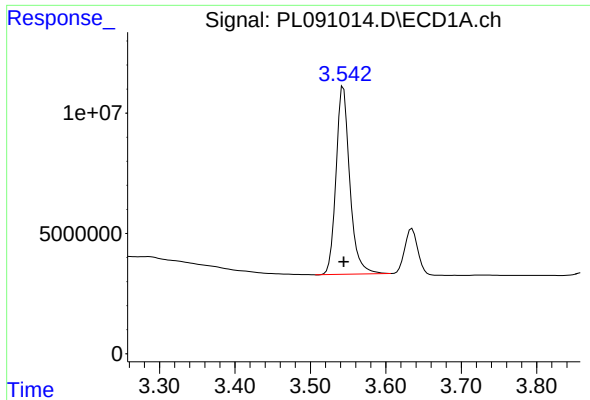

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 98905033
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

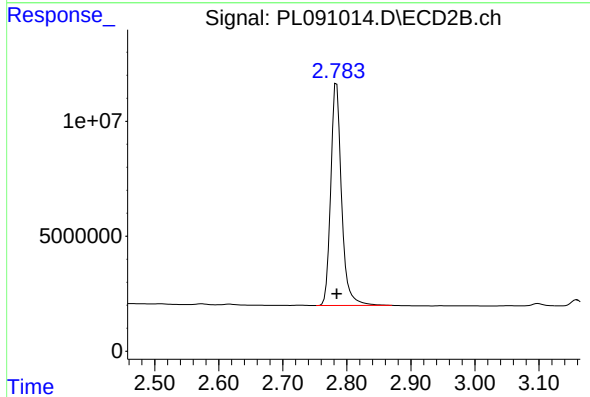


#1 Tetrachloro-m-xylene

R.T.: 2.784 min
Delta R.T.: 0.000 min
Response: 113530756
Conc: 50.00 ng/ml

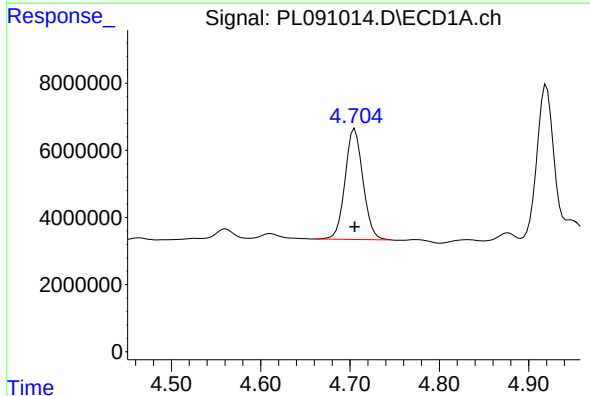


#23 Chlordane-1

R.T.: 4.705 min
Delta R.T.: 0.000 min
Response: 45800209
Conc: 500.00 ng/ml

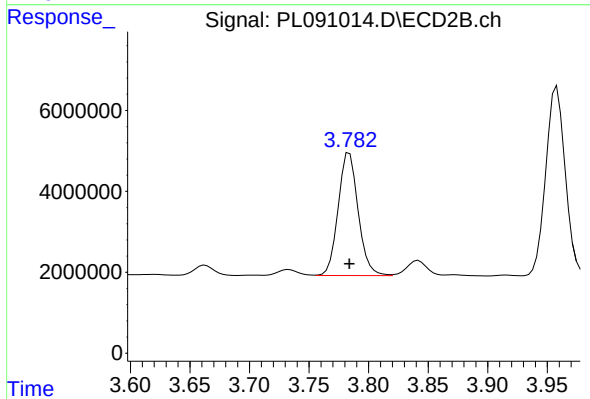

#23 Chlordane-1


R.T.: 3.784 min
Delta R.T.: 0.000 min
Response: 35404003
Conc: 500.00 ng/ml

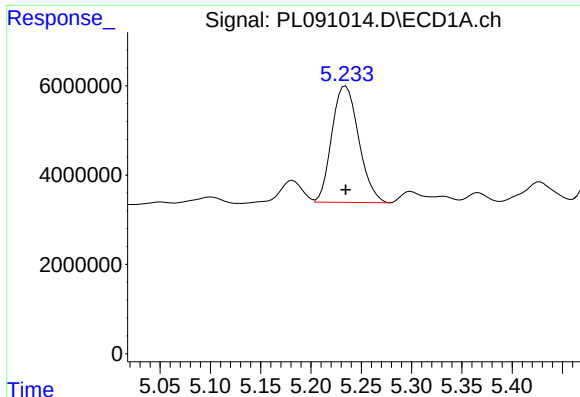

#24 Chlordane-2


R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 48358226
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

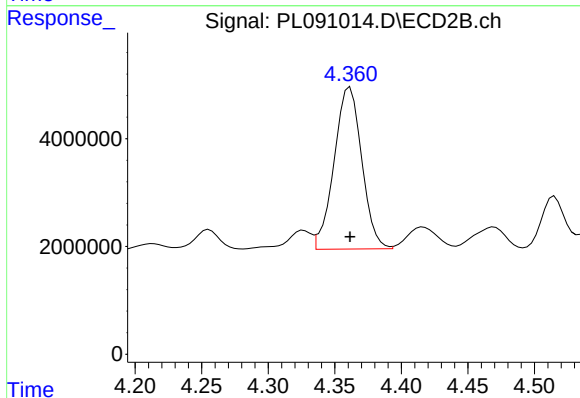


#24 Chlordane-2

R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 43489414
Conc: 500.00 ng/ml

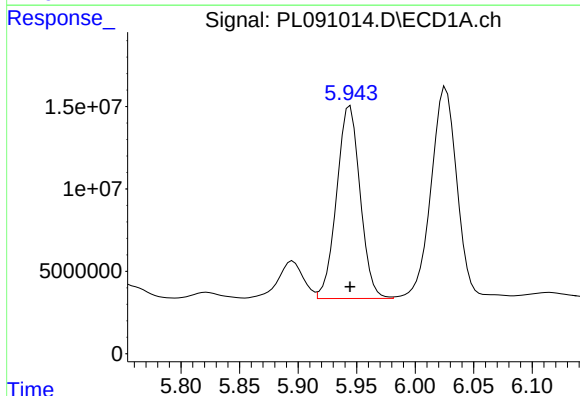


#25 Chlordane-3

R.T.: 5.944 min
Delta R.T.: 0.000 min
Response: 163257820
Conc: 500.00 ng/ml

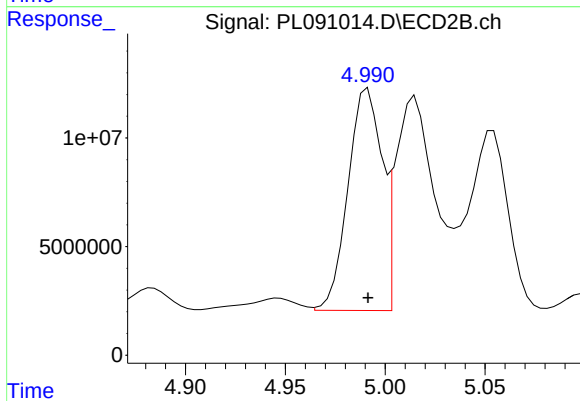

#25 Chlordane-3


R.T.: 4.991 min
Delta R.T.: 0.000 min
Response: 120496106
Conc: 500.00 ng/ml

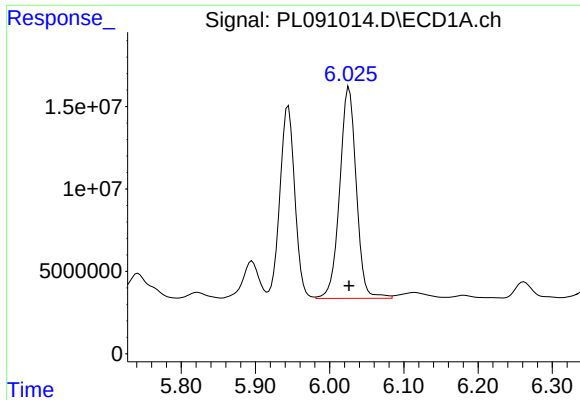

#26 Chlordane-4


R.T.: 6.026 min
Delta R.T.: 0.000 min
Response: 199374468
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

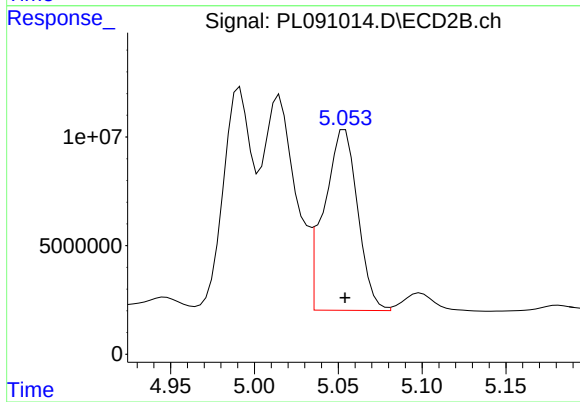


#26 Chlordane-4

R.T.: 5.054 min
Delta R.T.: 0.000 min
Response: 115554515
Conc: 500.00 ng/ml

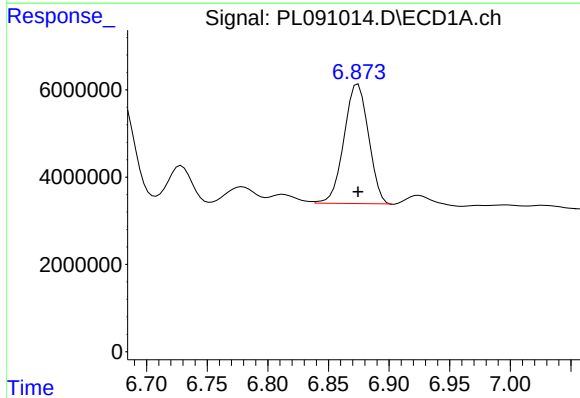


#27 Chlordane-5

R.T.: 6.874 min
Delta R.T.: 0.000 min
Response: 36670029
Conc: 500.00 ng/ml

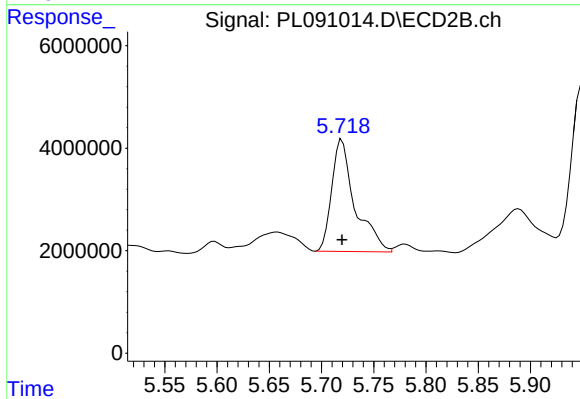

#27 Chlordane-5


R.T.: 5.720 min
Delta R.T.: 0.000 min
Response: 33881030
Conc: 500.00 ng/ml

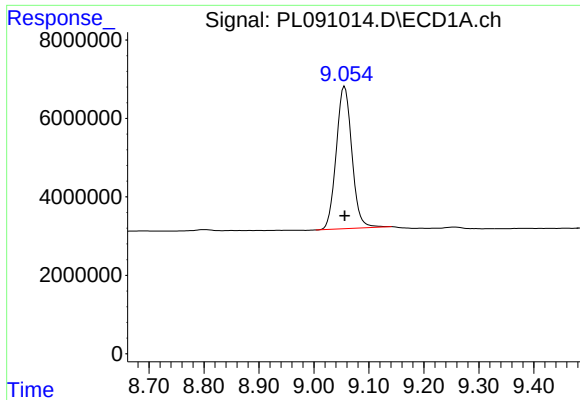

#28 Decachlorobiphenyl

R.T.: 9.056 min
Delta R.T.: 0.000 min
Response: 71795838
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

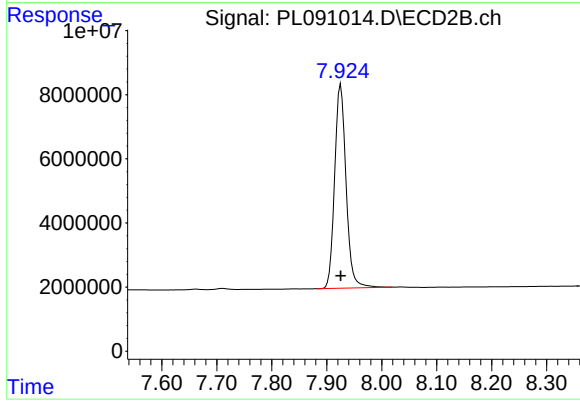

#28 Decachlorobiphenyl

R.T.: 7.925 min
Delta R.T.: 0.000 min
Response: 91765031
Conc: 50.00 ng/ml