

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081324\
 Data File : PL091015.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2024 00:17
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 04:52:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081324.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 14 03:38:39 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.784	52705990	56610160	26.314	24.634
28)	SA Decachlor...	9.055	7.925	39195307	48190874	27.361	26.300
Target Compounds							
23)	Chlordane-1	4.705	3.783	24586655	17806183	268.230	249.468
24)	Chlordane-2	5.234	4.361	26349962	23166447	273.401	258.203
25)	Chlordane-3	5.943	4.991	86098231	58566728	261.429	242.174
26)	Chlordane-4	6.026	5.054	104.9E6	57705410	261.739	249.436
27)	Chlordane-5	6.874	5.719	19874166	17228712	271.481	256.211



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081324\
Data File : PL091015.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2024 00:17
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 04:52:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081324.M
Quant Title : GC Extractables
QLast Update : Wed Aug 14 03:38:39 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

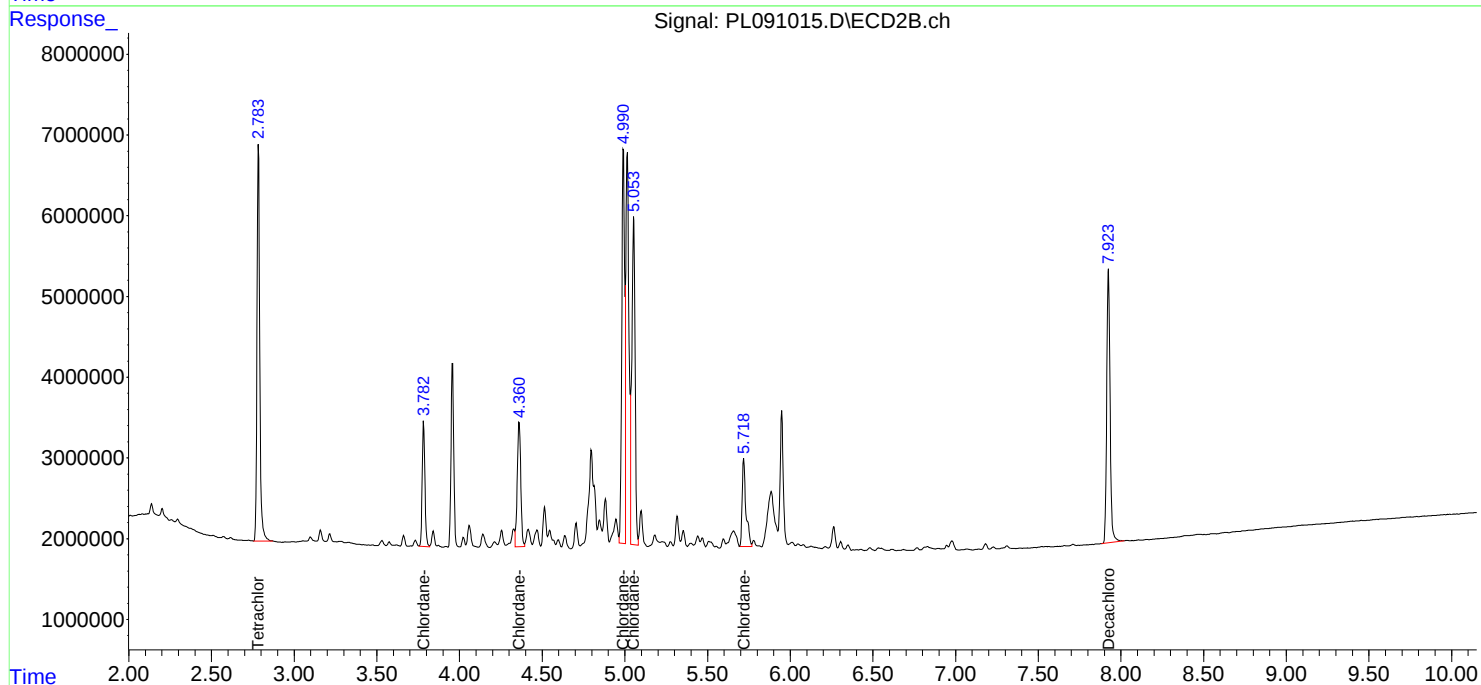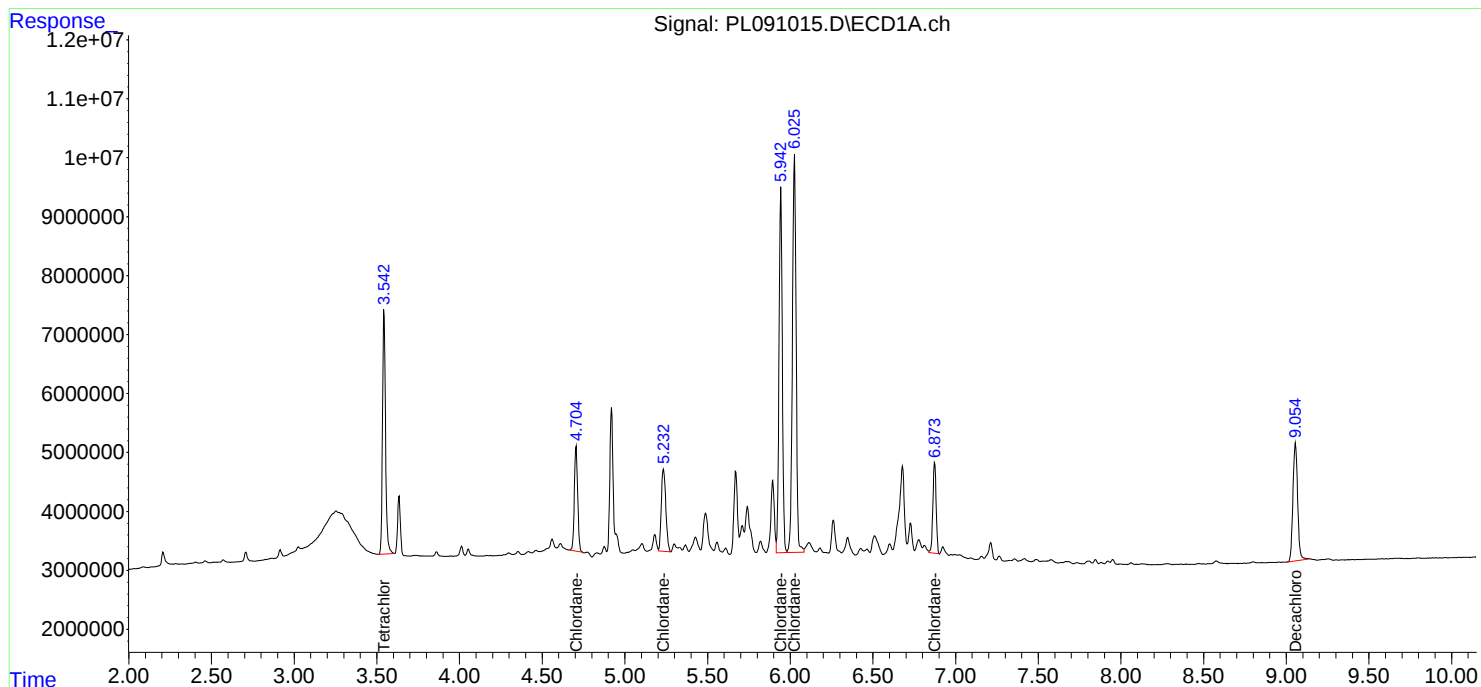


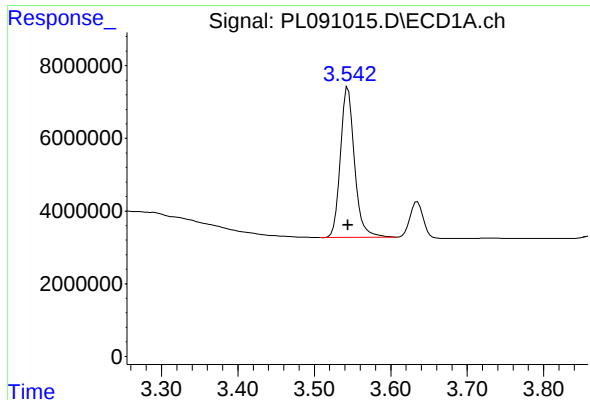

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 52705990
Conc: 26.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

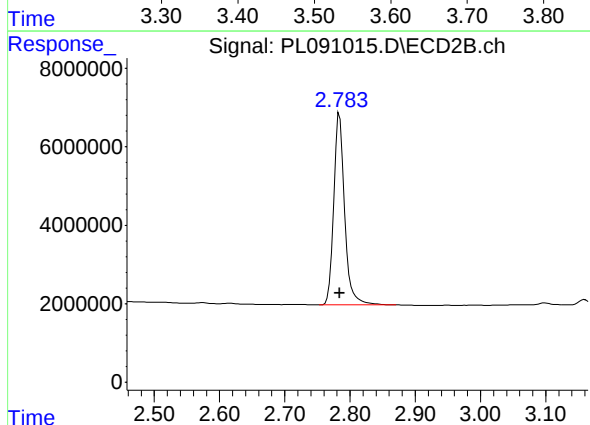


#1 Tetrachloro-m-xylene

R.T.: 2.784 min
Delta R.T.: 0.000 min
Response: 56610160
Conc: 24.63 ng/ml

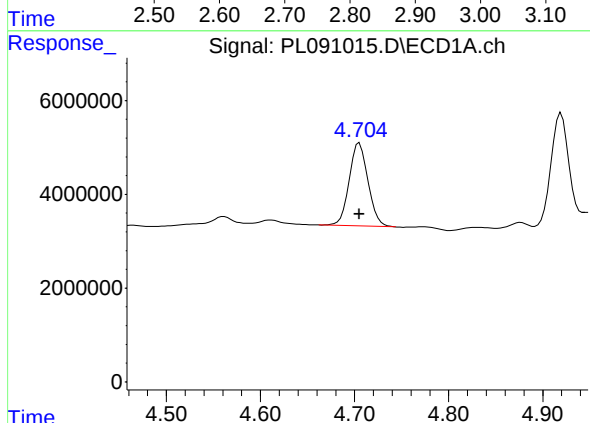


#23 Chlordane-1

R.T.: 4.705 min
Delta R.T.: 0.000 min
Response: 24586655
Conc: 268.23 ng/ml

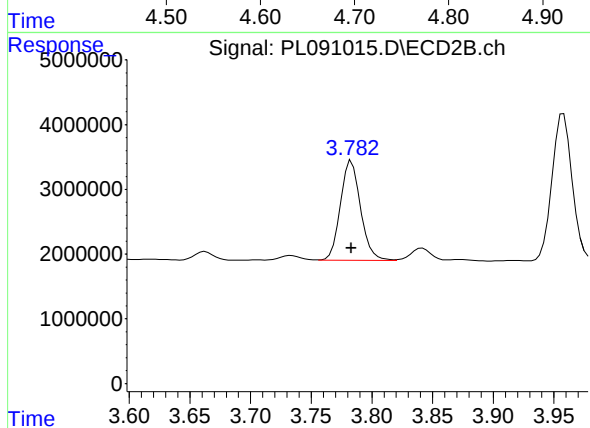

#23 Chlordane-1


R.T.: 3.783 min
Delta R.T.: 0.000 min
Response: 17806183
Conc: 249.47 ng/ml

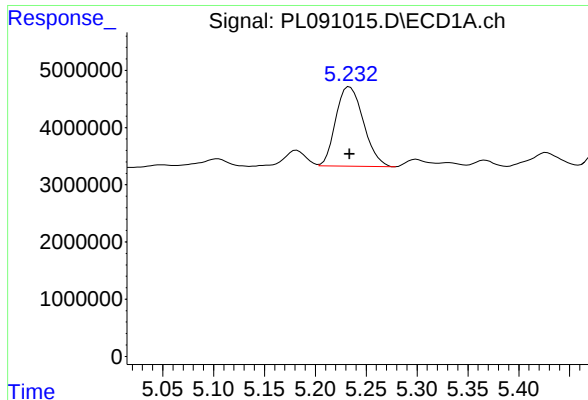

#24 Chlordane-2


R.T.: 5.234 min
Delta R.T.: 0.000 min
Response: 26349962
Conc: 273.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

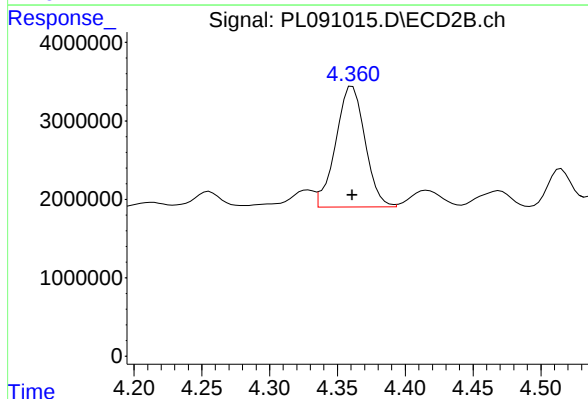


#24 Chlordane-2

R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 23166447
Conc: 258.20 ng/ml

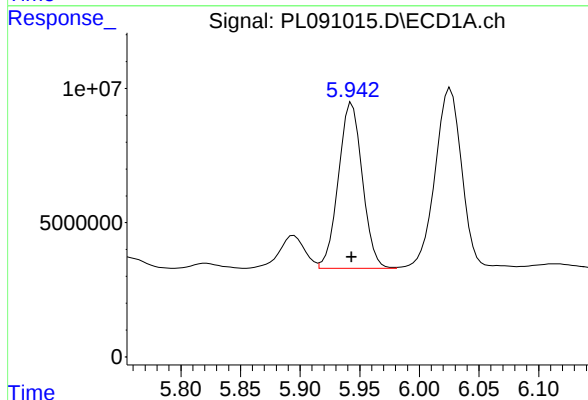


#25 Chlordane-3

R.T.: 5.943 min
Delta R.T.: 0.000 min
Response: 86098231
Conc: 261.43 ng/ml

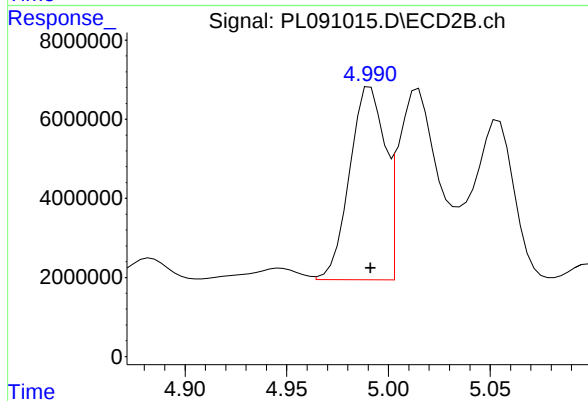

#25 Chlordane-3


R.T.: 4.991 min
Delta R.T.: 0.000 min
Response: 58566728
Conc: 242.17 ng/ml

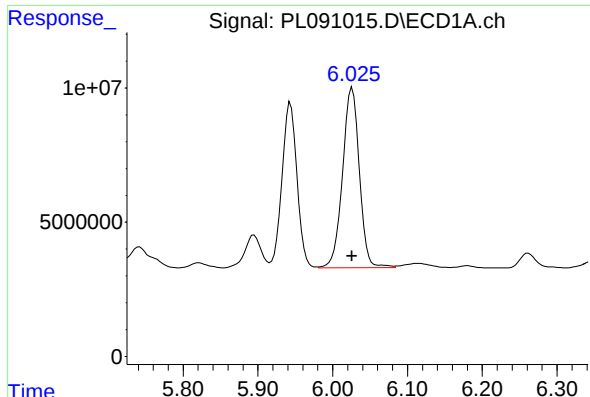

#26 Chlordane-4


R.T.: 6.026 min
Delta R.T.: 0.000 min
Response: 104922376
Conc: 261.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

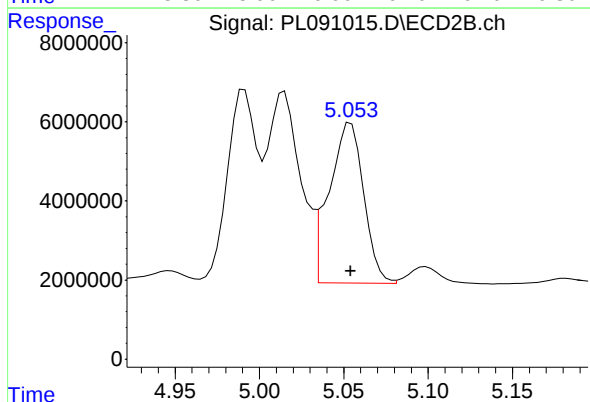


#26 Chlordane-4

R.T.: 5.054 min
Delta R.T.: 0.000 min
Response: 57705410
Conc: 249.44 ng/ml

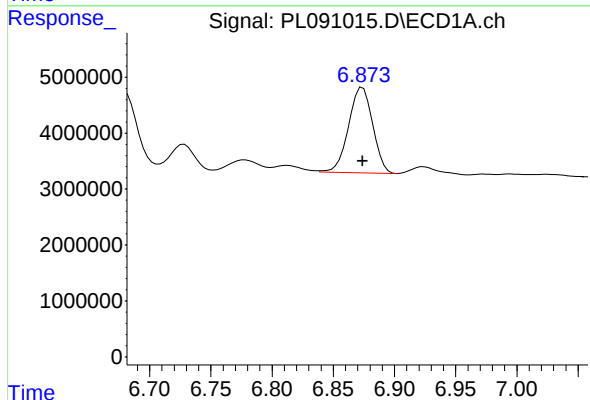


#27 Chlordane-5

R.T.: 6.874 min
Delta R.T.: 0.000 min
Response: 19874166
Conc: 271.48 ng/ml

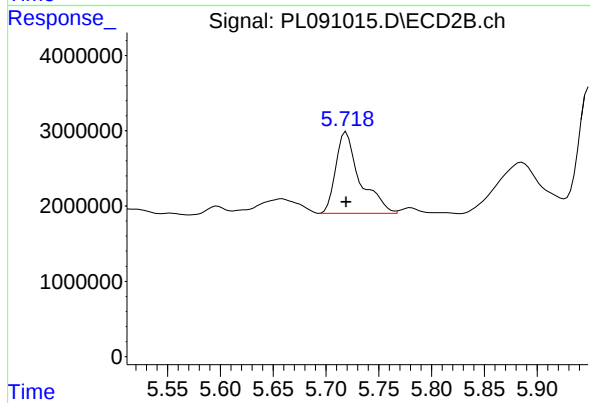

#27 Chlordane-5


R.T.: 5.719 min
Delta R.T.: 0.000 min
Response: 17228712
Conc: 256.21 ng/ml

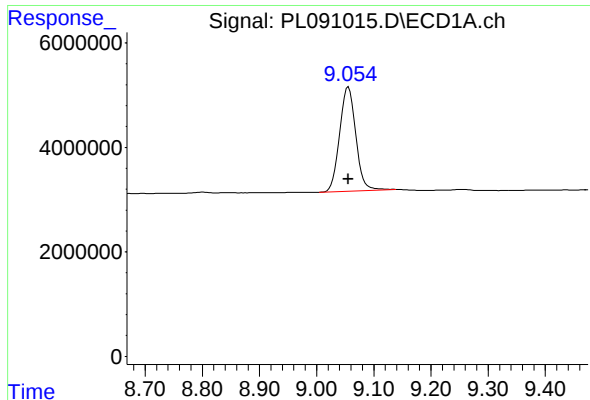

#28 Decachlorobiphenyl

R.T.: 9.055 min
Delta R.T.: 0.000 min
Response: 39195307
Conc: 27.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

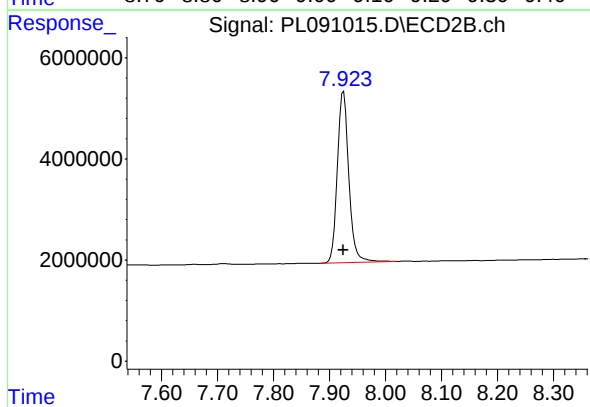

#28 Decachlorobiphenyl

R.T.: 7.925 min
Delta R.T.: 0.000 min
Response: 48190874
Conc: 26.30 ng/ml