

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081419\
 Data File : PL051450.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2019 08:44
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 08:58:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds									
10)	B	gamma-Chl...	5.197	0.000	3524440	0	0.223	N.D.	#
12)	B	4,4'-DDE	5.447f	0.000	22408571	0	1.495	N.D.	#
13)	MA	Dieldrin	5.530f	0.000	26283112	0	1.696	N.D.	#
16)	A	4,4'-DDD	5.940	0.000	7926029	0	0.661	N.D.	#
17)	MA	4,4'-DDT	6.166	0.000	228.9E6	0	18.482	N.D.	#
18)	B	Endrin al...	6.245	0.000	24744004	0	2.145	N.D.	#
21)	B	Endrin ke...	6.924	0.000	112.2E6	0	8.202	N.D.	#
24)		Chlordane-2	4.671f	0.000	75987249	0	169.764	N.D.	#
25)		Chlordane-3	5.197	0.000	3524440	0	2.518	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081419\
Data File : PL051450.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2019 08:44
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 08:58:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

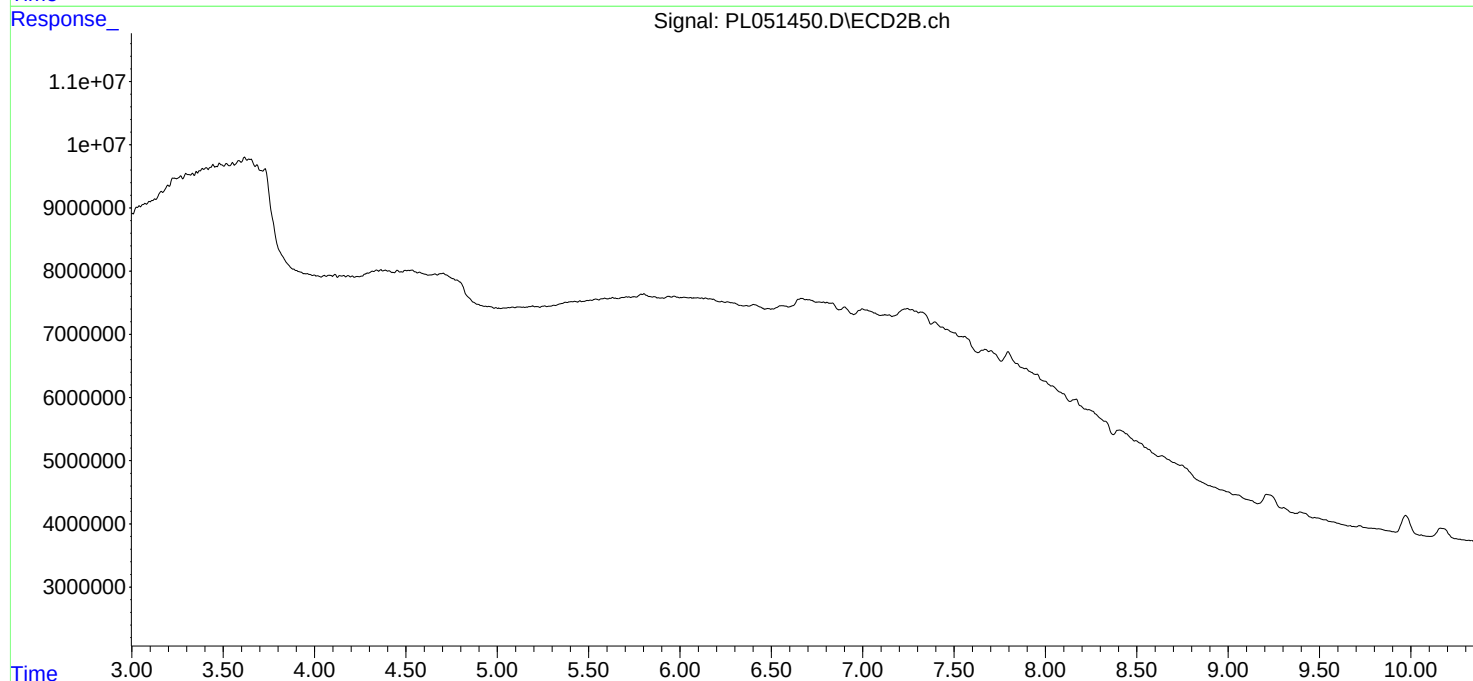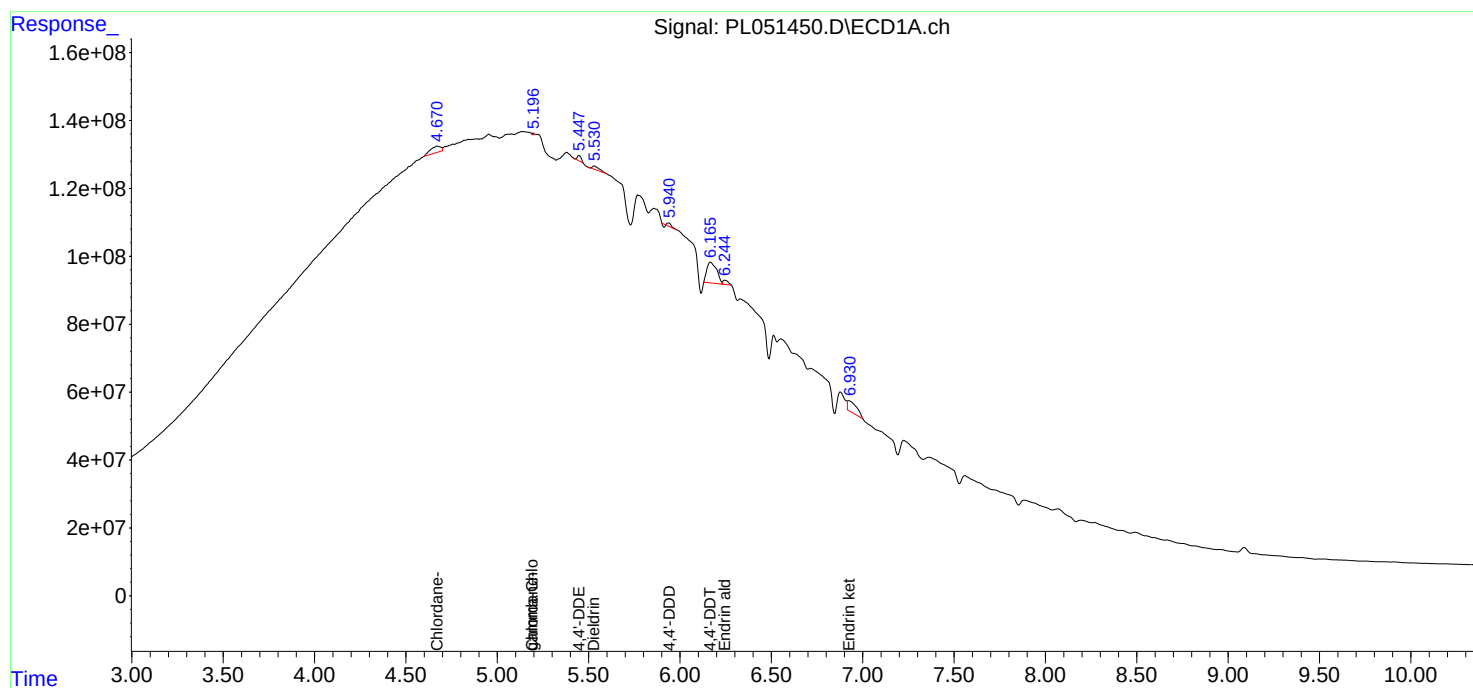


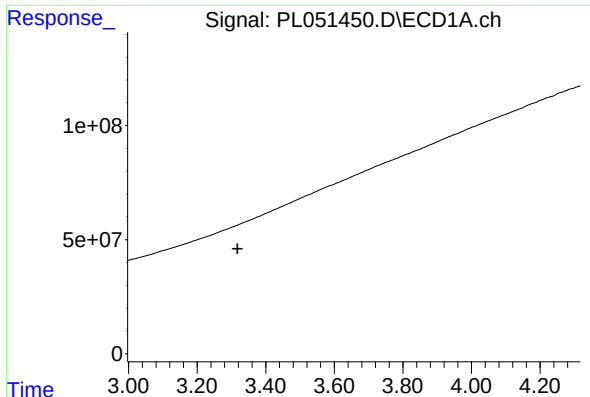

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.318 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

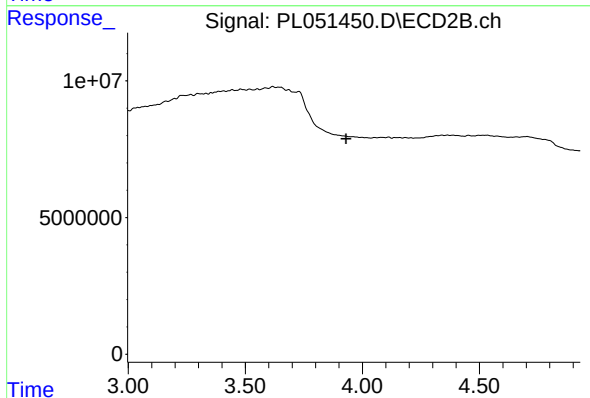


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.931 min
Response: 0
Conc: N.D.

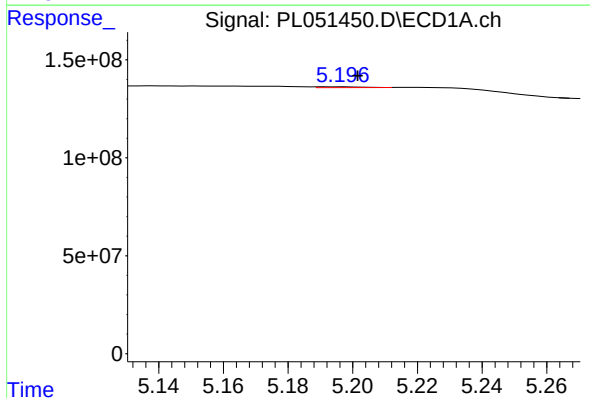


#10 gamma-Chlordane

R.T.: 5.197 min
Delta R.T.: -0.004 min
Response: 3524440
Conc: 0.22 ng/ml

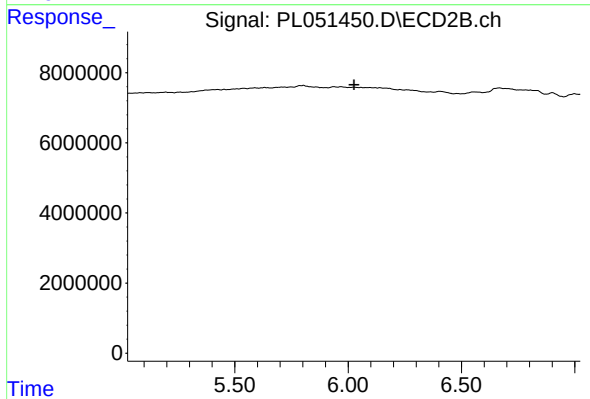

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.026 min
Response: 0
Conc: N.D.

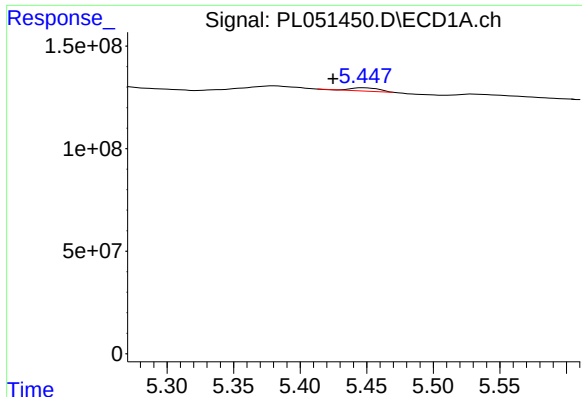

#12 4,4'-DDE


R.T.: 5.447 min
Delta R.T.: 0.023 min
Response: 22408571
Conc: 1.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

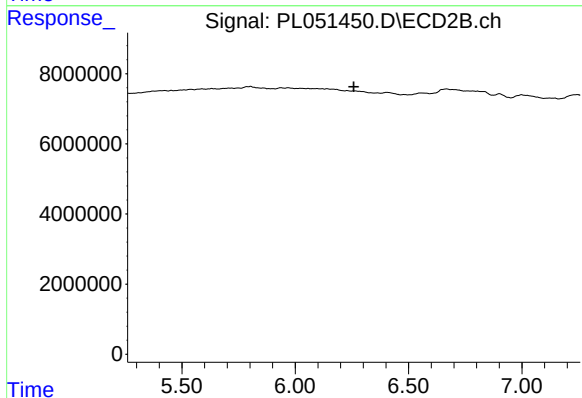


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.258 min
Response: 0
Conc: N.D.

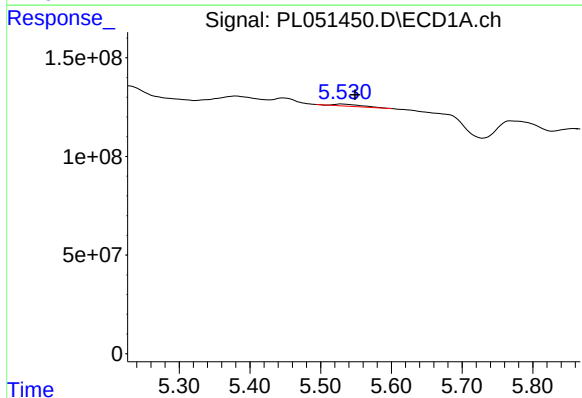


#13 Dieldrin

R.T.: 5.530 min
Delta R.T.: -0.019 min
Response: 26283112
Conc: 1.70 ng/ml

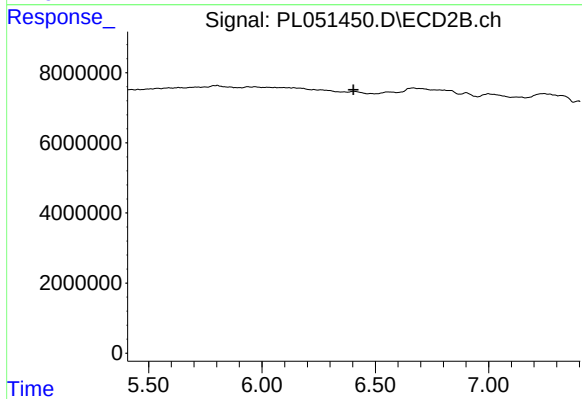

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.404 min
Response: 0
Conc: N.D.

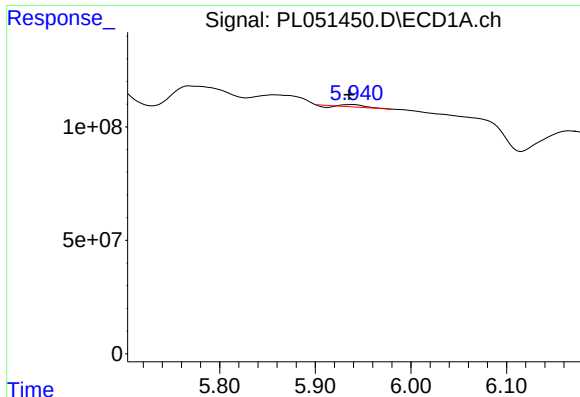

#16 4,4'-DDD


R.T.: 5.940 min
Delta R.T.: 0.004 min
Response: 7926029
Conc: 0.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

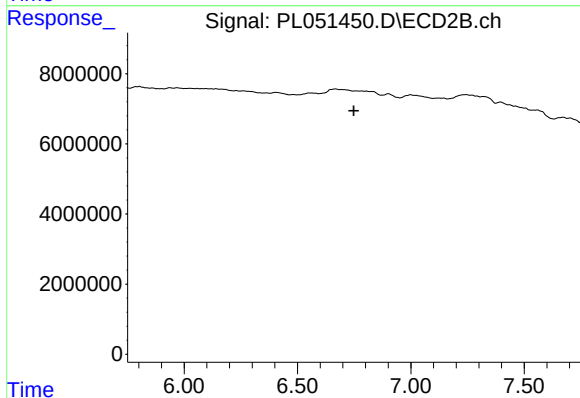


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.749 min
Response: 0
Conc: N.D.

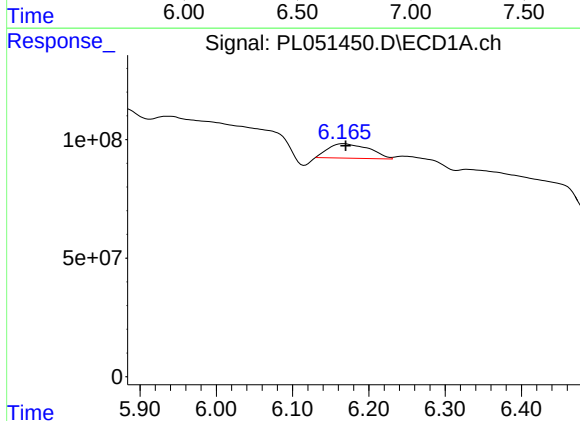


#17 4,4'-DDT

R.T.: 6.166 min
Delta R.T.: -0.003 min
Response: 228919125
Conc: 18.48 ng/ml

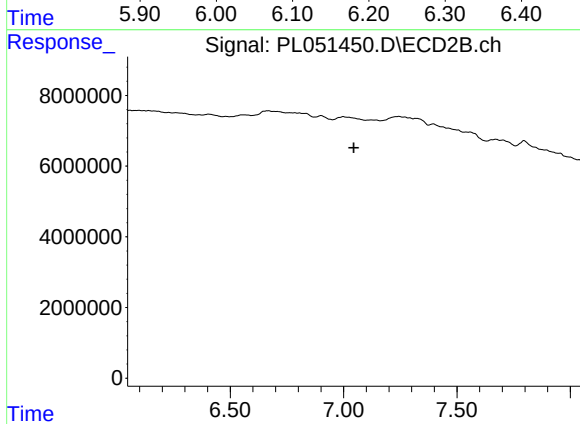

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.046 min
Response: 0
Conc: N.D.

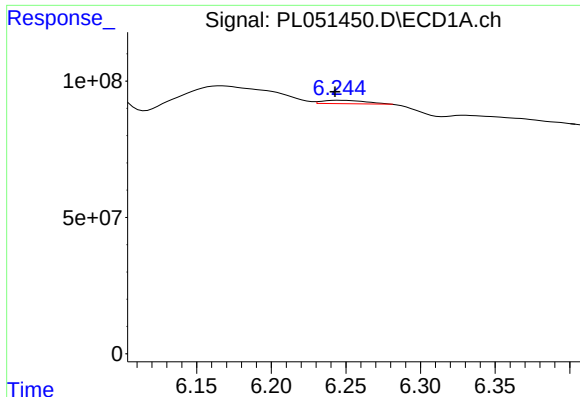

#18 Endrin aldehyde


R.T.: 6.245 min
Delta R.T.: 0.003 min
Response: 24744004
Conc: 2.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

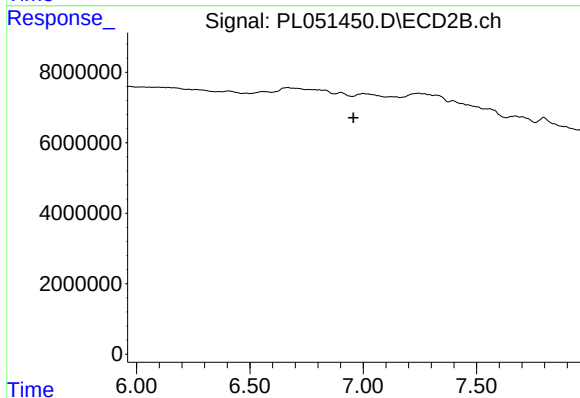


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.957 min
Response: 0
Conc: N.D.

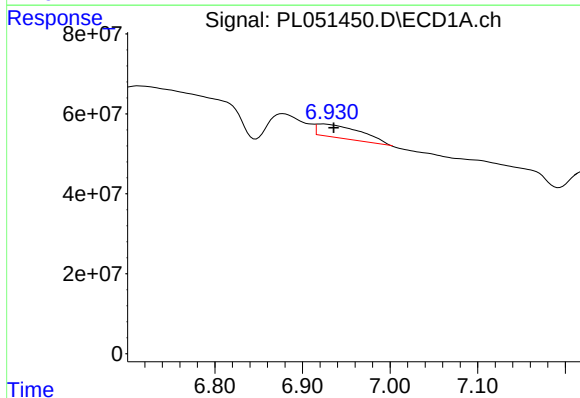


#21 Endrin ketone

R.T.: 6.924 min
Delta R.T.: -0.011 min
Response: 112183931
Conc: 8.20 ng/ml

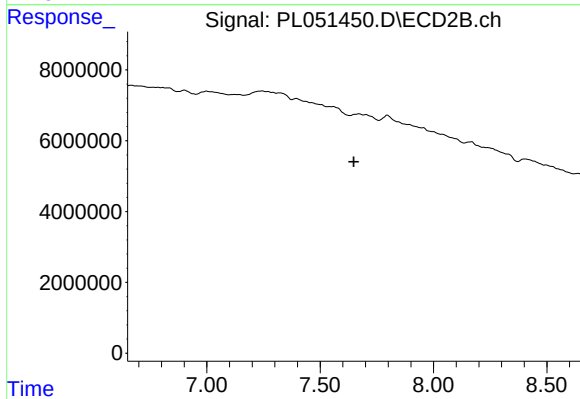

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.648 min
Response: 0
Conc: N.D.

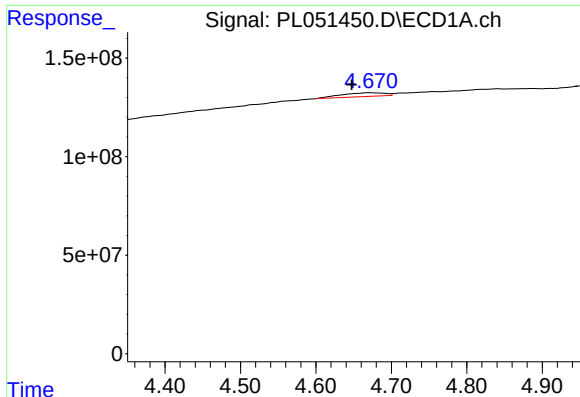

#24 Chlordane-2


R.T.: 4.671 min
Delta R.T.: 0.024 min
Response: 75987249
Conc: 169.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

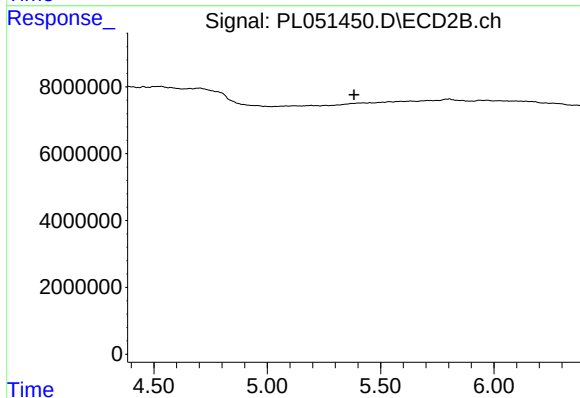


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.383 min
Response: 0
Conc: N.D.

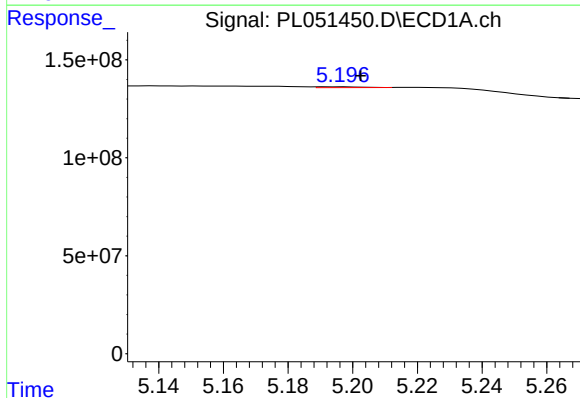


#25 Chlordane-3

R.T.: 5.197 min
Delta R.T.: -0.005 min
Response: 3524440
Conc: 2.52 ng/ml

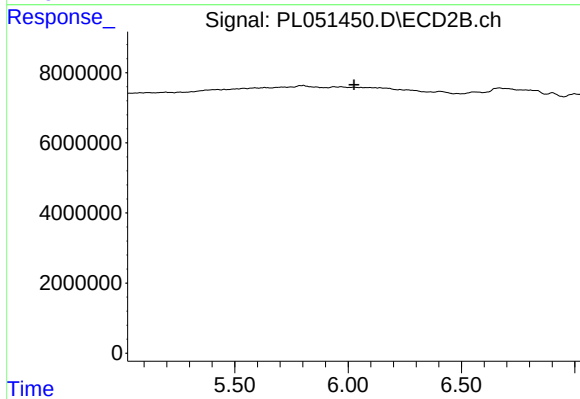

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

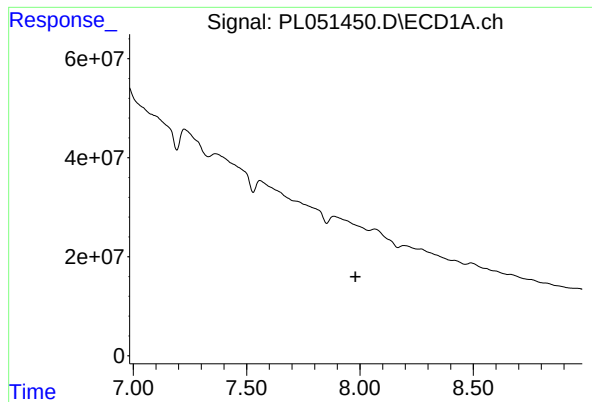

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.981 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

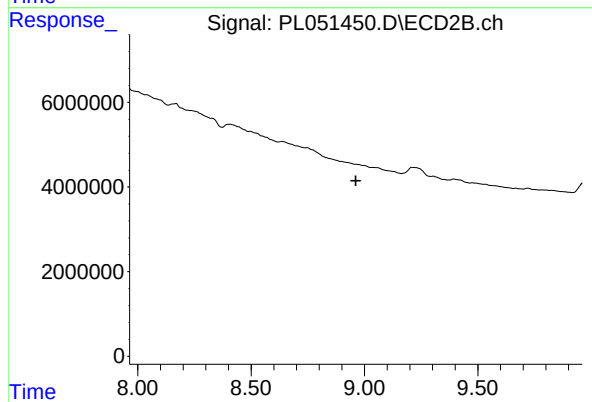

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.962 min
Response: 0
Conc: N.D.