

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081419\
 Data File : PL051475.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2019 15:58
 Operator : SM\AJ
 Sample : K4331-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 0623-FIELD-BLANK-VENICEAN

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 09:08:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	3.927	223.7E6	60668689	22.262	21.263
28)	SA Decachlor...	7.976	8.955	194.2E6	46950642	19.179	16.603
Target Compounds							
5)	MB Aldrin	4.529	0.000	10372112	0	0.670	N.D. #
9)	A Endosulfan I	5.316	6.148	670.7E6	87100645	46.115	25.328 #
16)	A 4,4'-DDD	5.922	0.000	6508707	0	0.543	N.D. #
17)	MA 4,4'-DDT	6.198f	0.000	44658078	0	3.606	N.D. #
18)	B Endrin al...	6.266f	0.000	12163683	0	1.054	N.D. #
19)	B Endosulfa...	6.433f	0.000	21730817	0	1.706	N.D. #
20)	A Methoxychlor	6.731f	0.000	51004396	0	8.175	N.D. #
27)	Chlordane-5	6.083	0.000	52870893	0	104.089	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081419\
Data File : PL051475.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2019 15:58
Operator : SM\AJ
Sample : K4331-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
0623-FIELD-BLANK-VENICEAN

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 09:08:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

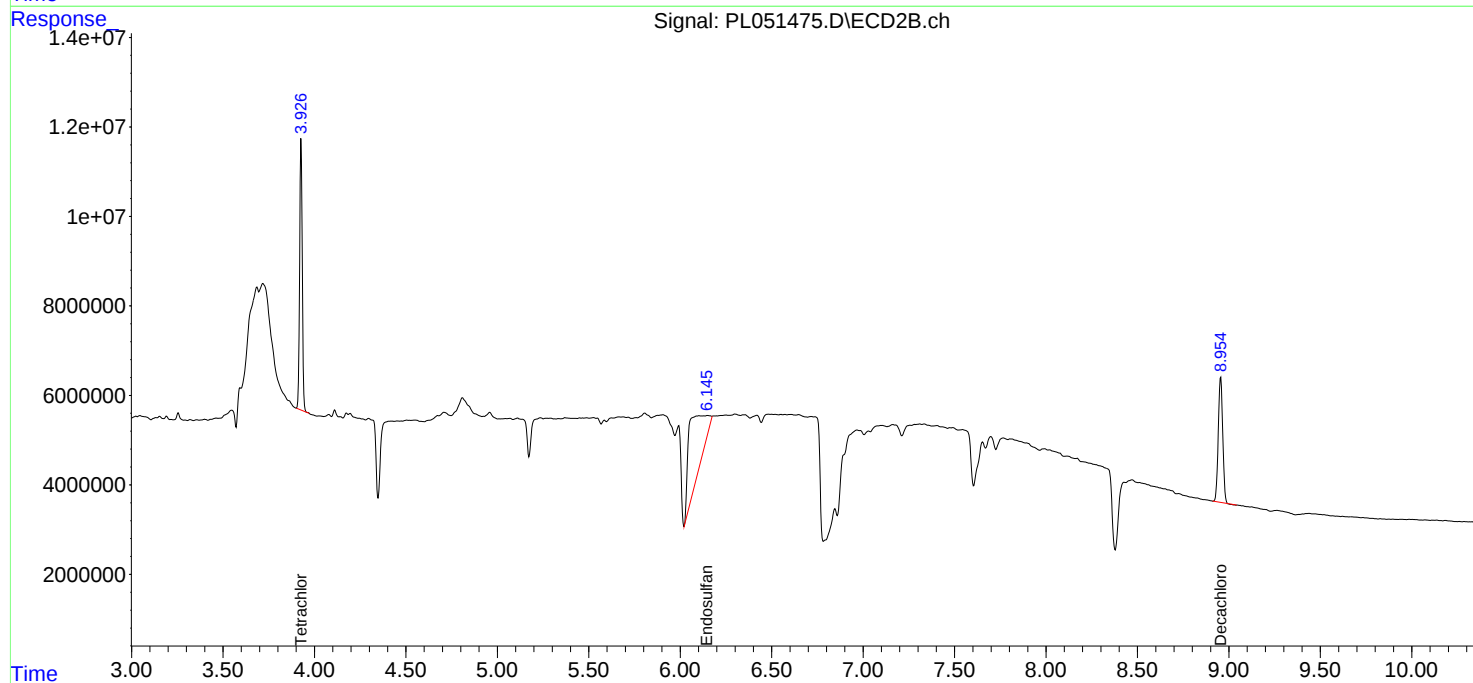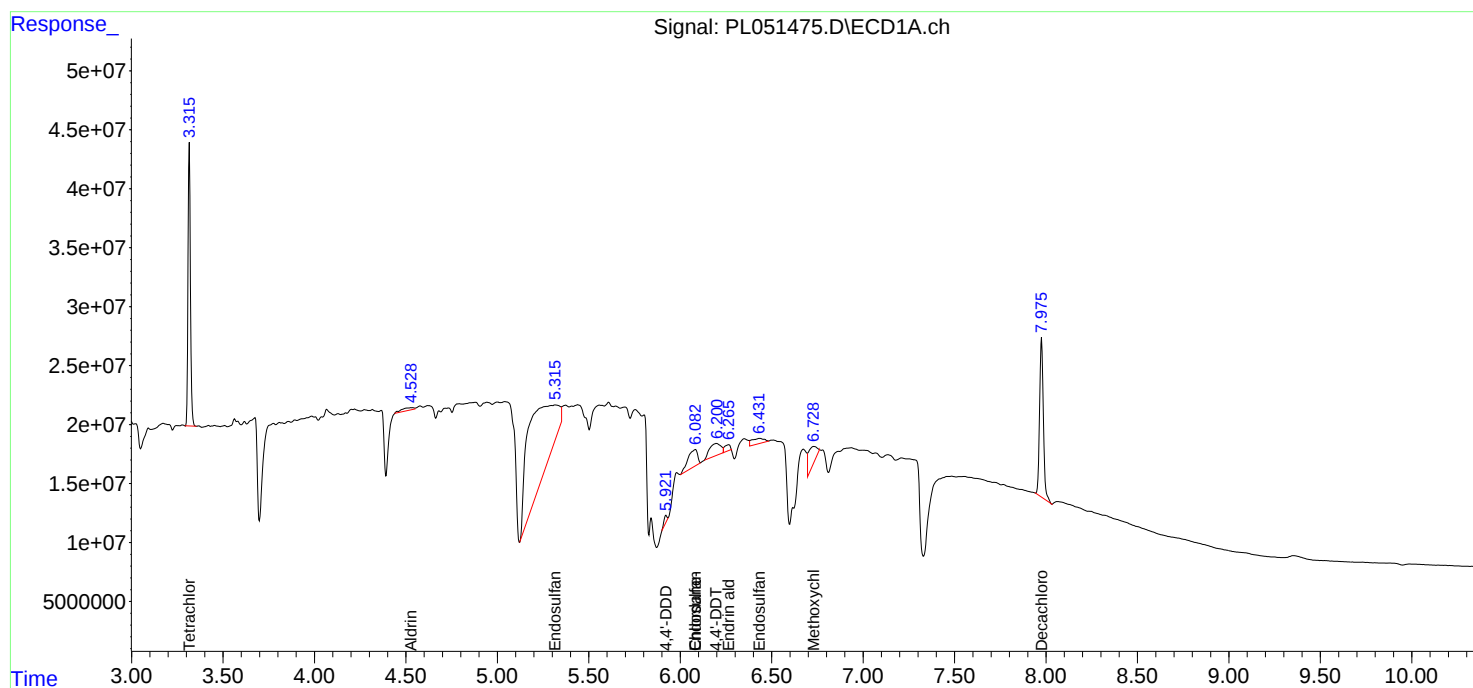


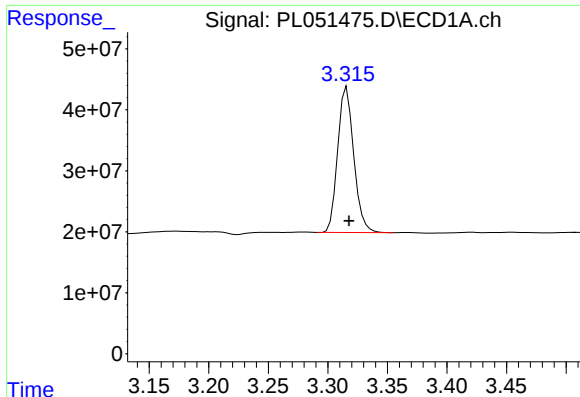

#1 Tetrachloro-m-xylene


R.T.: 3.316 min
Delta R.T.: -0.002 min
Response: 223687026
Conc: 22.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
0623-FIELD-BLANK-VENICEAN

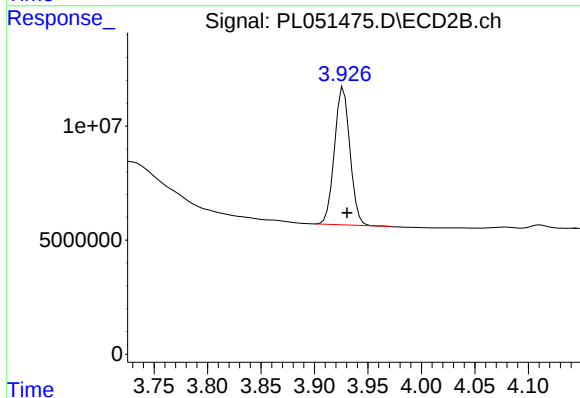


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.003 min
Response: 60668689
Conc: 21.26 ng/ml

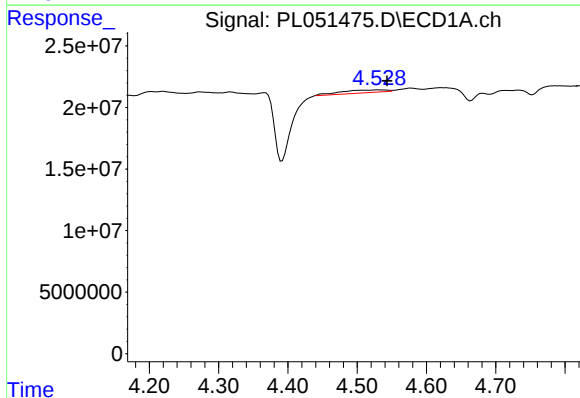


#5 Aldrin

R.T.: 4.529 min
Delta R.T.: -0.014 min
Response: 10372112
Conc: 0.67 ng/ml

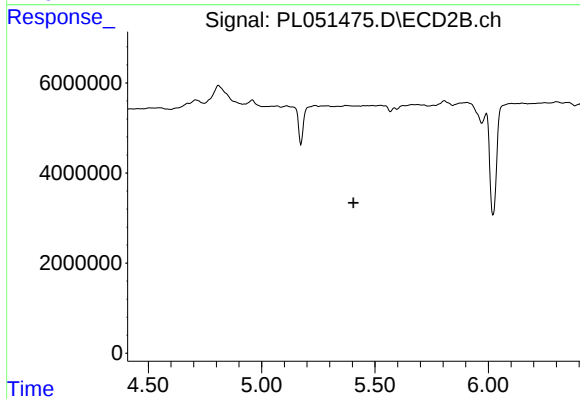

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.405 min
Response: 0
Conc: N.D.

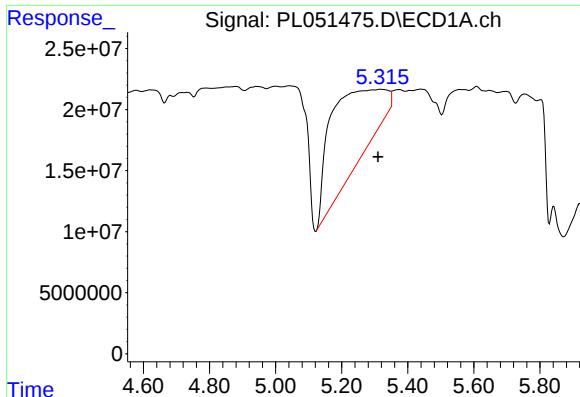

#9 Endosulfan I


R.T.: 5.316 min
Delta R.T.: 0.007 min
Response: 670684624
Conc: 46.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
0623-FIELD-BLANK-VENICEAN

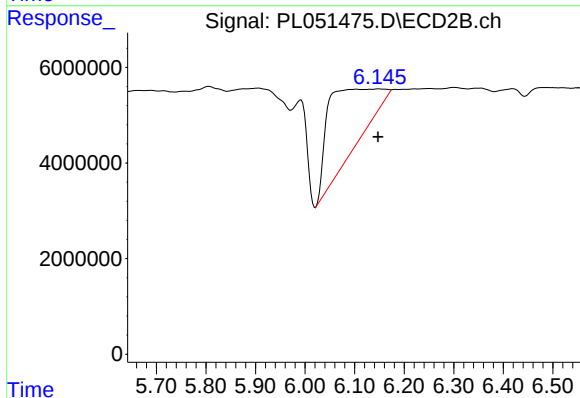


#9 Endosulfan I

R.T.: 6.148 min
Delta R.T.: 0.000 min
Response: 87100645
Conc: 25.33 ng/ml

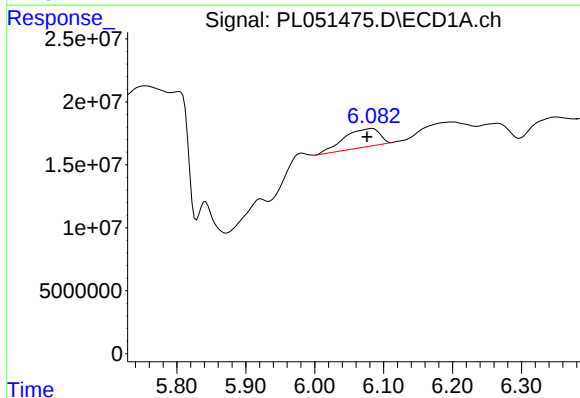


#15 Endosulfan II

R.T.: 6.083 min
Delta R.T.: 0.007 min
Response: 52870893
Conc: 3.78 ng/ml

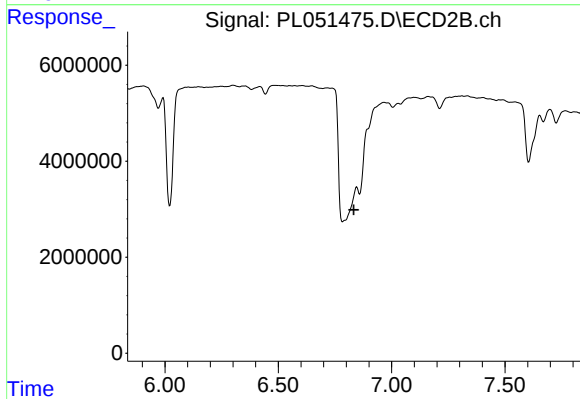

#15 Endosulfan II


R.T.: 6.846 min
Delta R.T.: 0.013 min
Response: -58501136
Conc: N.D.

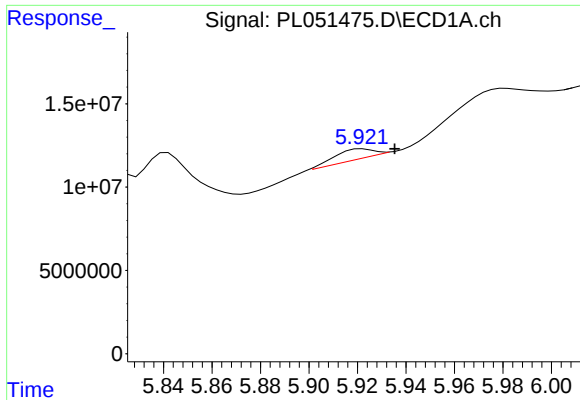

#16 4,4'-DDD


R.T.: 5.922 min
Delta R.T.: -0.013 min
Response: 6508707
Conc: 0.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
0623-FIELD-BLANK-VENICEAN

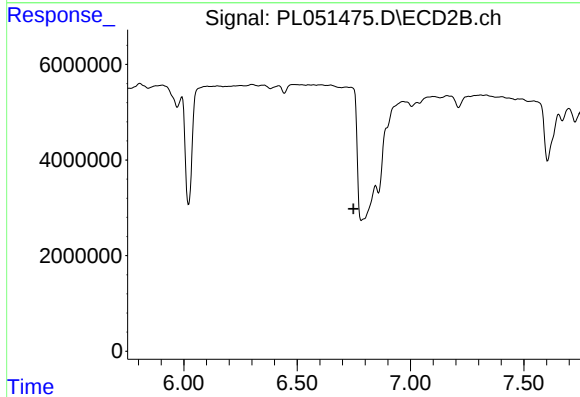


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.749 min
Response: 0
Conc: N.D.

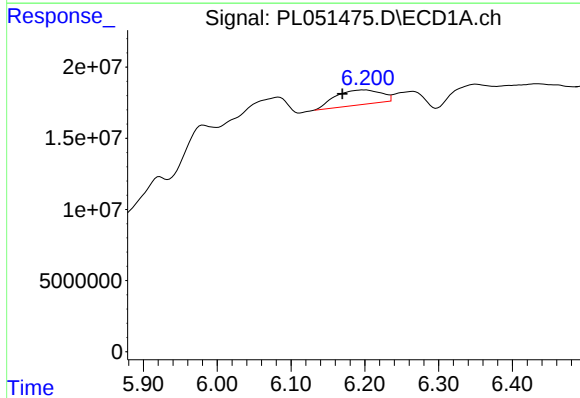


#17 4,4'-DDT

R.T.: 6.198 min
Delta R.T.: 0.028 min
Response: 44658078
Conc: 3.61 ng/ml

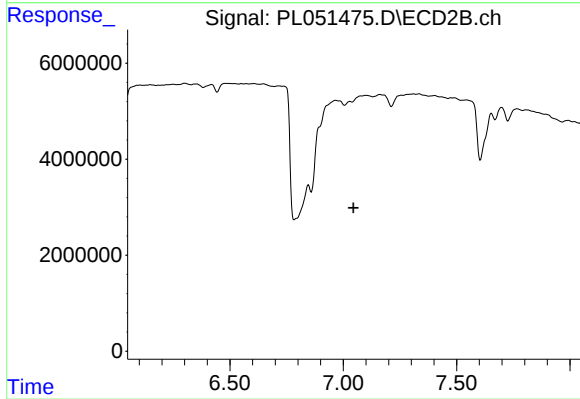

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.046 min
Response: 0
Conc: N.D.

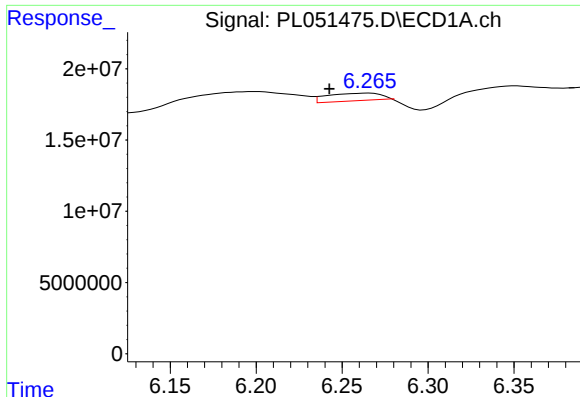

#18 Endrin aldehyde


R.T.: 6.266 min
Delta R.T.: 0.023 min
Response: 12163683
Conc: 1.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
0623-FIELD-BLANK-VENICEAN

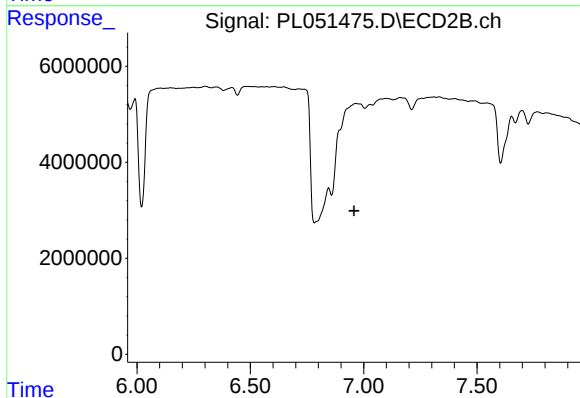


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.957 min
Response: 0
Conc: N.D.

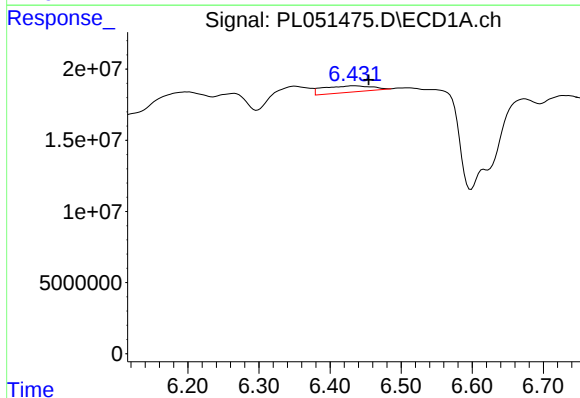


#19 Endosulfan Sulfate

R.T.: 6.433 min
Delta R.T.: -0.021 min
Response: 21730817
Conc: 1.71 ng/ml

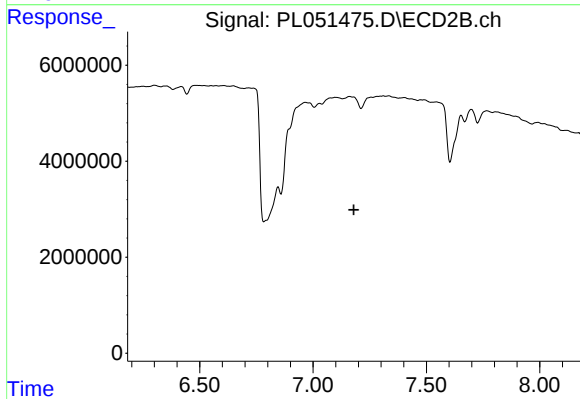

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.180 min
Response: 0
Conc: N.D.

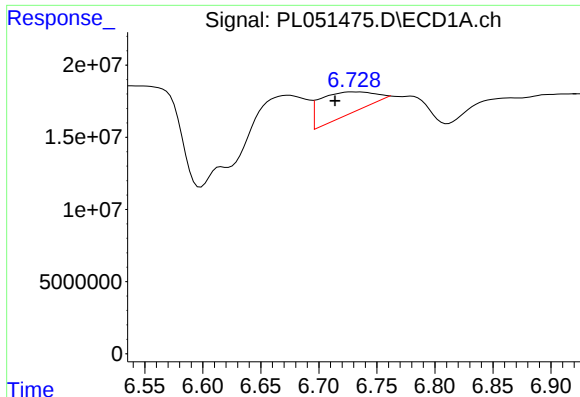

#20 Methoxychlor


R.T.: 6.731 min
Delta R.T.: 0.017 min
Response: 51004396
Conc: 8.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
0623-FIELD-BLANK-VENICEAN

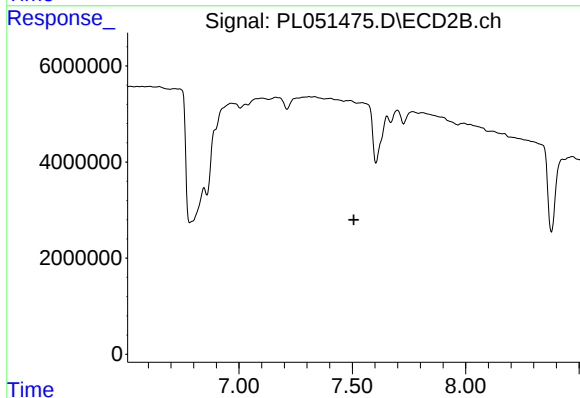


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.507 min
Response: 0
Conc: N.D.

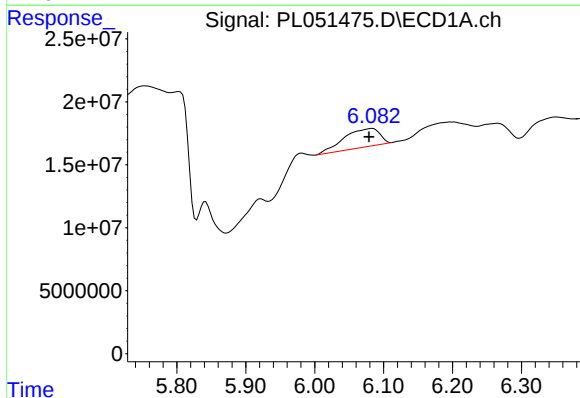


#27 Chlordane-5

R.T.: 6.083 min
Delta R.T.: 0.004 min
Response: 52870893
Conc: 104.09 ng/ml

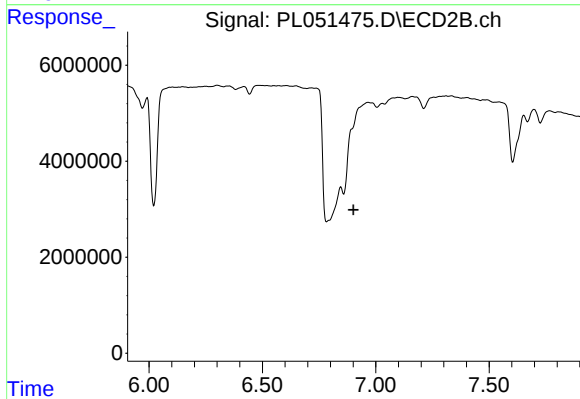

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.902 min
Response: 0
Conc: N.D.

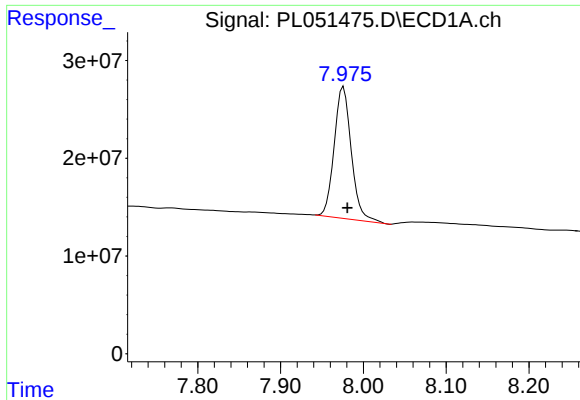

#28 Decachlorobiphenyl

R.T.: 7.976 min
Delta R.T.: -0.005 min
Response: 194189646
Conc: 19.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
0623-FIELD-BLANK-VENICEAN

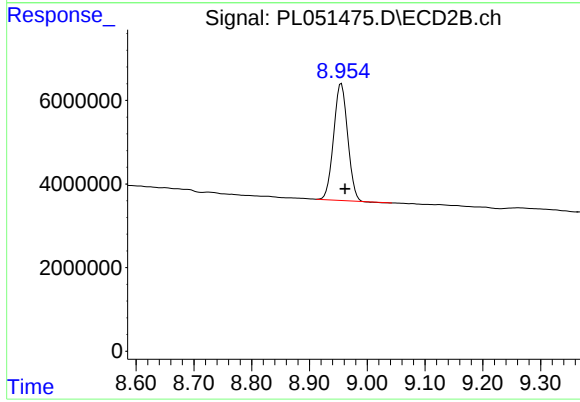

#28 Decachlorobiphenyl

R.T.: 8.955 min
Delta R.T.: -0.006 min
Response: 46950642
Conc: 16.60 ng/ml