

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081419\
 Data File : PL051488.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2019 19:03
 Operator : SM\AJ
 Sample : K4340-03
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 LS-SAMPLE-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 09:12:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	3.927	208.0E6	55341413	20.699	19.396
28)	SA Decachlor...	7.975	8.954	174.0E6	45874427	17.181	16.222
Target Compounds							
6)	B beta-BHC	0.000	4.803f	0	1286560	N.D.	0.744 #
9)	A Endosulfan I	5.332f	0.000	3710920	0	0.255	N.D. #
10)	B gamma-Chl...	5.222f	0.000	34103258	0	2.161	N.D. #
11)	B alpha-Chl...	5.261	0.000	23670723	0	1.552	N.D. #
15)	B Endosulfa...	0.000	6.844	0	6052267	N.D.	1.904 #
22)	Mirex	7.108	0.000	4951156	0	0.505	N.D. #
23)	Chlordane-1	4.167	0.000	2643074	0	7.183	N.D. #
25)	Chlordane-3	5.222f	0.000	34103258	0	24.363	N.D. #
26)	Chlordane-4	5.261	0.000	23670723	0	17.946	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081419\
Data File : PL051488.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2019 19:03
Operator : SM\AJ
Sample : K4340-03
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
LS-SAMPLE-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 09:12:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

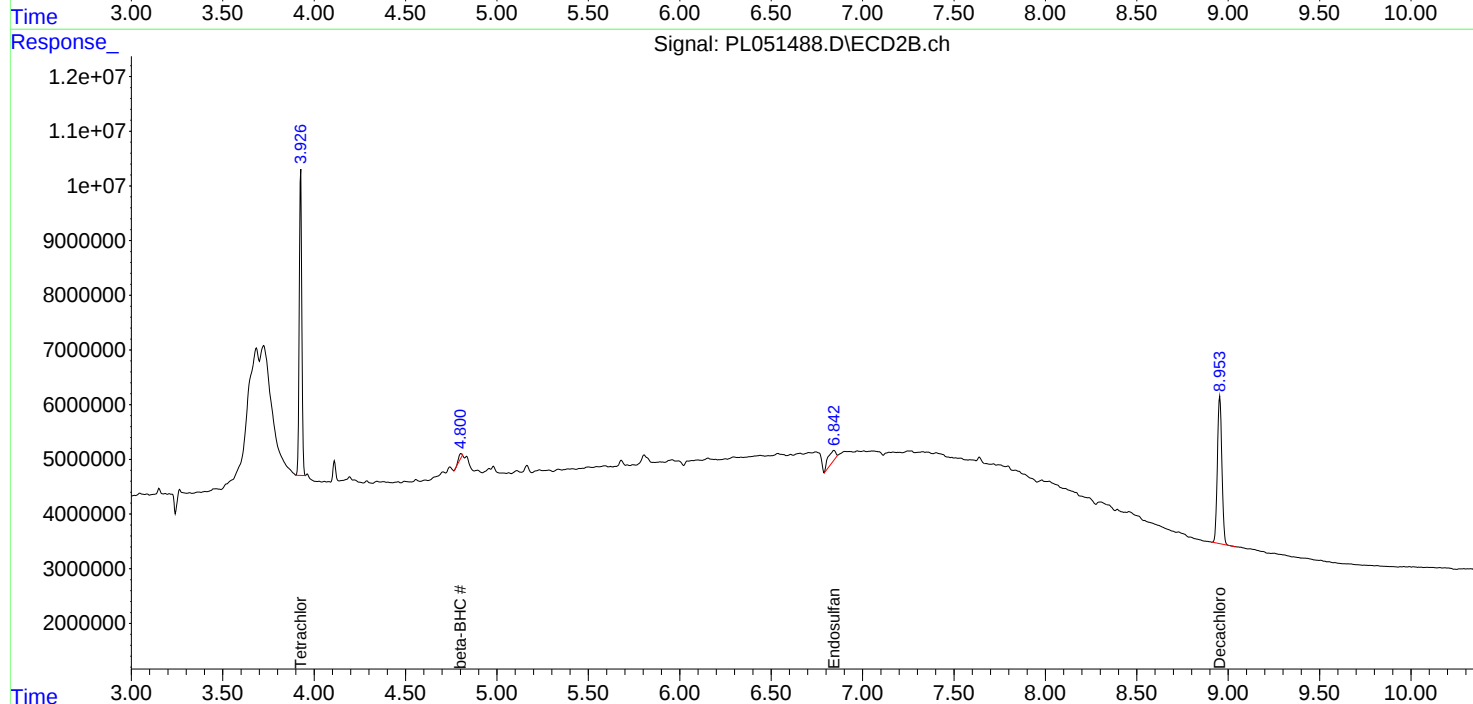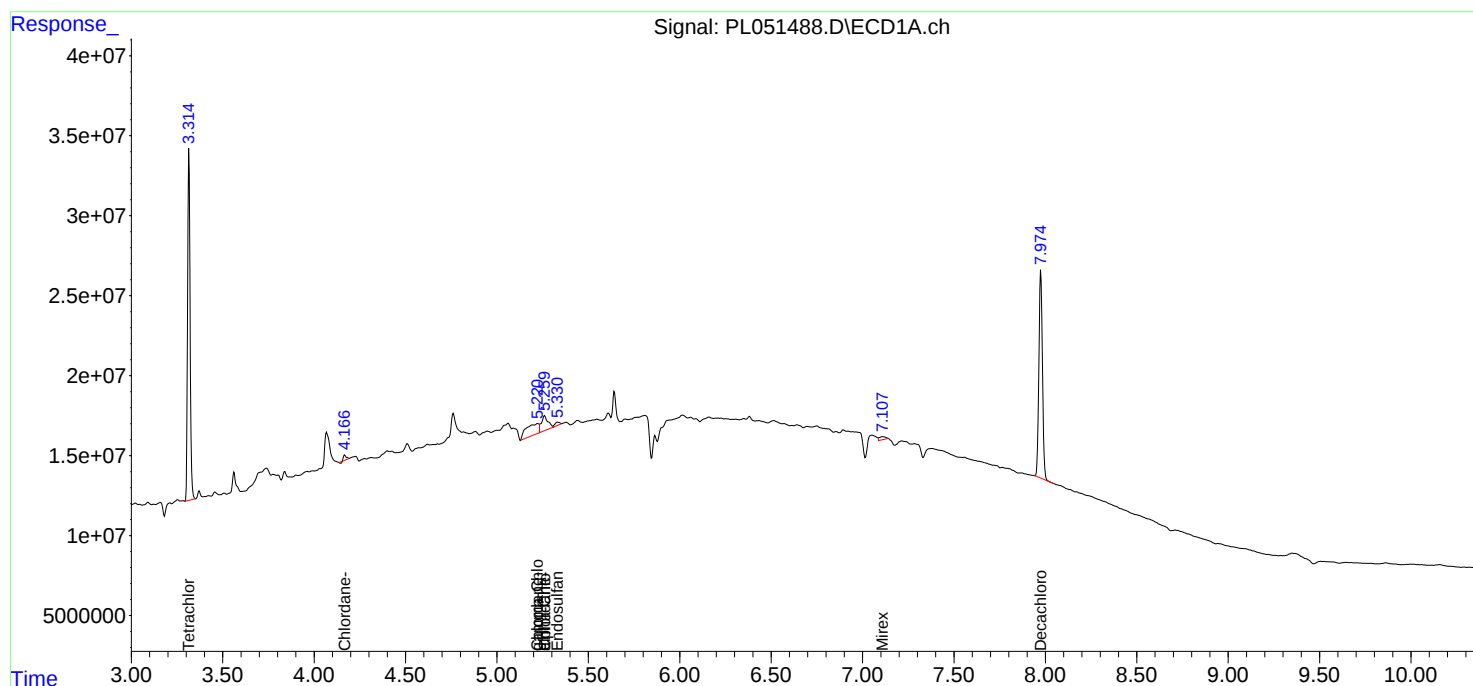


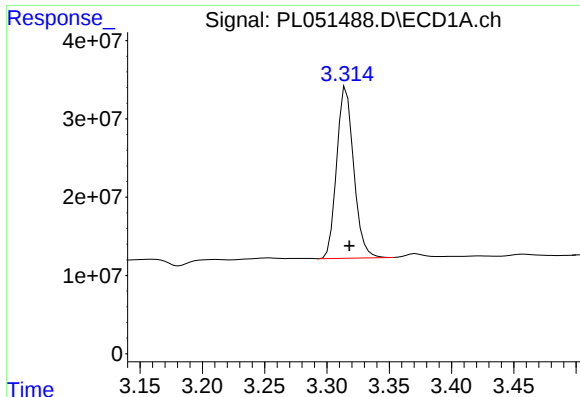

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: -0.003 min
Response: 207978736
Conc: 20.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
LS-SAMPLE-2

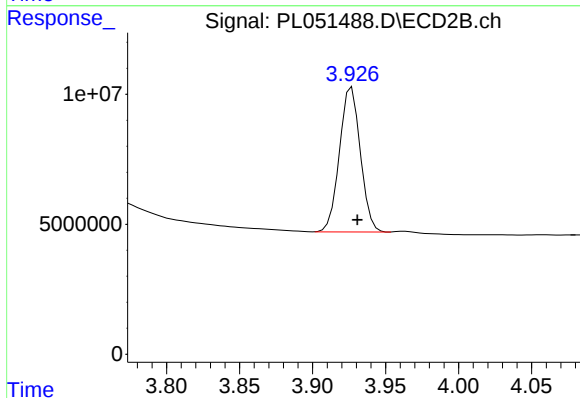


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.004 min
Response: 55341413
Conc: 19.40 ng/ml

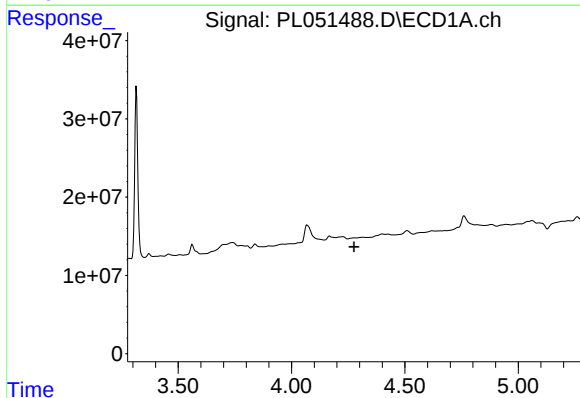


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

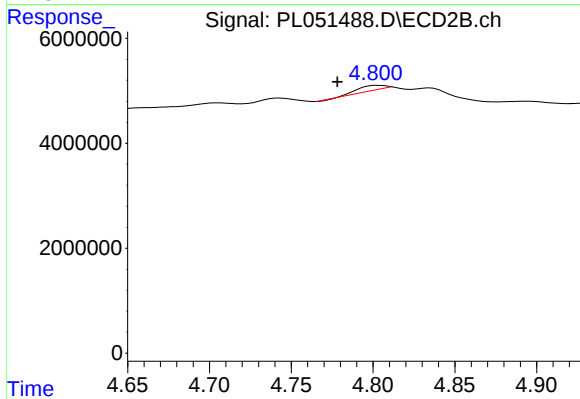

#6 beta-BHC


R.T.: 4.803 min
Delta R.T.: 0.025 min
Response: 1286560
Conc: 0.74 ng/ml

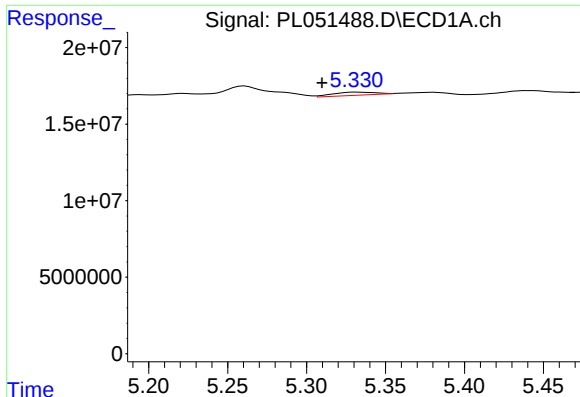

#9 Endosulfan I


R.T.: 5.332 min
Delta R.T.: 0.022 min
Response: 3710920
Conc: 0.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
LS-SAMPLE-2

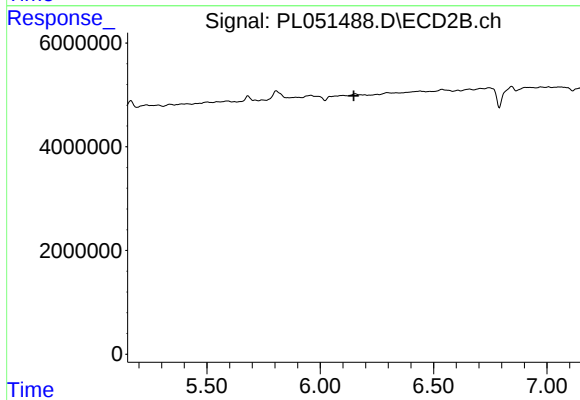


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.148 min
Response: 0
Conc: N.D.

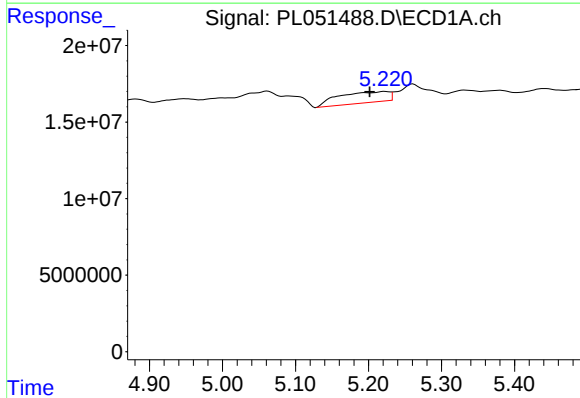


#10 gamma-Chlordane

R.T.: 5.222 min
Delta R.T.: 0.021 min
Response: 34103258
Conc: 2.16 ng/ml

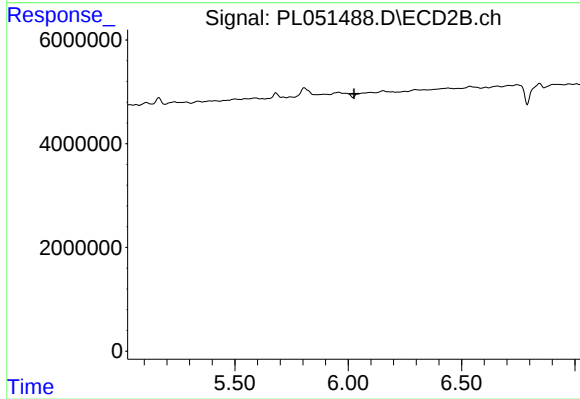

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

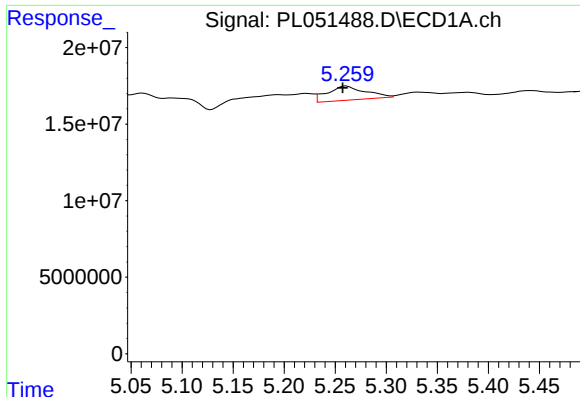

#11 alpha-Chlordane


R.T.: 5.261 min
Delta R.T.: 0.003 min
Response: 23670723
Conc: 1.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
LS-SAMPLE-2

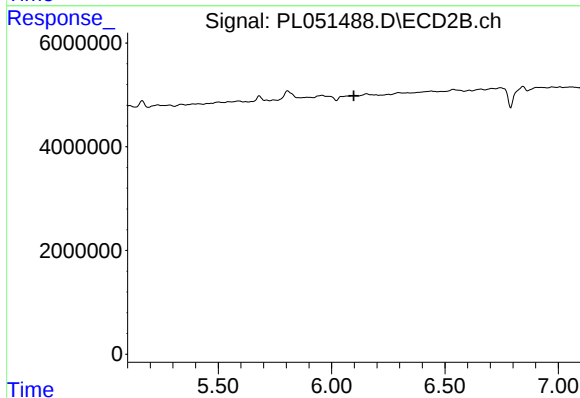


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

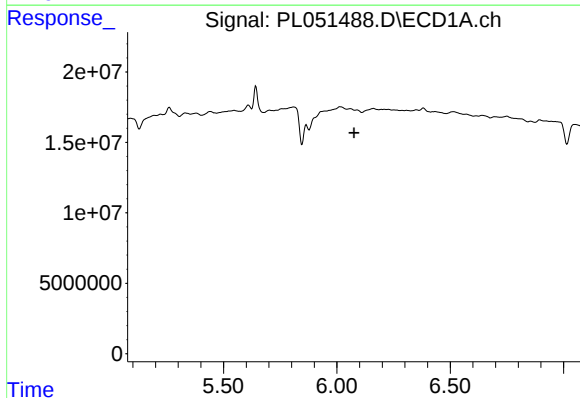


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.076 min
Response: 0
Conc: N.D.

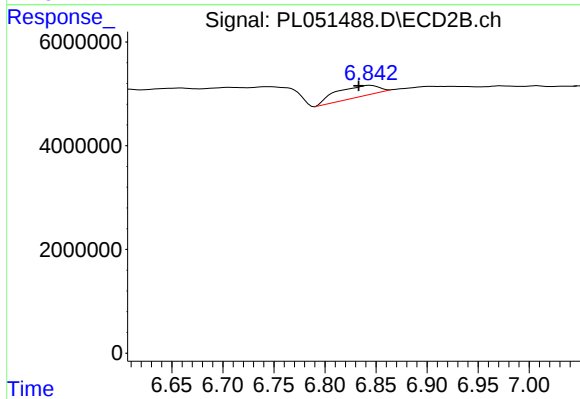

#15 Endosulfan II


R.T.: 6.844 min
Delta R.T.: 0.011 min
Response: 6052267
Conc: 1.90 ng/ml

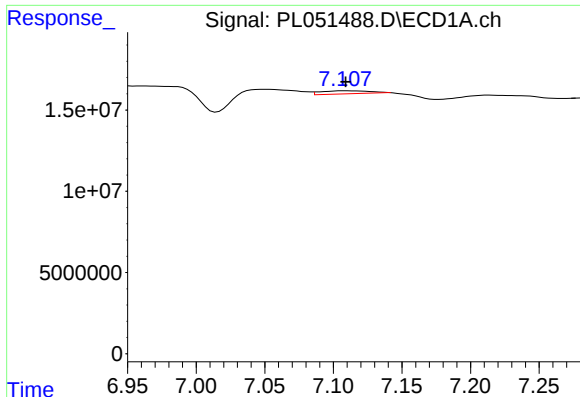

#22 Mirex


R.T.: 7.108 min
Delta R.T.: 0.000 min
Response: 4951156
Conc: 0.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
LS-SAMPLE-2

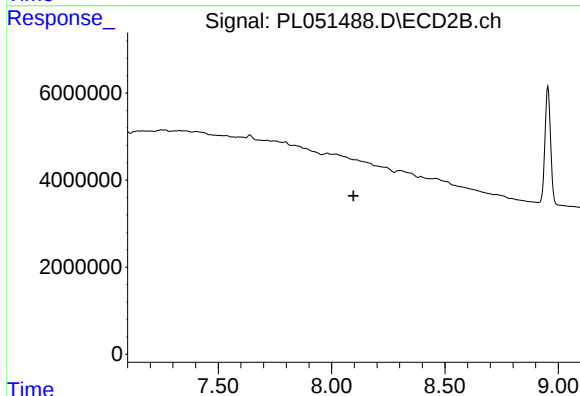


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.097 min
Response: 0
Conc: N.D.

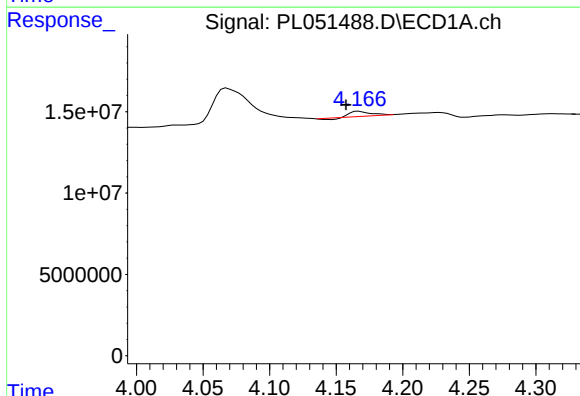


#23 Chlordane-1

R.T.: 4.167 min
Delta R.T.: 0.010 min
Response: 2643074
Conc: 7.18 ng/ml

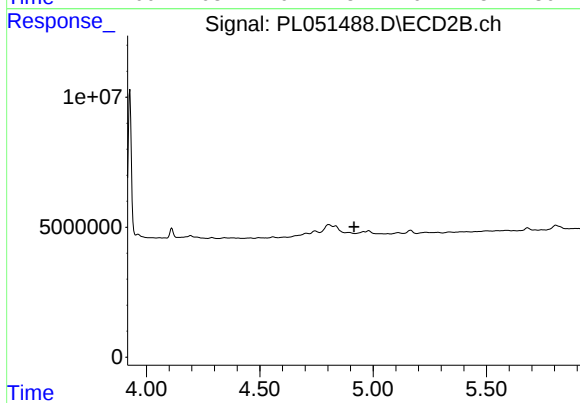

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.916 min
Response: 0
Conc: N.D.

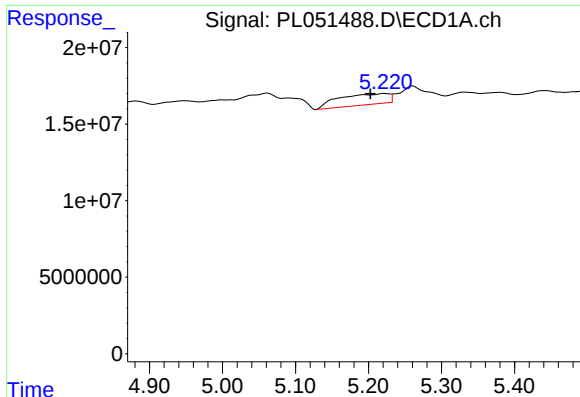

#25 Chlordane-3


R.T.: 5.222 min
Delta R.T.: 0.020 min
Response: 34103258
Conc: 24.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
LS-SAMPLE-2

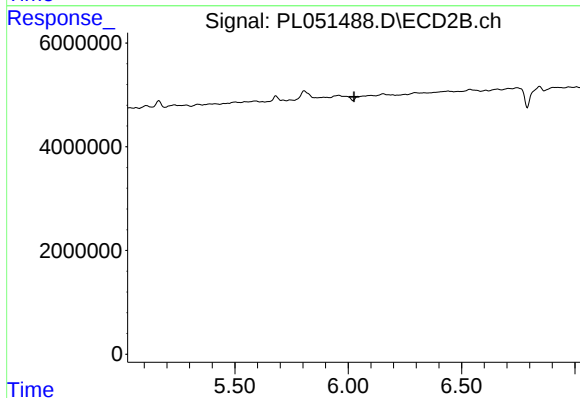


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

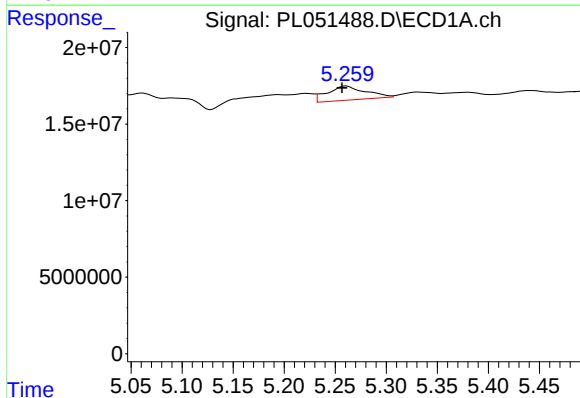


#26 Chlordane-4

R.T.: 5.261 min
Delta R.T.: 0.004 min
Response: 23670723
Conc: 17.95 ng/ml

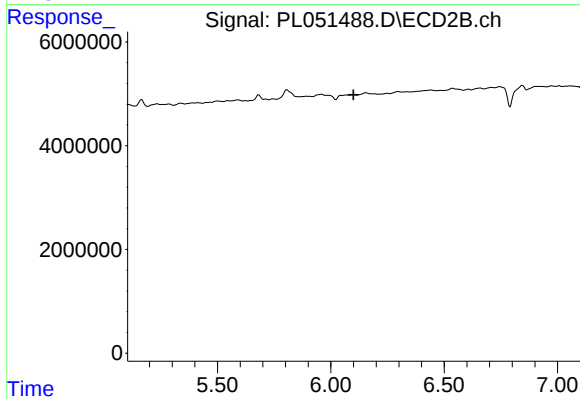

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.100 min
Response: 0
Conc: N.D.

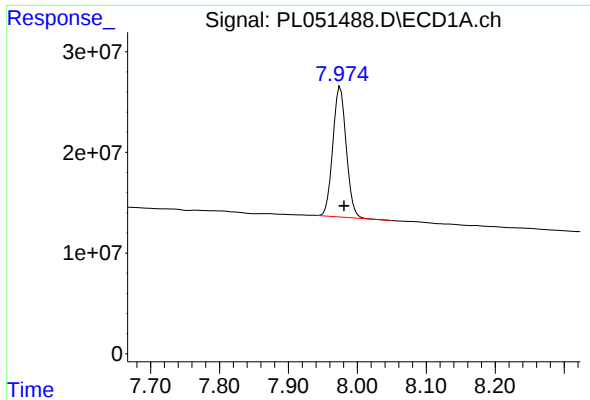

#28 Decachlorobiphenyl

R.T.: 7.975 min
Delta R.T.: -0.005 min
Response: 173958696
Conc: 17.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
LS-SAMPLE-2

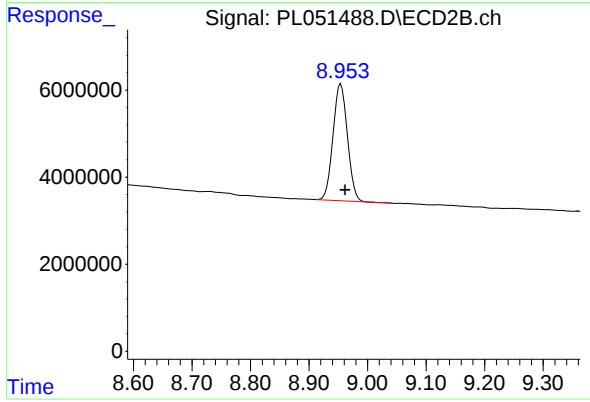

#28 Decachlorobiphenyl

R.T.: 8.954 min
Delta R.T.: -0.007 min
Response: 45874427
Conc: 16.22 ng/ml