

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081419\
 Data File : PL051505.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2019 23:04
 Operator : SM\AJ
 Sample : K4325-02
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20190612-LOC-14

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 09:16:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	3.927	234.4E6	68535430	23.325	24.020
28)	SA Decachlor...	7.974	8.954	274.4E6	70318392	27.101	24.866
Target Compounds							
5)	MB Aldrin	4.557	0.000	3647688	0	0.235	N.D. #
6)	B beta-BHC	0.000	4.769	0	23564714	N.D.	13.630 #
8)	B Heptachlo...	0.000	5.817f	0	47804356	N.D.	12.498 #
10)	B gamma-Chl...	5.199	0.000	9643962	0	0.611	N.D. #
11)	B alpha-Chl...	5.265	0.000	13162988	0	0.863	N.D. #
13)	MA Dieldrin	5.558	0.000	6007936	0	0.388	N.D. #
25)	Chlordane-3	5.199	0.000	9643962	0	6.890	N.D. #
26)	Chlordane-4	5.265	0.000	13162988	0	9.980	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081419\
Data File : PL051505.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2019 23:04
Operator : SM\AJ
Sample : K4325-02
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
20190612-LOC-14

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 09:16:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

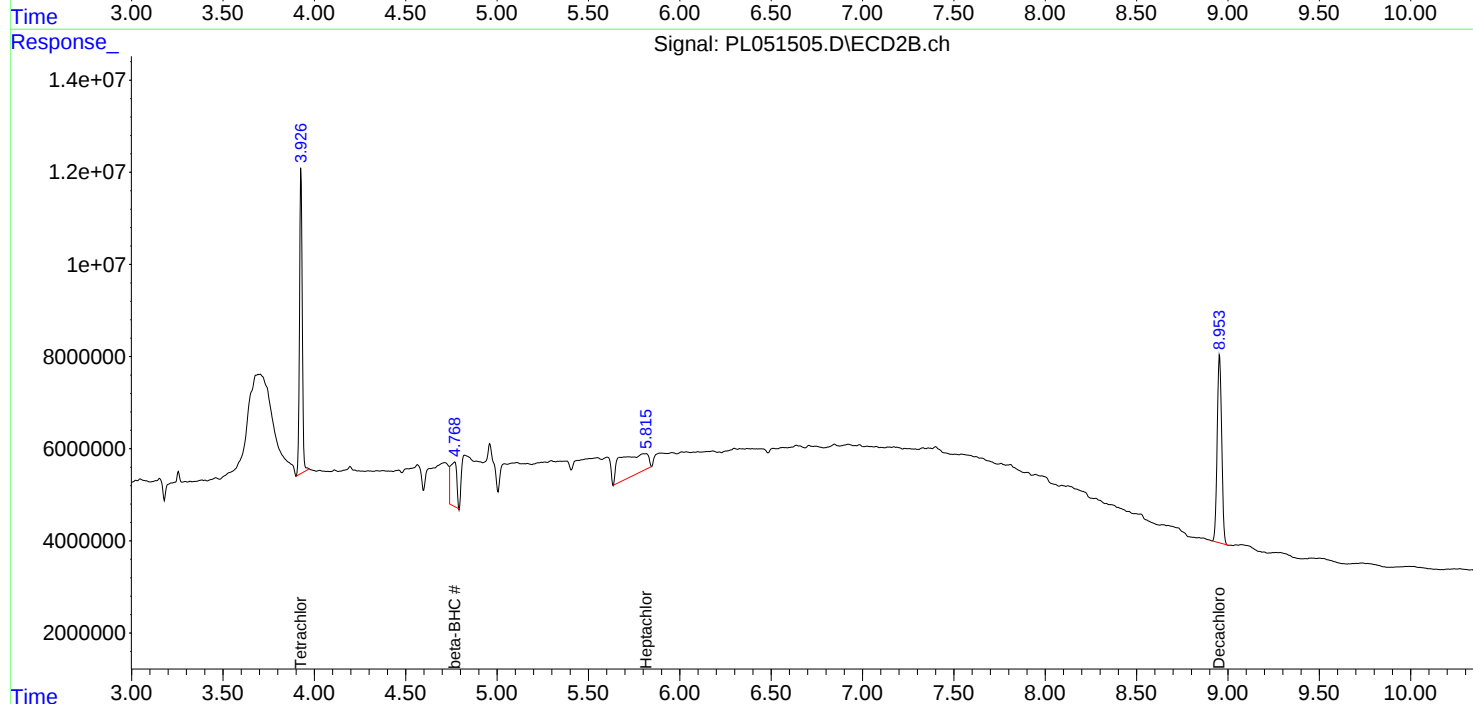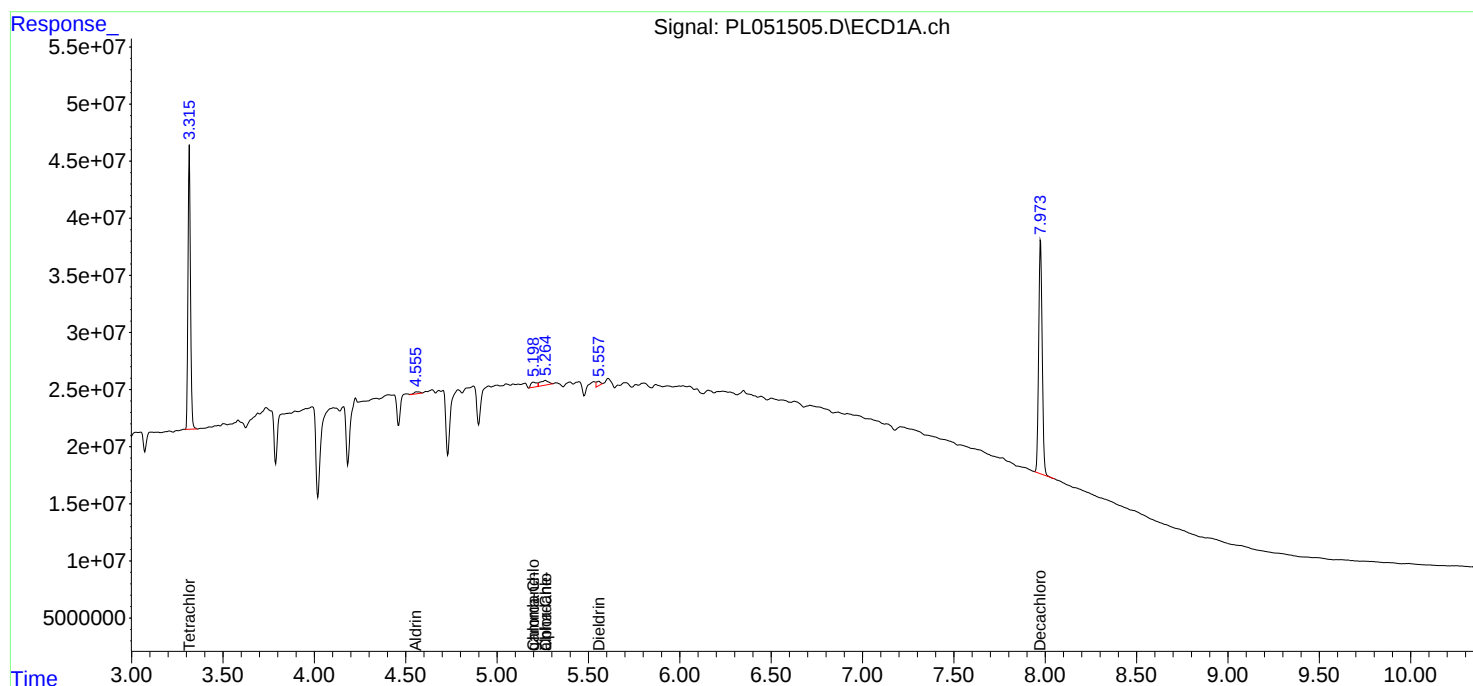


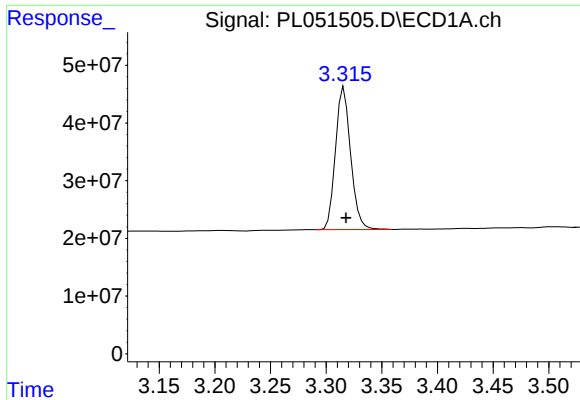

#1 Tetrachloro-m-xylene


R.T.: 3.316 min
Delta R.T.: -0.002 min
Response: 234364053
Conc: 23.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
20190612-LOC-14

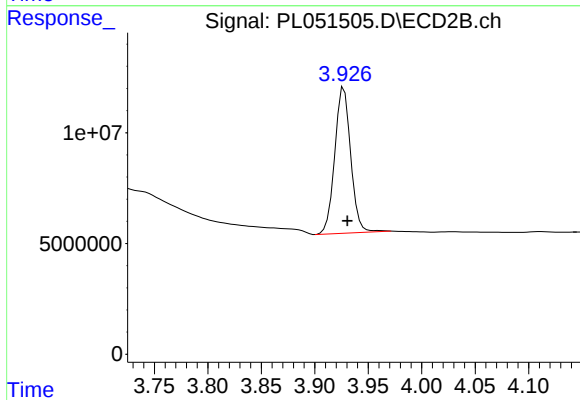


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.003 min
Response: 68535430
Conc: 24.02 ng/ml

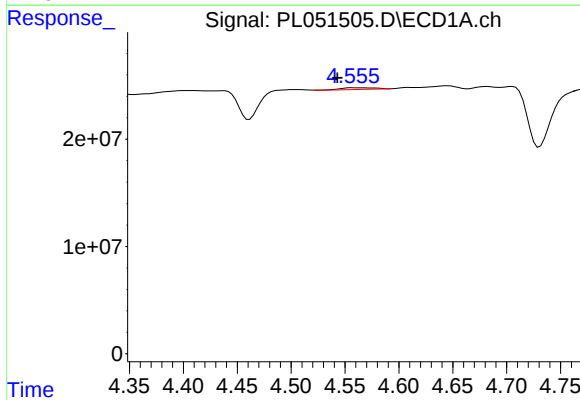


#5 Aldrin

R.T.: 4.557 min
Delta R.T.: 0.014 min
Response: 3647688
Conc: 0.24 ng/ml

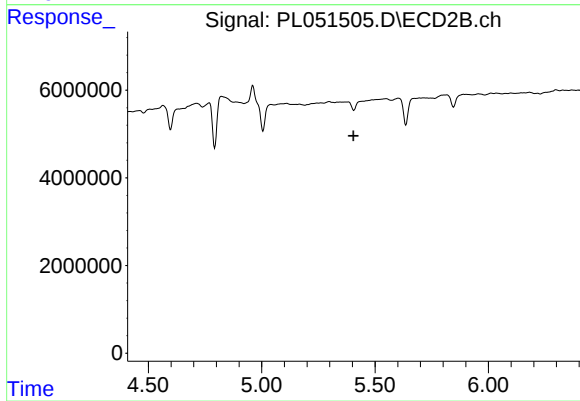

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.405 min
Response: 0
Conc: N.D.

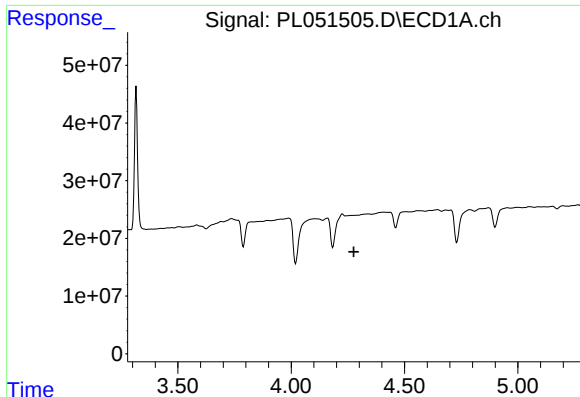

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20190612-LOC-14

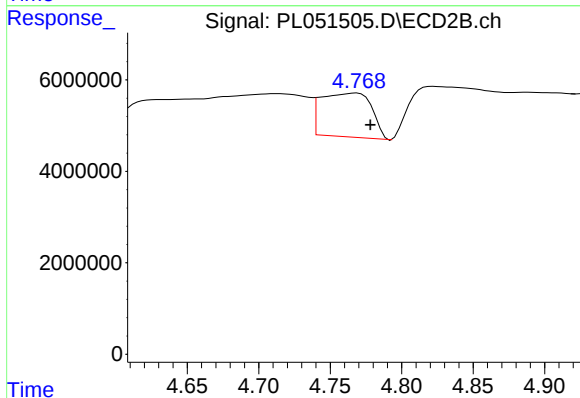


#6 beta-BHC

R.T.: 4.769 min
Delta R.T.: -0.010 min
Response: 23564714
Conc: 13.63 ng/ml

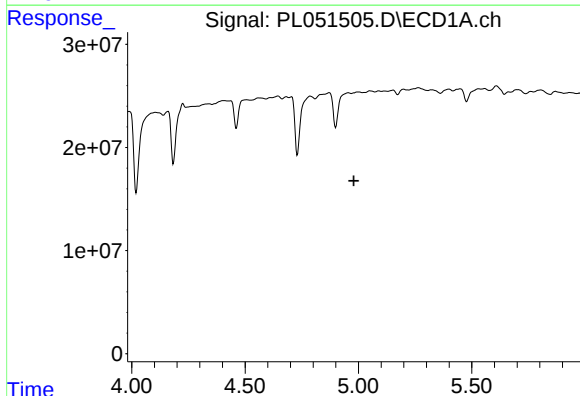


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

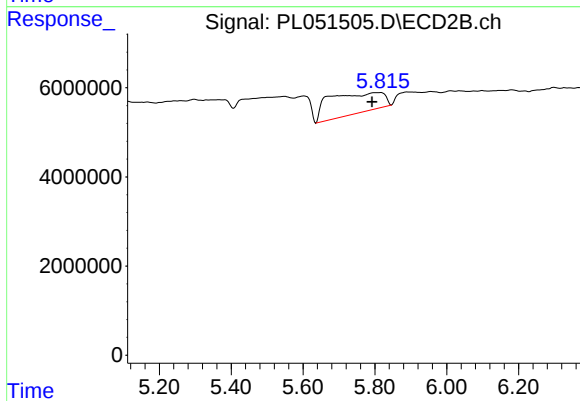

#8 Heptachlor epoxide


R.T.: 5.817 min
Delta R.T.: 0.024 min
Response: 47804356
Conc: 12.50 ng/ml

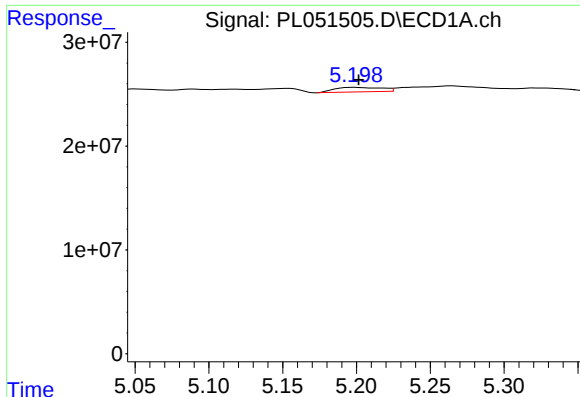

#10 gamma-Chlordane


R.T.: 5.199 min
Delta R.T.: -0.002 min
Response: 9643962
Conc: 0.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
20190612-LOC-14

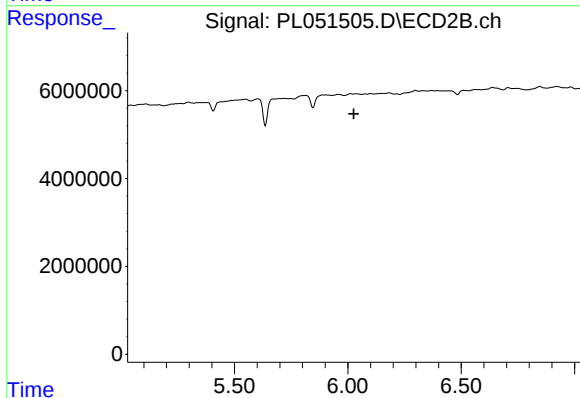


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

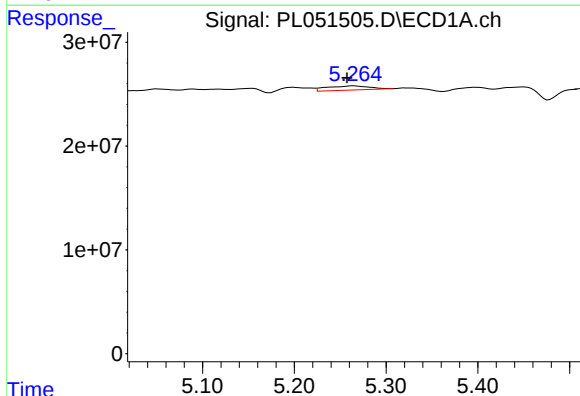


#11 alpha-Chlordane

R.T.: 5.265 min
Delta R.T.: 0.008 min
Response: 13162988
Conc: 0.86 ng/ml

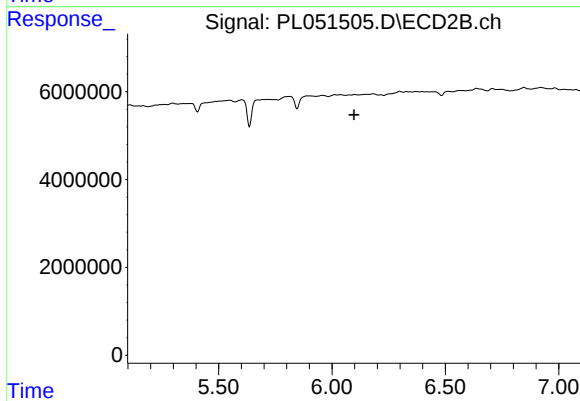

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

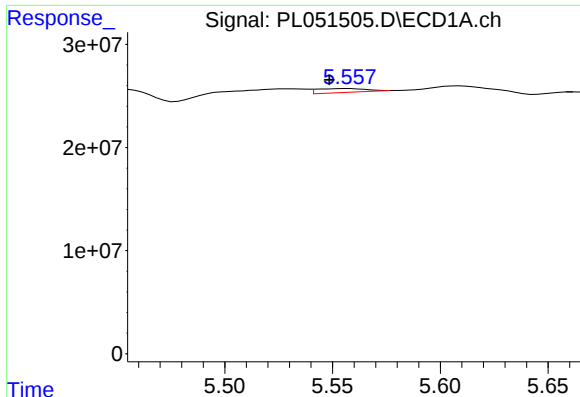

#13 Dieldrin


R.T.: 5.558 min
Delta R.T.: 0.009 min
Response: 6007936
Conc: 0.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
20190612-LOC-14

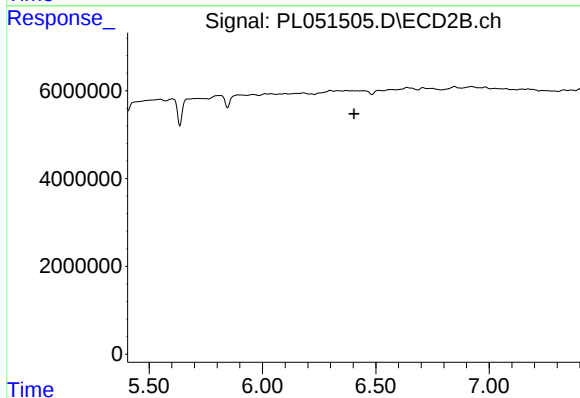


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.404 min
Response: 0
Conc: N.D.

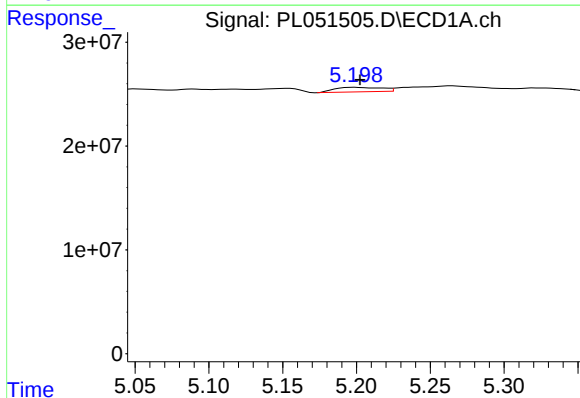


#25 Chlordane-3

R.T.: 5.199 min
Delta R.T.: -0.003 min
Response: 9643962
Conc: 6.89 ng/ml

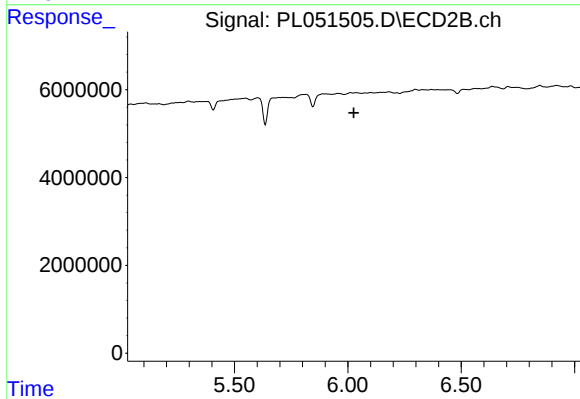

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

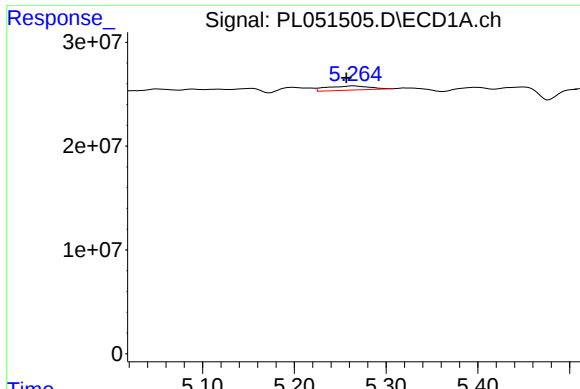

#26 Chlordane-4


R.T.: 5.265 min
Delta R.T.: 0.008 min
Response: 13162988
Conc: 9.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
20190612-LOC-14

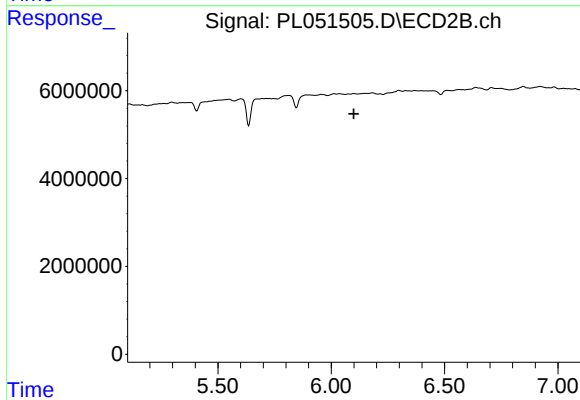


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.100 min
Response: 0
Conc: N.D.

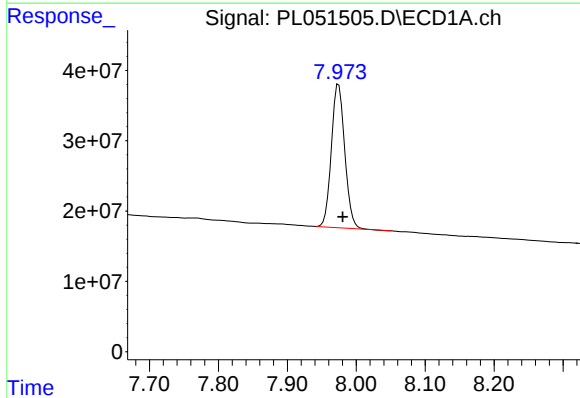

#28 Decachlorobiphenyl

R.T.: 7.974 min
Delta R.T.: -0.006 min
Response: 274411735
Conc: 27.10 ng/ml

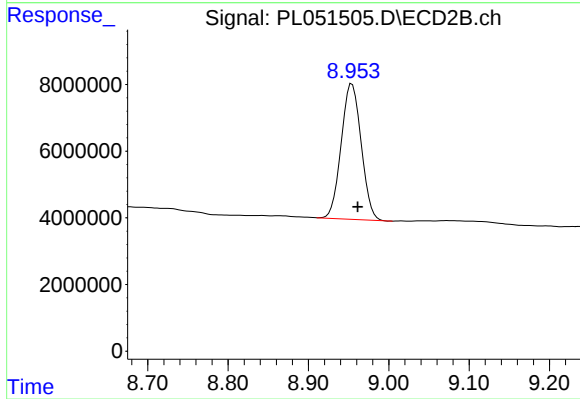

#28 Decachlorobiphenyl

R.T.: 8.954 min
Delta R.T.: -0.007 min
Response: 70318392
Conc: 24.87 ng/ml