

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081419\
 Data File : PL051462.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2019 12:15
 Operator : SM\AJ
 Sample : K4319-05DL 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TEST-PIT-1DL

Manual Integrations
 APPROVED

Ankita
 8/16/2019 2:42:00 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 12:48:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	3.927	42978060	10978331	4.277	3.848
28)	SA Decachlor...	7.977	8.956	37877359	9804585	3.741	3.467
Target Compounds							
15)	B Endosulfa...	6.091	6.847	979.5E6	267.1E6	69.992	84.010m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081419\
Data File : PL051462.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2019 12:15
Operator : SM\AJ
Sample : K4319-05DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TEST-PIT-1DL


Manual Integrations
APPROVED

Ankita
8/16/2019 2:42:00 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 12:48:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

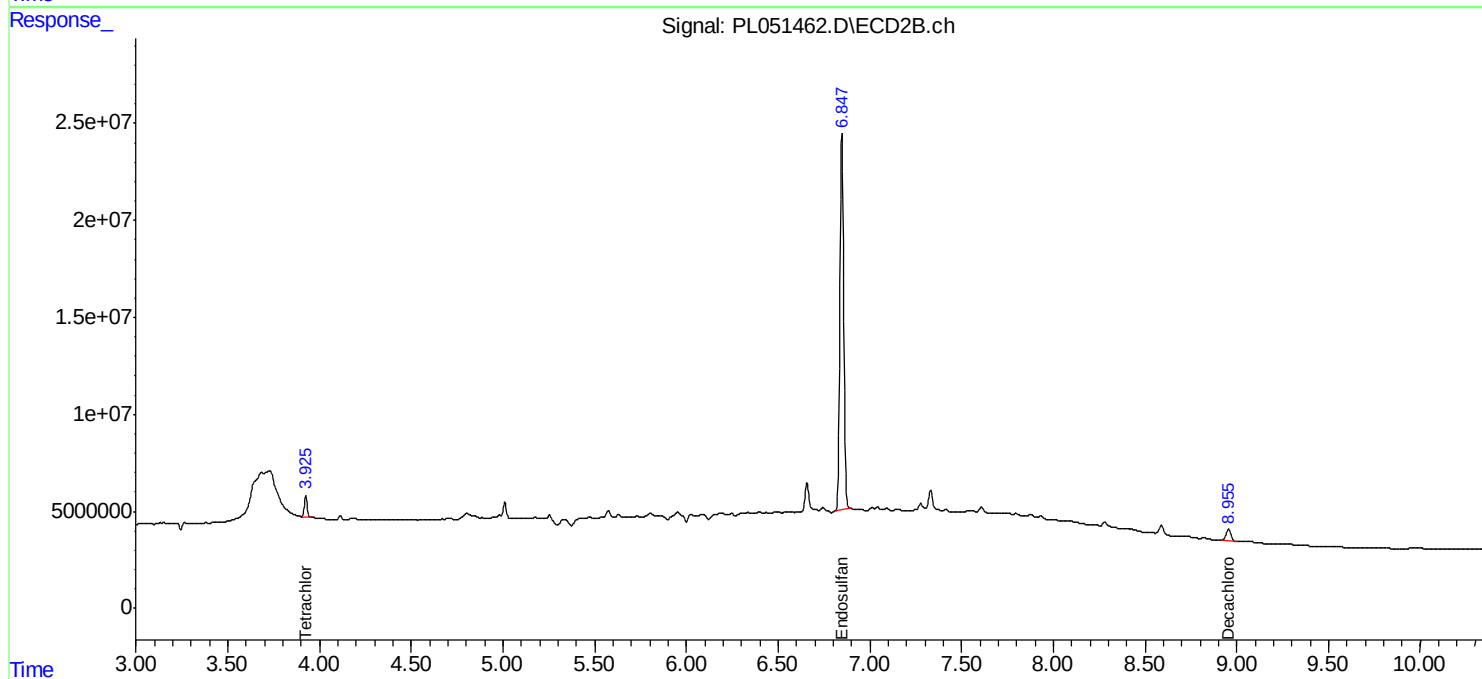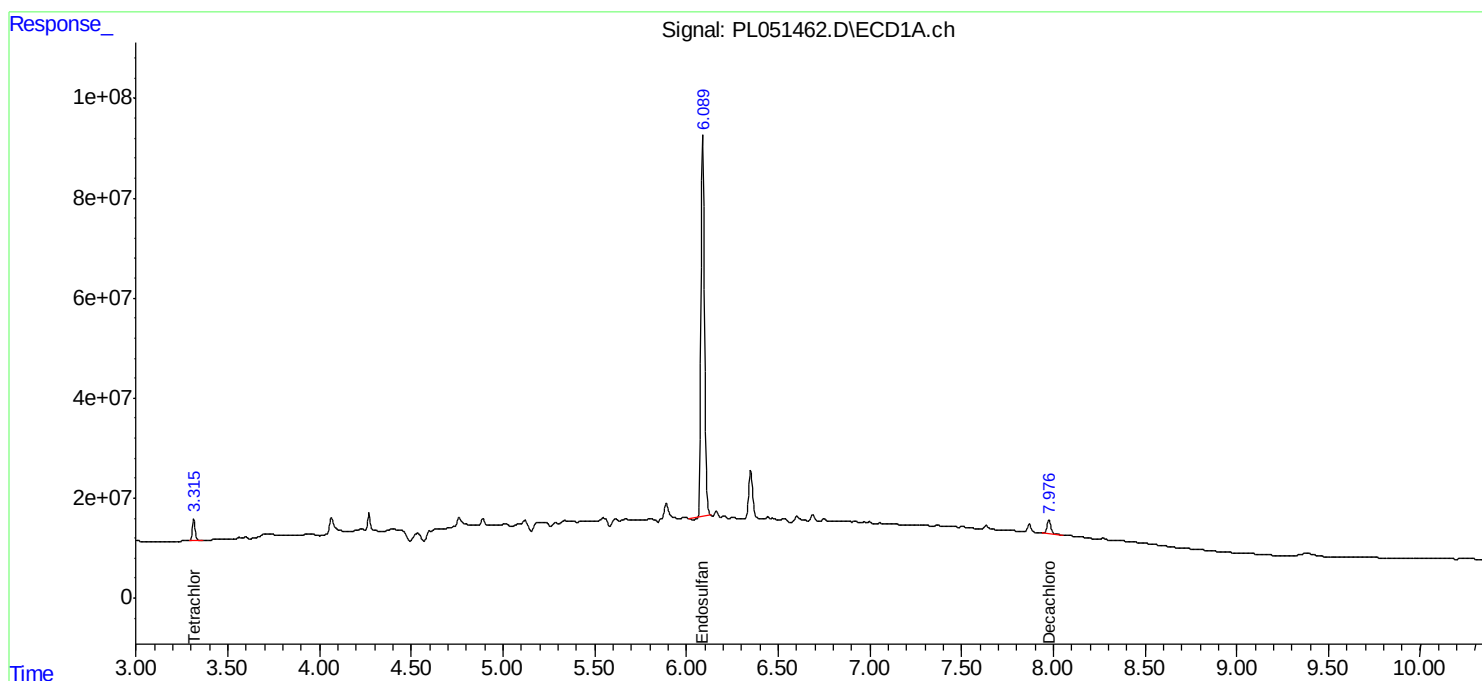

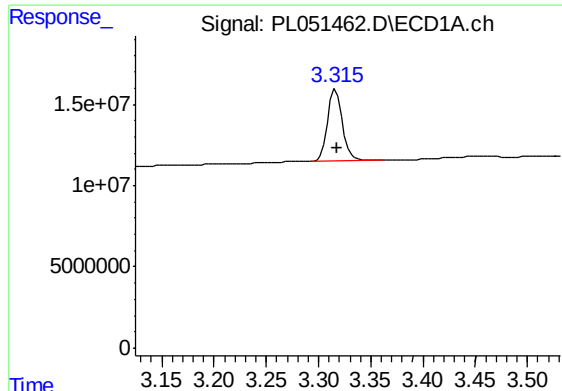


#1 Tetrachloro-m-xylene

R.T.: 3.316 min
Delta R.T.: -0.002 min
Response: 42978060
Conc: 4.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-1DL


Manual Integrations
APPROVED

Ankita
8/16/2019 2:42:00 PM

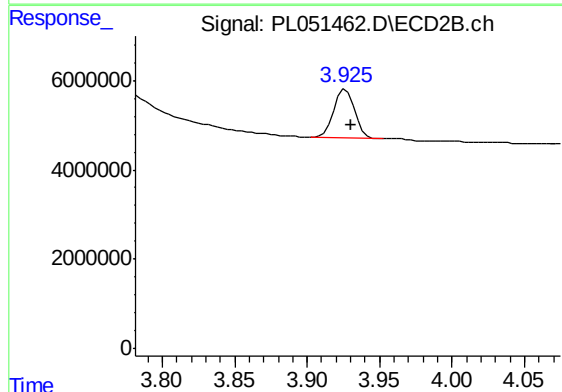


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.004 min
Response: 10978331
Conc: 3.85 ng/ml

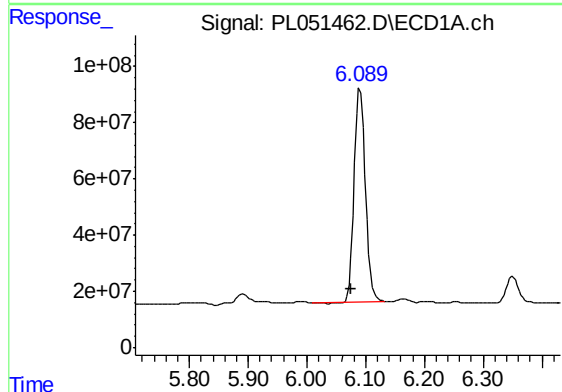


#15 Endosulfan II

R.T.: 6.091 min
Delta R.T.: 0.015 min
Response: 979538768
Conc: 69.99 ng/ml

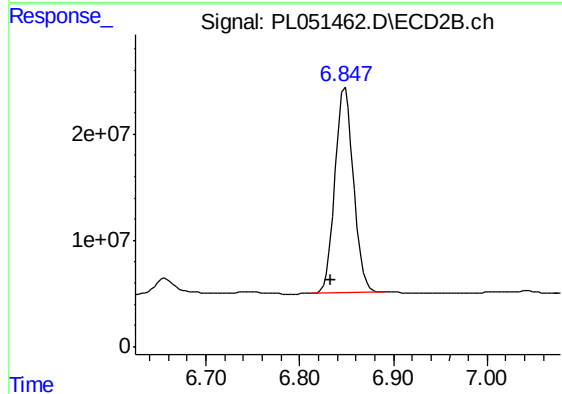

#15 Endosulfan II

R.T.: 6.847 min
Delta R.T.: 0.014 min
Response: 267084180
Conc: 84.01 ng/ml m

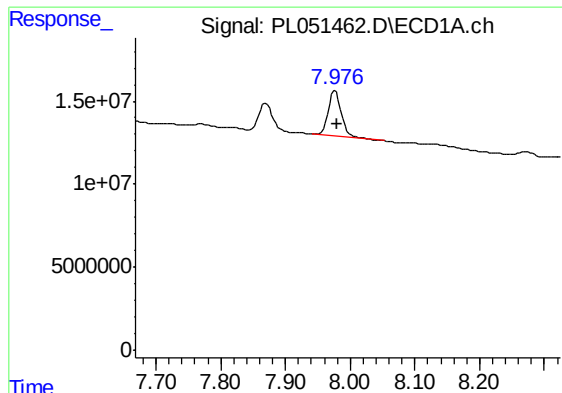


#28 Decachlorobiphenyl

R.T.: 7.977 min
Delta R.T.: -0.004 min
Response: 37877359
Conc: 3.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-1DL

Manual Integrations
APPROVED

Ankita
8/16/2019 2:42:00 PM

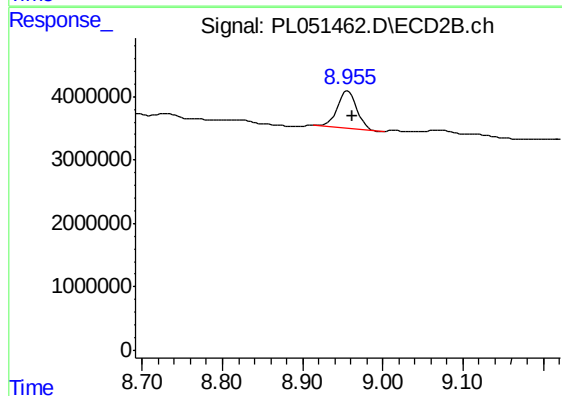

#28 Decachlorobiphenyl

R.T.: 8.956 min
Delta R.T.: -0.005 min
Response: 9804585
Conc: 3.47 ng/ml