

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081419\
 Data File : PL051463.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2019 12:30
 Operator : SM\AJ
 Sample : K4319-04DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TRANSFORMER-CONTAINMENT-S

Manual Integrations
 APPROVED

Ankita
 8/19/2019 10:22:04 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 12:49:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	3.927	45687368	11600064	4.547	4.066
28)	SA Decachlor...	7.976	8.956	43820673	11085390	4.328	3.920
Target Compounds							
15)	B Endosulfa...	6.089	6.848	127.8E6	34126448	9.133m	10.734m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081419\
Data File : PL051463.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2019 12:30
Operator : SM\AJ
Sample : K4319-04DL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TRANSFORMER-CONTAINMENT-S


Manual Integrations
APPROVED

Ankita
8/19/2019 10:22:04 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 12:49:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

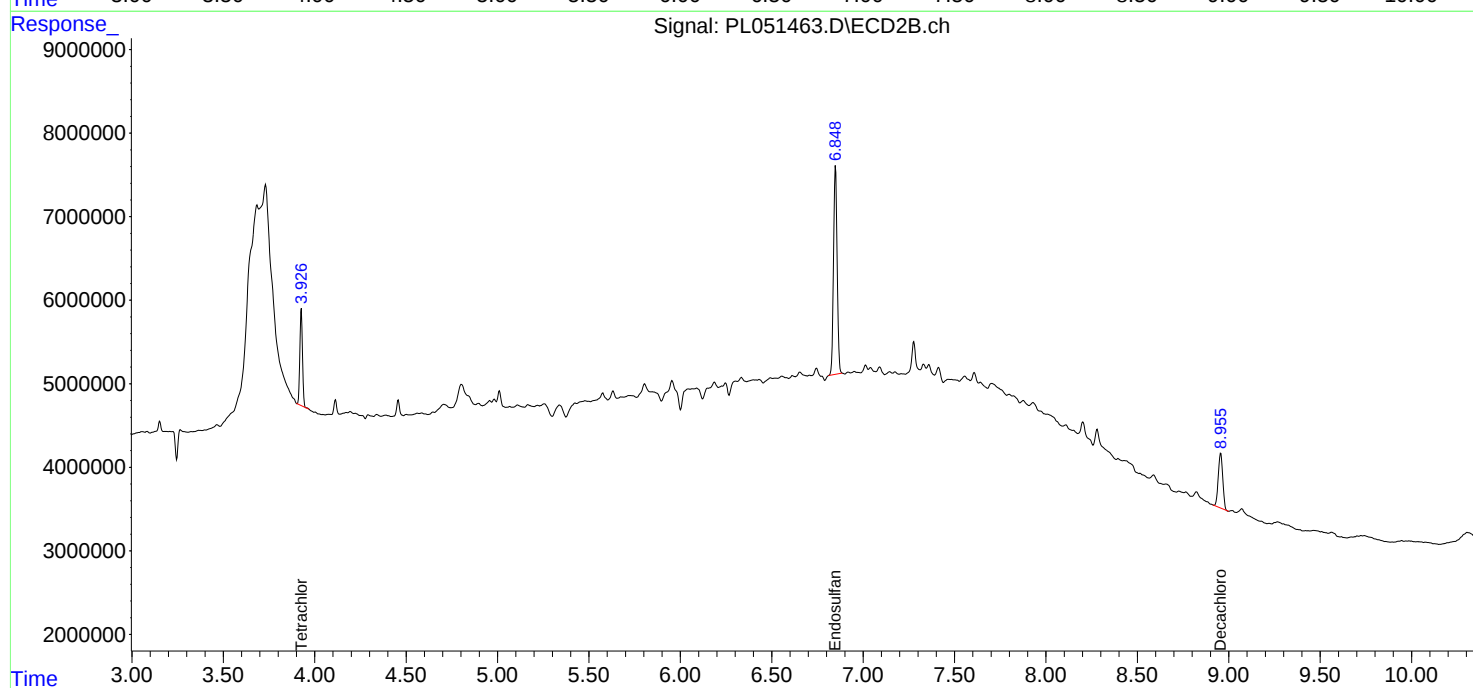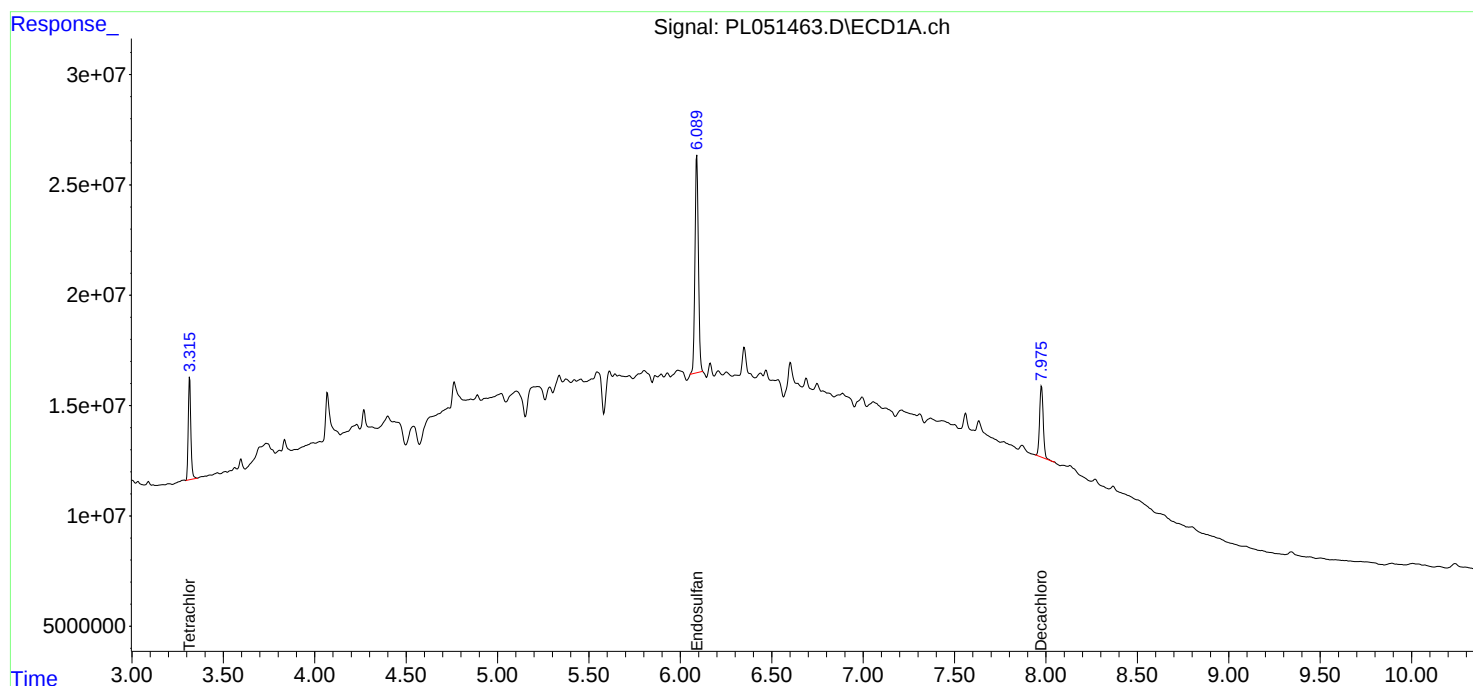

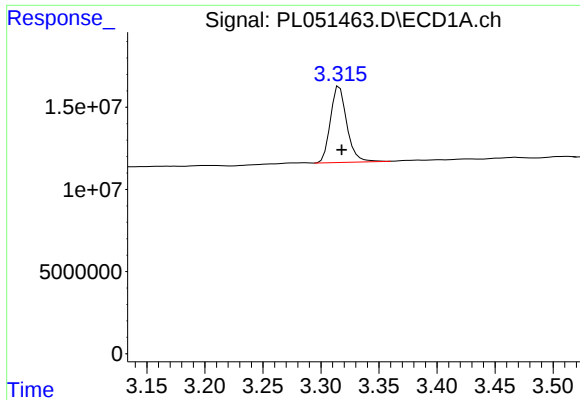


#1 Tetrachloro-m-xylene

R.T.: 3.316 min
Delta R.T.: -0.002 min
Response: 45687368
Conc: 4.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
TRANSFORMER-CONTAINMENT-S


Manual Integrations
APPROVED

Ankita
8/19/2019 10:22:04 AM

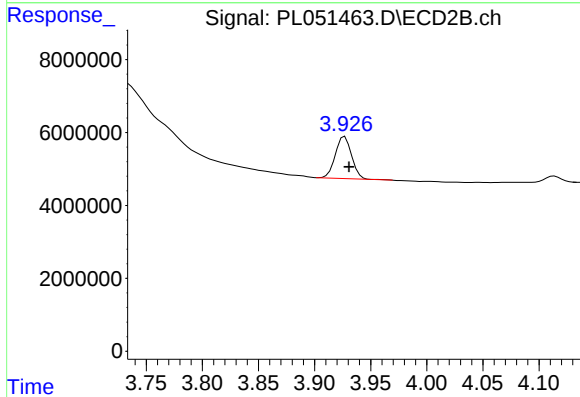


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.004 min
Response: 11600064
Conc: 4.07 ng/ml

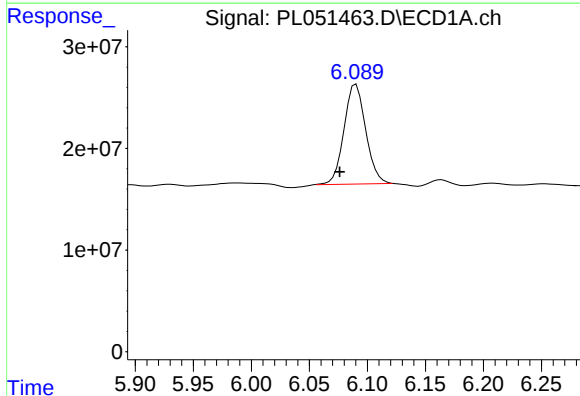


#15 Endosulfan II

R.T.: 6.089 min
Delta R.T.: 0.013 min
Response: 127809361
Conc: 9.13 ng/ml m

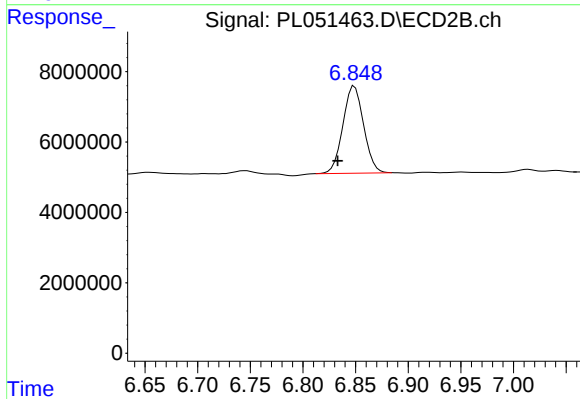

#15 Endosulfan II

R.T.: 6.848 min
Delta R.T.: 0.014 min
Response: 34126448
Conc: 10.73 ng/ml m

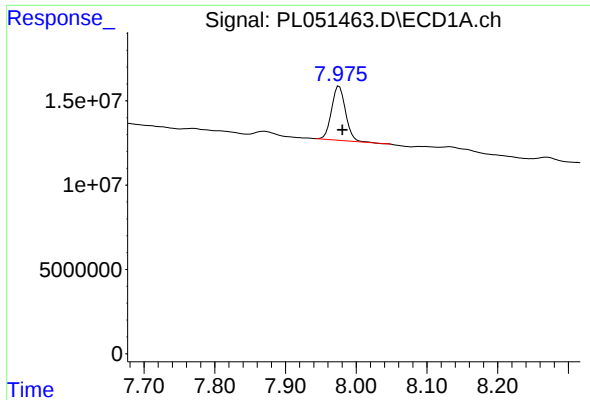


#28 Decachlorobiphenyl

R.T.: 7.976 min
Delta R.T.: -0.005 min
Response: 43820673
Conc: 4.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
TRANSFORMER-CONTAINMENT-S

Manual Integrations
APPROVED

Ankita
8/19/2019 10:22:04 AM

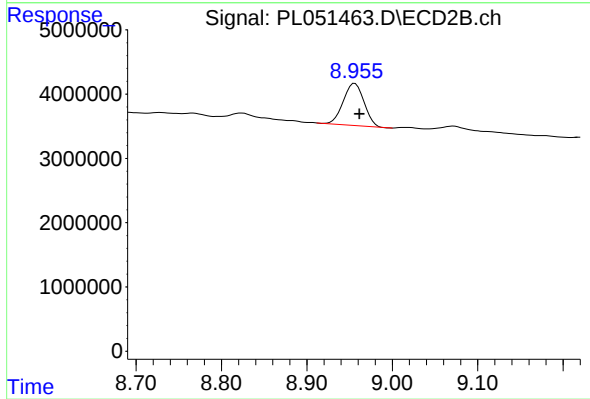

#28 Decachlorobiphenyl

R.T.: 8.956 min
Delta R.T.: -0.005 min
Response: 11085390
Conc: 3.92 ng/ml