

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081419\
 Data File : PL051474.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2019 15:44
 Operator : SM\AJ
 Sample : K4330-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 0631-SITE-WATER-MUNICIPAL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 13:21:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	3.927	210.2E6	55574595	20.917	19.478
28)	SA Decachlor...	7.976	8.955	210.8E6	55206184	20.821	19.522

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081419\
Data File : PL051474.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2019 15:44
Operator : SM\AJ
Sample : K4330-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
0631-SITE-WATER-MUNICIPAL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 13:21:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

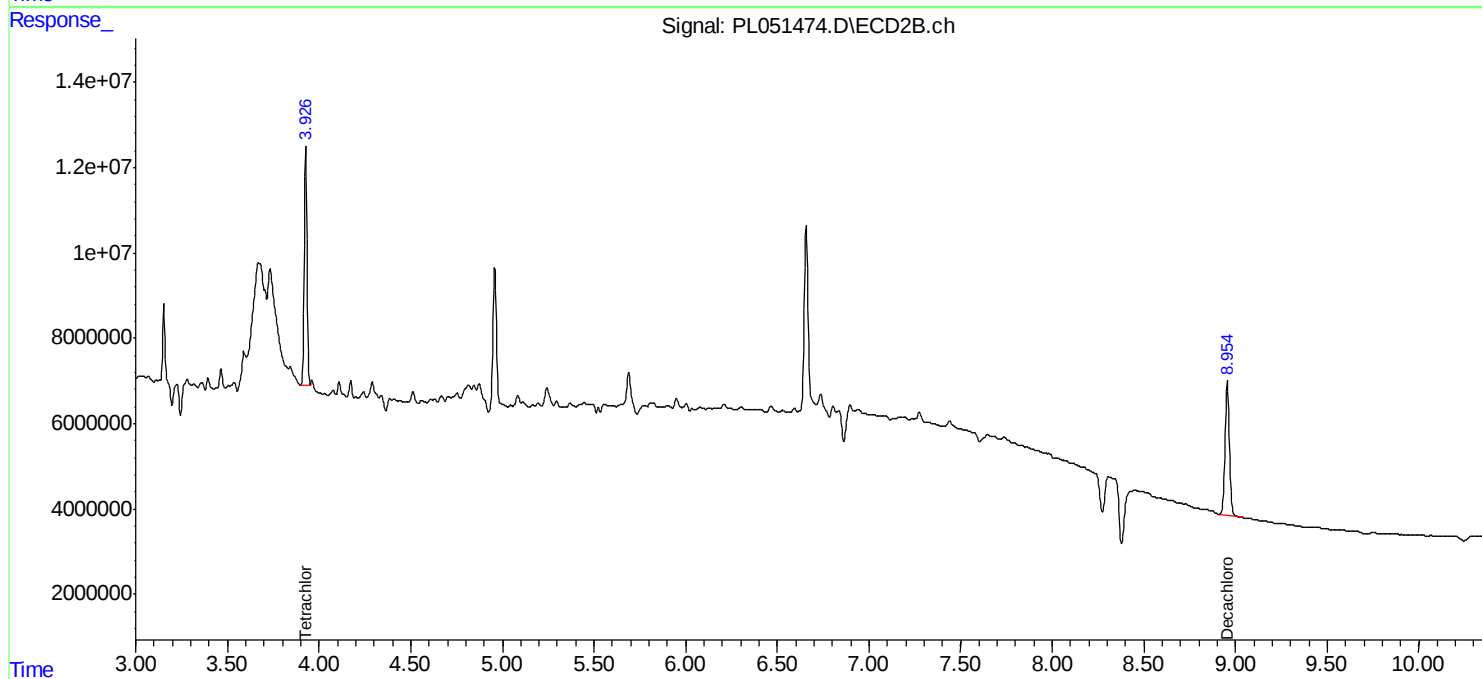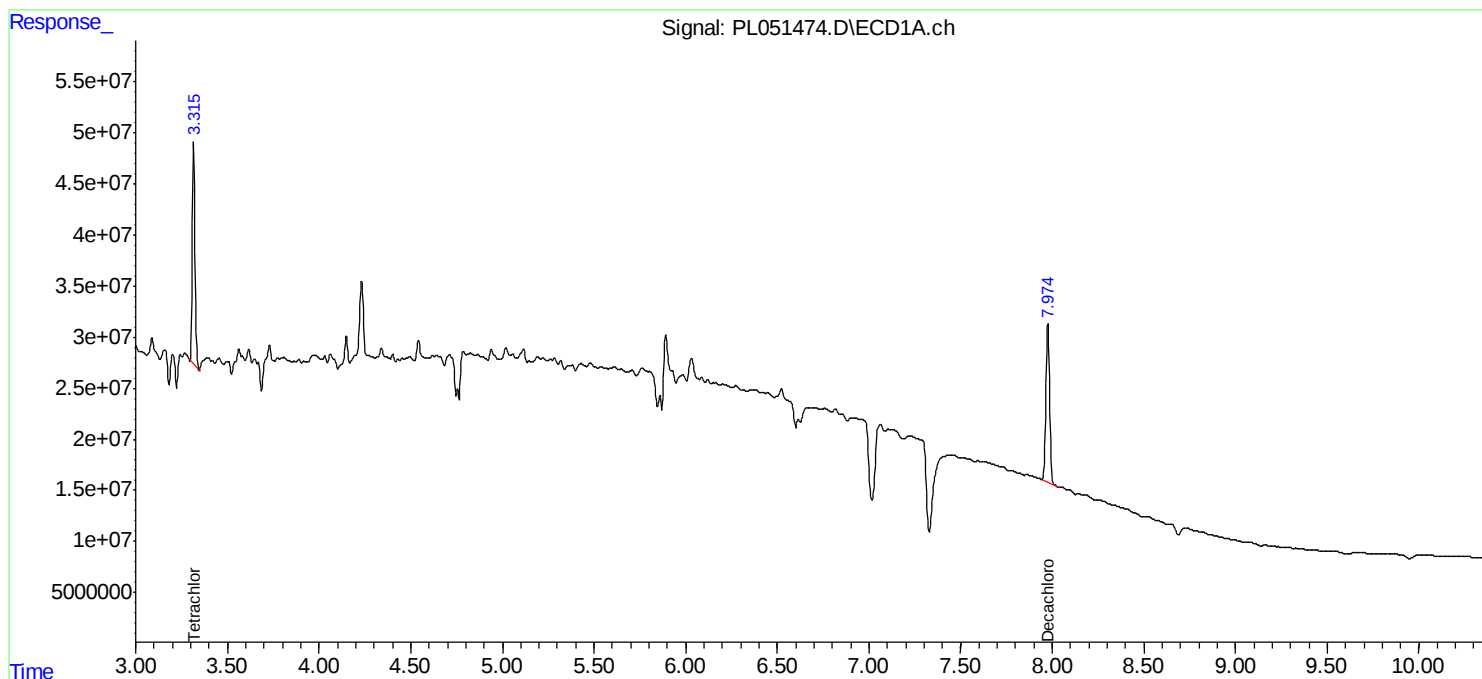


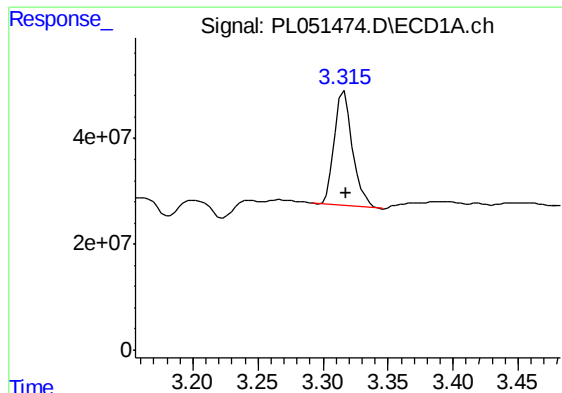

#1 Tetrachloro-m-xylene


R.T.: 3.316 min
Delta R.T.: -0.002 min
Response: 210172838
Conc: 20.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
0631-SITE-WATER-MUNICIPAL

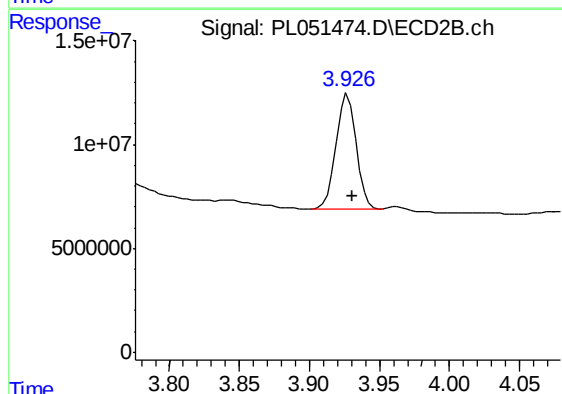


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.003 min
Response: 55574595
Conc: 19.48 ng/ml

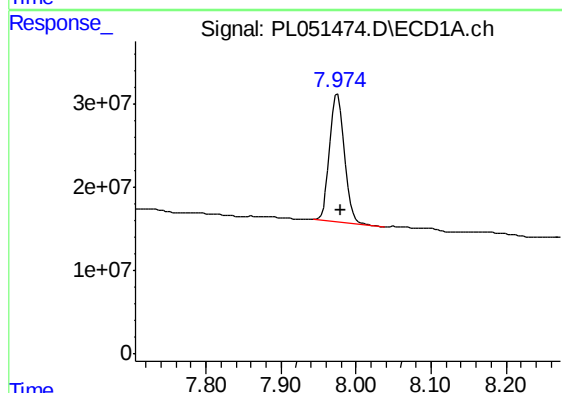

#28 Decachlorobiphenyl

R.T.: 7.976 min
Delta R.T.: -0.005 min
Response: 210822217
Conc: 20.82 ng/ml

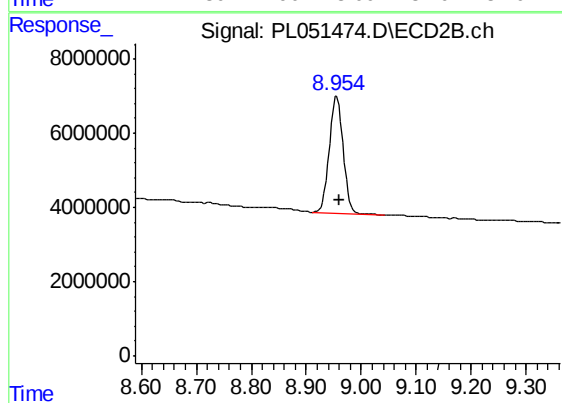

#28 Decachlorobiphenyl

R.T.: 8.955 min
Delta R.T.: -0.006 min
Response: 55206184
Conc: 19.52 ng/ml