

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081420\
 Data File : PL060735.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2020 10:41
 Operator : DD\AJ
 Sample : L3677-05DL2 100X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 16:37:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 11 01:39:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
10)	B	gamma-Chl...	5.403	6.125	4077652	5782324	1.923 1.913
11)	B	alpha-Chl...	0.000	6.199	0	10294054	N.D. 3.349 #
12)	B	4,4'-DDE	5.627	6.355	24356642	34150618	12.284 11.997
13)	MA	Dieldrin	5.778f	0.000	19199028	0	9.286 N.D. #
14)	MA	Endrin	6.017	6.752f	27227780	32657895	13.943 12.906
16)	A	4,4'-DDD	6.142	6.847	107.8E6	143.7E6	64.012 62.618
17)	MA	4,4'-DDT	6.383	7.147	163.7E6	207.0E6	99.015 94.694
25)		Chlordane-3	5.403	6.125	4077652	5782324	23.267 15.969 #
26)		Chlordane-4	0.000	6.199	0	10294054	N.D. 23.746 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081420\
Data File : PL060735.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2020 10:41
Operator : DD\AJ
Sample : L3677-05DL2 100X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 16:37:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
Quant Title : GC Extractables
QLast Update : Tue Aug 11 01:39:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

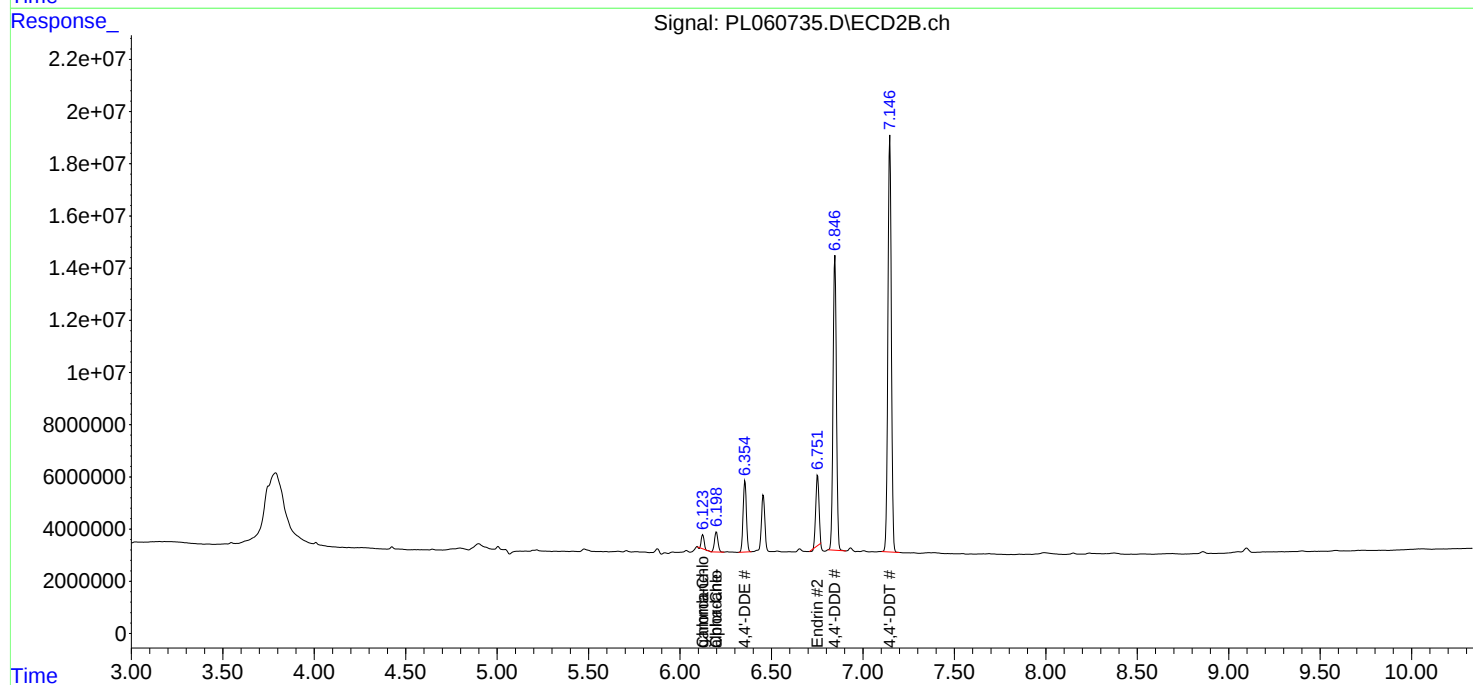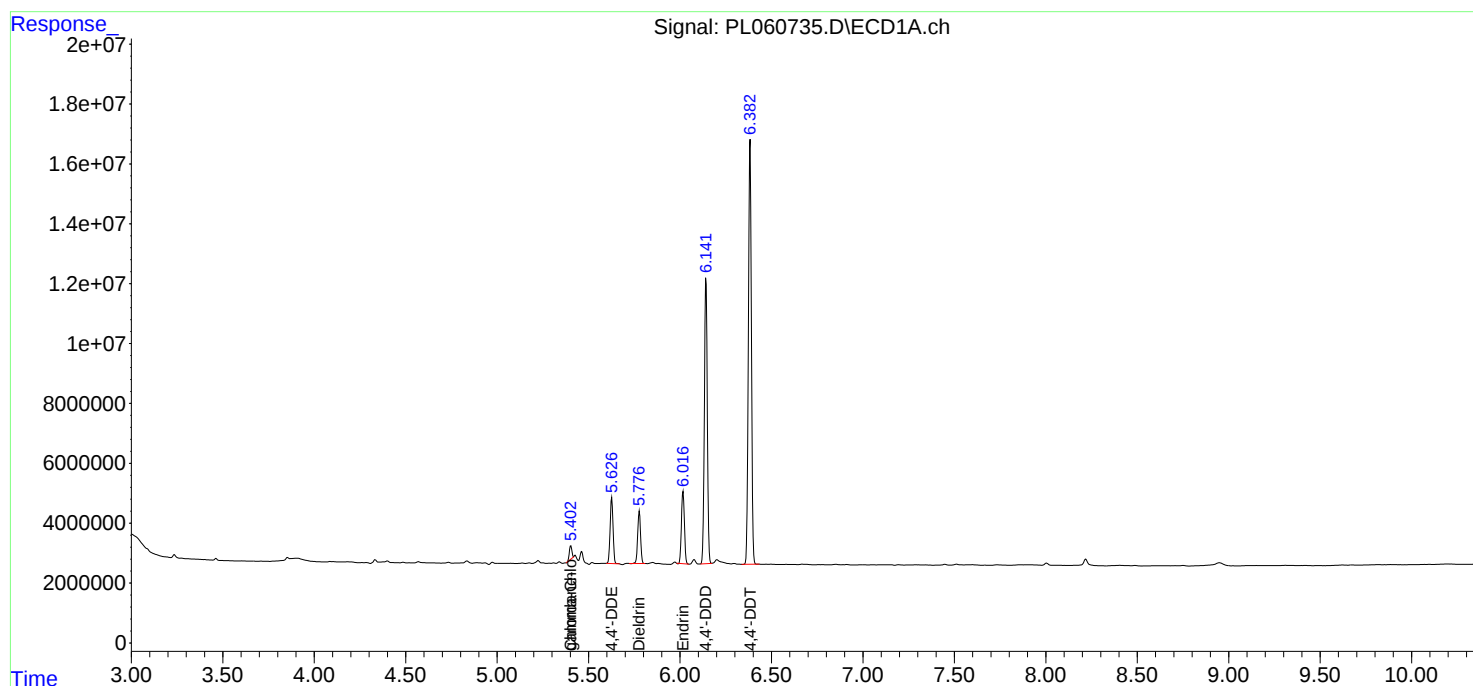


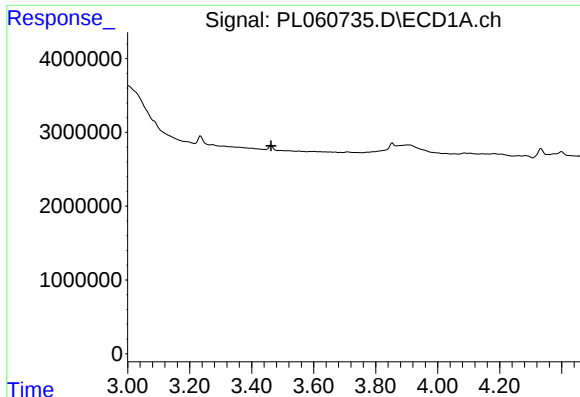

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.463 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

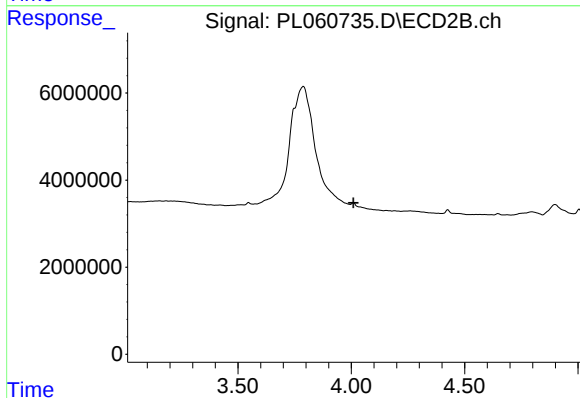


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.010 min
Response: 0
Conc: N.D.

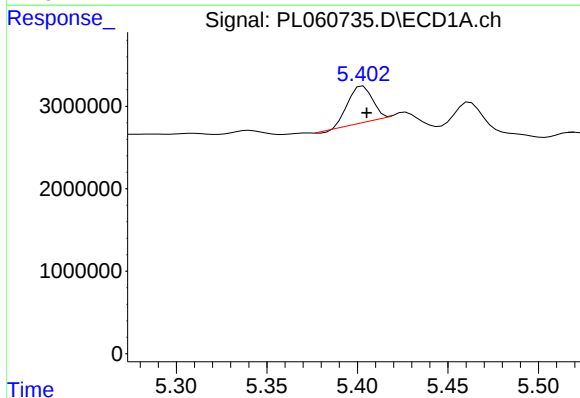


#10 gamma-Chlordane

R.T.: 5.403 min
Delta R.T.: -0.002 min
Response: 4077652
Conc: 1.92 ng/ml

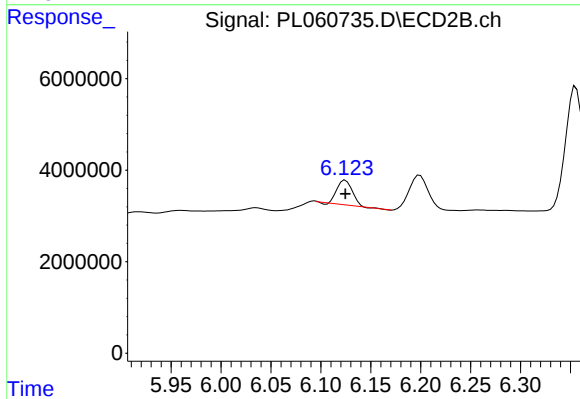

#10 gamma-Chlordane


R.T.: 6.125 min
Delta R.T.: 0.000 min
Response: 5782324
Conc: 1.91 ng/ml

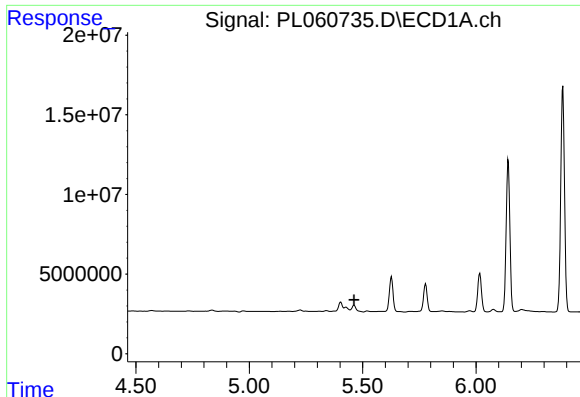

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.463 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

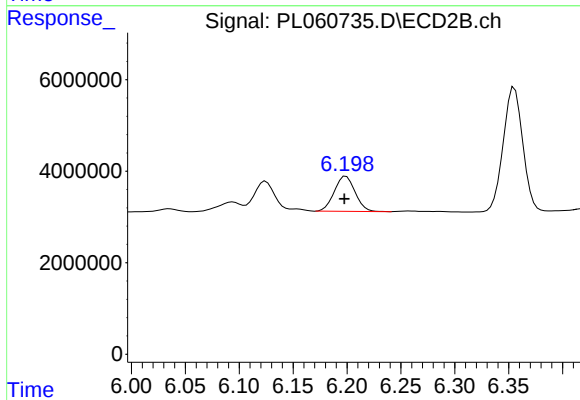


#11 alpha-Chlordane

R.T.: 6.199 min
Delta R.T.: 0.002 min
Response: 10294054
Conc: 3.35 ng/ml

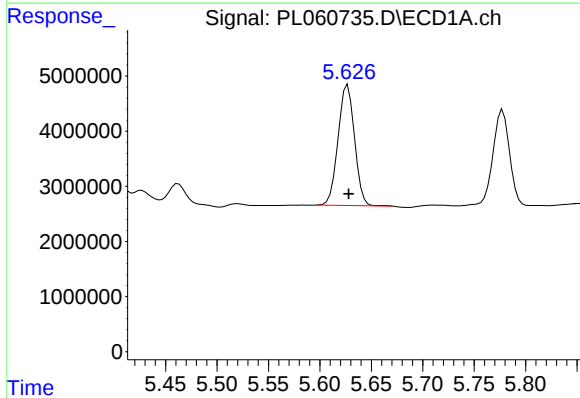


#12 4,4'-DDE

R.T.: 5.627 min
Delta R.T.: -0.001 min
Response: 24356642
Conc: 12.28 ng/ml

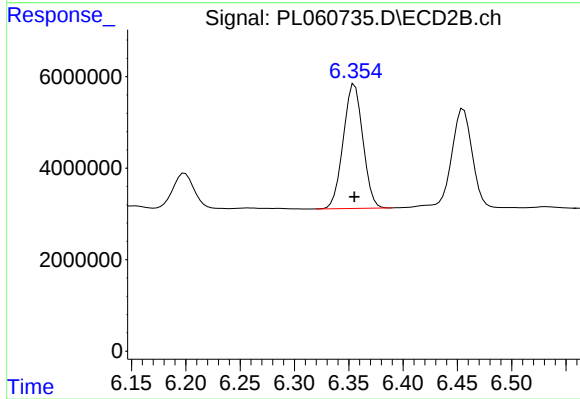

#12 4,4'-DDE


R.T.: 6.355 min
Delta R.T.: 0.000 min
Response: 34150618
Conc: 12.00 ng/ml

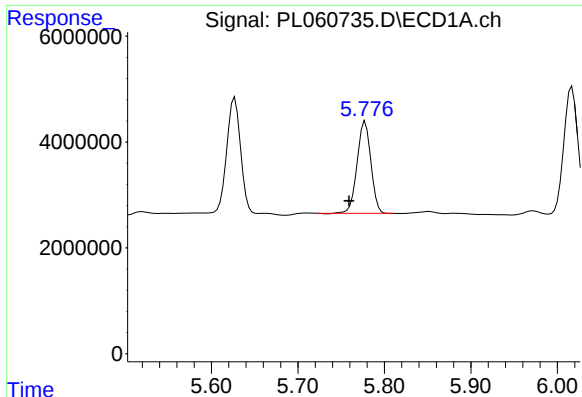

#13 Dieldrin


R.T.: 5.778 min
Delta R.T.: 0.019 min
Response: 19199028
Conc: 9.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

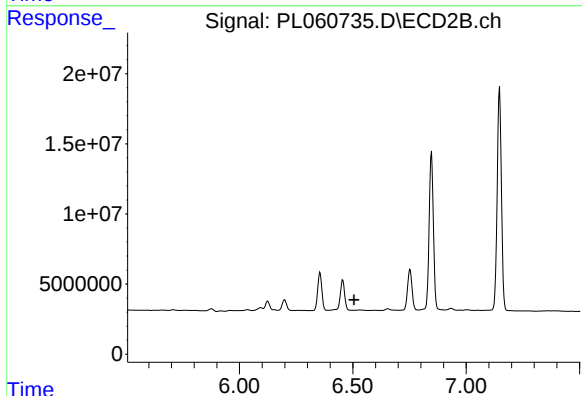


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.506 min
Response: 0
Conc: N.D.

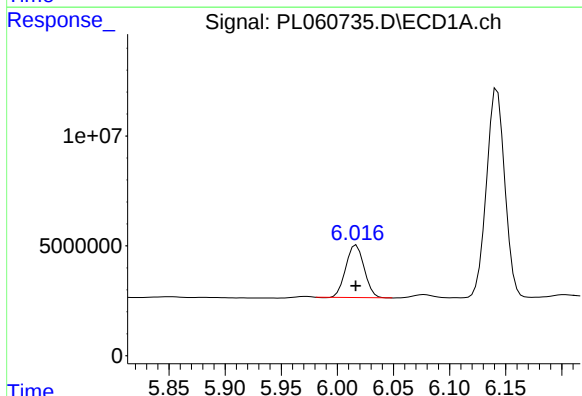


#14 Endrin

R.T.: 6.017 min
Delta R.T.: 0.000 min
Response: 27227780
Conc: 13.94 ng/ml

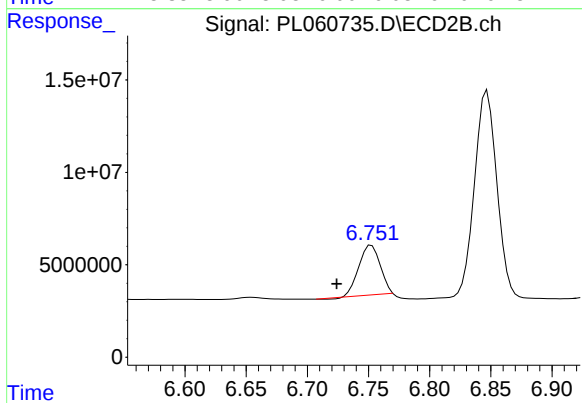

#14 Endrin


R.T.: 6.752 min
Delta R.T.: 0.028 min
Response: 32657895
Conc: 12.91 ng/ml

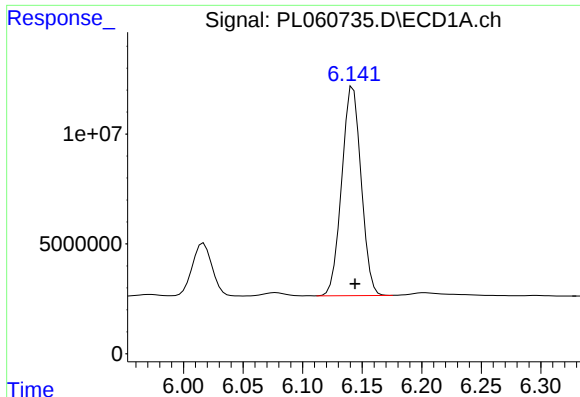

#16 4,4'-DDD


R.T.: 6.142 min
Delta R.T.: -0.002 min
Response: 107772704
Conc: 64.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

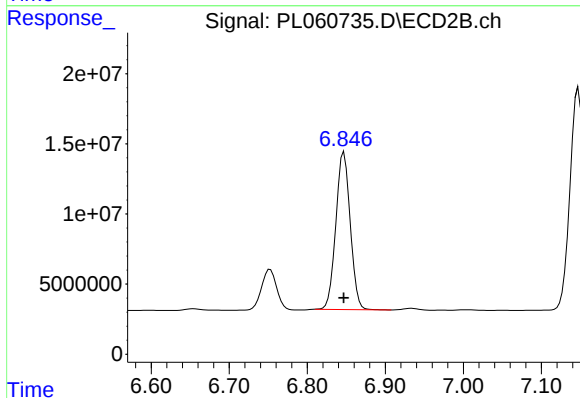


#16 4,4'-DDD

R.T.: 6.847 min
Delta R.T.: 0.000 min
Response: 143684946
Conc: 62.62 ng/ml

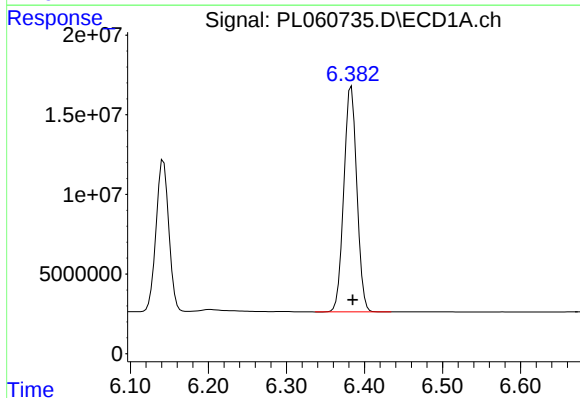


#17 4,4'-DDT

R.T.: 6.383 min
Delta R.T.: -0.002 min
Response: 163670663
Conc: 99.02 ng/ml

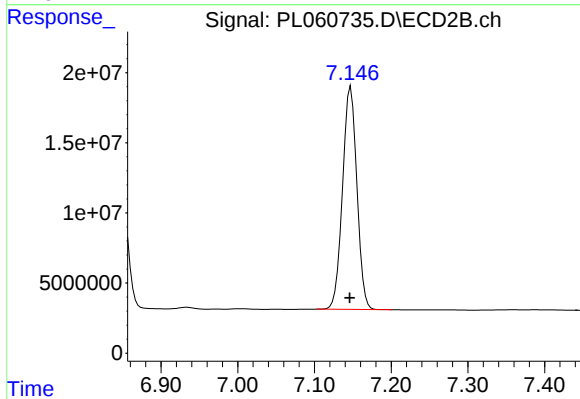

#17 4,4'-DDT


R.T.: 7.147 min
Delta R.T.: 0.001 min
Response: 207001772
Conc: 94.69 ng/ml

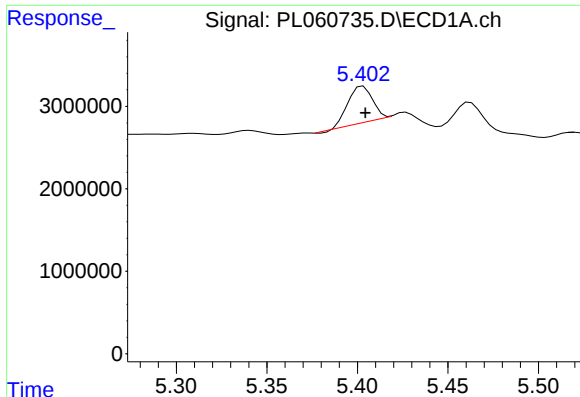

#25 Chlordane-3


R.T.: 5.403 min
Delta R.T.: -0.001 min
Response: 4077652
Conc: 23.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

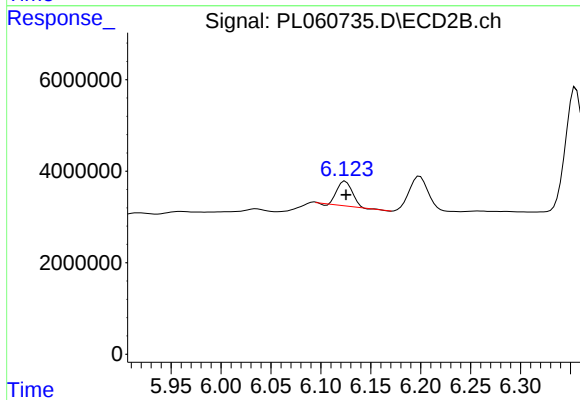


#25 Chlordane-3

R.T.: 6.125 min
Delta R.T.: 0.000 min
Response: 5782324
Conc: 15.97 ng/ml

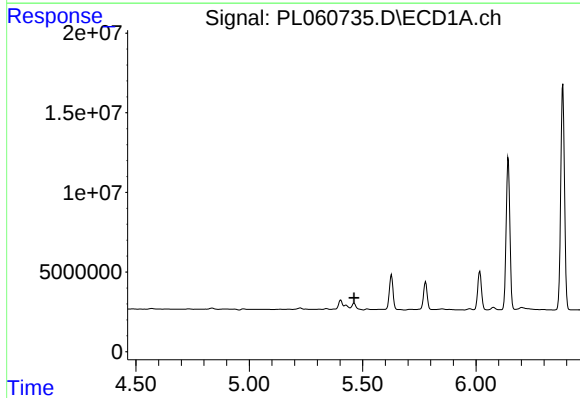


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.463 min
Response: 0
Conc: N.D.

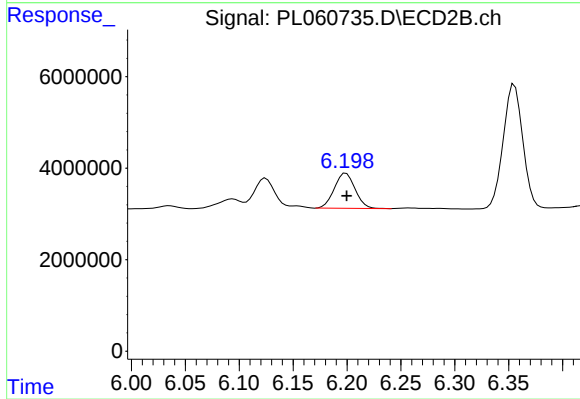

#26 Chlordane-4


R.T.: 6.199 min
Delta R.T.: 0.000 min
Response: 10294054
Conc: 23.75 ng/ml

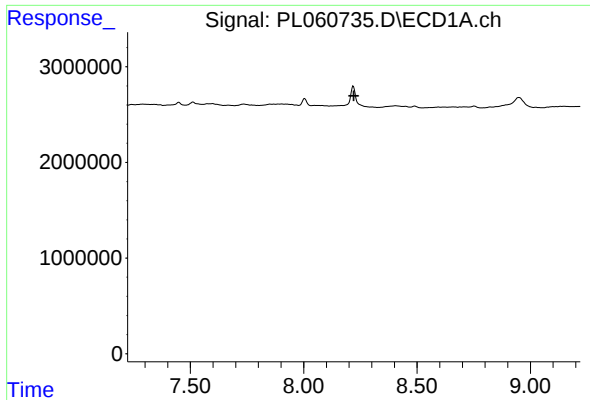

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.220 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

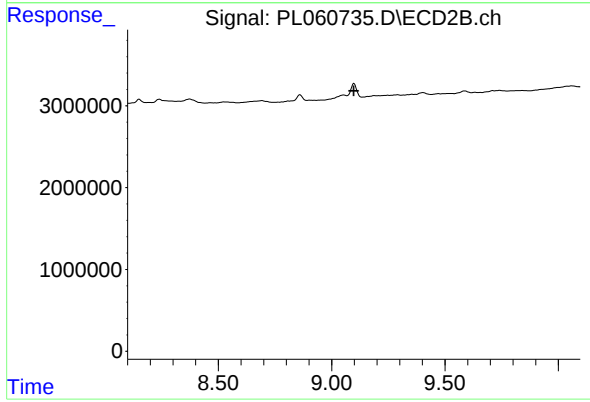

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.098 min
Response: 0
Conc: N.D.