

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081420\
 Data File : PL060738.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2020 12:33
 Operator : DD\AJ
 Sample : L3502-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 16:38:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 11 01:39:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.012	29604687	38767830	15.792	14.579
28)	SA Decachlor...	8.226	9.105	23905010	27940656	13.096	14.892
Target Compounds							
4)	MA Heptachlor	0.000	5.222f	0	1837442	N.D.	0.519 #
5)	MB Aldrin	4.720	0.000	7203145	0	3.291	N.D. #
10)	B gamma-Chl...	5.412	6.129	11774288	9505902	5.553	3.144 #
11)	B alpha-Chl...	5.470	6.202	17931312	15576583	8.450	5.067 #
12)	B 4,4'-DDE	0.000	6.356	0	9634525	N.D.	3.385 #
24)	Chlordane-2	4.846	0.000	19288182	0	304.444	N.D. #
25)	Chlordane-3	5.412	6.129	11774288	9505902	67.183	26.252 #
26)	Chlordane-4	5.470	6.202	17931312	15576583	128.257	35.932 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081420\
Data File : PL060738.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2020 12:33
Operator : DD\AJ
Sample : L3502-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 16:38:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
Quant Title : GC Extractables
QLast Update : Tue Aug 11 01:39:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

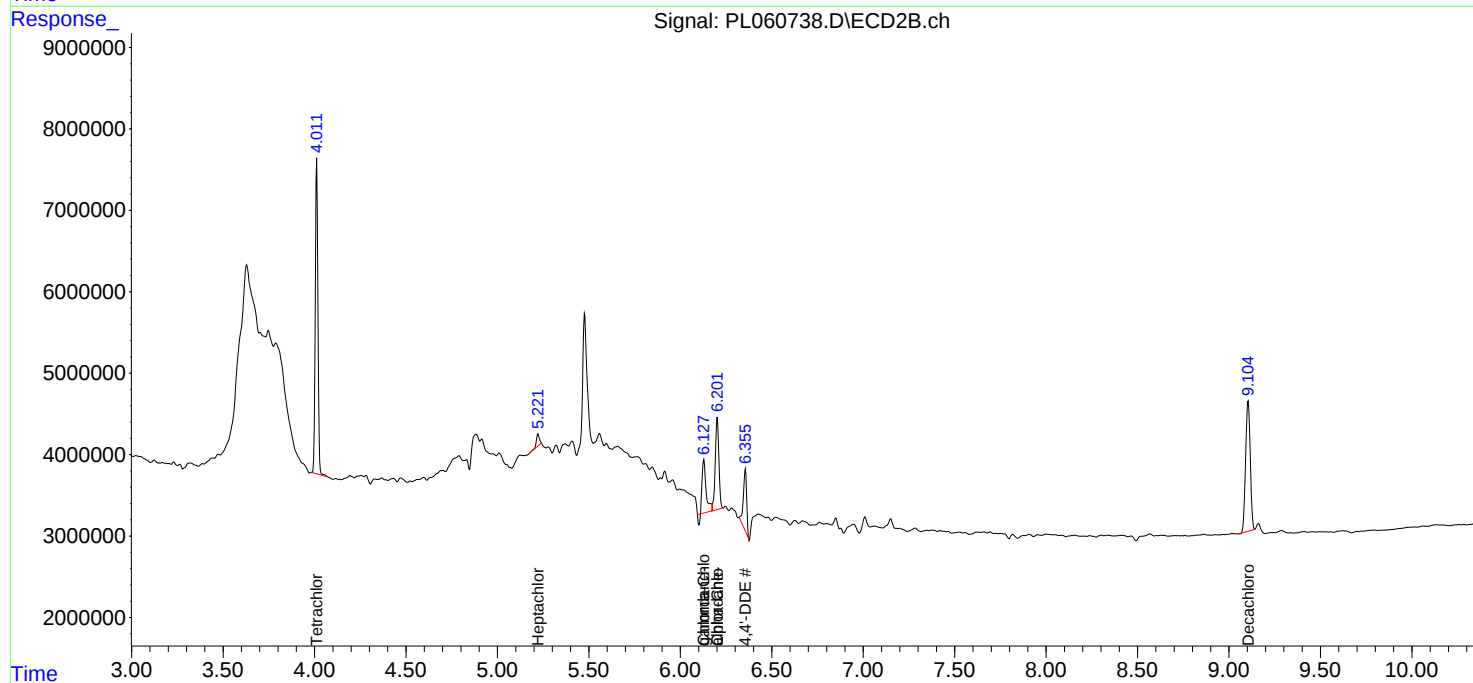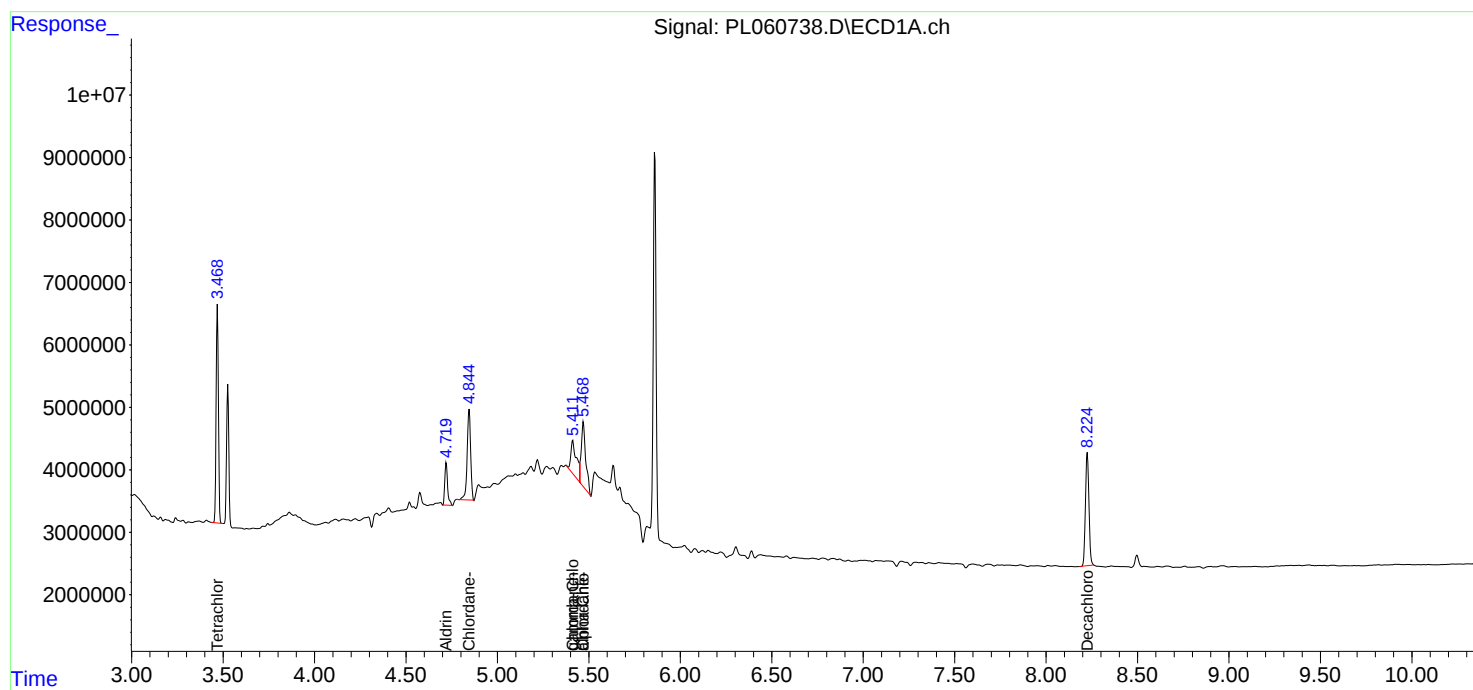


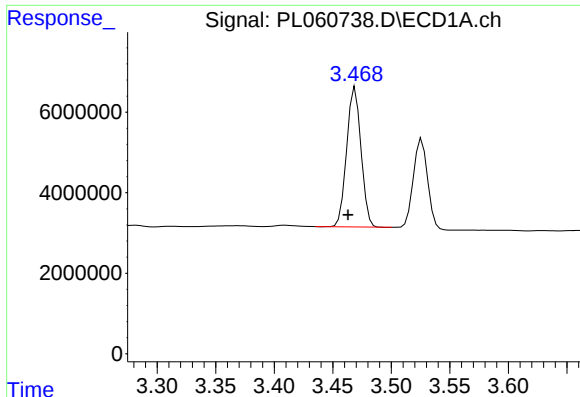

#1 Tetrachloro-m-xylene


R.T.: 3.469 min
Delta R.T.: 0.006 min
Response: 29604687
Conc: 15.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

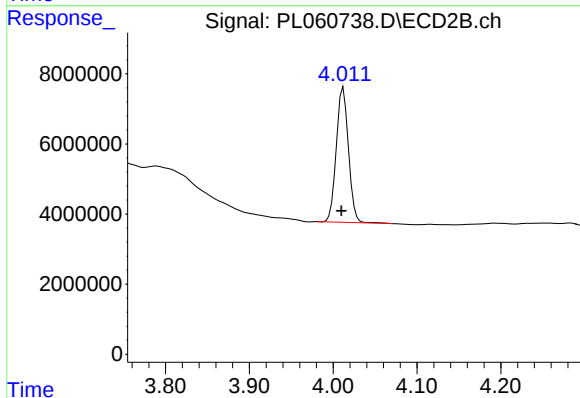


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.002 min
Response: 38767830
Conc: 14.58 ng/ml

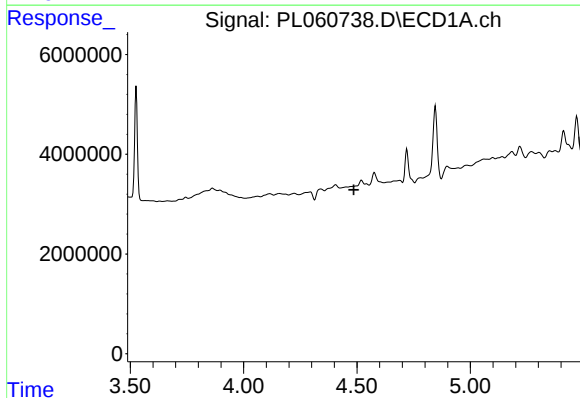


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.486 min
Response: 0
Conc: N.D.

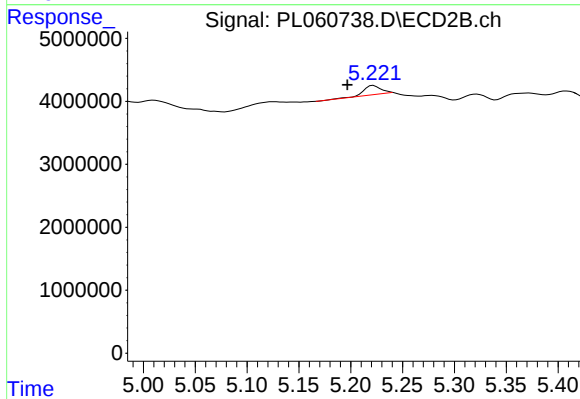

#4 Heptachlor


R.T.: 5.222 min
Delta R.T.: 0.025 min
Response: 1837442
Conc: 0.52 ng/ml

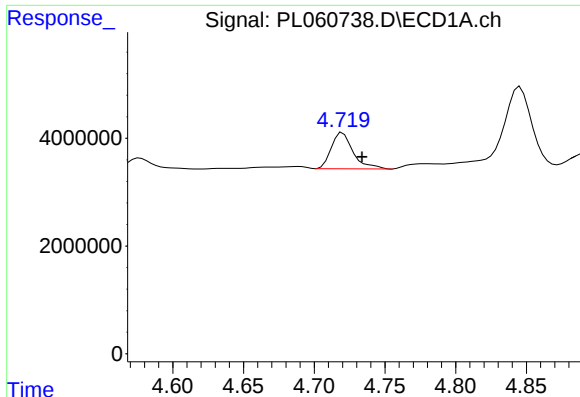

#5 Aldrin


R.T.: 4.720 min
Delta R.T.: -0.014 min
Response: 7203145
Conc: 3.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

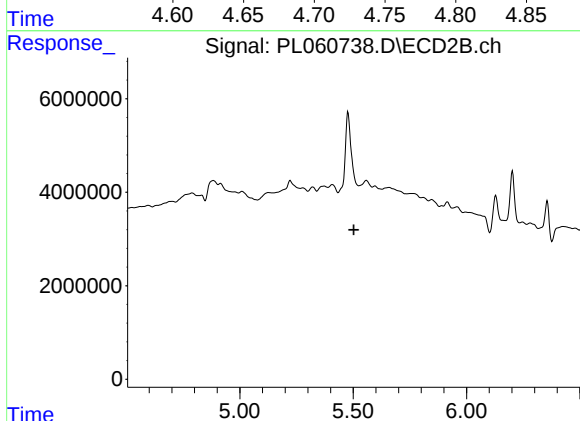


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.502 min
Response: 0
Conc: N.D.

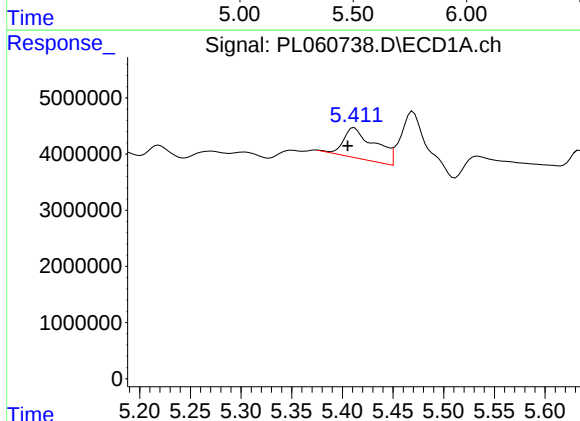


#10 gamma-Chlordane

R.T.: 5.412 min
Delta R.T.: 0.007 min
Response: 11774288
Conc: 5.55 ng/ml

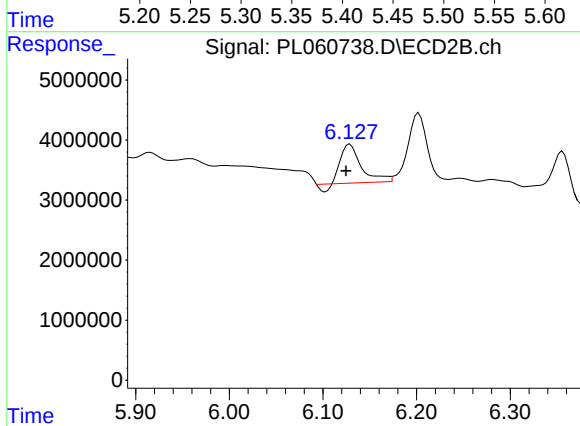

#10 gamma-Chlordane


R.T.: 6.129 min
Delta R.T.: 0.004 min
Response: 9505902
Conc: 3.14 ng/ml

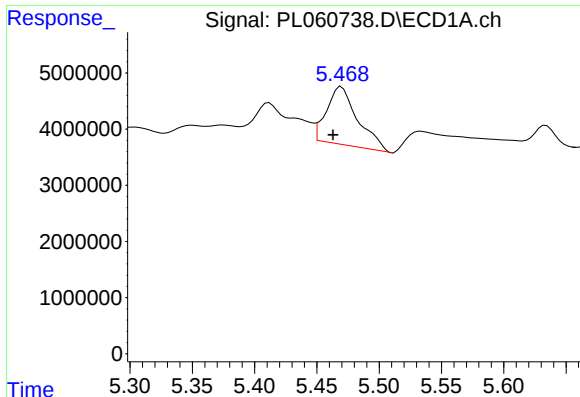

#11 alpha-Chlordane


R.T.: 5.470 min
Delta R.T.: 0.007 min
Response: 17931312
Conc: 8.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

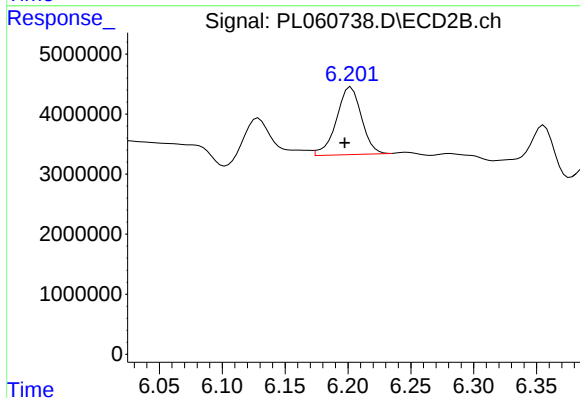


#11 alpha-Chlordane

R.T.: 6.202 min
Delta R.T.: 0.005 min
Response: 15576583
Conc: 5.07 ng/ml

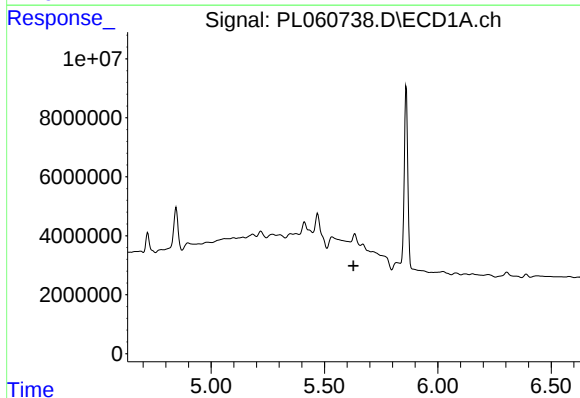


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.628 min
Response: 0
Conc: N.D.

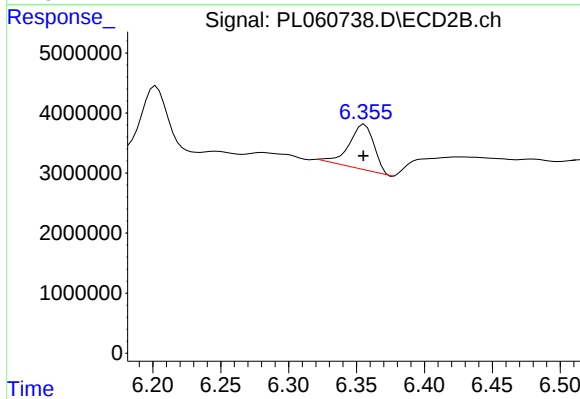

#12 4,4'-DDE


R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 9634525
Conc: 3.38 ng/ml

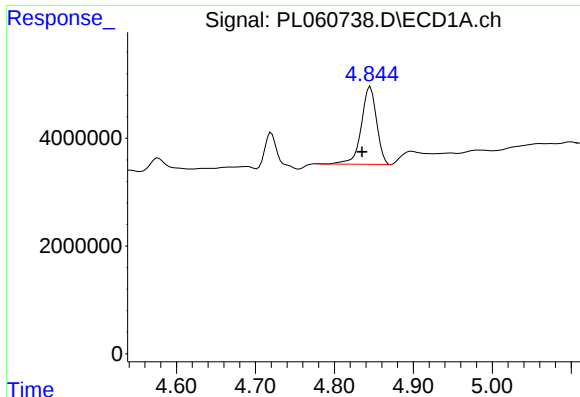

#24 Chlordane-2


R.T.: 4.846 min
Delta R.T.: 0.010 min
Response: 19288182
Conc: 304.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

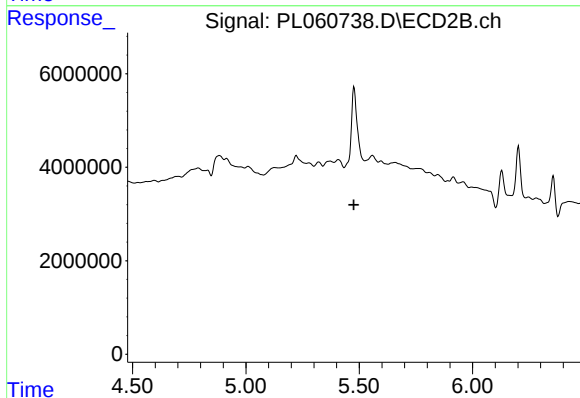


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.476 min
Response: 0
Conc: N.D.

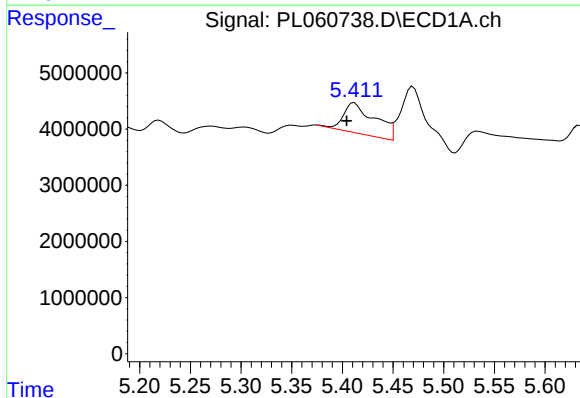


#25 Chlordane-3

R.T.: 5.412 min
Delta R.T.: 0.007 min
Response: 11774288
Conc: 67.18 ng/ml

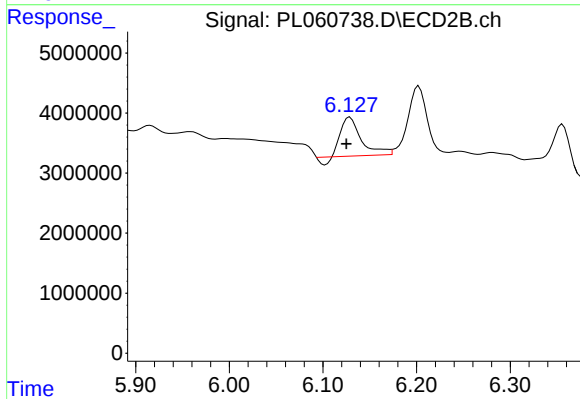

#25 Chlordane-3


R.T.: 6.129 min
Delta R.T.: 0.004 min
Response: 9505902
Conc: 26.25 ng/ml

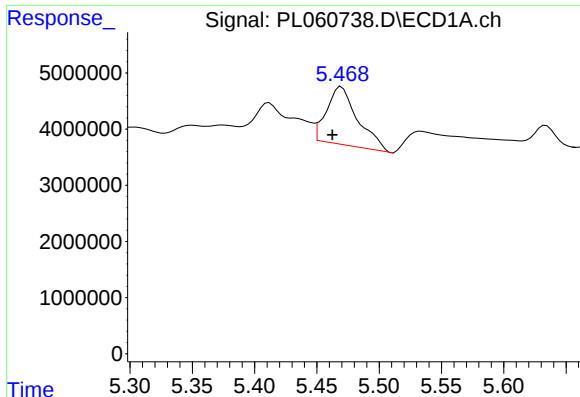

#26 Chlordane-4


R.T.: 5.470 min
Delta R.T.: 0.007 min
Response: 17931312
Conc: 128.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

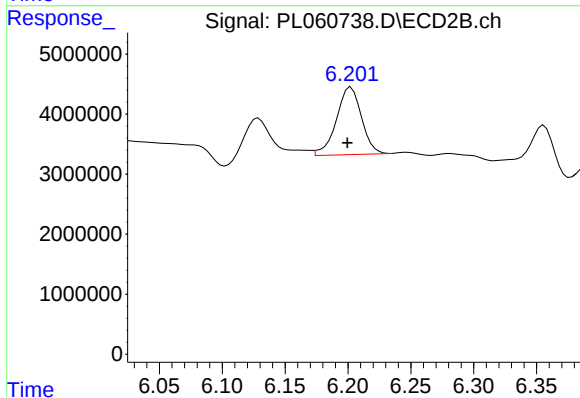


#26 Chlordane-4

R.T.: 6.202 min
Delta R.T.: 0.003 min
Response: 15576583
Conc: 35.93 ng/ml

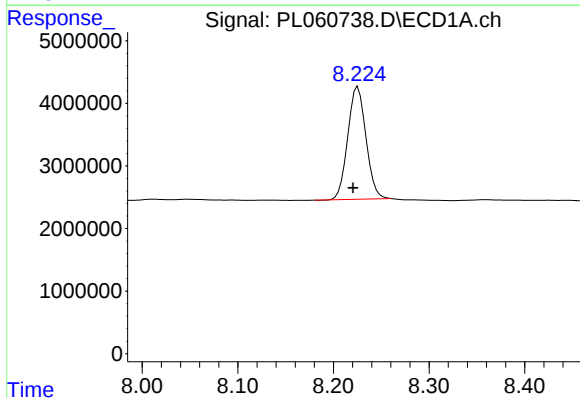

#28 Decachlorobiphenyl

R.T.: 8.226 min
Delta R.T.: 0.005 min
Response: 23905010
Conc: 13.10 ng/ml

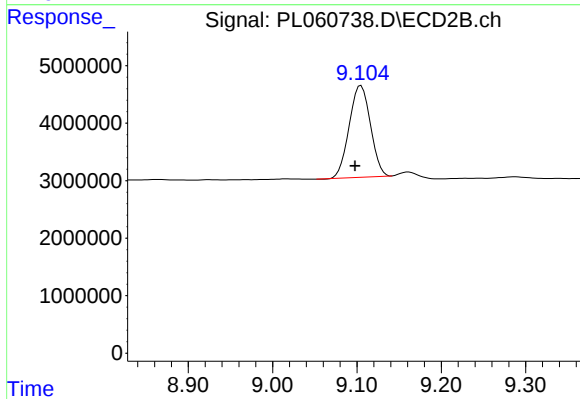

#28 Decachlorobiphenyl

R.T.: 9.105 min
Delta R.T.: 0.007 min
Response: 27940656
Conc: 14.89 ng/ml