

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081420\
 Data File : PL060742.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2020 13:29
 Operator : DD\AJ
 Sample : L3681-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 16:39:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 11 01:39:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.463	4.011	24489680	32608202	13.063	12.263
28)	SA Decachlor...	8.219	9.099	18882509	20569435	10.345	10.963
Target Compounds							
10)	B gamma-Chl...	0.000	6.131	0	3764269	N.D.	1.245 #
25)	Chlordane-3	0.000	6.131	0	3764269	N.D.	10.395 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081420\
Data File : PL060742.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2020 13:29
Operator : DD\AJ
Sample : L3681-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 16:39:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
Quant Title : GC Extractables
QLast Update : Tue Aug 11 01:39:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

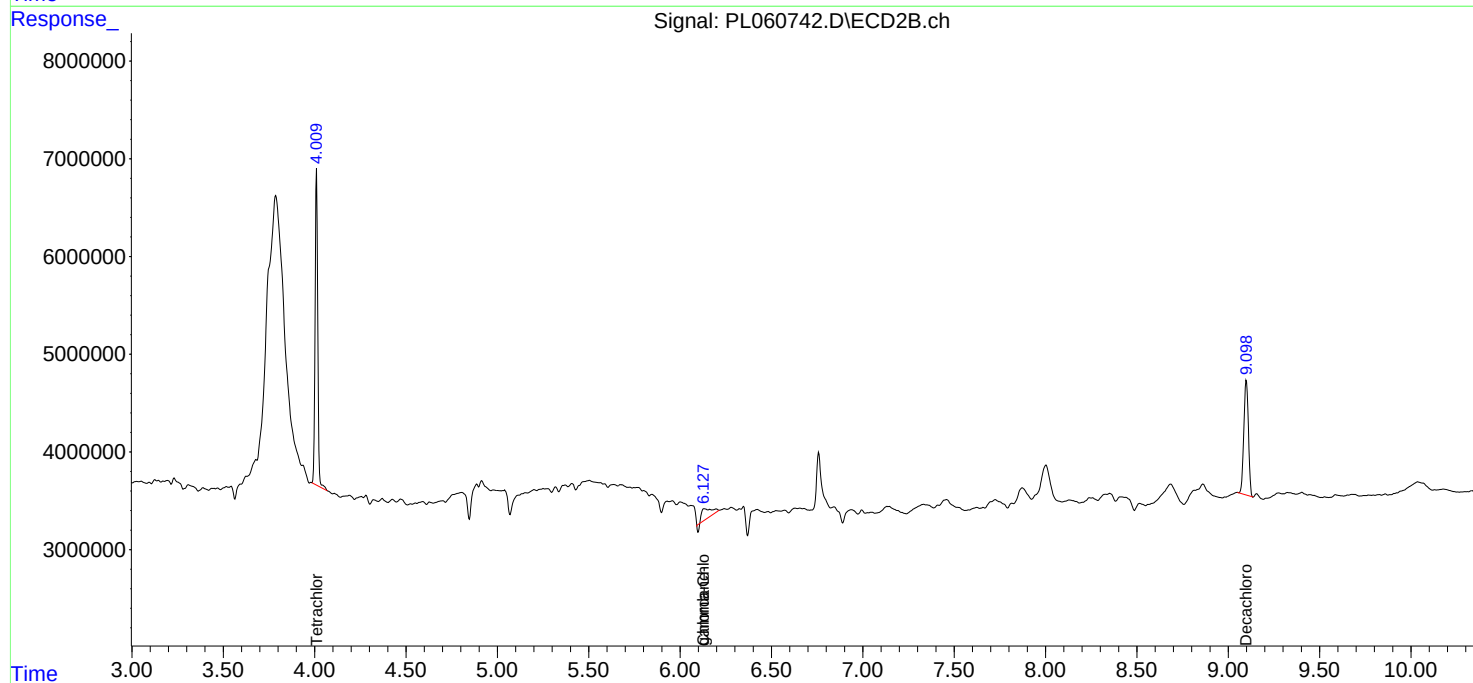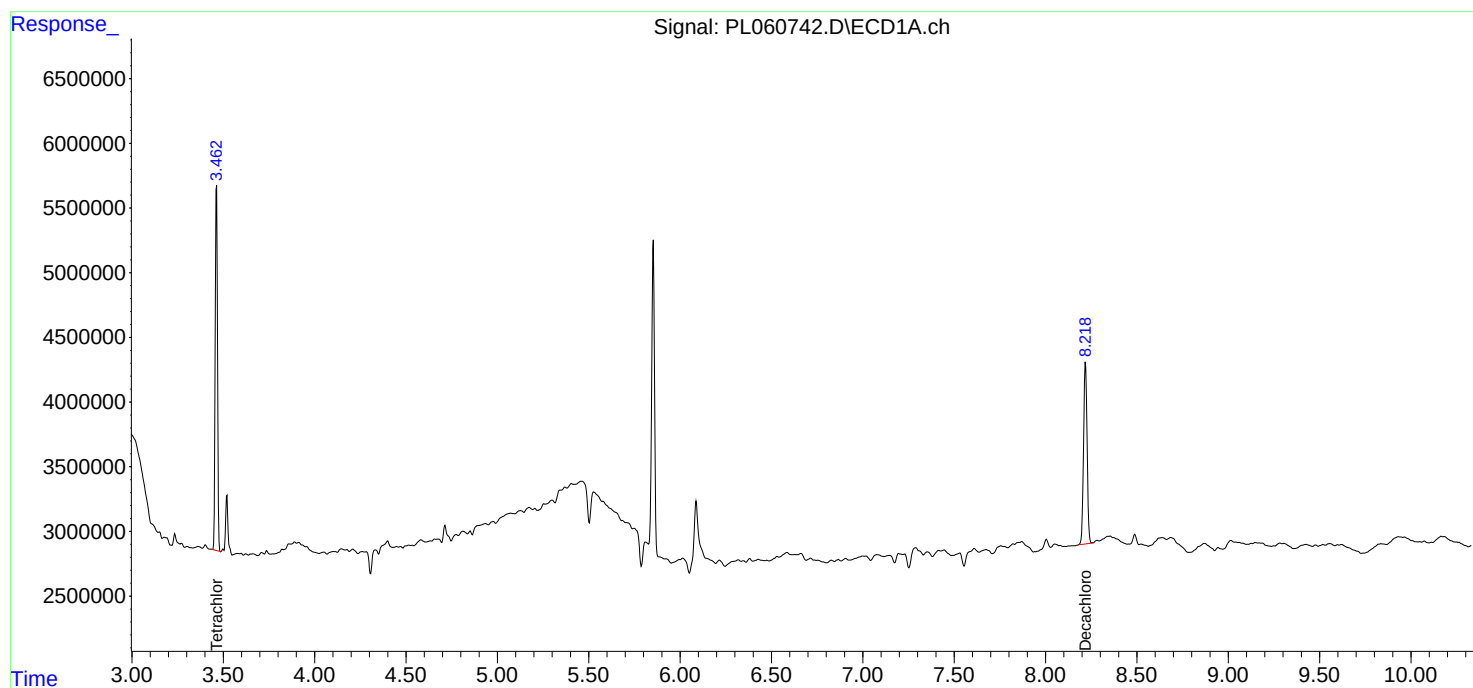


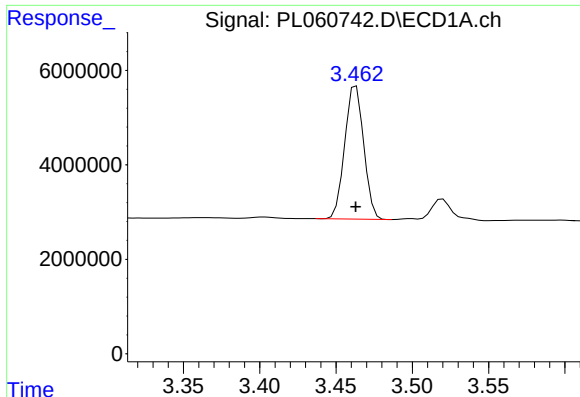

#1 Tetrachloro-m-xylene


R.T.: 3.463 min
Delta R.T.: 0.000 min
Response: 24489680
Conc: 13.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

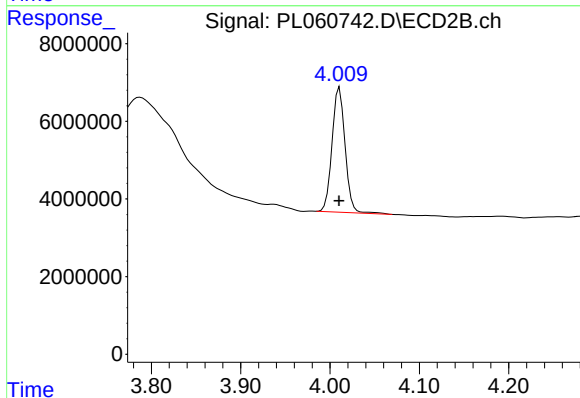


#1 Tetrachloro-m-xylene

R.T.: 4.011 min
Delta R.T.: 0.000 min
Response: 32608202
Conc: 12.26 ng/ml

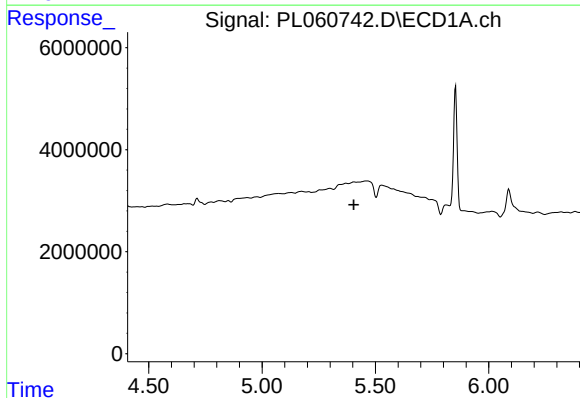


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.405 min
Response: 0
Conc: N.D.

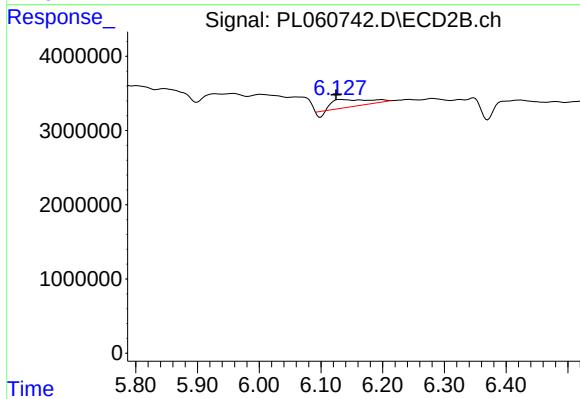

#10 gamma-Chlordane


R.T.: 6.131 min
Delta R.T.: 0.007 min
Response: 3764269
Conc: 1.25 ng/ml

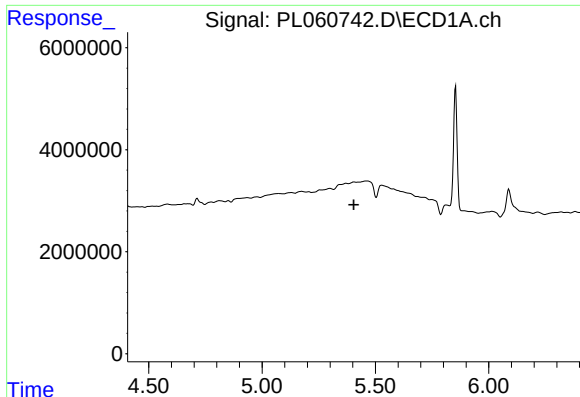

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.404 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

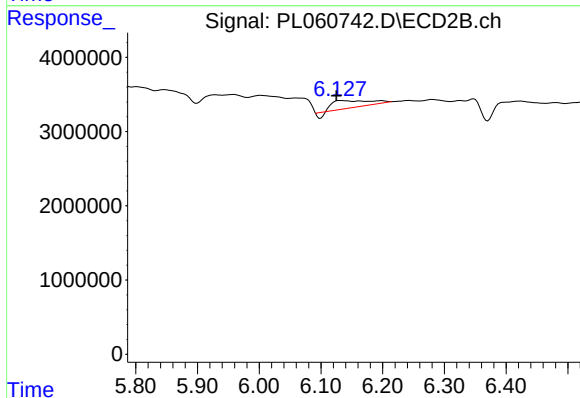


#25 Chlordane-3

R.T.: 6.131 min
Delta R.T.: 0.006 min
Response: 3764269
Conc: 10.40 ng/ml

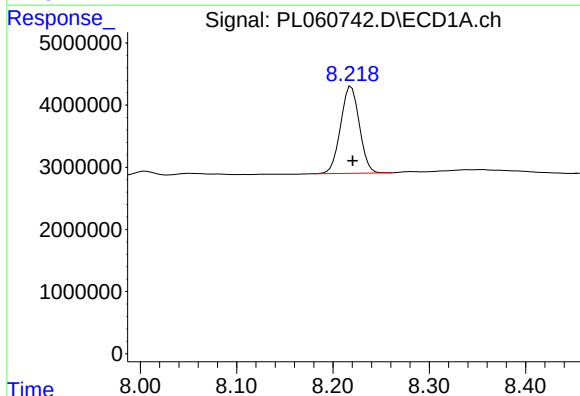

#28 Decachlorobiphenyl

R.T.: 8.219 min
Delta R.T.: -0.001 min
Response: 18882509
Conc: 10.34 ng/ml

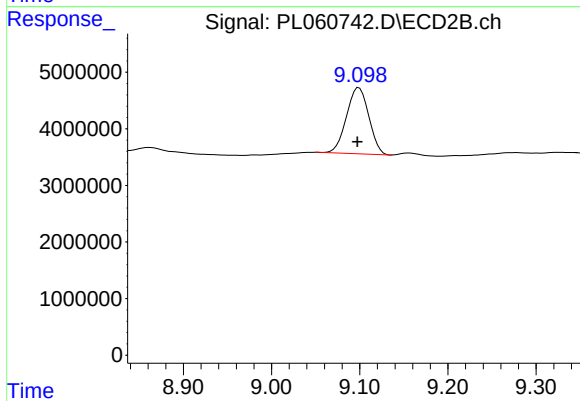

#28 Decachlorobiphenyl

R.T.: 9.099 min
Delta R.T.: 0.001 min
Response: 20569435
Conc: 10.96 ng/ml