

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081424\
 Data File : PL091073.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2024 21:14
 Operator : AR\AJ
 Sample : P3579-02
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VCPS-B1-081224-0-16

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/19/2024
 Supervised By :Ankita Jodhani 08/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 03:54:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081324.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 14 13:09:19 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.542	2.784	26517996	23340787	12.350m	11.957
2) SA Decachlor...	9.054	7.924	19760690	19477976	12.962	10.283

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081424\
Data File : PL091073.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2024 21:14
Operator : AR\AJ
Sample : P3579-02
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
VCPS-B1-081224-0-16


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/19/2024
Supervised By : Ankita Jodhani 08/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 03:54:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081324.M
Quant Title : GC Extractables
QLast Update : Wed Aug 14 13:09:19 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

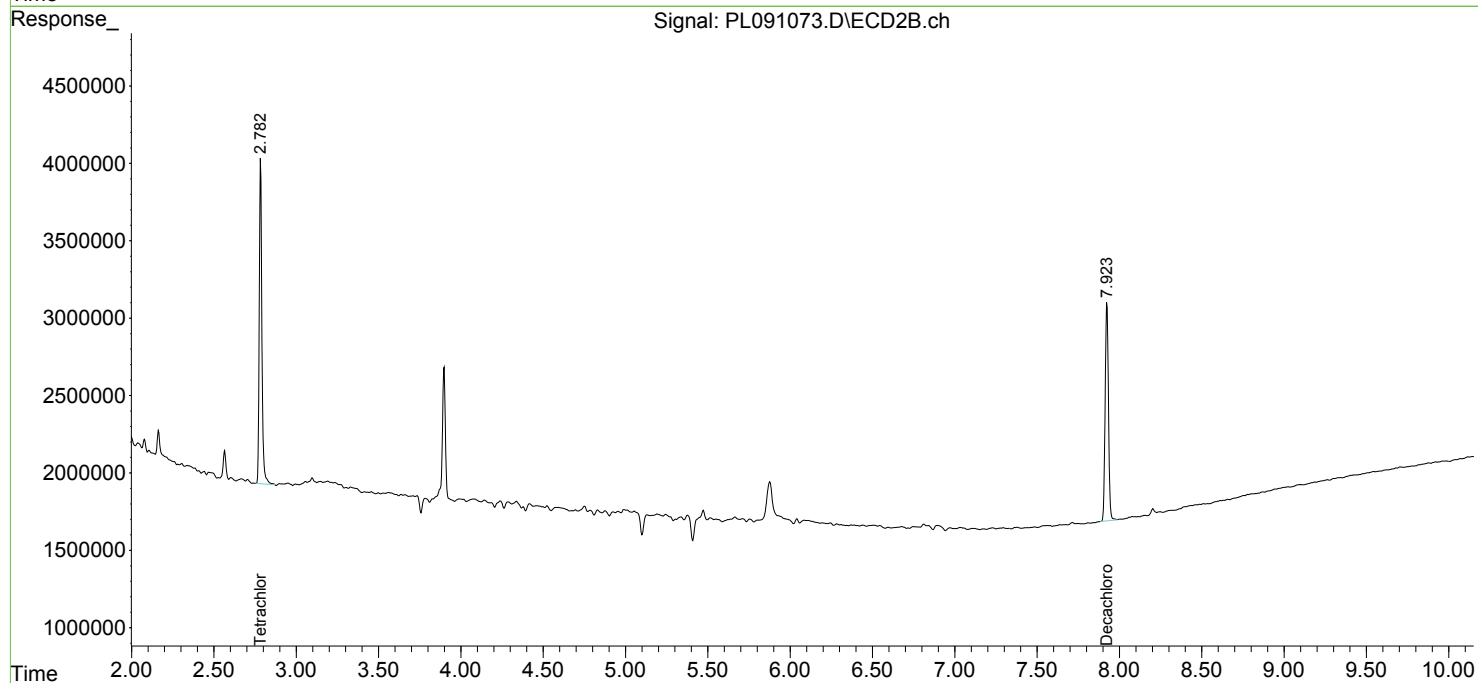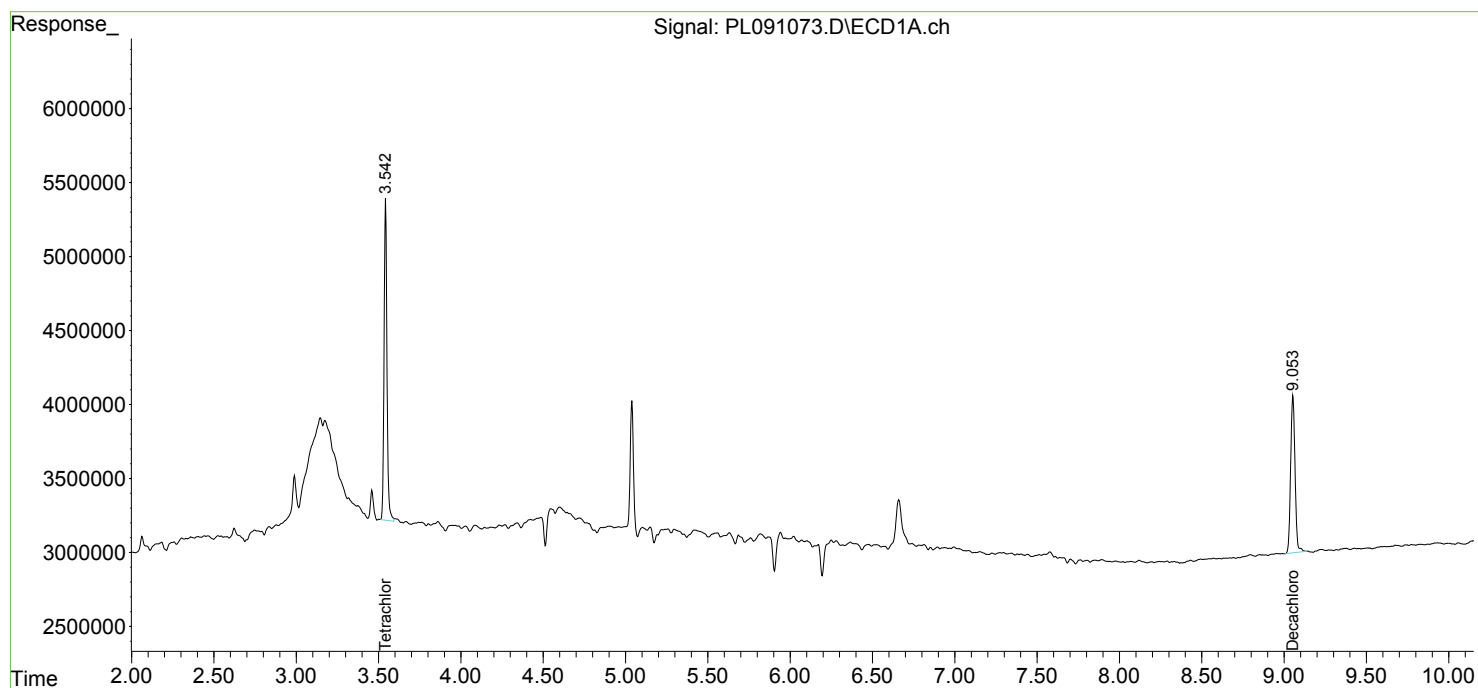

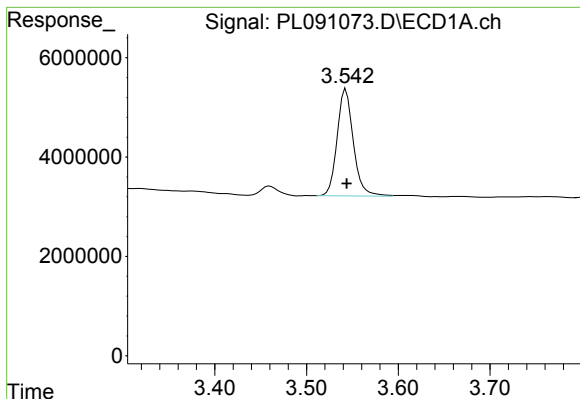


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: -0.002 min
Response: 26517996
Conc: 12.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
VCPS-B1-081224-0-16


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/19/2024
Supervised By :Ankita Jodhani 08/19/2024

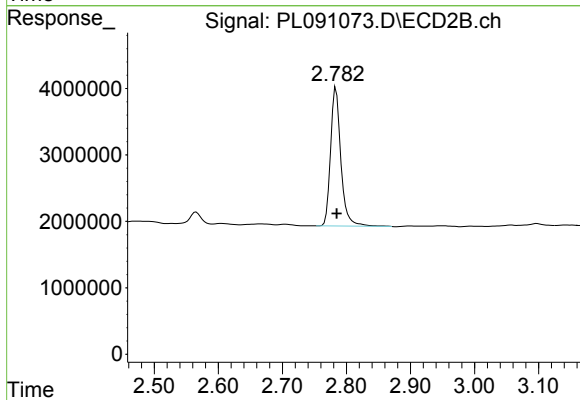


#1 Tetrachloro-m-xylene

R.T.: 2.784 min
Delta R.T.: -0.001 min
Response: 23340787
Conc: 11.96 ng/ml

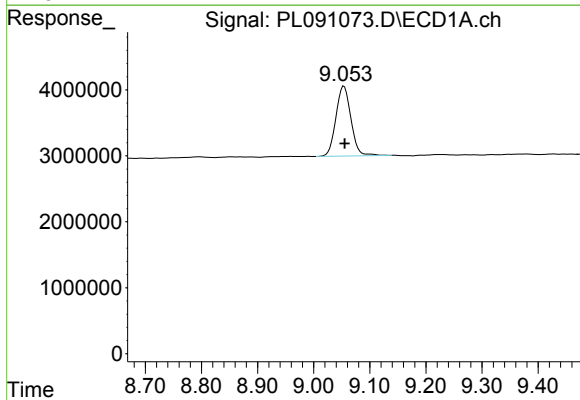

#28 Decachlorobiphenyl

R.T.: 9.054 min
Delta R.T.: -0.001 min
Response: 19760690
Conc: 12.96 ng/ml

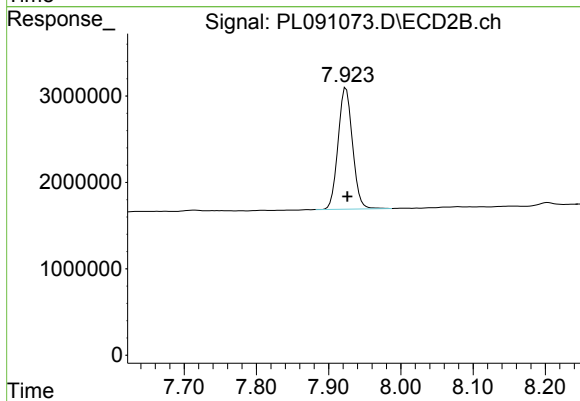

#28 Decachlorobiphenyl

R.T.: 7.924 min
Delta R.T.: -0.002 min
Response: 19477976
Conc: 10.28 ng/ml