

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081518\
 Data File : PL039141.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2018 10:23
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 15:04:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
1)	SA Tetrachlo...	3.322	0.000	1718686	0	0.246	N.D.	#
28)	SA Decachlor...	7.913f	0.000	118.6E6	0	16.883	N.D.	#
Target Compounds								
4)	MA Heptachlor	4.230f	0.000	5661465	0	0.538	N.D.	#
6)	B beta-BHC	4.230f	0.000	5661465	0	1.219	N.D.	#
9)	A Endosulfan I	5.273	0.000	3405634	0	0.389	N.D.	#
11)	B alpha-Chl...	5.273	0.000	3405634	0	0.354	N.D.	#
14)	MA Endrin	5.778	0.000	8472002	0	0.946	N.D.	#
16)	A 4,4'-DDD	5.946	0.000	1717151	0	0.215	N.D.	#
17)	MA 4,4'-DDT	6.172	0.000	98427406	0	12.984	N.D.	#
18)	B Endrin al...	6.260	0.000	5317422	0	0.785	N.D.	#
23)	Chlordane-1	4.075	0.000	5532269	0	17.475	N.D.	#
24)	Chlordane-2	4.703	0.000	36641614	0	104.813	N.D.	#
26)	Chlordane-4	5.273	0.000	3405634	0	3.408	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081518\
Data File : PL039141.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2018 10:23
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 15:04:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

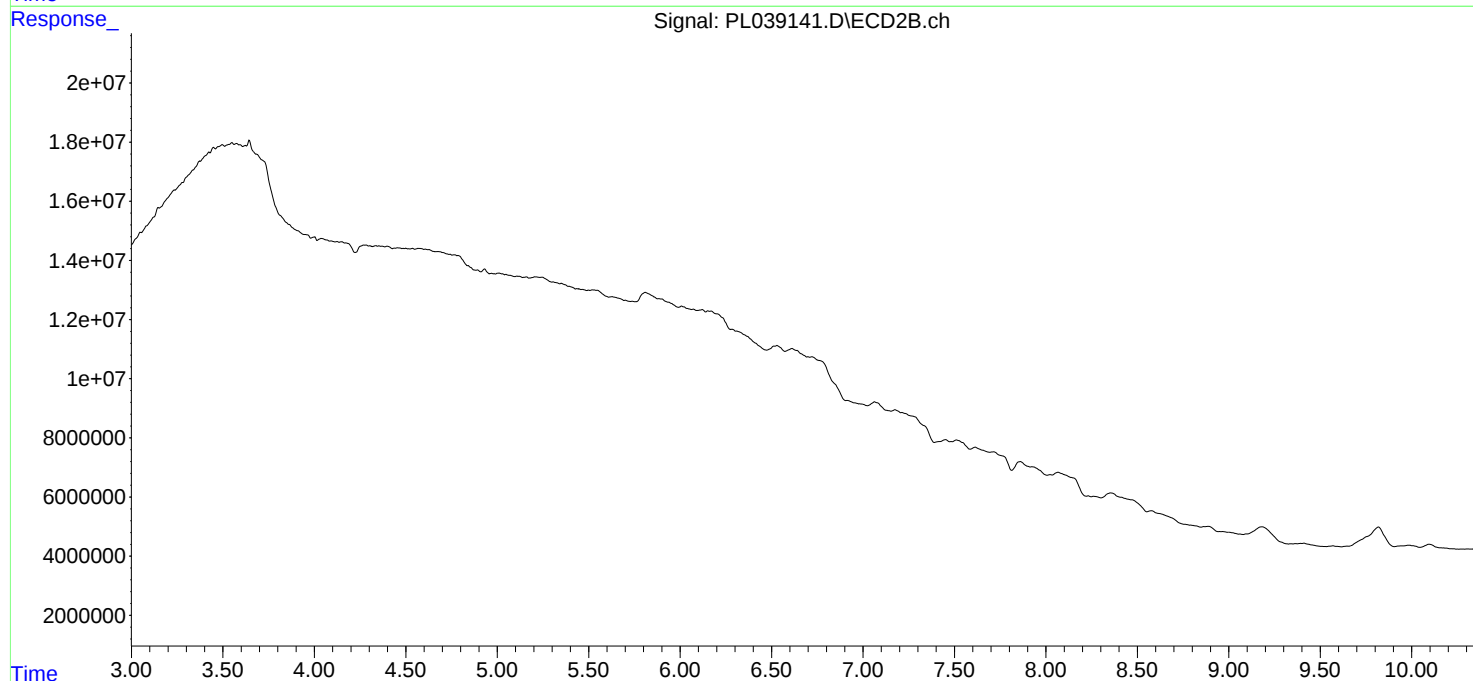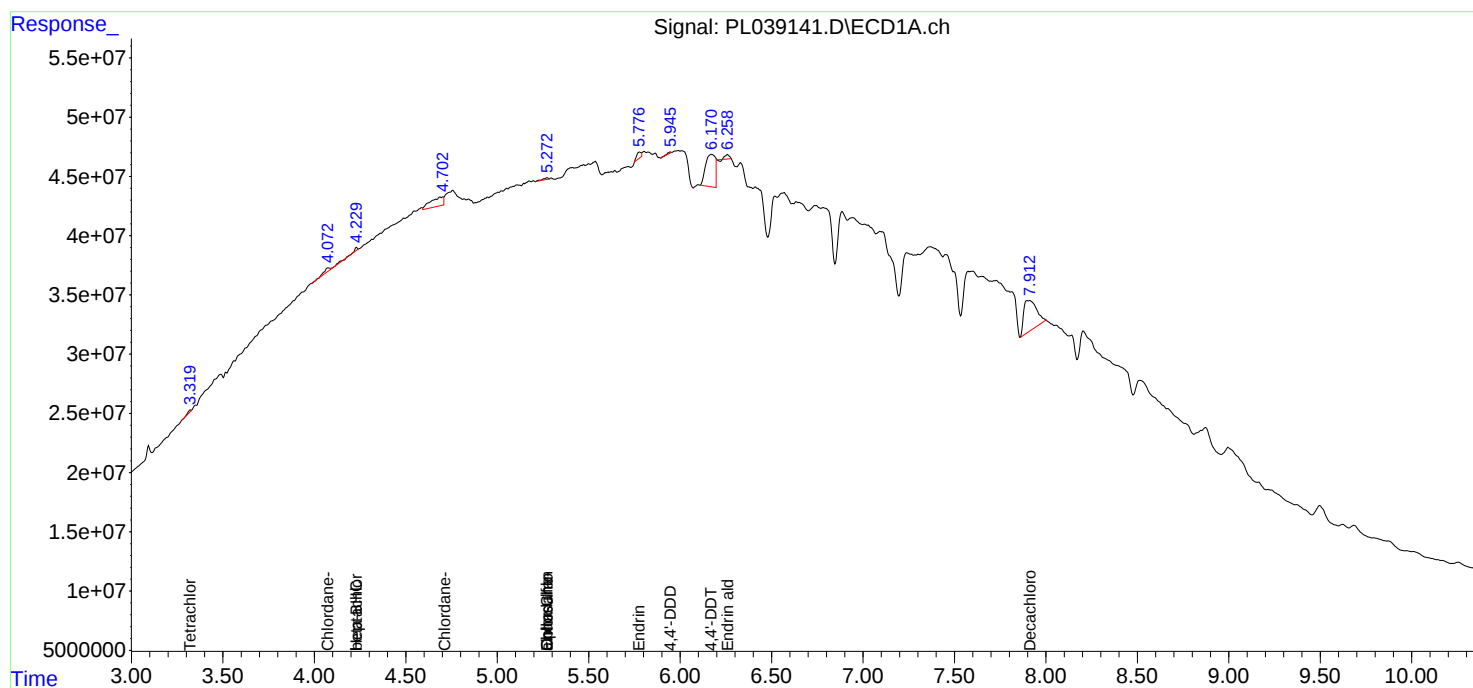


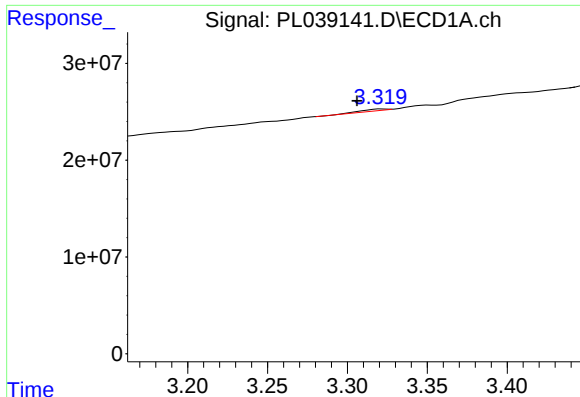

#1 Tetrachloro-m-xylene


R.T.: 3.322 min
Delta R.T.: 0.016 min
Response: 1718686
Conc: 0.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

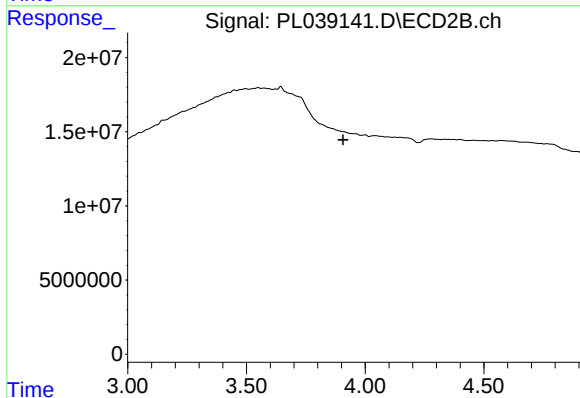


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.907 min
Response: 0
Conc: N.D.

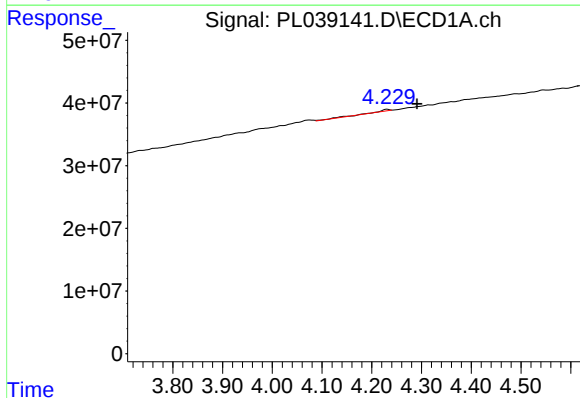


#4 Heptachlor

R.T.: 4.230 min
Delta R.T.: -0.061 min
Response: 5661465
Conc: 0.54 ng/ml

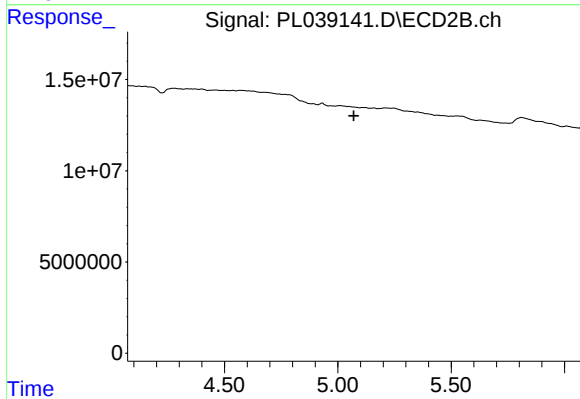

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.071 min
Response: 0
Conc: N.D.

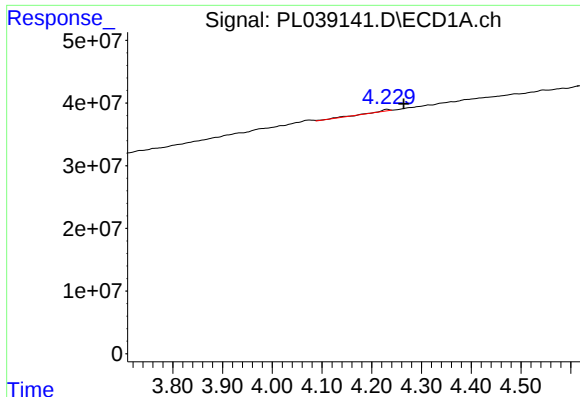

#6 beta-BHC


R.T.: 4.230 min
Delta R.T.: -0.034 min
Response: 5661465
Conc: 1.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

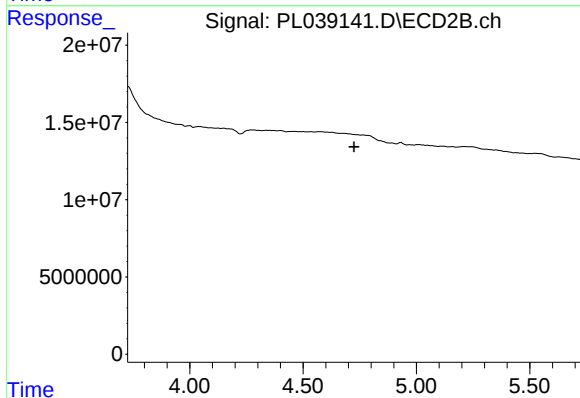


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

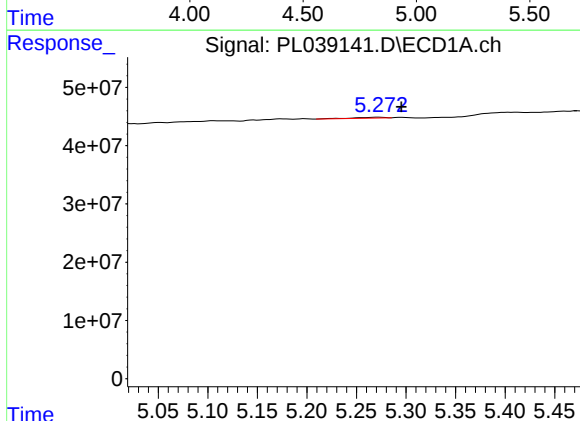


#9 Endosulfan I

R.T.: 5.273 min
Delta R.T.: -0.022 min
Response: 3405634
Conc: 0.39 ng/ml

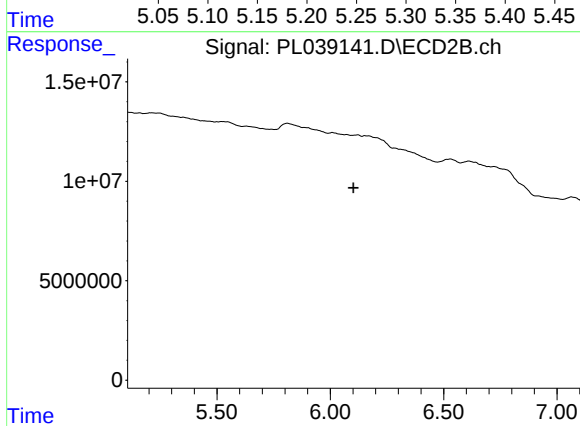

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.102 min
Response: 0
Conc: N.D.

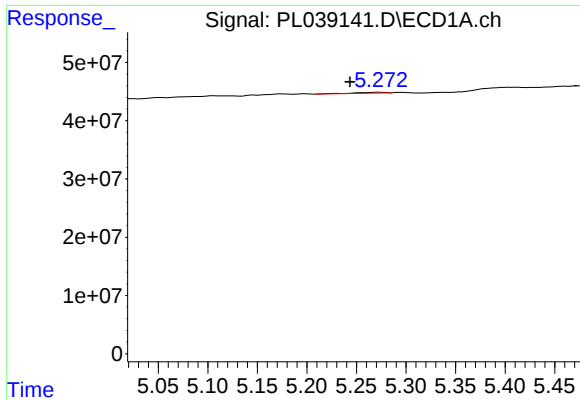

#11 alpha-Chlordane


R.T.: 5.273 min
Delta R.T.: 0.030 min
Response: 3405634
Conc: 0.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

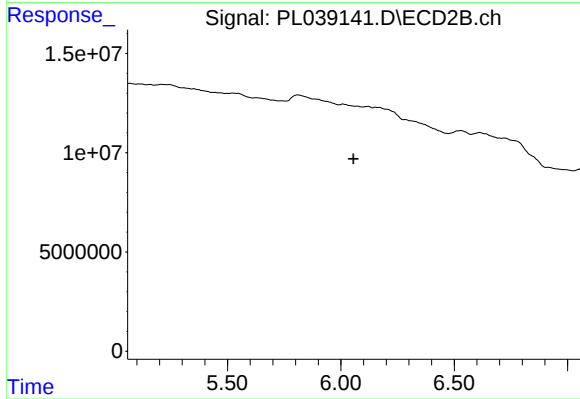


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.056 min
Response: 0
Conc: N.D.

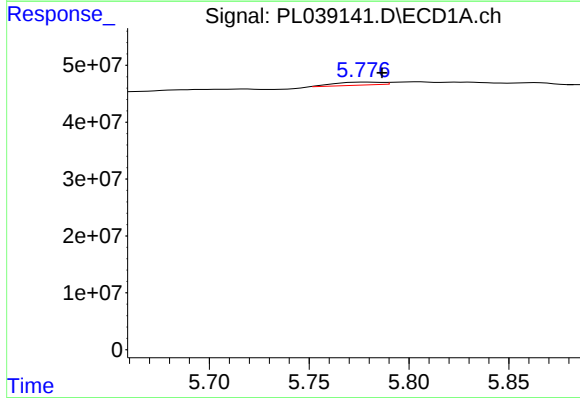


#14 Endrin

R.T.: 5.778 min
Delta R.T.: -0.009 min
Response: 8472002
Conc: 0.95 ng/ml

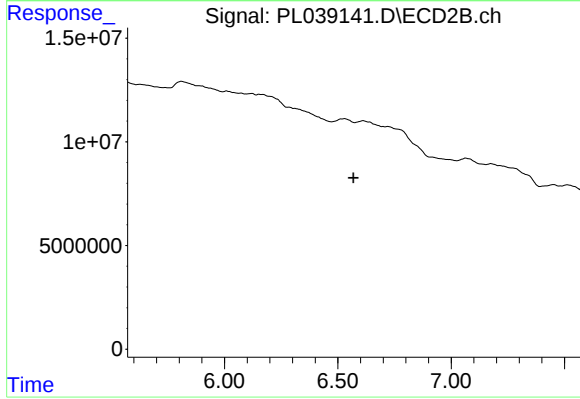

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.570 min
Response: 0
Conc: N.D.

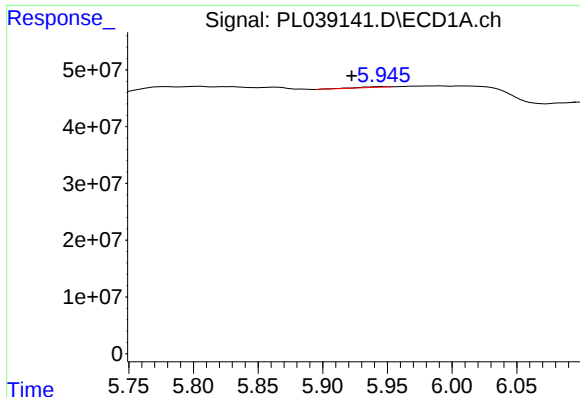

#16 4,4'-DDD


R.T.: 5.946 min
Delta R.T.: 0.024 min
Response: 1717151
Conc: 0.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

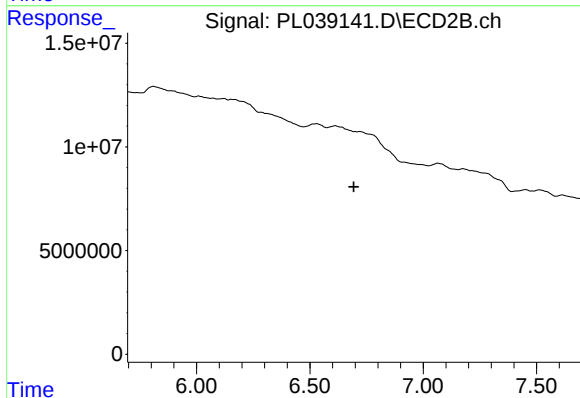


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.693 min
Response: 0
Conc: N.D.

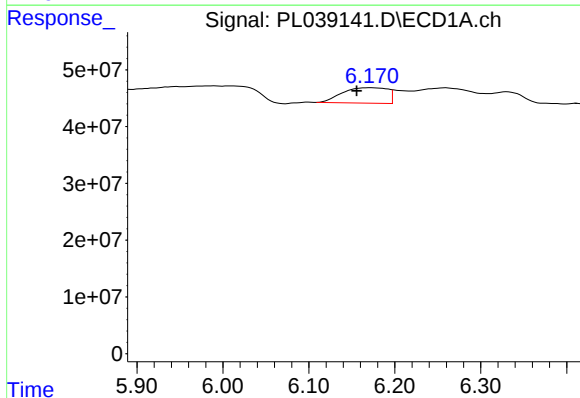


#17 4,4'-DDT

R.T.: 6.172 min
Delta R.T.: 0.016 min
Response: 98427406
Conc: 12.98 ng/ml

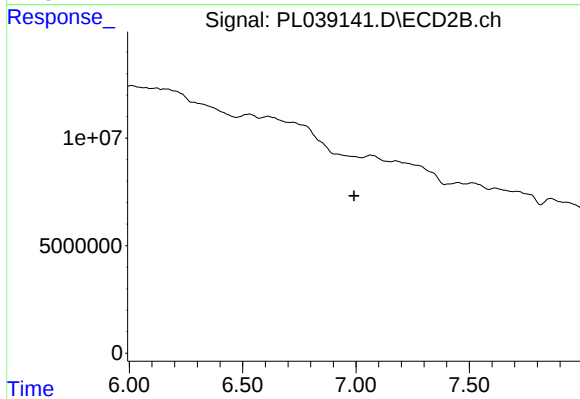

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.991 min
Response: 0
Conc: N.D.

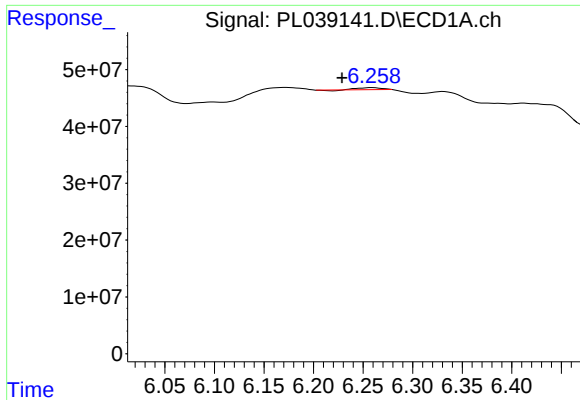

#18 Endrin aldehyde


R.T.: 6.260 min
Delta R.T.: 0.031 min
Response: 5317422
Conc: 0.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

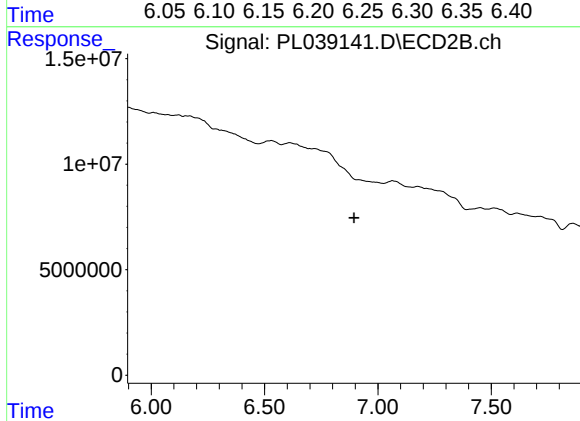


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.895 min
Response: 0
Conc: N.D.

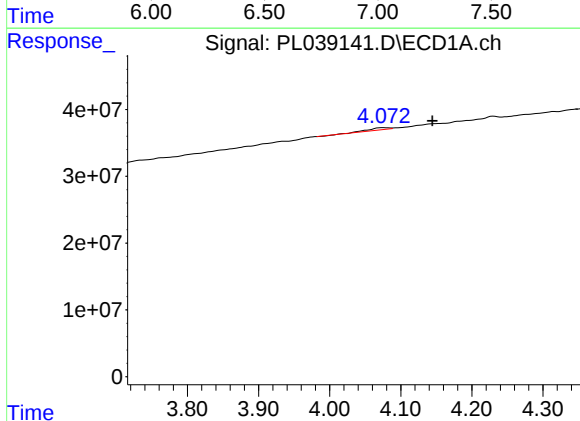


#23 Chlordane-1

R.T.: 4.075 min
Delta R.T.: -0.070 min
Response: 5532269
Conc: 17.47 ng/ml

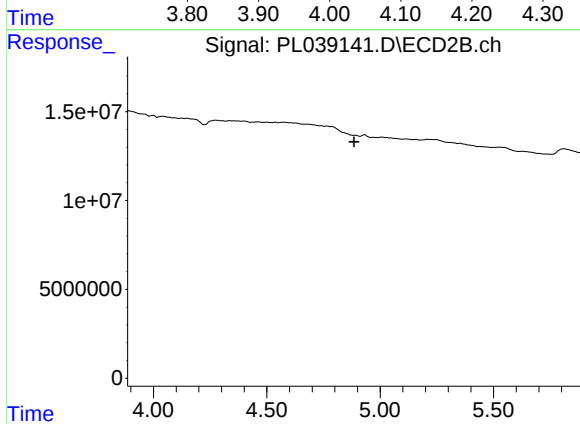

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

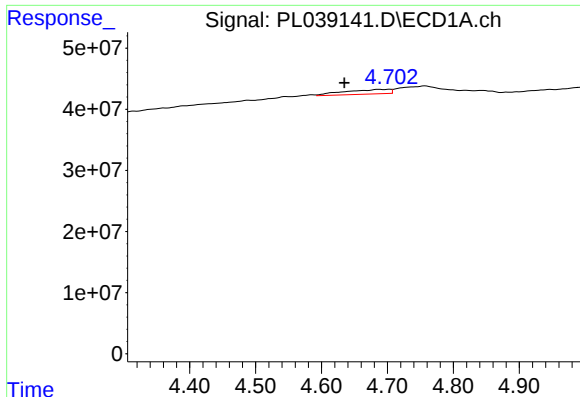

#24 Chlordane-2


R.T.: 4.703 min
Delta R.T.: 0.069 min
Response: 36641614
Conc: 104.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

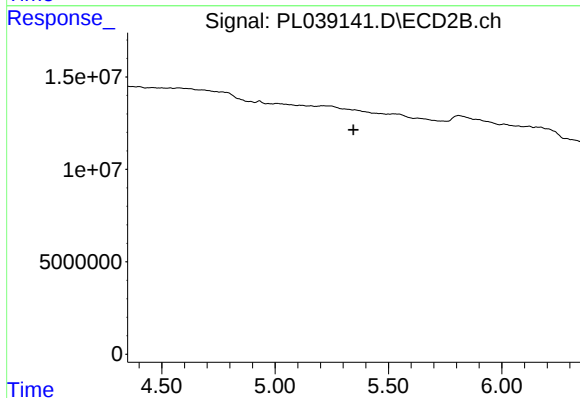


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.346 min
Response: 0
Conc: N.D.

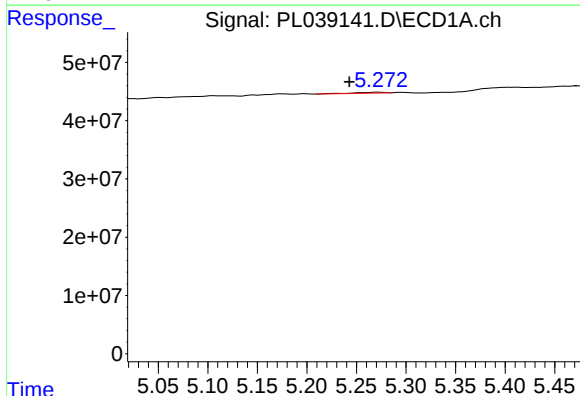


#26 Chlordane-4

R.T.: 5.273 min
Delta R.T.: 0.030 min
Response: 3405634
Conc: 3.41 ng/ml

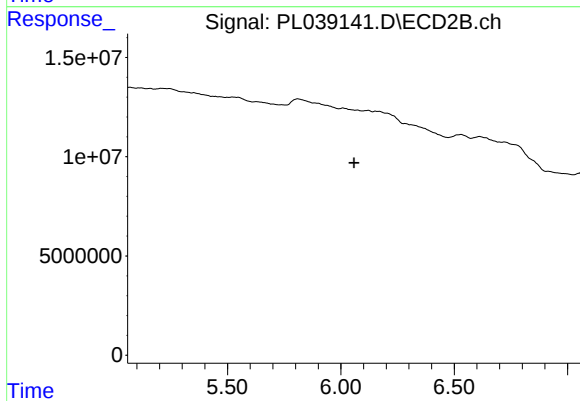

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.058 min
Response: 0
Conc: N.D.

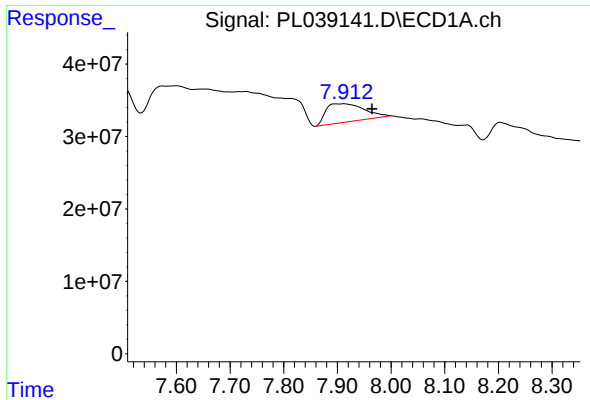

#28 Decachlorobiphenyl

R.T.: 7.913 min
Delta R.T.: -0.051 min
Response: 118577769
Conc: 16.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

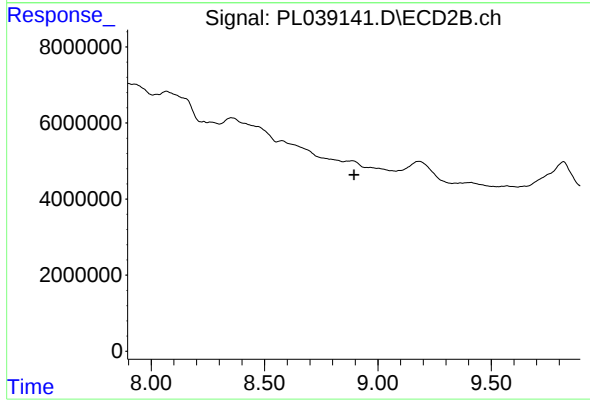

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.896 min
Response: 0
Conc: N.D.