

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081518\
 Data File : PL039175.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2018 04:43
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 06:57:21 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.906	138.2E6	53561244	19.769	19.979
28)	SA Decachlor...	7.972	8.898	133.5E6	47607989	19.003	20.444
Target Compounds							
4)	MA Heptachlor	4.226f	0.000	6863055	0	0.652	N.D. #
8)	B Heptachlo...	0.000	5.769	0	6509841	N.D.	1.886 #
9)	A Endosulfan I	5.267	0.000	9806441	0	1.120	N.D. #
11)	B alpha-Chl...	5.267	0.000	9806441	0	1.021	N.D. #
23)	Chlordane-1	4.073	0.000	61689143	0	194.857	N.D. #
26)	Chlordane-4	5.267	0.000	9806441	0	9.813	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081518\
Data File : PL039175.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2018 04:43
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 06:57:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

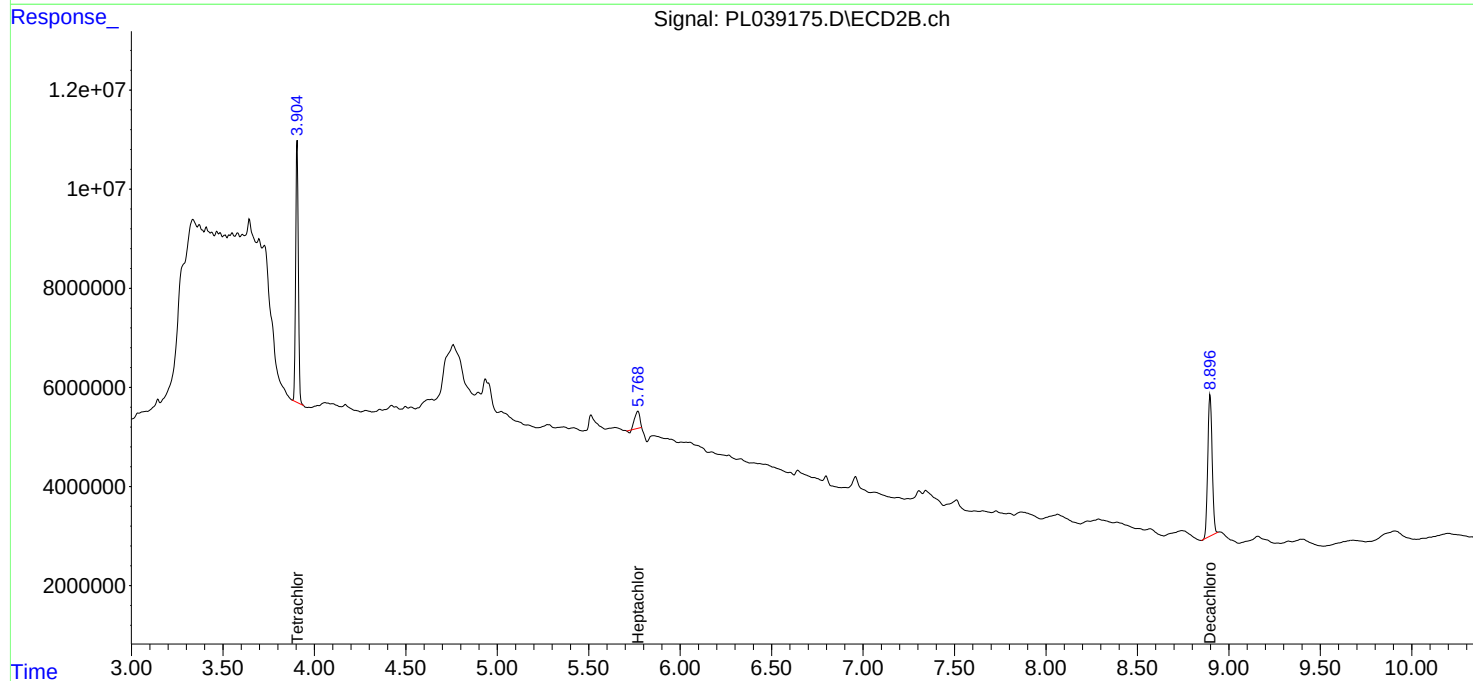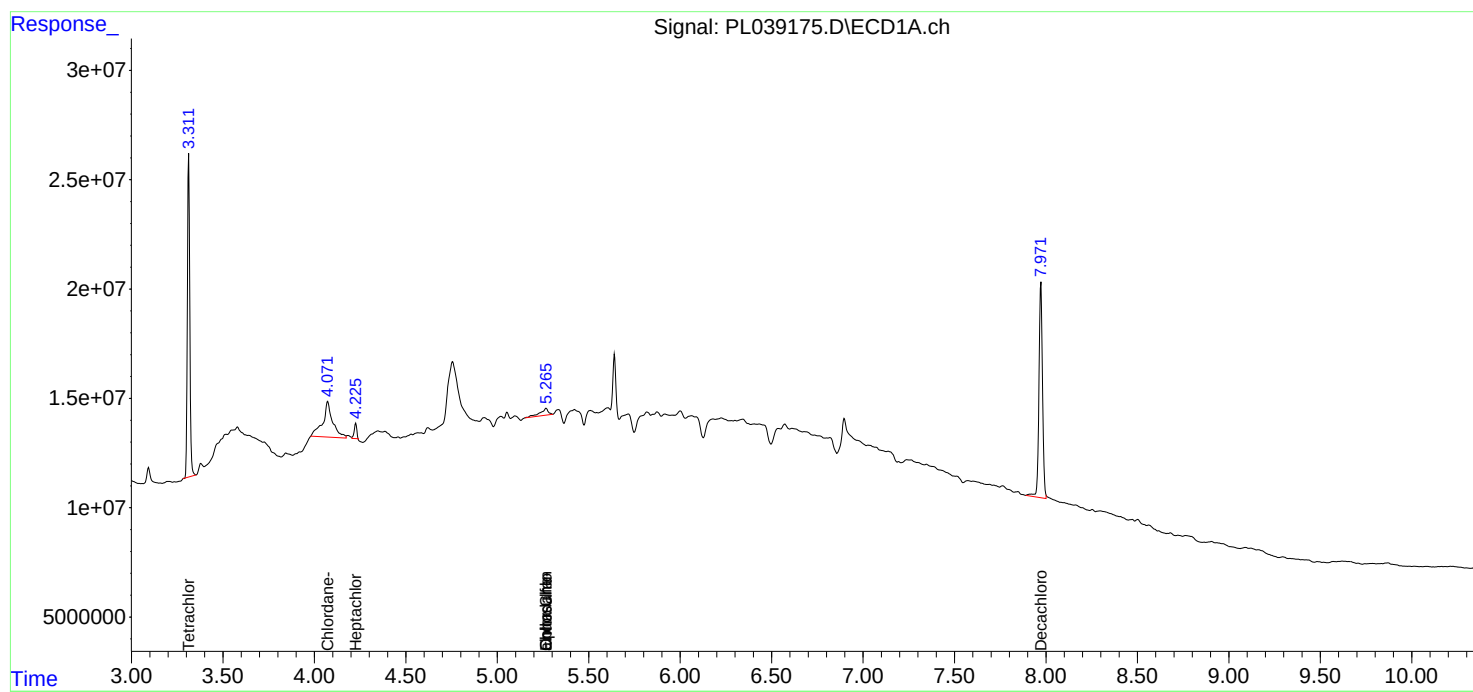


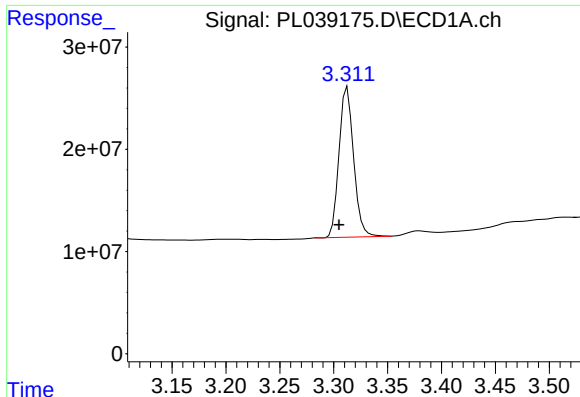

#1 Tetrachloro-m-xylene


R.T.: 3.313 min
Delta R.T.: 0.008 min
Response: 138190847
Conc: 19.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

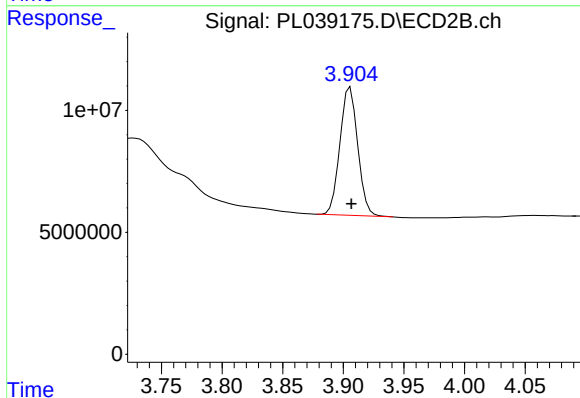


#1 Tetrachloro-m-xylene

R.T.: 3.906 min
Delta R.T.: -0.001 min
Response: 53561244
Conc: 19.98 ng/ml

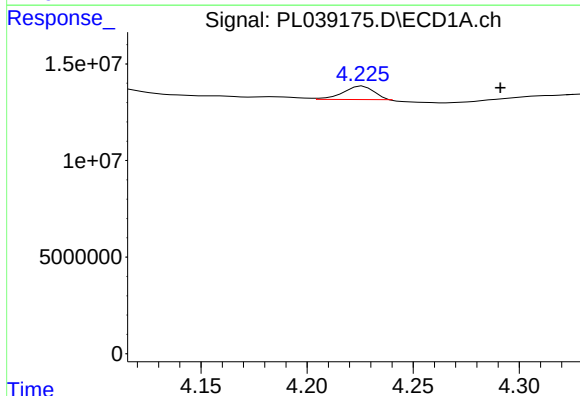


#4 Heptachlor

R.T.: 4.226 min
Delta R.T.: -0.065 min
Response: 6863055
Conc: 0.65 ng/ml

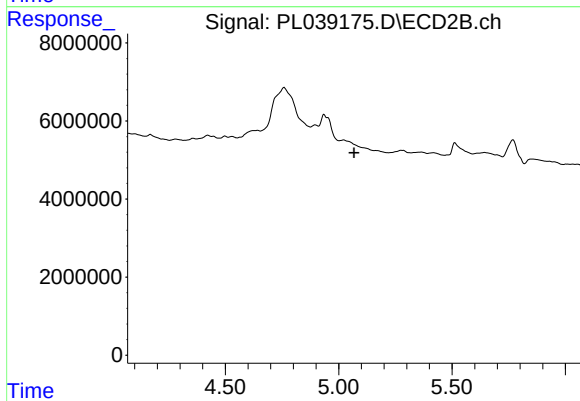

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.069 min
Response: 0
Conc: N.D.

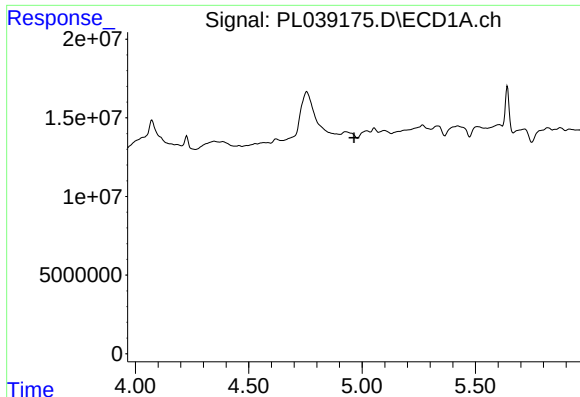

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.965 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

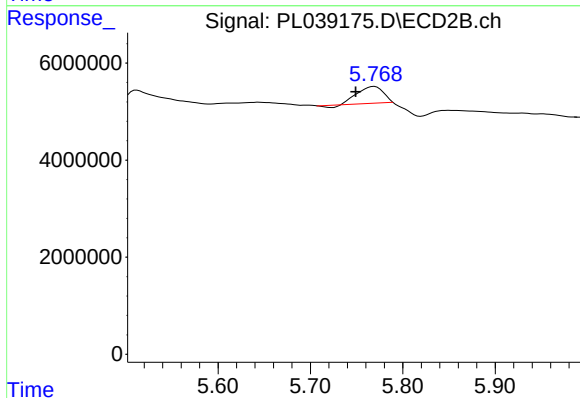


#8 Heptachlor epoxide

R.T.: 5.769 min
Delta R.T.: 0.020 min
Response: 6509841
Conc: 1.89 ng/ml

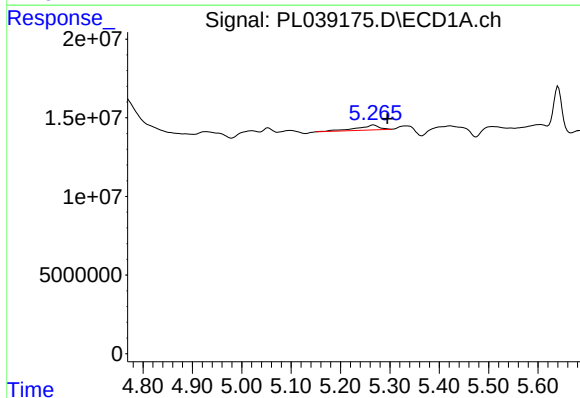


#9 Endosulfan I

R.T.: 5.267 min
Delta R.T.: -0.028 min
Response: 9806441
Conc: 1.12 ng/ml

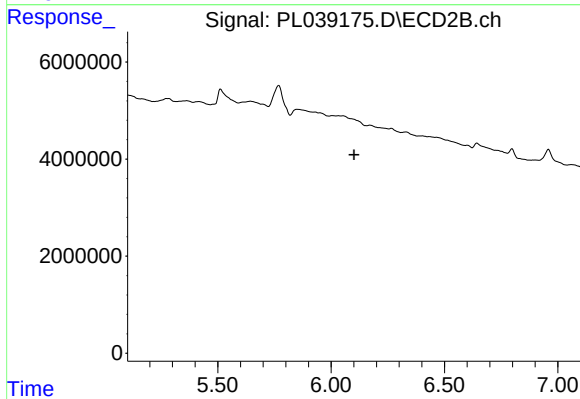

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.101 min
Response: 0
Conc: N.D.

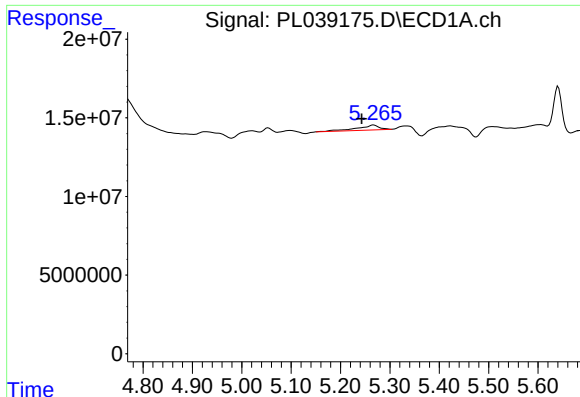

#11 alpha-Chlordane


R.T.: 5.267 min
Delta R.T.: 0.024 min
Response: 9806441
Conc: 1.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

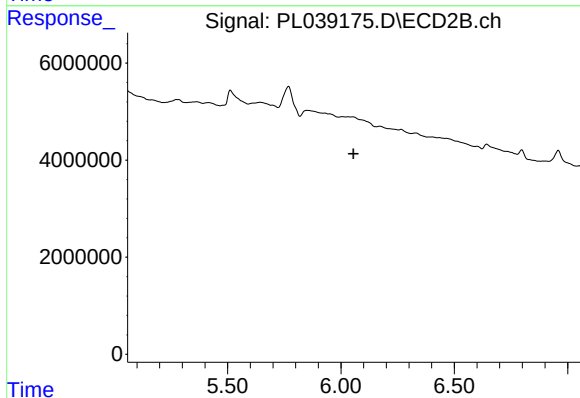


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.055 min
Response: 0
Conc: N.D.

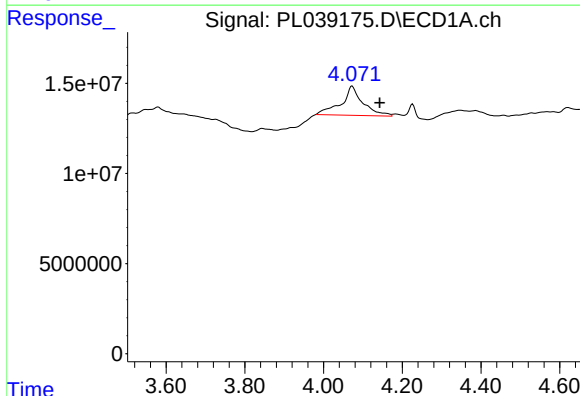


#23 Chlordane-1

R.T.: 4.073 min
Delta R.T.: -0.070 min
Response: 61689143
Conc: 194.86 ng/ml

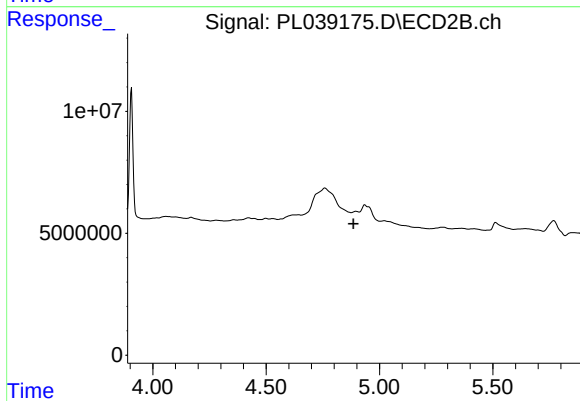

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

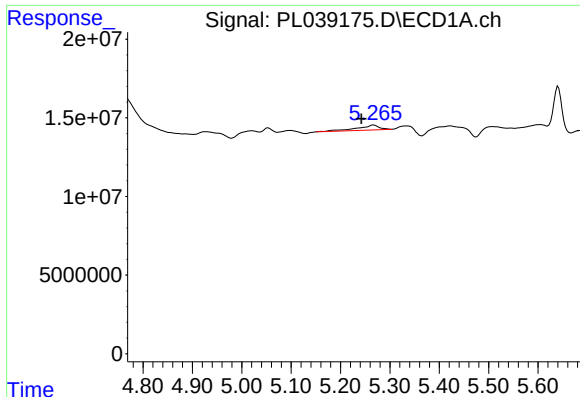

#26 Chlordane-4


R.T.: 5.267 min
Delta R.T.: 0.024 min
Response: 9806441
Conc: 9.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

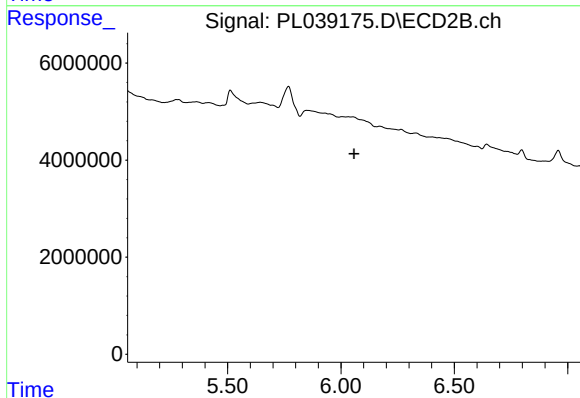


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.058 min
Response: 0
Conc: N.D.

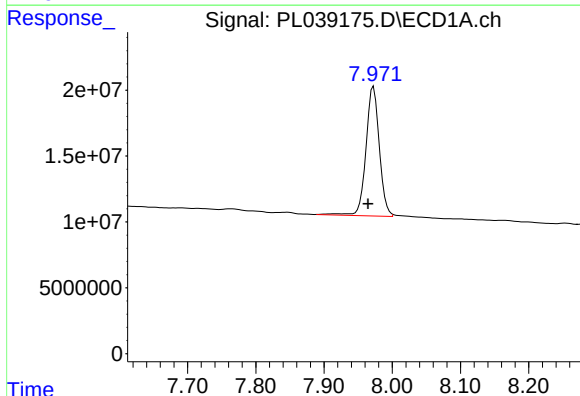

#28 Decachlorobiphenyl

R.T.: 7.972 min
Delta R.T.: 0.008 min
Response: 133462813
Conc: 19.00 ng/ml

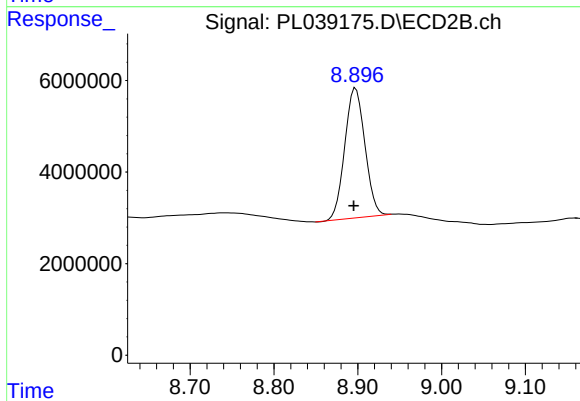

#28 Decachlorobiphenyl

R.T.: 8.898 min
Delta R.T.: 0.002 min
Response: 47607989
Conc: 20.44 ng/ml