

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081518\
 Data File : PL039184.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2018 06:51
 Operator : AJ\SJ
 Sample : J4477-01
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 08:19:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.304	3.907	88100734	35723217	12.603	13.325
28)	SA Decachlor...	7.963	8.894	165.3E6	32749386	23.540	14.063 #
Target Compounds							
9)	A Endosulfan I	5.240f	0.000	9654271	0	1.103	N.D. #
10)	B gamma-Chl...	5.205	0.000	14953004	0	1.514	N.D. #
11)	B alpha-Chl...	5.240	0.000	9654271	0	1.005	N.D. #
12)	B 4,4'-DDE	5.410	0.000	8805327	0	0.920	N.D. #
17)	MA 4,4'-DDT	6.153	0.000	27490726	0	3.626	N.D. #
20)	A Methoxychlor	6.676	0.000	9865699	0	2.411	N.D. #
23)	Chlordane-1	4.143	0.000	8333298	0	26.322	N.D. #
24)	Chlordane-2	4.634	0.000	8818463	0	25.225	N.D. #
25)	Chlordane-3	5.205	0.000	14953004	0	13.690	N.D. #
26)	Chlordane-4	5.240	0.000	9654271	0	9.661	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081518\
Data File : PL039184.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2018 06:51
Operator : AJ\SJ
Sample : J4477-01
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 08:19:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

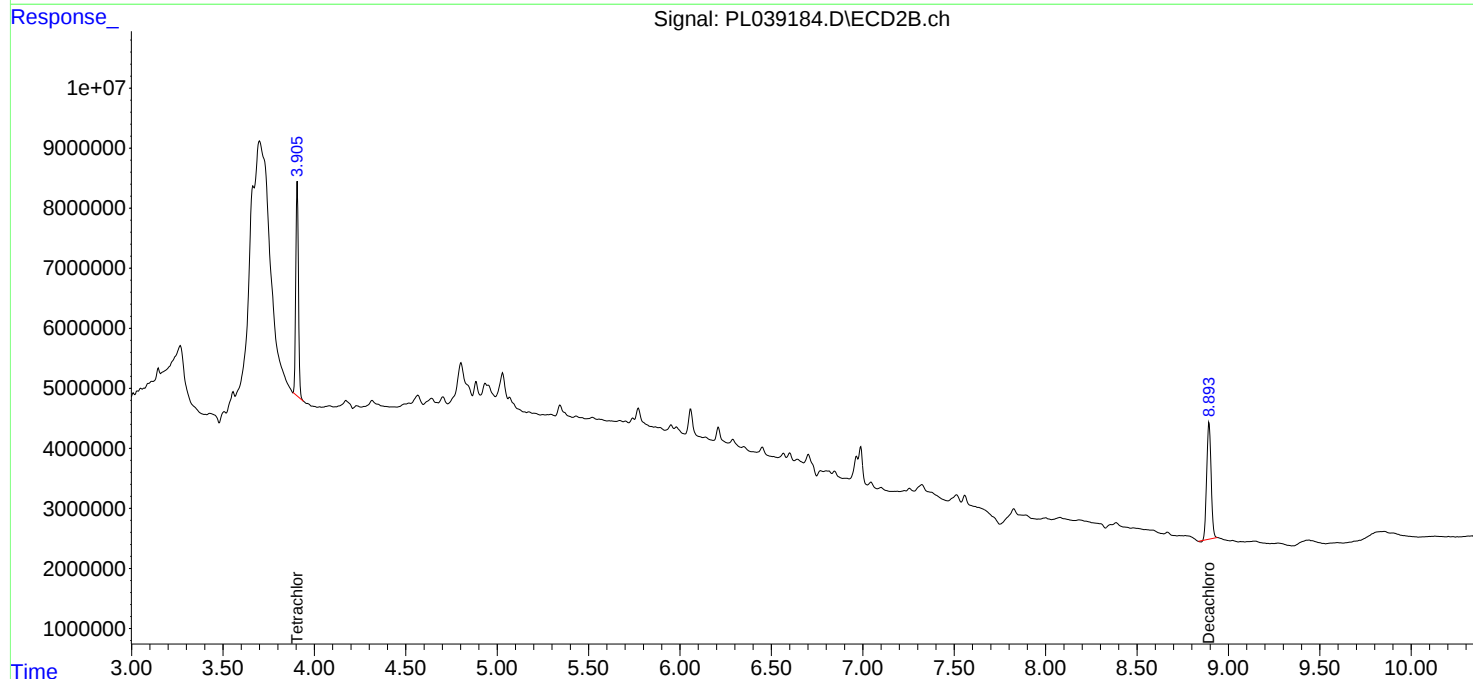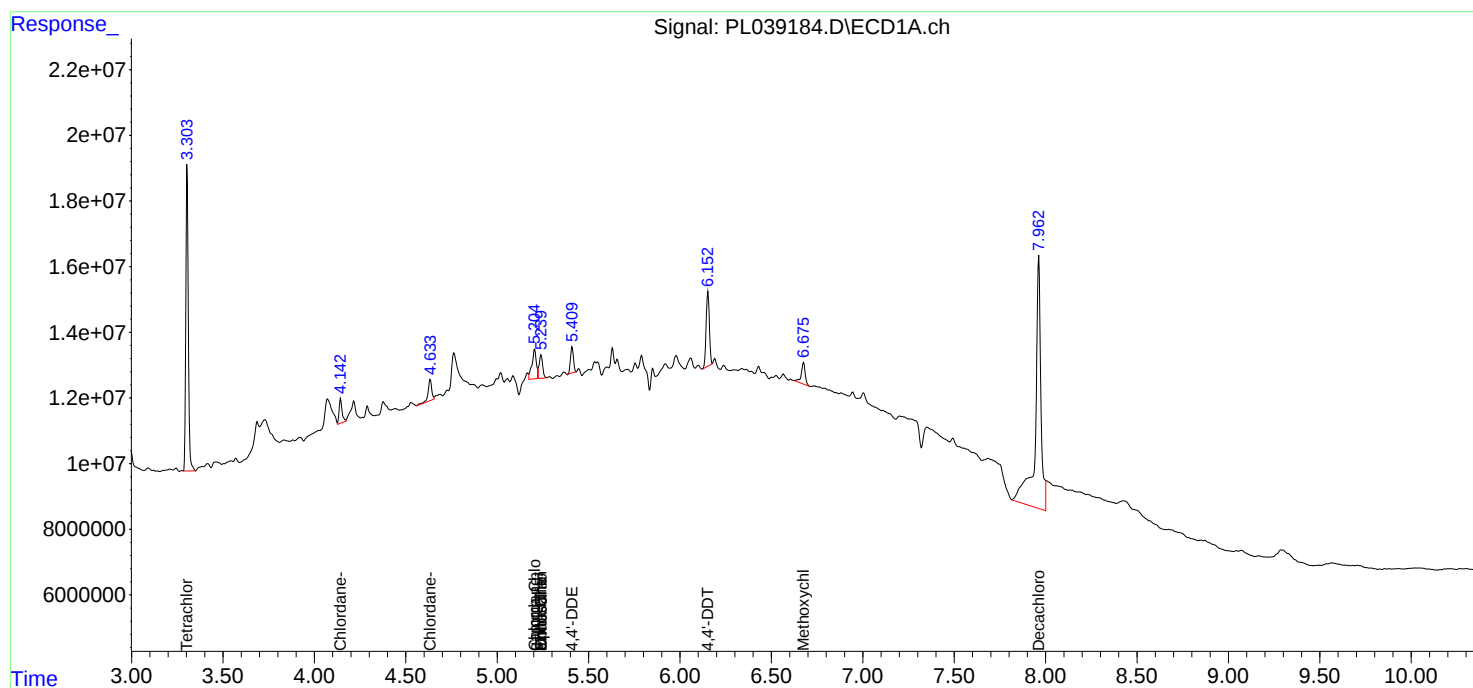


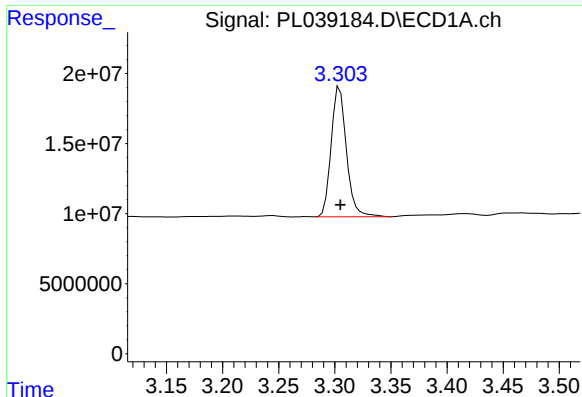

#1 Tetrachloro-m-xylene


R.T.: 3.304 min
Delta R.T.: 0.000 min
Response: 88100734
Conc: 12.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

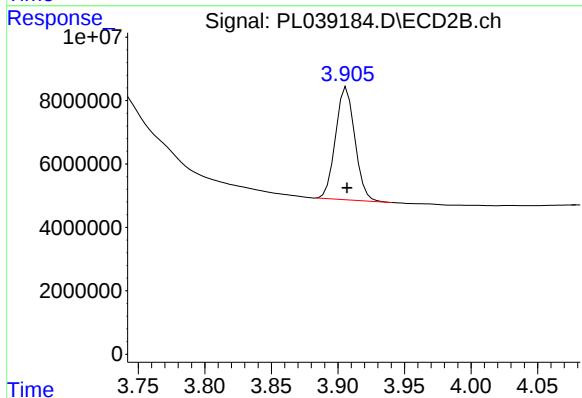


#1 Tetrachloro-m-xylene

R.T.: 3.907 min
Delta R.T.: 0.000 min
Response: 35723217
Conc: 13.33 ng/ml

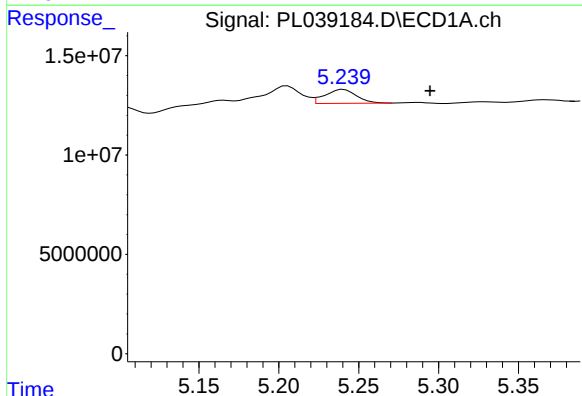


#9 Endosulfan I

R.T.: 5.240 min
Delta R.T.: -0.054 min
Response: 9654271
Conc: 1.10 ng/ml

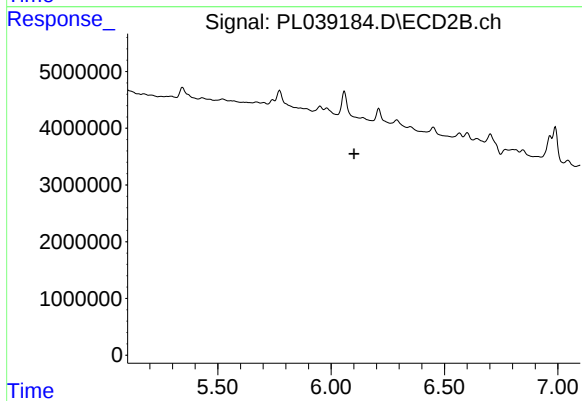

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.101 min
Response: 0
Conc: N.D.

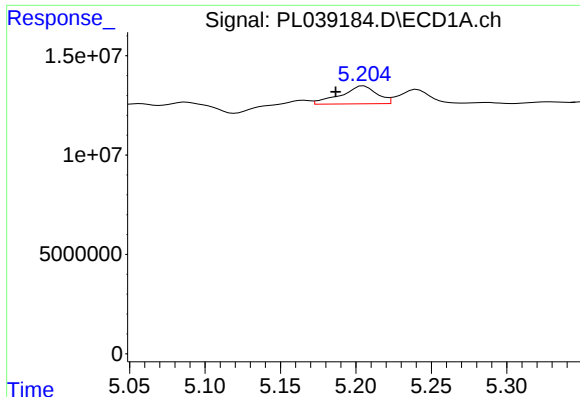

#10 gamma-Chlordane


R.T.: 5.205 min
Delta R.T.: 0.019 min
Response: 14953004
Conc: 1.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

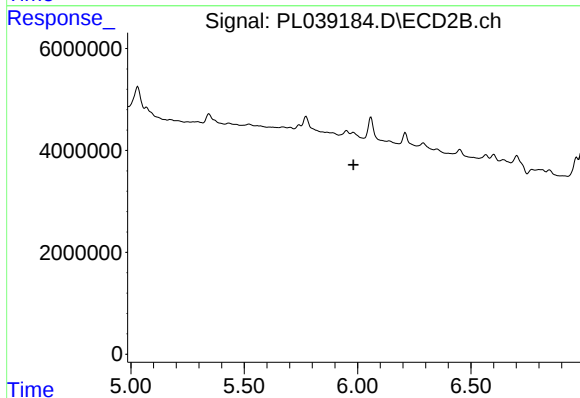


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.982 min
Response: 0
Conc: N.D.

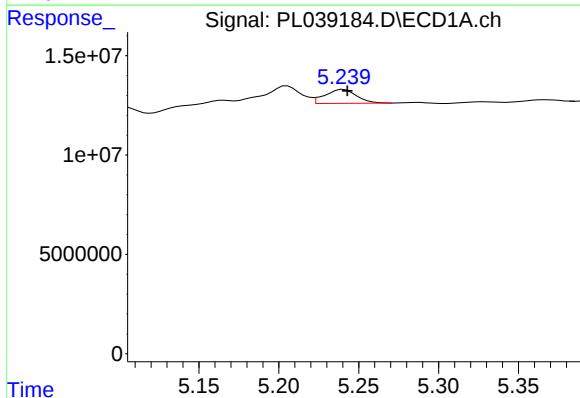


#11 alpha-Chlordane

R.T.: 5.240 min
Delta R.T.: -0.003 min
Response: 9654271
Conc: 1.00 ng/ml

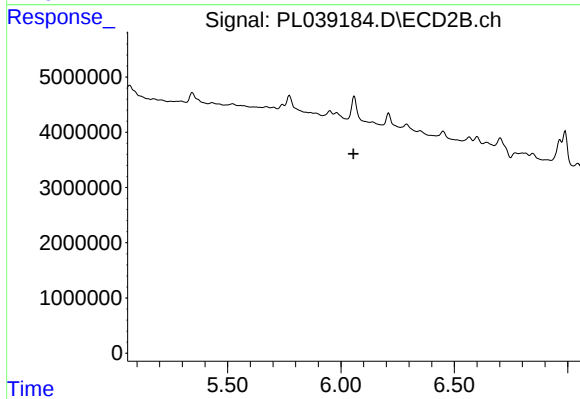

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.055 min
Response: 0
Conc: N.D.

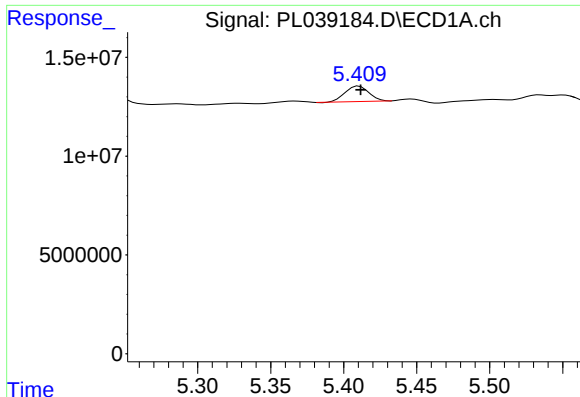

#12 4,4'-DDE


R.T.: 5.410 min
Delta R.T.: -0.001 min
Response: 8805327
Conc: 0.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

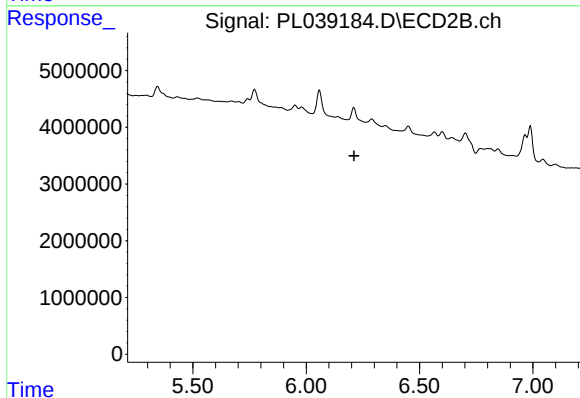


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.212 min
Response: 0
Conc: N.D.

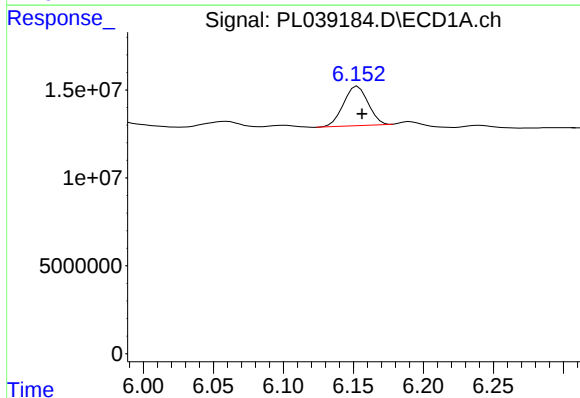


#17 4,4'-DDT

R.T.: 6.153 min
Delta R.T.: -0.003 min
Response: 27490726
Conc: 3.63 ng/ml

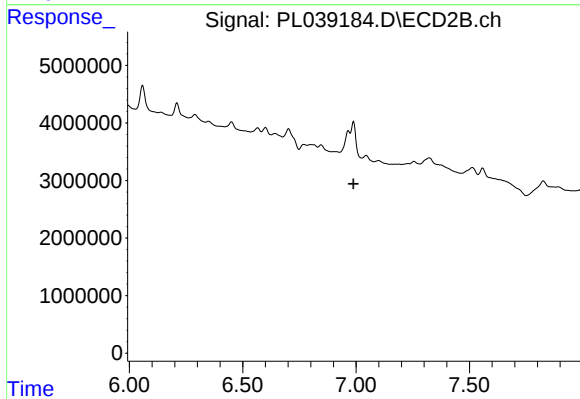

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.989 min
Response: 0
Conc: N.D.

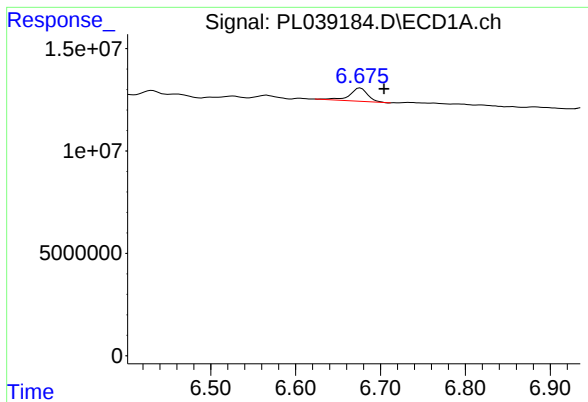

#20 Methoxychlor


R.T.: 6.676 min
Delta R.T.: -0.028 min
Response: 9865699
Conc: 2.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

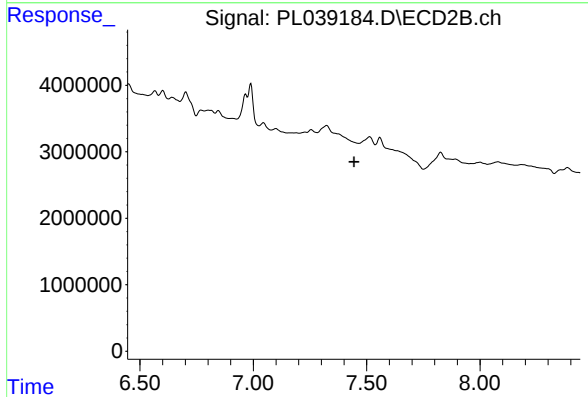


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.445 min
Response: 0
Conc: N.D.

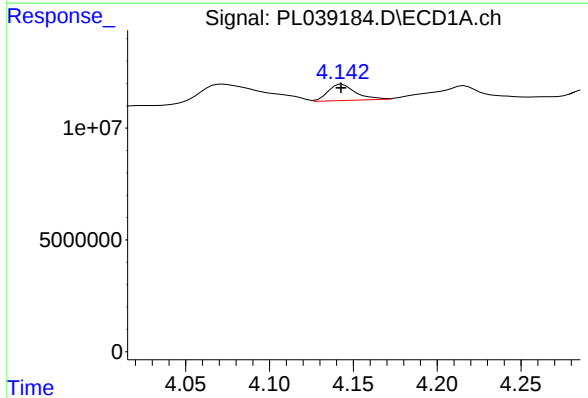


#23 Chlordane-1

R.T.: 4.143 min
Delta R.T.: 0.000 min
Response: 8333298
Conc: 26.32 ng/ml

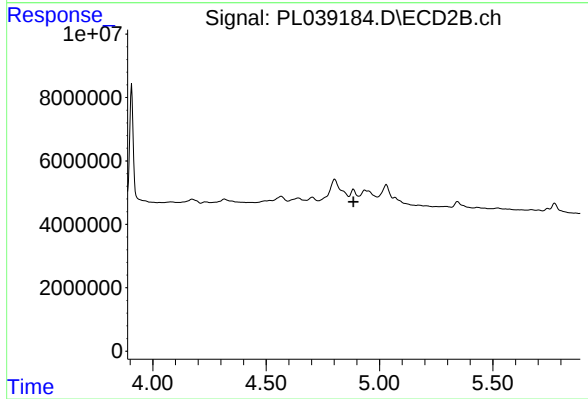

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

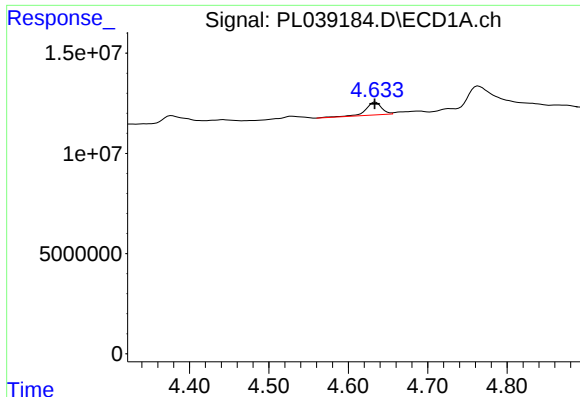

#24 Chlordane-2


R.T.: 4.634 min
Delta R.T.: 0.000 min
Response: 8818463
Conc: 25.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

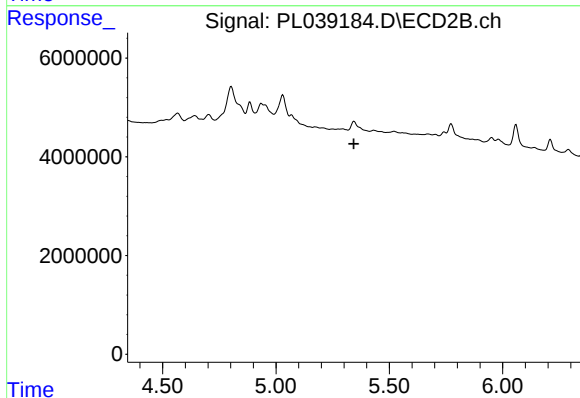


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.344 min
Response: 0
Conc: N.D.

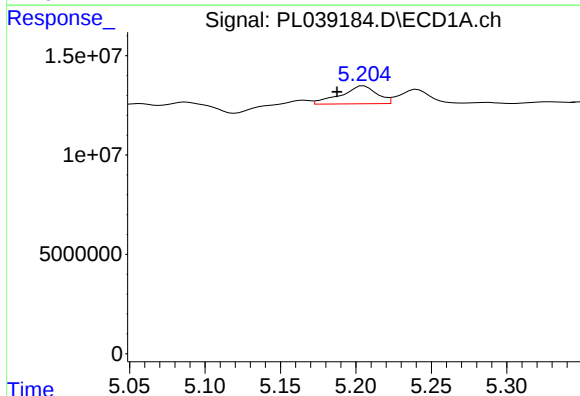


#25 Chlordane-3

R.T.: 5.205 min
Delta R.T.: 0.018 min
Response: 14953004
Conc: 13.69 ng/ml

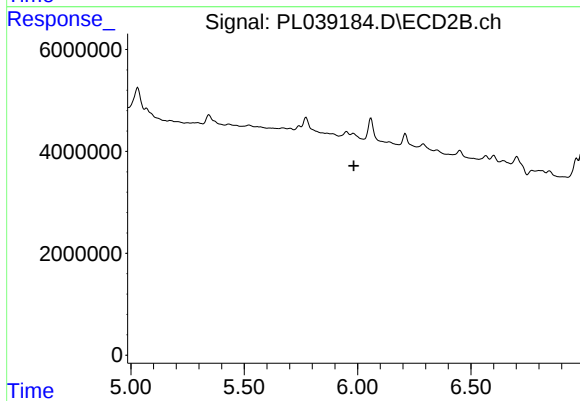

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

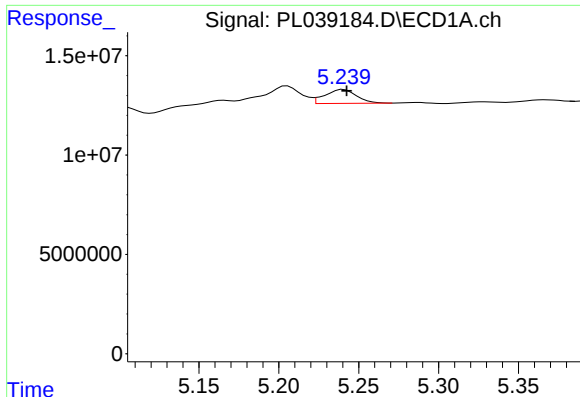

#26 Chlordane-4


R.T.: 5.240 min
Delta R.T.: -0.002 min
Response: 9654271
Conc: 9.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

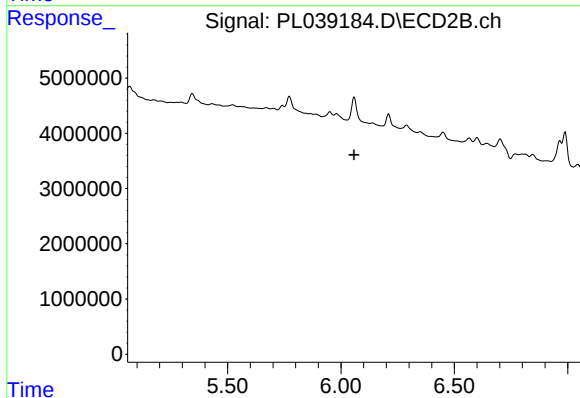


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.058 min
Response: 0
Conc: N.D.

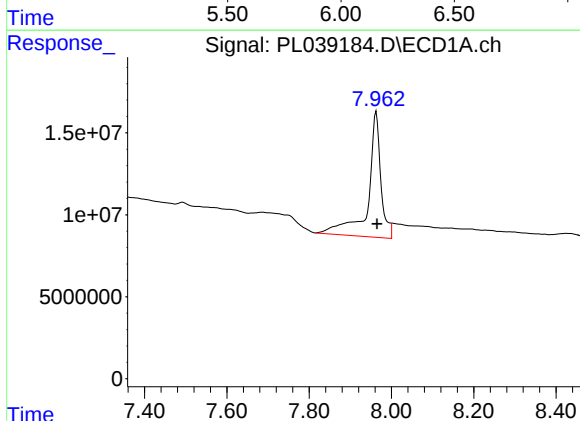

#28 Decachlorobiphenyl

R.T.: 7.963 min
Delta R.T.: -0.002 min
Response: 165332584
Conc: 23.54 ng/ml

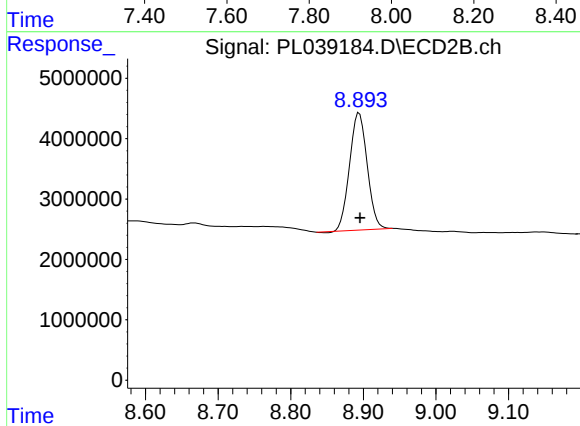

#28 Decachlorobiphenyl

R.T.: 8.894 min
Delta R.T.: -0.001 min
Response: 32749386
Conc: 14.06 ng/ml