

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081518\
 Data File : PL039188.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2018 07:47
 Operator : AJ\SJ
 Sample : PB112087BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 08:20:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.304	3.906	140.9E6	56227683	20.153	20.973
28)	SA Decachlor...	7.962	8.893	149.0E6	52698014	21.211	22.630
Target Compounds							
8)	B Heptachlo...	4.920f	0.000	2056876	0	0.215	N.D. #
9)	A Endosulfan I	5.256f	0.000	8245385	0	0.942	N.D. #
10)	B gamma-Chl...	5.256f	0.000	8245385	0	0.835	N.D. #
11)	B alpha-Chl...	5.256	0.000	8245385	0	0.858	N.D. #
25)	Chlordane-3	5.256	0.000	8245385	0	7.549	N.D. #
26)	Chlordane-4	5.256	0.000	8245385	0	8.251	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081518\
Data File : PL039188.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2018 07:47
Operator : AJ\SJ
Sample : PB112087BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 08:20:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

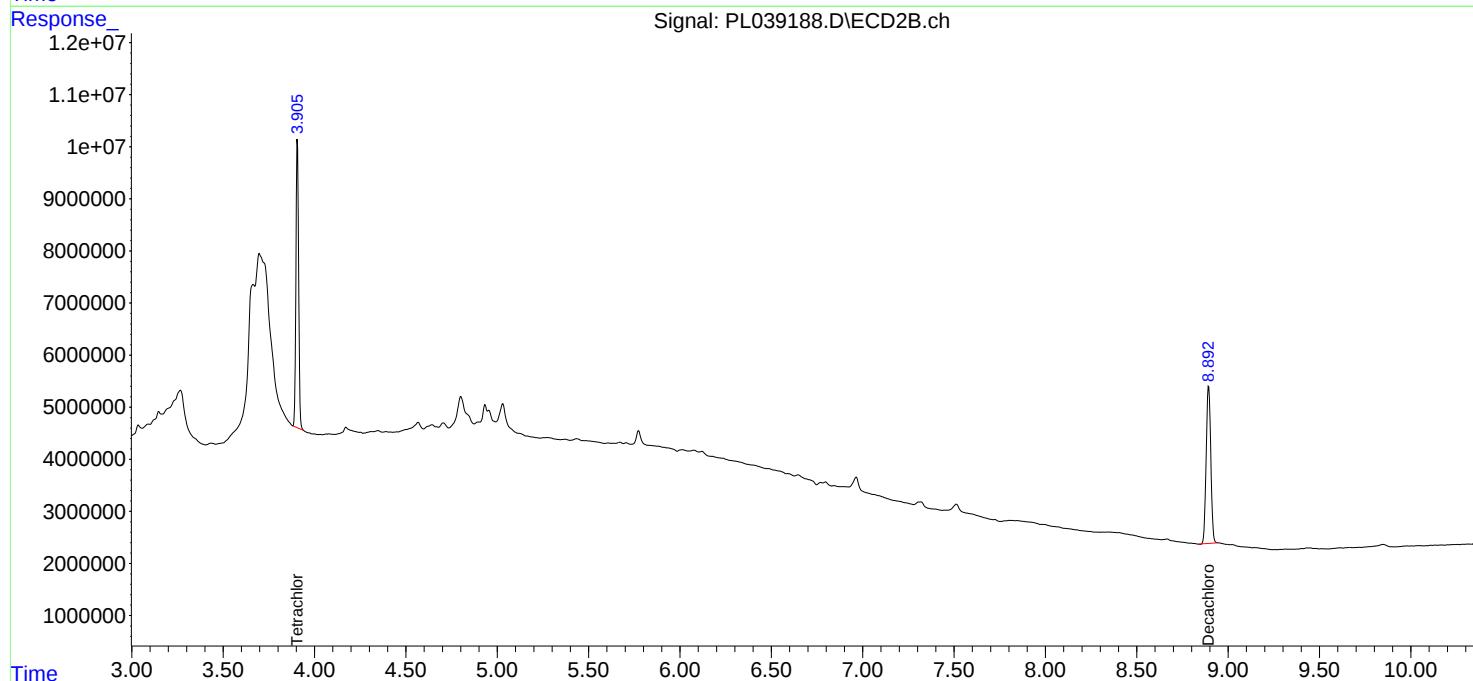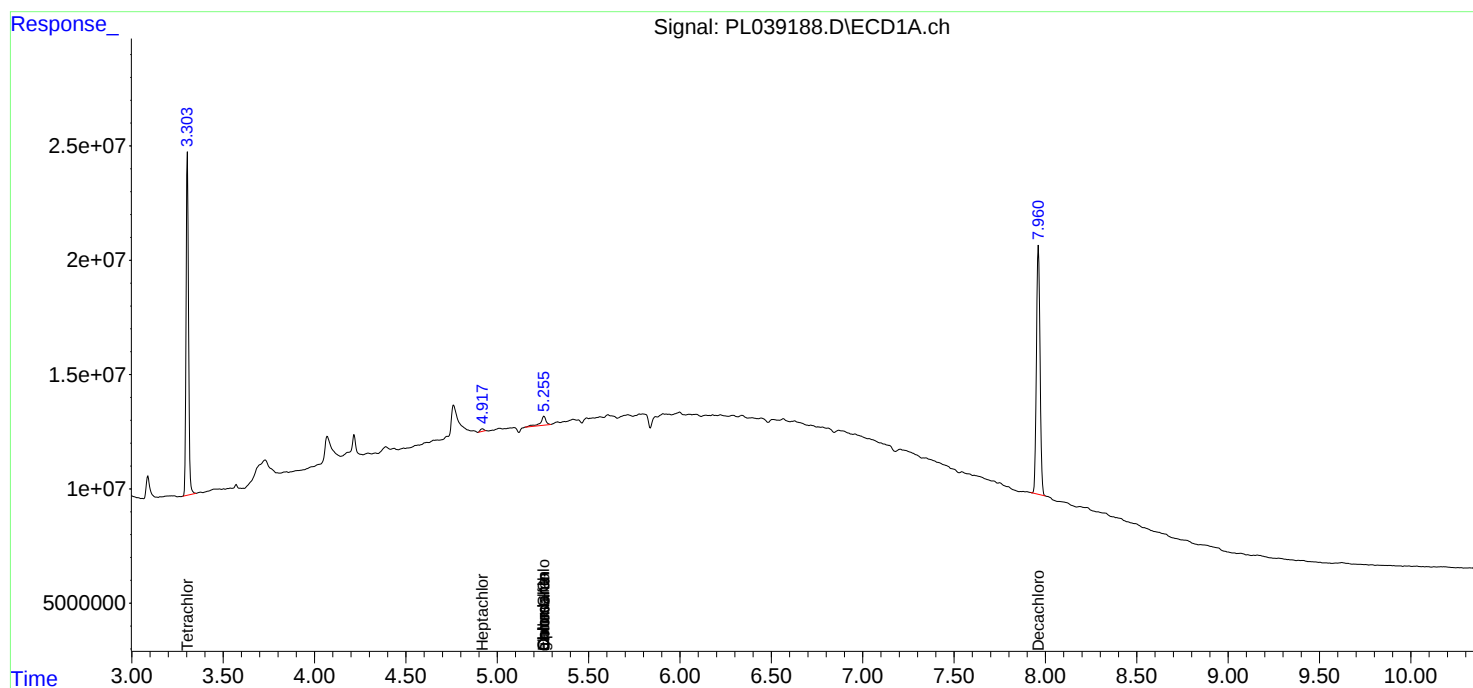


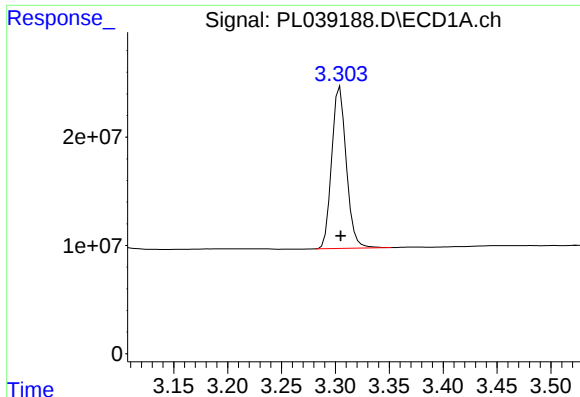

#1 Tetrachloro-m-xylene


R.T.: 3.304 min
Delta R.T.: 0.000 min
Response: 140880141
Conc: 20.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

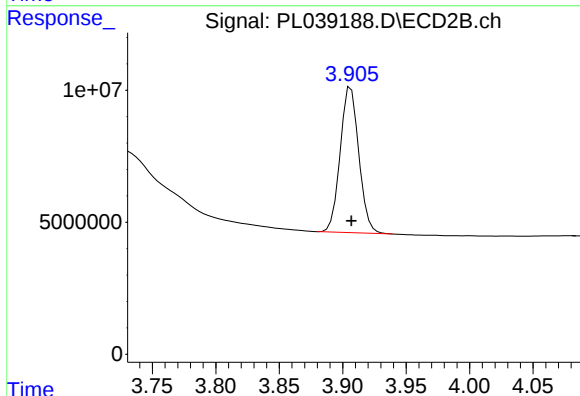


#1 Tetrachloro-m-xylene

R.T.: 3.906 min
Delta R.T.: 0.000 min
Response: 56227683
Conc: 20.97 ng/ml

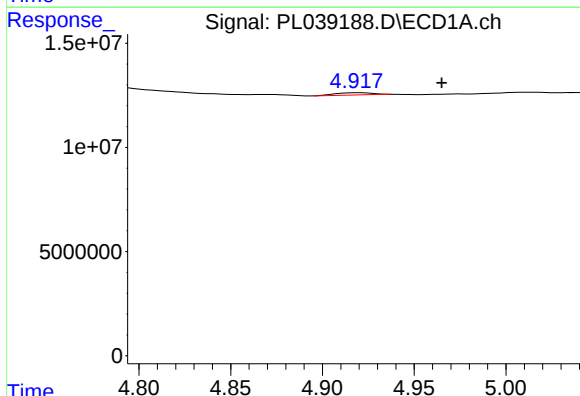


#8 Heptachlor epoxide

R.T.: 4.920 min
Delta R.T.: -0.045 min
Response: 2056876
Conc: 0.22 ng/ml

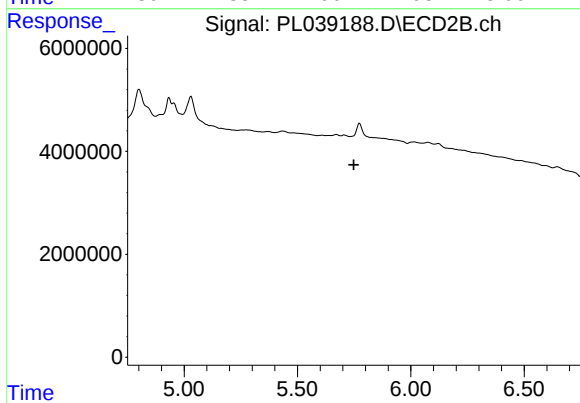

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.749 min
Response: 0
Conc: N.D.

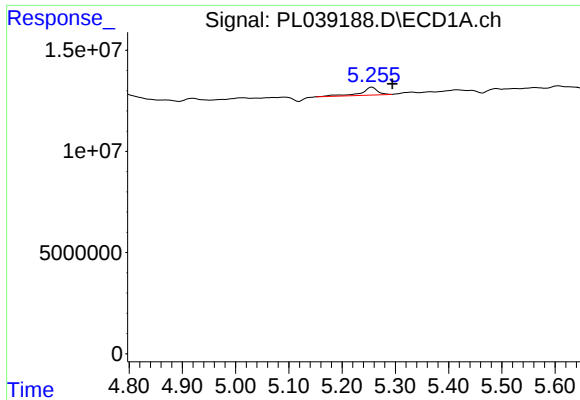

#9 Endosulfan I


R.T.: 5.256 min
Delta R.T.: -0.039 min
Response: 8245385
Conc: 0.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

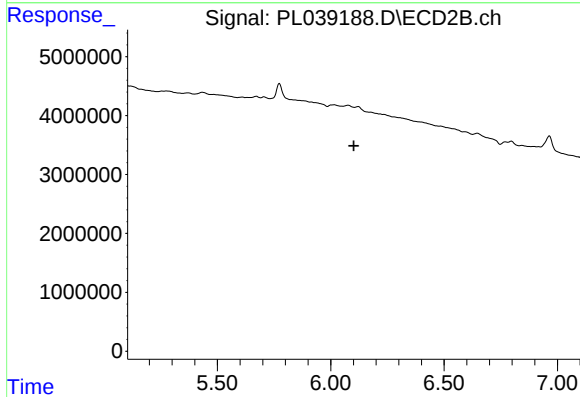


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.101 min
Response: 0
Conc: N.D.

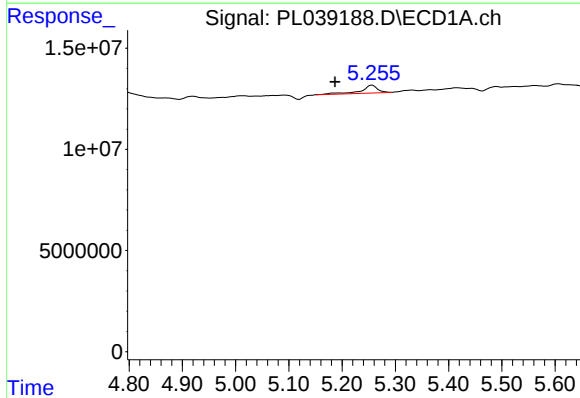


#10 gamma-Chlordane

R.T.: 5.256 min
Delta R.T.: 0.069 min
Response: 8245385
Conc: 0.83 ng/ml

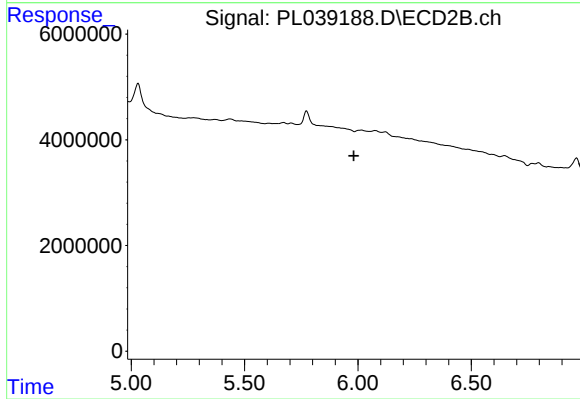

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.982 min
Response: 0
Conc: N.D.

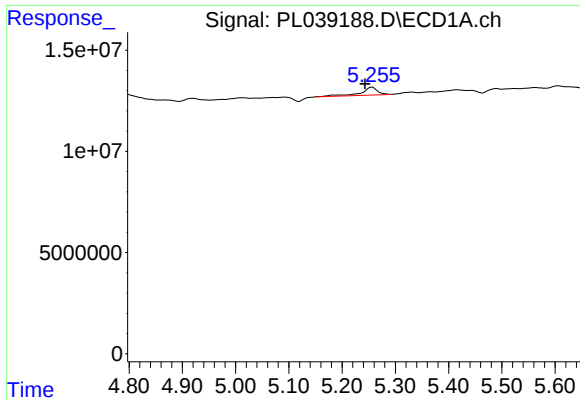

#11 alpha-Chlordane


R.T.: 5.256 min
Delta R.T.: 0.013 min
Response: 8245385
Conc: 0.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

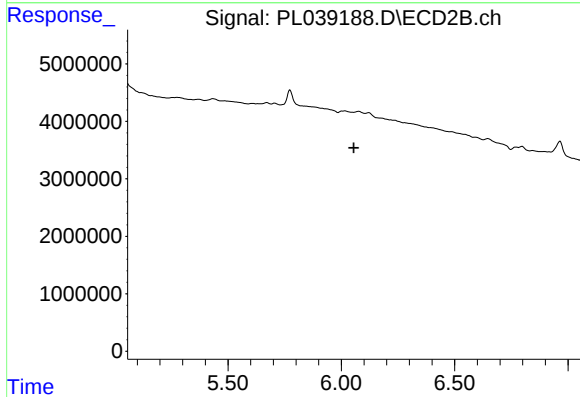


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.055 min
Response: 0
Conc: N.D.

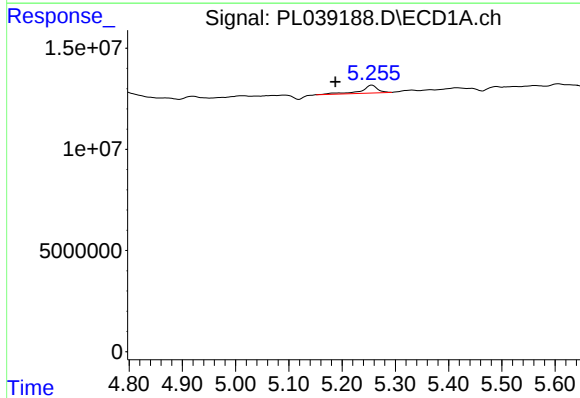


#25 Chlordane-3

R.T.: 5.256 min
Delta R.T.: 0.069 min
Response: 8245385
Conc: 7.55 ng/ml

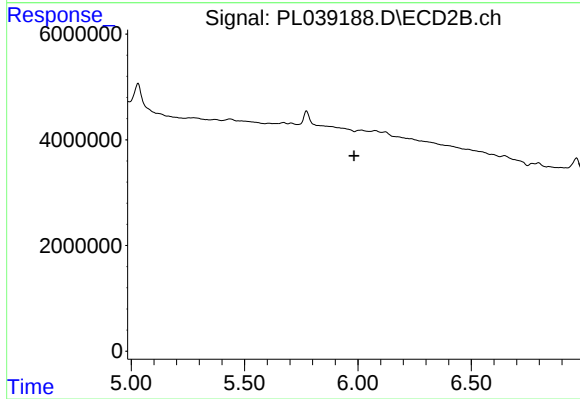

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

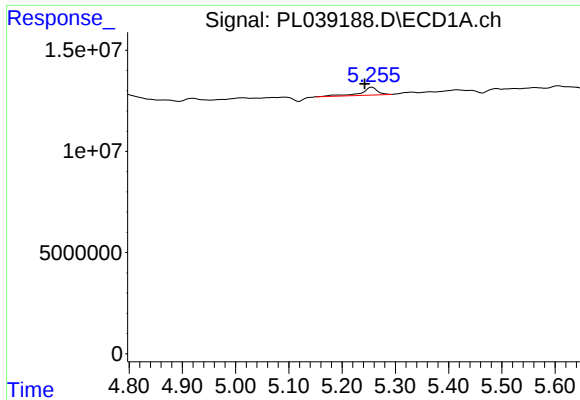

#26 Chlordane-4


R.T.: 5.256 min
Delta R.T.: 0.013 min
Response: 8245385
Conc: 8.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

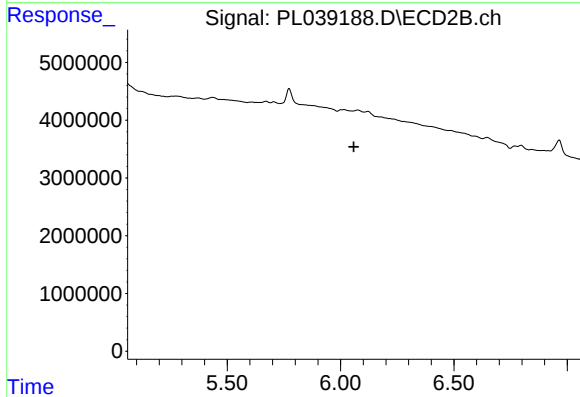


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.058 min
Response: 0
Conc: N.D.

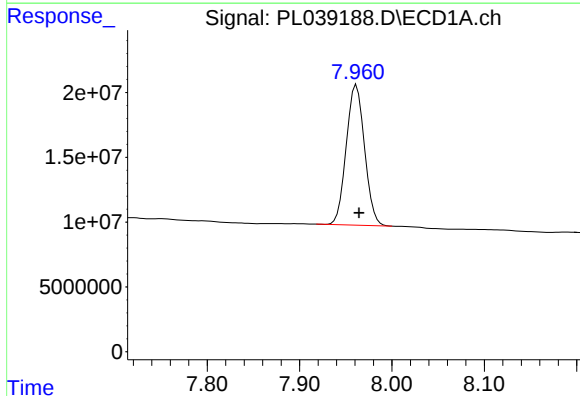

#28 Decachlorobiphenyl

R.T.: 7.962 min
Delta R.T.: -0.003 min
Response: 148973466
Conc: 21.21 ng/ml

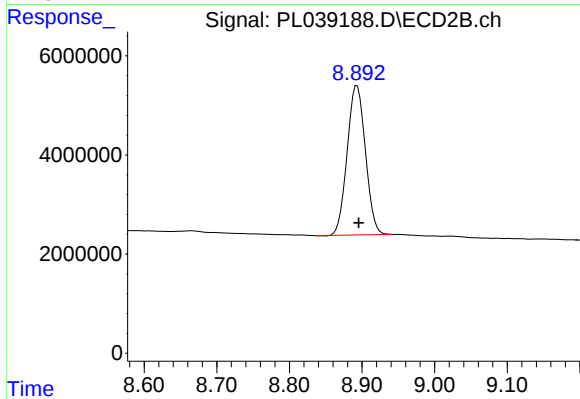

#28 Decachlorobiphenyl

R.T.: 8.893 min
Delta R.T.: -0.002 min
Response: 52698014
Conc: 22.63 ng/ml