

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081518\
 Data File : PL039191.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2018 08:30
 Operator : AJ\SJ
 Sample : J4474-01 10X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 09:52:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.304	0.000	15976477	0	2.285	N.D. #
28)	SA Decachlor...	7.961	0.000	17236447	0	2.454	N.D. #
Target Compounds							
3)	MA gamma-BHC...	4.022	0.000	3349053	0	0.316	N.D. #
6)	B beta-BHC	4.218f	0.000	15646670	0	3.368	N.D. #
8)	B Heptachlo...	0.000	5.772	0	8170578	N.D.	2.430 #
9)	A Endosulfan I	5.324	0.000	3684722	0	0.421	N.D. #
10)	B gamma-Chl...	5.252f	0.000	26149765	0	2.648	N.D. #
11)	B alpha-Chl...	5.252	0.000	26149765	0	2.722	N.D. #
13)	MA Dieldrin	5.528	0.000	25799593	0	2.646	N.D. #
15)	B Endosulfa...	6.056	0.000	8164152	0	0.939	N.D. #
17)	MA 4,4'-DDT	6.151	0.000	2217181	0	0.292	N.D. #
24)	Chlordane-2	4.629	0.000	6746850	0	19.299	N.D. #
25)	Chlordane-3	5.252	0.000	26149765	0	23.941	N.D. #
26)	Chlordane-4	5.252	0.000	26149765	0	26.167	N.D. #
27)	Chlordane-5	6.056	0.000	8164152	0	25.172	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081518\
Data File : PL039191.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2018 08:30
Operator : AJ\SJ
Sample : J4474-01 10X
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 09:52:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

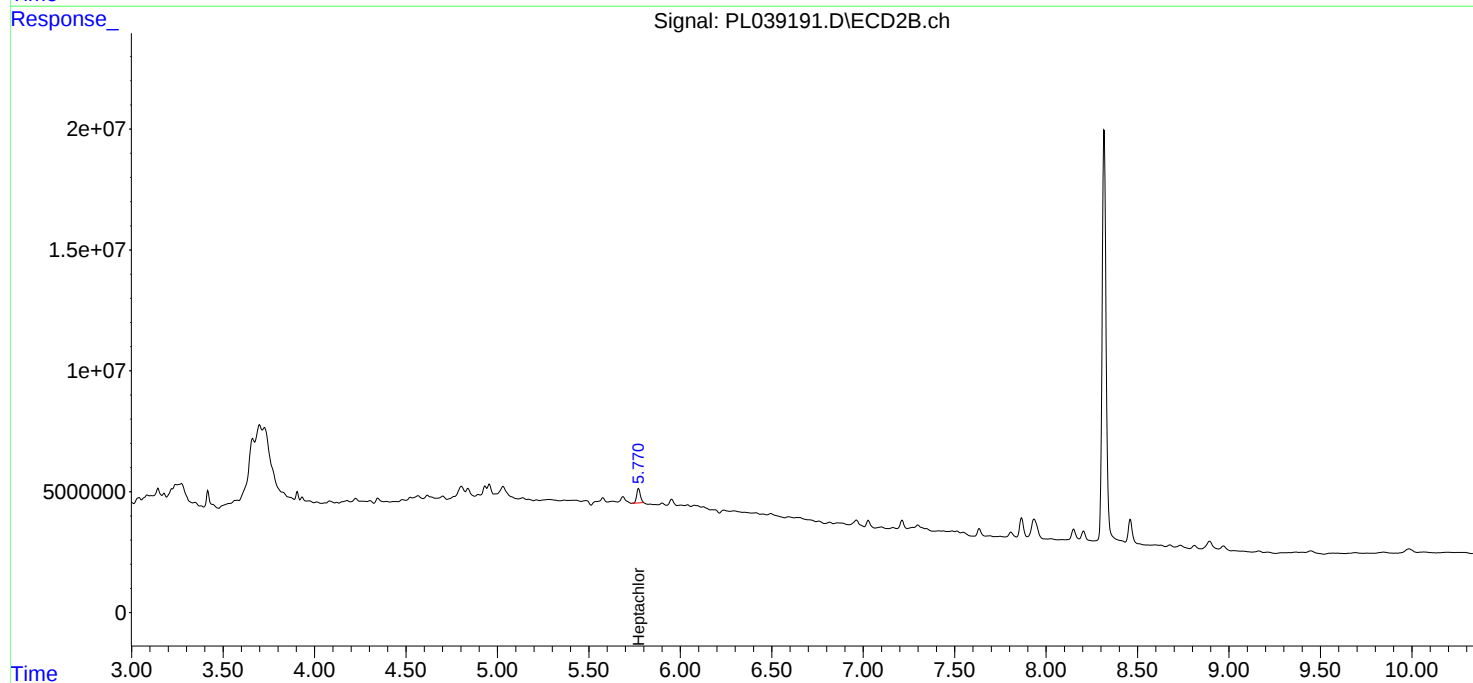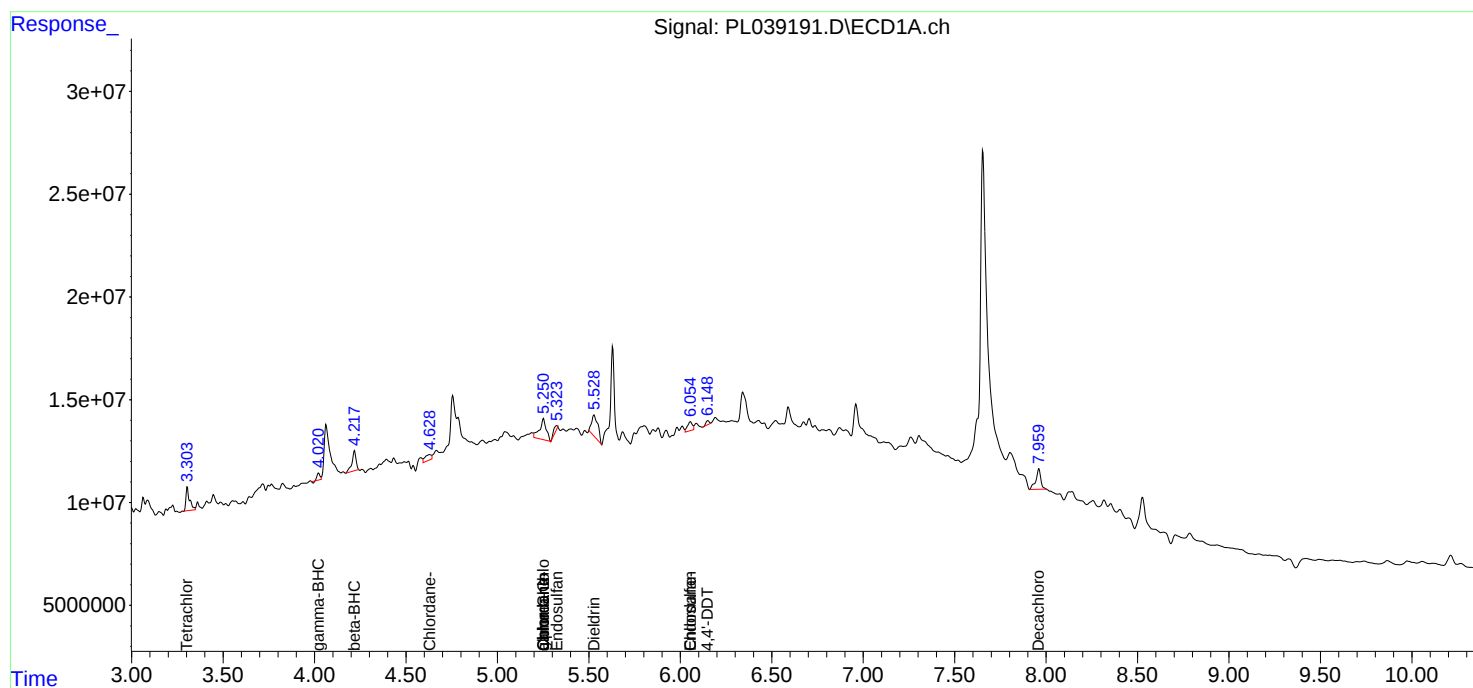


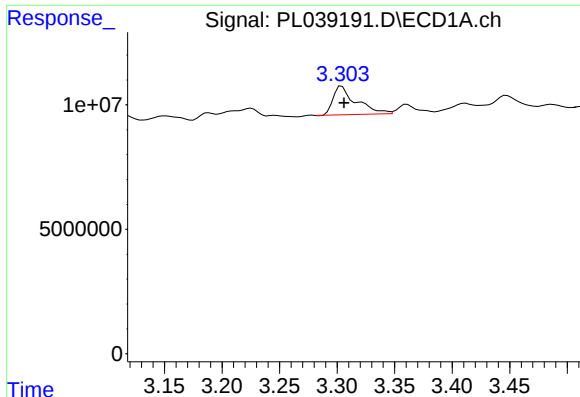

#1 Tetrachloro-m-xylene


R.T.: 3.304 min
Delta R.T.: -0.002 min
Response: 15976477
Conc: 2.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

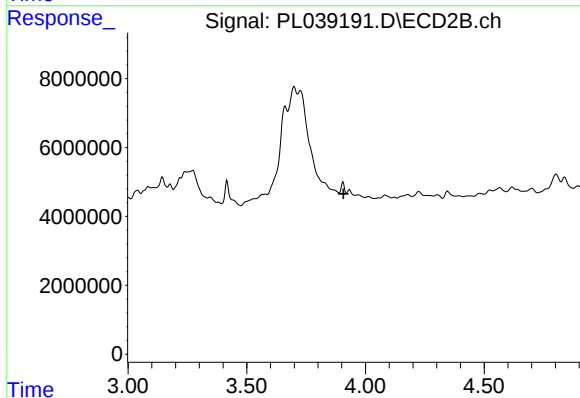


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.907 min
Response: 0
Conc: N.D.

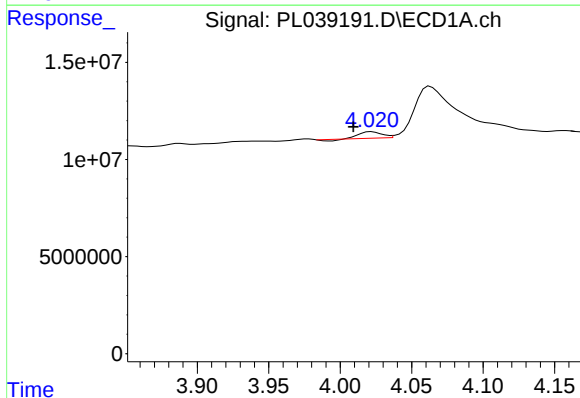


#3 gamma-BHC (Lindane)

R.T.: 4.022 min
Delta R.T.: 0.012 min
Response: 3349053
Conc: 0.32 ng/ml

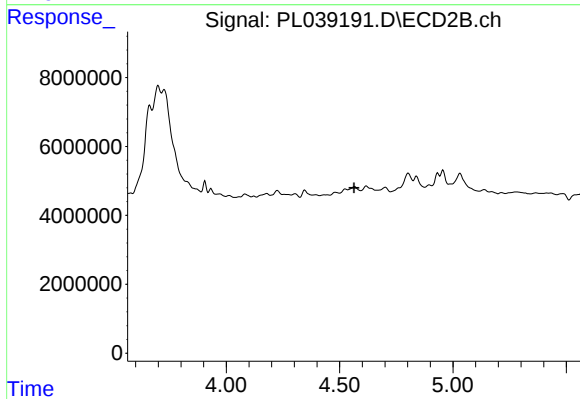

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.563 min
Response: 0
Conc: N.D.

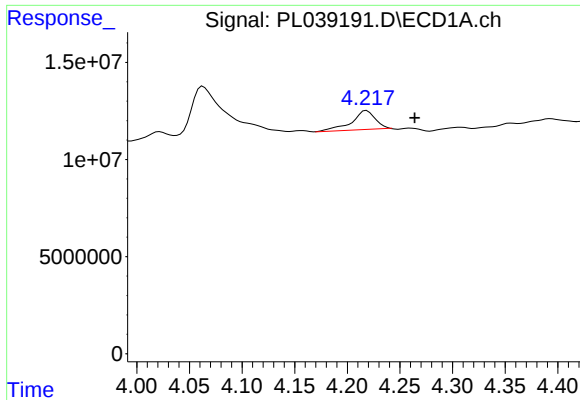

#6 beta-BHC


R.T.: 4.218 min
Delta R.T.: -0.046 min
Response: 15646670
Conc: 3.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

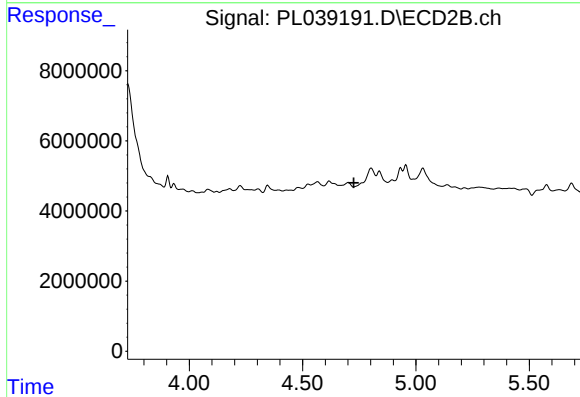


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

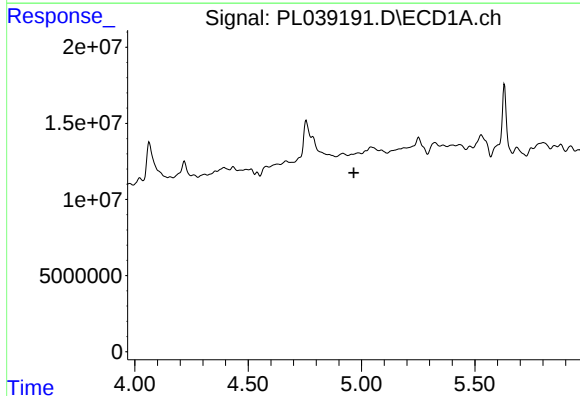


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.966 min
Response: 0
Conc: N.D.

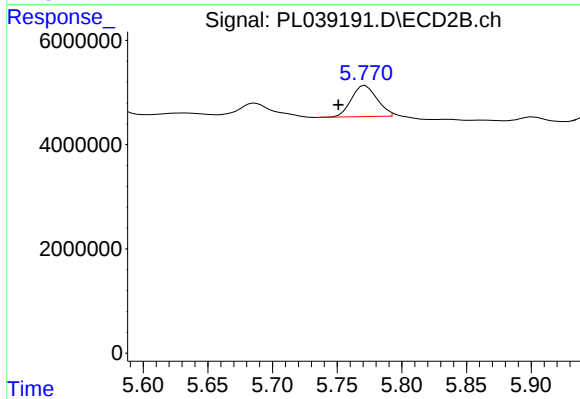

#8 Heptachlor epoxide


R.T.: 5.772 min
Delta R.T.: 0.021 min
Response: 8170578
Conc: 2.43 ng/ml

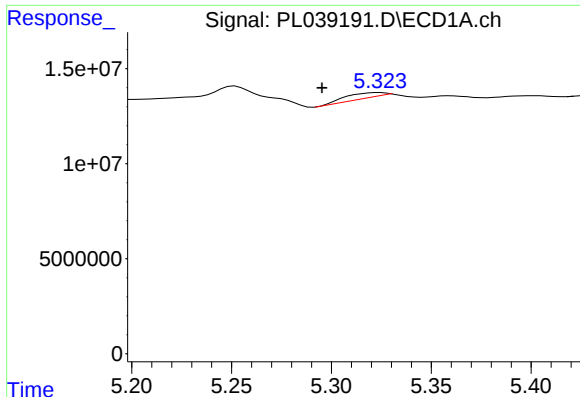

#9 Endosulfan I


R.T.: 5.324 min
Delta R.T.: 0.029 min
Response: 3684722
Conc: 0.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

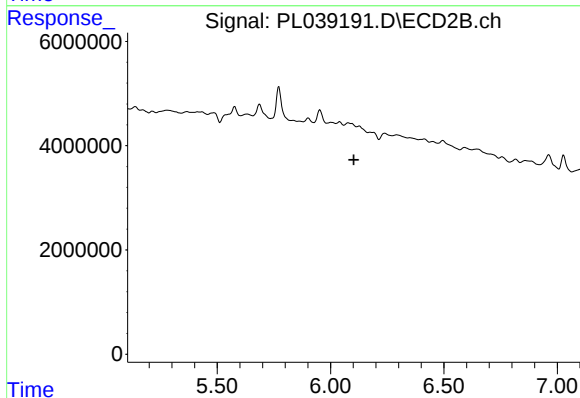


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.102 min
Response: 0
Conc: N.D.

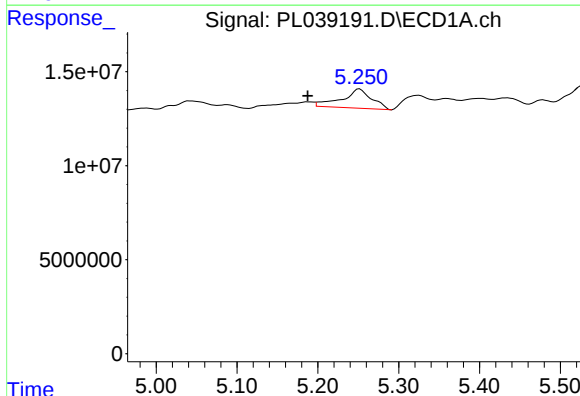


#10 gamma-Chlordane

R.T.: 5.252 min
Delta R.T.: 0.064 min
Response: 26149765
Conc: 2.65 ng/ml

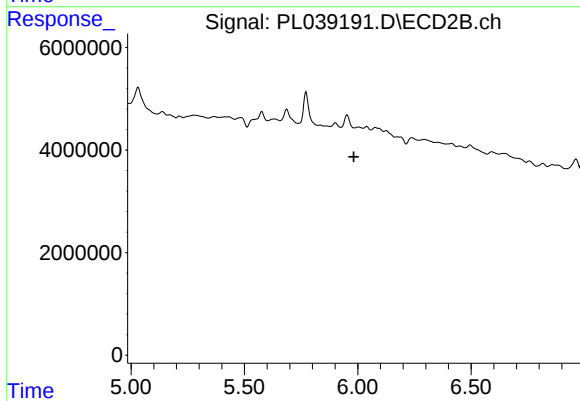

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

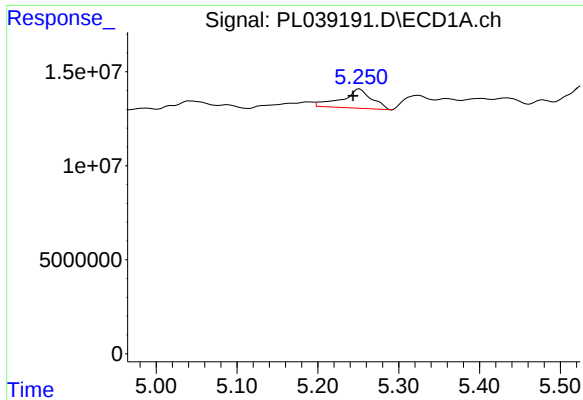

#11 alpha-Chlordane


R.T.: 5.252 min
Delta R.T.: 0.008 min
Response: 26149765
Conc: 2.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

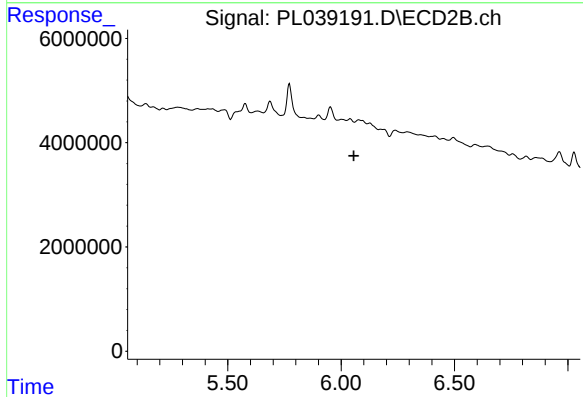


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.056 min
Response: 0
Conc: N.D.

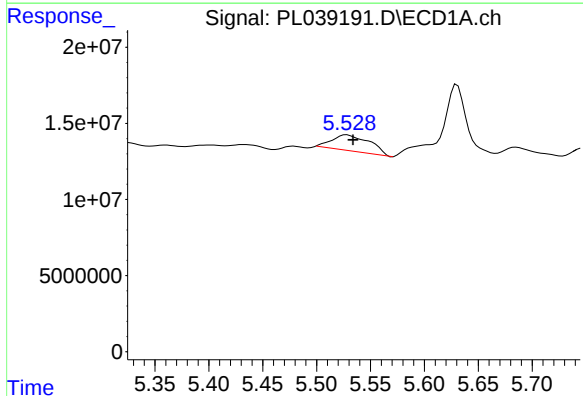


#13 Dieldrin

R.T.: 5.528 min
Delta R.T.: -0.006 min
Response: 25799593
Conc: 2.65 ng/ml

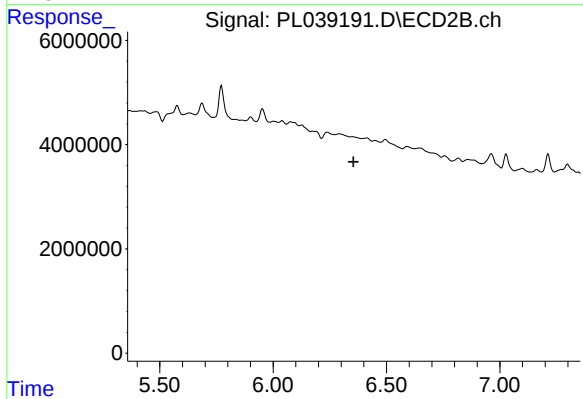

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.355 min
Response: 0
Conc: N.D.

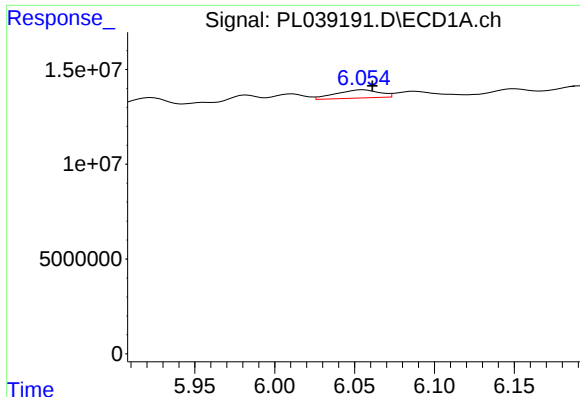

#15 Endosulfan II


R.T.: 6.056 min
Delta R.T.: -0.006 min
Response: 8164152
Conc: 0.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

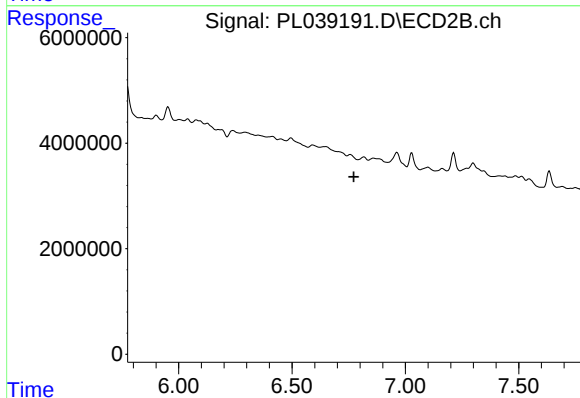


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.773 min
Response: 0
Conc: N.D.

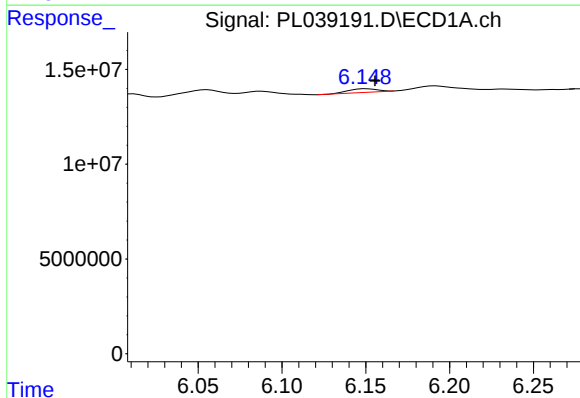


#17 4,4'-DDT

R.T.: 6.151 min
Delta R.T.: -0.005 min
Response: 2217181
Conc: 0.29 ng/ml

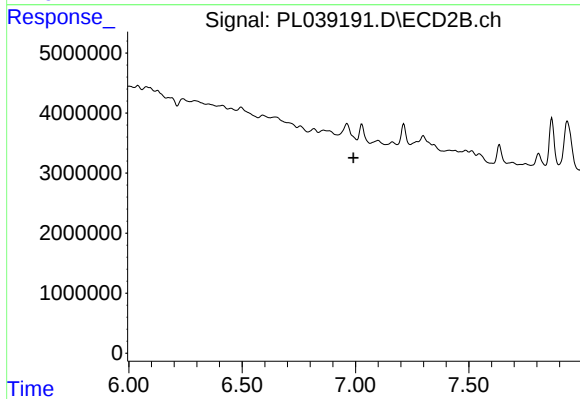

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.991 min
Response: 0
Conc: N.D.

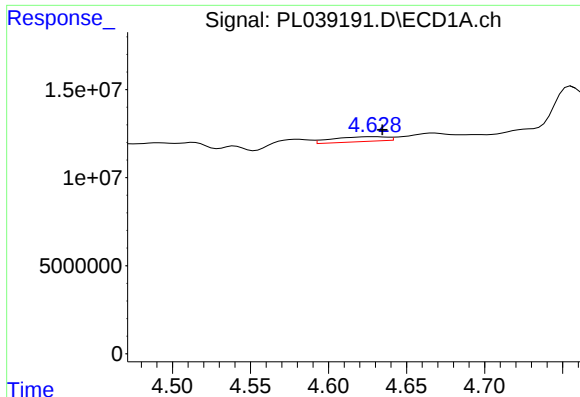

#24 Chlordane-2


R.T.: 4.629 min
Delta R.T.: -0.005 min
Response: 6746850
Conc: 19.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

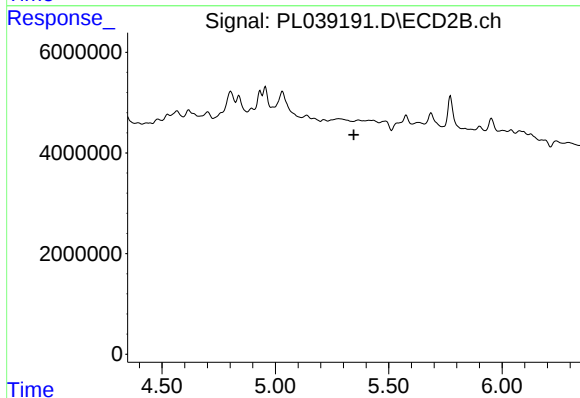


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.346 min
Response: 0
Conc: N.D.

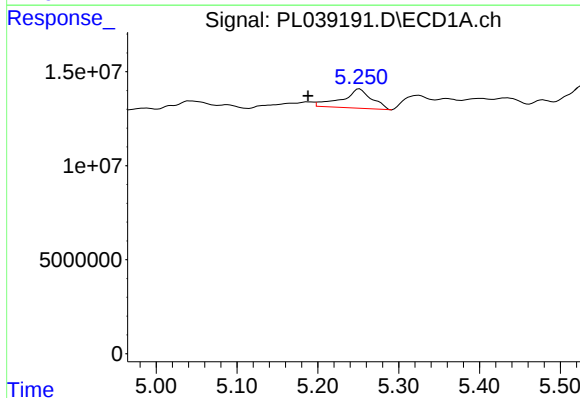


#25 Chlordane-3

R.T.: 5.252 min
Delta R.T.: 0.064 min
Response: 26149765
Conc: 23.94 ng/ml

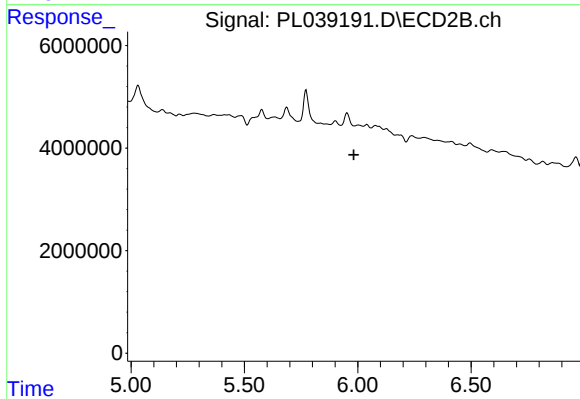

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

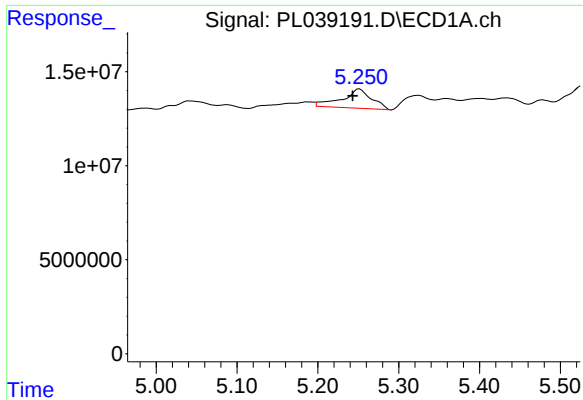

#26 Chlordane-4


R.T.: 5.252 min
Delta R.T.: 0.009 min
Response: 26149765
Conc: 26.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

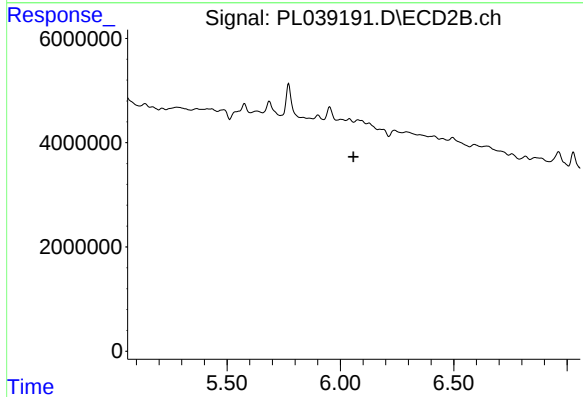


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.058 min
Response: 0
Conc: N.D.

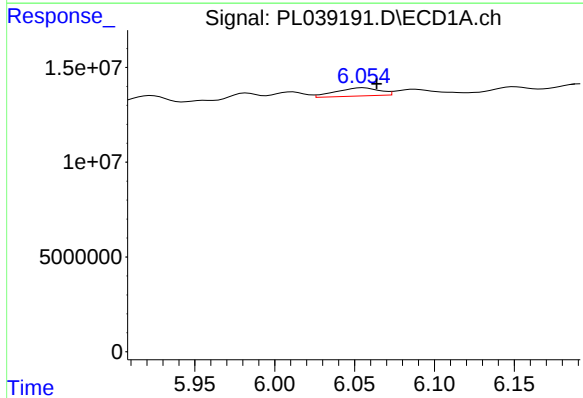


#27 Chlordane-5

R.T.: 6.056 min
Delta R.T.: -0.008 min
Response: 8164152
Conc: 25.17 ng/ml

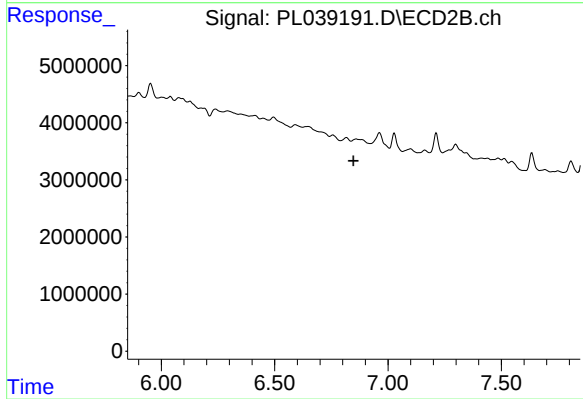

#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.848 min
Response: 0
Conc: N.D.

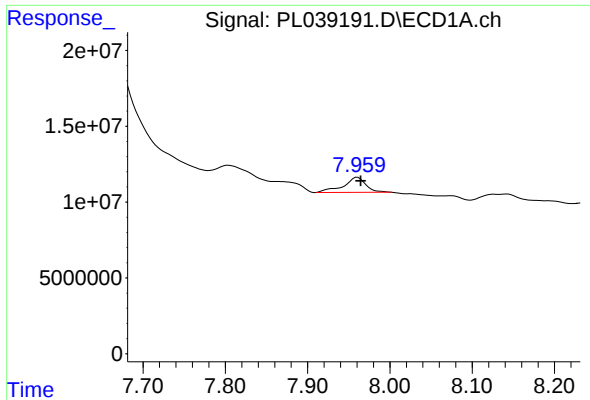

#28 Decachlorobiphenyl


R.T.: 7.961 min

Delta R.T.: -0.004 min

Response: 17236447

Conc: 2.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

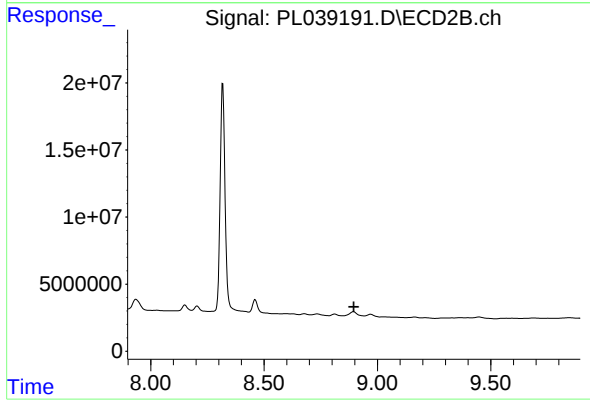

#28 Decachlorobiphenyl

R.T.: 0.000 min

Exp R.T. : 8.896 min

Response: 0

Conc: N.D.