

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081519\
 Data File : PL051514.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2019 10:26
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 00:48:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) A	alpha-BHC	3.765f	0.000	23486812	0	1.402	N.D. #
6) B	beta-BHC	0.000	4.785	0	7647241	N.D.	4.423 #
8) B	Heptachlo...	5.005f	5.805	1613735	39548922	0.109	10.340 #
9) A	Endosulfan I	5.322	0.000	12200652	0	0.839	N.D. #
10) B	gamma-Chl...	5.227f	0.000	35524075	0	2.251	N.D. #
13) MA	Dieldrin	5.551	0.000	18783136	0	1.212	N.D. #
17) MA	4,4'-DDT	6.187f	0.000	24767921	0	2.000	N.D. #
24)	Chlordane-2	4.659	0.000	10558508	0	23.589	N.D. #
25)	Chlordane-3	5.227f	0.000	35524075	0	25.378	N.D. #
26)	Chlordane-4	5.227f	0.000	35524075	0	26.933	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051519\
Data File : PL051514.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2019 10:26
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 00:48:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

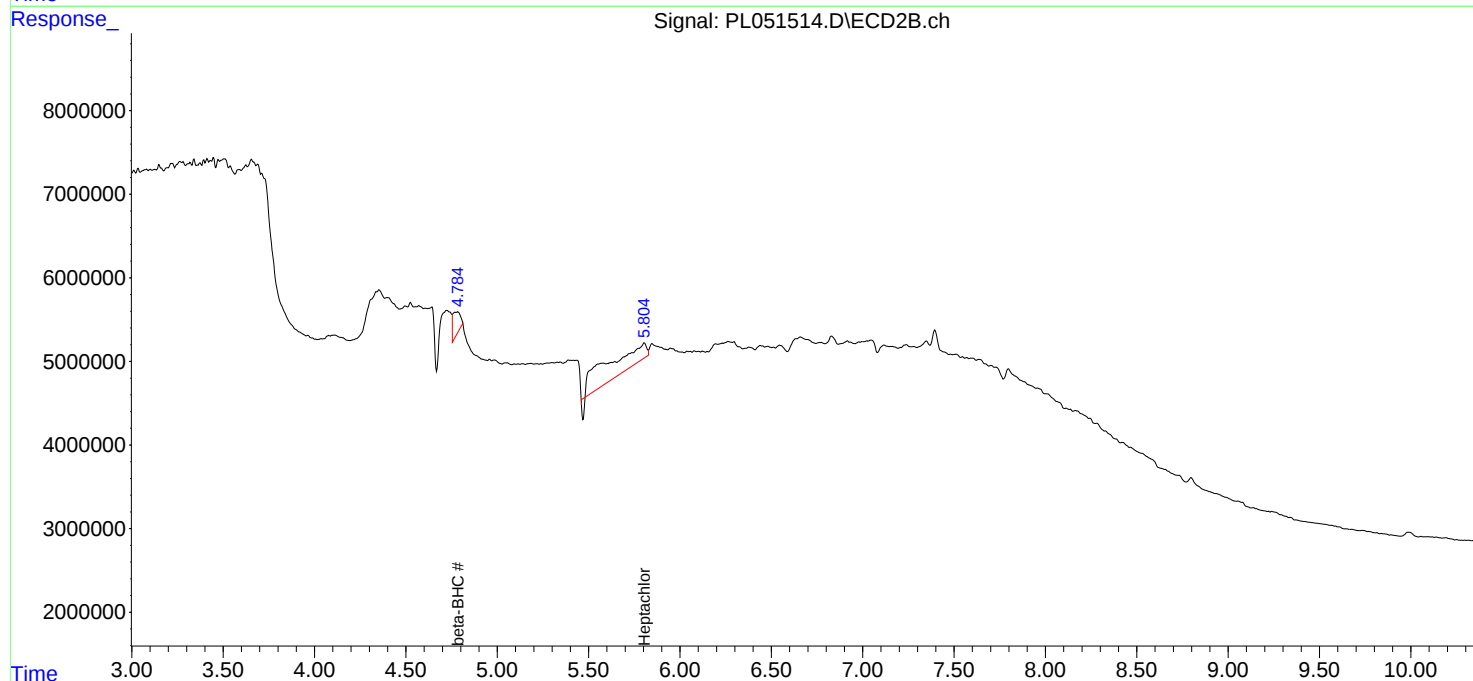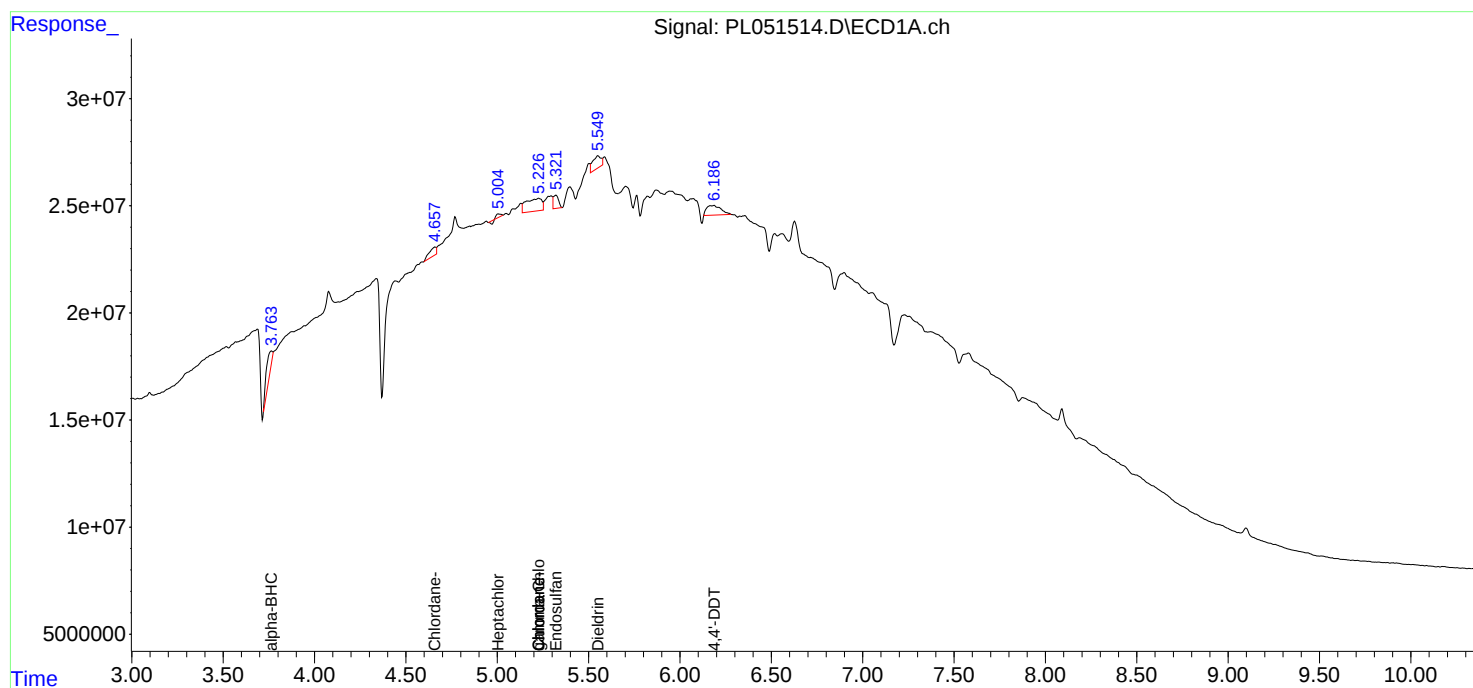


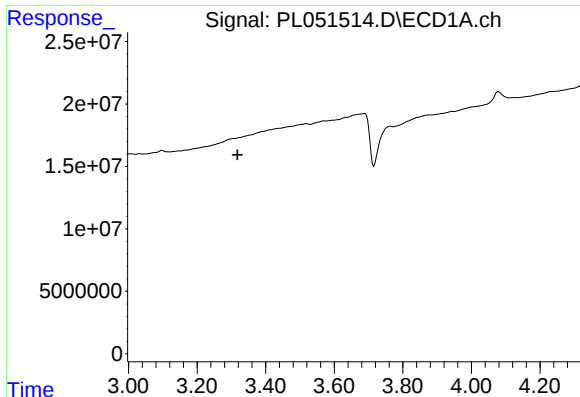

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.318 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

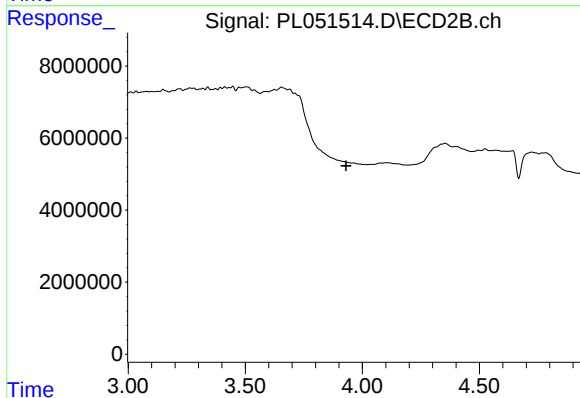


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.931 min
Response: 0
Conc: N.D.

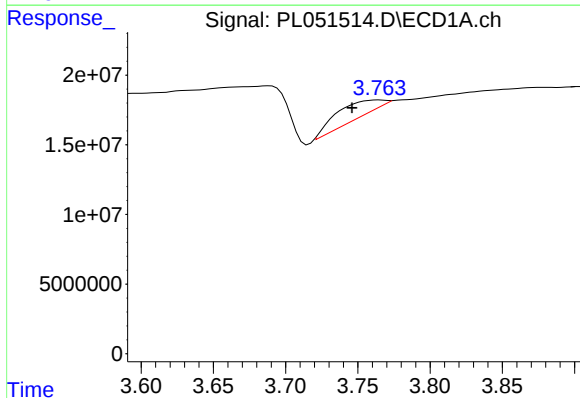


#2 alpha-BHC

R.T.: 3.765 min
Delta R.T.: 0.019 min
Response: 23486812
Conc: 1.40 ng/ml

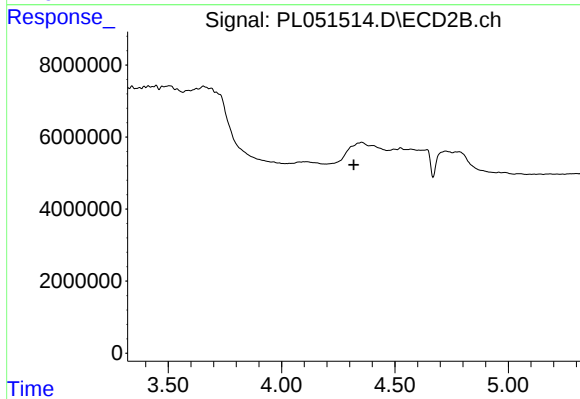

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.319 min
Response: 0
Conc: N.D.

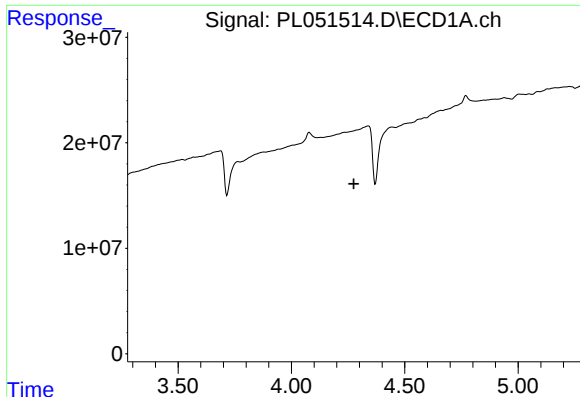

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

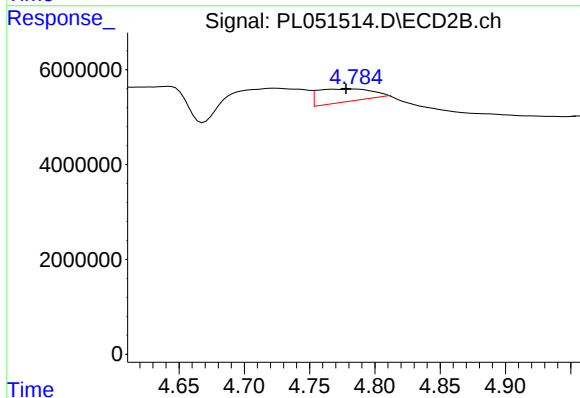


#6 beta-BHC

R.T.: 4.785 min
Delta R.T.: 0.006 min
Response: 7647241
Conc: 4.42 ng/ml

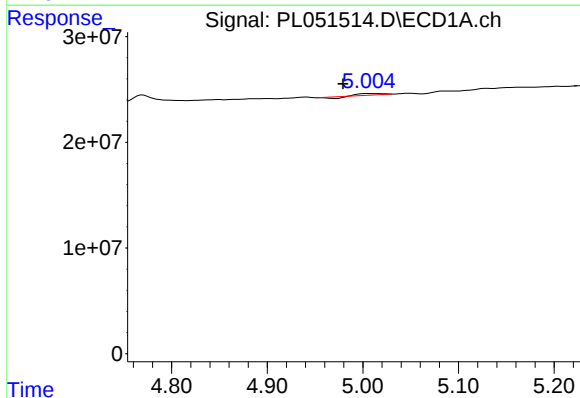


#8 Heptachlor epoxide

R.T.: 5.005 min
Delta R.T.: 0.025 min
Response: 1613735
Conc: 0.11 ng/ml

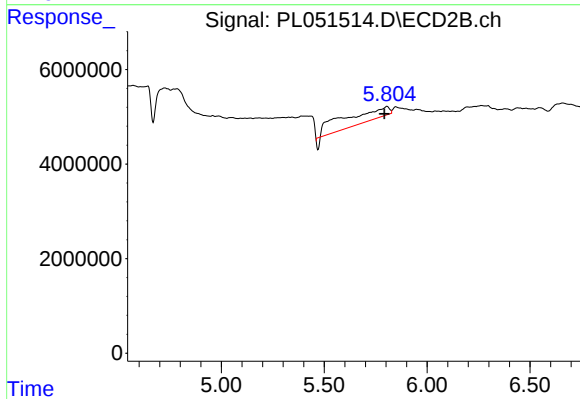

#8 Heptachlor epoxide


R.T.: 5.805 min
Delta R.T.: 0.012 min
Response: 39548922
Conc: 10.34 ng/ml

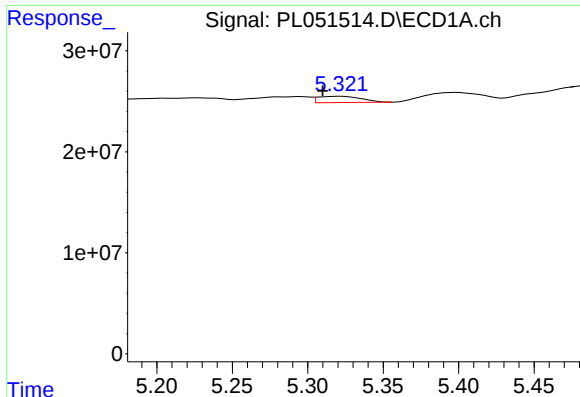

#9 Endosulfan I


R.T.: 5.322 min
Delta R.T.: 0.012 min
Response: 12200652
Conc: 0.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

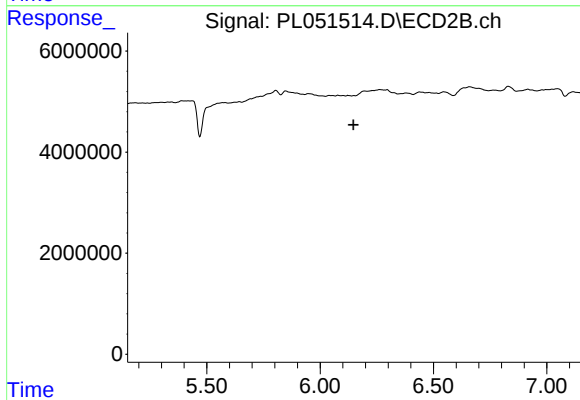


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.148 min
Response: 0
Conc: N.D.

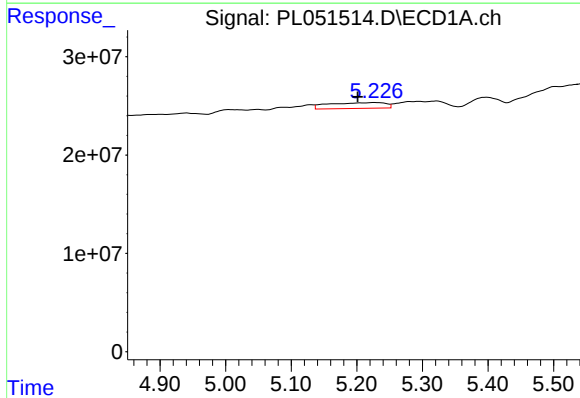


#10 gamma-Chlordane

R.T.: 5.227 min
Delta R.T.: 0.026 min
Response: 35524075
Conc: 2.25 ng/ml

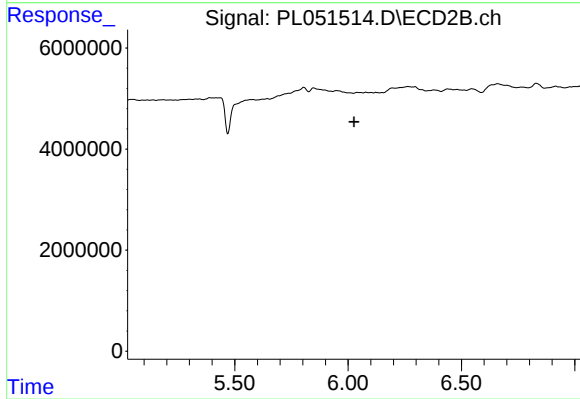

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

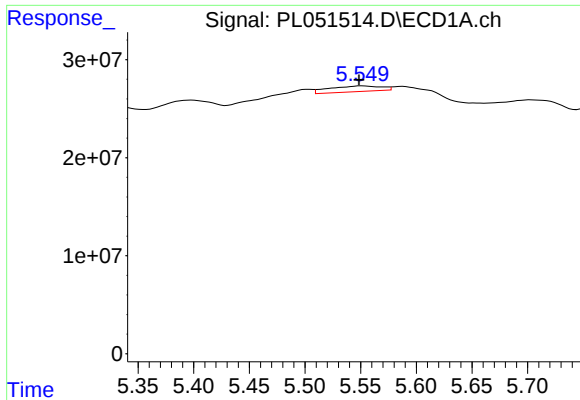

#13 Dieldrin


R.T.: 5.551 min
Delta R.T.: 0.002 min
Response: 18783136
Conc: 1.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

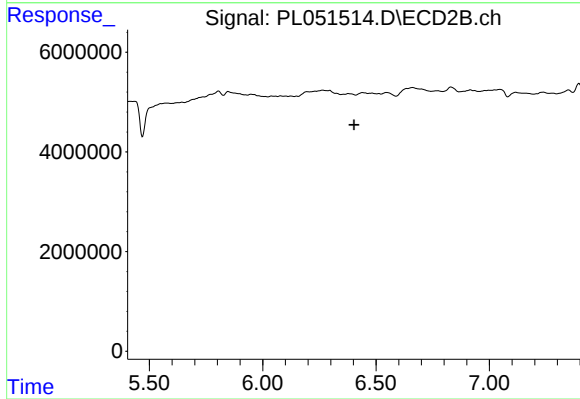


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.404 min
Response: 0
Conc: N.D.

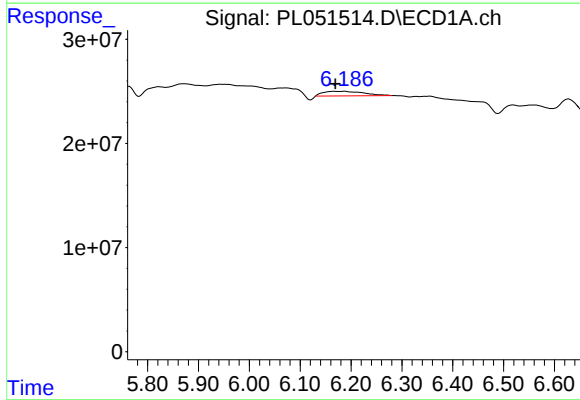


#17 4,4'-DDT

R.T.: 6.187 min
Delta R.T.: 0.018 min
Response: 24767921
Conc: 2.00 ng/ml

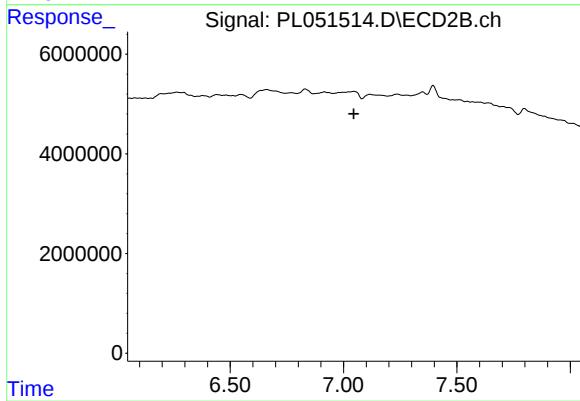

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.046 min
Response: 0
Conc: N.D.

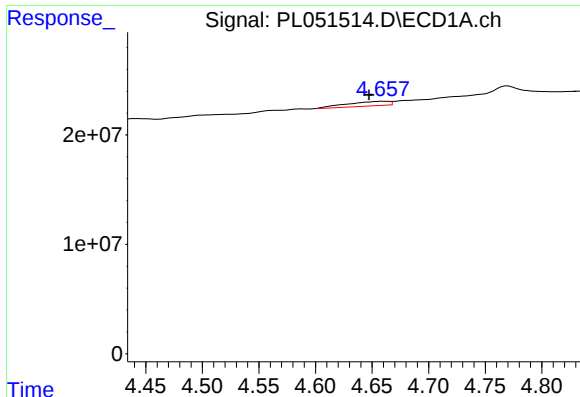

#24 Chlordane-2


R.T.: 4.659 min
Delta R.T.: 0.012 min
Response: 10558508
Conc: 23.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

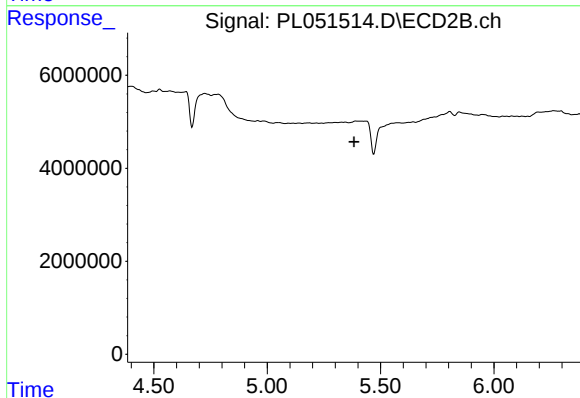


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.383 min
Response: 0
Conc: N.D.

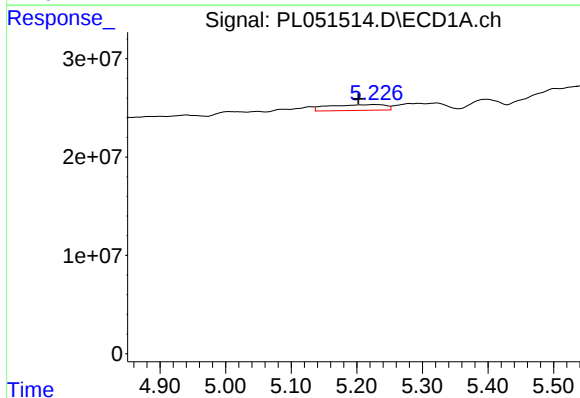


#25 Chlordane-3

R.T.: 5.227 min
Delta R.T.: 0.025 min
Response: 35524075
Conc: 25.38 ng/ml

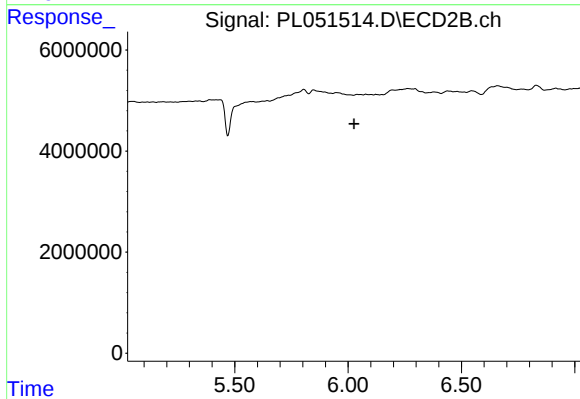

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

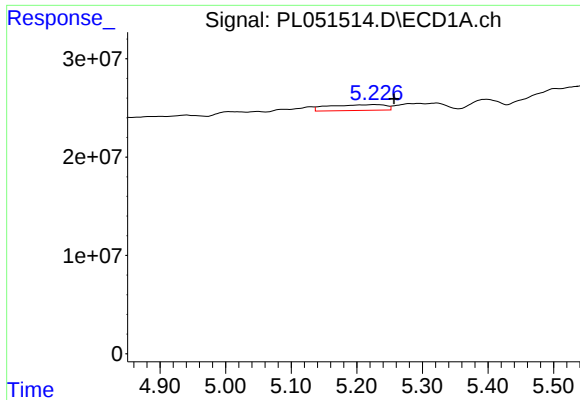

#26 Chlordane-4


R.T.: 5.227 min
Delta R.T.: -0.030 min
Response: 35524075
Conc: 26.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

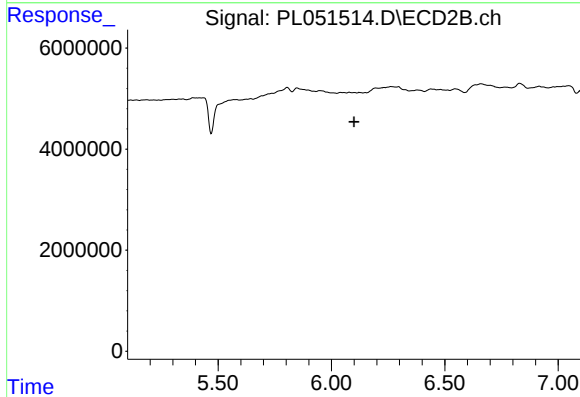


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.100 min
Response: 0
Conc: N.D.

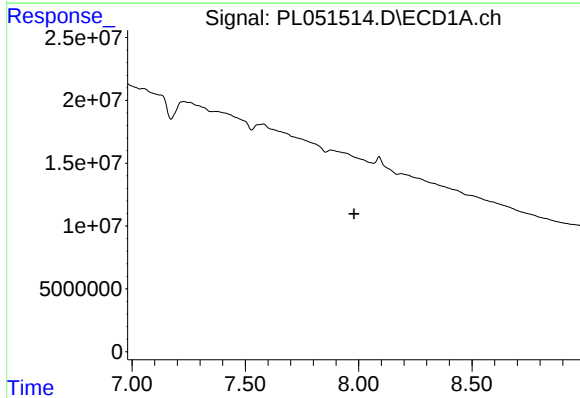

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.981 min
Response: 0
Conc: N.D.

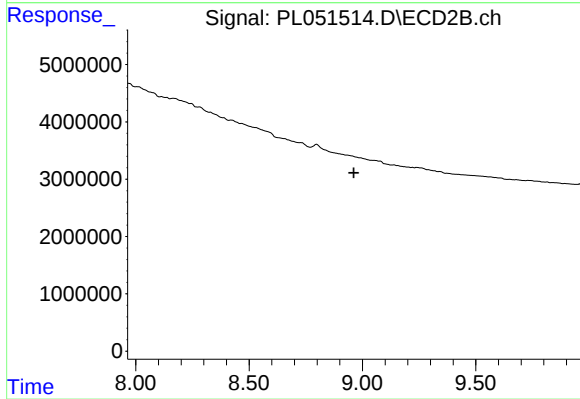

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.962 min
Response: 0
Conc: N.D.