

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081519\
 Data File : PL051521.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2019 15:45
 Operator : SG\AJ
 Sample : K4330-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 0633-COMP-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 00:51:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	3.926	198.6E6	51049794	19.764	17.892
28)	SA Decachlor...	7.975	8.953	150.2E6	37157751	14.839	13.140
Target Compounds							
6)	B beta-BHC	0.000	4.801f	0	2678834	N.D.	1.549 #
8)	B Heptachlo...	0.000	5.803	0	3007742	N.D.	0.786 #
9)	A Endosulfan I	5.336f	0.000	2664683	0	0.183	N.D. #
11)	B alpha-Chl...	5.265	0.000	36962922	0	2.423	N.D. #
15)	B Endosulfa...	0.000	6.843	0	4116516	N.D.	1.295 #
16)	A 4,4'-DDD	5.933	0.000	3165066	0	0.264	N.D. #
22)	Mirex	7.109	0.000	5163979	0	0.527	N.D. #
26)	Chlordane-4	5.265	0.000	36962922	0	28.024	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081519\
Data File : PL051521.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2019 15:45
Operator : SG\AJ
Sample : K4330-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
0633-COMP-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 00:51:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

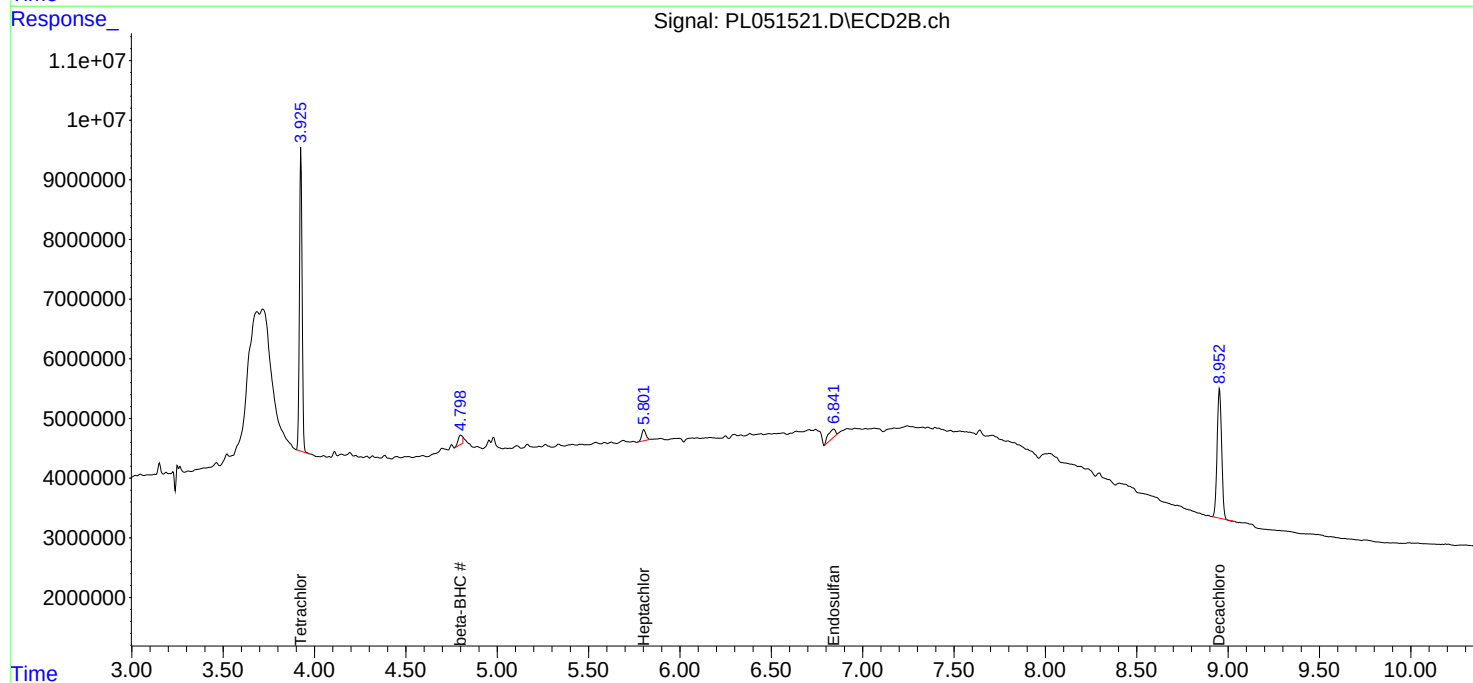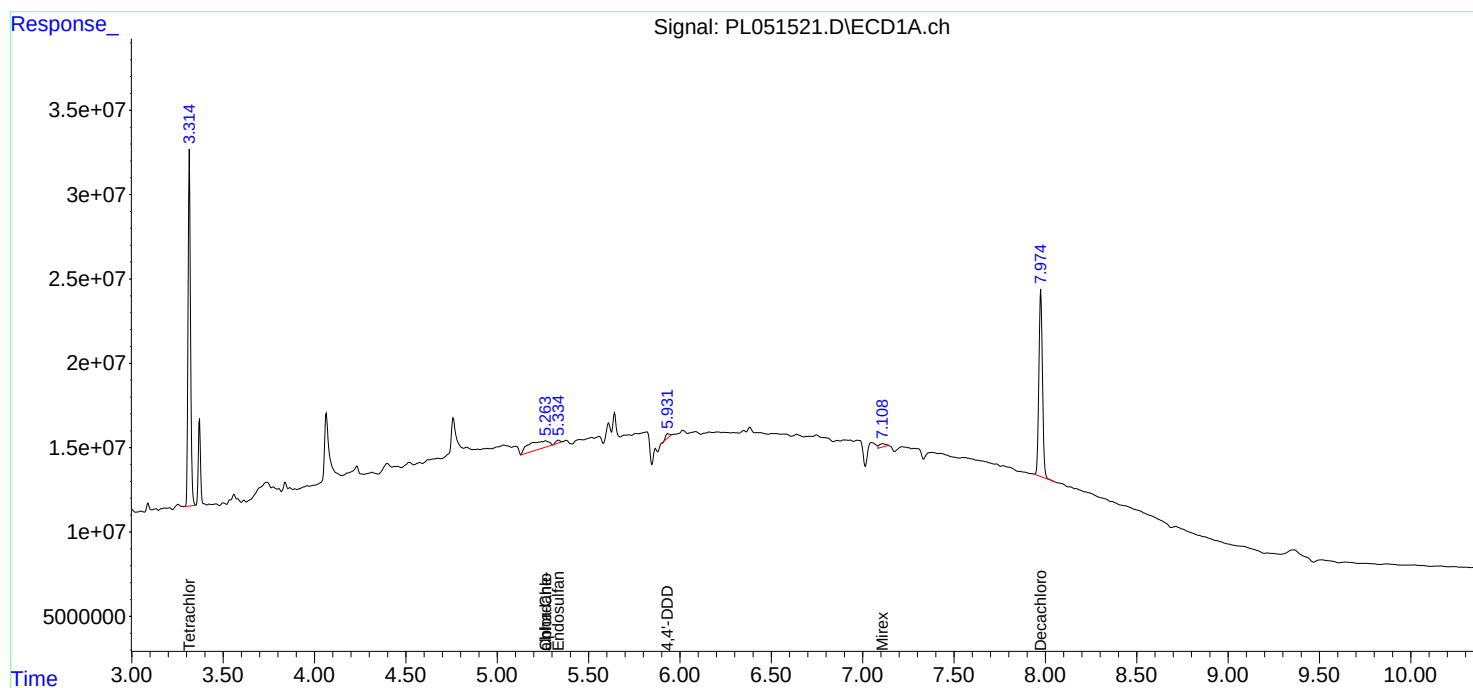


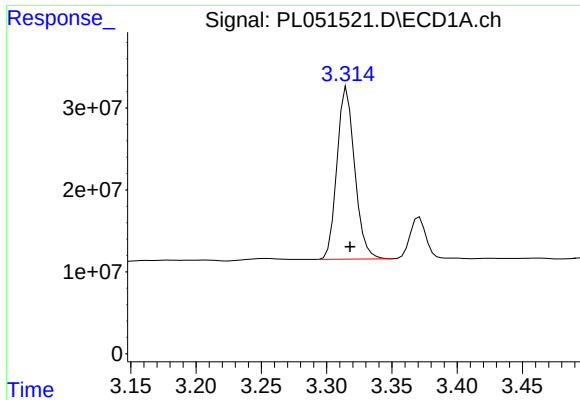

#1 Tetrachloro-m-xylene


R.T.: 3.316 min
Delta R.T.: -0.002 min
Response: 198581774
Conc: 19.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
0633-COMP-D

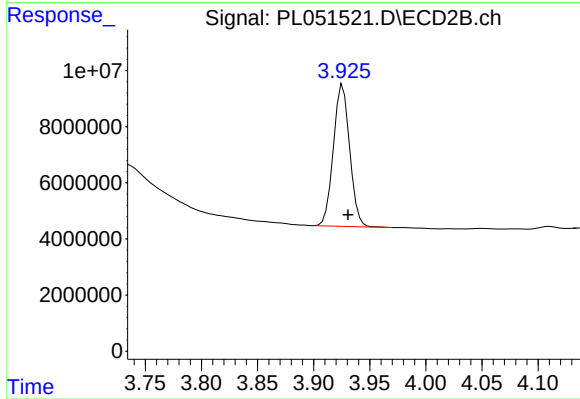


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.005 min
Response: 51049794
Conc: 17.89 ng/ml

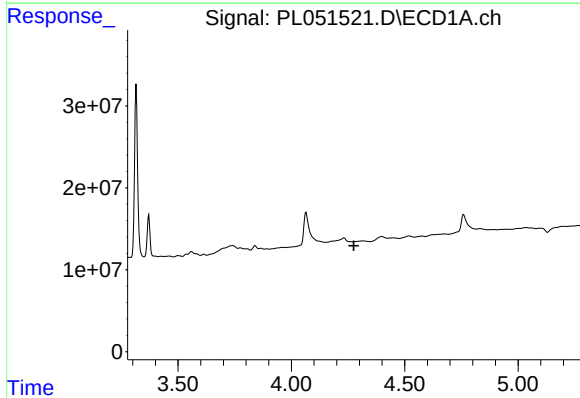


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

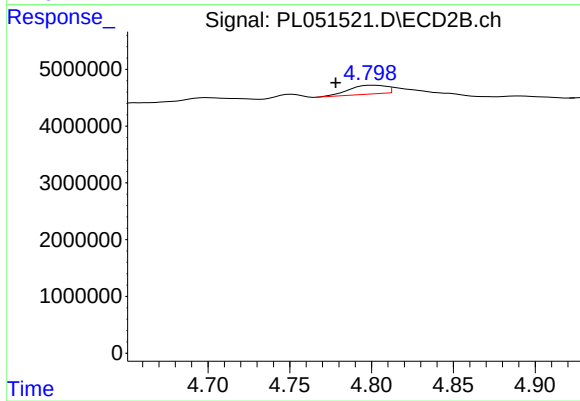

#6 beta-BHC


R.T.: 4.801 min
Delta R.T.: 0.023 min
Response: 2678834
Conc: 1.55 ng/ml

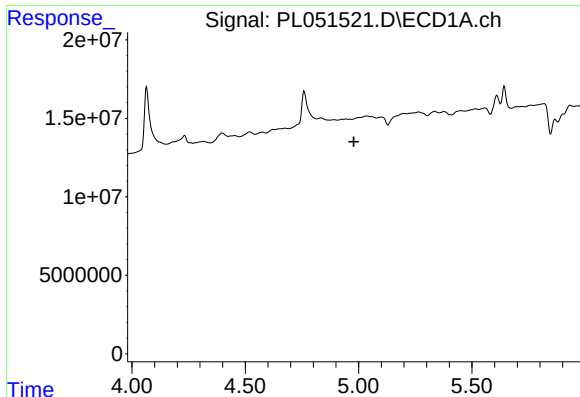

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
0633-COMP-D

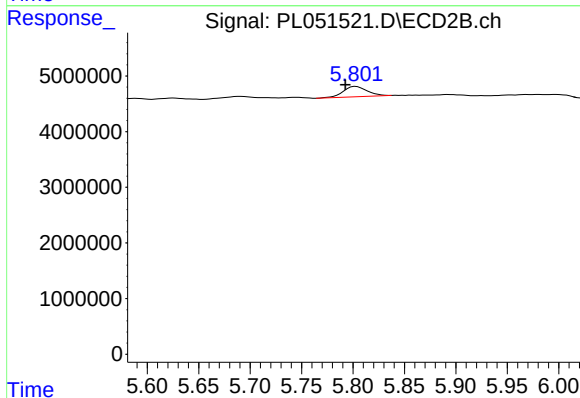


#8 Heptachlor epoxide

R.T.: 5.803 min
Delta R.T.: 0.010 min
Response: 3007742
Conc: 0.79 ng/ml

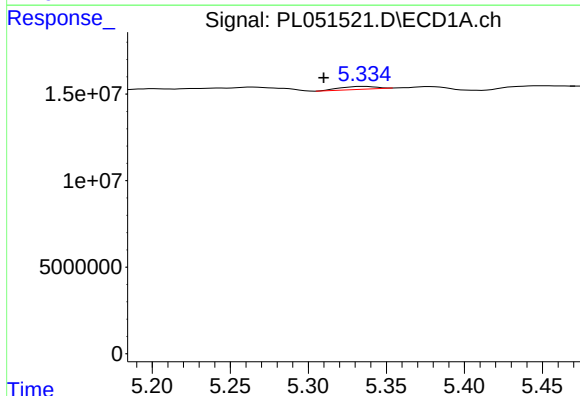


#9 Endosulfan I

R.T.: 5.336 min
Delta R.T.: 0.026 min
Response: 2664683
Conc: 0.18 ng/ml

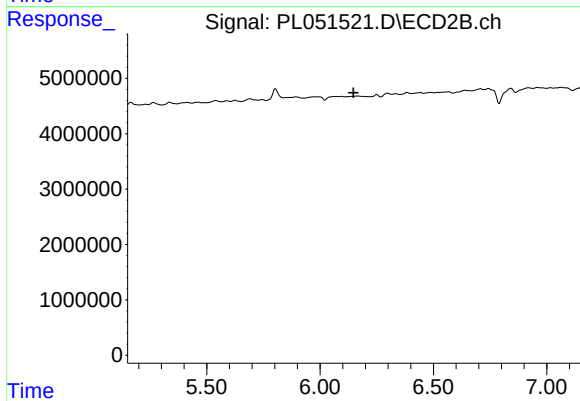

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.148 min
Response: 0
Conc: N.D.

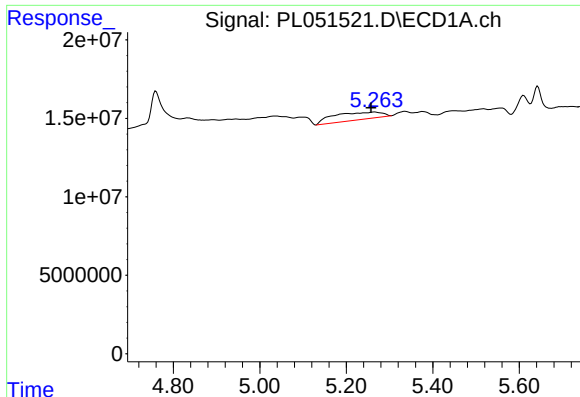

#11 alpha-Chlordane


R.T.: 5.265 min
Delta R.T.: 0.007 min
Response: 36962922
Conc: 2.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
0633-COMP-D

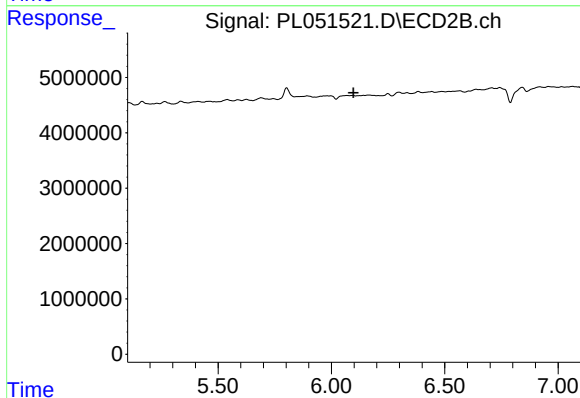


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

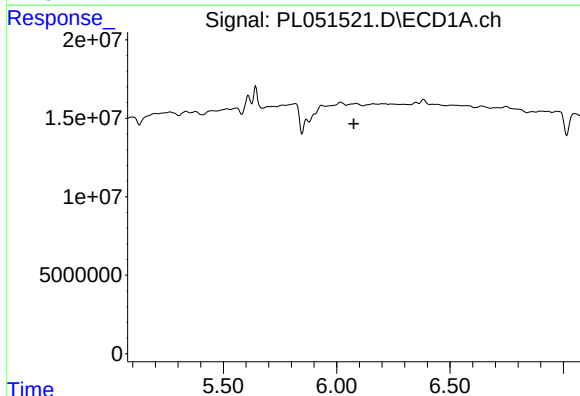


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.076 min
Response: 0
Conc: N.D.

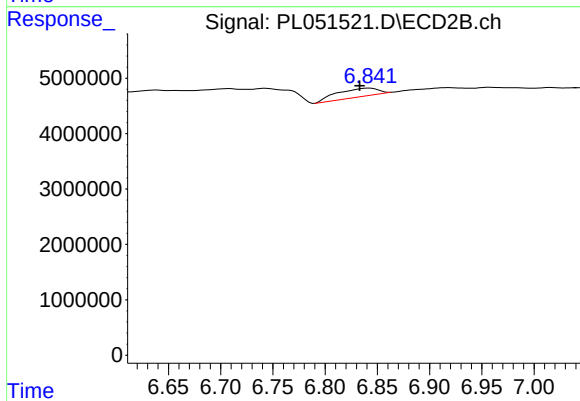

#15 Endosulfan II


R.T.: 6.843 min
Delta R.T.: 0.009 min
Response: 4116516
Conc: 1.29 ng/ml

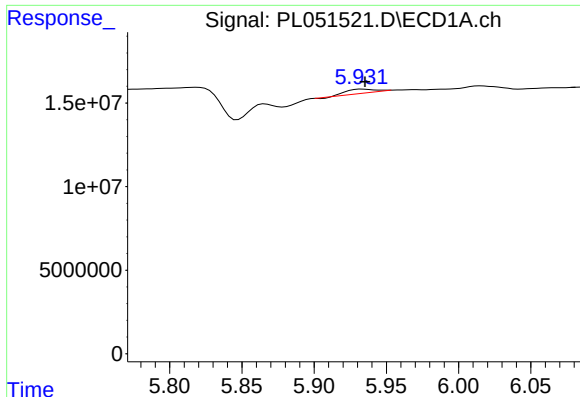

#16 4,4'-DDD


R.T.: 5.933 min
Delta R.T.: -0.002 min
Response: 3165066
Conc: 0.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
0633-COMP-D

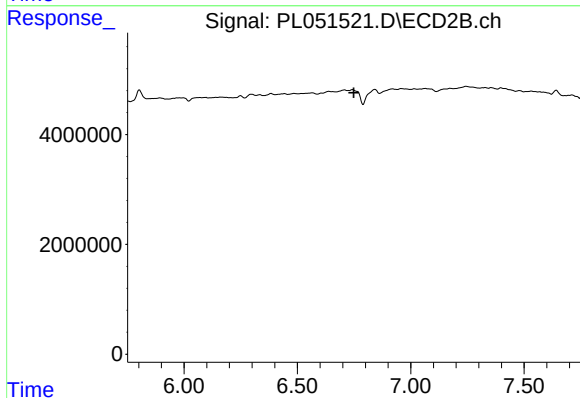


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.749 min
Response: 0
Conc: N.D.

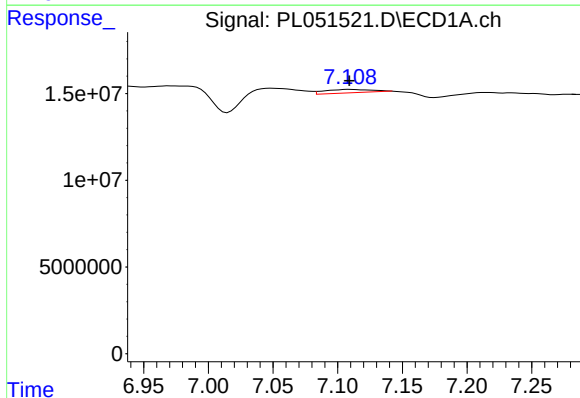


#22 Mirex

R.T.: 7.109 min
Delta R.T.: 0.000 min
Response: 5163979
Conc: 0.53 ng/ml

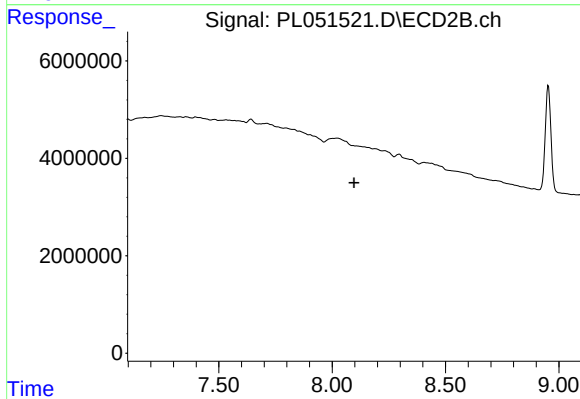

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 8.097 min
Response: 0
Conc: N.D.

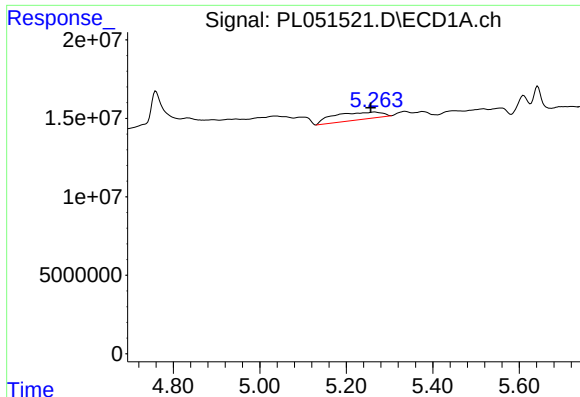

#26 Chlordane-4


R.T.: 5.265 min
Delta R.T.: 0.008 min
Response: 36962922
Conc: 28.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
0633-COMP-D

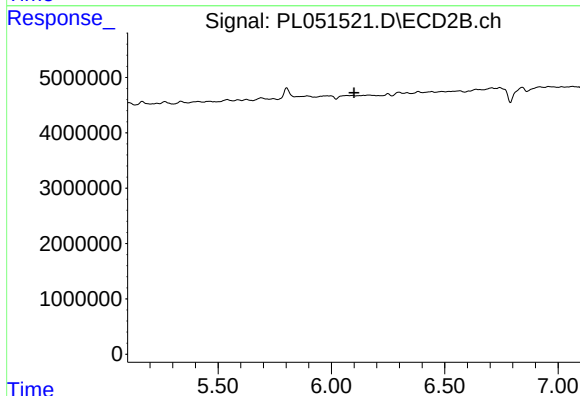


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.100 min
Response: 0
Conc: N.D.

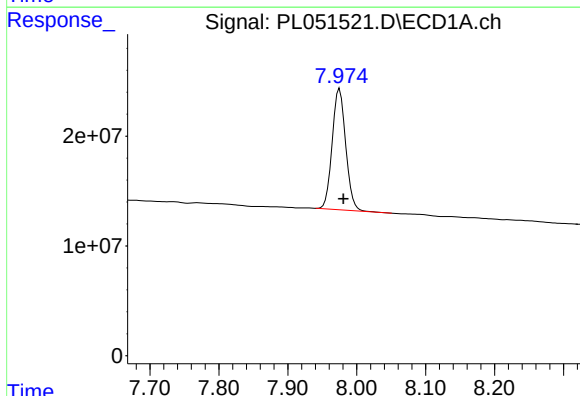

#28 Decachlorobiphenyl

R.T.: 7.975 min
Delta R.T.: -0.005 min
Response: 150247822
Conc: 14.84 ng/ml

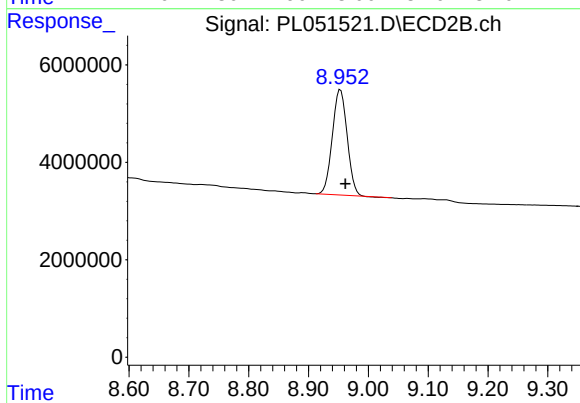

#28 Decachlorobiphenyl

R.T.: 8.953 min
Delta R.T.: -0.008 min
Response: 37157751
Conc: 13.14 ng/ml