

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081519\
 Data File : PL051522.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2019 15:59
 Operator : SG\AJ
 Sample : K4331-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 0625-COMP-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 00:51:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	3.926	227.1E6	61107077	22.605	21.417
28)	SA Decachlor...	7.974	8.953	165.1E6	41180018	16.307	14.562
Target Compounds							
5)	MB Aldrin	4.528f	0.000	25374975	0	1.638	N.D. #
6)	B beta-BHC	0.000	4.801f	0	1598758	N.D.	0.925 #
10)	B gamma-Chl...	5.188	0.000	21944708	0	1.390	N.D. #
15)	B Endosulfa...	0.000	6.844	0	796493	N.D.	0.251 #
22)	Mirex	7.108	0.000	4635786	0	0.473	N.D. #
25)	Chlordane-3	5.188	0.000	21944708	0	15.677	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081519\
Data File : PL051522.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2019 15:59
Operator : SG\AJ
Sample : K4331-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
0625-COMP-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 00:51:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

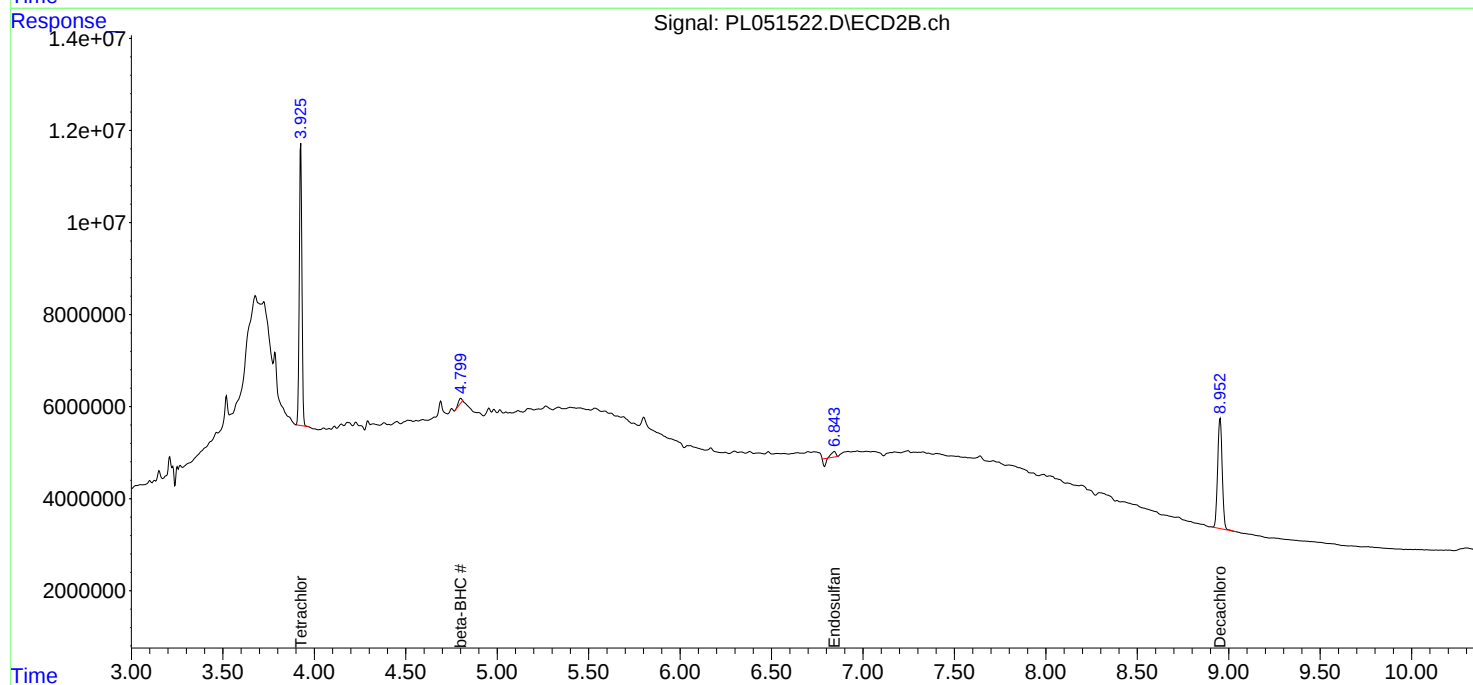


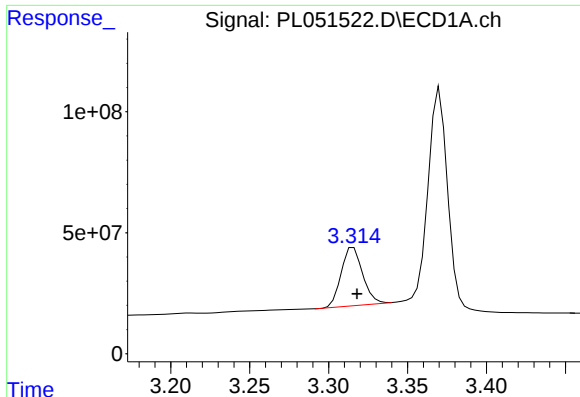

#1 Tetrachloro-m-xylene


R.T.: 3.316 min
Delta R.T.: -0.002 min
Response: 227129852
Conc: 22.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
0625-COMP-B

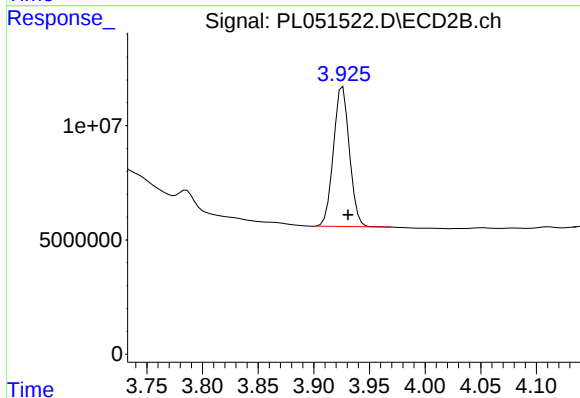


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.005 min
Response: 61107077
Conc: 21.42 ng/ml

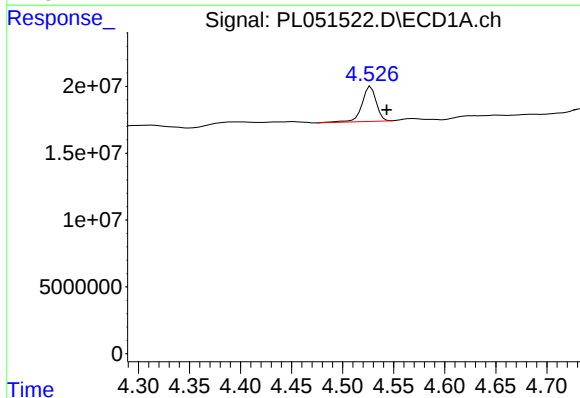


#5 Aldrin

R.T.: 4.528 min
Delta R.T.: -0.016 min
Response: 25374975
Conc: 1.64 ng/ml

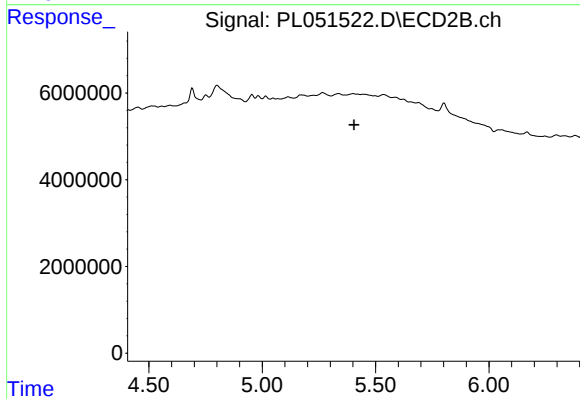

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.405 min
Response: 0
Conc: N.D.

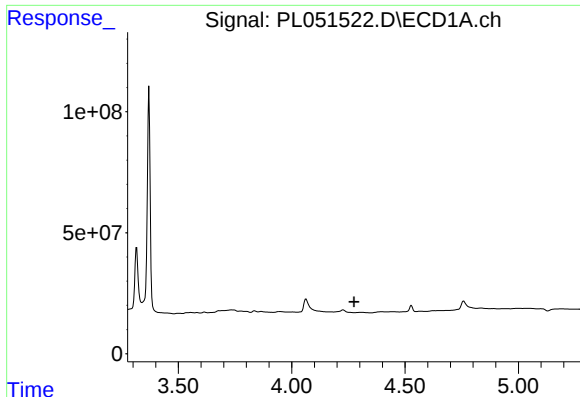

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
0625-COMP-B

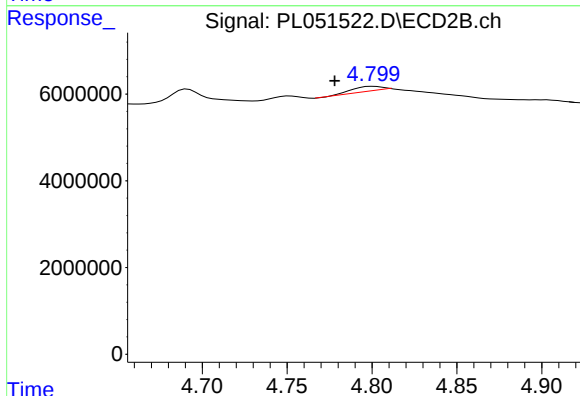


#6 beta-BHC

R.T.: 4.801 min
Delta R.T.: 0.023 min
Response: 1598758
Conc: 0.92 ng/ml

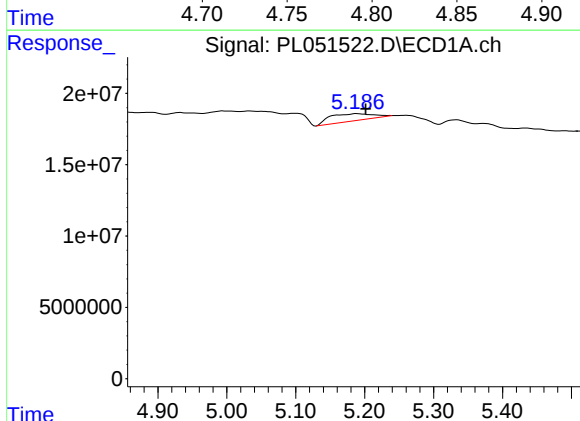


#10 gamma-Chlordane

R.T.: 5.188 min
Delta R.T.: -0.014 min
Response: 21944708
Conc: 1.39 ng/ml

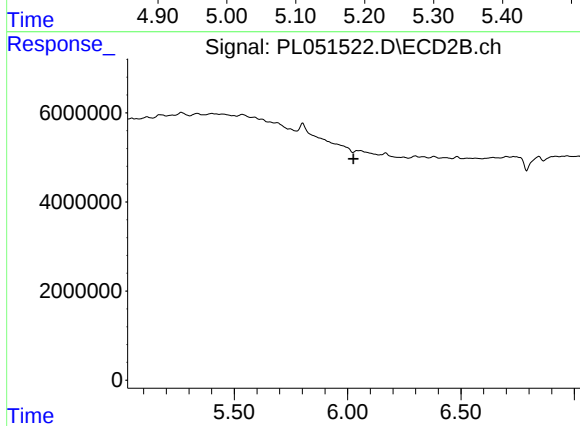

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.026 min
Response: 0
Conc: N.D.

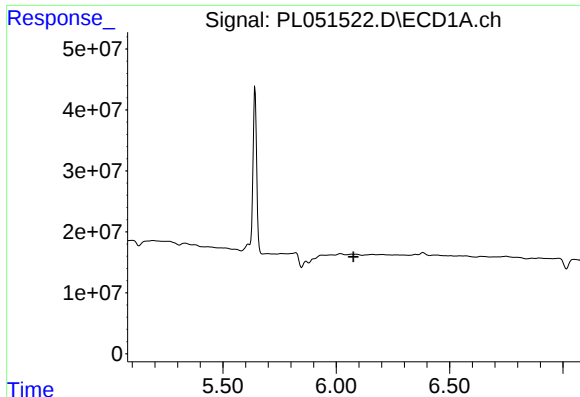

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.076 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
0625-COMP-B

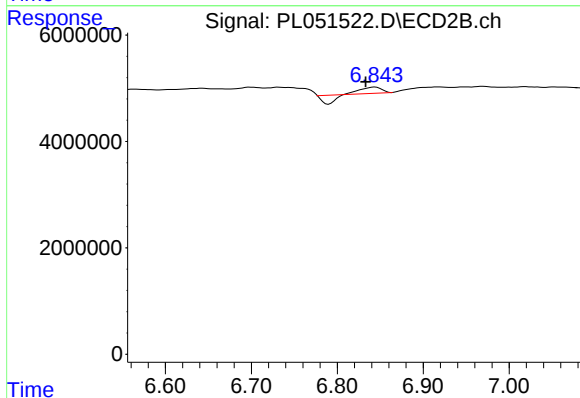


#15 Endosulfan II

R.T.: 6.844 min
Delta R.T.: 0.011 min
Response: 796493
Conc: 0.25 ng/ml

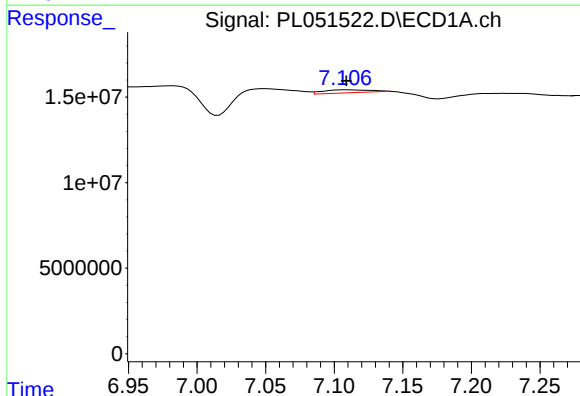


#22 Mirex

R.T.: 7.108 min
Delta R.T.: 0.000 min
Response: 4635786
Conc: 0.47 ng/ml

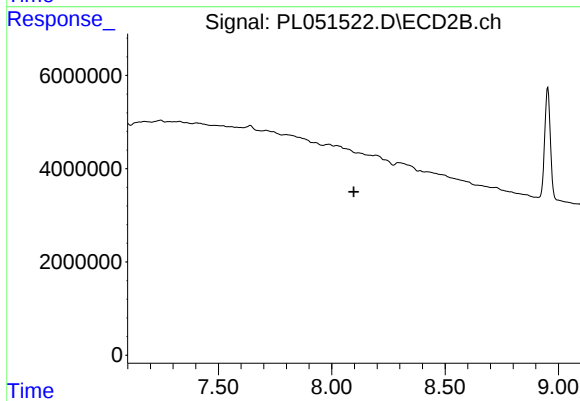

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 8.097 min
Response: 0
Conc: N.D.

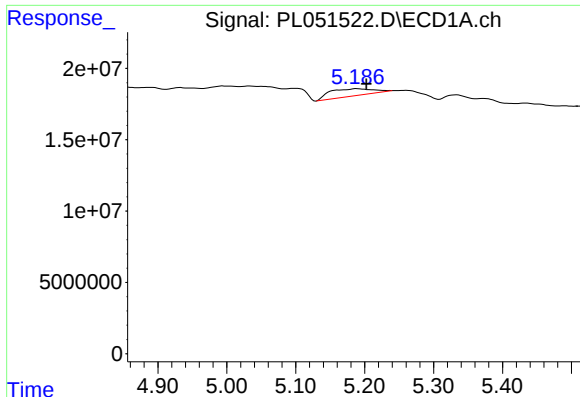

#25 Chlordane-3


R.T.: 5.188 min
Delta R.T.: -0.015 min
Response: 21944708
Conc: 15.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
0625-COMP-B

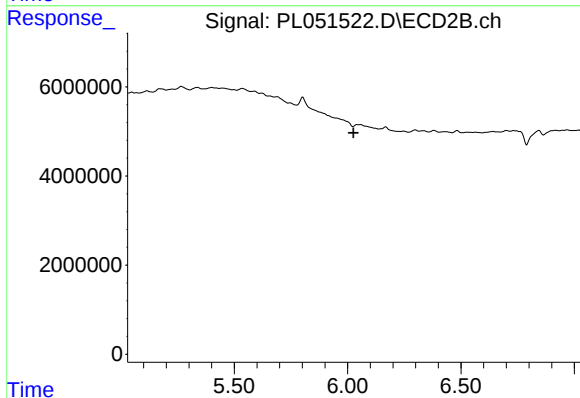


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 6.027 min
Response: 0
Conc: N.D.

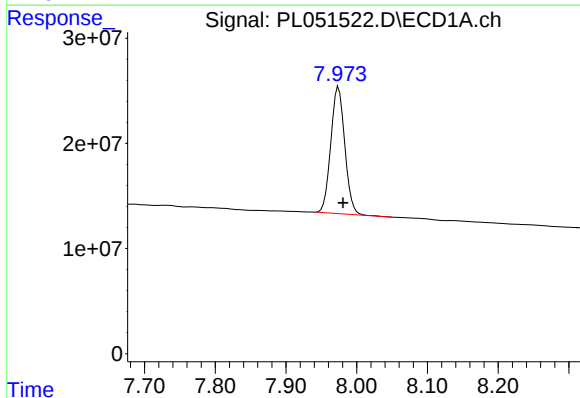

#28 Decachlorobiphenyl

R.T.: 7.974 min
Delta R.T.: -0.006 min
Response: 165109104
Conc: 16.31 ng/ml

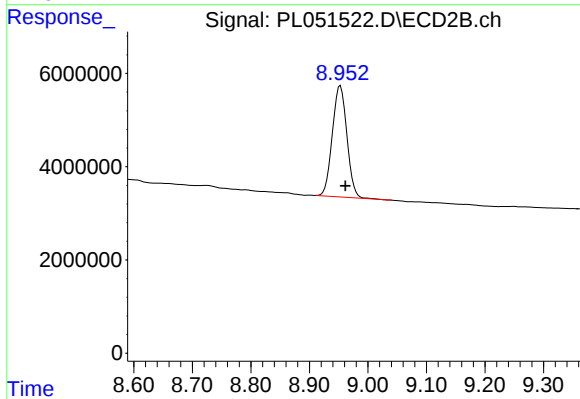

#28 Decachlorobiphenyl

R.T.: 8.953 min
Delta R.T.: -0.009 min
Response: 41180018
Conc: 14.56 ng/ml