

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081519\
 Data File : PL051524.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2019 16:27
 Operator : SG\AJ
 Sample : K4356-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 00:52:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	3.926	124.6E6	31991842	12.396	11.213
28)	SA Decachlor...	7.974	8.953	50360463	12569839	4.974	4.445
Target Compounds							
6)	B beta-BHC	0.000	4.805f	0	1439892	N.D.	0.833 #
8)	B Heptachlo...	0.000	5.802	0	5765599	N.D.	1.507 #
9)	A Endosulfan I	5.327f	0.000	3904474	0	0.268	N.D. #
10)	B gamma-Chl...	5.220f	0.000	30843473	0	1.954	N.D. #
11)	B alpha-Chl...	5.281f	0.000	9073673	0	0.595	N.D. #
15)	B Endosulfa...	0.000	6.845	0	13793930	N.D.	4.339 #
25)	Chlordane-3	5.220f	0.000	30843473	0	22.034	N.D. #
26)	Chlordane-4	5.281f	0.000	9073673	0	6.879	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081519\
Data File : PL051524.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2019 16:27
Operator : SG\AJ
Sample : K4356-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 00:52:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

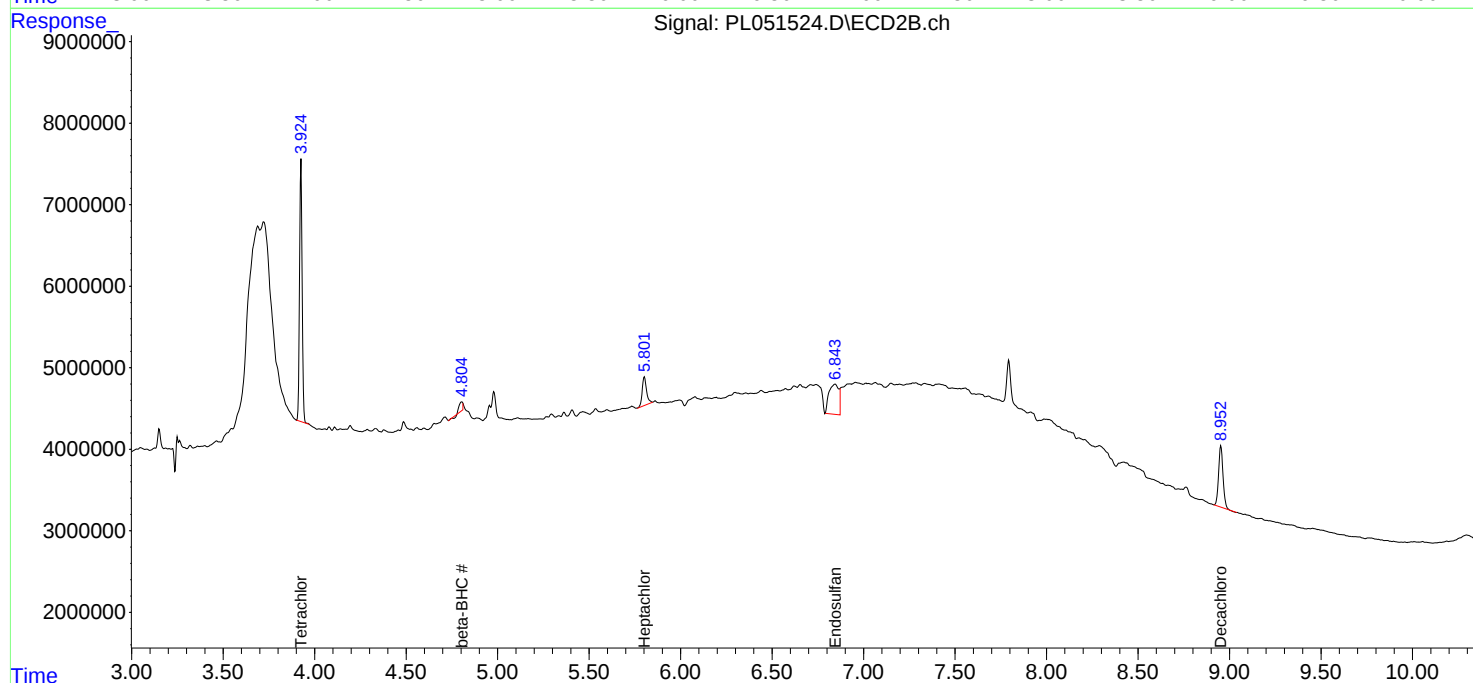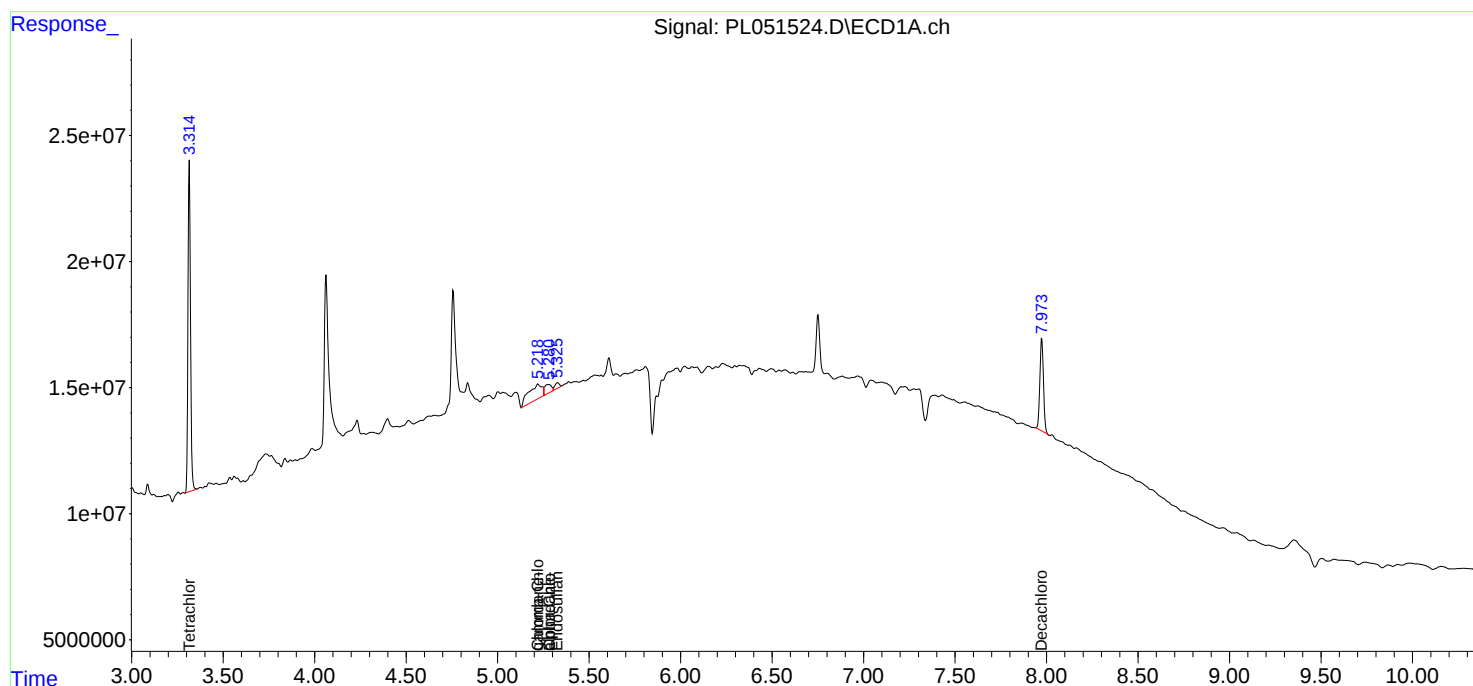


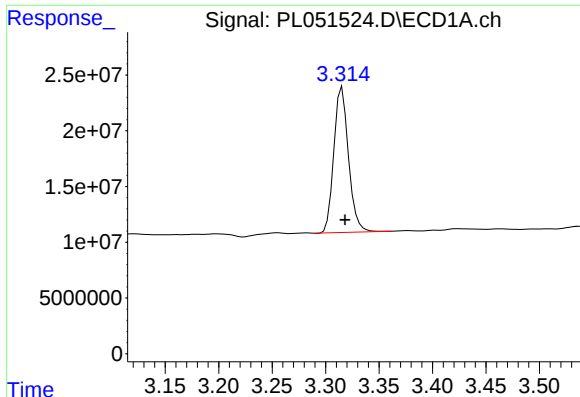

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: -0.003 min
Response: 124555951
Conc: 12.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

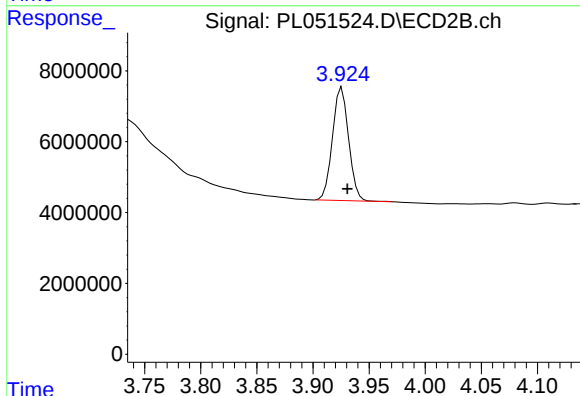


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.005 min
Response: 31991842
Conc: 11.21 ng/ml

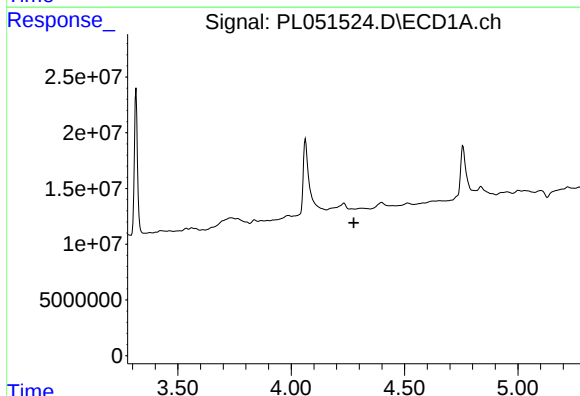


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

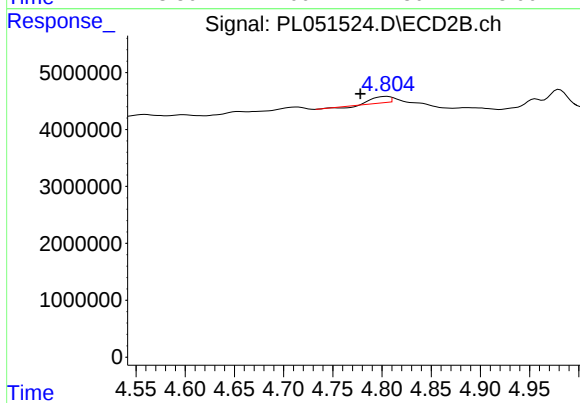

#6 beta-BHC


R.T.: 4.805 min
Delta R.T.: 0.027 min
Response: 1439892
Conc: 0.83 ng/ml

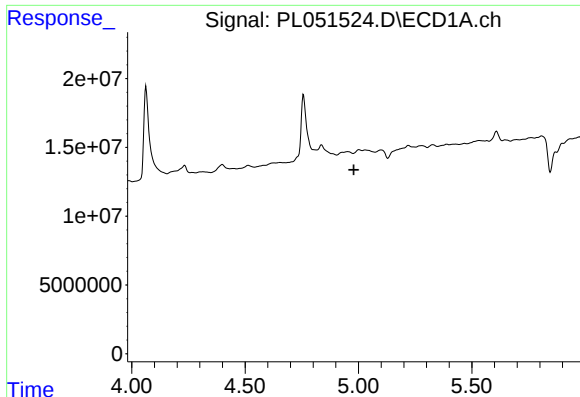

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-1

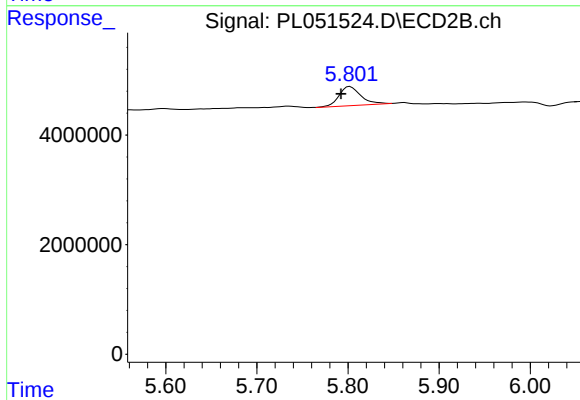


#8 Heptachlor epoxide

R.T.: 5.802 min
Delta R.T.: 0.010 min
Response: 5765599
Conc: 1.51 ng/ml

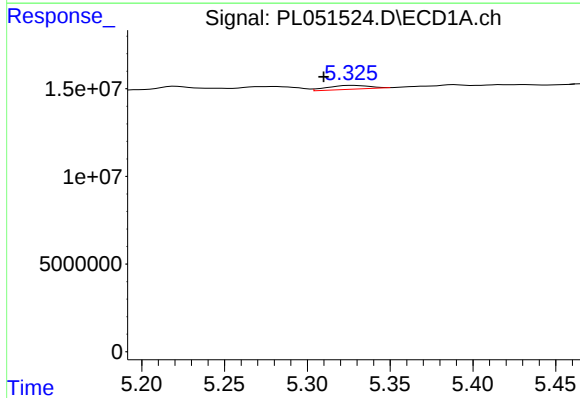


#9 Endosulfan I

R.T.: 5.327 min
Delta R.T.: 0.018 min
Response: 3904474
Conc: 0.27 ng/ml

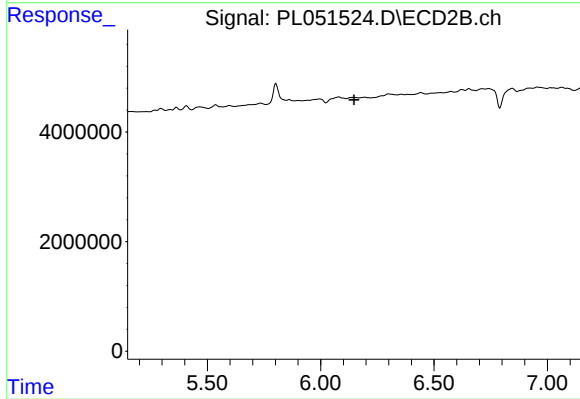

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.148 min
Response: 0
Conc: N.D.

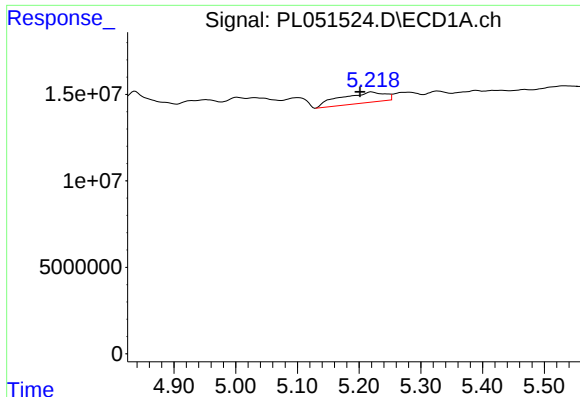

#10 gamma-Chlordane


R.T.: 5.220 min
Delta R.T.: 0.019 min
Response: 30843473
Conc: 1.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

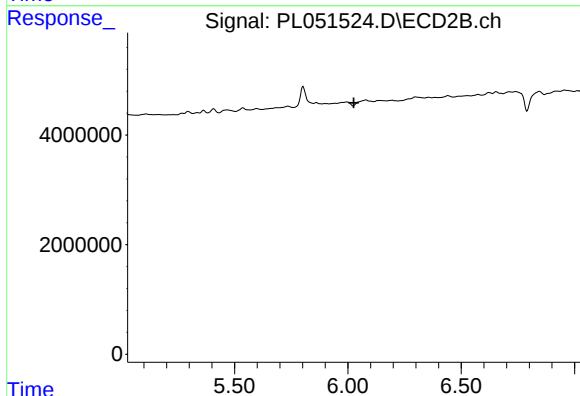


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

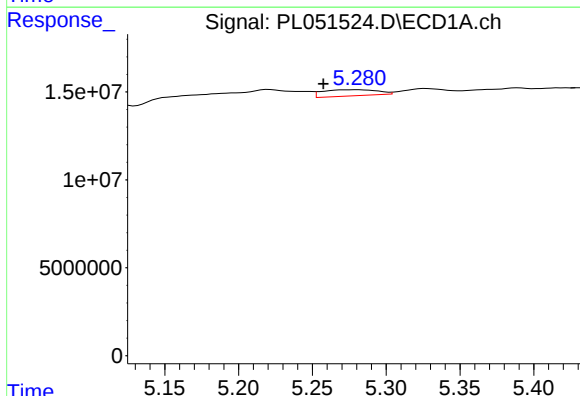


#11 alpha-Chlordane

R.T.: 5.281 min
Delta R.T.: 0.024 min
Response: 9073673
Conc: 0.59 ng/ml

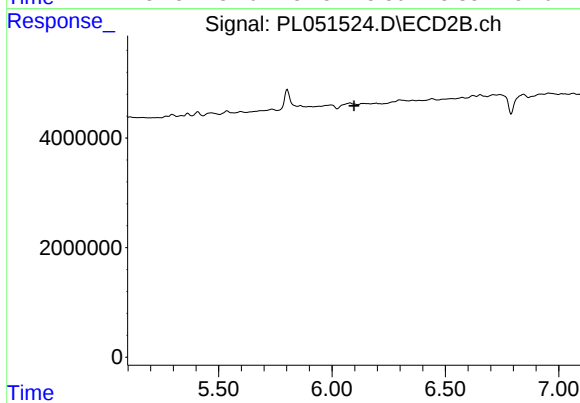

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

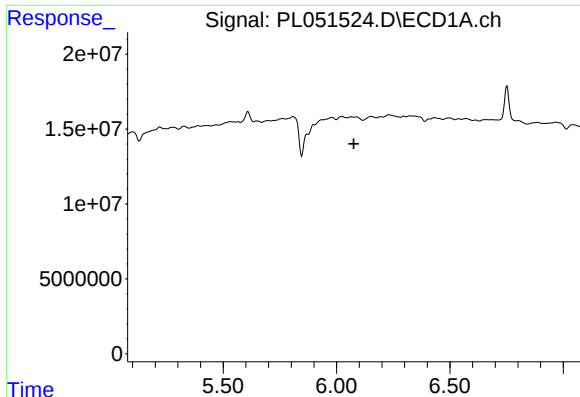

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.076 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-1

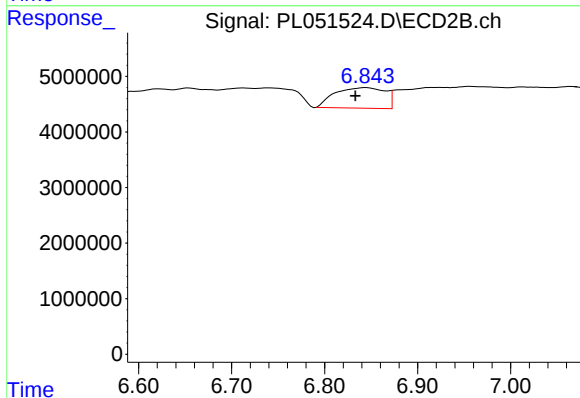


#15 Endosulfan II

R.T.: 6.845 min
Delta R.T.: 0.011 min
Response: 13793930
Conc: 4.34 ng/ml

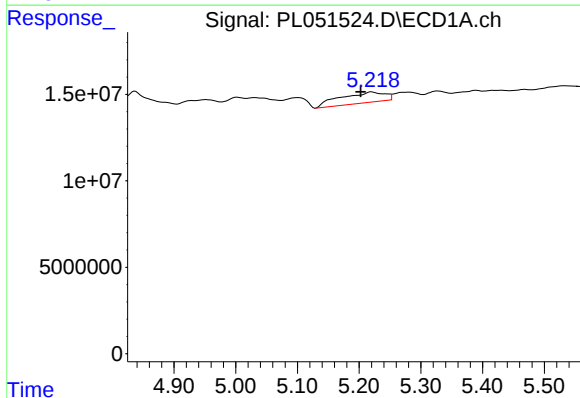


#25 Chlordane-3

R.T.: 5.220 min
Delta R.T.: 0.018 min
Response: 30843473
Conc: 22.03 ng/ml

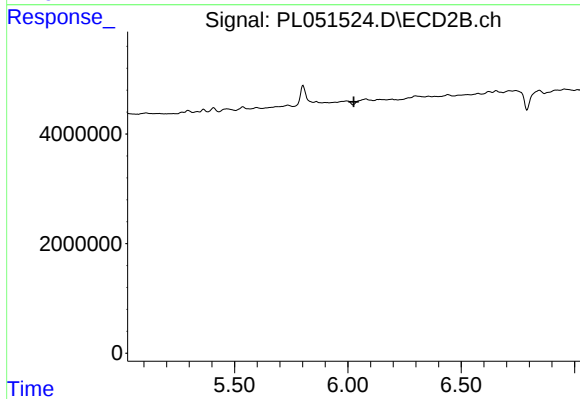

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.027 min
Response: 0
Conc: N.D.

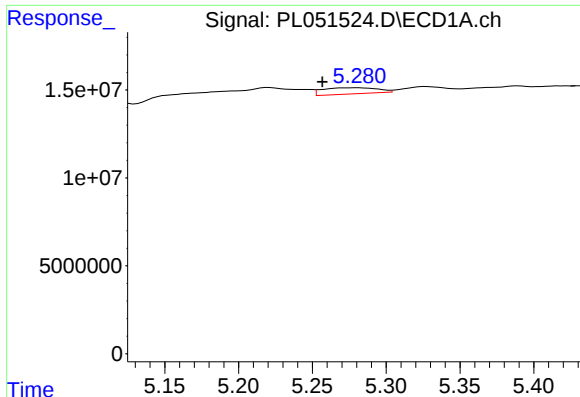

#26 Chlordane-4


R.T.: 5.281 min
Delta R.T.: 0.024 min
Response: 9073673
Conc: 6.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

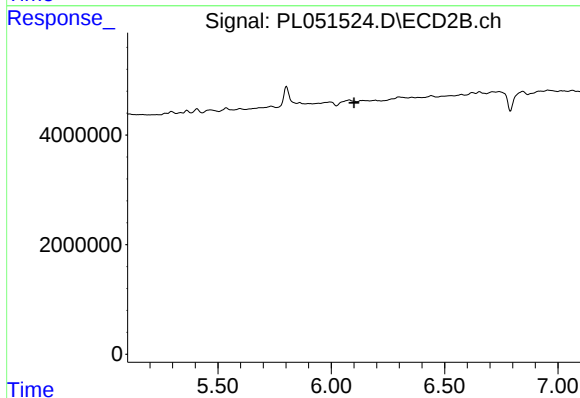


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.100 min
Response: 0
Conc: N.D.

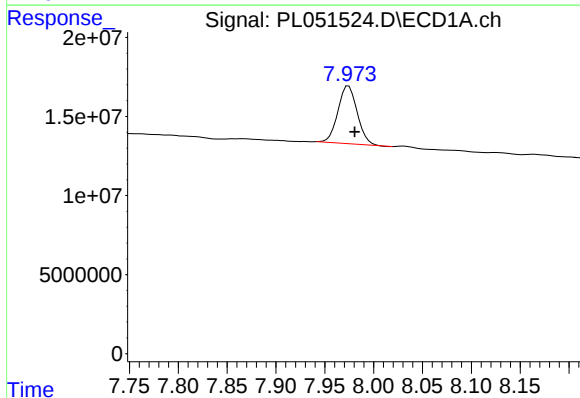

#28 Decachlorobiphenyl

R.T.: 7.974 min
Delta R.T.: -0.006 min
Response: 50360463
Conc: 4.97 ng/ml

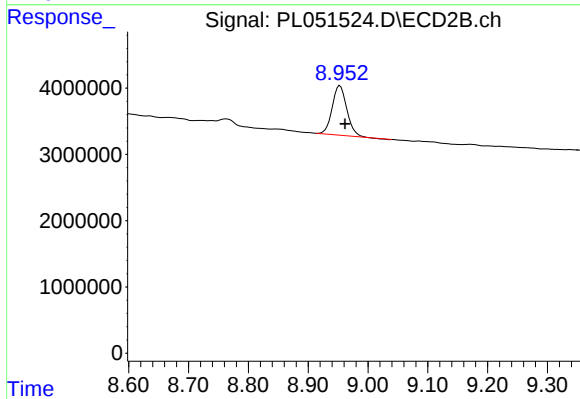

#28 Decachlorobiphenyl

R.T.: 8.953 min
Delta R.T.: -0.009 min
Response: 12569839
Conc: 4.44 ng/ml