

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081519\
 Data File : PL051526.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2019 16:56
 Operator : SG\AJ
 Sample : K4365-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 00:52:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	3.925	117.4E6	30469899	11.683	10.679
28)	SA Decachlor...	7.974	8.953	57966656	15504499	5.725	5.483
Target Compounds							
6)	B beta-BHC	0.000	4.804f	0	1259049	N.D.	0.728 #
7)	B delta-BHC	0.000	4.979	0	3460024	N.D.	0.895 #
8)	B Heptachlo...	0.000	5.801	0	9638483	N.D.	2.520 #
9)	A Endosulfan I	5.326f	0.000	5391336	0	0.371	N.D. #
10)	B gamma-Chl...	5.220f	0.000	51060907	0	3.235	N.D. #
11)	B alpha-Chl...	5.271	0.000	14212046	0	0.932	N.D. #
13)	MA Dieldrin	5.535	0.000	9678463	0	0.625	N.D. #
15)	B Endosulfa...	0.000	6.844	0	7876061	N.D.	2.477 #
16)	A 4,4'-DDD	5.929	0.000	3367307	0	0.281	N.D. #
25)	Chlordane-3	5.220f	0.000	51060907	0	36.478	N.D. #
26)	Chlordane-4	5.271	0.000	14212046	0	10.775	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081519\
Data File : PL051526.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2019 16:56
Operator : SG\AJ
Sample : K4365-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 00:52:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

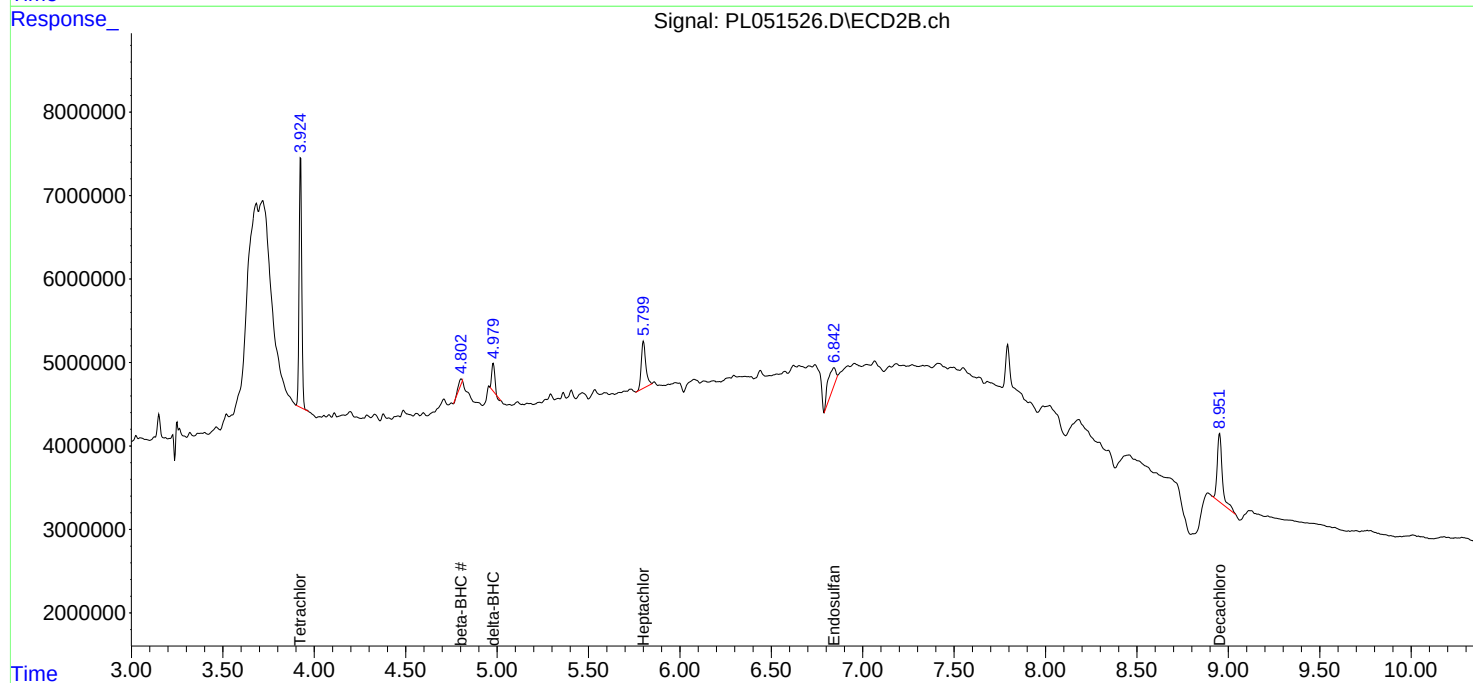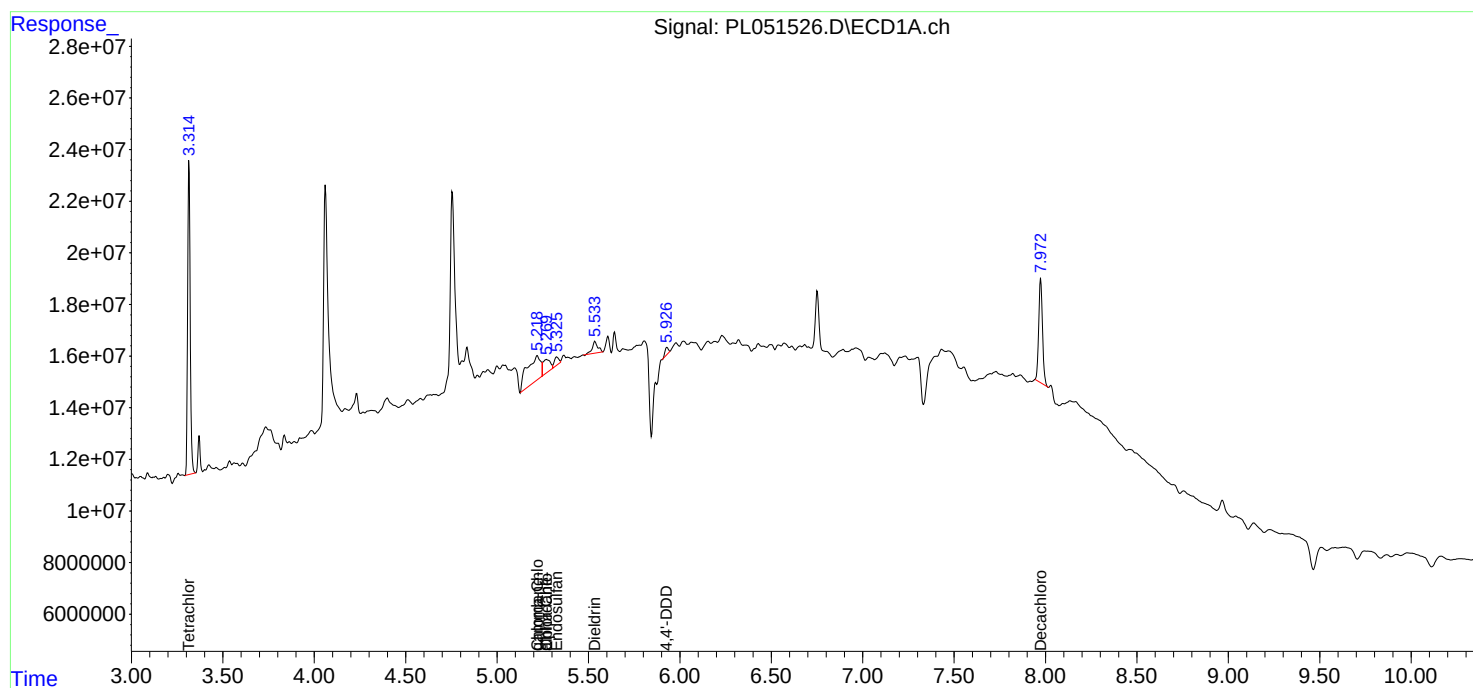


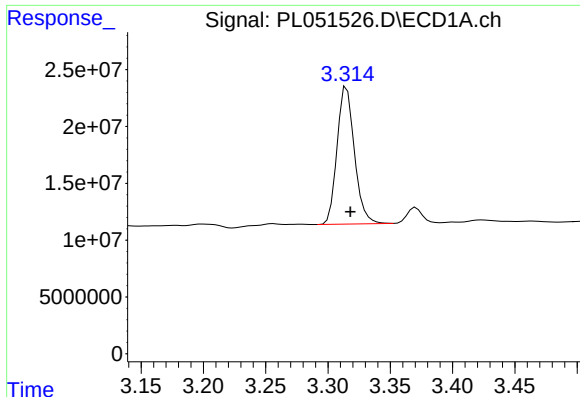

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: -0.003 min
Response: 117392255
Conc: 11.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

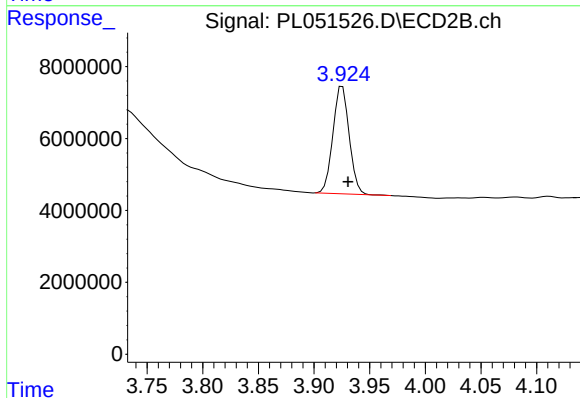


#1 Tetrachloro-m-xylene

R.T.: 3.925 min
Delta R.T.: -0.005 min
Response: 30469899
Conc: 10.68 ng/ml

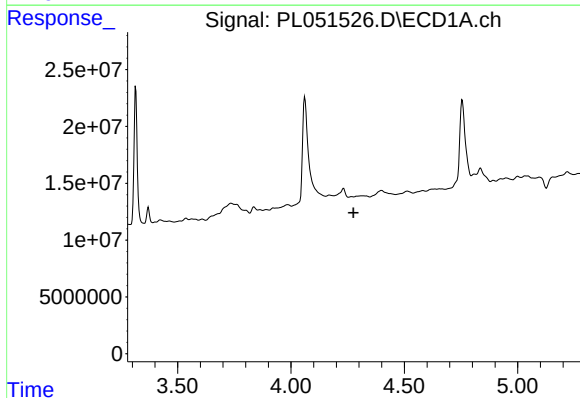


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

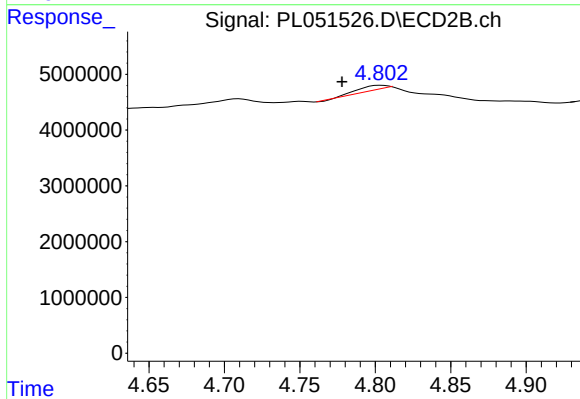

#6 beta-BHC


R.T.: 4.804 min
Delta R.T.: 0.026 min
Response: 1259049
Conc: 0.73 ng/ml

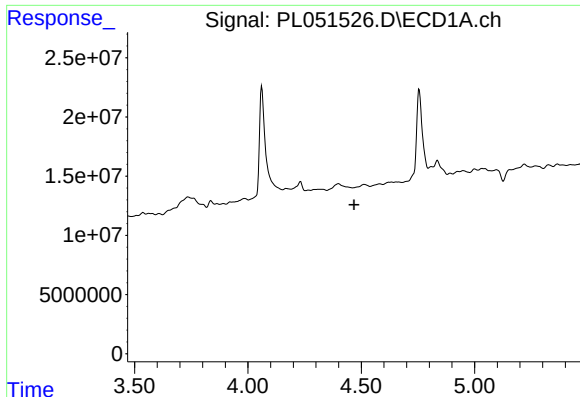

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.469 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-3

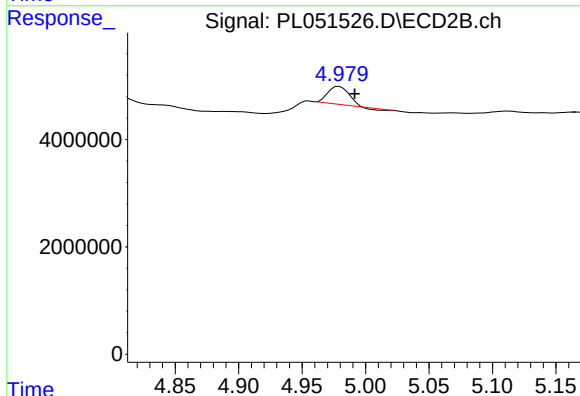


#7 delta-BHC

R.T.: 4.979 min
Delta R.T.: -0.012 min
Response: 3460024
Conc: 0.89 ng/ml

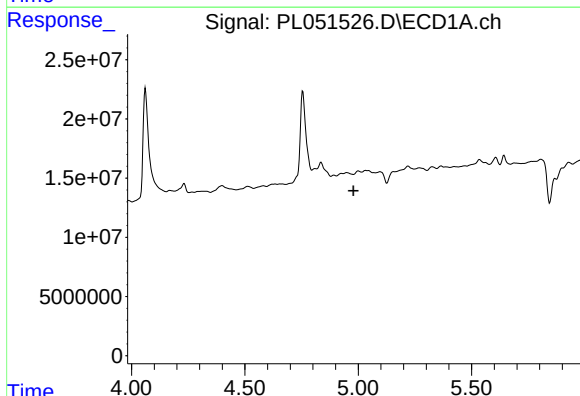


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.979 min
Response: 0
Conc: N.D.

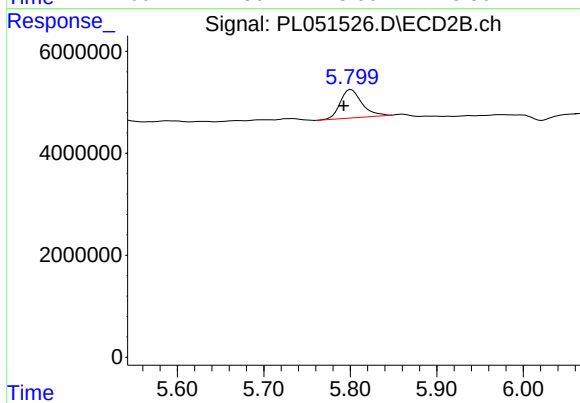

#8 Heptachlor epoxide


R.T.: 5.801 min
Delta R.T.: 0.008 min
Response: 9638483
Conc: 2.52 ng/ml

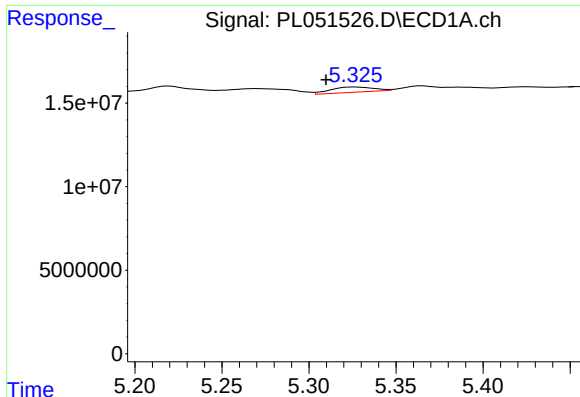

#9 Endosulfan I


R.T.: 5.326 min
Delta R.T.: 0.016 min
Response: 5391336
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

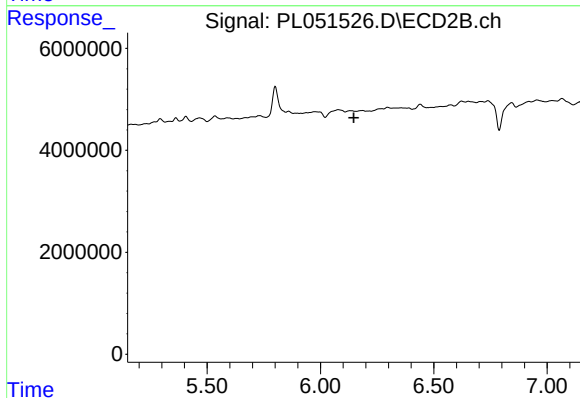


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.148 min
Response: 0
Conc: N.D.

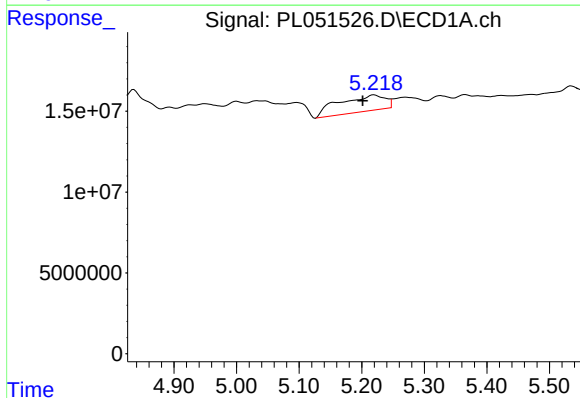


#10 gamma-Chlordane

R.T.: 5.220 min
Delta R.T.: 0.018 min
Response: 51060907
Conc: 3.24 ng/ml

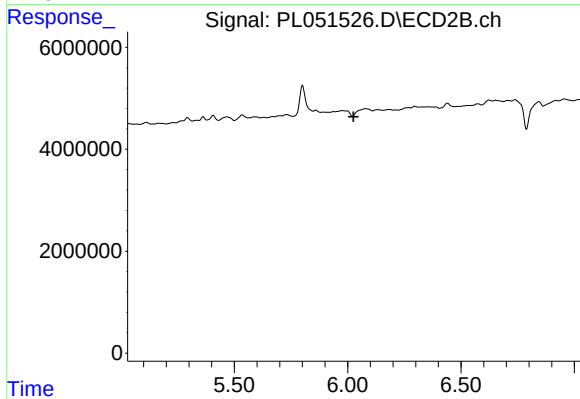

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

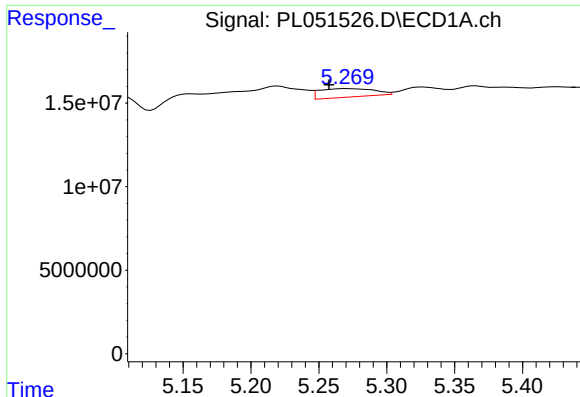

#11 alpha-Chlordane


R.T.: 5.271 min
Delta R.T.: 0.013 min
Response: 14212046
Conc: 0.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

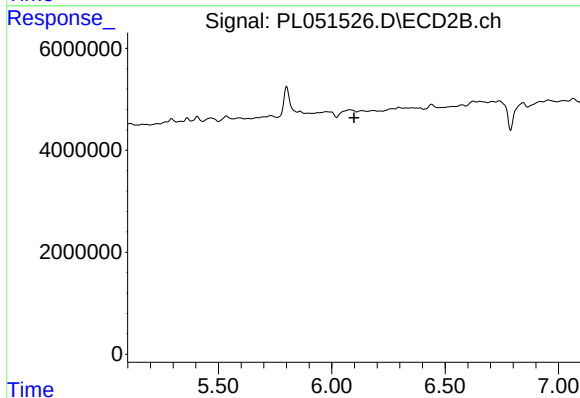


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

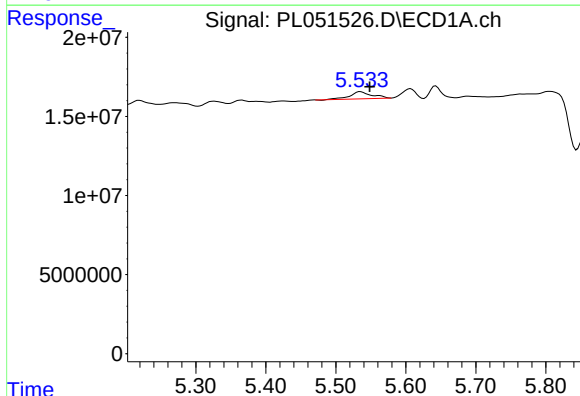


#13 Dieldrin

R.T.: 5.535 min
Delta R.T.: -0.014 min
Response: 9678463
Conc: 0.62 ng/ml

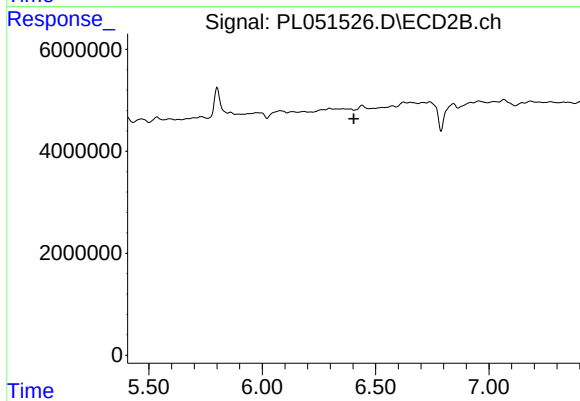

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.404 min
Response: 0
Conc: N.D.

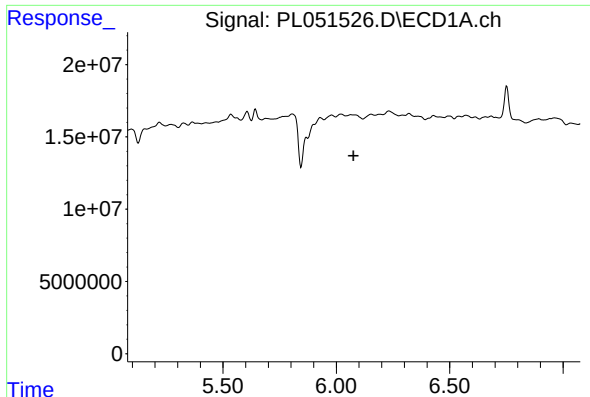

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.076 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-3

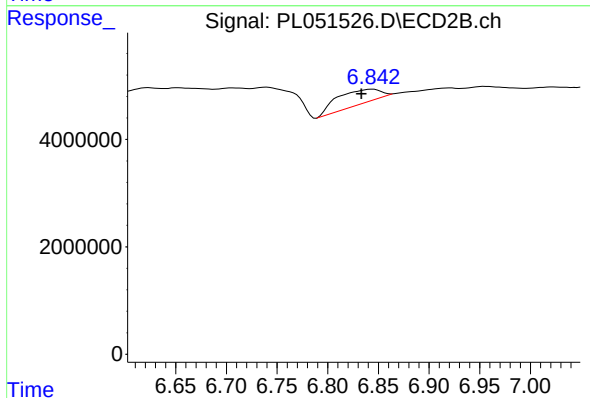


#15 Endosulfan II

R.T.: 6.844 min
Delta R.T.: 0.011 min
Response: 7876061
Conc: 2.48 ng/ml

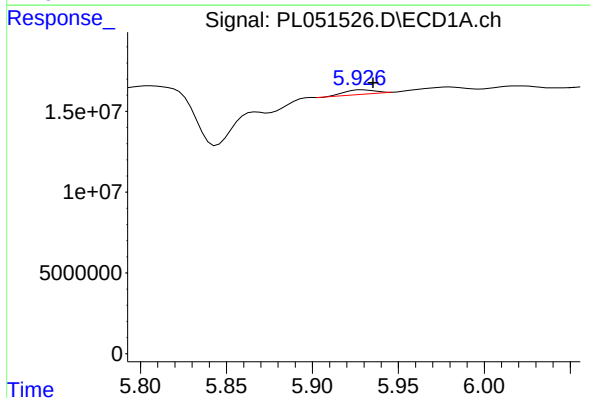


#16 4,4'-DDD

R.T.: 5.929 min
Delta R.T.: -0.006 min
Response: 3367307
Conc: 0.28 ng/ml

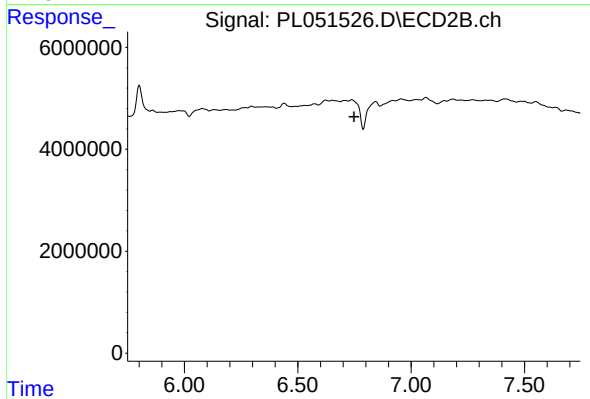

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.749 min
Response: 0
Conc: N.D.

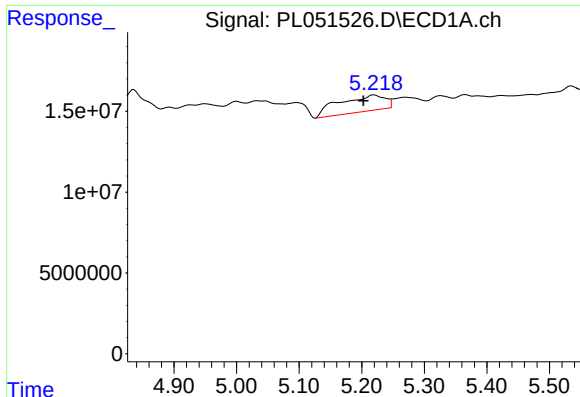

#25 Chlordane-3


R.T.: 5.220 min
Delta R.T.: 0.017 min
Response: 51060907
Conc: 36.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

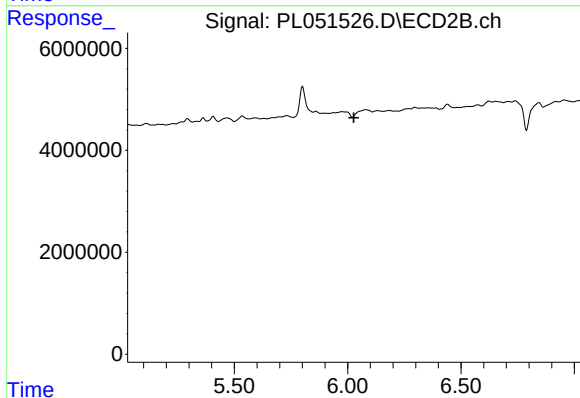


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 6.027 min
Response: 0
Conc: N.D.

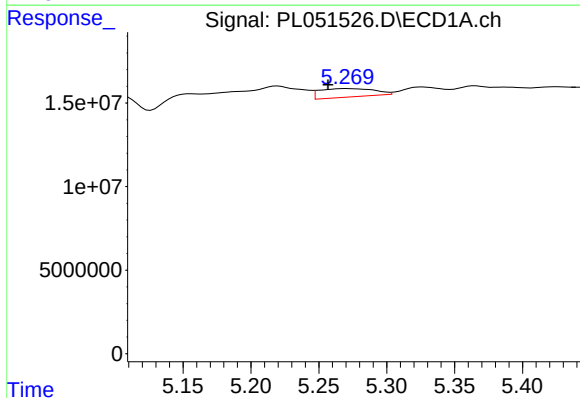


#26 Chlordane-4

R.T.: 5.271 min
Delta R.T.: 0.014 min
Response: 14212046
Conc: 10.78 ng/ml

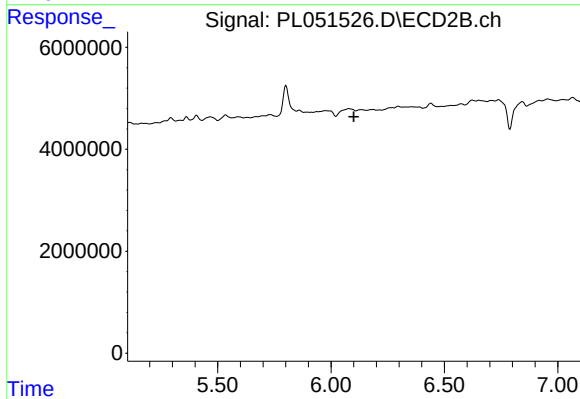

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 6.100 min
Response: 0
Conc: N.D.

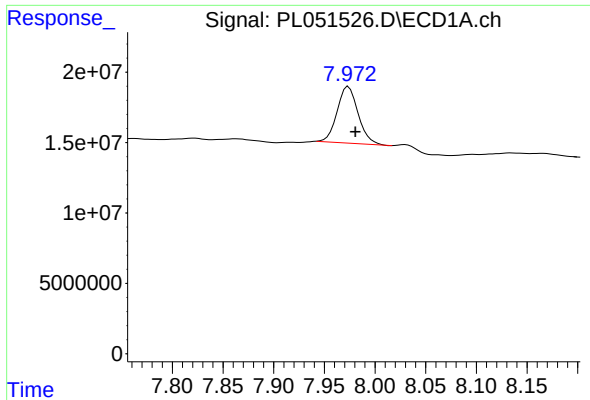

#28 Decachlorobiphenyl

R.T.: 7.974 min
Delta R.T.: -0.007 min
Response: 57966656
Conc: 5.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

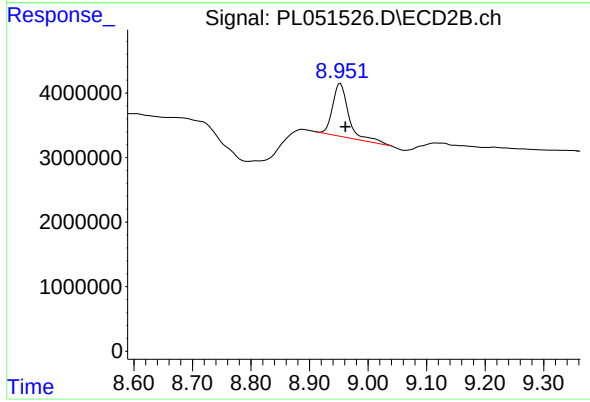

#28 Decachlorobiphenyl

R.T.: 8.953 min
Delta R.T.: -0.009 min
Response: 15504499
Conc: 5.48 ng/ml