

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081519\
 Data File : PL051540.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2019 20:14
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 00:57:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	3.926	243.8E6	62527992	24.263	21.915
28)	SA Decachlor...	7.974	8.952	256.1E6	65649136	25.294	23.215
Target Compounds							
6)	B beta-BHC	0.000	4.802f	0	4734179	N.D.	2.738 #
8)	B Heptachlo...	4.984	0.000	4205271	0	0.285	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081519\
Data File : PL051540.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2019 20:14
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 00:57:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

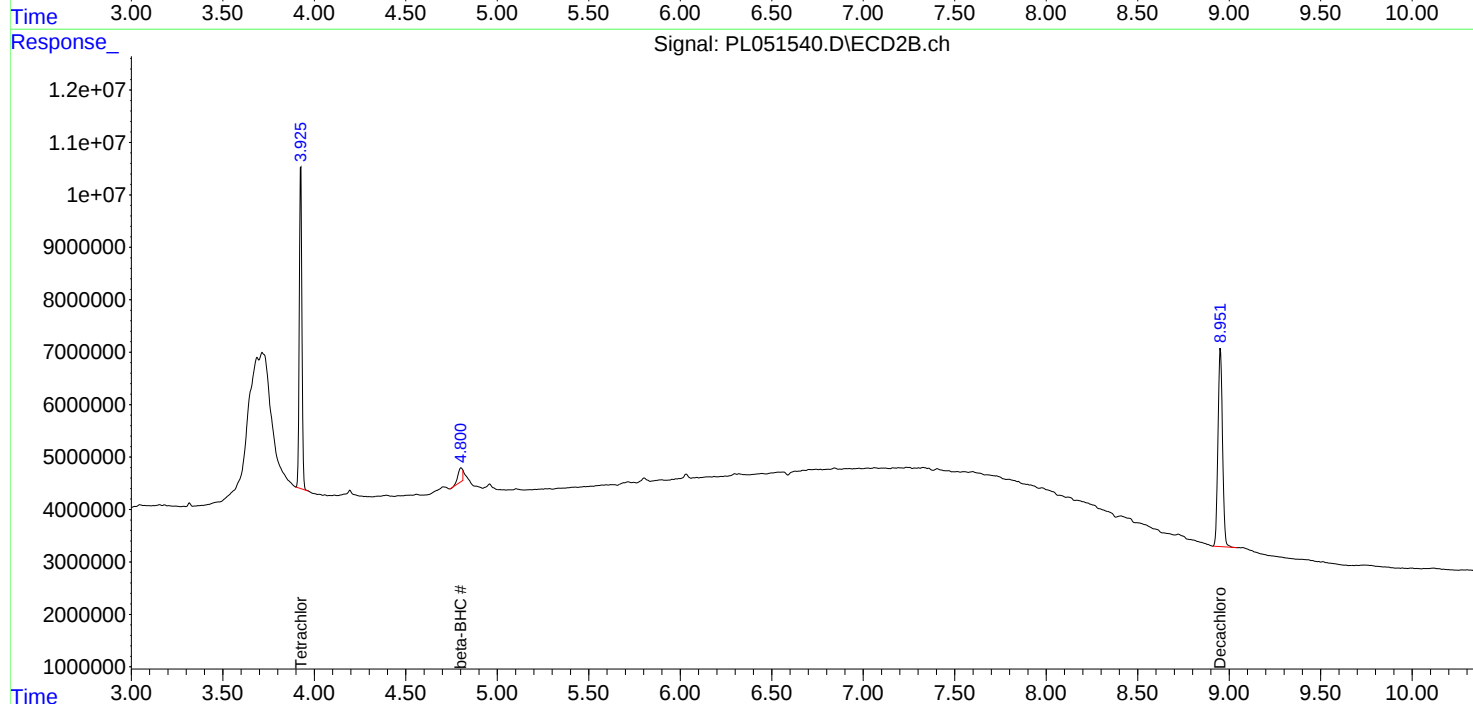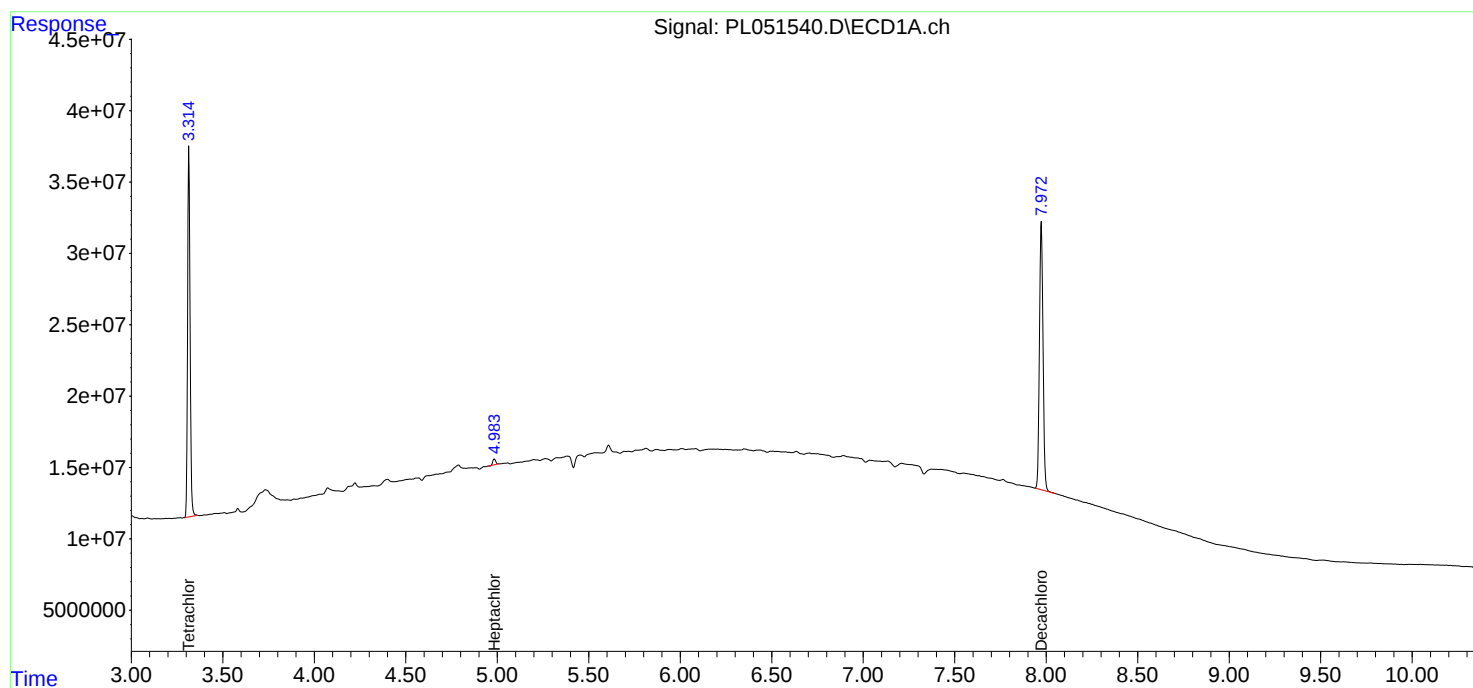


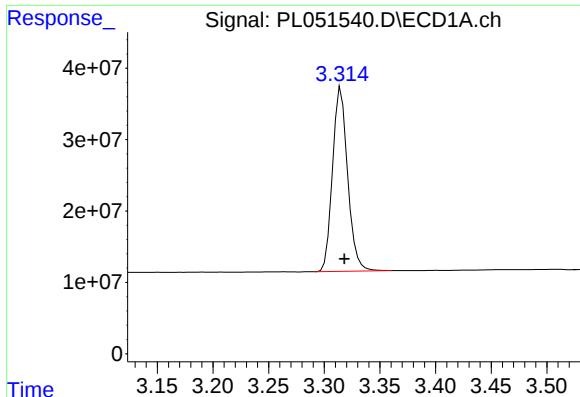

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: -0.003 min
Response: 243787973
Conc: 24.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

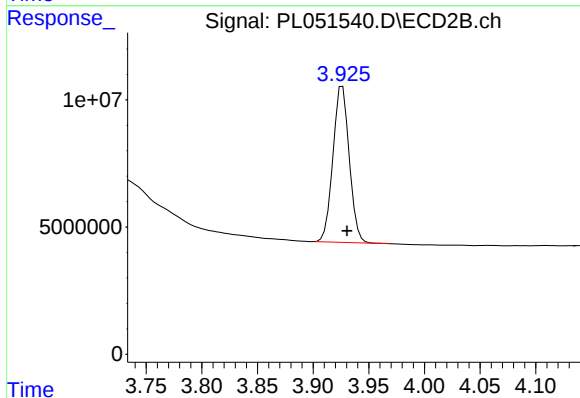


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.004 min
Response: 62527992
Conc: 21.91 ng/ml

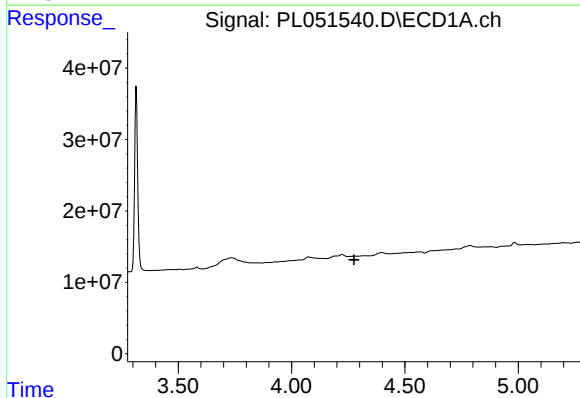


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

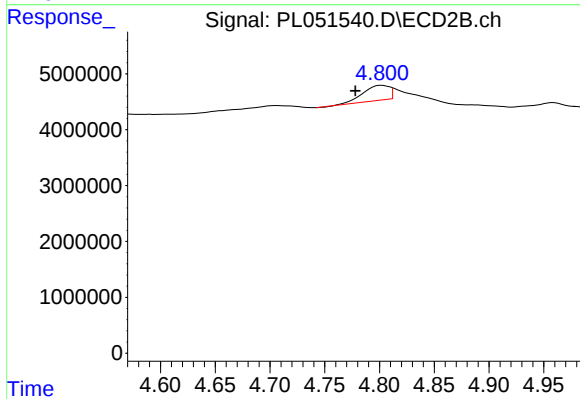

#6 beta-BHC


R.T.: 4.802 min
Delta R.T.: 0.024 min
Response: 4734179
Conc: 2.74 ng/ml

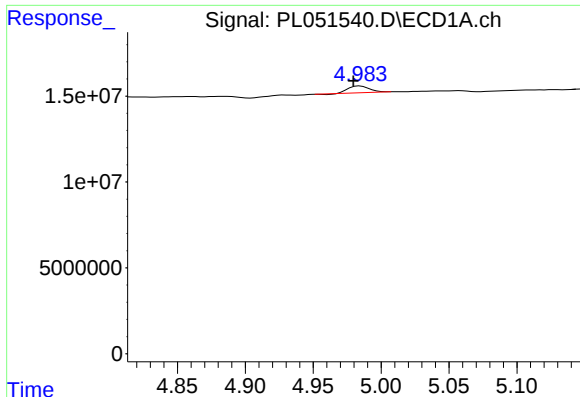

#8 Heptachlor epoxide


R.T.: 4.984 min
Delta R.T.: 0.005 min
Response: 4205271
Conc: 0.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

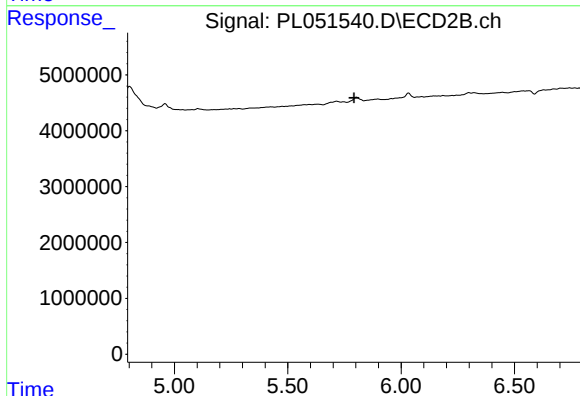


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.793 min
Response: 0
Conc: N.D.

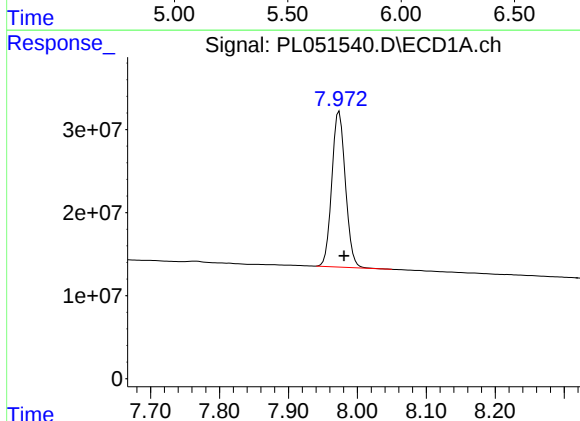

#28 Decachlorobiphenyl

R.T.: 7.974 min
Delta R.T.: -0.007 min
Response: 256115731
Conc: 25.29 ng/ml

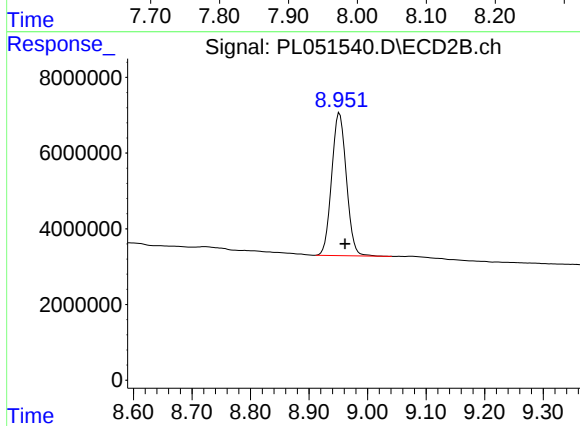

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: -0.010 min
Response: 65649136
Conc: 23.21 ng/ml