

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081519\
 Data File : PL051555.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2019 23:47
 Operator : SG\AJ
 Sample : K4272-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 2S-K-(0-1)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 01:02:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	3.926	240.4E6	64316660	23.922	22.542
28)	SA Decachlor...	7.973	8.952	247.0E6	63049450	24.399	22.295
Target Compounds							
6)	B beta-BHC	0.000	4.801f	0	4443299	N.D.	2.570 #
11)	B alpha-Chl...	5.261	0.000	18266974	0	1.197	N.D. #
12)	B 4,4'-DDE	5.448f	0.000	840528	0	0.056	N.D. #
13)	MA Dieldrin	5.538	0.000	12568252	0	0.811	N.D. #
20)	A Methoxychlor	6.716	0.000	31593520	0	5.064	N.D. #
26)	Chlordane-4	5.261	0.000	18266974	0	13.849	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081519\
Data File : PL051555.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2019 23:47
Operator : SG\AJ
Sample : K4272-11
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
2S-K-(0-1)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 01:02:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

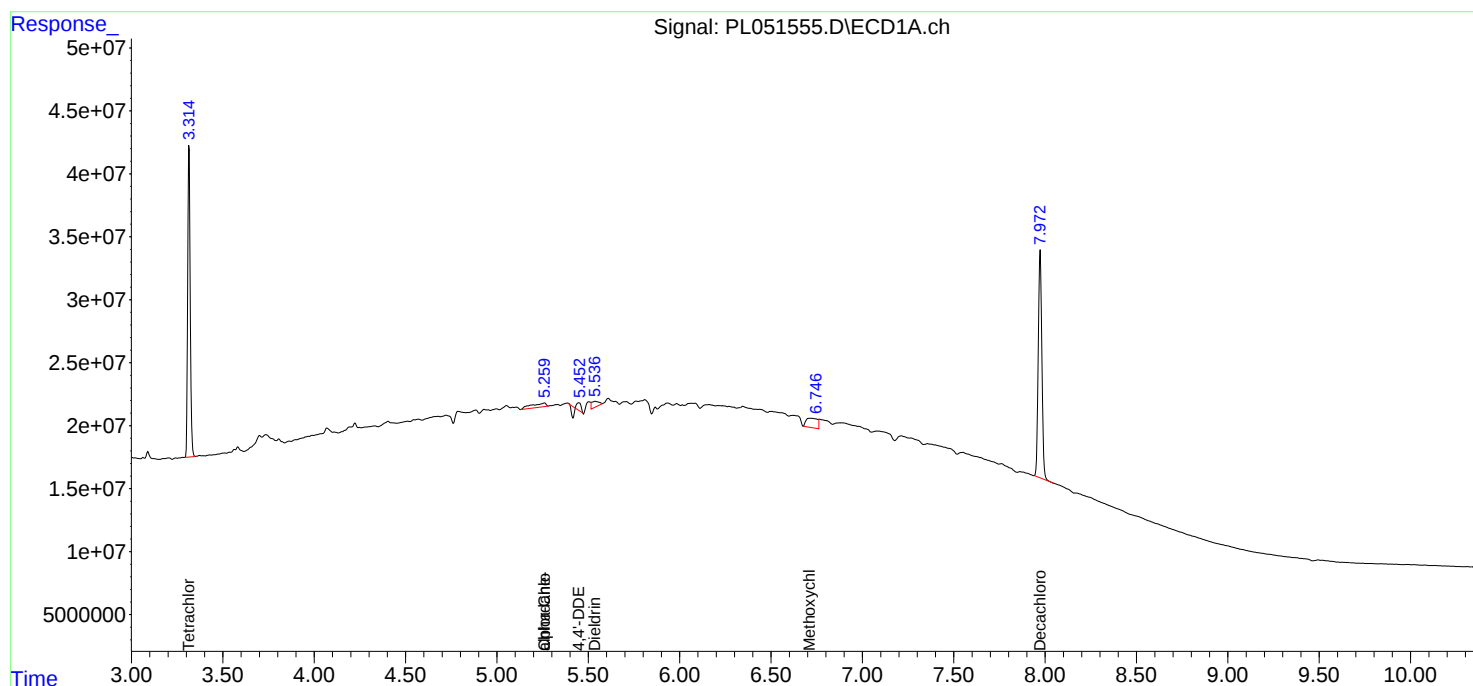


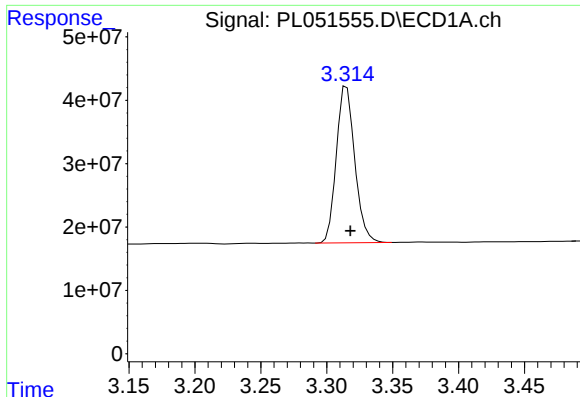

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: -0.003 min
Response: 240364897
Conc: 23.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
2S-K-(0-1)

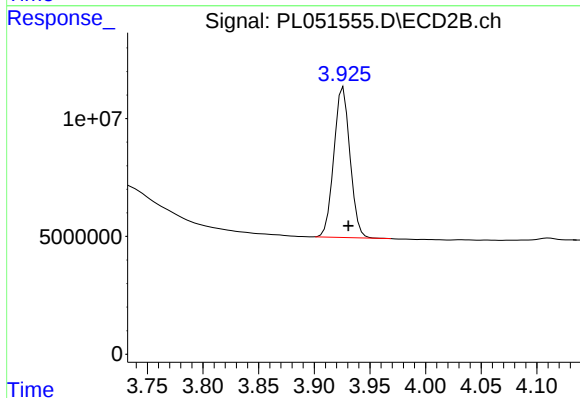


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.005 min
Response: 64316660
Conc: 22.54 ng/ml

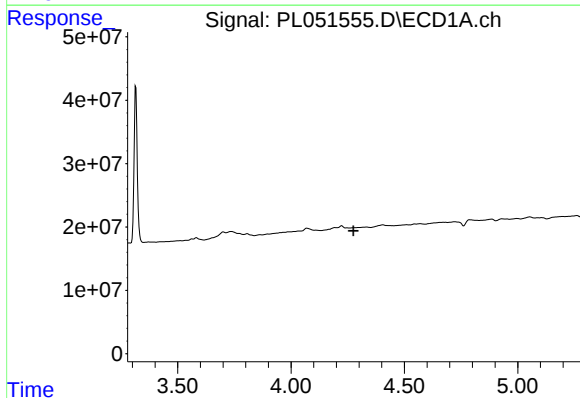


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

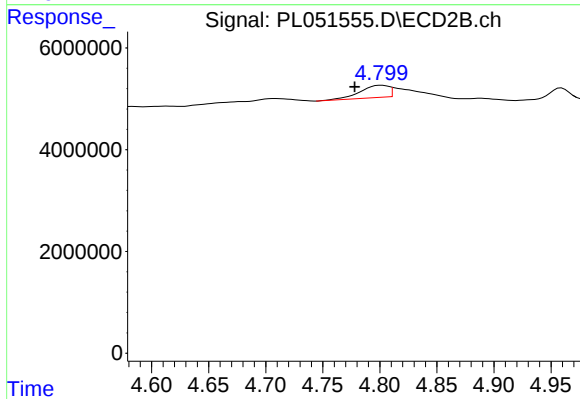

#6 beta-BHC


R.T.: 4.801 min
Delta R.T.: 0.023 min
Response: 4443299
Conc: 2.57 ng/ml

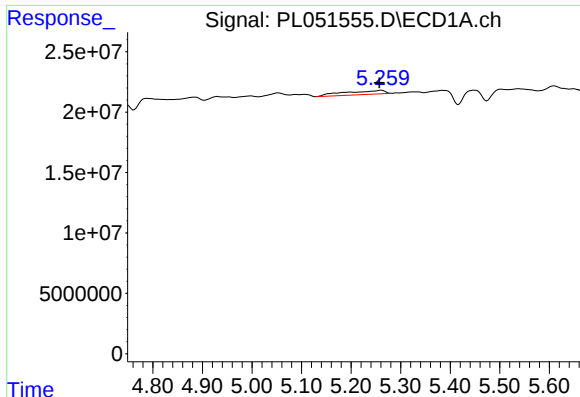

#11 alpha-Chlordane


R.T.: 5.261 min
Delta R.T.: 0.004 min
Response: 18266974
Conc: 1.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
2S-K-(0-1)

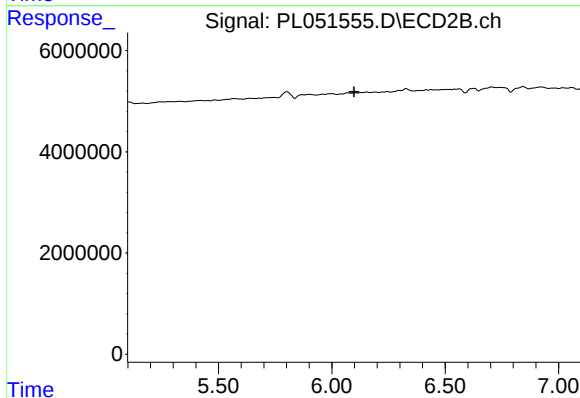


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

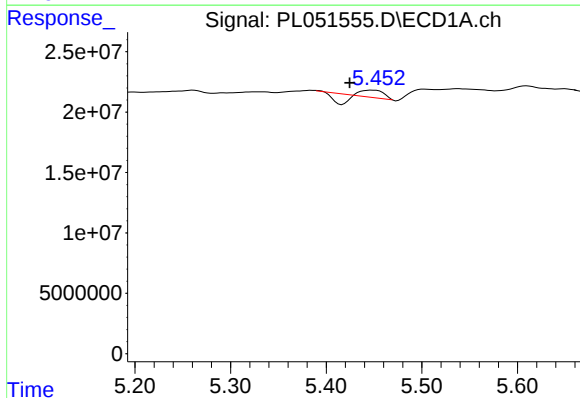


#12 4,4'-DDE

R.T.: 5.448 min
Delta R.T.: 0.024 min
Response: 840528
Conc: 0.06 ng/ml

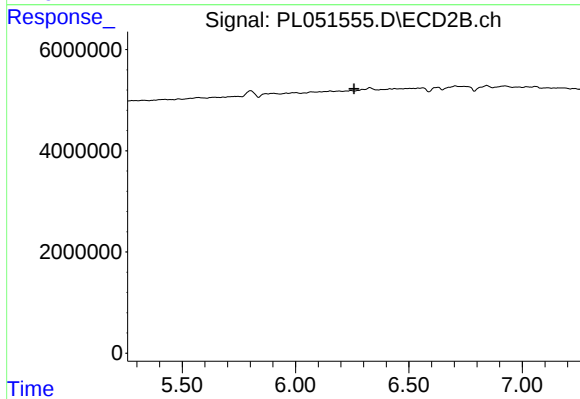

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.258 min
Response: 0
Conc: N.D.

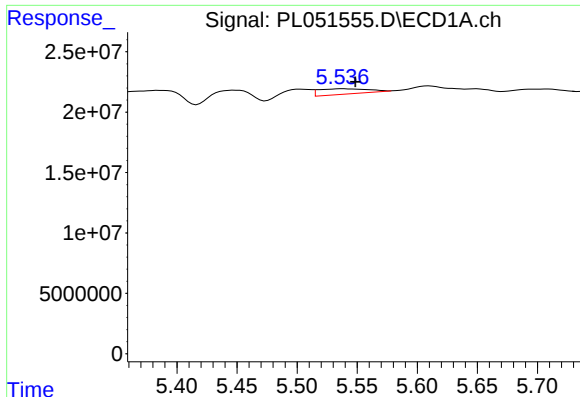

#13 Dieldrin


R.T.: 5.538 min
Delta R.T.: -0.011 min
Response: 12568252
Conc: 0.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
2S-K-(0-1)

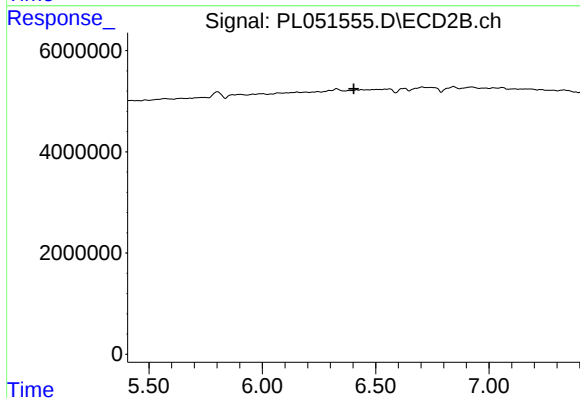


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.404 min
Response: 0
Conc: N.D.

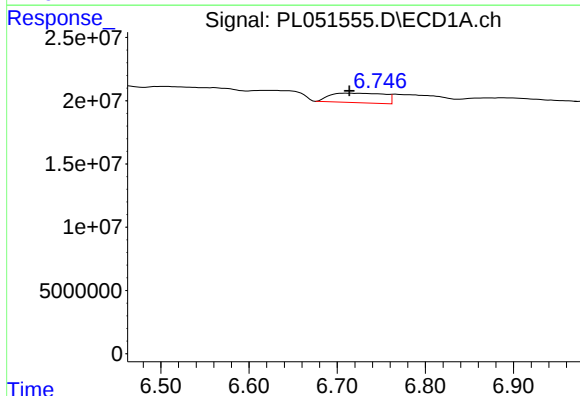


#20 Methoxychlor

R.T.: 6.716 min
Delta R.T.: 0.002 min
Response: 31593520
Conc: 5.06 ng/ml

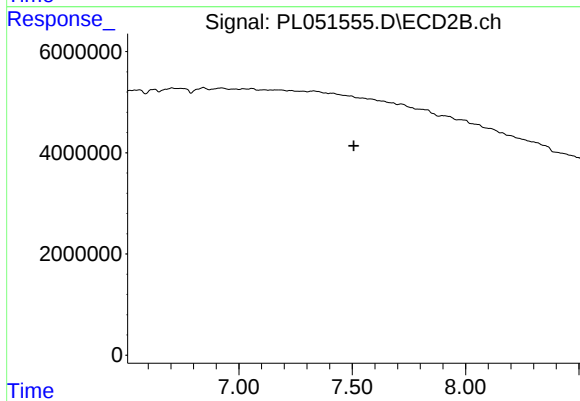

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.507 min
Response: 0
Conc: N.D.

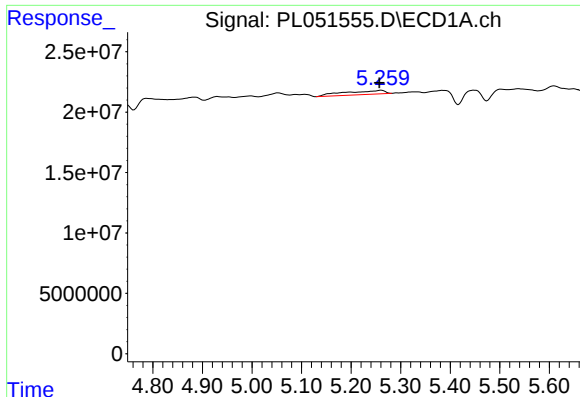

#26 Chlordane-4


R.T.: 5.261 min
Delta R.T.: 0.004 min
Response: 18266974
Conc: 13.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
2S-K-(0-1)

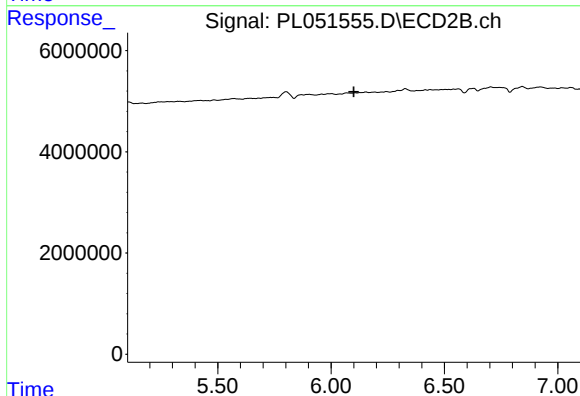


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.100 min
Response: 0
Conc: N.D.

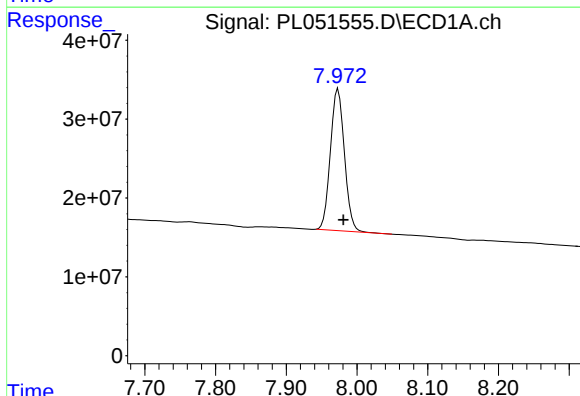

#28 Decachlorobiphenyl

R.T.: 7.973 min
Delta R.T.: -0.007 min
Response: 247046321
Conc: 24.40 ng/ml

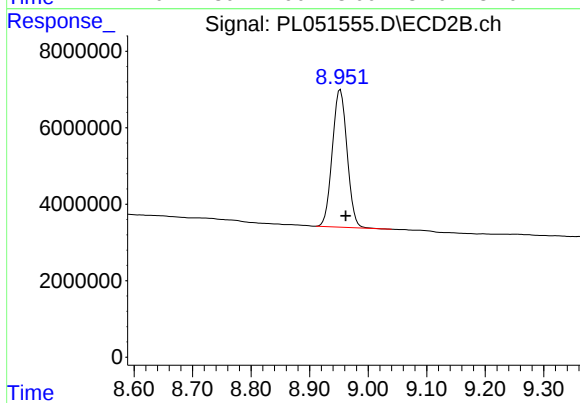

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: -0.009 min
Response: 63049450
Conc: 22.30 ng/ml