

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081519\
 Data File : PL051556.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2019 00:01
 Operator : SG\AJ
 Sample : K4356-02
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 01:02:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	3.926	229.6E6	62124947	22.853	21.774
28)	SA Decachlor...	7.974	8.953	265.7E6	67692066	26.238	23.937
Target Compounds							
6)	B beta-BHC	0.000	4.803f	0	4209704	N.D.	2.435 #
10)	B gamma-Chl...	5.178f	0.000	15137987	0	0.959	N.D. #
11)	B alpha-Chl...	5.261	0.000	23057473	0	1.511	N.D. #
20)	A Methoxychlor	6.729	0.000	41785955	0	6.698	N.D. #
25)	Chlordane-3	5.178f	0.000	15137987	0	10.814	N.D. #
26)	Chlordane-4	5.261	0.000	23057473	0	17.481	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081519\
Data File : PL051556.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2019 00:01
Operator : SG\AJ
Sample : K4356-02
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 01:02:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

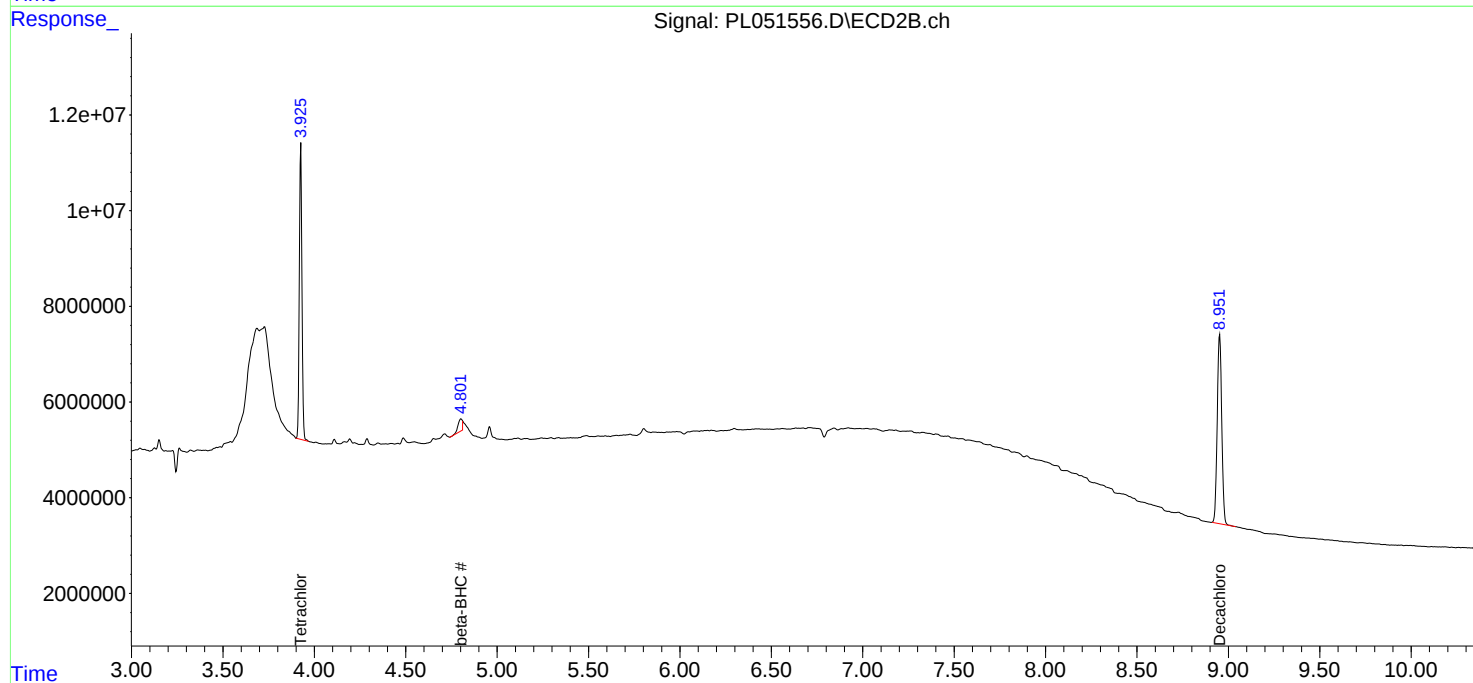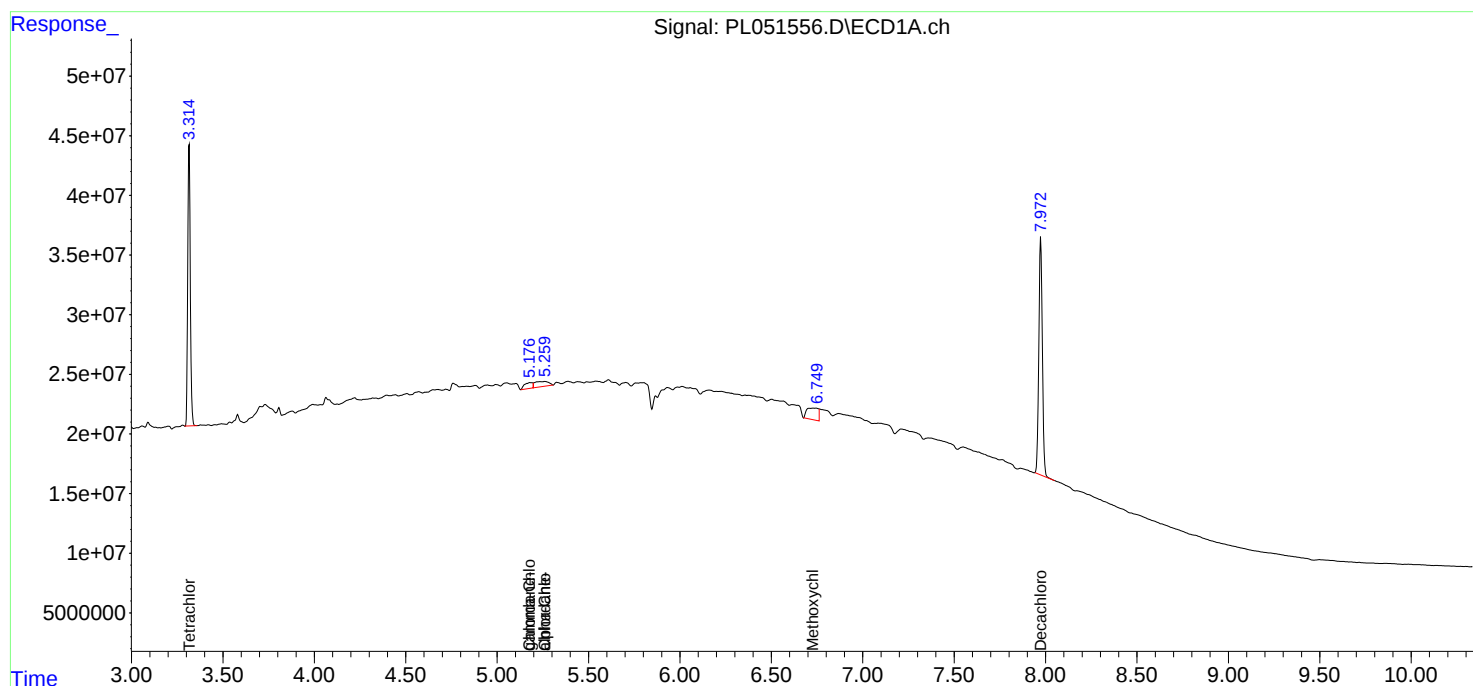


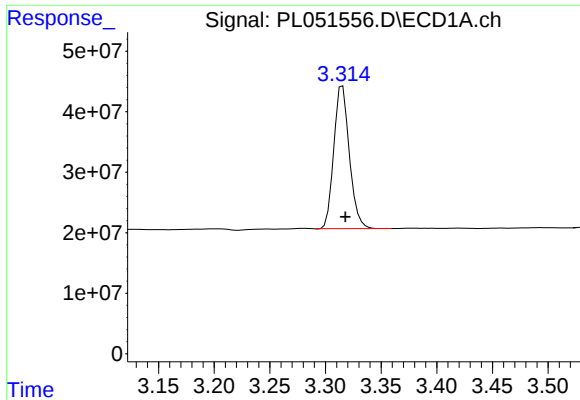

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: -0.003 min
Response: 229623066
Conc: 22.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

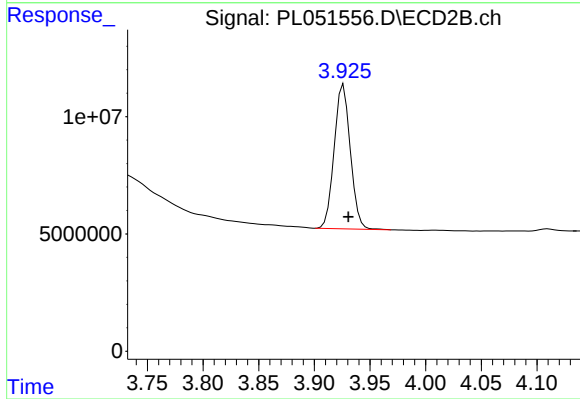


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.004 min
Response: 62124947
Conc: 21.77 ng/ml

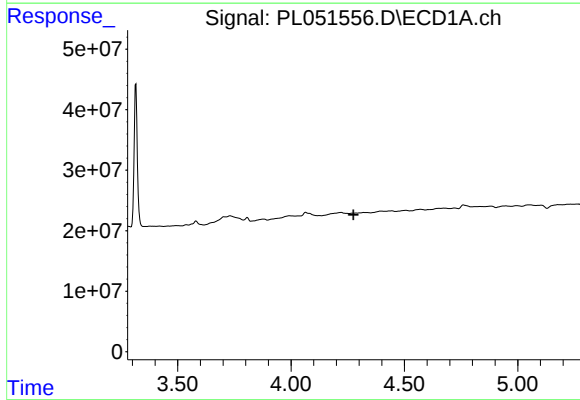


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

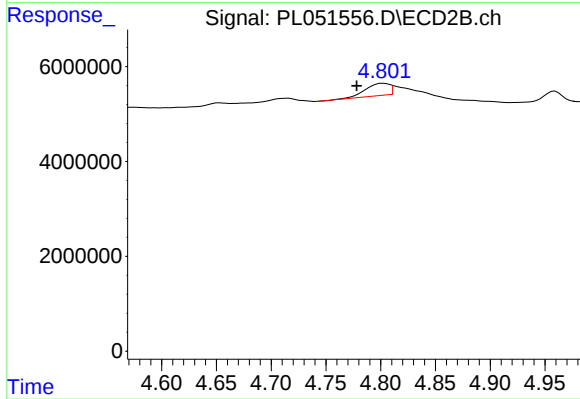

#6 beta-BHC


R.T.: 4.803 min
Delta R.T.: 0.024 min
Response: 4209704
Conc: 2.43 ng/ml

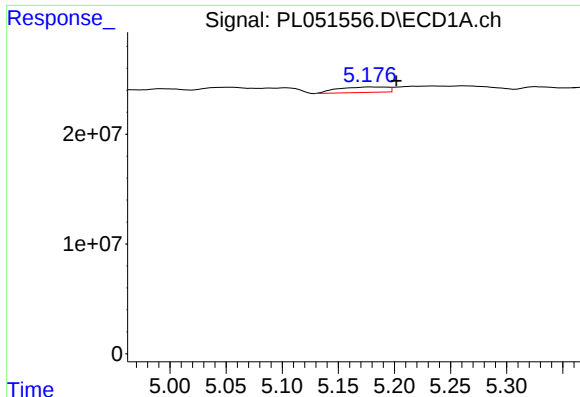

#10 gamma-Chlordane


R.T.: 5.178 min
Delta R.T.: -0.023 min
Response: 15137987
Conc: 0.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

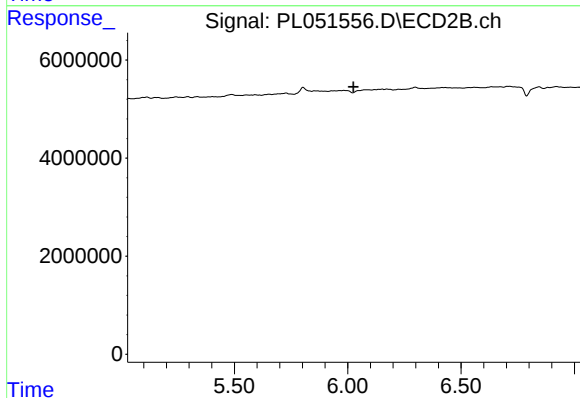


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

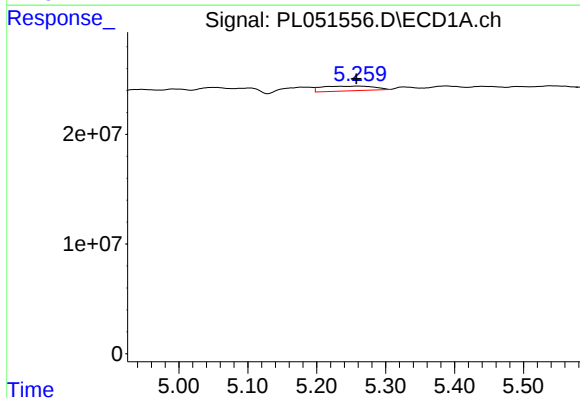


#11 alpha-Chlordane

R.T.: 5.261 min
Delta R.T.: 0.004 min
Response: 23057473
Conc: 1.51 ng/ml

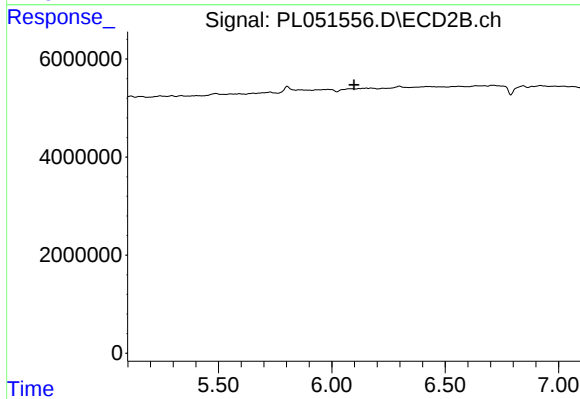

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

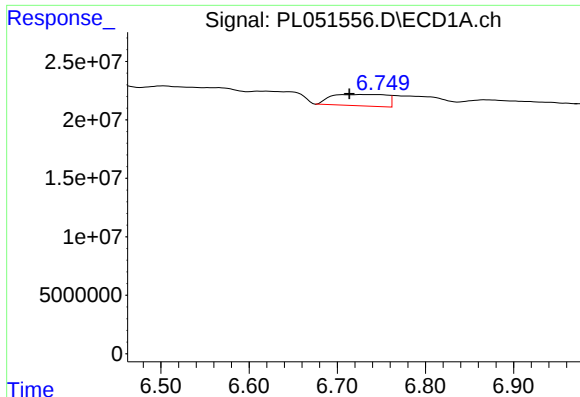

#20 Methoxychlor


R.T.: 6.729 min
Delta R.T.: 0.015 min
Response: 41785955
Conc: 6.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

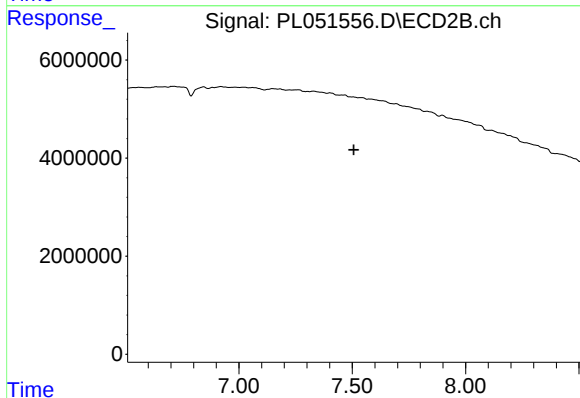


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.507 min
Response: 0
Conc: N.D.

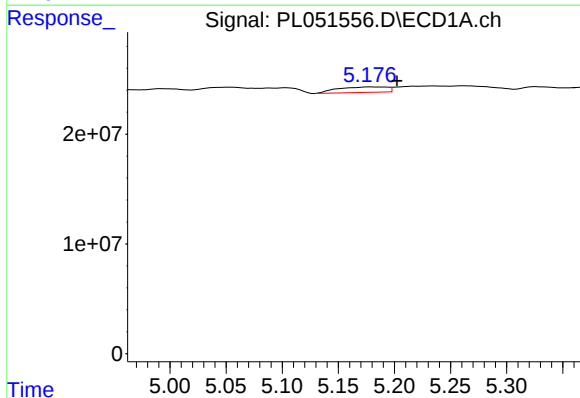


#25 Chlordane-3

R.T.: 5.178 min
Delta R.T.: -0.024 min
Response: 15137987
Conc: 10.81 ng/ml

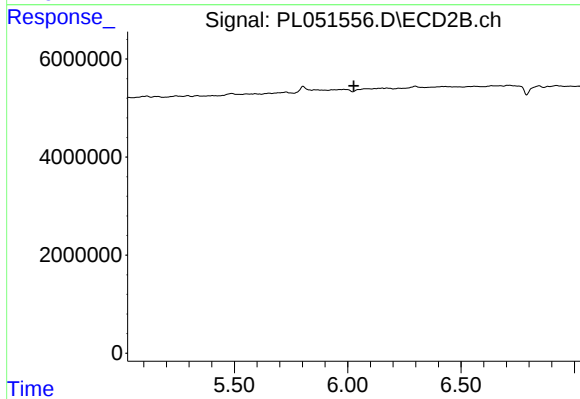

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.027 min
Response: 0
Conc: N.D.

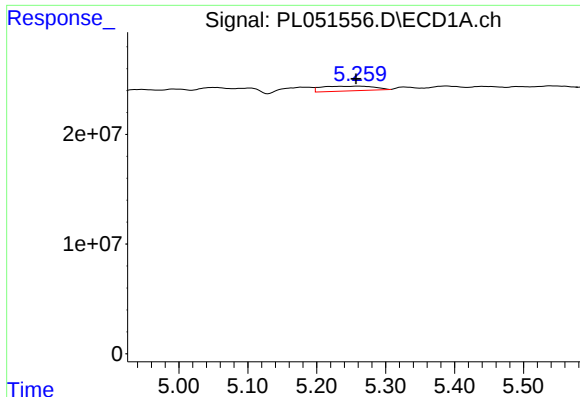

#26 Chlordane-4


R.T.: 5.261 min
Delta R.T.: 0.004 min
Response: 23057473
Conc: 17.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

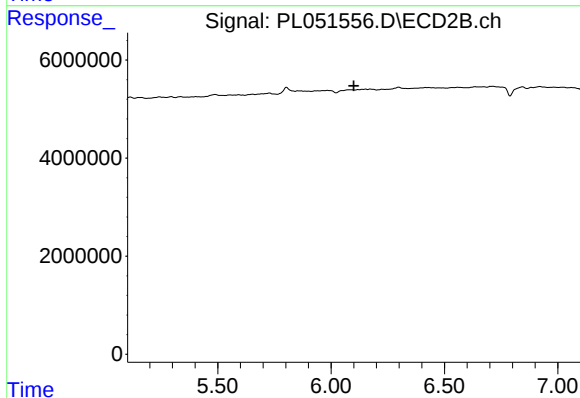


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.100 min
Response: 0
Conc: N.D.

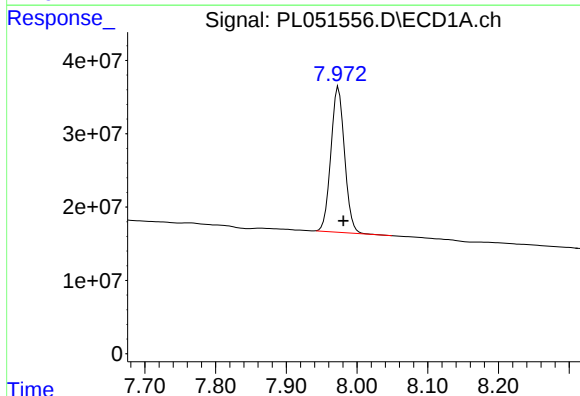

#28 Decachlorobiphenyl

R.T.: 7.974 min
Delta R.T.: -0.007 min
Response: 265666559
Conc: 26.24 ng/ml

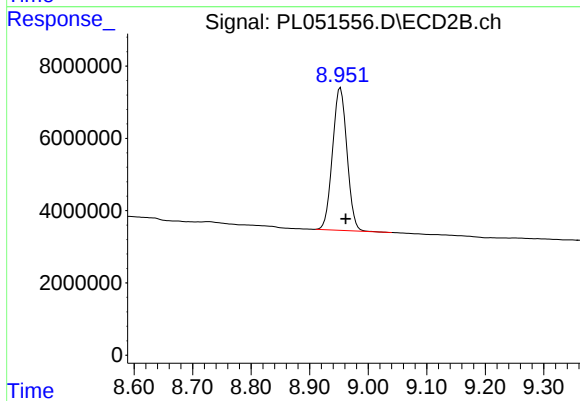

#28 Decachlorobiphenyl

R.T.: 8.953 min
Delta R.T.: -0.009 min
Response: 67692066
Conc: 23.94 ng/ml