

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081519\
 Data File : PL051558.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2019 00:29
 Operator : SG\AJ
 Sample : K4356-06
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 01:02:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	3.926	228.4E6	62722059	22.734	21.983
28)	SA Decachlor...	7.974	8.952	241.7E6	65402640	23.869	23.128
Target Compounds							
5)	MB Aldrin	4.570f	0.000	6006944	0	0.388	N.D. #
6)	B beta-BHC	0.000	4.804f	0	4102185	N.D.	2.373 #
10)	B gamma-Chl...	5.182f	0.000	22977010	0	1.456	N.D. #
11)	B alpha-Chl...	5.261	0.000	6301552	0	0.413	N.D. #
16)	A 4,4'-DDD	5.937	0.000	5509831	0	0.460	N.D. #
20)	A Methoxychlor	6.705	0.000	6342286	0	1.017	N.D. #
25)	Chlordane-3	5.182f	0.000	22977010	0	16.415	N.D. #
26)	Chlordane-4	5.261	0.000	6301552	0	4.778	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081519\
Data File : PL051558.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2019 00:29
Operator : SG\AJ
Sample : K4356-06
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 01:02:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

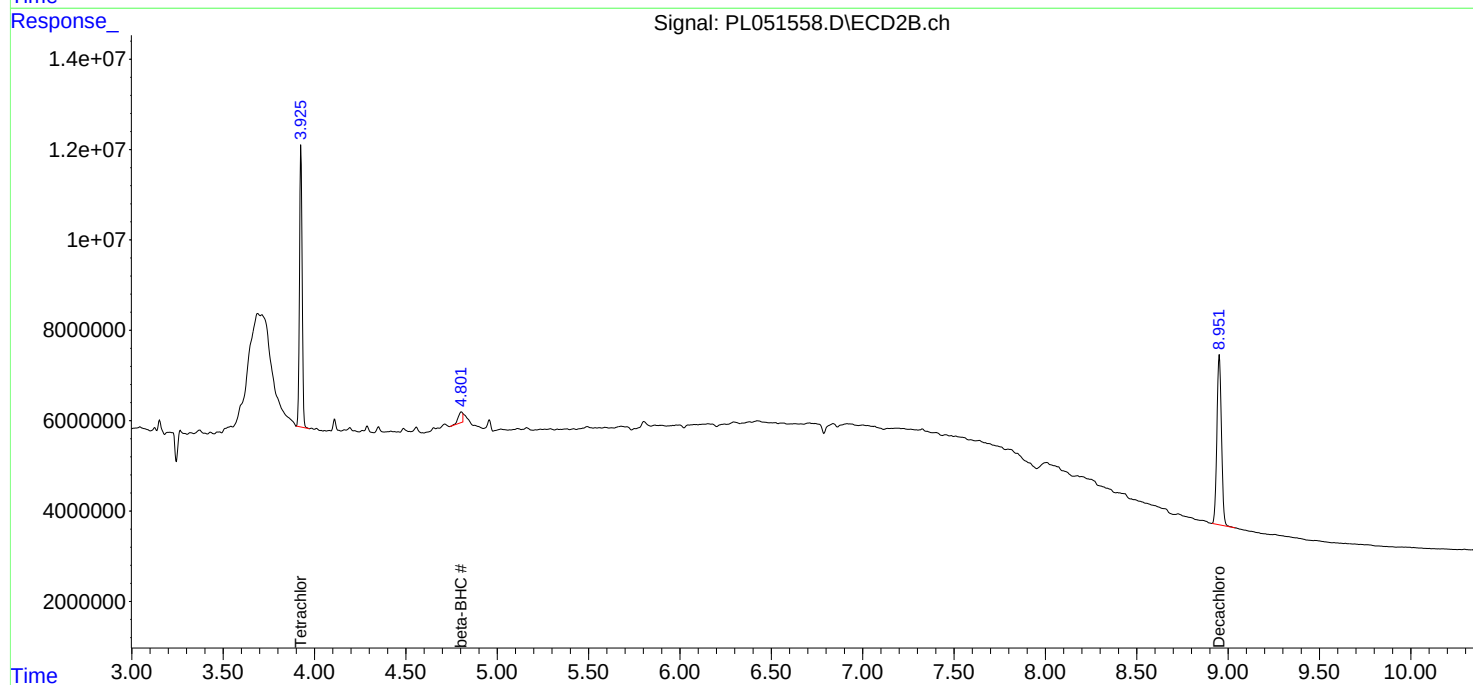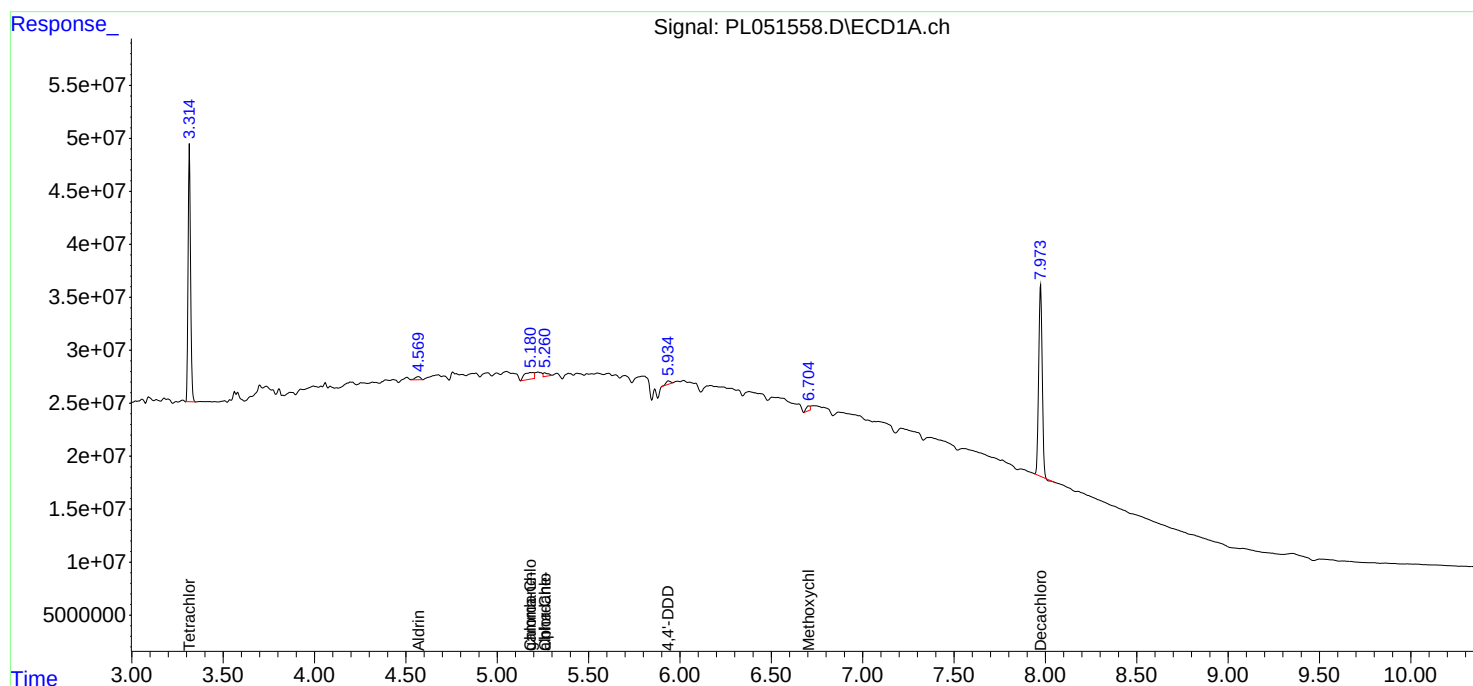


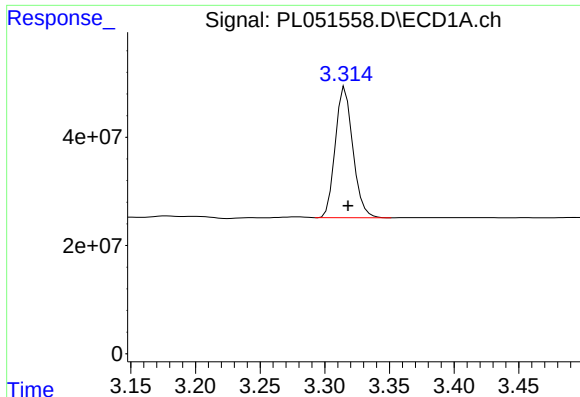

#1 Tetrachloro-m-xylene


R.T.: 3.316 min
Delta R.T.: -0.002 min
Response: 228422738
Conc: 22.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

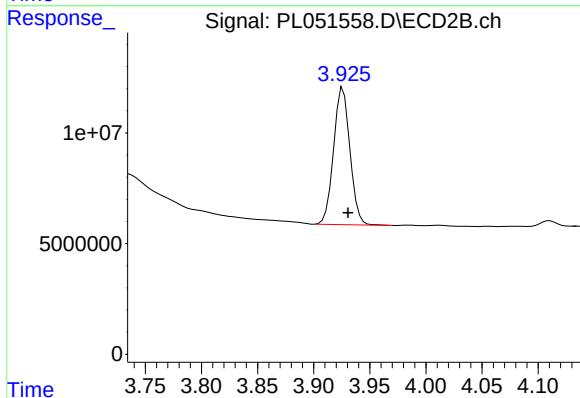


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.004 min
Response: 62722059
Conc: 21.98 ng/ml

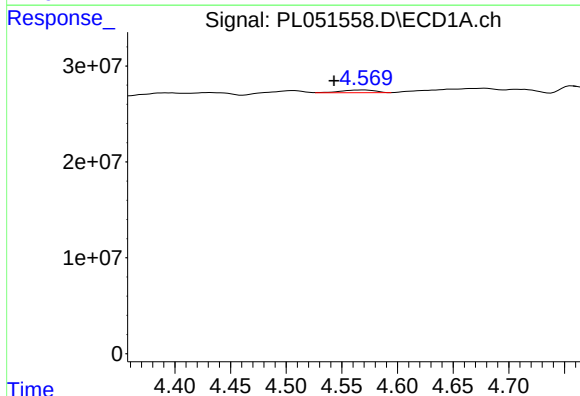


#5 Aldrin

R.T.: 4.570 min
Delta R.T.: 0.027 min
Response: 6006944
Conc: 0.39 ng/ml

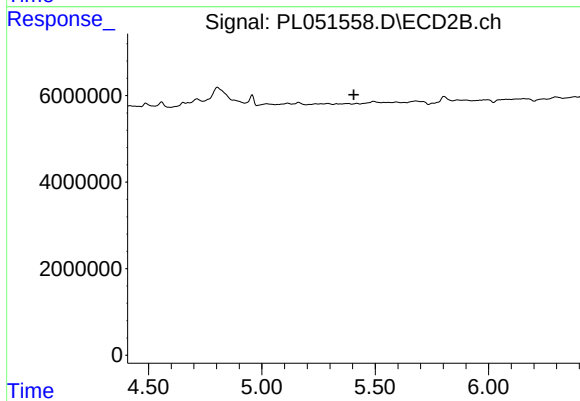

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.405 min
Response: 0
Conc: N.D.

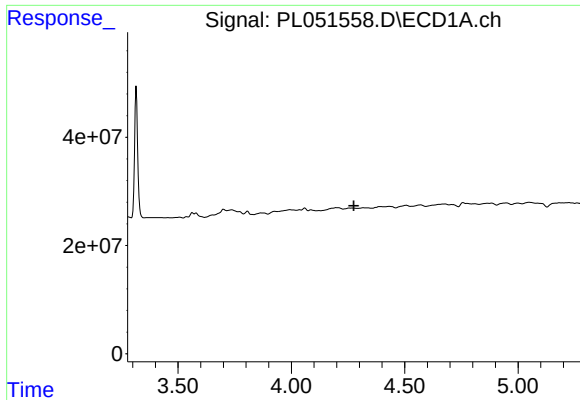

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-3

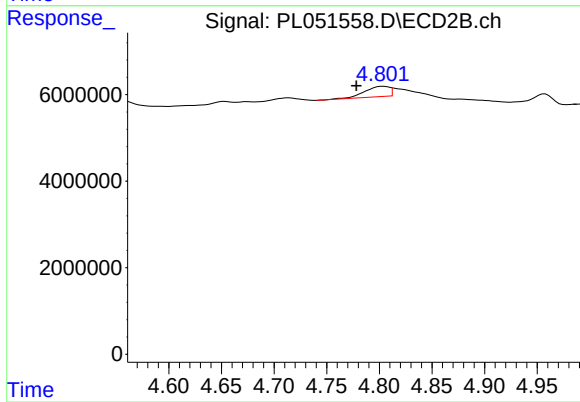


#6 beta-BHC

R.T.: 4.804 min
Delta R.T.: 0.026 min
Response: 4102185
Conc: 2.37 ng/ml

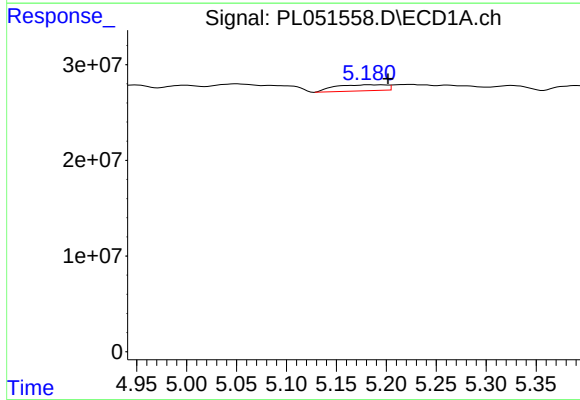


#10 gamma-Chlordane

R.T.: 5.182 min
Delta R.T.: -0.020 min
Response: 22977010
Conc: 1.46 ng/ml

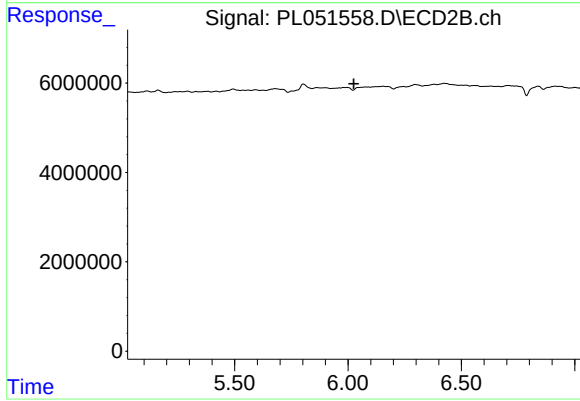

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.026 min
Response: 0
Conc: N.D.

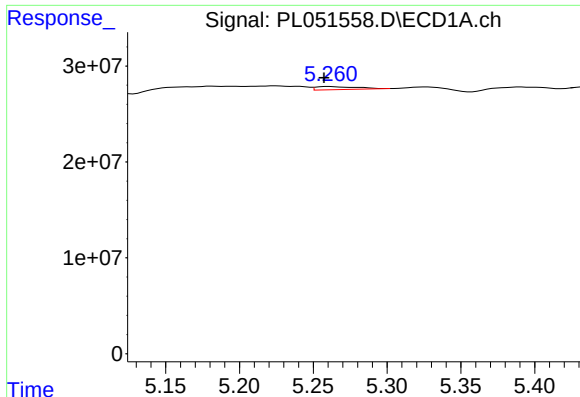

#11 alpha-Chlordane


R.T.: 5.261 min
Delta R.T.: 0.004 min
Response: 6301552
Conc: 0.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

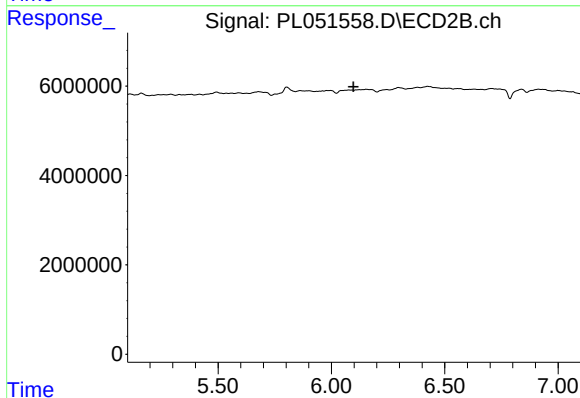


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

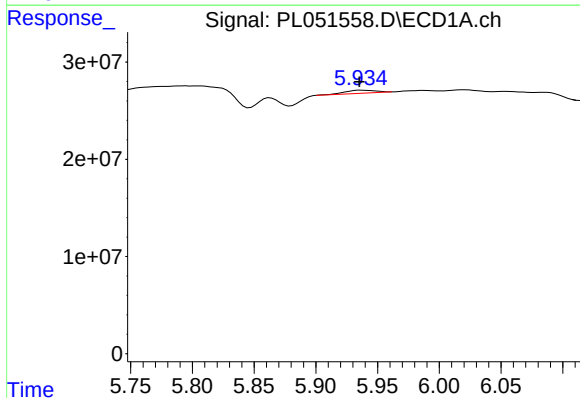


#16 4,4'-DDD

R.T.: 5.937 min
Delta R.T.: 0.001 min
Response: 5509831
Conc: 0.46 ng/ml

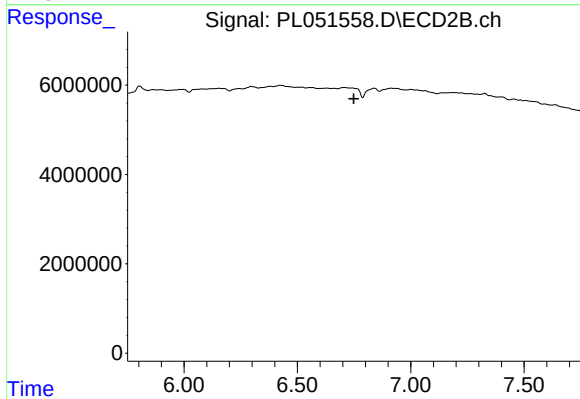

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.749 min
Response: 0
Conc: N.D.

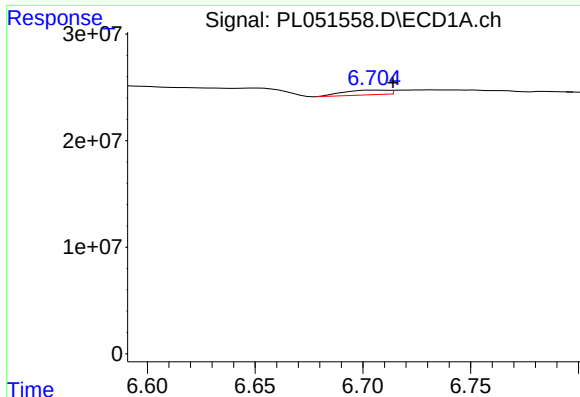

#20 Methoxychlor


R.T.: 6.705 min
Delta R.T.: -0.009 min
Response: 6342286
Conc: 1.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

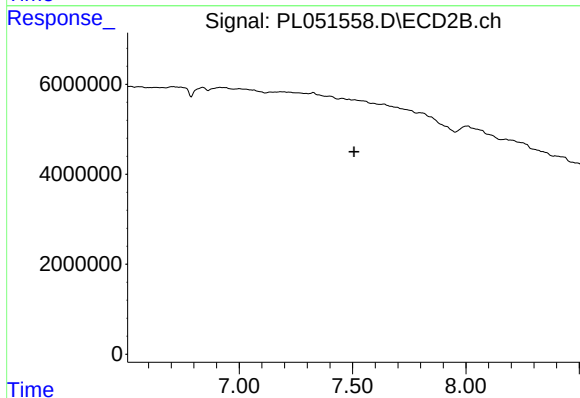


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.507 min
Response: 0
Conc: N.D.

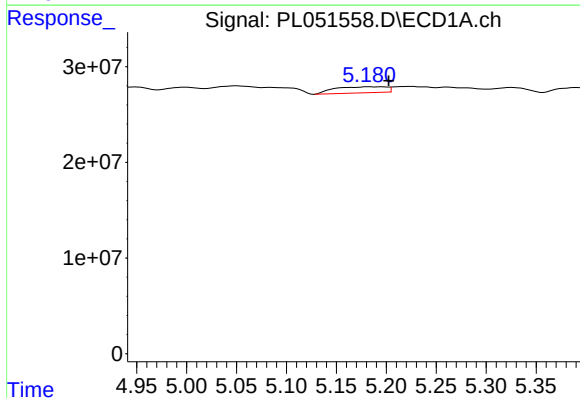


#25 Chlordane-3

R.T.: 5.182 min
Delta R.T.: -0.021 min
Response: 22977010
Conc: 16.41 ng/ml

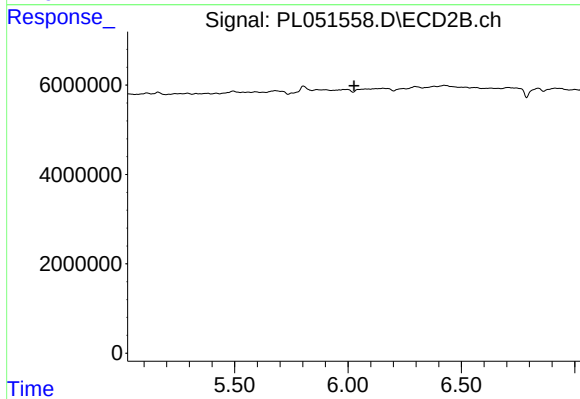

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

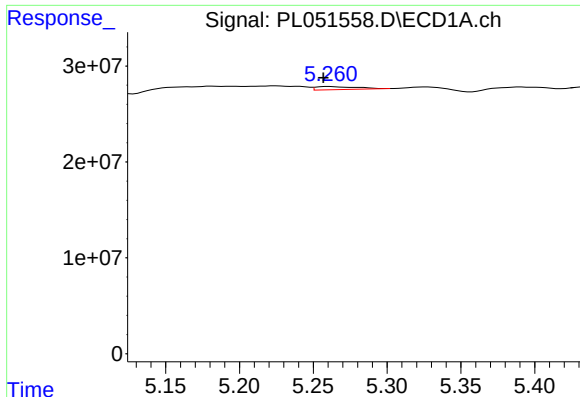

#26 Chlordane-4


R.T.: 5.261 min
Delta R.T.: 0.004 min
Response: 6301552
Conc: 4.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

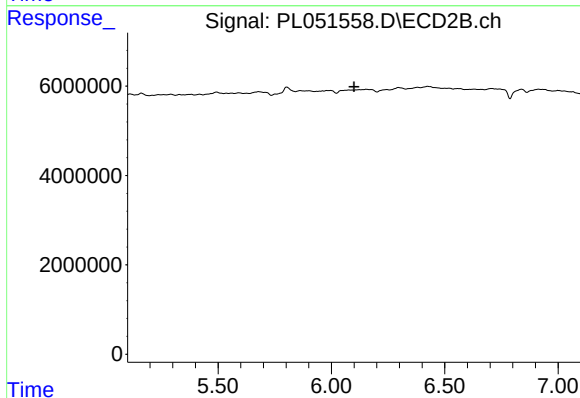


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.100 min
Response: 0
Conc: N.D.

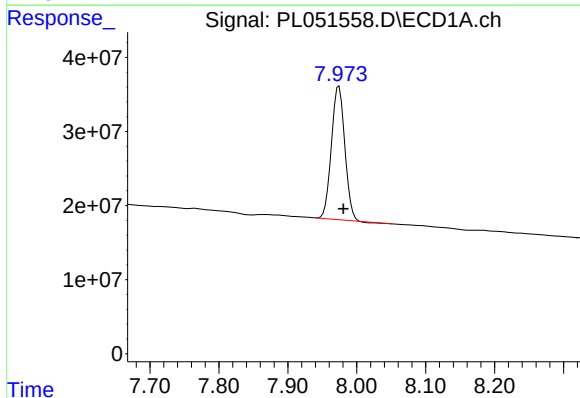

#28 Decachlorobiphenyl

R.T.: 7.974 min
Delta R.T.: -0.006 min
Response: 241686179
Conc: 23.87 ng/ml

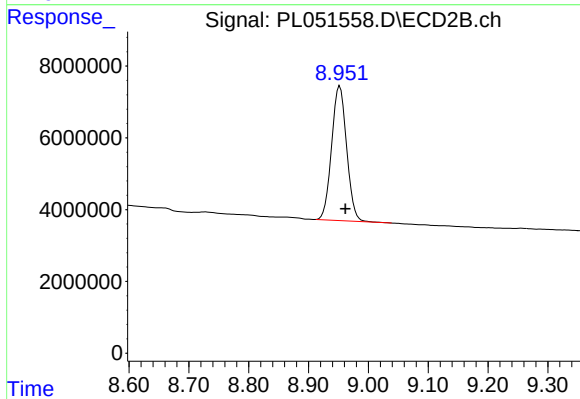

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: -0.009 min
Response: 65402640
Conc: 23.13 ng/ml