

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081519\
 Data File : PL051559.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2019 00:43
 Operator : SG\AJ
 Sample : K4356-08
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 03:07:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	3.926	233.1E6	62600652	23.202	21.940
28)	SA Decachlor...	7.973	8.953	261.1E6	66952819	25.789	23.676
Target Compounds							
4)	MA Heptachlor	4.334f	0.000	2702767	0	0.165	N.D. #
6)	B beta-BHC	0.000	4.803f	0	4781625	N.D.	2.766 #
9)	A Endosulfan I	5.324	0.000	15573513	0	1.071	N.D. #
10)	B gamma-Chl...	5.189	0.000	55649235	0	3.526	N.D. #
13)	MA Dieldrin	5.548	0.000	15752752	0	1.017	N.D. #
16)	A 4,4'-DDD	5.931	0.000	10109542	0	0.844	N.D. #
20)	A Methoxychlor	6.733f	0.000	49592729	0	7.949	N.D. #
25)	Chlordane-3	5.189	0.000	55649235	0	39.755	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081519\
Data File : PL051559.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2019 00:43
Operator : SG\AJ
Sample : K4356-08
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 03:07:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

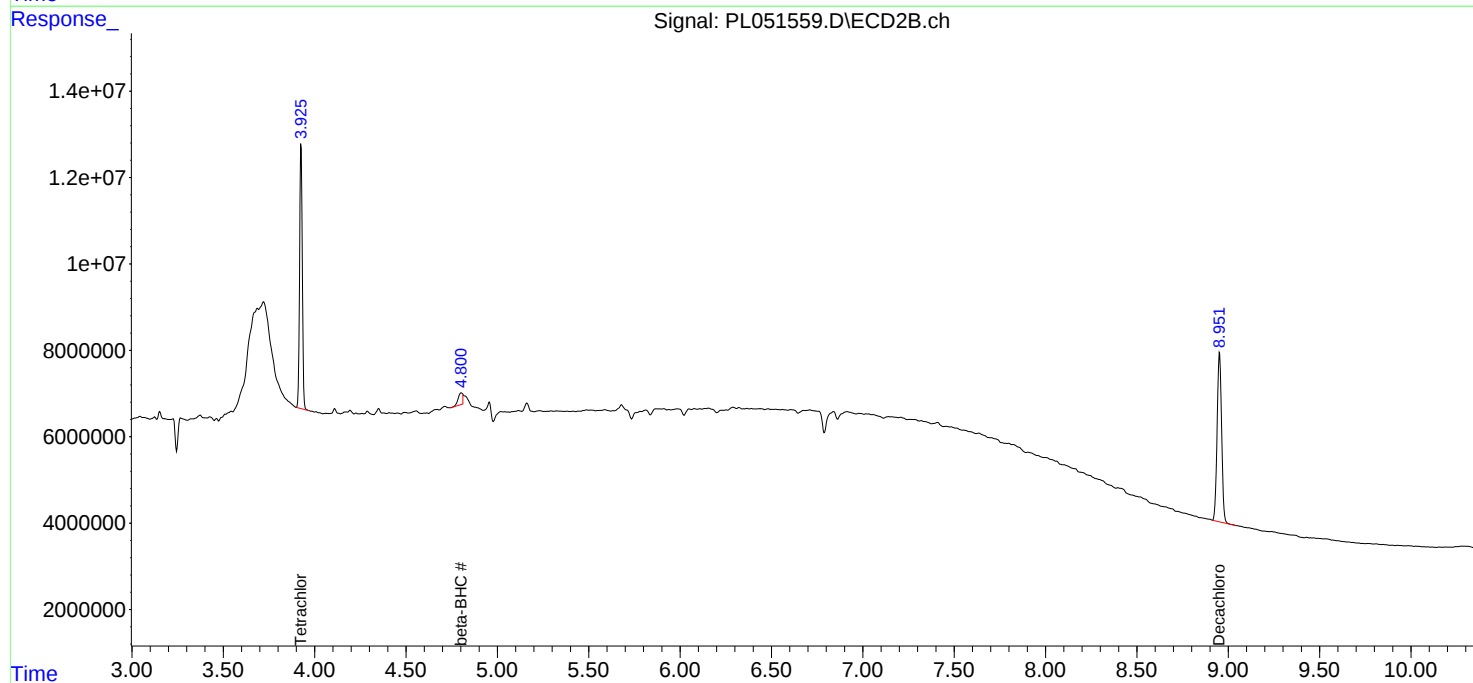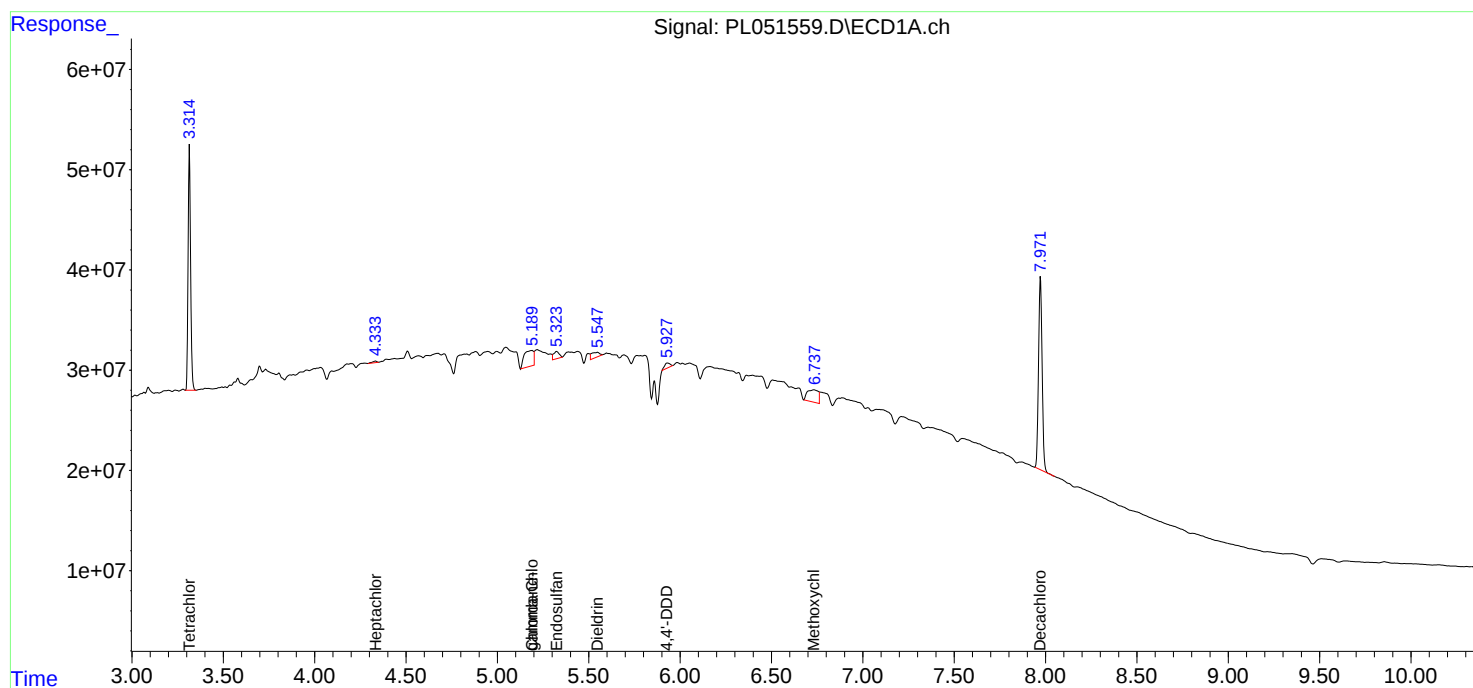


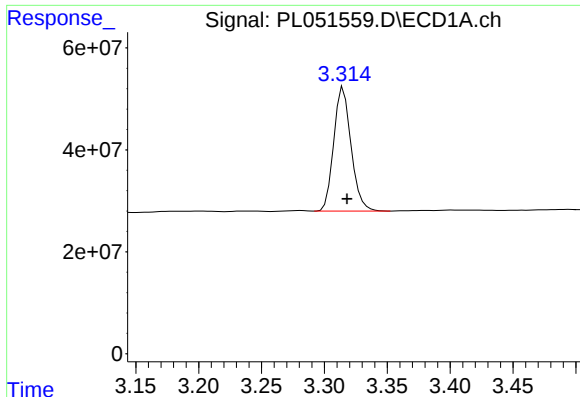

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: -0.003 min
Response: 233134424
Conc: 23.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4

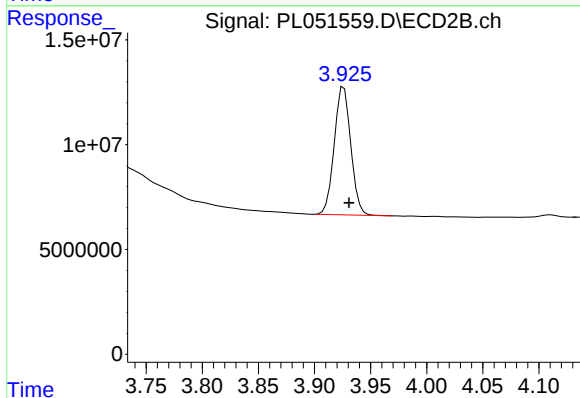


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.004 min
Response: 62600652
Conc: 21.94 ng/ml

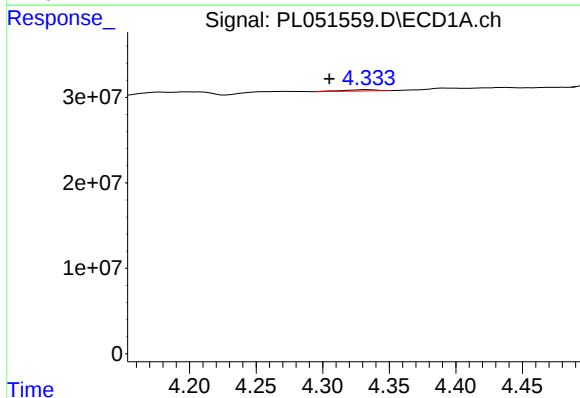


#4 Heptachlor

R.T.: 4.334 min
Delta R.T.: 0.029 min
Response: 2702767
Conc: 0.16 ng/ml

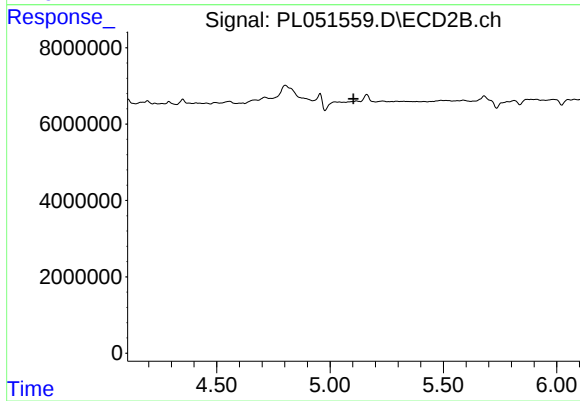

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.104 min
Response: 0
Conc: N.D.

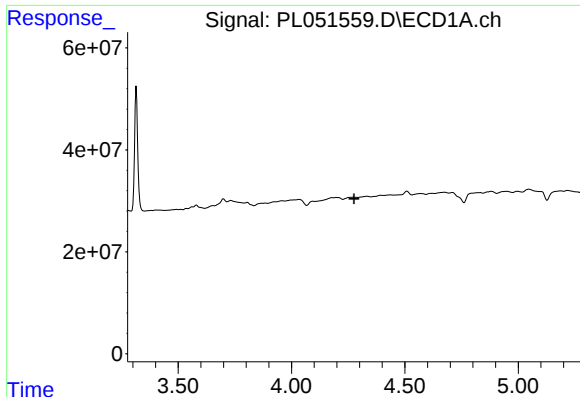

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-4

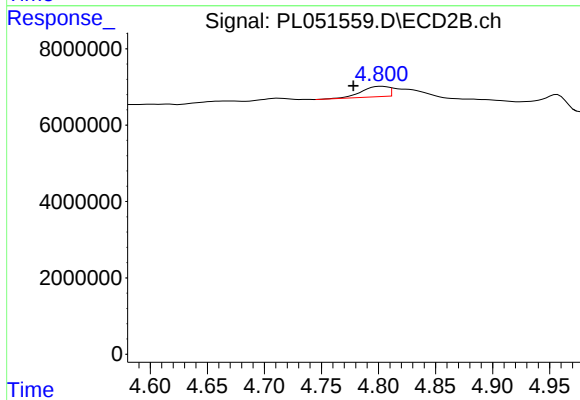


#6 beta-BHC

R.T.: 4.803 min
Delta R.T.: 0.025 min
Response: 4781625
Conc: 2.77 ng/ml

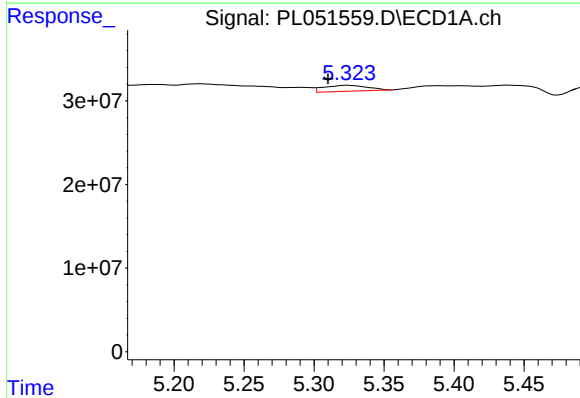


#9 Endosulfan I

R.T.: 5.324 min
Delta R.T.: 0.014 min
Response: 15573513
Conc: 1.07 ng/ml

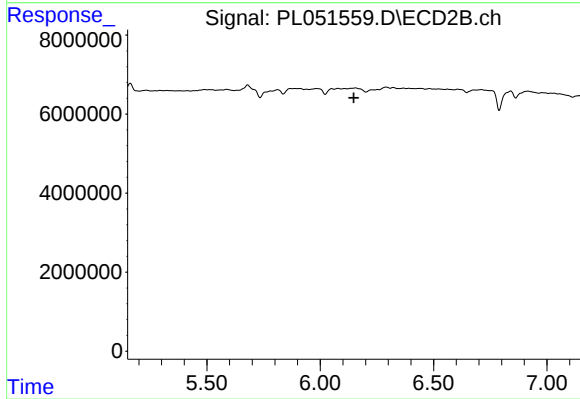

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.148 min
Response: 0
Conc: N.D.

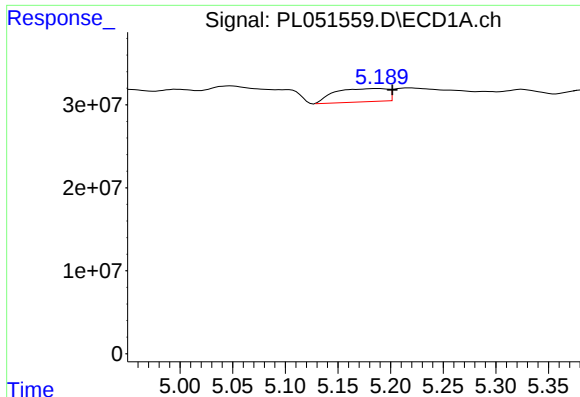

#10 gamma-Chlordane


R.T.: 5.189 min
Delta R.T.: -0.012 min
Response: 55649235
Conc: 3.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4

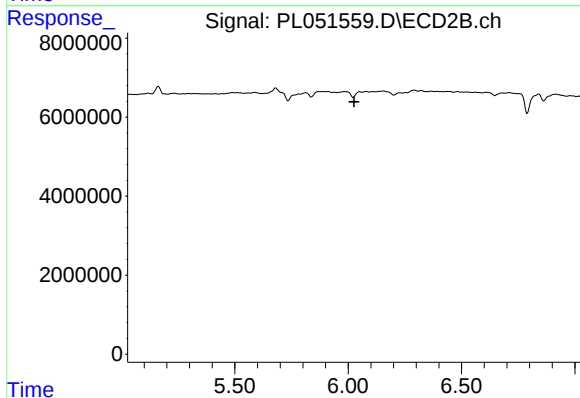


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

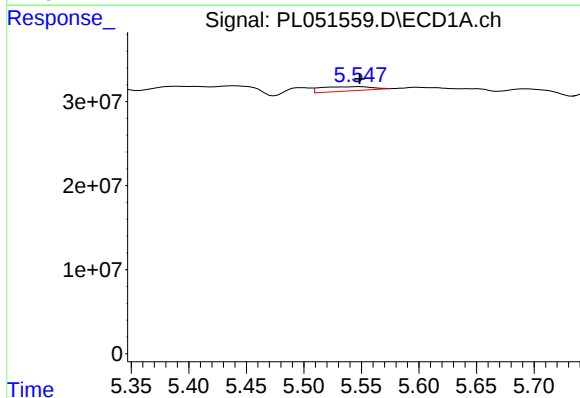


#13 Dieldrin

R.T.: 5.548 min
Delta R.T.: 0.000 min
Response: 15752752
Conc: 1.02 ng/ml

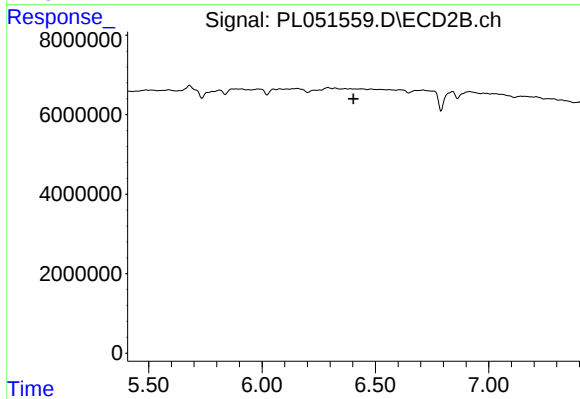

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.404 min
Response: 0
Conc: N.D.

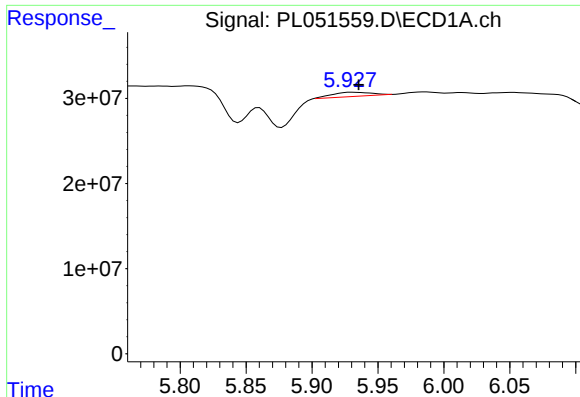

#16 4,4'-DDD


R.T.: 5.931 min
Delta R.T.: -0.005 min
Response: 10109542
Conc: 0.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4

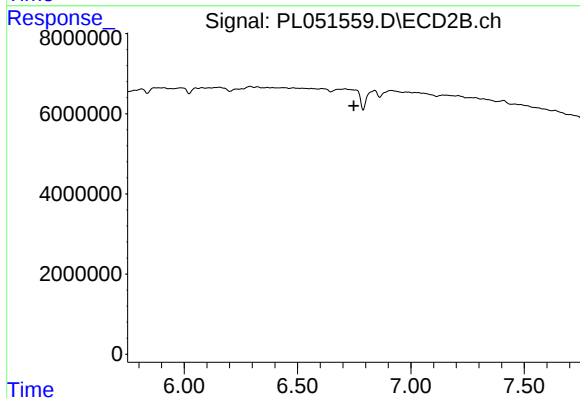


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.749 min
Response: 0
Conc: N.D.

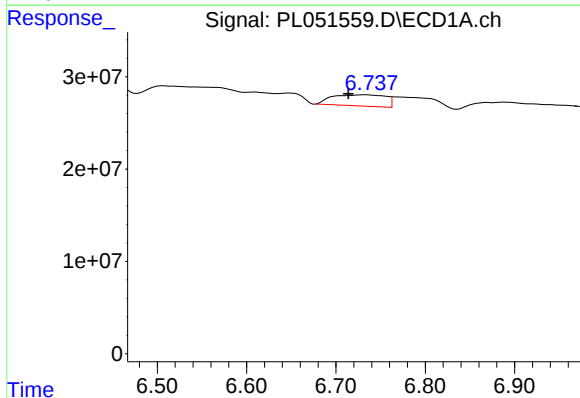


#20 Methoxychlor

R.T.: 6.733 min
Delta R.T.: 0.019 min
Response: 49592729
Conc: 7.95 ng/ml

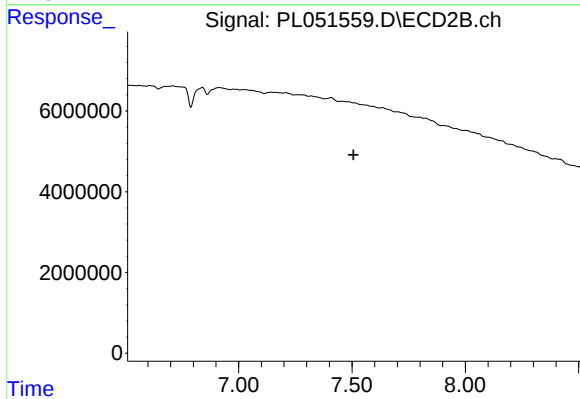

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.507 min
Response: 0
Conc: N.D.

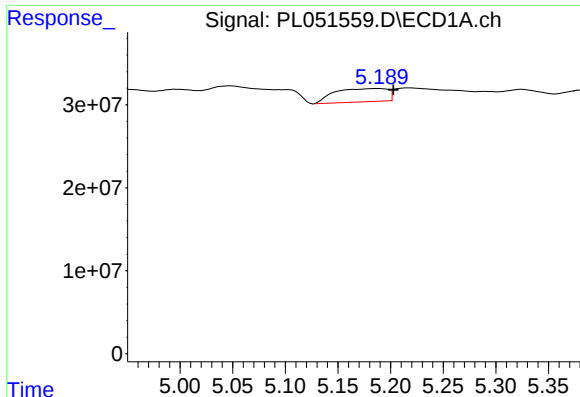

#25 Chlordane-3


R.T.: 5.189 min
Delta R.T.: -0.013 min
Response: 55649235
Conc: 39.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4

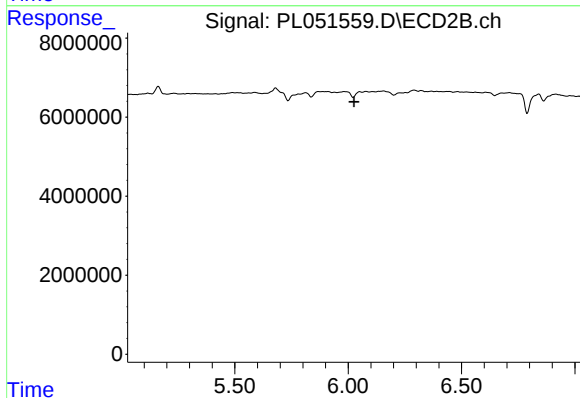


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

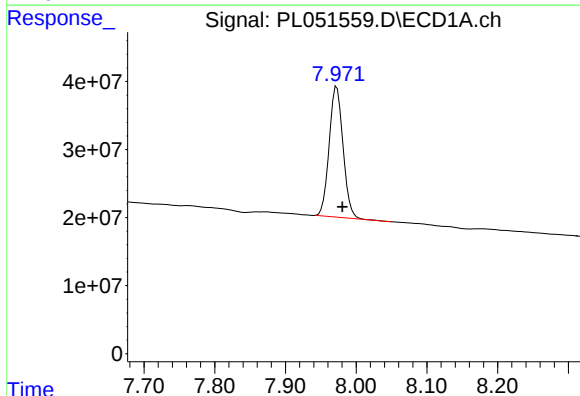

#28 Decachlorobiphenyl

R.T.: 7.973 min
Delta R.T.: -0.008 min
Response: 261117783
Conc: 25.79 ng/ml

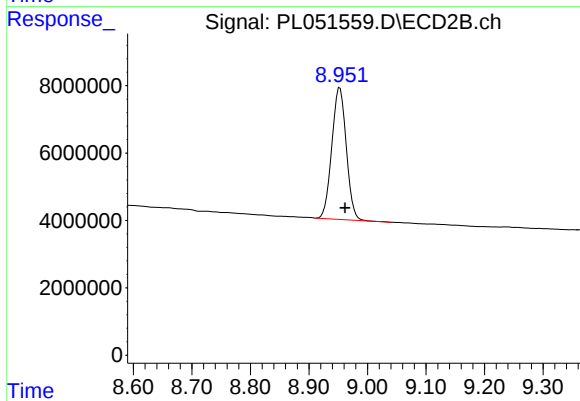

#28 Decachlorobiphenyl

R.T.: 8.953 min
Delta R.T.: -0.009 min
Response: 66952819
Conc: 23.68 ng/ml