

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081519\
 Data File : PL051561.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2019 01:11
 Operator : SG\AJ
 Sample : K4356-12
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 03:07:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	3.926	225.4E6	60806874	22.433	21.312
28)	SA Decachlor...	7.973	8.953	264.1E6	67419631	26.086	23.841
Target Compounds							
8)	B Heptachlo...	0.000	5.803	0	3578002	N.D.	0.935 #
9)	A Endosulfan I	5.325f	0.000	7105074	0	0.489	N.D. #
10)	B gamma-Chl...	5.198	0.000	27443042	0	1.739	N.D. #
11)	B alpha-Chl...	5.259	0.000	16935273	0	1.110	N.D. #
16)	A 4,4'-DDD	5.938	0.000	2431935	0	0.203	N.D. #
20)	A Methoxychlor	6.736f	0.000	27998991	0	4.488	N.D. #
25)	Chlordane-3	5.198	0.000	27443042	0	19.605	N.D. #
26)	Chlordane-4	5.259	0.000	16935273	0	12.840	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081519\
Data File : PL051561.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2019 01:11
Operator : SG\AJ
Sample : K4356-12
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 03:07:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

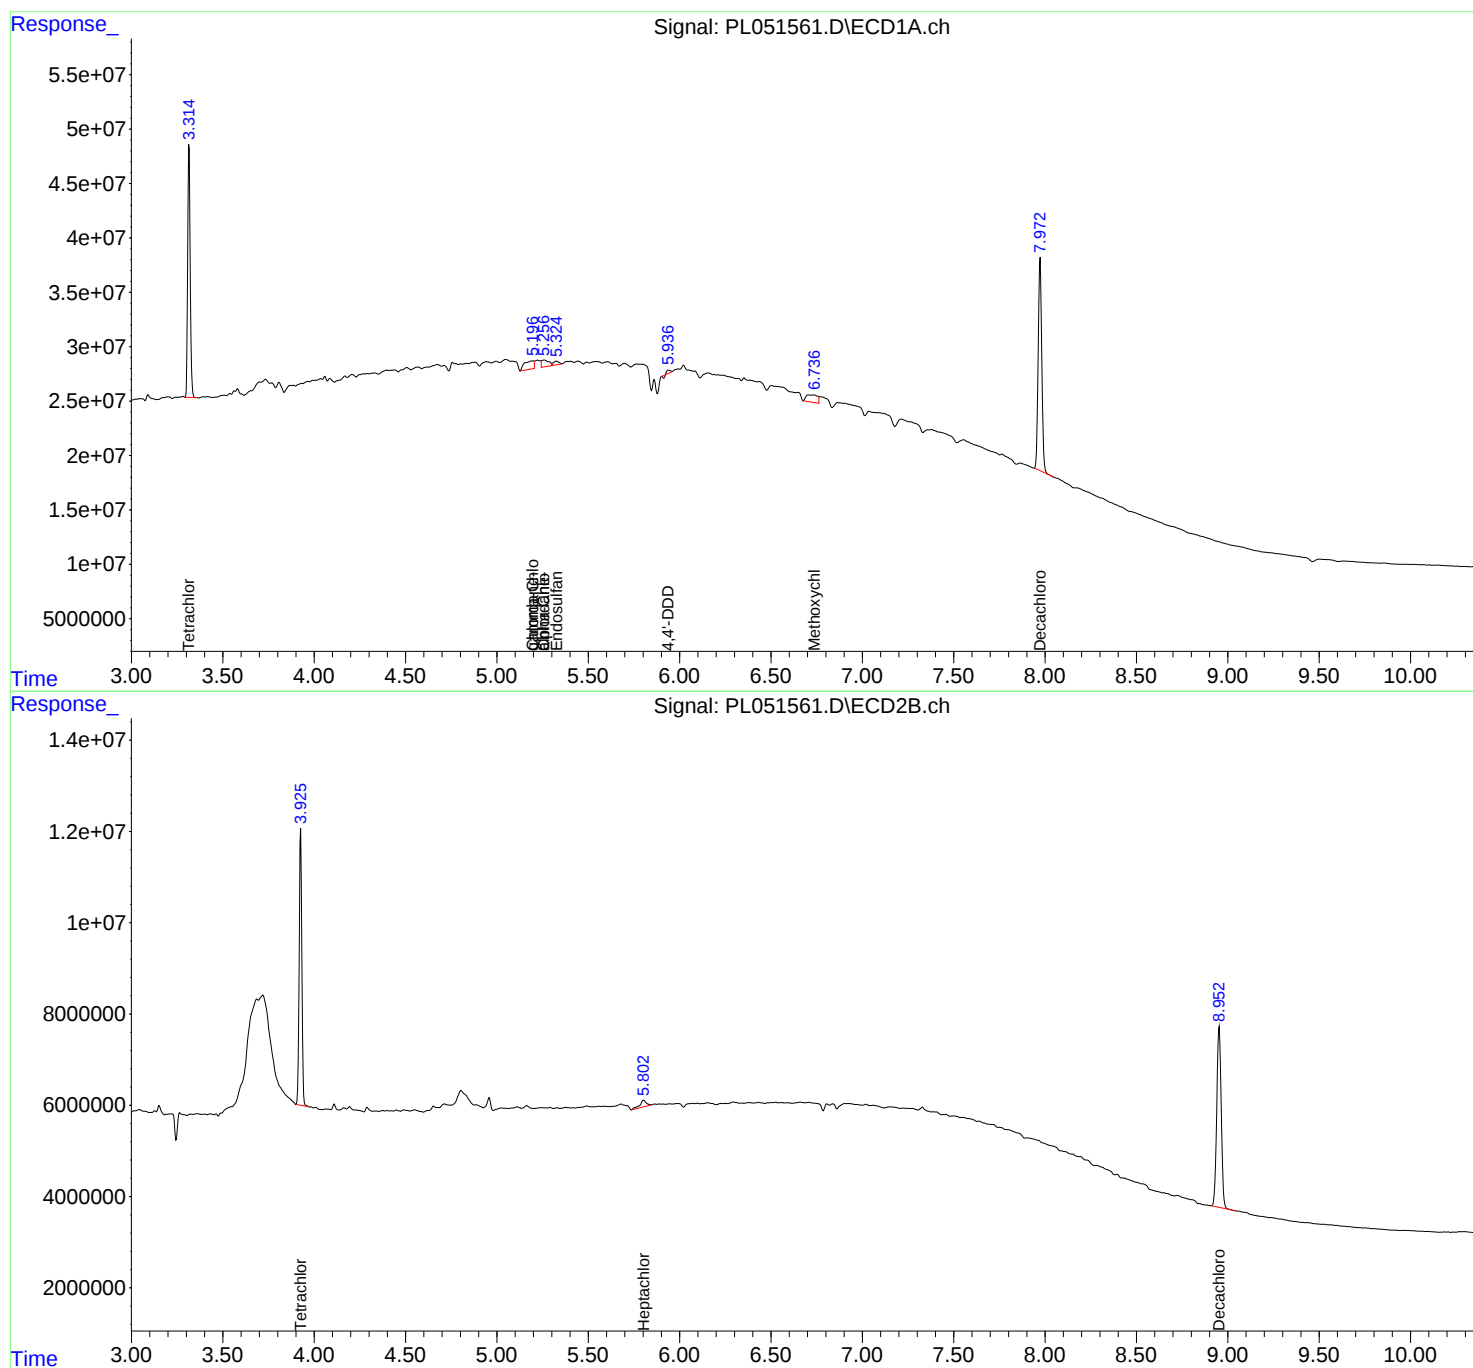


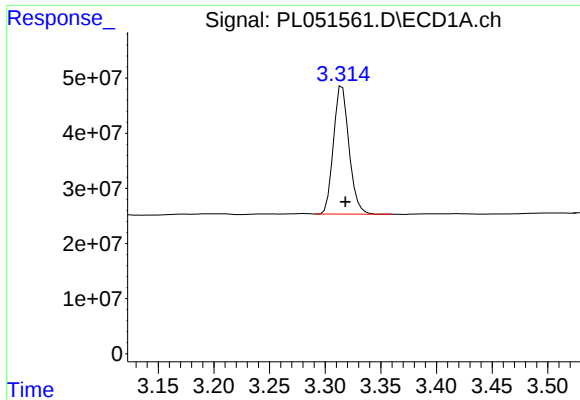

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: -0.003 min
Response: 225401771
Conc: 22.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6

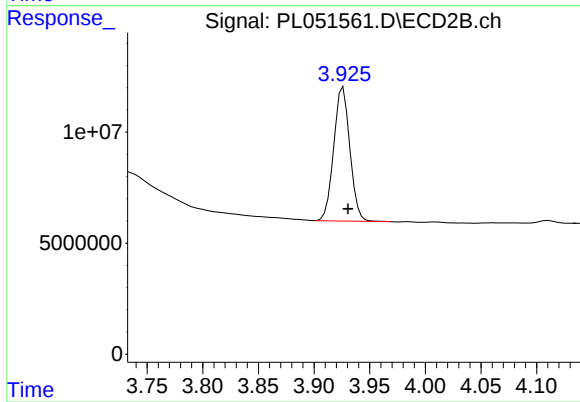


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.004 min
Response: 60806874
Conc: 21.31 ng/ml

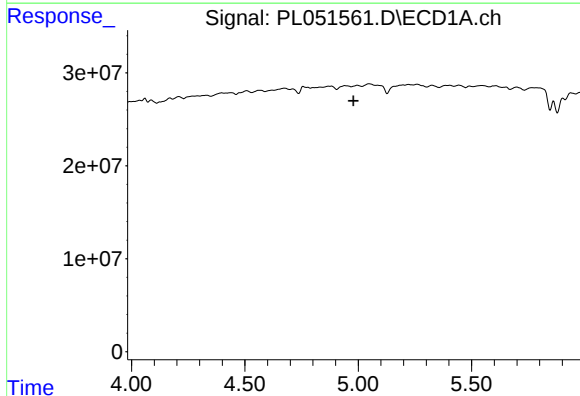


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.979 min
Response: 0
Conc: N.D.

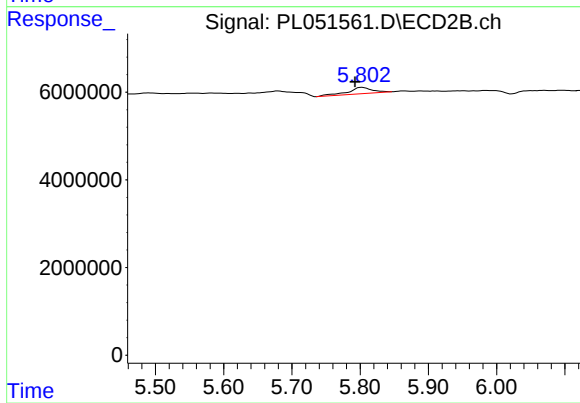

#8 Heptachlor epoxide


R.T.: 5.803 min
Delta R.T.: 0.010 min
Response: 3578002
Conc: 0.94 ng/ml

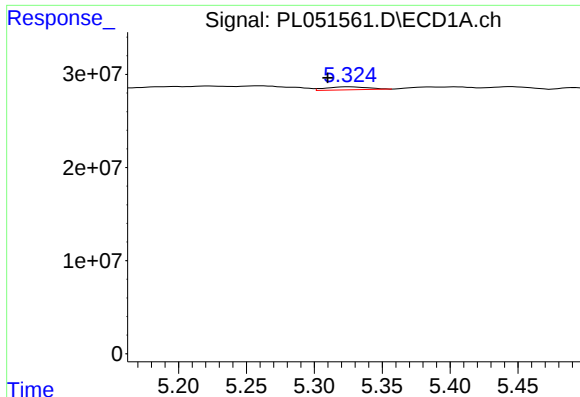

#9 Endosulfan I


R.T.: 5.325 min
Delta R.T.: 0.015 min
Response: 7105074
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6

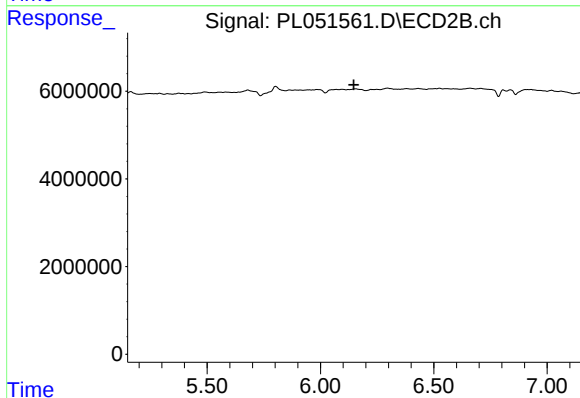


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.148 min
Response: 0
Conc: N.D.

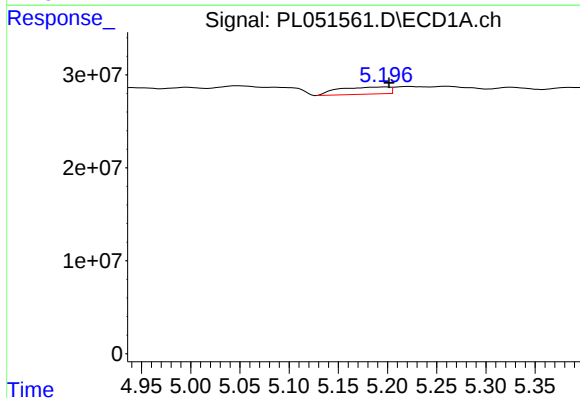


#10 gamma-Chlordane

R.T.: 5.198 min
Delta R.T.: -0.004 min
Response: 27443042
Conc: 1.74 ng/ml

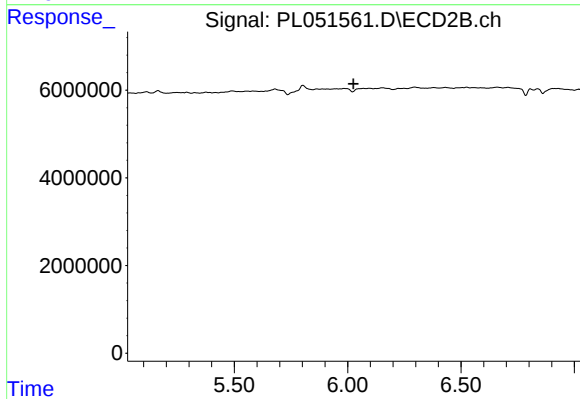

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

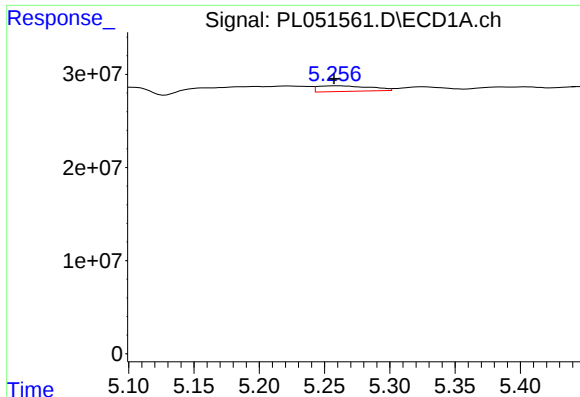

#11 alpha-Chlordane


R.T.: 5.259 min
Delta R.T.: 0.002 min
Response: 16935273
Conc: 1.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6

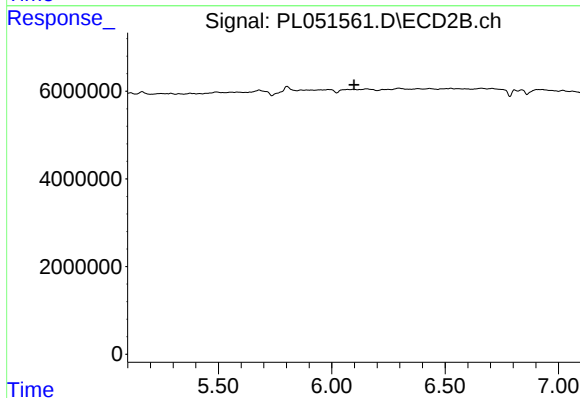


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

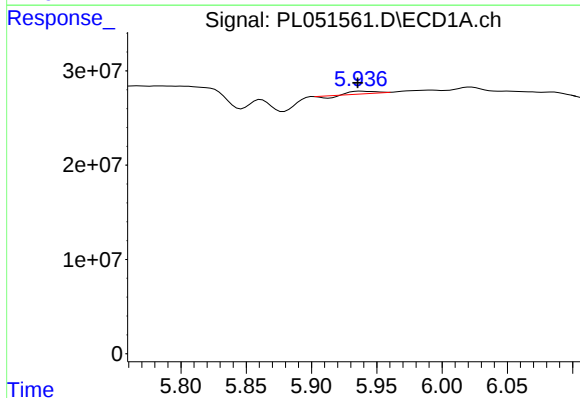


#16 4,4'-DDD

R.T.: 5.938 min
Delta R.T.: 0.002 min
Response: 2431935
Conc: 0.20 ng/ml

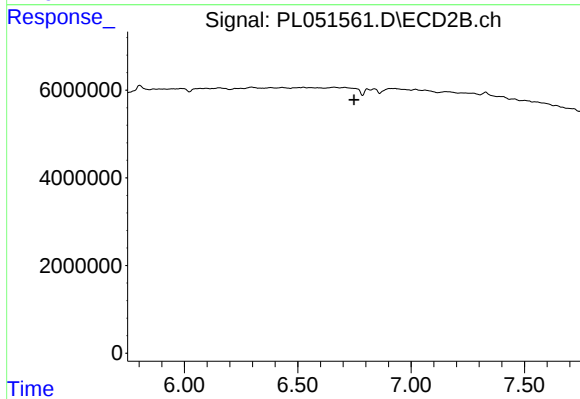

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.749 min
Response: 0
Conc: N.D.

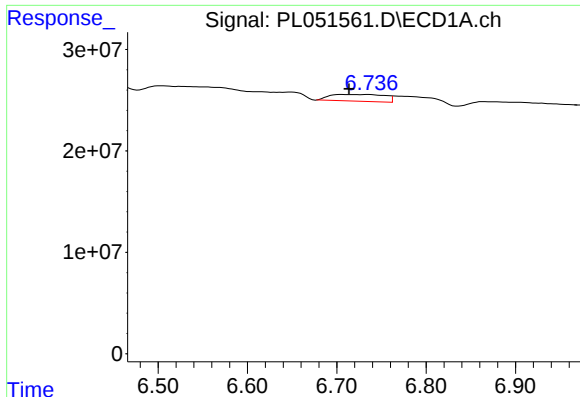

#20 Methoxychlor


R.T.: 6.736 min
Delta R.T.: 0.022 min
Response: 27998991
Conc: 4.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6

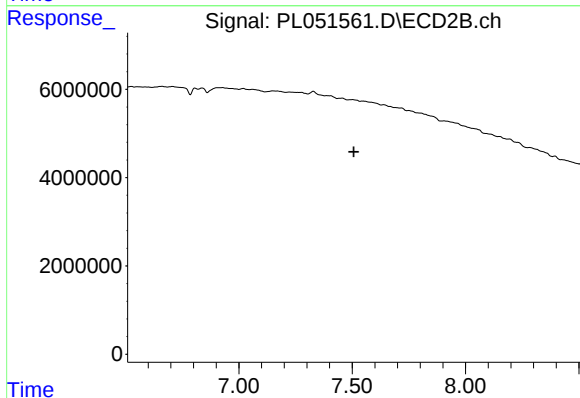


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.507 min
Response: 0
Conc: N.D.

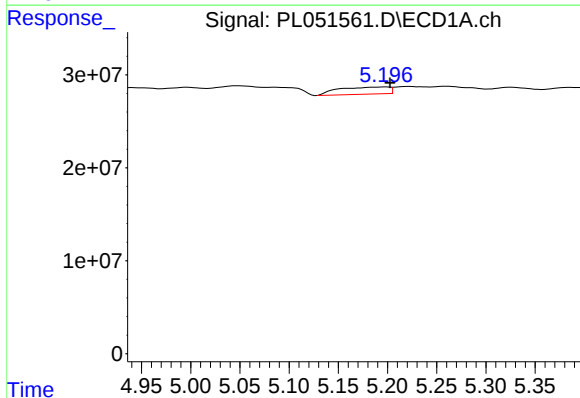


#25 Chlordane-3

R.T.: 5.198 min
Delta R.T.: -0.004 min
Response: 27443042
Conc: 19.61 ng/ml

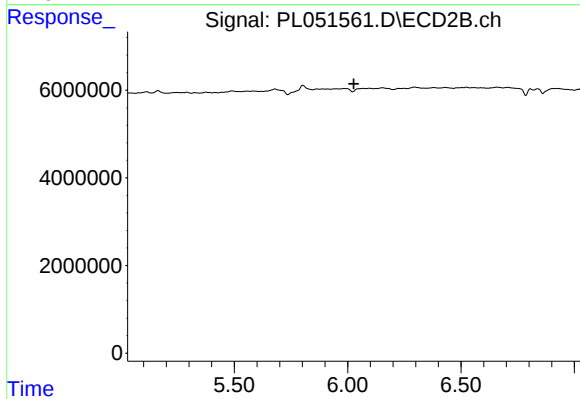

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

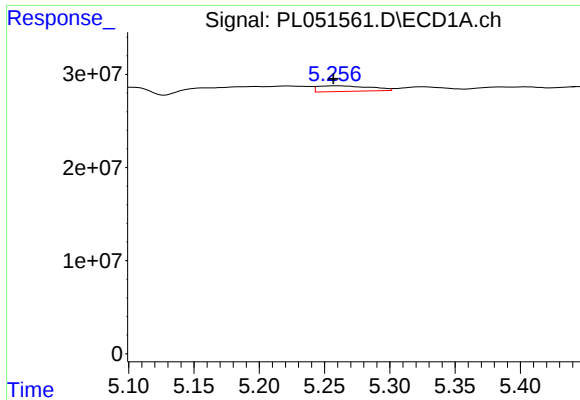

#26 Chlordane-4


R.T.: 5.259 min
Delta R.T.: 0.002 min
Response: 16935273
Conc: 12.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6

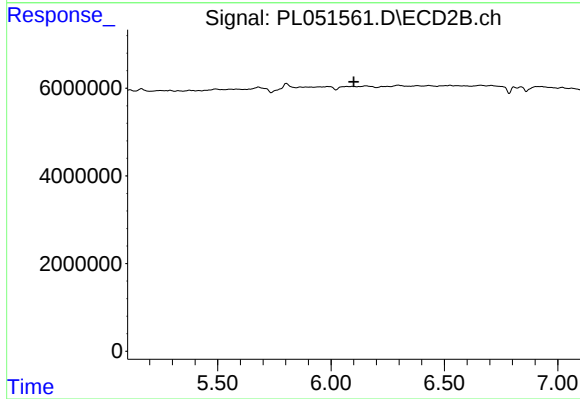


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.100 min
Response: 0
Conc: N.D.

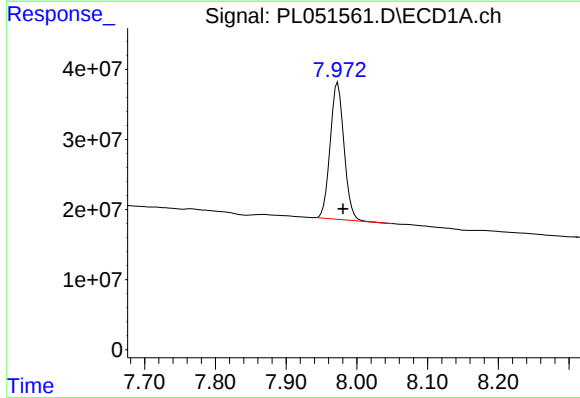

#28 Decachlorobiphenyl

R.T.: 7.973 min
Delta R.T.: -0.008 min
Response: 264134320
Conc: 26.09 ng/ml

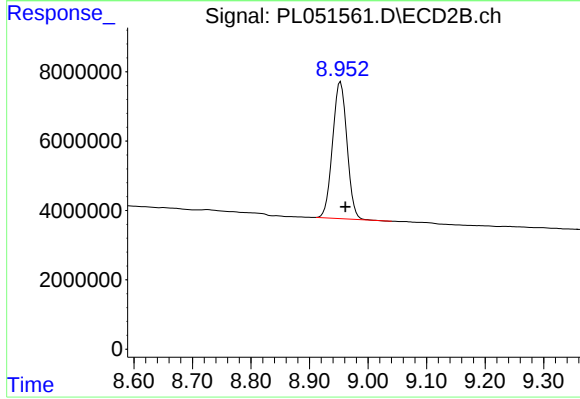

#28 Decachlorobiphenyl

R.T.: 8.953 min
Delta R.T.: -0.009 min
Response: 67419631
Conc: 23.84 ng/ml