

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
 Data File : PD064946.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2021 06:26
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 04:05:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081421.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 16 03:35:15 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.509	4.020	38717713	423.3E6	19.811	20.843
28)	SA Decachlor...	8.280	9.106	50108744	242.0E6	20.389	21.770
Target Compounds							
4)	MA Heptachlor	0.000	5.180f	0	2792534	N.D.	0.094 #
8)	B Heptachlo...	0.000	5.899	0	8160091	N.D.	0.319 #
15)	B Endosulfa...	0.000	6.955	0	1940461	N.D.	0.101 #
23)	Chlordane-1	4.414f	0.000	1936372	0	26.654	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
Data File : PD064946.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2021 06:26
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 04:05:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081421.M
Quant Title : GC Extractables
QLast Update : Mon Aug 16 03:35:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

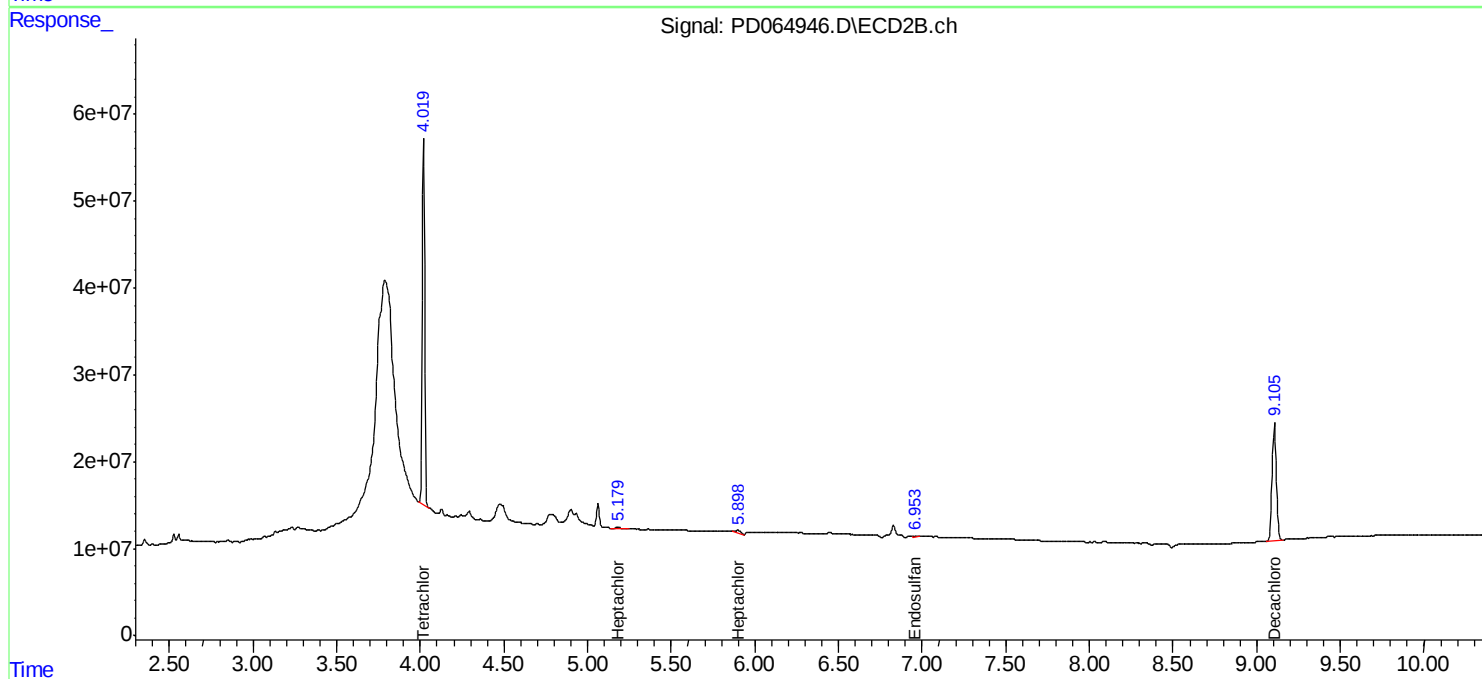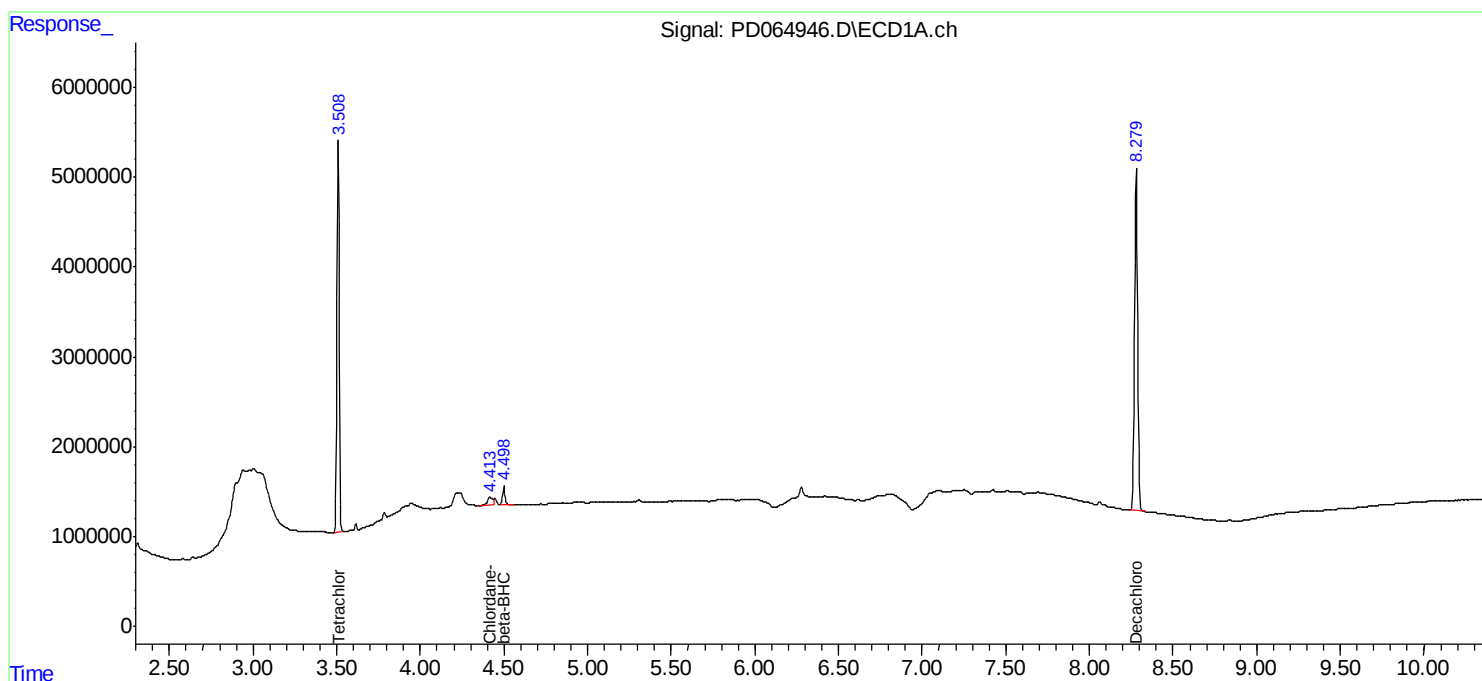


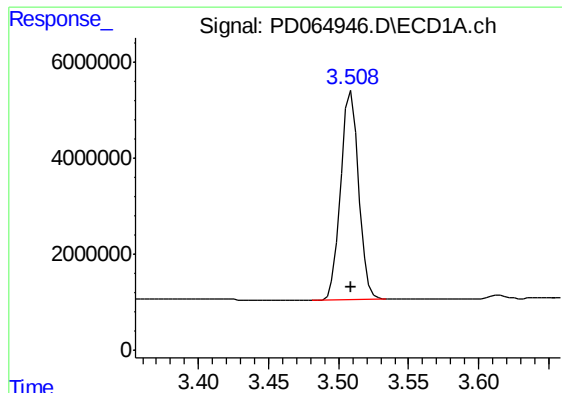

#1 Tetrachloro-m-xylene


R.T.: 3.509 min
Delta R.T.: 0.000 min
Response: 38717713
Conc: 19.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

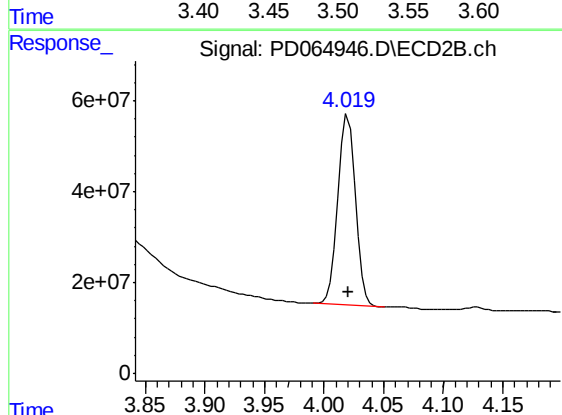


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 423260456
Conc: 20.84 ng/ml

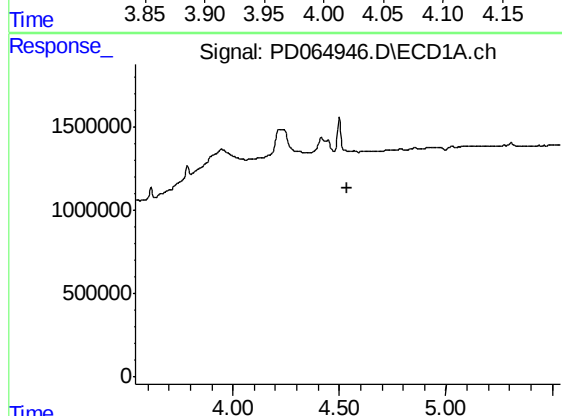


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.539 min
Response: 0
Conc: N.D.

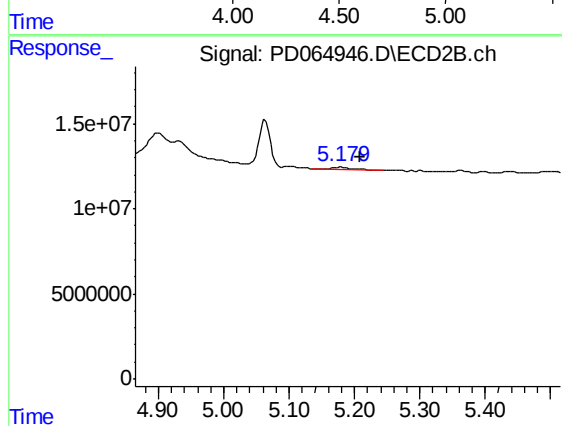

#4 Heptachlor


R.T.: 5.180 min
Delta R.T.: -0.028 min
Response: 2792534
Conc: 0.09 ng/ml

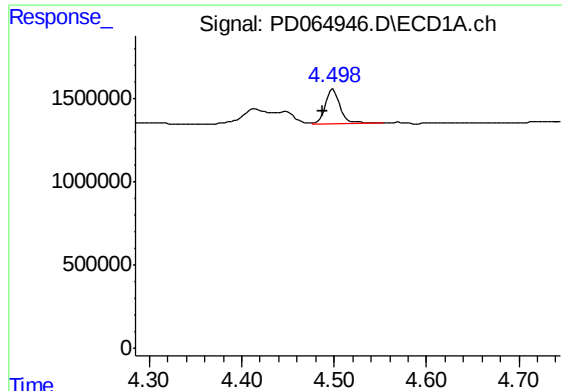

#6 beta-BHC


R.T.: 4.499 min
Delta R.T.: 0.011 min
Response: 2356597
Conc: 1.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

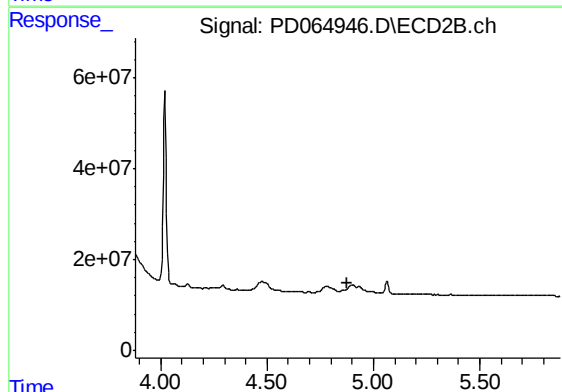


#6 beta-BHC

R.T.: 4.901 min
Delta R.T.: 0.022 min
Response: 12635838
Conc: N.D.

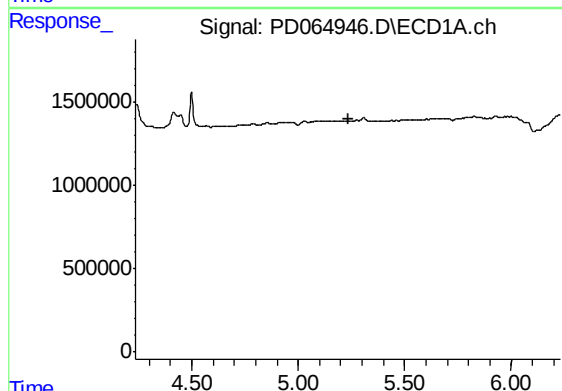


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.234 min
Response: 0
Conc: N.D.

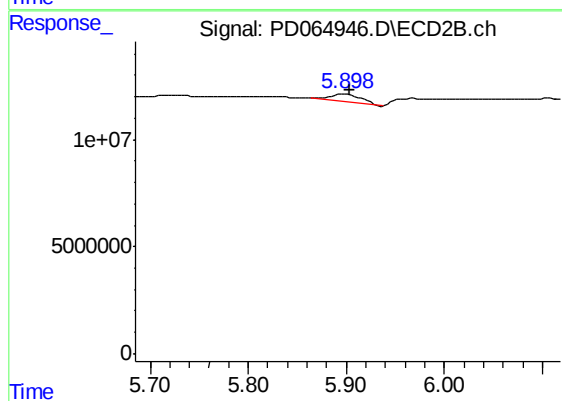

#8 Heptachlor epoxide


R.T.: 5.899 min
Delta R.T.: -0.005 min
Response: 8160091
Conc: 0.32 ng/ml

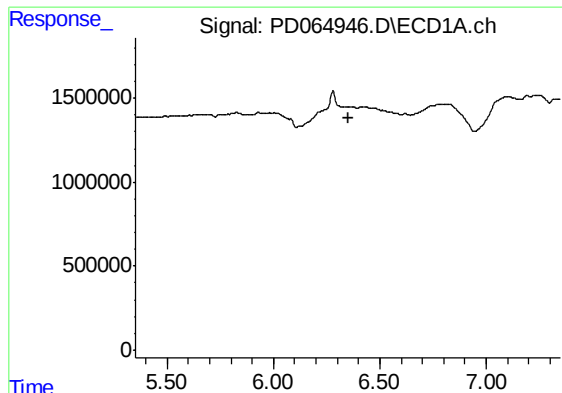

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.351 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

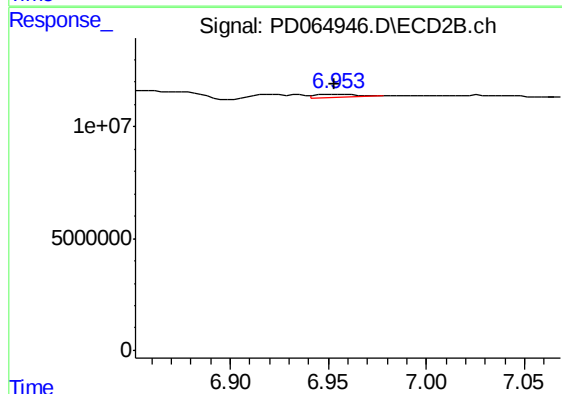


#15 Endosulfan II

R.T.: 6.955 min
Delta R.T.: 0.002 min
Response: 1940461
Conc: 0.10 ng/ml

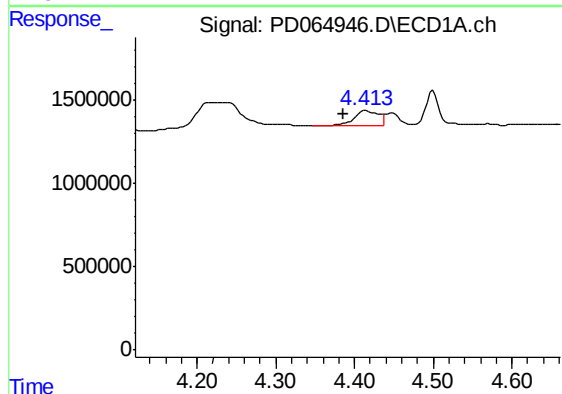


#23 Chlordane-1

R.T.: 4.414 min
Delta R.T.: 0.028 min
Response: 1936372
Conc: 26.65 ng/ml

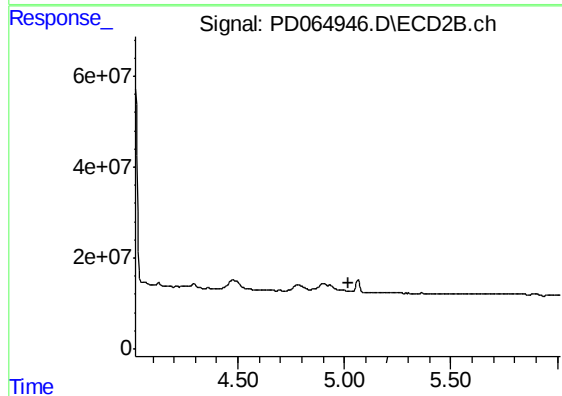

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.018 min
Response: 0
Conc: N.D.

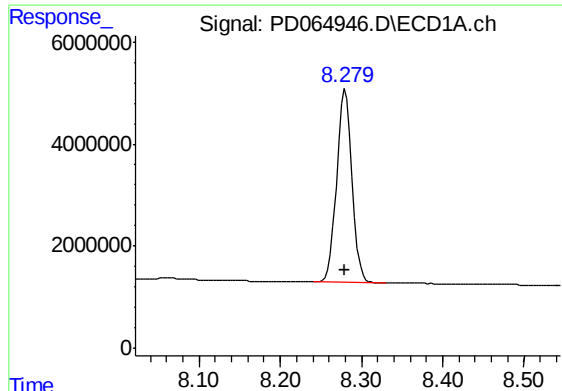

#28 Decachlorobiphenyl

R.T.: 8.280 min
Delta R.T.: 0.000 min
Response: 50108744
Conc: 20.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

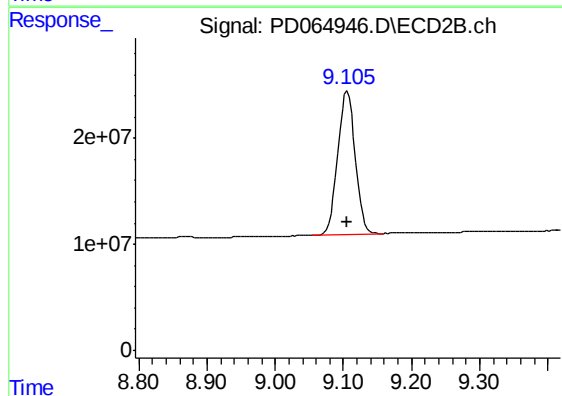

#28 Decachlorobiphenyl

R.T.: 9.106 min
Delta R.T.: 0.000 min
Response: 241951307
Conc: 21.77 ng/ml