

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
 Data File : PD064949.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2021 07:09
 Operator : AR\AJ
 Sample : PB137641BL
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB137641BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 04:06:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081421.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 16 03:35:15 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.511	4.020	42508947	463.3E6	21.751	22.817
28)	SA Decachlor...	8.284	9.108	55885903	266.2E6	22.740	23.951
Target Compounds							
2)	A alpha-BHC	3.948	4.432f	1134907	48018216	0.377	1.514 #
4)	MA Heptachlor	0.000	5.186f	0	6288117	N.D.	0.212 #
15)	B Endosulfa...	0.000	6.956	0	2974147	N.D.	0.155 #
23)	Chlordane-1	4.416f	0.000	2732380	0	37.611	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
Data File : PD064949.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2021 07:09
Operator : AR\AJ
Sample : PB137641BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB137641BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 04:06:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081421.M
Quant Title : GC Extractables
QLast Update : Mon Aug 16 03:35:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

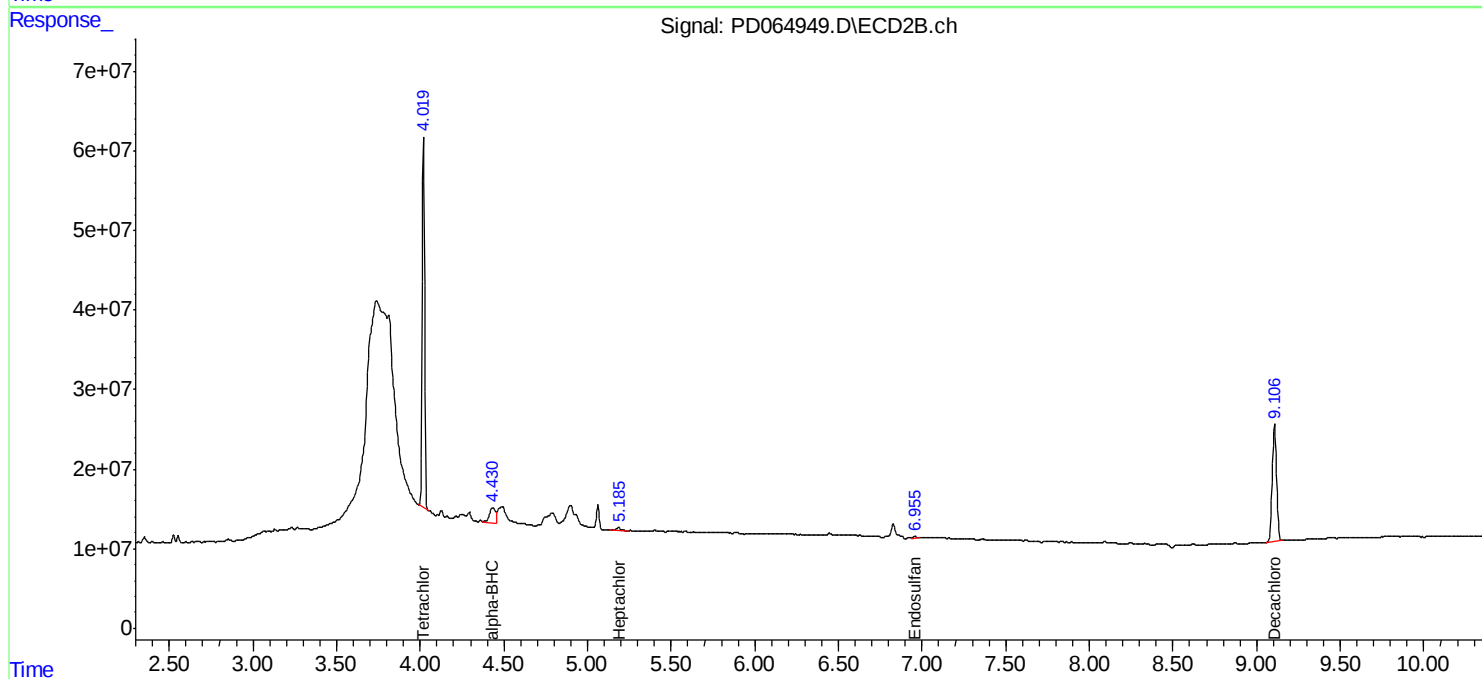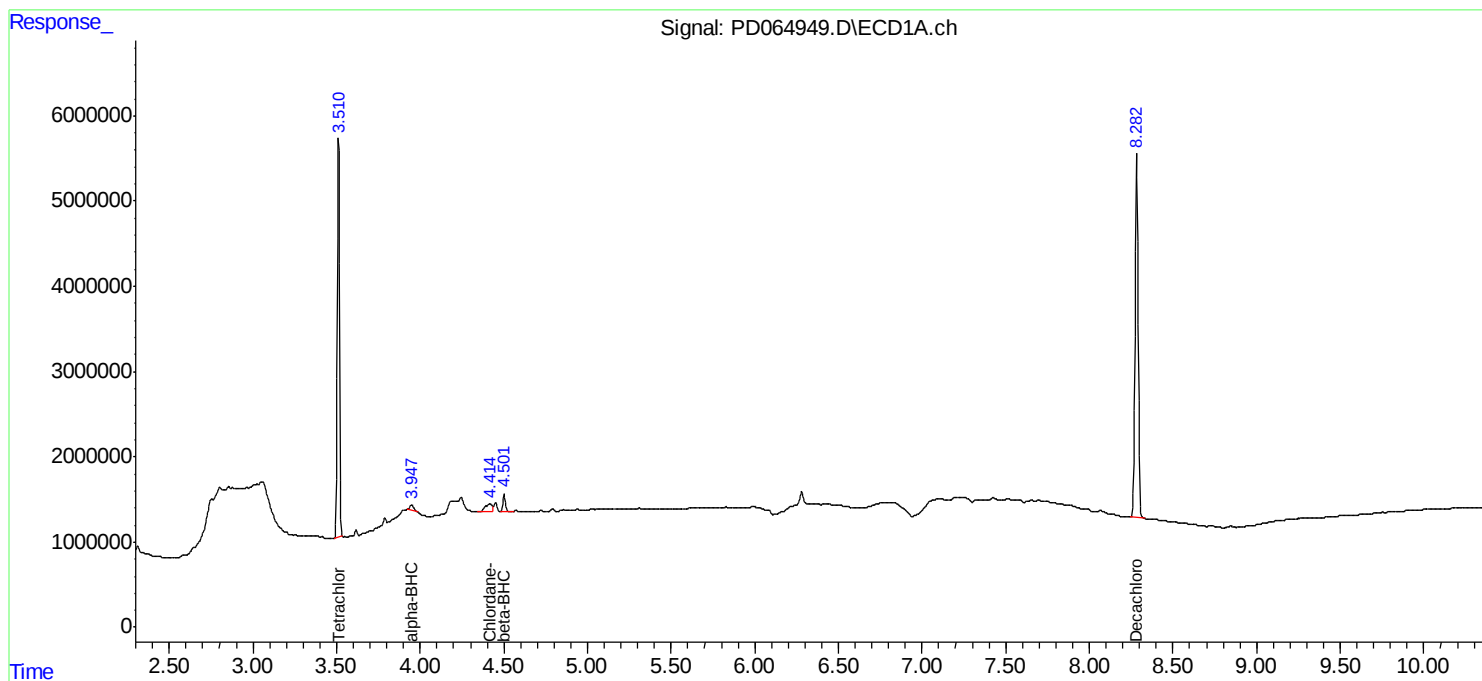


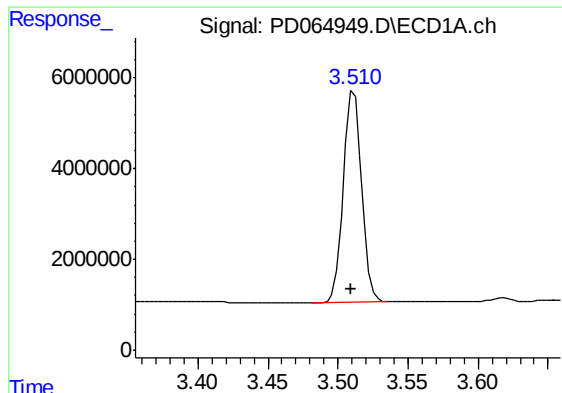

#1 Tetrachloro-m-xylene


R.T.: 3.511 min
Delta R.T.: 0.002 min
Response: 42508947
Conc: 21.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB137641BL

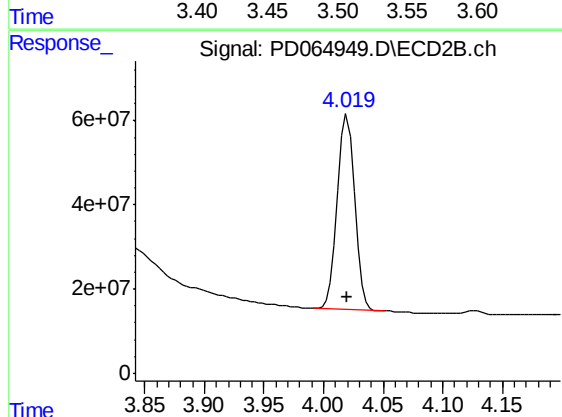


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 463342590
Conc: 22.82 ng/ml

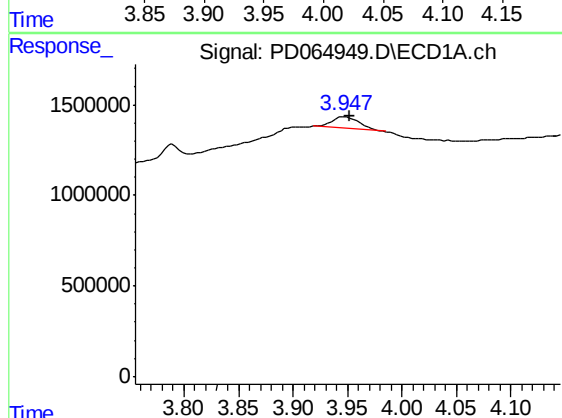


#2 alpha-BHC

R.T.: 3.948 min
Delta R.T.: -0.005 min
Response: 1134907
Conc: 0.38 ng/ml

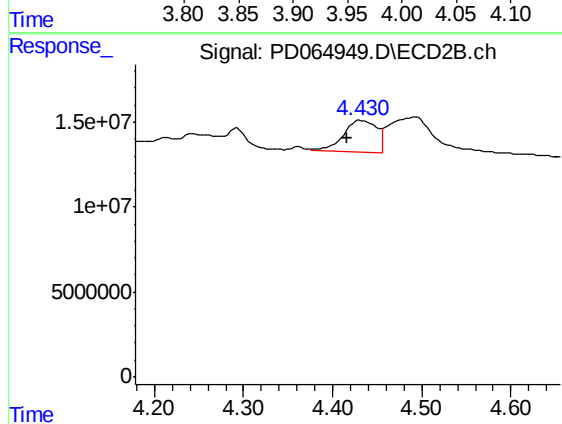

#2 alpha-BHC


R.T.: 4.432 min
Delta R.T.: 0.016 min
Response: 48018216
Conc: 1.51 ng/ml

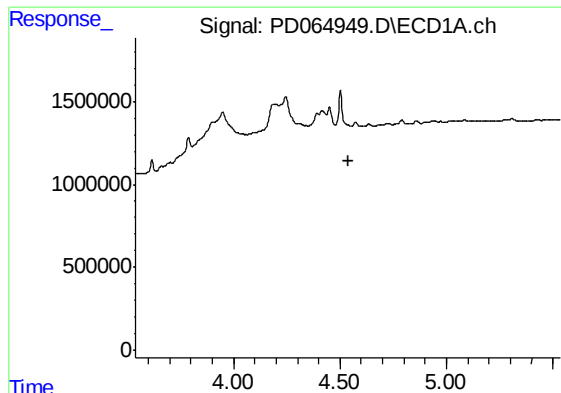

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.539 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB137641BL

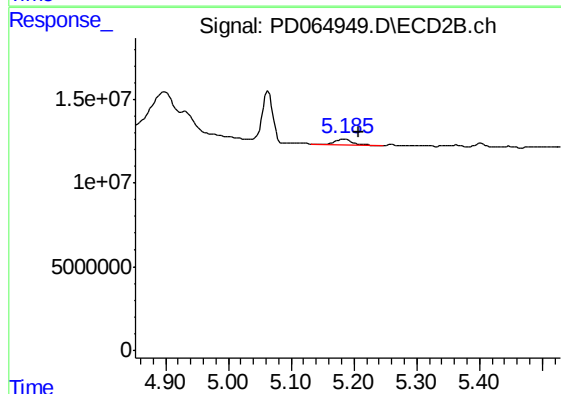


#4 Heptachlor

R.T.: 5.186 min
Delta R.T.: -0.021 min
Response: 6288117
Conc: 0.21 ng/ml

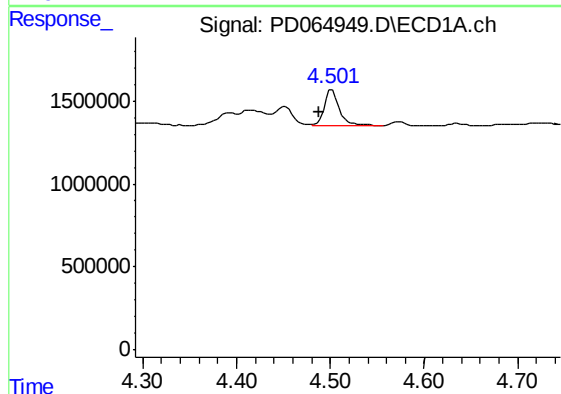


#6 beta-BHC

R.T.: 4.502 min
Delta R.T.: 0.014 min
Response: 2341600
Conc: 1.88 ng/ml

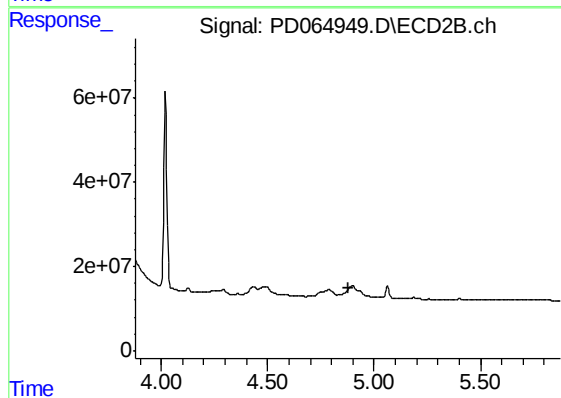

#6 beta-BHC


R.T.: 4.899 min
Delta R.T.: 0.020 min
Response: 30179158
Conc: N.D.

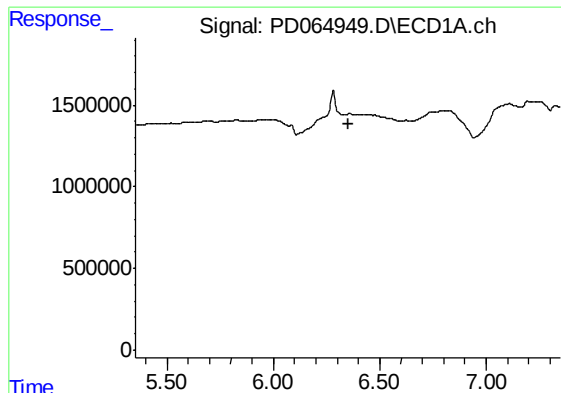

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.351 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB137641BL

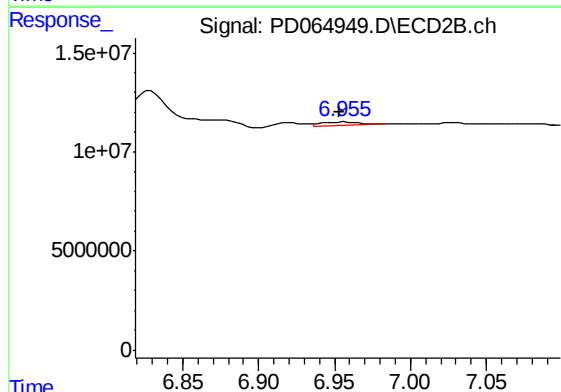


#15 Endosulfan II

R.T.: 6.956 min
Delta R.T.: 0.003 min
Response: 2974147
Conc: 0.15 ng/ml

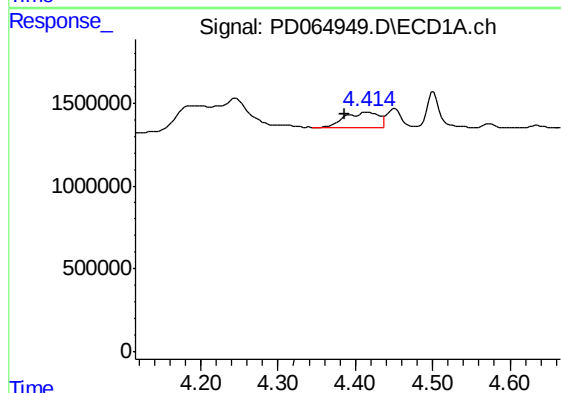


#23 Chlordane-1

R.T.: 4.416 min
Delta R.T.: 0.030 min
Response: 2732380
Conc: 37.61 ng/ml

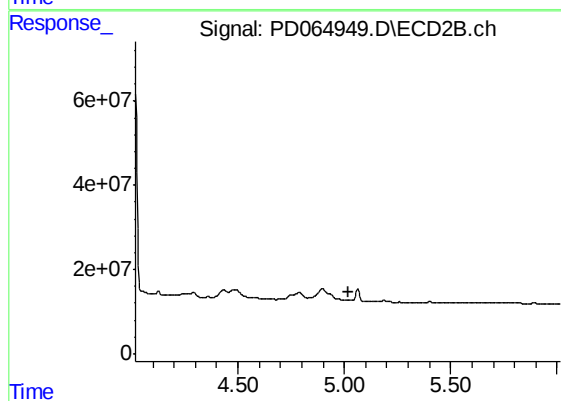

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.018 min
Response: 0
Conc: N.D.

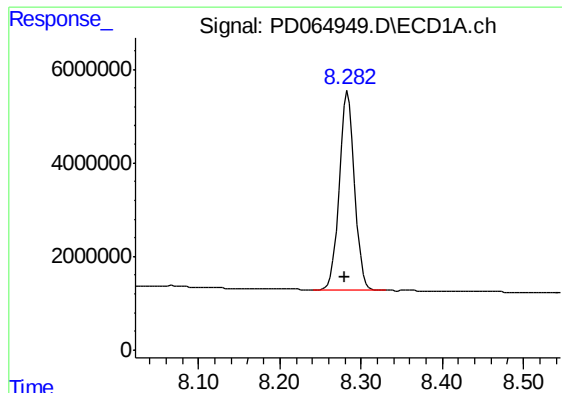

#28 Decachlorobiphenyl

R.T.: 8.284 min
Delta R.T.: 0.004 min
Response: 55885903
Conc: 22.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB137641BL

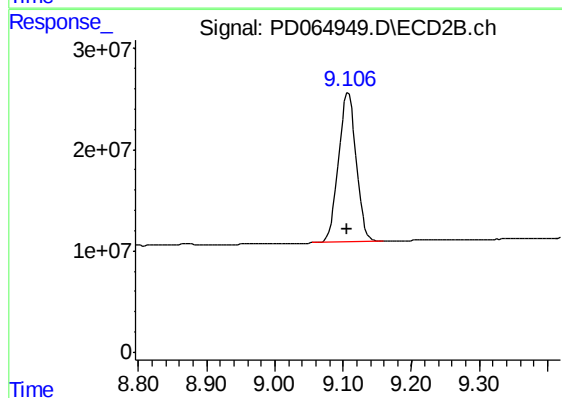

#28 Decachlorobiphenyl

R.T.: 9.108 min
Delta R.T.: 0.003 min
Response: 266192717
Conc: 23.95 ng/ml