

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
 Data File : PD064957.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2021 08:59
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 04:09:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081421.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 16 03:35:15 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.508	4.020	38272711	420.3E6	19.583	20.695
28)	SA Decachlor...	8.279	9.105	50305863	244.3E6	20.470	21.981
Target Compounds							
8)	B Heptachlo...	0.000	5.897	0	8851052	N.D.	0.346 #
10)	B gamma-Chl...	0.000	6.140	0	3322012	N.D.	0.127 #
15)	B Endosulfa...	0.000	6.957	0	2333795	N.D.	0.122 #
23)	Chlordane-1	4.414f	0.000	1913232	0	26.335	N.D. #
25)	Chlordane-3	0.000	6.140	0	3322012	N.D.	0.991 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
Data File : PD064957.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2021 08:59
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 04:09:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081421.M
Quant Title : GC Extractables
QLast Update : Mon Aug 16 03:35:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

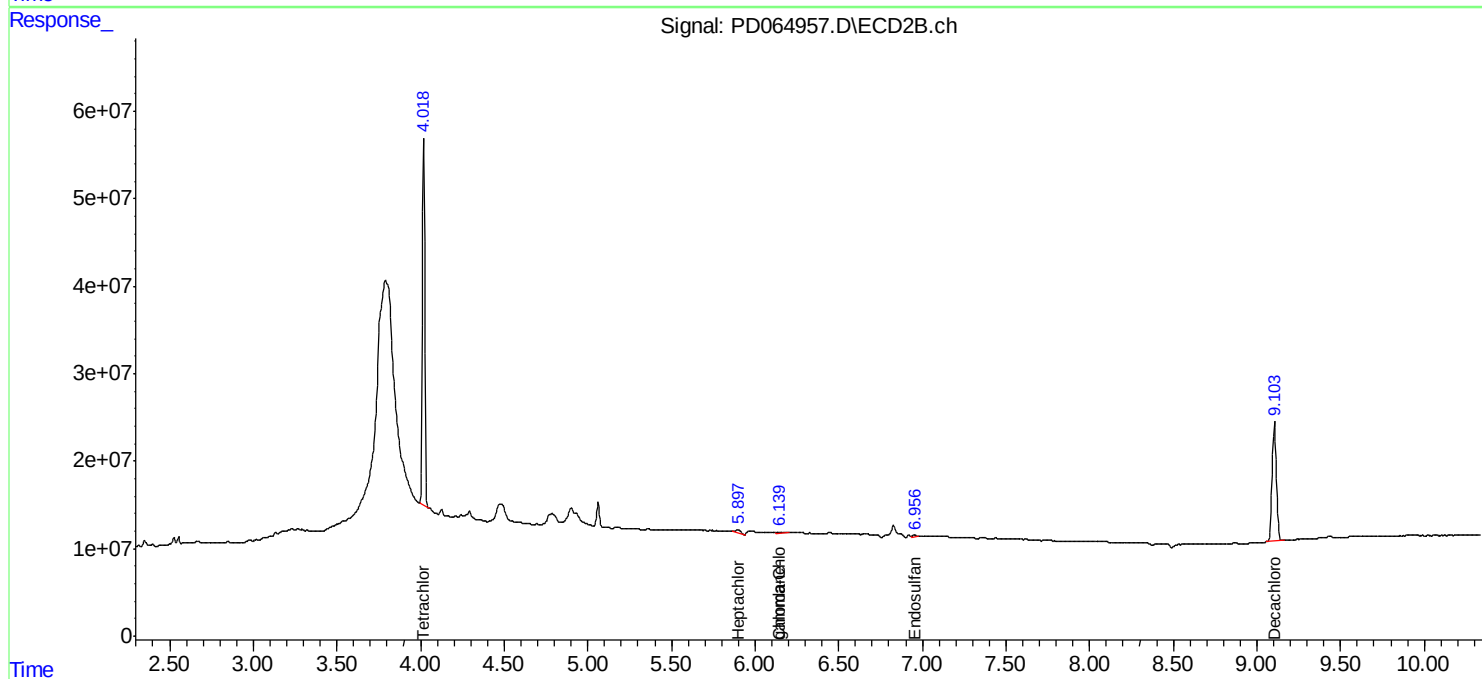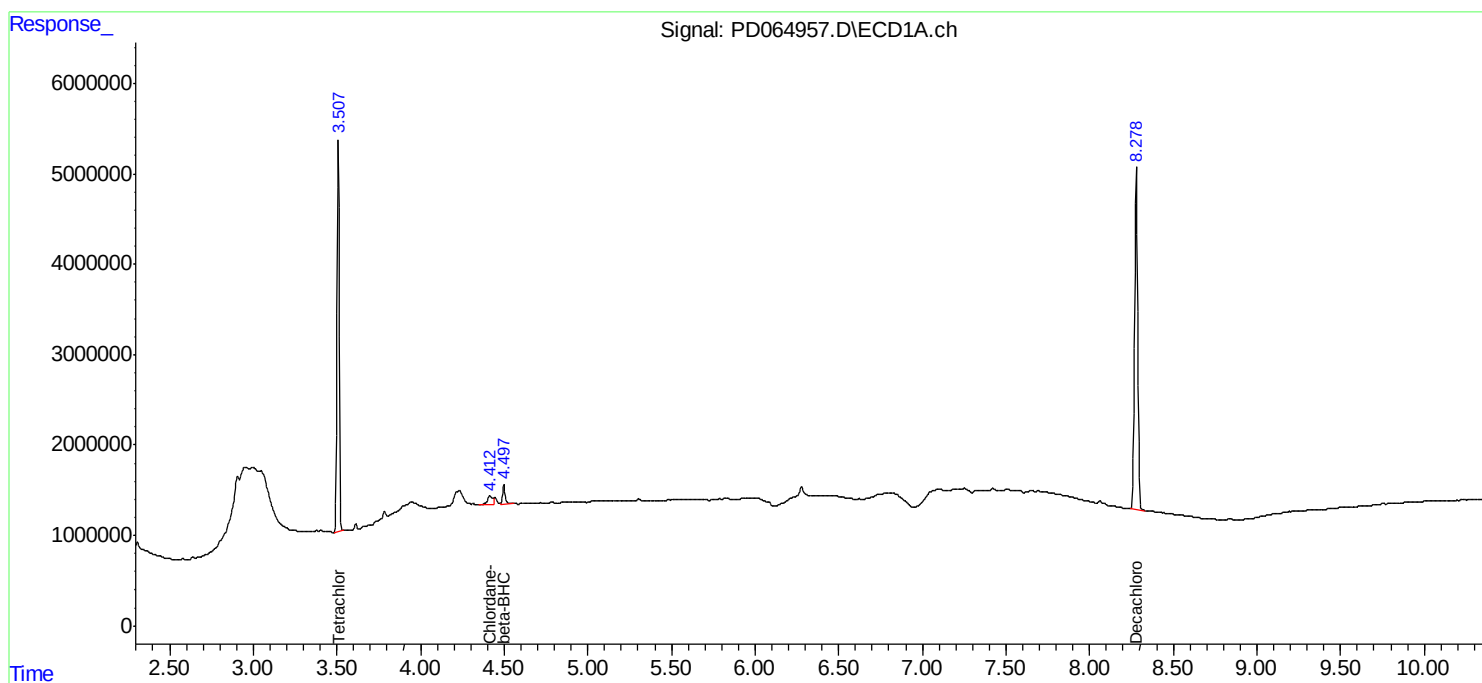


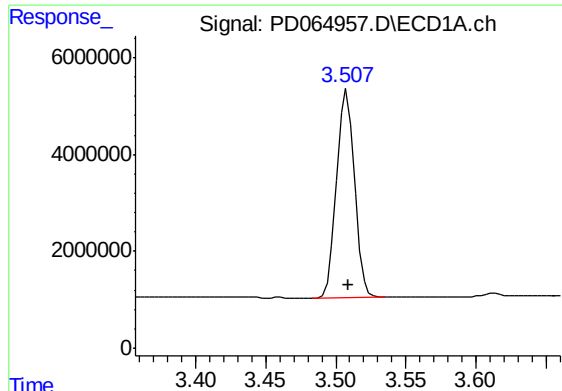

#1 Tetrachloro-m-xylene


R.T.: 3.508 min
Delta R.T.: 0.000 min
Response: 38272711
Conc: 19.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

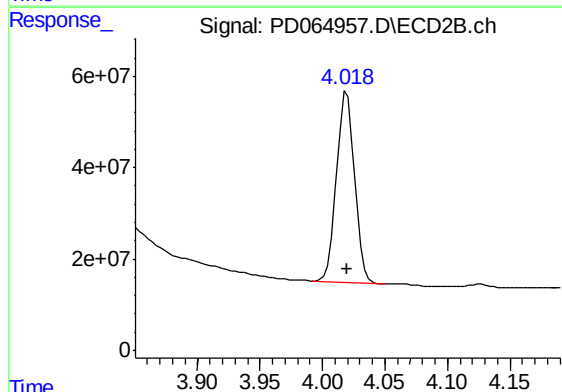


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 420263510
Conc: 20.70 ng/ml

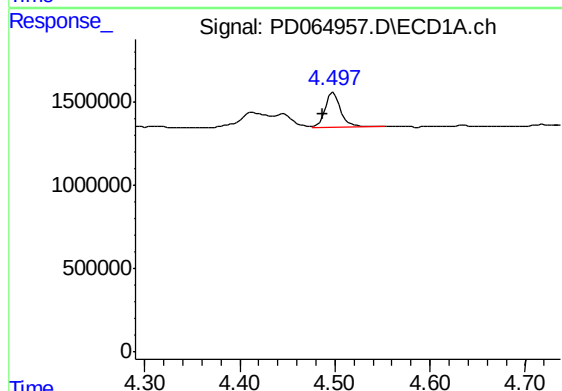


#6 beta-BHC

R.T.: 4.499 min
Delta R.T.: 0.011 min
Response: 2323041
Conc: 1.87 ng/ml

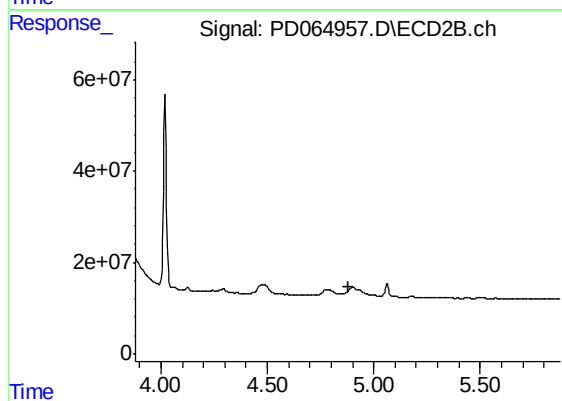

#6 beta-BHC


R.T.: 4.901 min
Delta R.T.: 0.022 min
Response: 14395512
Conc: N.D.

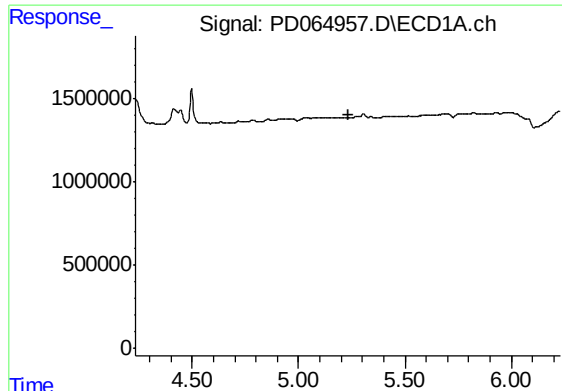

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.234 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

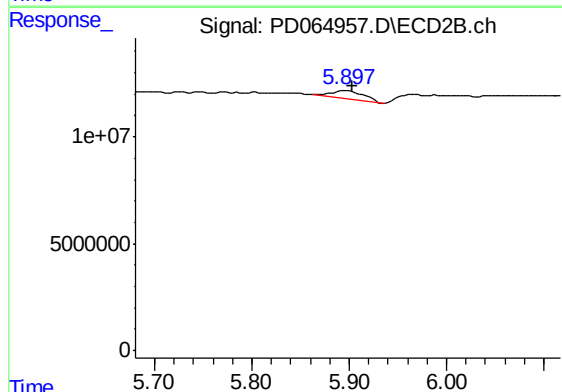


#8 Heptachlor epoxide

R.T.: 5.897 min
Delta R.T.: -0.007 min
Response: 8851052
Conc: 0.35 ng/ml

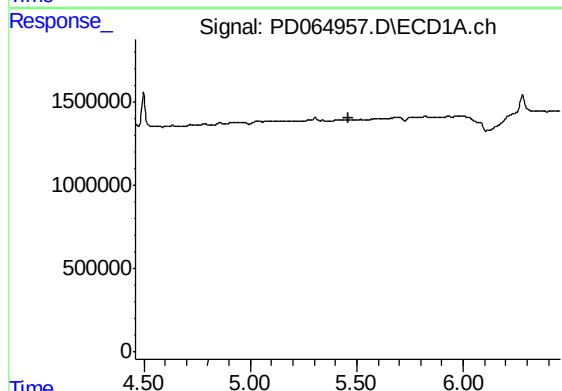


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.460 min
Response: 0
Conc: N.D.

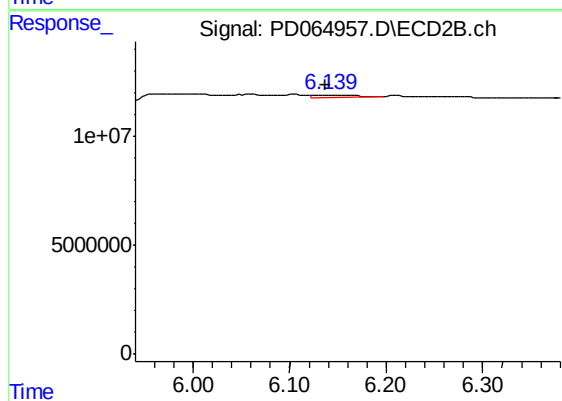

#10 gamma-Chlordane


R.T.: 6.140 min
Delta R.T.: 0.002 min
Response: 3322012
Conc: 0.13 ng/ml

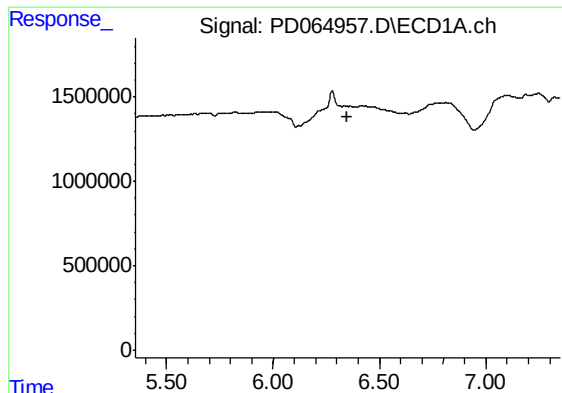

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.351 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

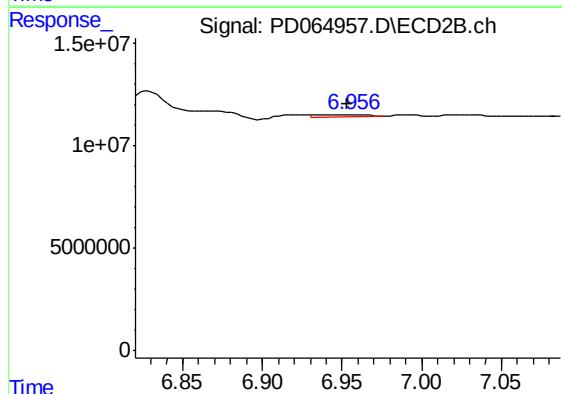


#15 Endosulfan II

R.T.: 6.957 min
Delta R.T.: 0.003 min
Response: 2333795
Conc: 0.12 ng/ml

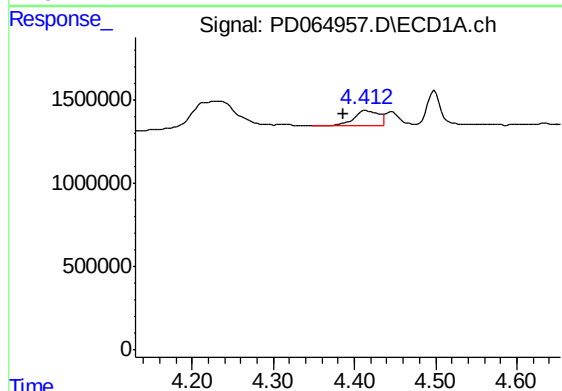


#23 Chlordane-1

R.T.: 4.414 min
Delta R.T.: 0.028 min
Response: 1913232
Conc: 26.34 ng/ml

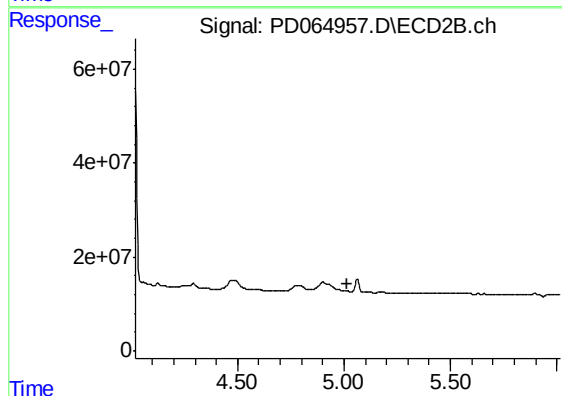

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.018 min
Response: 0
Conc: N.D.

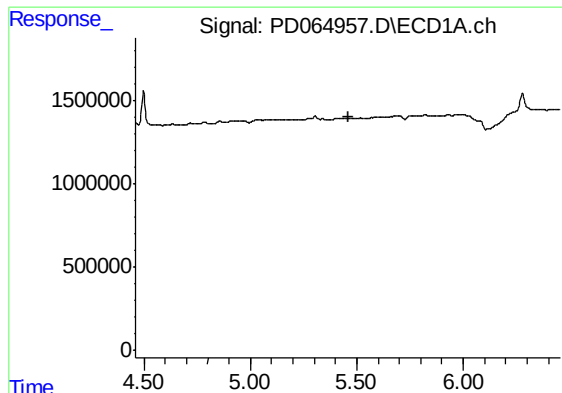

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.460 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

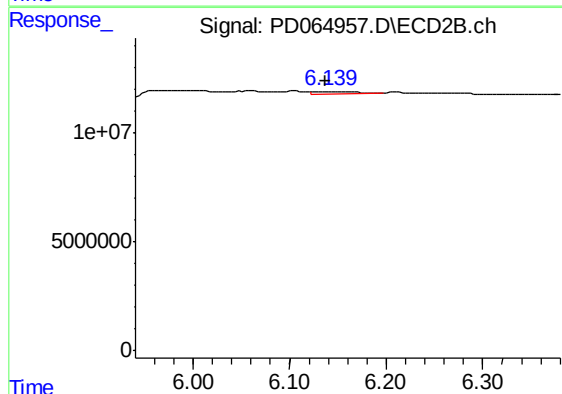


#25 Chlordane-3

R.T.: 6.140 min
Delta R.T.: 0.002 min
Response: 3322012
Conc: 0.99 ng/ml

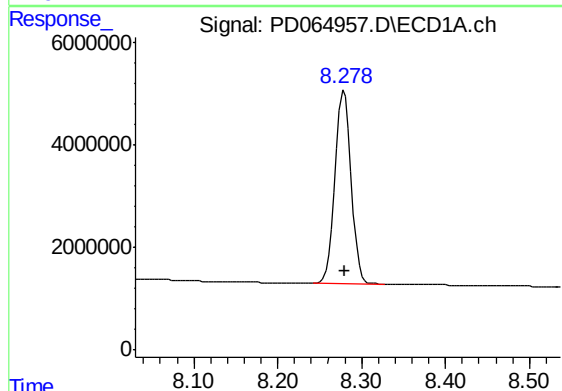

#28 Decachlorobiphenyl

R.T.: 8.279 min
Delta R.T.: 0.000 min
Response: 50305863
Conc: 20.47 ng/ml

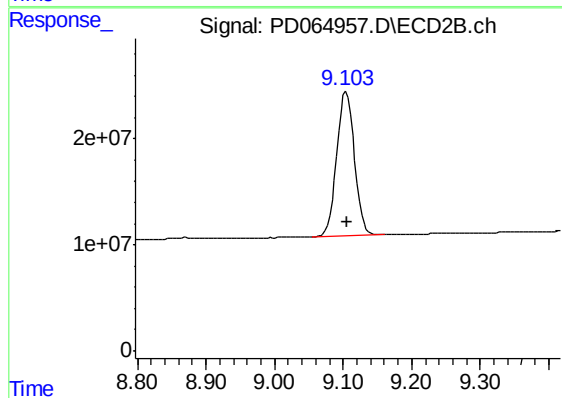

#28 Decachlorobiphenyl

R.T.: 9.105 min
Delta R.T.: 0.000 min
Response: 244294216
Conc: 21.98 ng/ml