

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
 Data File : PD064969.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2021 11:59
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 04:10:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081421.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 16 03:35:15 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.508	4.020	38014291	422.4E6	19.451	20.800
28)	SA Decachlor...	8.280	9.106	31633415	250.1E6	12.872	22.505 #
Target Compounds							
8)	B Heptachlo...	0.000	5.899	0 24821851	N.D.	0.971	#
10)	B gamma-Chl...	0.000	6.136	0 8710205	N.D.	0.333	#
11)	B alpha-Chl...	0.000	6.210	0 2022586	N.D.	0.080	#
15)	B Endosulfa...	0.000	6.955	0 3386737	N.D.	0.176	#
23)	Chlordane-1	4.414f	0.000	2067961	0 28.465	N.D.	#
25)	Chlordane-3	0.000	6.136	0 8710205	N.D.	2.597	#
26)	Chlordane-4	0.000	6.210	0 2022586	N.D.	0.520	#


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
Data File : PD064969.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2021 11:59
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 04:10:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081421.M
Quant Title : GC Extractables
QLast Update : Mon Aug 16 03:35:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

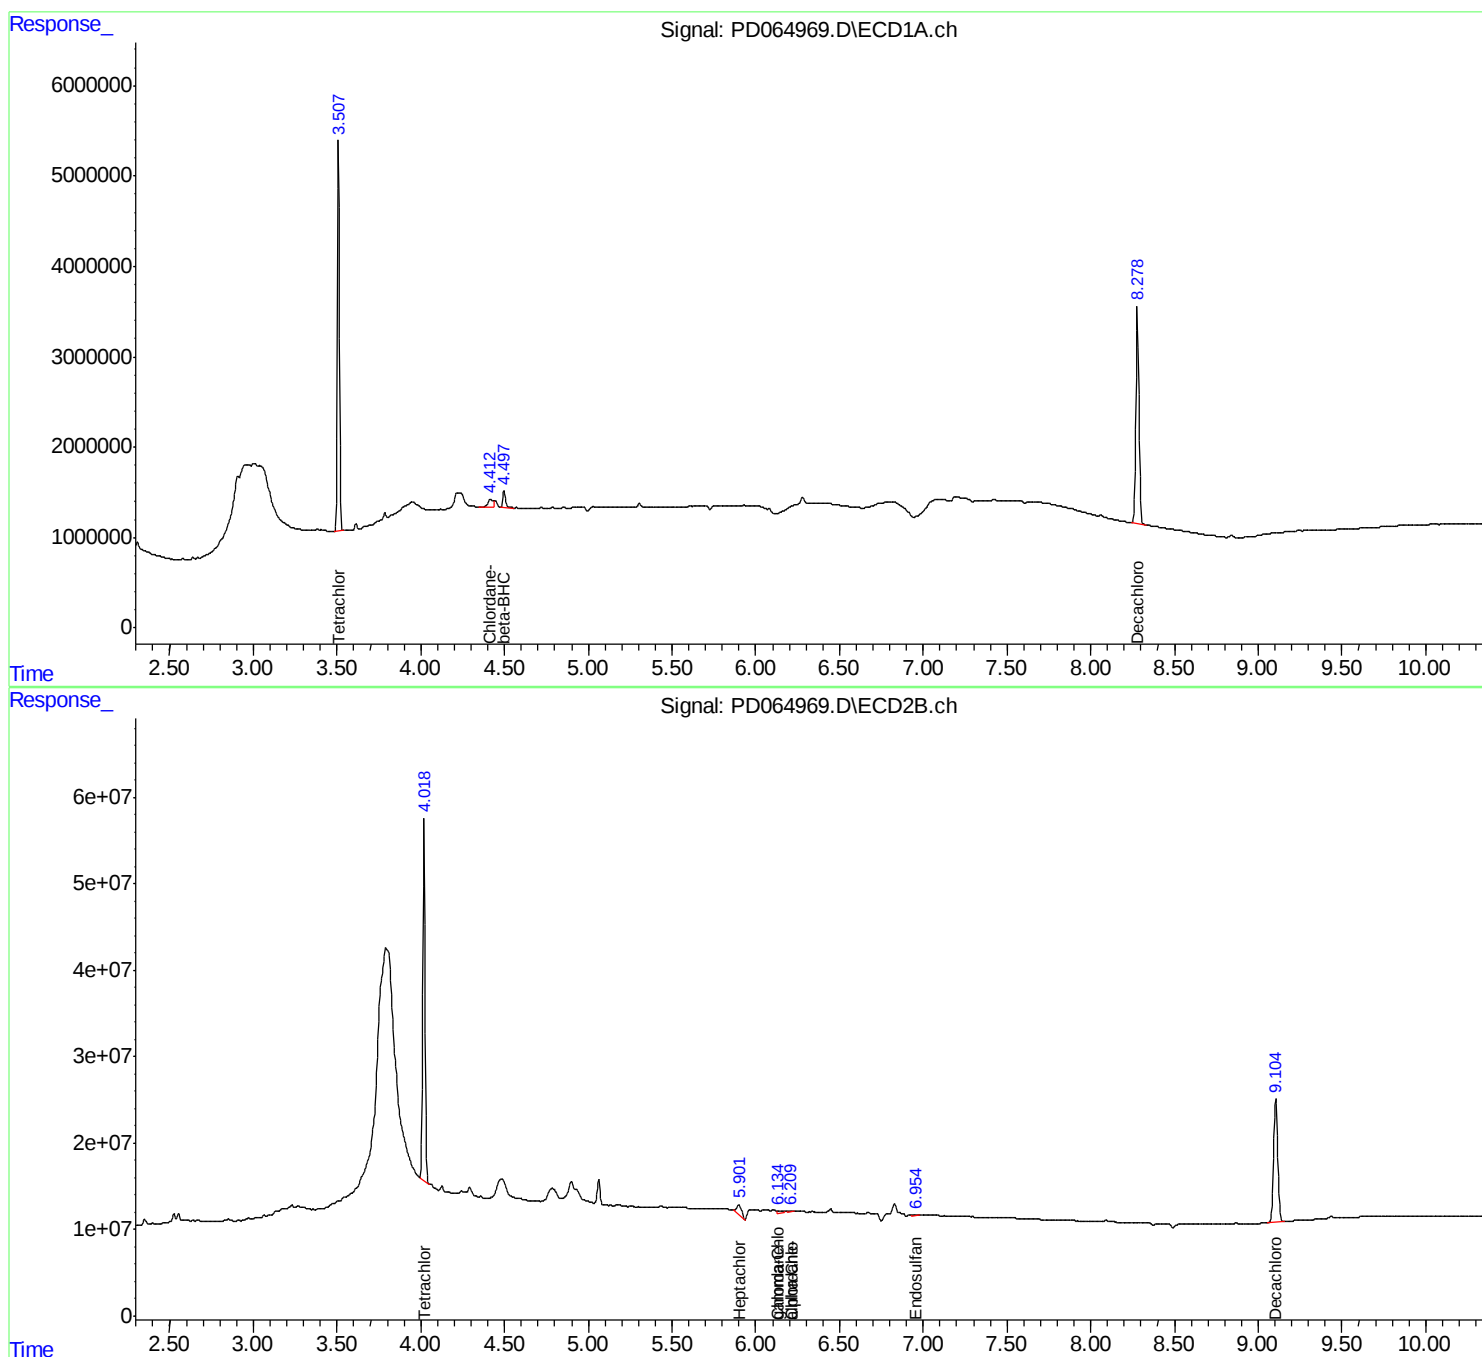


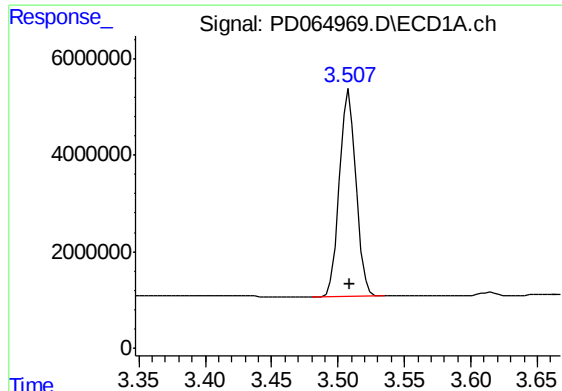

#1 Tetrachloro-m-xylene


R.T.: 3.508 min
Delta R.T.: 0.000 min
Response: 38014291
Conc: 19.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

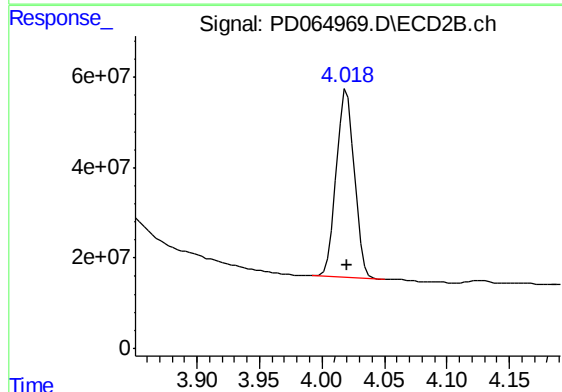


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 422389018
Conc: 20.80 ng/ml

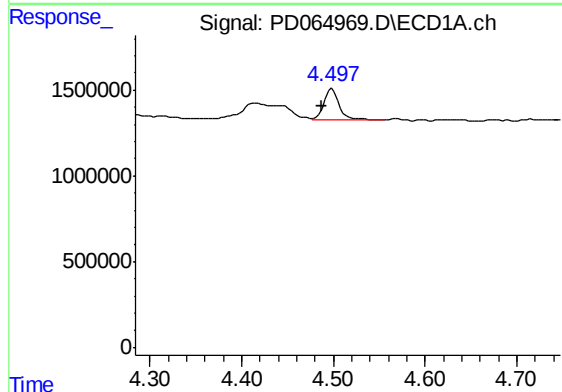


#6 beta-BHC

R.T.: 4.498 min
Delta R.T.: 0.011 min
Response: 2034612
Conc: 1.64 ng/ml

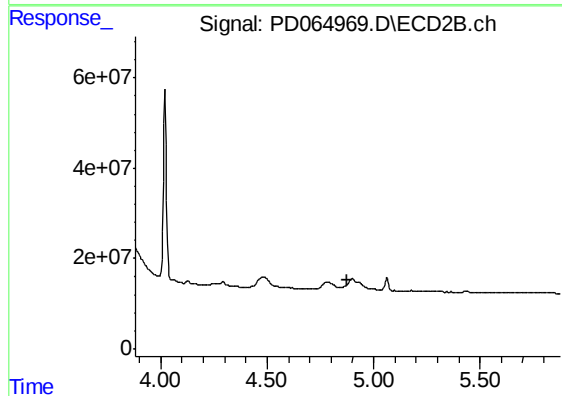

#6 beta-BHC


R.T.: 4.900 min
Delta R.T.: 0.021 min
Response: 20513317
Conc: N.D.

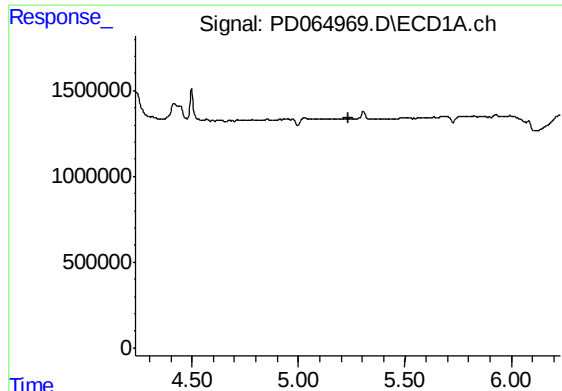

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.234 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

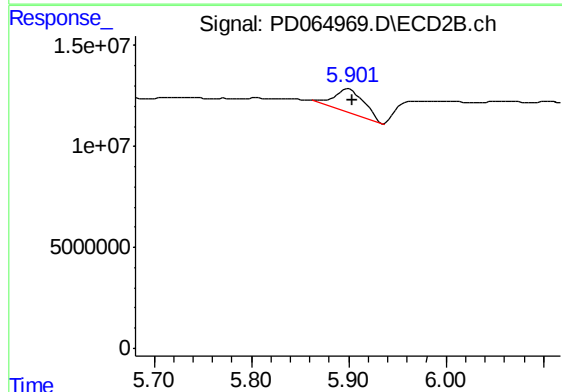


#8 Heptachlor epoxide

R.T.: 5.899 min
Delta R.T.: -0.004 min
Response: 24821851
Conc: 0.97 ng/ml

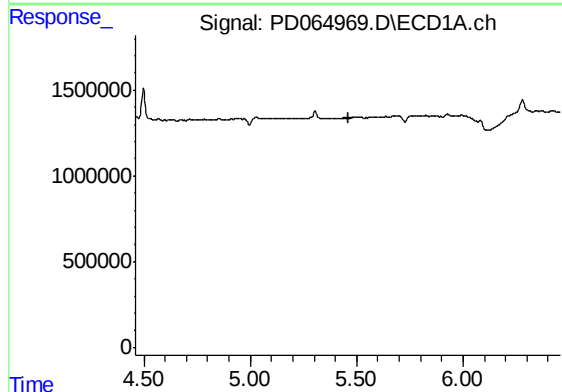


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.460 min
Response: 0
Conc: N.D.

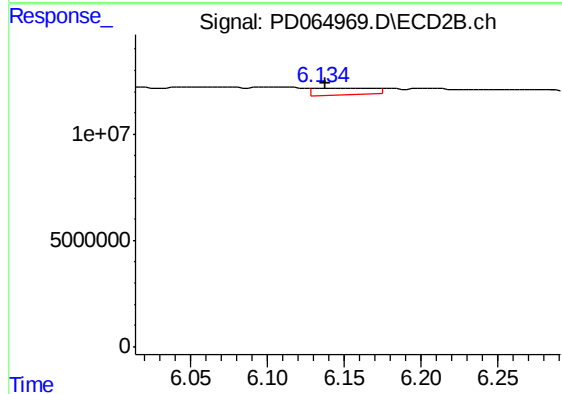

#10 gamma-Chlordane


R.T.: 6.136 min
Delta R.T.: -0.002 min
Response: 8710205
Conc: 0.33 ng/ml

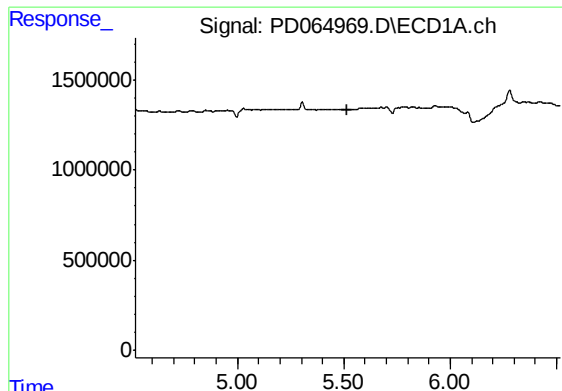

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.519 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

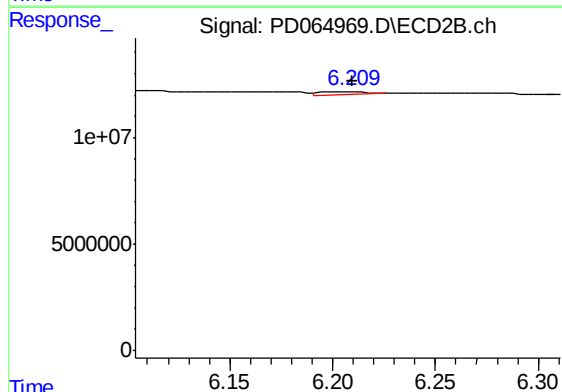


#11 alpha-Chlordane

R.T.: 6.210 min
Delta R.T.: 0.000 min
Response: 2022586
Conc: 0.08 ng/ml

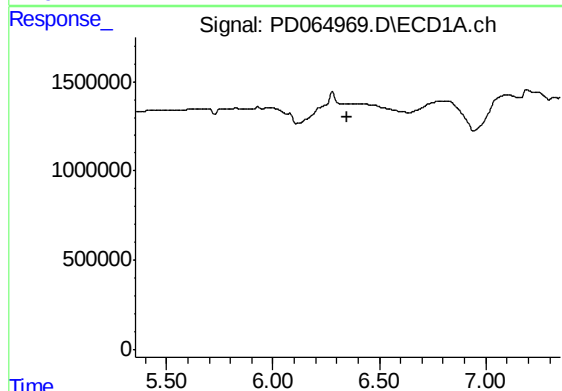


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.351 min
Response: 0
Conc: N.D.

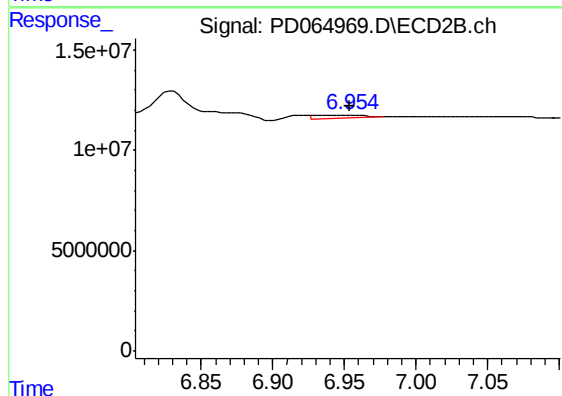

#15 Endosulfan II


R.T.: 6.955 min
Delta R.T.: 0.002 min
Response: 3386737
Conc: 0.18 ng/ml

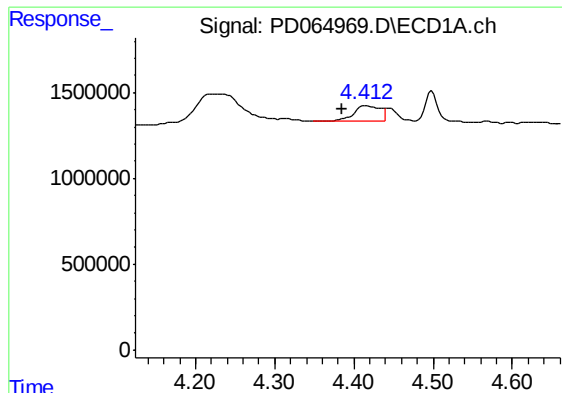

#23 Chlordane-1


R.T.: 4.414 min
Delta R.T.: 0.028 min
Response: 2067961
Conc: 28.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

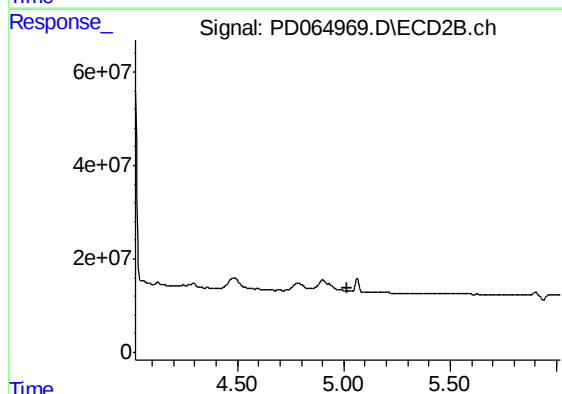


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.018 min
Response: 0
Conc: N.D.

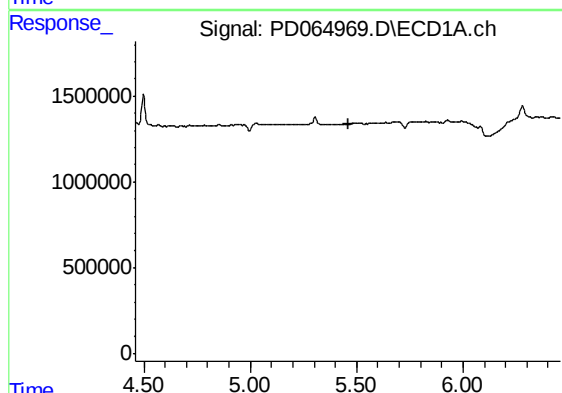


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.460 min
Response: 0
Conc: N.D.

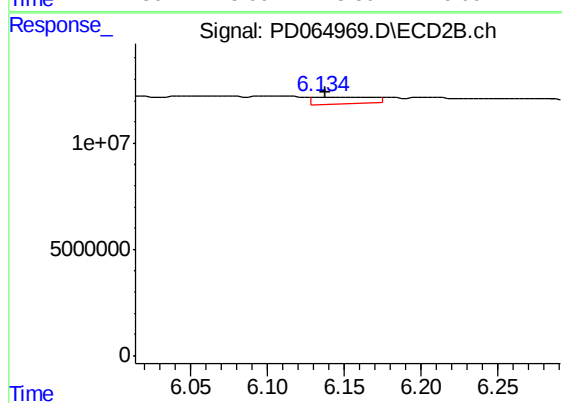

#25 Chlordane-3


R.T.: 6.136 min
Delta R.T.: -0.002 min
Response: 8710205
Conc: 2.60 ng/ml

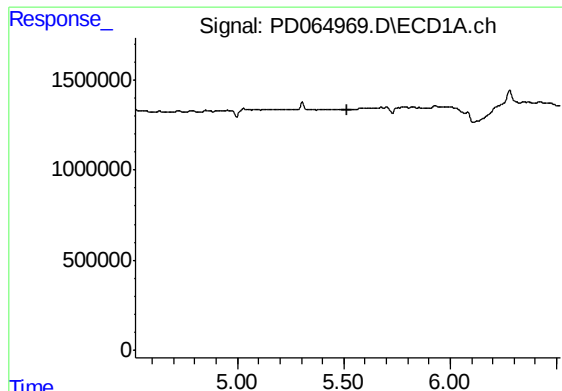

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.518 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

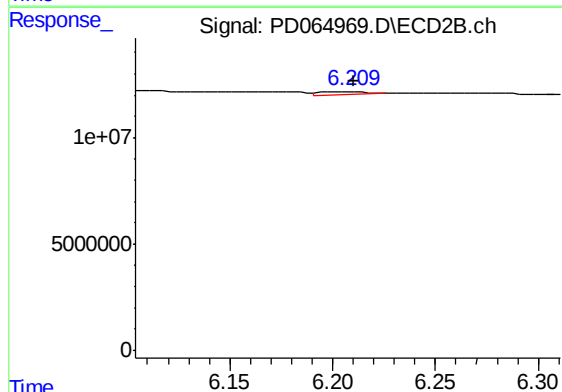


#26 Chlordane-4

R.T.: 6.210 min
Delta R.T.: 0.000 min
Response: 2022586
Conc: 0.52 ng/ml

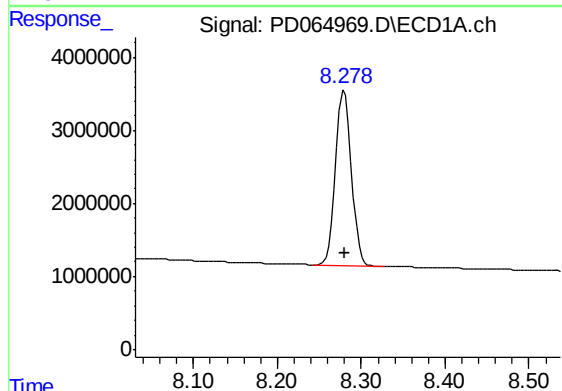

#28 Decachlorobiphenyl

R.T.: 8.280 min
Delta R.T.: 0.000 min
Response: 31633415
Conc: 12.87 ng/ml

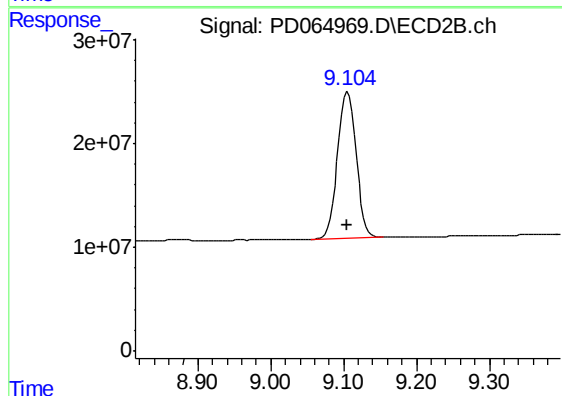

#28 Decachlorobiphenyl

R.T.: 9.106 min
Delta R.T.: 0.000 min
Response: 250117650
Conc: 22.50 ng/ml