

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081521\
 Data File : PL068991.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2021 11:20
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PTOXCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 23:13:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

4) MA	Heptachlor	6.154f	0.000	349754	0	0.595	N.D.	#
5) MB	Aldrin	0.000	7.583	0	105495	N.D.	0.087	#
6) B	beta-BHC	6.154	0.000	349754	0	1.241	N.D.	#
8) B	Heptachlo...	0.000	8.036	0	7543432	N.D.	6.525	#
14) MA	Endrin	8.081f	0.000	3819615	0	7.926	N.D.	#
15) B	Endosulfa...	0.000	9.218f	0	142233	N.D.	0.155	#
17) MA	4,4'-DDT	0.000	9.427	0	1243757	N.D.	1.314	#
22)	Mirex	0.000	10.568f	0	352990	N.D.	0.446	#
23)	Chlordane-1	0.000	6.973f	0	144855	N.D.	3.435	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081521\
Data File : PL068991.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2021 11:20
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PTOXCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 23:13:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

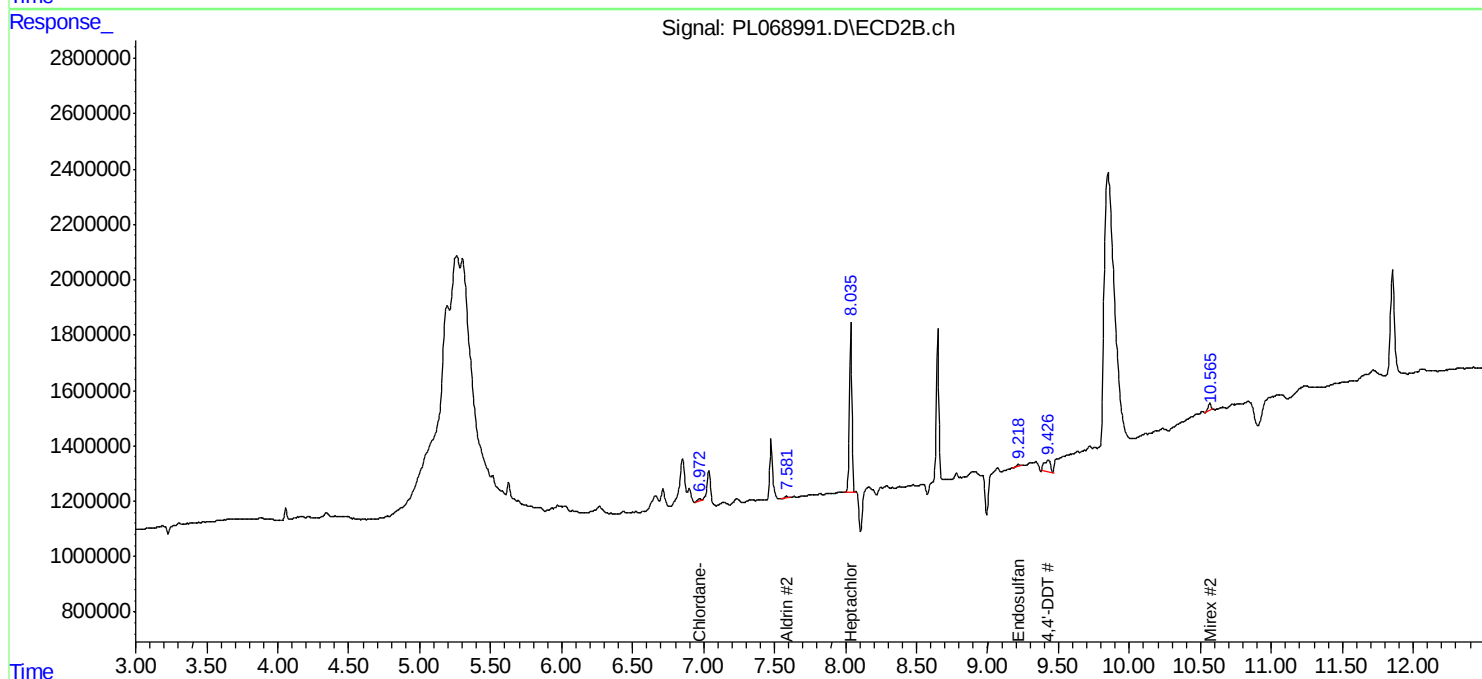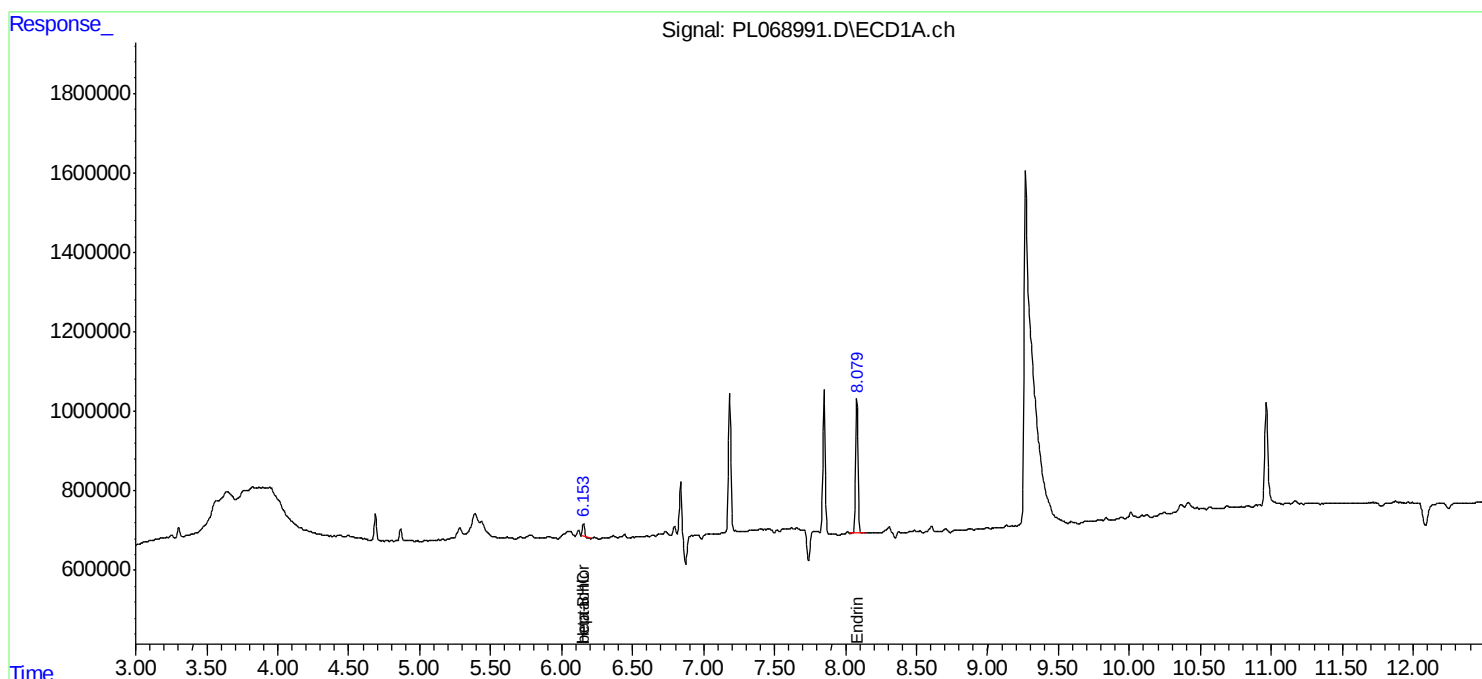


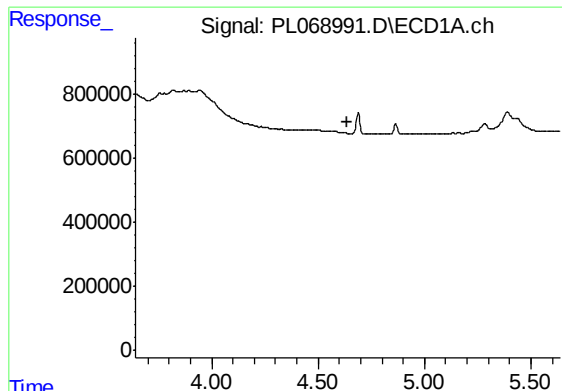

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.640 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PTOXCCC500

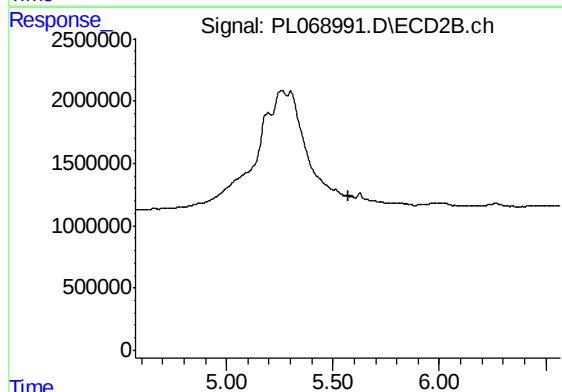


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.571 min
Response: 0
Conc: N.D.

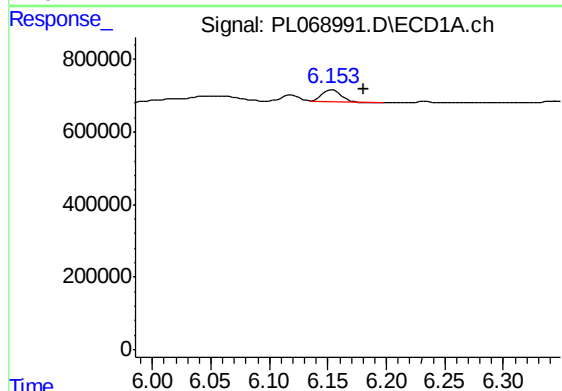


#4 Heptachlor

R.T.: 6.154 min
Delta R.T.: -0.026 min
Response: 349754
Conc: 0.60 ng/ml

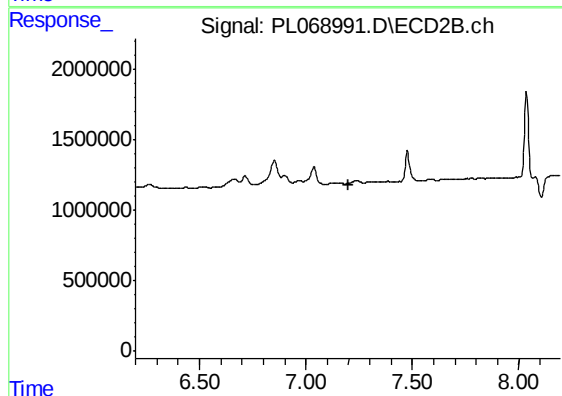

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 7.197 min
Response: 0
Conc: N.D.

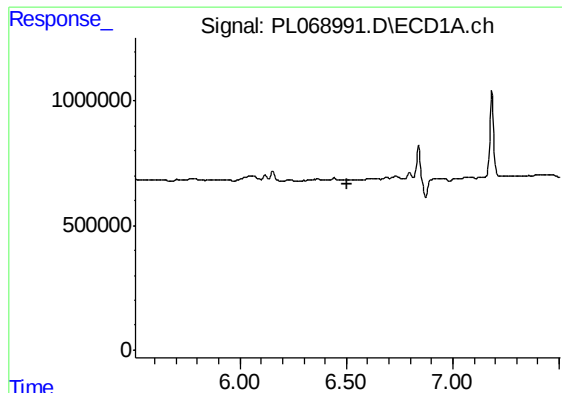

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 6.507 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PTOXCCC500

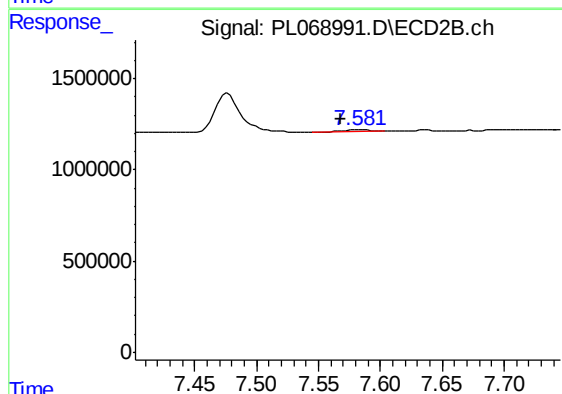


#5 Aldrin

R.T.: 7.583 min
Delta R.T.: 0.015 min
Response: 105495
Conc: 0.09 ng/ml

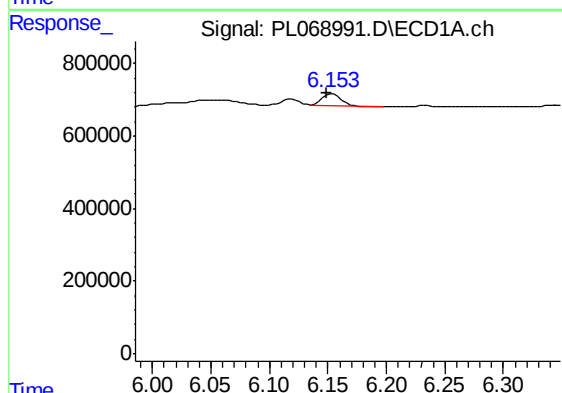


#6 beta-BHC

R.T.: 6.154 min
Delta R.T.: 0.006 min
Response: 349754
Conc: 1.24 ng/ml

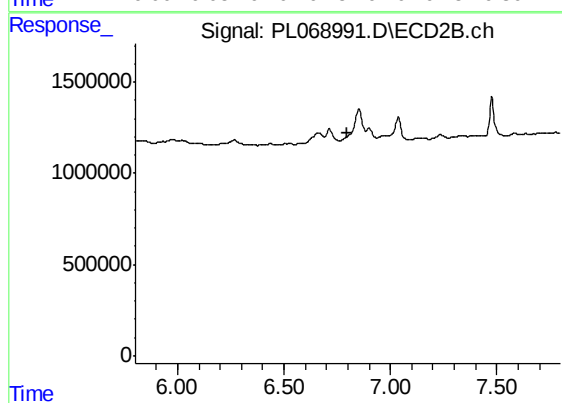

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.800 min
Response: 0
Conc: N.D.

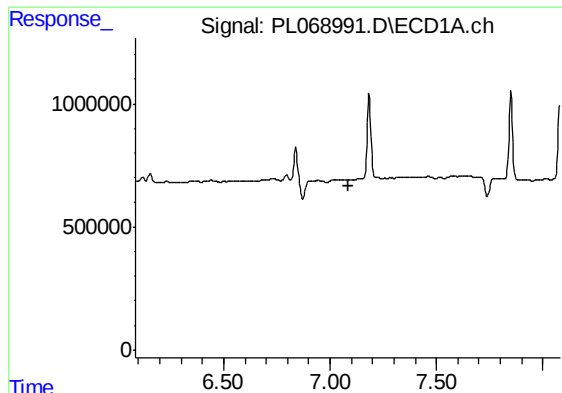

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 7.084 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PTOXCCC500

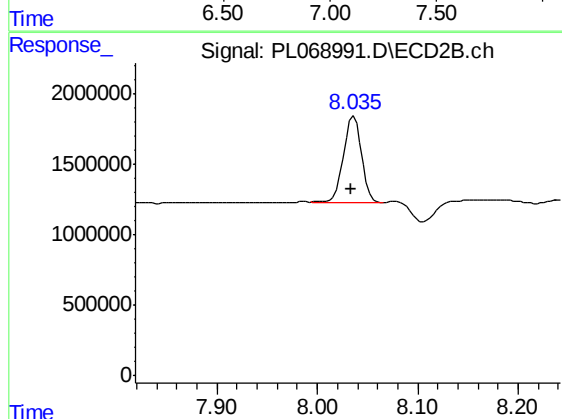


#8 Heptachlor epoxide

R.T.: 8.036 min
Delta R.T.: 0.002 min
Response: 7543432
Conc: 6.53 ng/ml

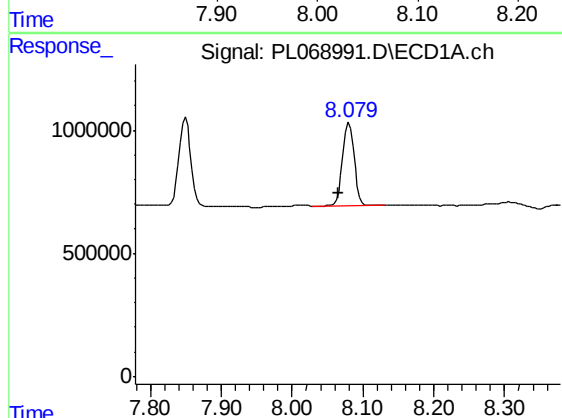


#14 Endrin

R.T.: 8.081 min
Delta R.T.: 0.016 min
Response: 3819615
Conc: 7.93 ng/ml

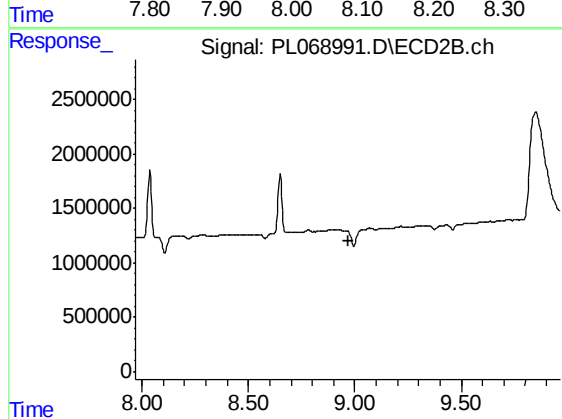

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 8.968 min
Response: 0
Conc: N.D.

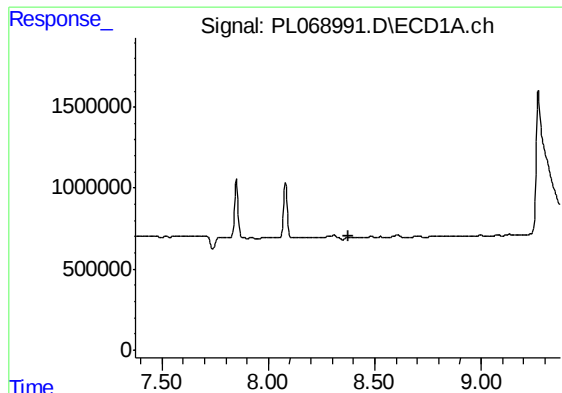

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PTOXCCC500

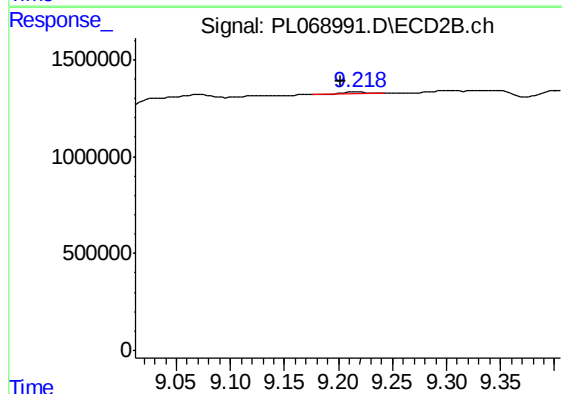


#15 Endosulfan II

R.T.: 9.218 min
Delta R.T.: 0.017 min
Response: 142233
Conc: 0.16 ng/ml

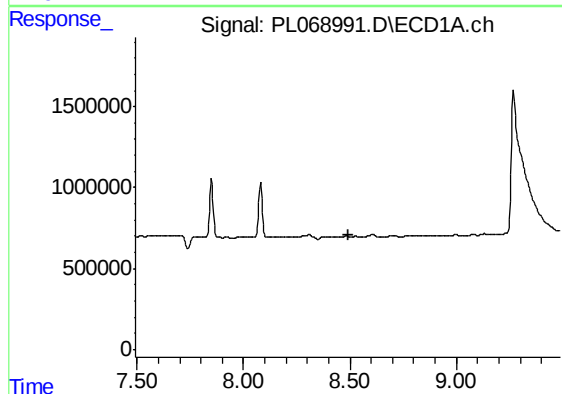


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 8.492 min
Response: 0
Conc: N.D.

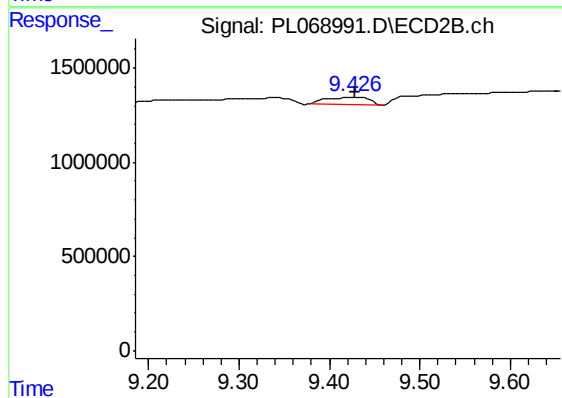

#17 4,4'-DDT


R.T.: 9.427 min
Delta R.T.: -0.001 min
Response: 1243757
Conc: 1.31 ng/ml

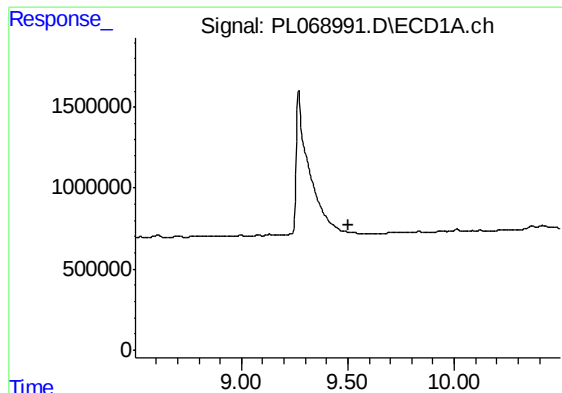

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 9.502 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PTOXCCC500

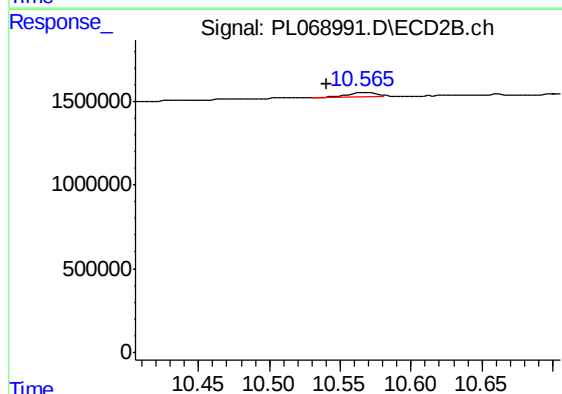


#22 Mirex

R.T.: 10.568 min
Delta R.T.: 0.028 min
Response: 352990
Conc: 0.45 ng/ml

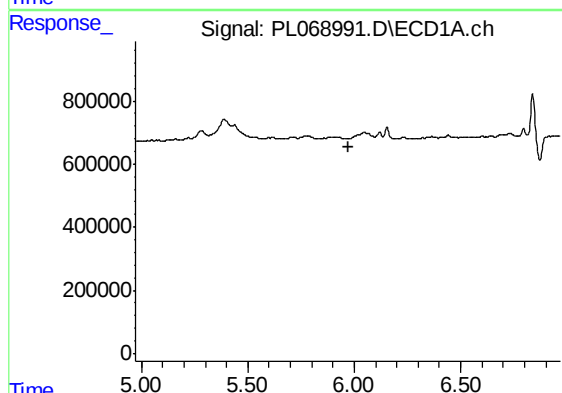


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.971 min
Response: 0
Conc: N.D.

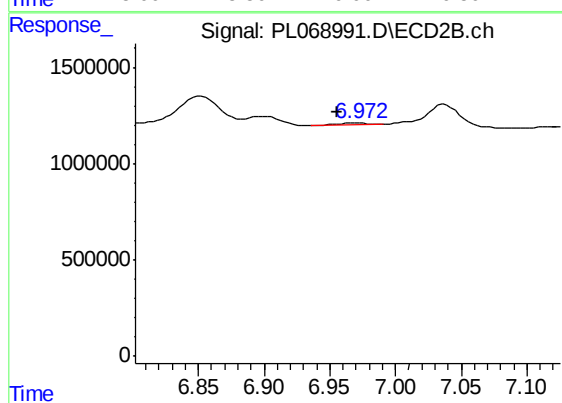

#23 Chlordane-1


R.T.: 6.973 min
Delta R.T.: 0.017 min
Response: 144855
Conc: 3.44 ng/ml

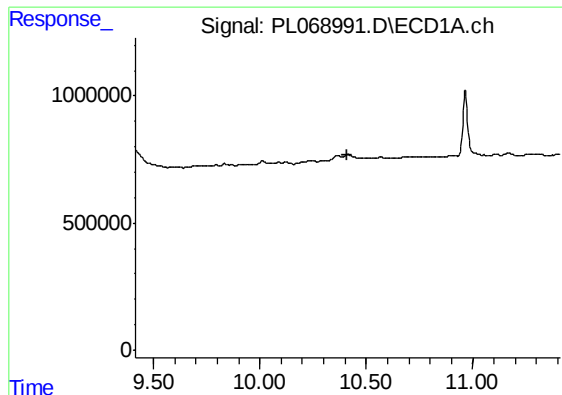

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.414 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PTOXCCC500

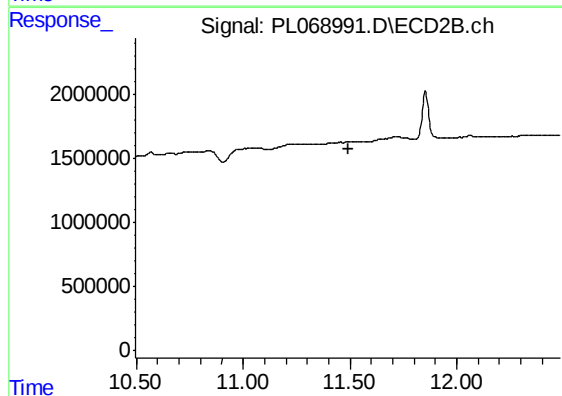

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.495 min
Response: 0
Conc: N.D.