

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081521\
 Data File : PL069000.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2021 14:41
 Operator : AR\AJ
 Sample : M3404-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP3-1-6FT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 23:18:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.636	5.568	9324983	23942539	22.544	23.581
28)	SA Decachlor...	10.404	11.488	11308717	19125893	19.678	19.712
Target Compounds							
4)	MA Heptachlor	6.207f	0.000	429183	0	0.731	N.D. #
8)	B Heptachlo...	0.000	8.030	0	618111	N.D.	0.535 #
12)	B 4,4'-DDE	0.000	8.566	0	211856	N.D.	0.200 #
14)	MA Endrin	0.000	8.963	0	233409	N.D.	0.257 #
15)	B Endosulfa...	0.000	9.217f	0	15634	N.D.	0.017 #
23)	Chlordane-1	0.000	6.976f	0	150146	N.D.	3.561 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081521\
Data File : PL069000.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2021 14:41
Operator : AR\AJ
Sample : M3404-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP3-1-6FT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 23:18:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

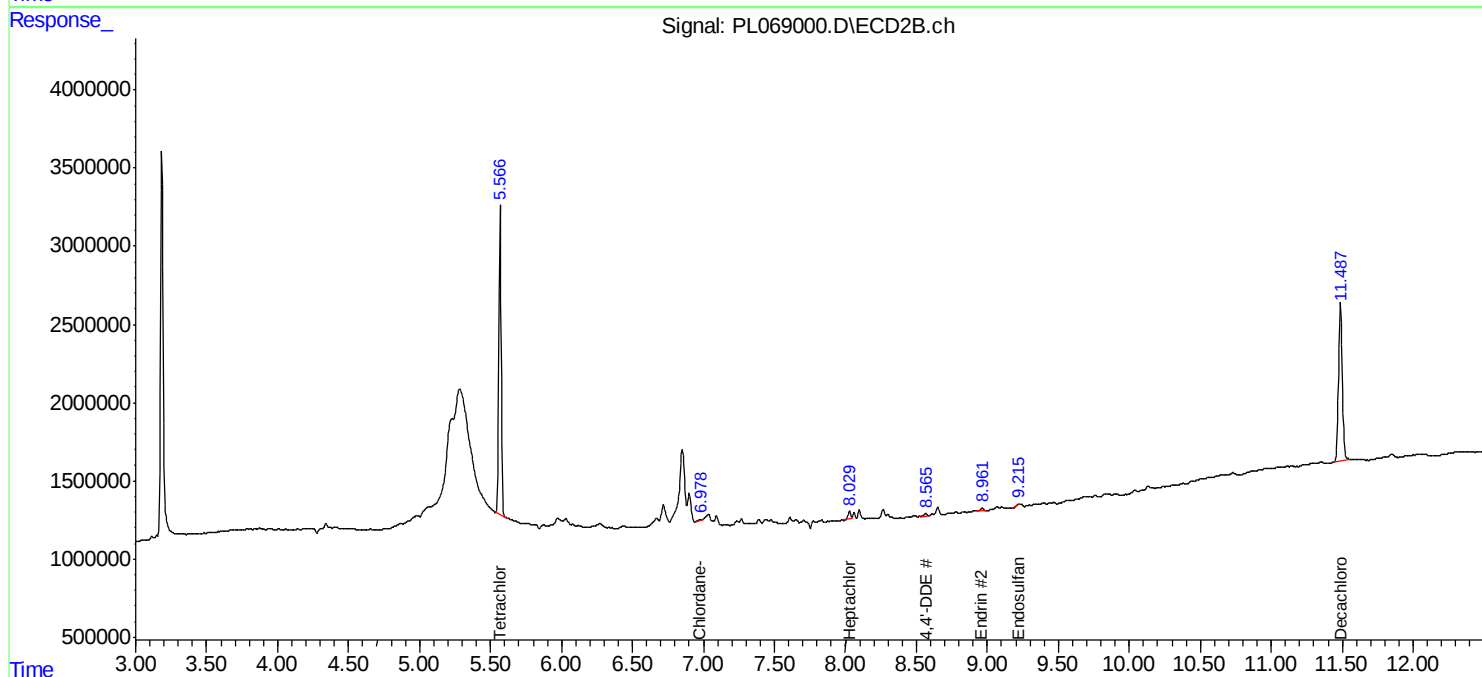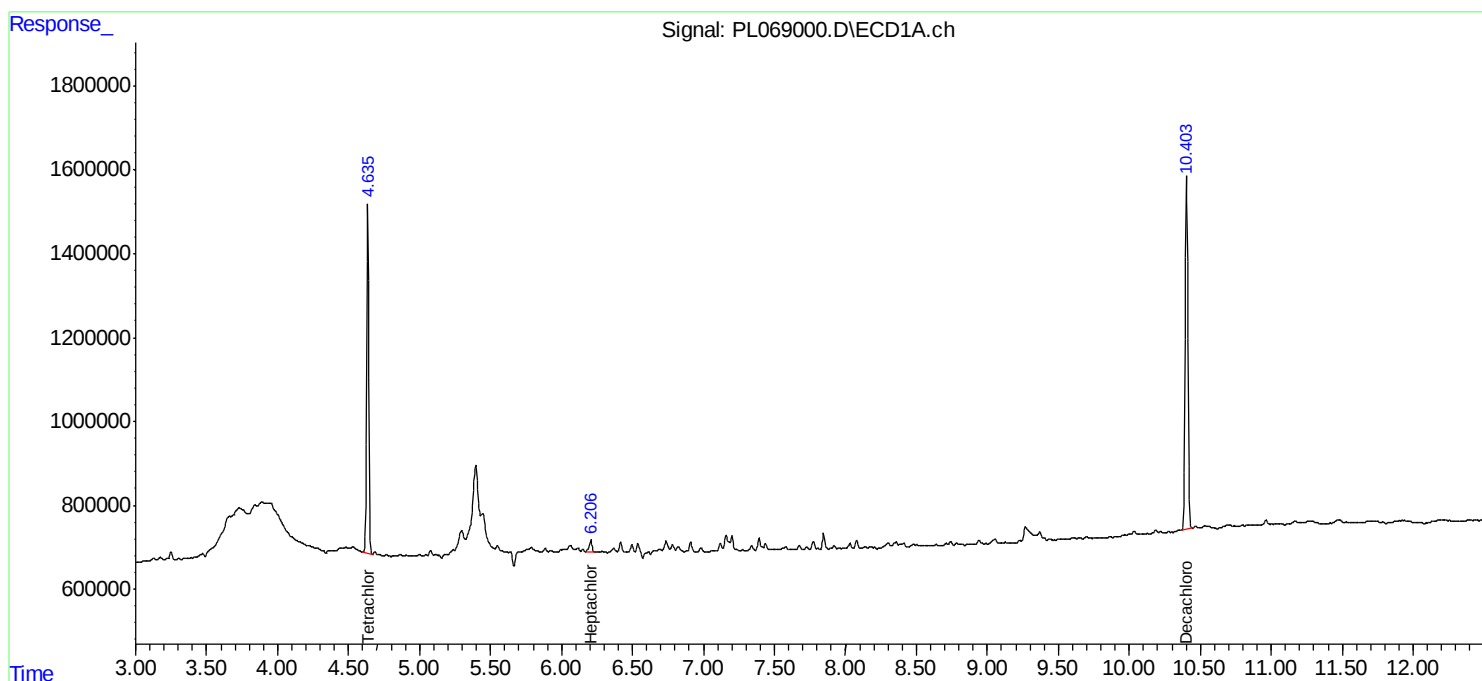


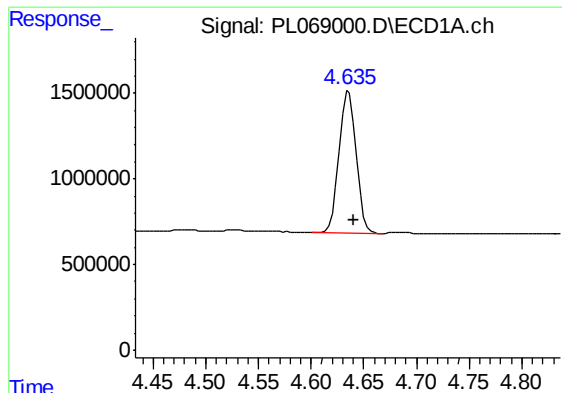

#1 Tetrachloro-m-xylene


R.T.: 4.636 min
Delta R.T.: -0.004 min
Response: 9324983
Conc: 22.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP3-1-6FT

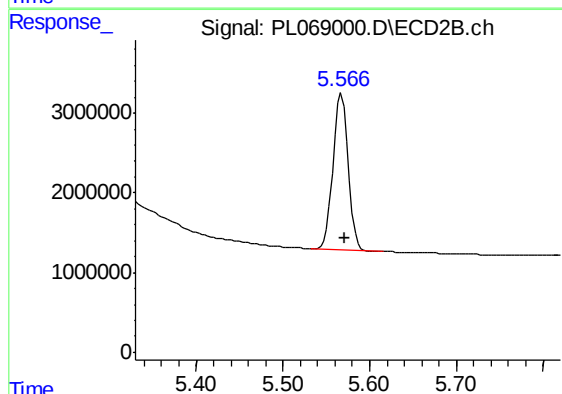


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 23942539
Conc: 23.58 ng/ml

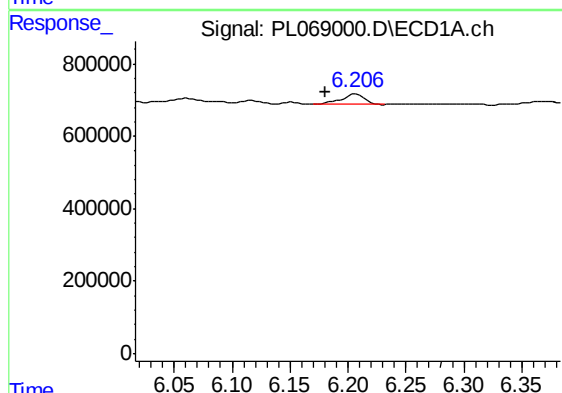


#4 Heptachlor

R.T.: 6.207 min
Delta R.T.: 0.027 min
Response: 429183
Conc: 0.73 ng/ml

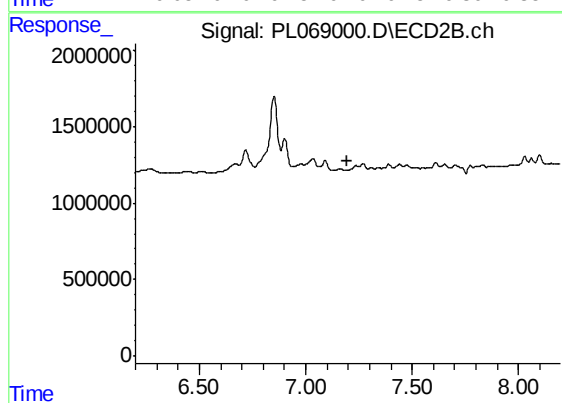

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 7.197 min
Response: 0
Conc: N.D.

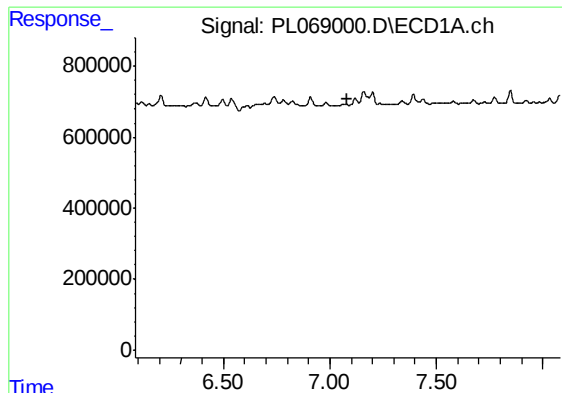

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 7.084 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP3-1-6FT

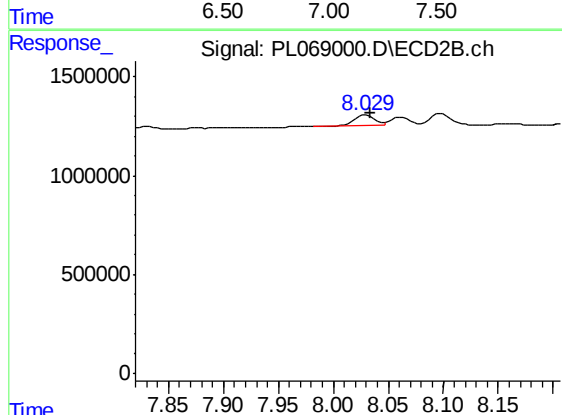


#8 Heptachlor epoxide

R.T.: 8.030 min
Delta R.T.: -0.004 min
Response: 618111
Conc: 0.53 ng/ml

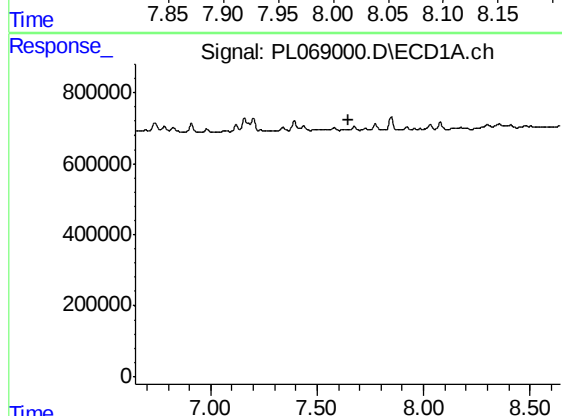


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 7.645 min
Response: 0
Conc: N.D.

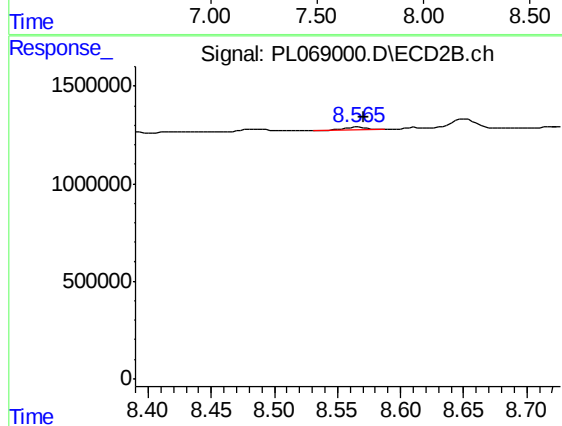

#12 4,4'-DDE


R.T.: 8.566 min
Delta R.T.: -0.005 min
Response: 211856
Conc: 0.20 ng/ml

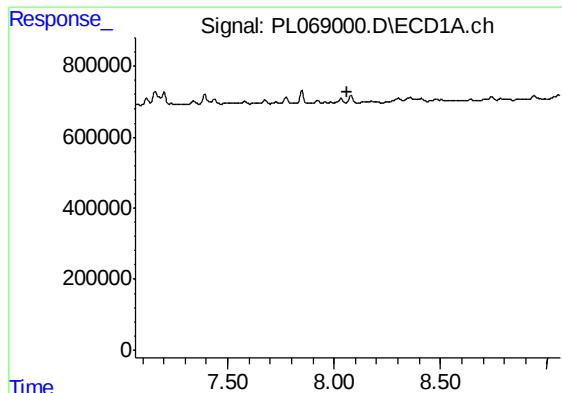

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 8.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP3-1-6FT

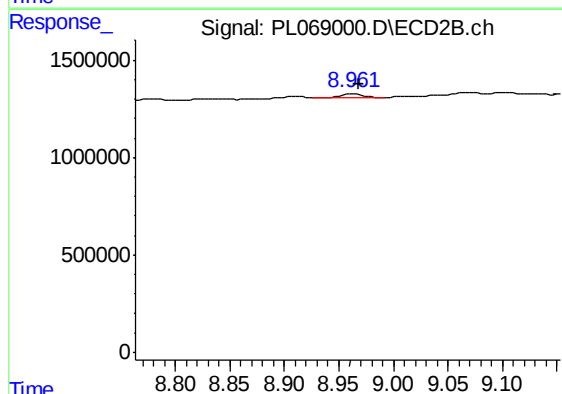


#14 Endrin

R.T.: 8.963 min
Delta R.T.: -0.005 min
Response: 233409
Conc: 0.26 ng/ml

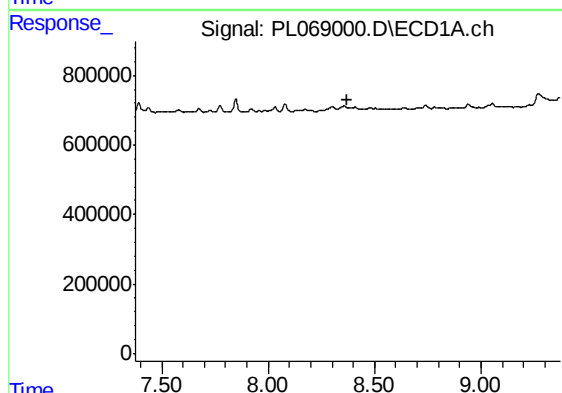


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

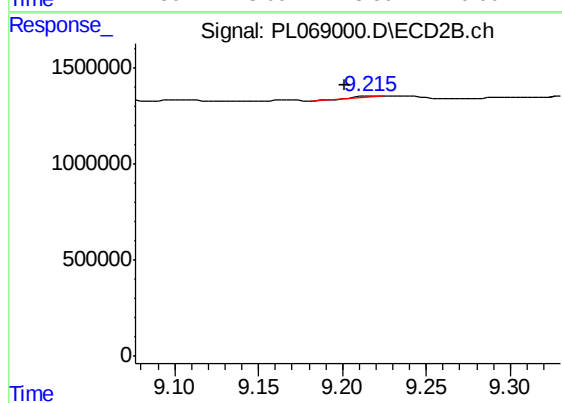

#15 Endosulfan II


R.T.: 9.217 min
Delta R.T.: 0.015 min
Response: 15634
Conc: 0.02 ng/ml

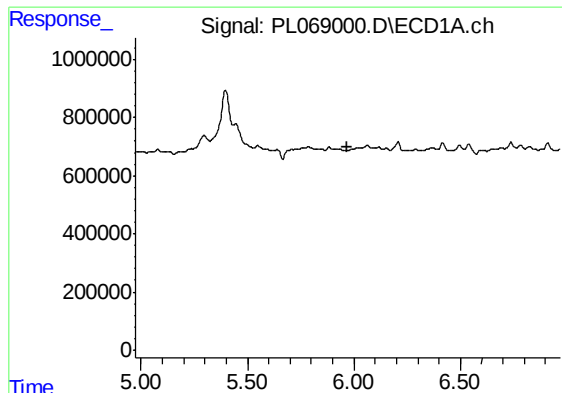

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.971 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP3-1-6FT

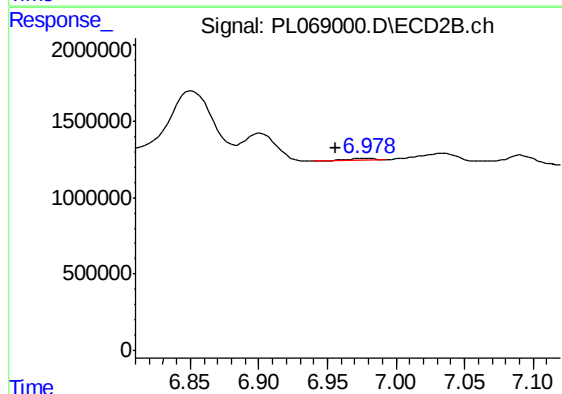


#23 Chlordane-1

R.T.: 6.976 min
Delta R.T.: 0.020 min
Response: 150146
Conc: 3.56 ng/ml

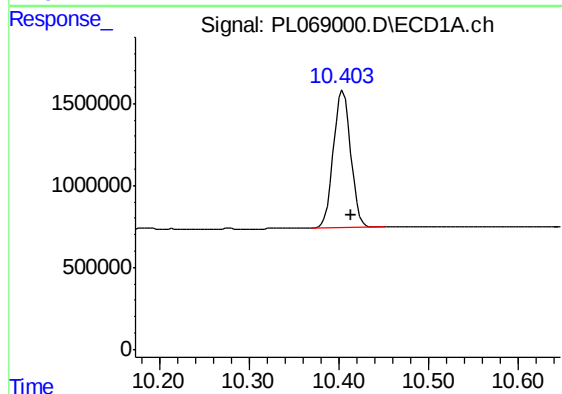

#28 Decachlorobiphenyl

R.T.: 10.404 min
Delta R.T.: -0.009 min
Response: 11308717
Conc: 19.68 ng/ml

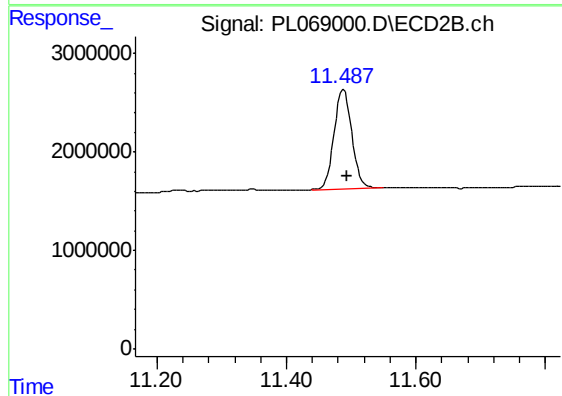

#28 Decachlorobiphenyl

R.T.: 11.488 min
Delta R.T.: -0.006 min
Response: 19125893
Conc: 19.71 ng/ml