

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081521\
 Data File : PL069001.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2021 14:57
 Operator : AR\AJ
 Sample : PB138438BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB138438BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 23:18:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.636	5.568	8539535	22126266	20.645	21.792
28)	SA Decachlor...	10.405	11.489	12263755	20770546	21.340	21.408
Target Compounds							
15)	B Endosulfa...	0.000	9.213	0	1170955	N.D.	1.277 #
23)	Chlordane-1	0.000	6.979f	0	111398	N.D.	2.642 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081521\
Data File : PL069001.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2021 14:57
Operator : AR\AJ
Sample : PB138438BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB138438BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 23:18:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

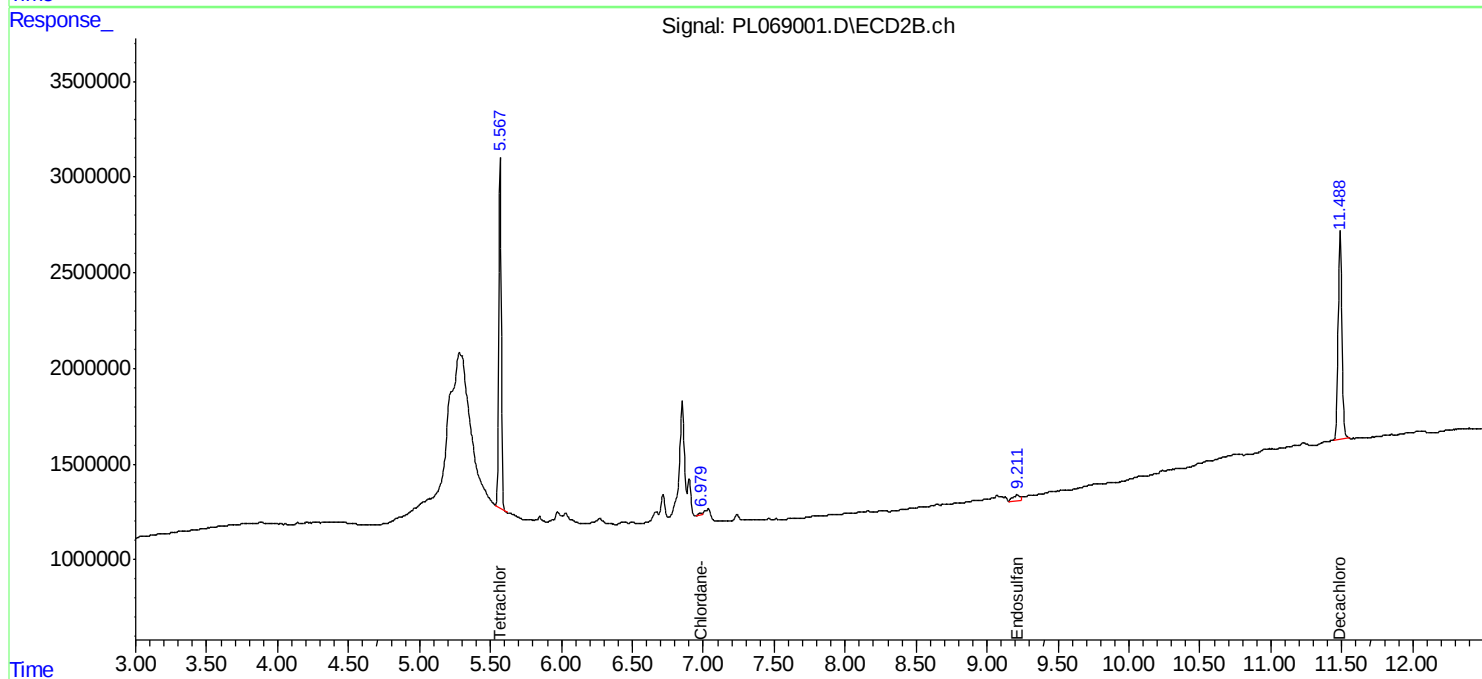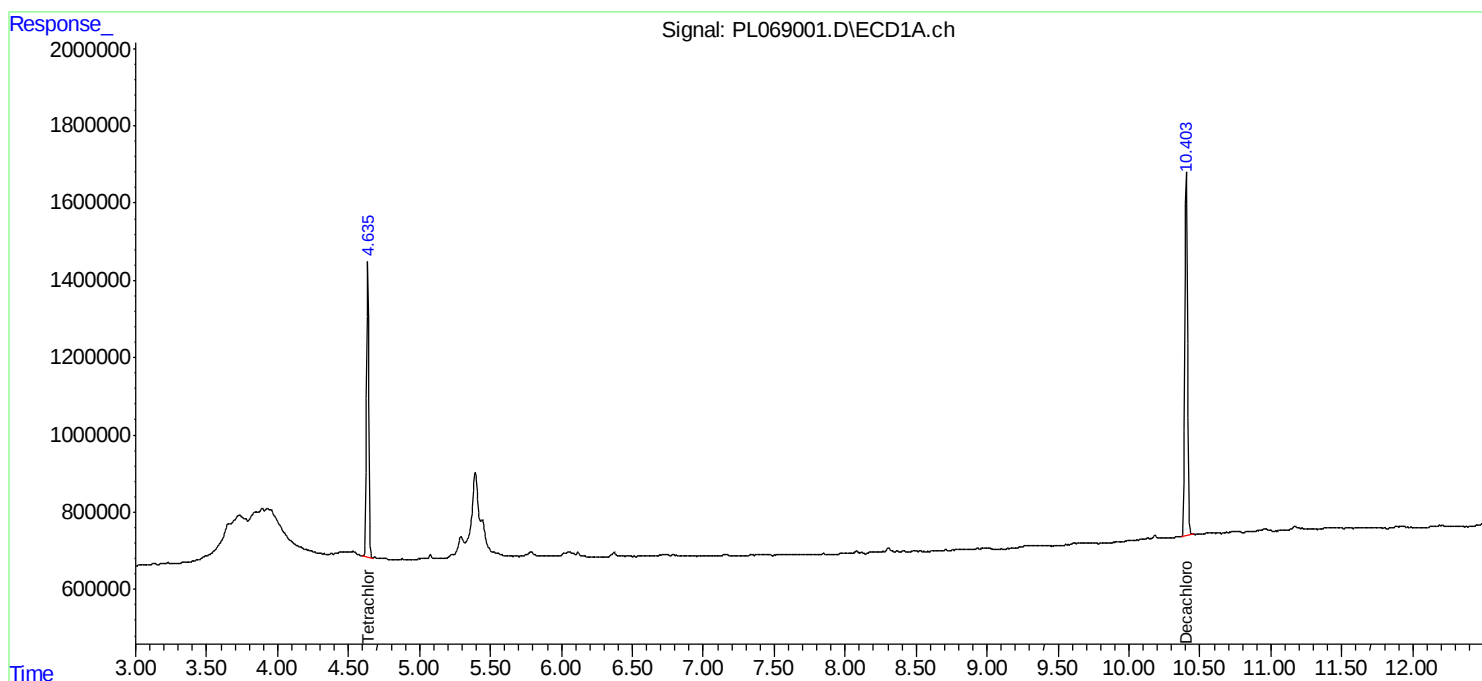


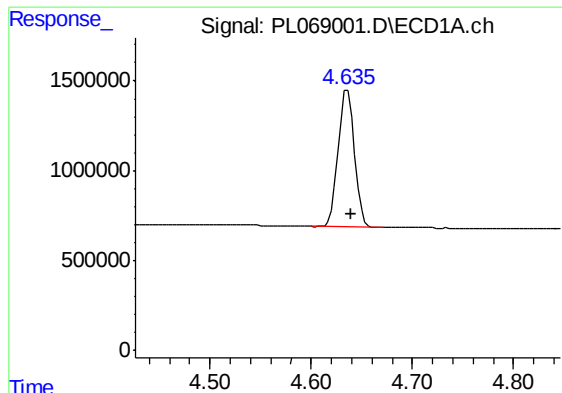

#1 Tetrachloro-m-xylene


R.T.: 4.636 min
Delta R.T.: -0.004 min
Response: 8539535
Conc: 20.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB138438BL

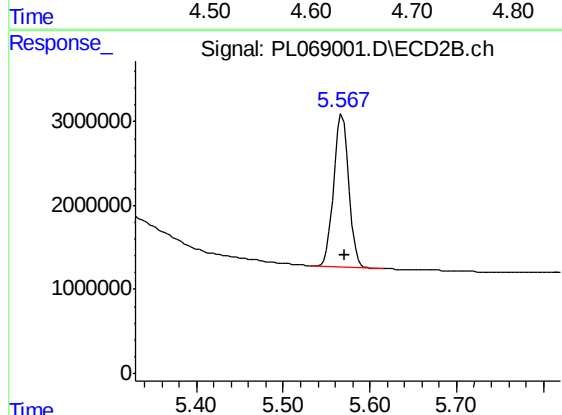


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 22126266
Conc: 21.79 ng/ml

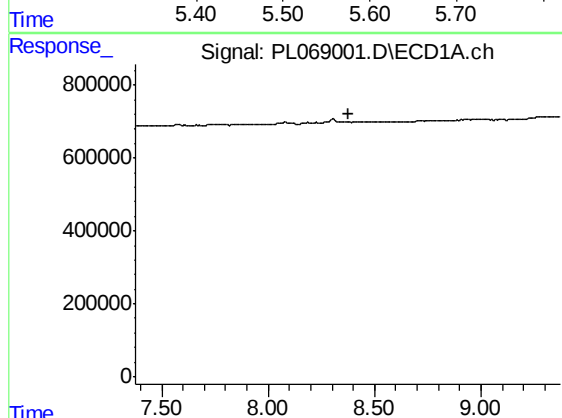


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

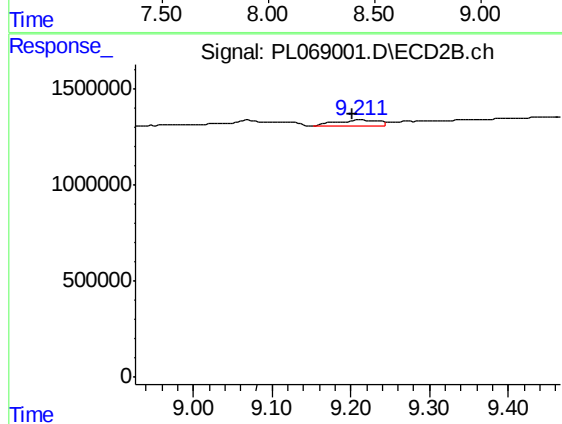

#15 Endosulfan II


R.T.: 9.213 min
Delta R.T.: 0.011 min
Response: 1170955
Conc: 1.28 ng/ml

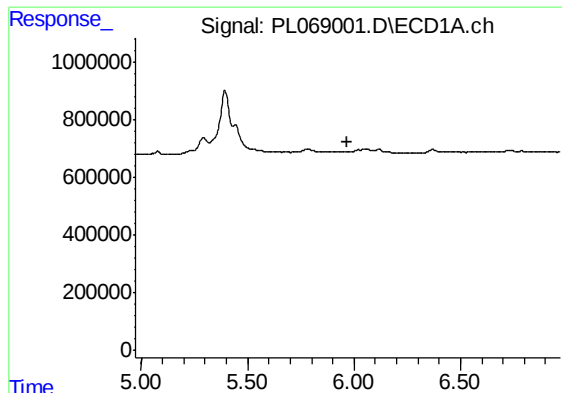

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.971 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138438BL

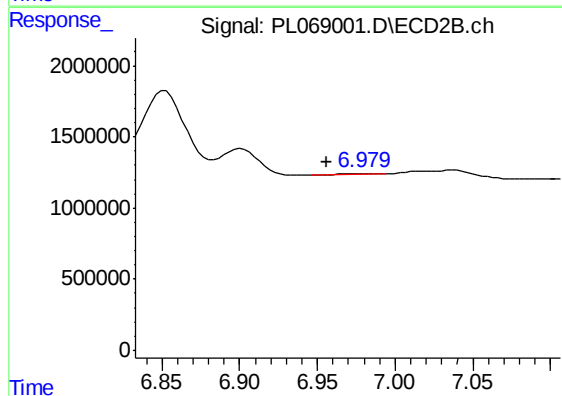


#23 Chlordane-1

R.T.: 6.979 min
Delta R.T.: 0.024 min
Response: 111398
Conc: 2.64 ng/ml

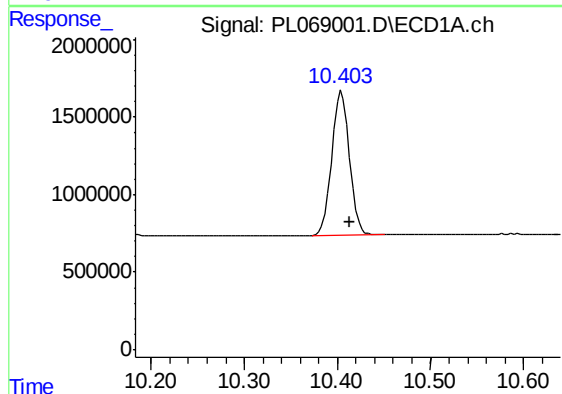

#28 Decachlorobiphenyl

R.T.: 10.405 min
Delta R.T.: -0.009 min
Response: 12263755
Conc: 21.34 ng/ml

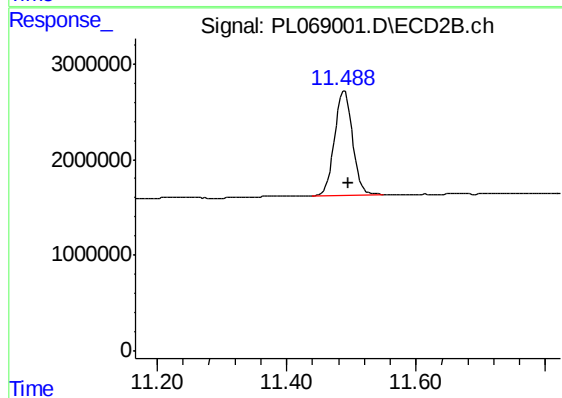

#28 Decachlorobiphenyl

R.T.: 11.489 min
Delta R.T.: -0.005 min
Response: 20770546
Conc: 21.41 ng/ml