

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081521\
 Data File : PL069009.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2021 17:16
 Operator : AR\AJ
 Sample : M3419-15
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SWCS-08-0205

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 23:22:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	4.636	5.568	8703691	23016803	21.042	22.669
28) SA	Decachlor...	10.404	11.488	10807719	19979752	18.806	20.593
Target Compounds							
8) B	Heptachlo...	0.000	8.059f	0	306295	N.D.	0.265 #
9) A	Endosulfan I	0.000	8.462f	0	814933	N.D.	0.773 #
15) B	Endosulfa...	0.000	9.216	0	87478	N.D.	0.095 #
23)	Chlordane-1	0.000	6.980f	0	91396	N.D.	2.167 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081521\
Data File : PL069009.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2021 17:16
Operator : AR\AJ
Sample : M3419-15
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SWCS-08-0205

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 23:22:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

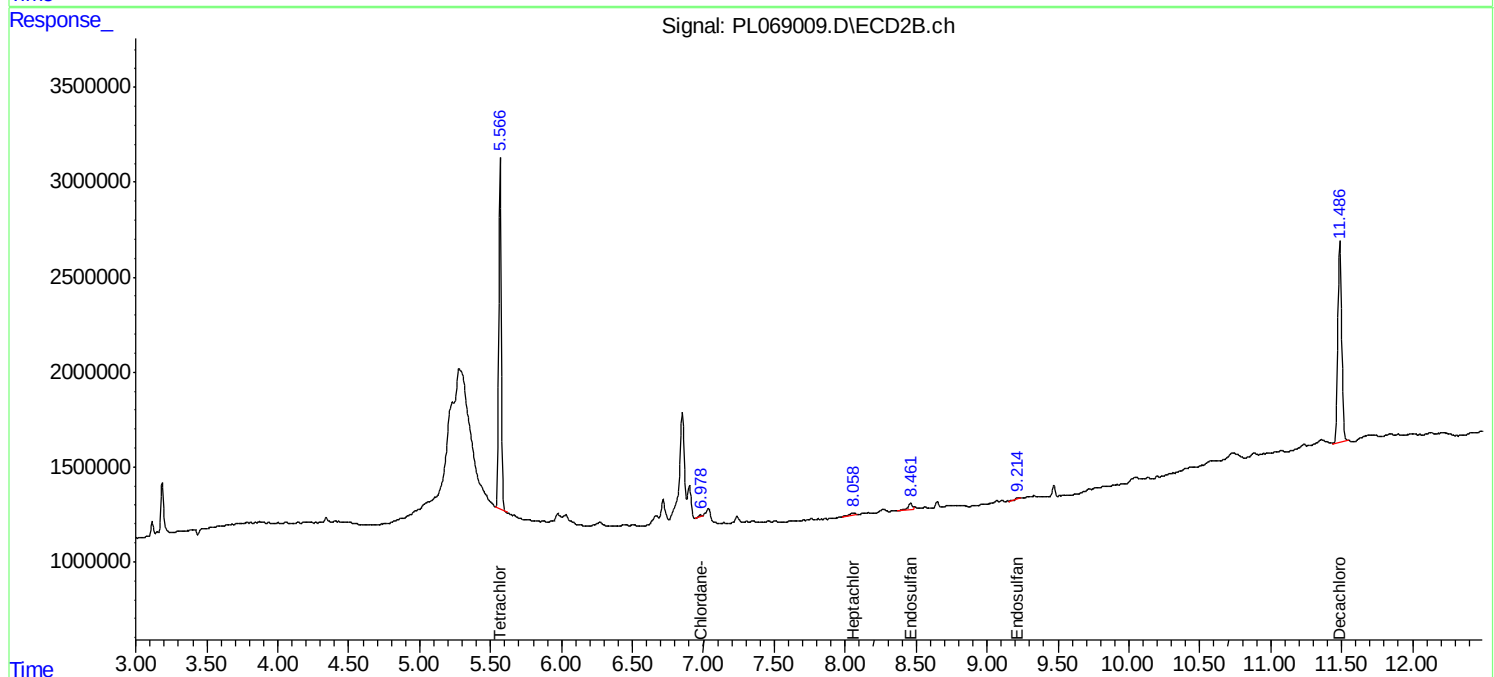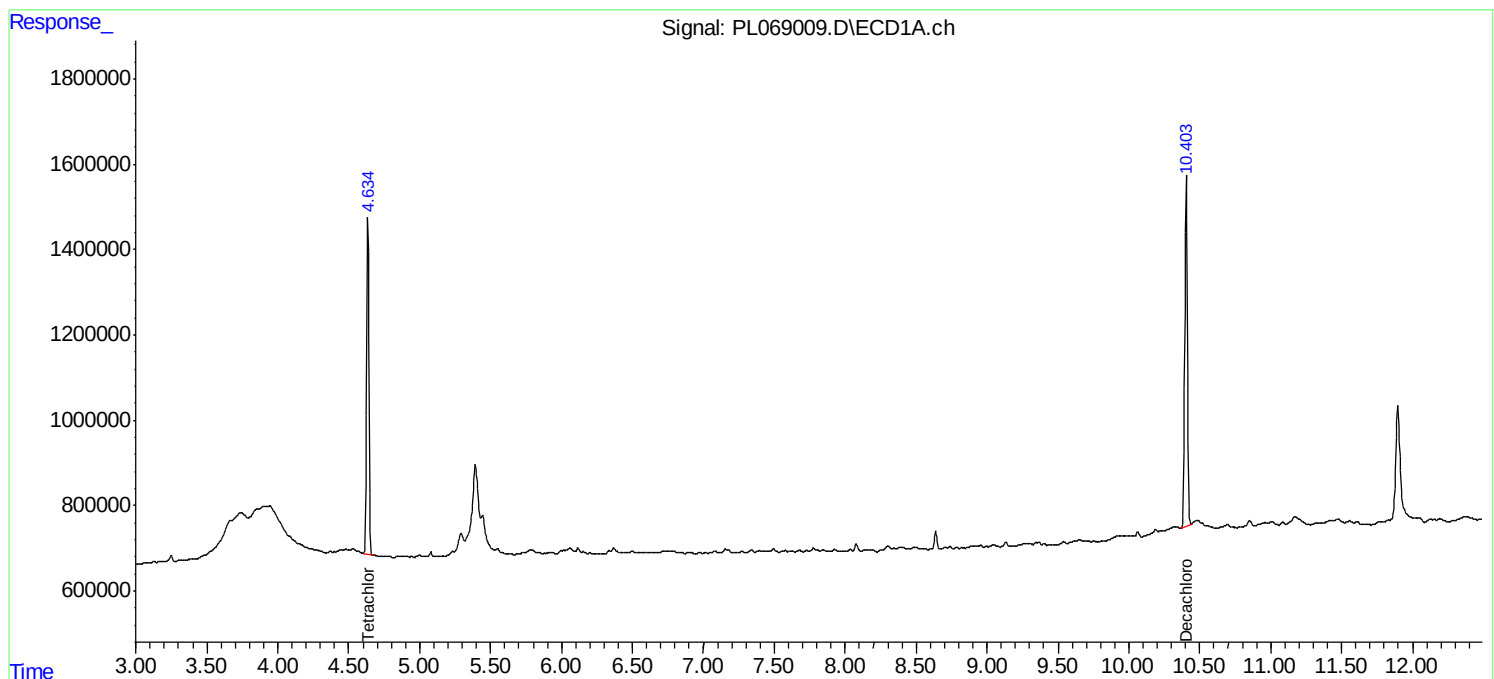


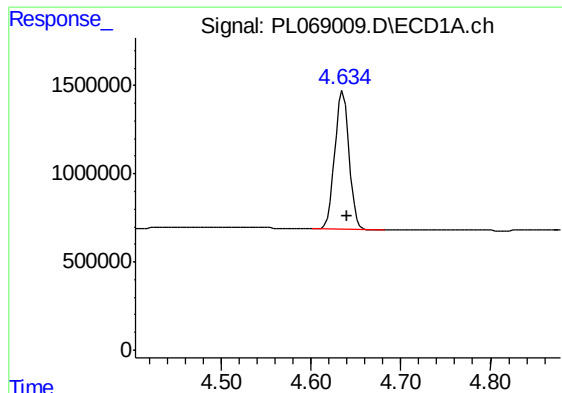

#1 Tetrachloro-m-xylene


R.T.: 4.636 min
Delta R.T.: -0.004 min
Response: 8703691
Conc: 21.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
SWCS-08-0205

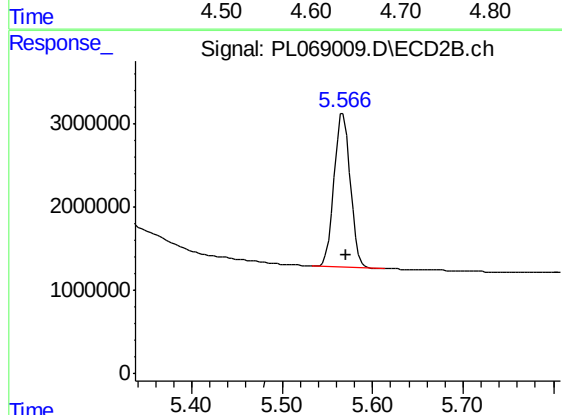


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 23016803
Conc: 22.67 ng/ml

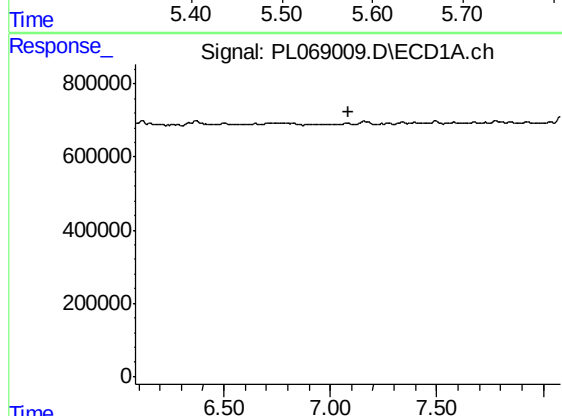


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.084 min
Response: 0
Conc: N.D.

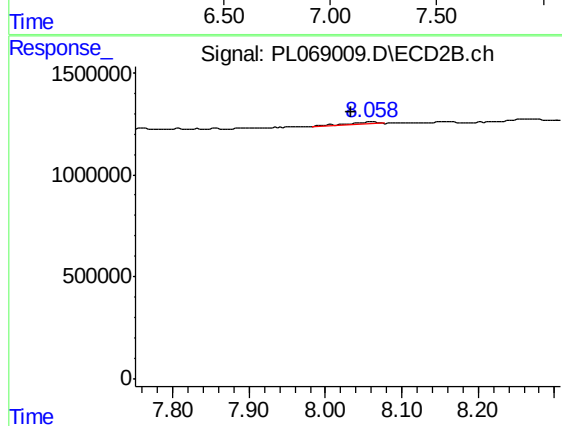

#8 Heptachlor epoxide


R.T.: 8.059 min
Delta R.T.: 0.025 min
Response: 306295
Conc: 0.26 ng/ml

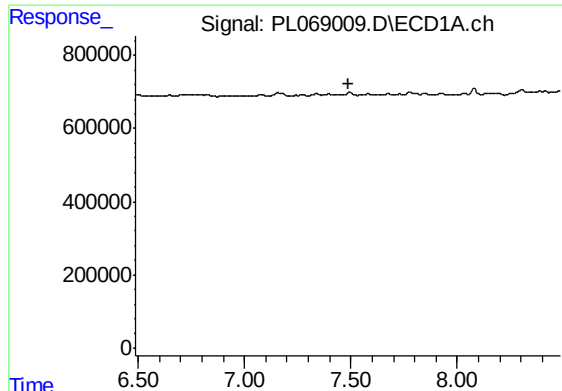

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 7.487 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SWCS-08-0205

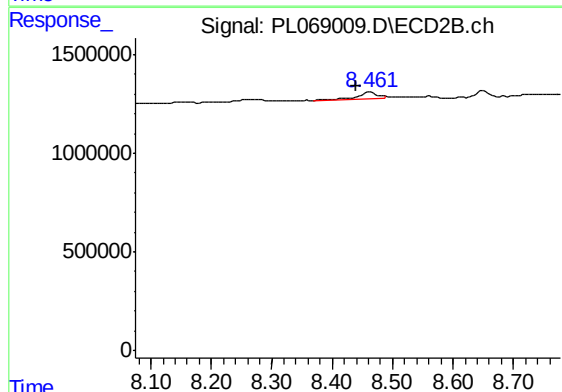


#9 Endosulfan I

R.T.: 8.462 min
Delta R.T.: 0.022 min
Response: 814933
Conc: 0.77 ng/ml

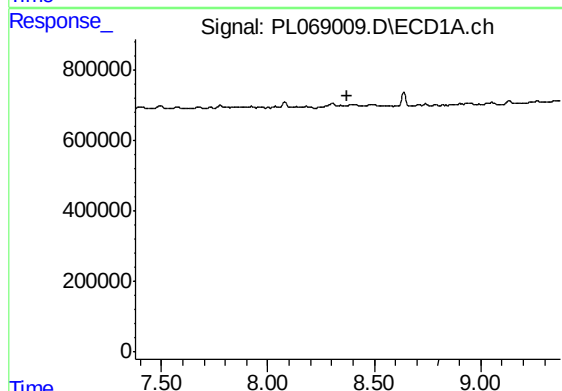


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

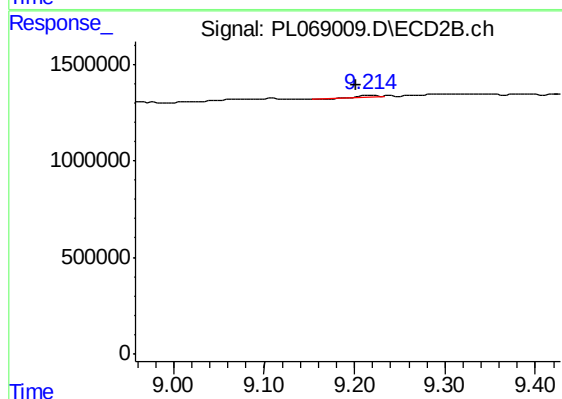

#15 Endosulfan II


R.T.: 9.216 min
Delta R.T.: 0.014 min
Response: 87478
Conc: 0.10 ng/ml

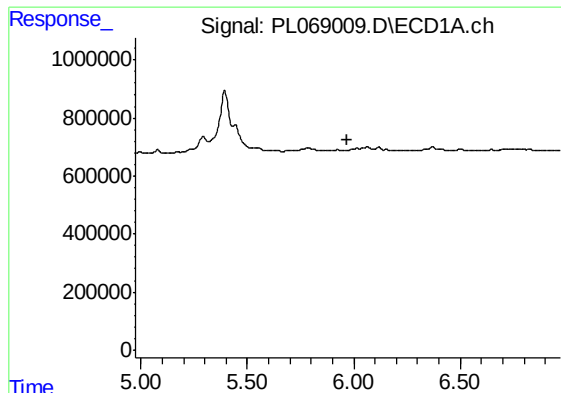

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.971 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SWCS-08-0205

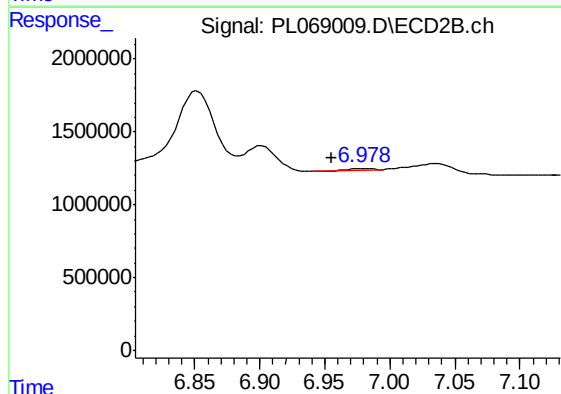


#23 Chlordane-1

R.T.: 6.980 min
Delta R.T.: 0.024 min
Response: 91396
Conc: 2.17 ng/ml

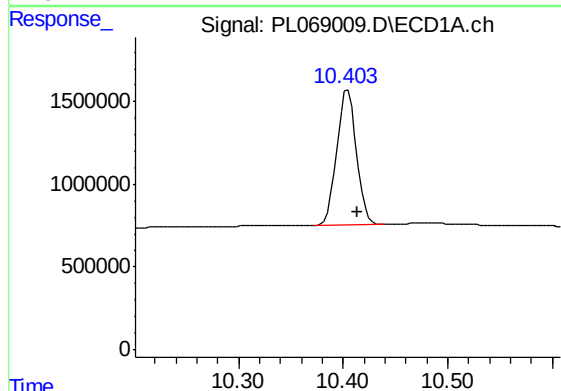

#28 Decachlorobiphenyl

R.T.: 10.404 min
Delta R.T.: -0.009 min
Response: 10807719
Conc: 18.81 ng/ml

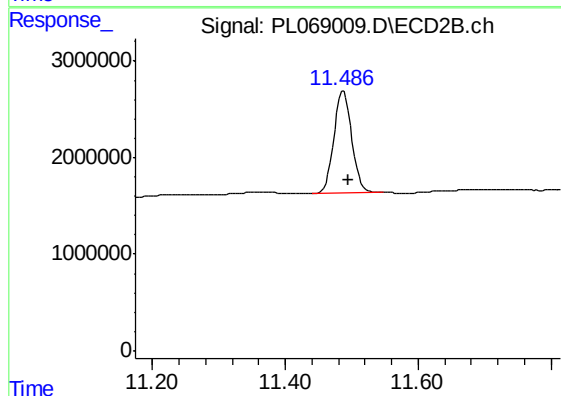

#28 Decachlorobiphenyl

R.T.: 11.488 min
Delta R.T.: -0.007 min
Response: 19979752
Conc: 20.59 ng/ml