

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081521\
 Data File : PL069010.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2021 17:33
 Operator : AR\AJ
 Sample : M3419-19
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SWCS-08-1015

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 23:22:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.635	5.568	8801509	23005195	21.278	22.658
28)	SA Decachlor...	10.404	11.489	10978155	19467042	19.103	20.064
Target Compounds							
8)	B Heptachlo...	0.000	8.058f	0	236493	N.D.	0.205 #
9)	A Endosulfan I	0.000	8.461f	0	850489	N.D.	0.806 #
13)	MA Dieldrin	0.000	8.724	0	276409	N.D.	0.255 #
15)	B Endosulfa...	0.000	9.215	0	637806	N.D.	0.695 #
22)	Mirex	0.000	10.549	0	67469	N.D.	0.085 #
23)	Chlordane-1	0.000	6.978f	0	70943	N.D.	1.682 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081521\
Data File : PL069010.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2021 17:33
Operator : AR\AJ
Sample : M3419-19
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SWCS-08-1015

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 23:22:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

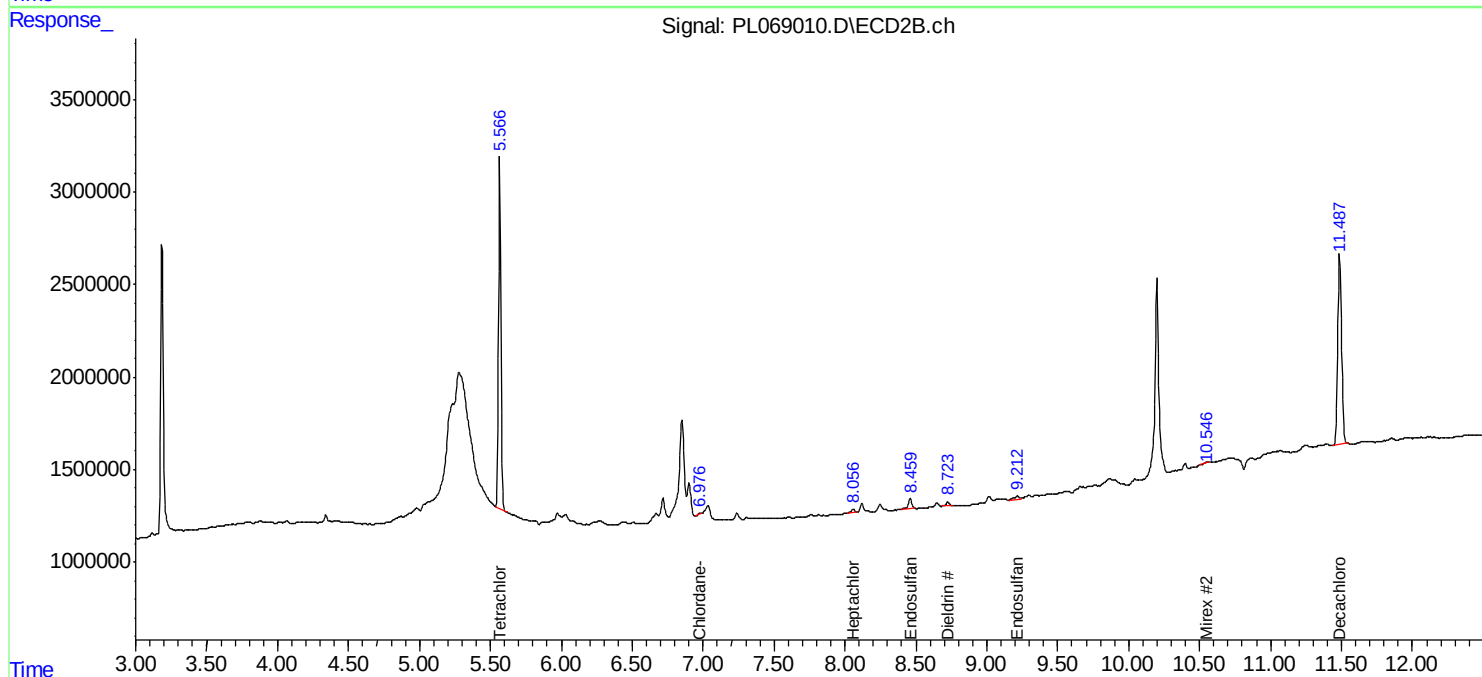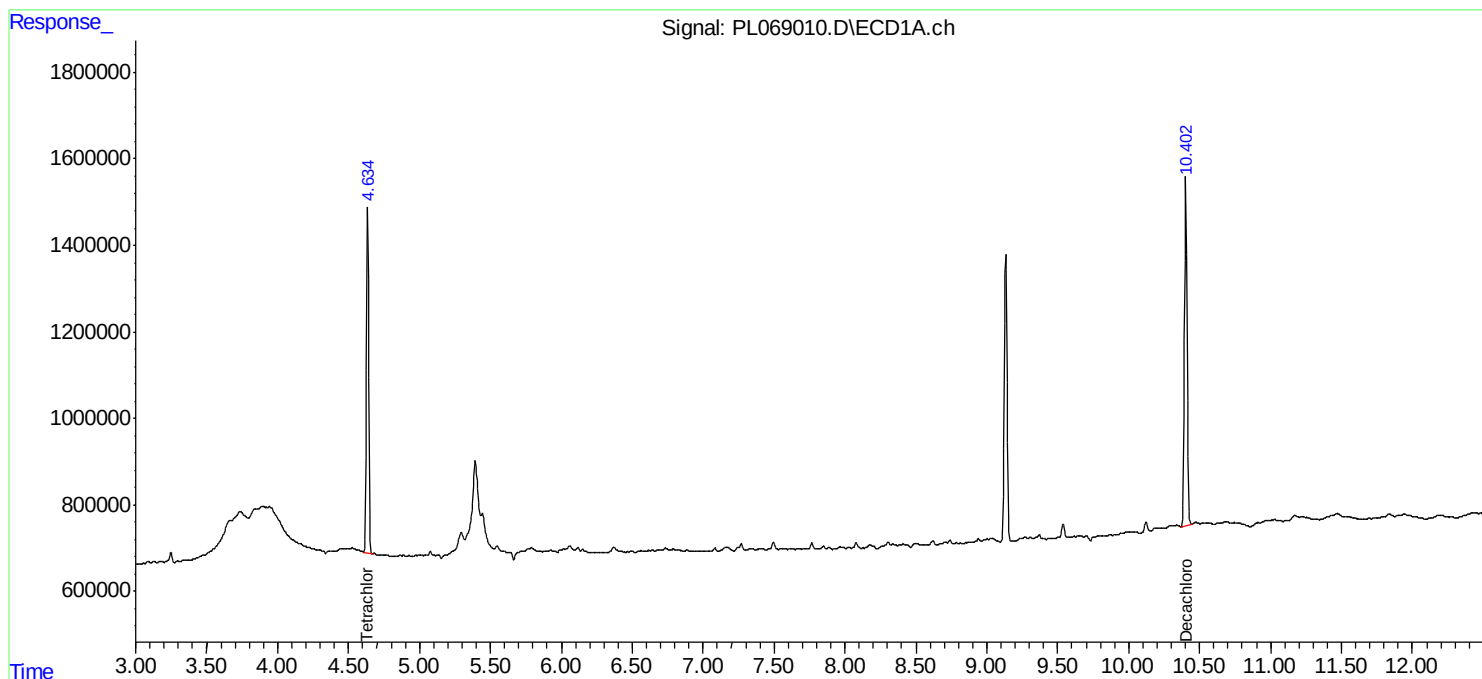


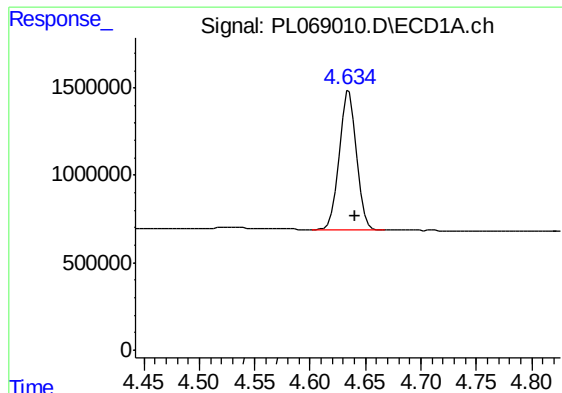

#1 Tetrachloro-m-xylene


R.T.: 4.635 min
Delta R.T.: -0.005 min
Response: 8801509
Conc: 21.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
SWCS-08-1015

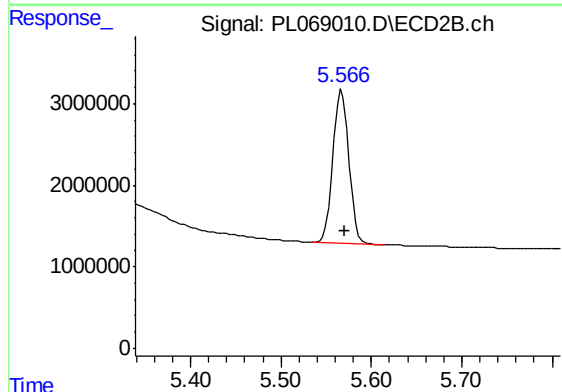


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 23005195
Conc: 22.66 ng/ml

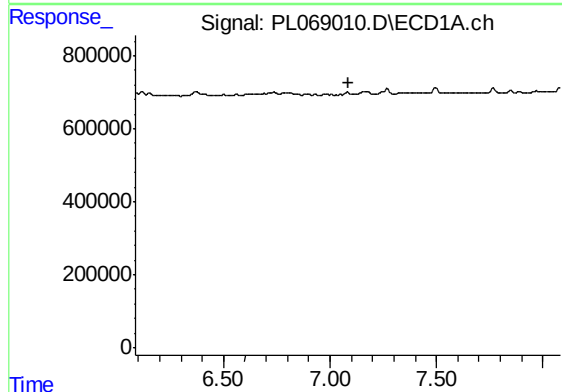


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.084 min
Response: 0
Conc: N.D.

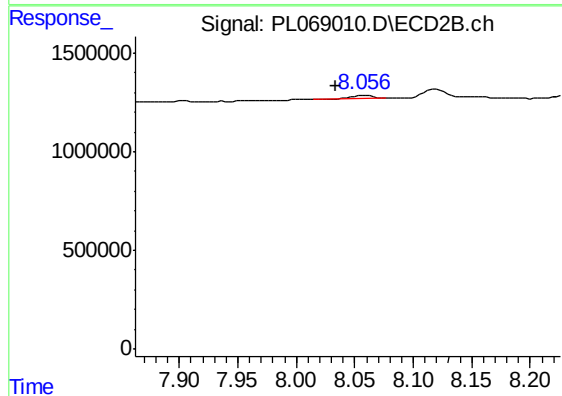

#8 Heptachlor epoxide


R.T.: 8.058 min
Delta R.T.: 0.024 min
Response: 236493
Conc: 0.20 ng/ml

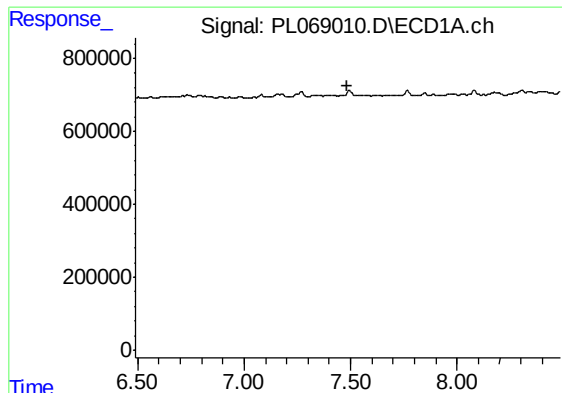

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 7.487 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SWCS-08-1015

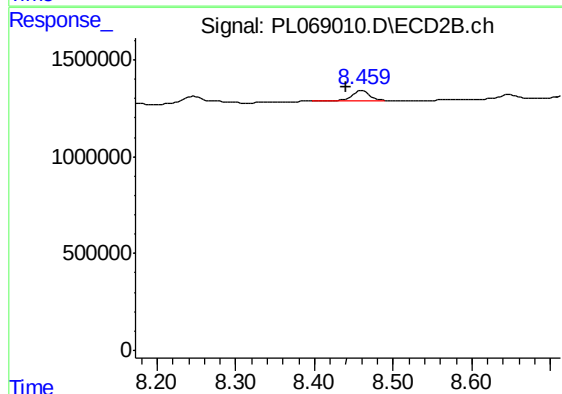


#9 Endosulfan I

R.T.: 8.461 min
Delta R.T.: 0.021 min
Response: 850489
Conc: 0.81 ng/ml

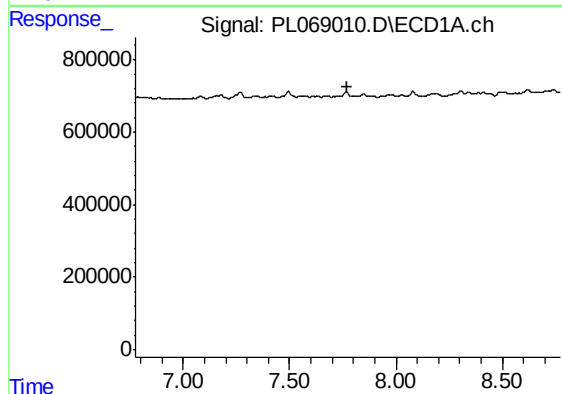


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 7.774 min
Response: 0
Conc: N.D.

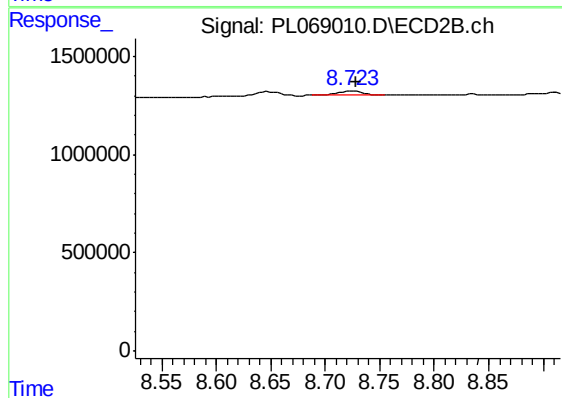

#13 Dieldrin


R.T.: 8.724 min
Delta R.T.: -0.005 min
Response: 276409
Conc: 0.26 ng/ml

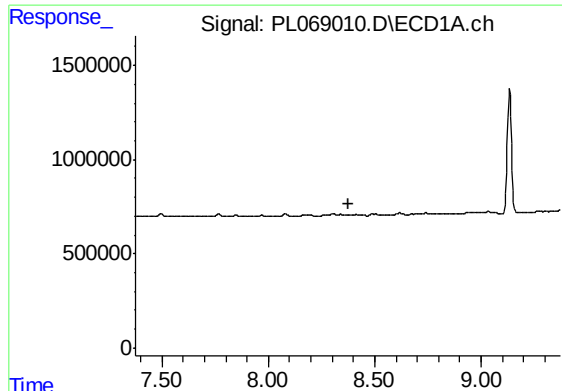

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SWCS-08-1015

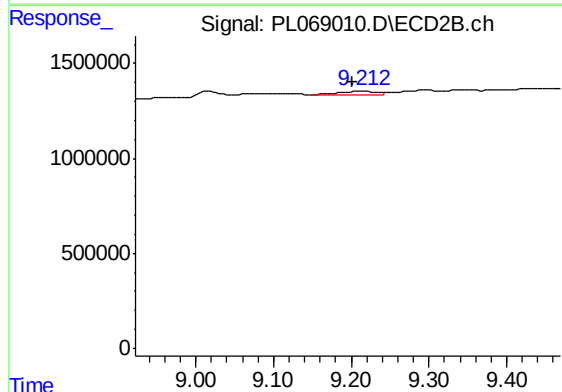


#15 Endosulfan II

R.T.: 9.215 min
Delta R.T.: 0.013 min
Response: 637806
Conc: 0.70 ng/ml

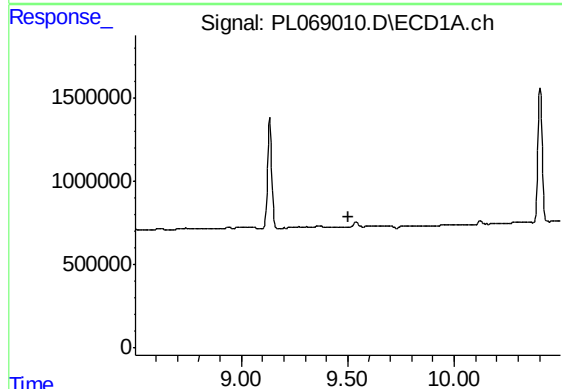


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 9.502 min
Response: 0
Conc: N.D.

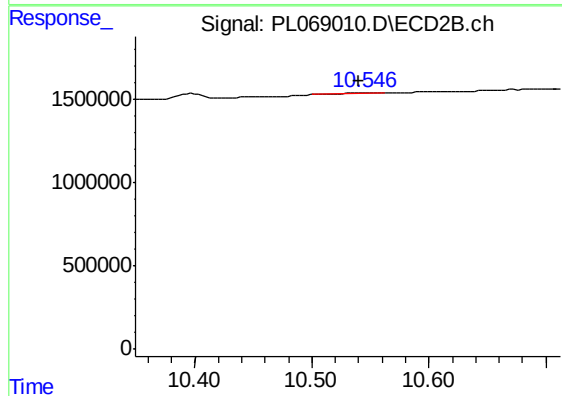

#22 Mirex


R.T.: 10.549 min
Delta R.T.: 0.009 min
Response: 67469
Conc: 0.09 ng/ml

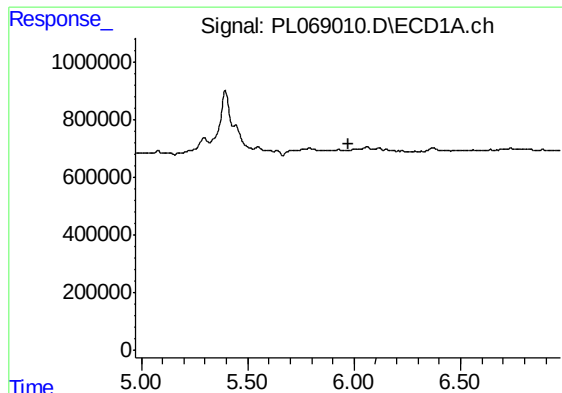

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.971 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SWCS-08-1015

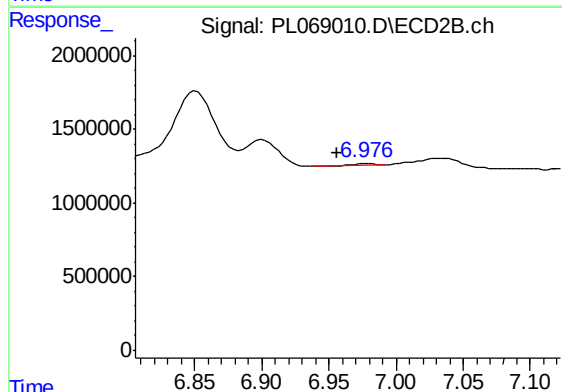


#23 Chlordane-1

R.T.: 6.978 min
Delta R.T.: 0.022 min
Response: 70943
Conc: 1.68 ng/ml

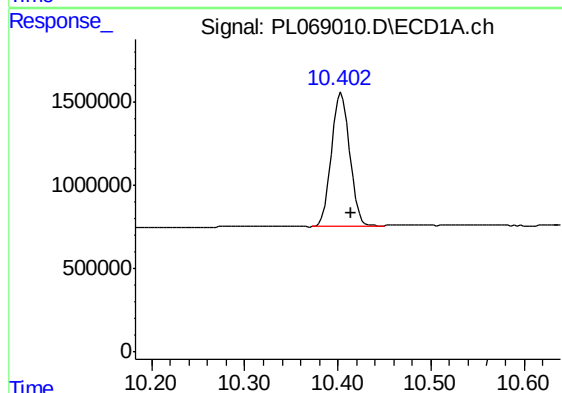

#28 Decachlorobiphenyl

R.T.: 10.404 min
Delta R.T.: -0.010 min
Response: 10978155
Conc: 19.10 ng/ml

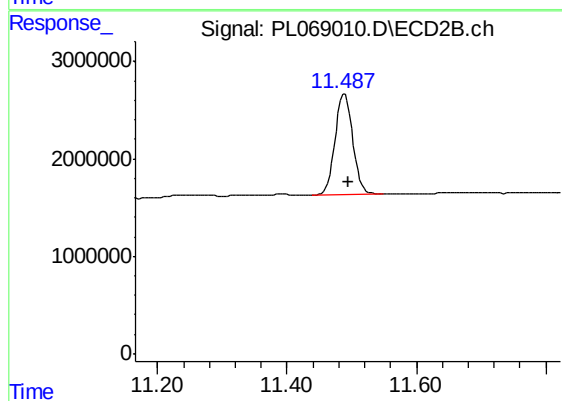

#28 Decachlorobiphenyl

R.T.: 11.489 min
Delta R.T.: -0.006 min
Response: 19467042
Conc: 20.06 ng/ml