

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081521\
 Data File : PL069015.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2021 19:47
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 23:24:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.634	5.568	9163478	24307053	22.153	23.940
28)	SA Decachlor...	10.402	11.488	12722274	21771302	22.137	22.439
Target Compounds							
2)	A alpha-BHC	5.373f	0.000	1201735	0	2.173	N.D. #
4)	MA Heptachlor	6.150f	0.000	483887	0	0.824	N.D. #
6)	B beta-BHC	6.150	0.000	483887	0	1.717	N.D. #
15)	B Endosulfa...	0.000	9.214	0	290605	N.D.	0.317 #
22)	Mirex	0.000	10.568f	0	51002	N.D.	0.064 #
23)	Chlordane-1	0.000	6.970	0	542068	N.D.	12.855 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081521\
Data File : PL069015.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2021 19:47
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 23:24:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

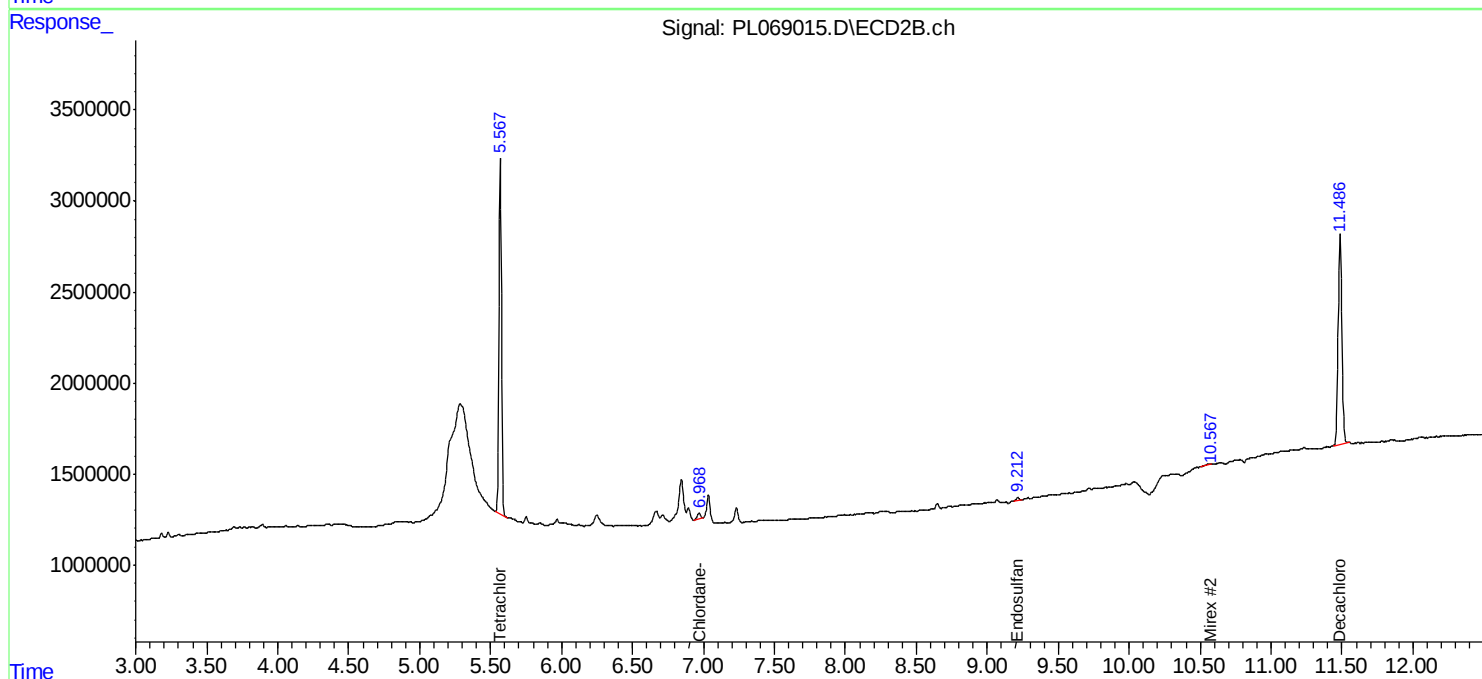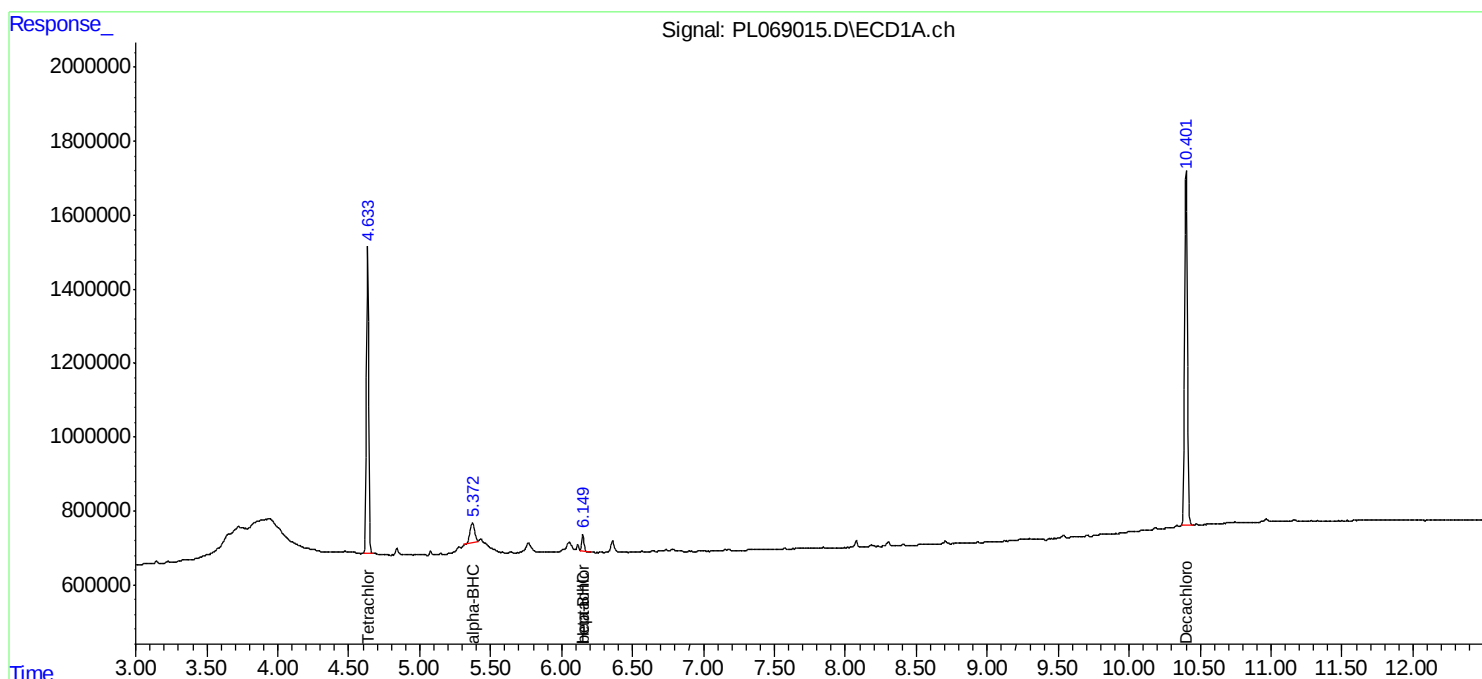


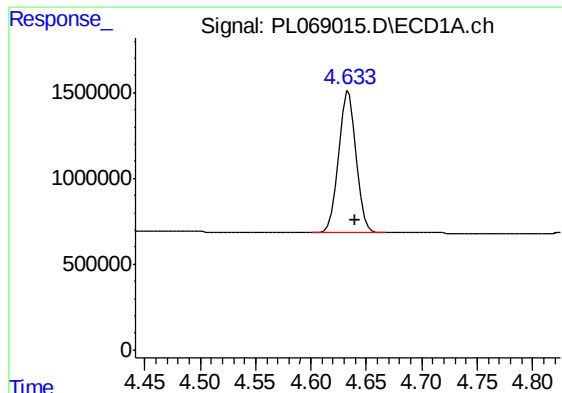

#1 Tetrachloro-m-xylene


R.T.: 4.634 min
Delta R.T.: -0.006 min
Response: 9163478
Conc: 22.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

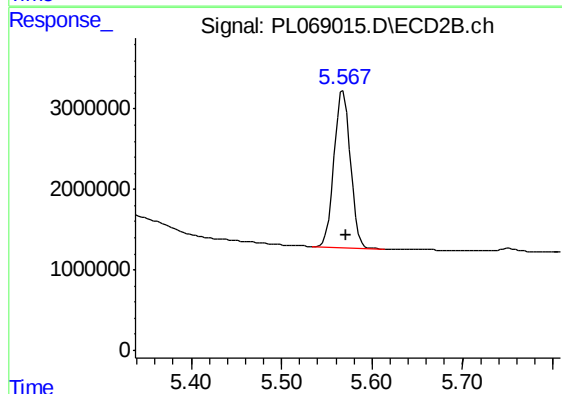


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 24307053
Conc: 23.94 ng/ml

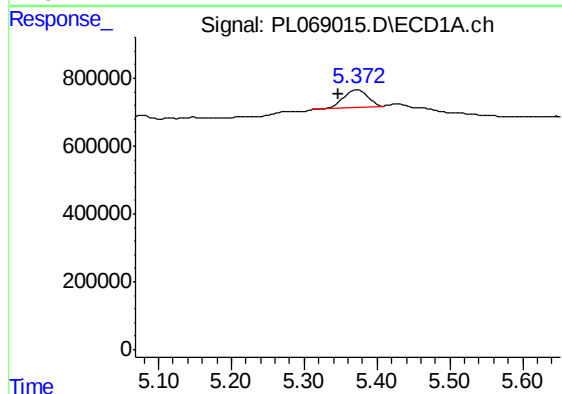


#2 alpha-BHC

R.T.: 5.373 min
Delta R.T.: 0.026 min
Response: 1201735
Conc: 2.17 ng/ml

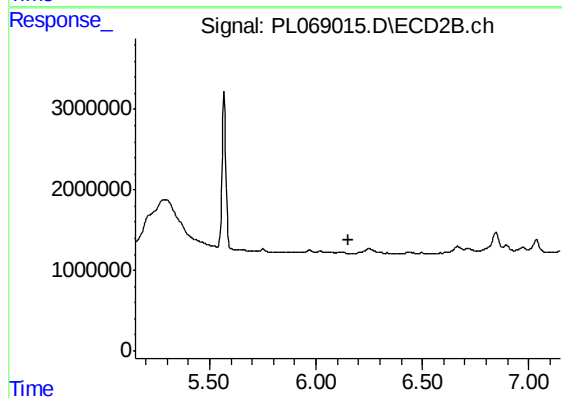

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.151 min
Response: 0
Conc: N.D.

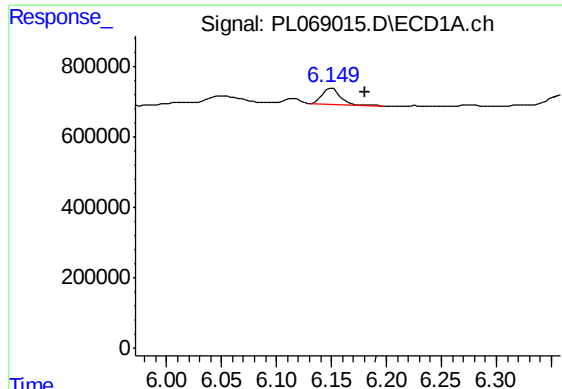

#4 Heptachlor


R.T.: 6.150 min
Delta R.T.: -0.030 min
Response: 483887
Conc: 0.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

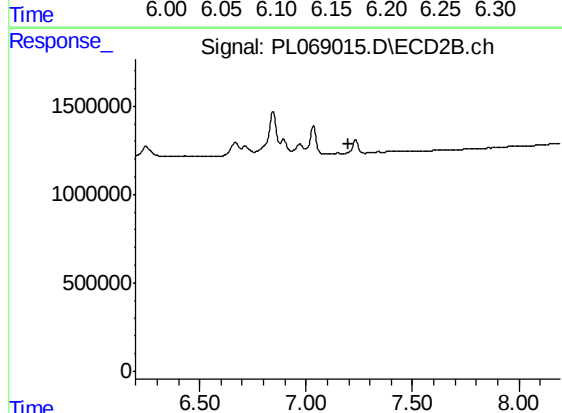


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.197 min
Response: 0
Conc: N.D.

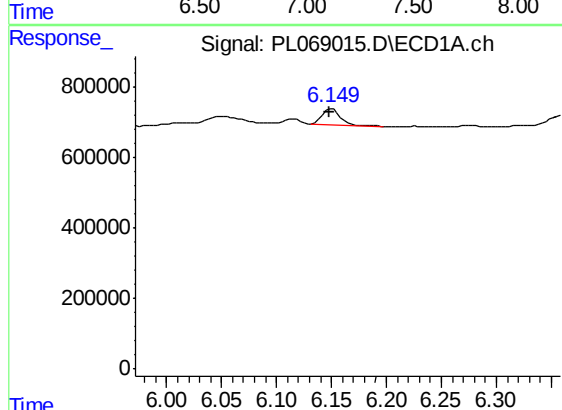


#6 beta-BHC

R.T.: 6.150 min
Delta R.T.: 0.002 min
Response: 483887
Conc: 1.72 ng/ml

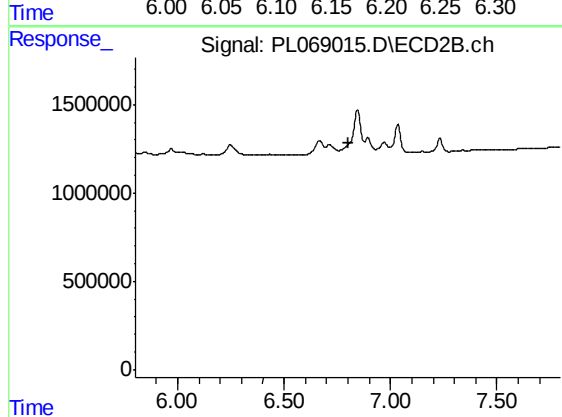

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.800 min
Response: 0
Conc: N.D.

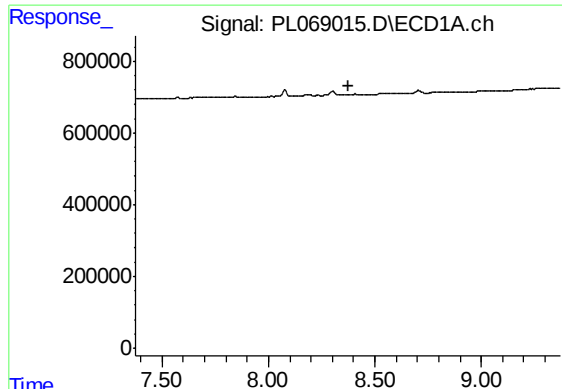

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

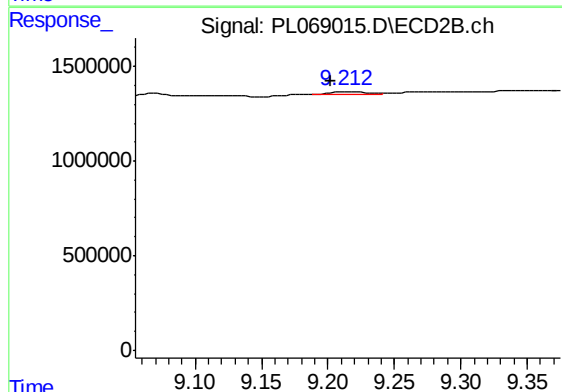


#15 Endosulfan II

R.T.: 9.214 min
Delta R.T.: 0.012 min
Response: 290605
Conc: 0.32 ng/ml

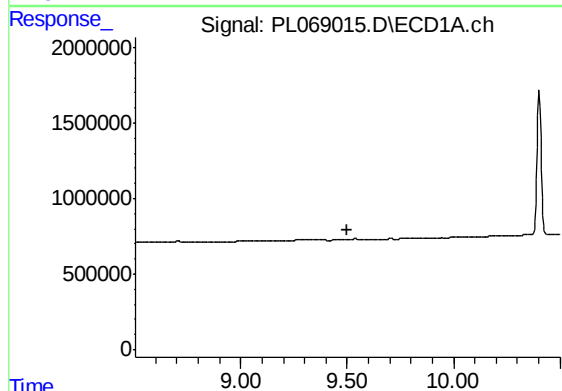


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 9.502 min
Response: 0
Conc: N.D.

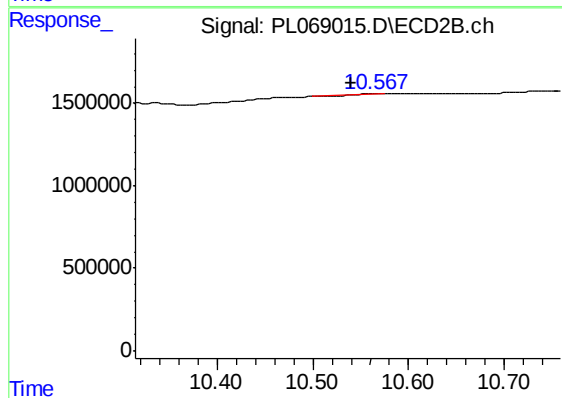

#22 Mirex


R.T.: 10.568 min
Delta R.T.: 0.028 min
Response: 51002
Conc: 0.06 ng/ml

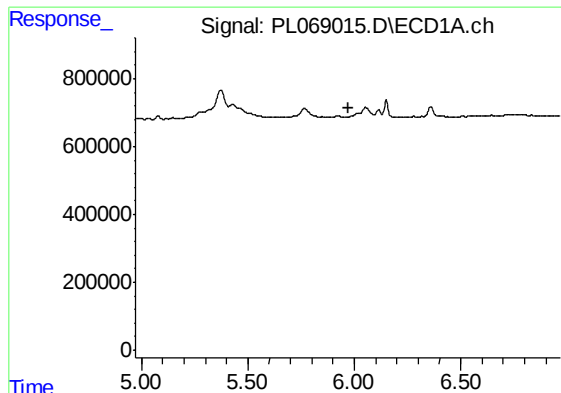

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.971 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

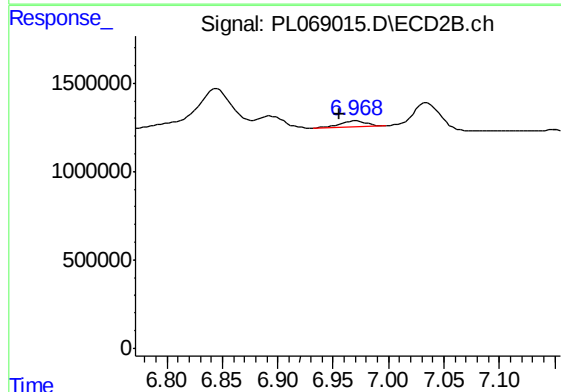


#23 Chlordane-1

R.T.: 6.970 min
Delta R.T.: 0.015 min
Response: 542068
Conc: 12.85 ng/ml

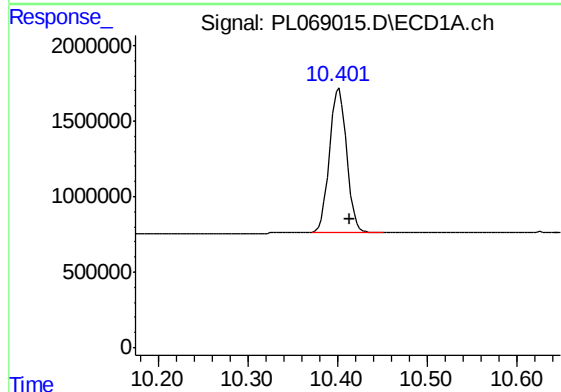

#28 Decachlorobiphenyl

R.T.: 10.402 min
Delta R.T.: -0.012 min
Response: 12722274
Conc: 22.14 ng/ml

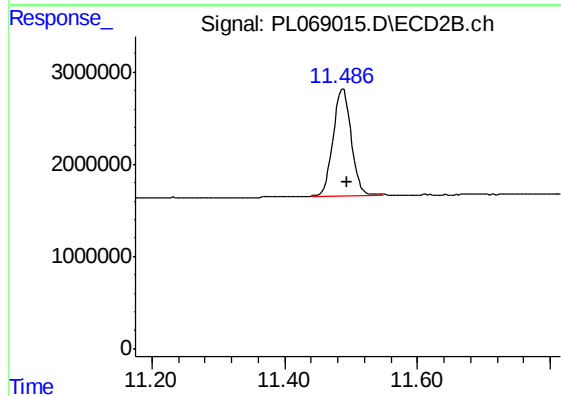

#28 Decachlorobiphenyl

R.T.: 11.488 min
Delta R.T.: -0.007 min
Response: 21771302
Conc: 22.44 ng/ml