

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081521\
 Data File : PL069019.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2021 22:00
 Operator : AR\AJ
 Sample : PB138438TB
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB138438TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 23:25:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.636	5.568	8566664	20771175	20.710	20.457
28)	SA Decachlor...	10.404	11.487	9943889	17915267	17.303	18.465
Target Compounds							
14)	MA Endrin	8.078	8.975	2964819	289807	6.152	0.319 #
22)	Mirex	0.000	10.532	0	1740143	N.D.	2.200 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081521\
Data File : PL069019.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2021 22:00
Operator : AR\AJ
Sample : PB138438TB
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
PB138438TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 23:25:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

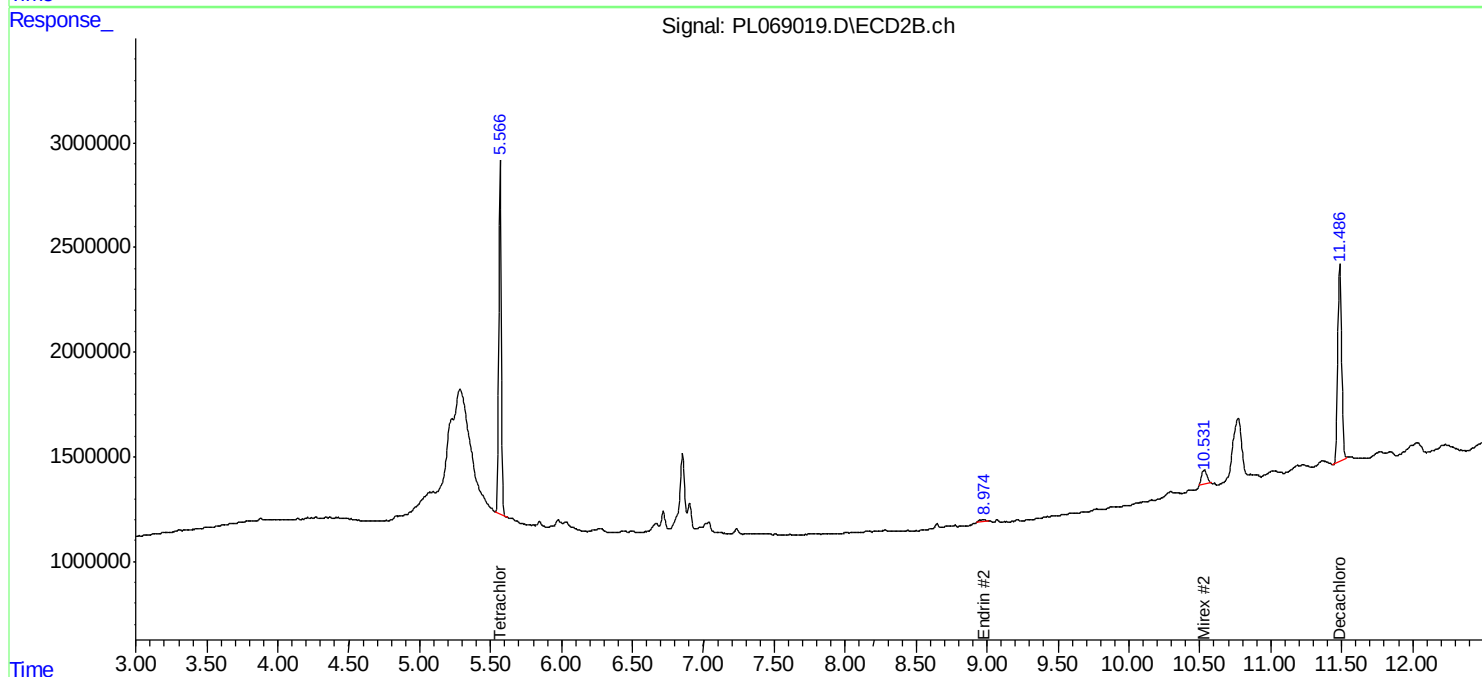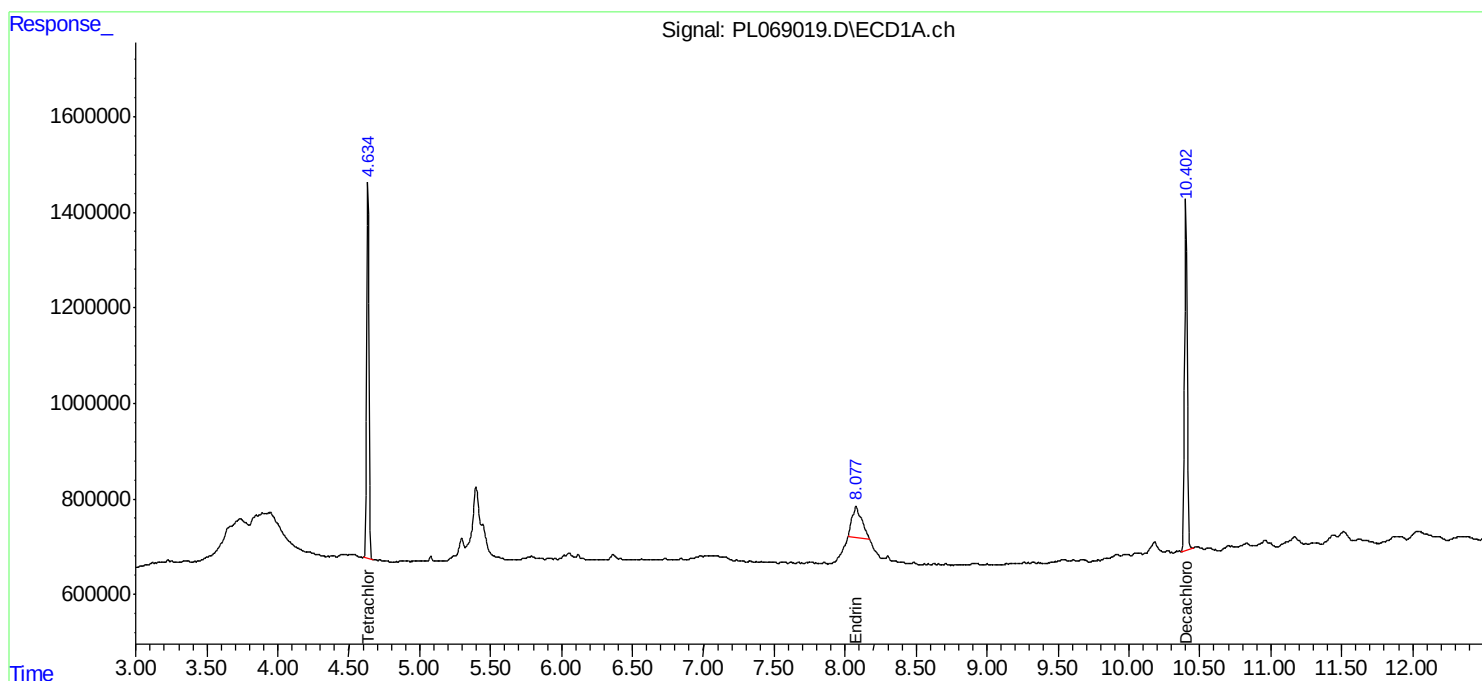


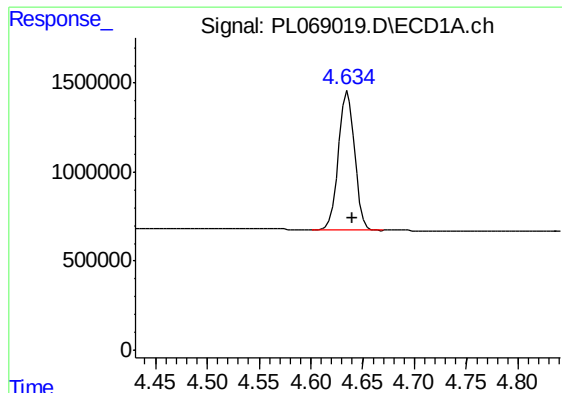

#1 Tetrachloro-m-xylene


R.T.: 4.636 min
Delta R.T.: -0.004 min
Response: 8566664
Conc: 20.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB138438TB

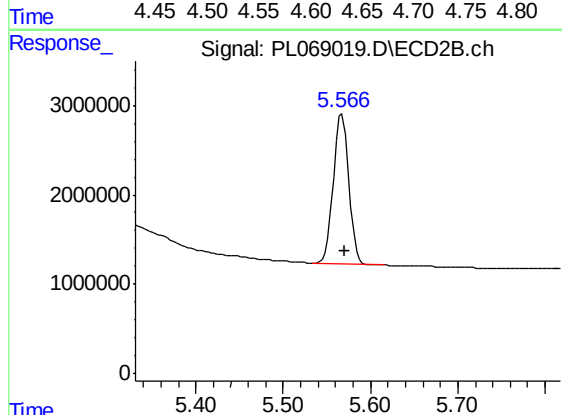


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 20771175
Conc: 20.46 ng/ml

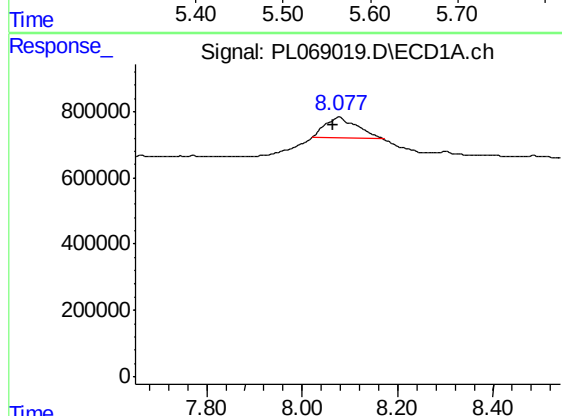


#14 Endrin

R.T.: 8.078 min
Delta R.T.: 0.014 min
Response: 2964819
Conc: 6.15 ng/ml

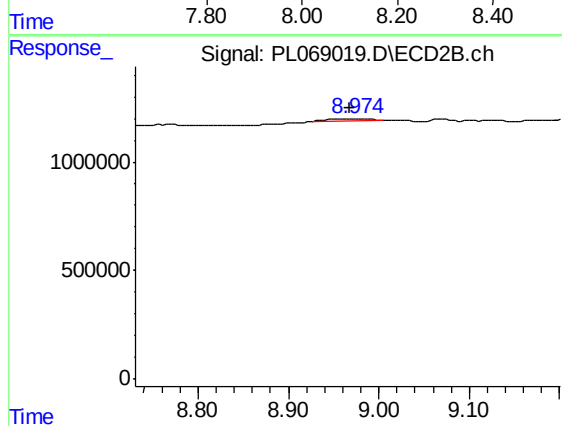

#14 Endrin


R.T.: 8.975 min
Delta R.T.: 0.008 min
Response: 289807
Conc: 0.32 ng/ml

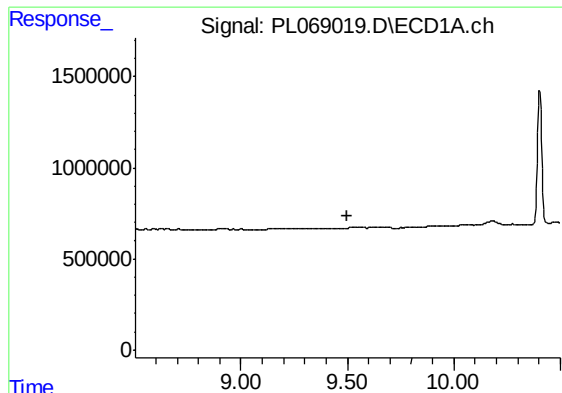

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.502 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138438TB

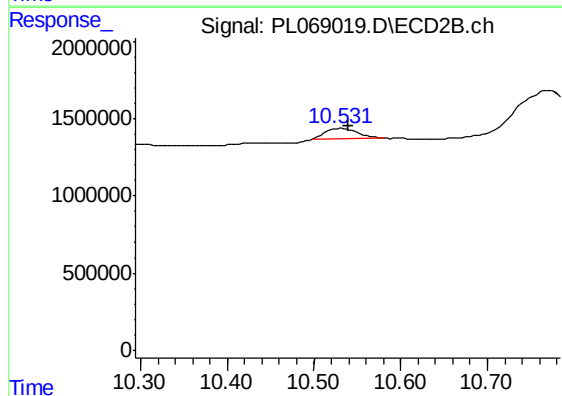


#22 Mirex

R.T.: 10.532 min
Delta R.T.: -0.008 min
Response: 1740143
Conc: 2.20 ng/ml

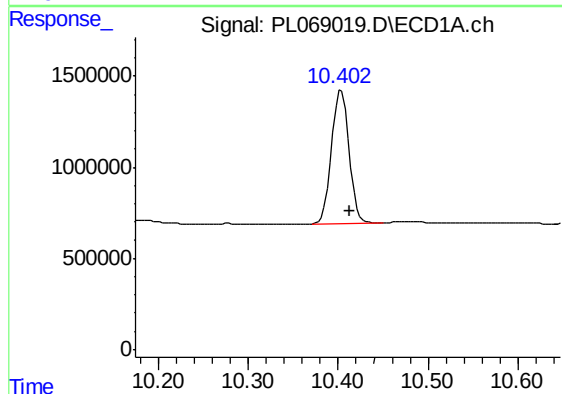

#28 Decachlorobiphenyl

R.T.: 10.404 min
Delta R.T.: -0.010 min
Response: 9943889
Conc: 17.30 ng/ml

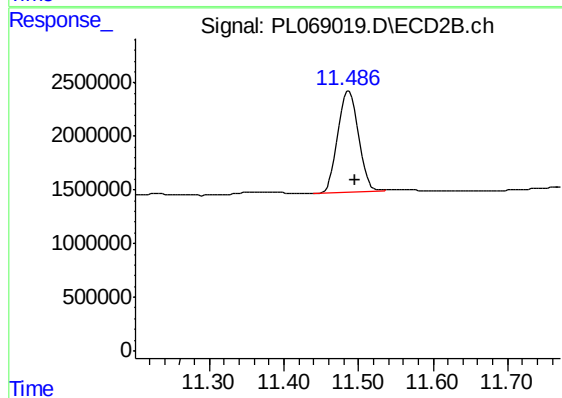

#28 Decachlorobiphenyl

R.T.: 11.487 min
Delta R.T.: -0.007 min
Response: 17915267
Conc: 18.46 ng/ml