

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081521\
 Data File : PL069020.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2021 22:17
 Operator : AR\AJ
 Sample : M3371-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 JET-GROUT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 23:26:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.636	5.567	8375683	21727668	20.249	21.399
28)	SA Decachlor...	10.403	11.488	10495613	19336092	18.263	19.929
Target Compounds							
15)	B Endosulfa...	0.000	9.213	0	487352	N.D.	0.531 #
22)	Mirex	0.000	10.570f	0	171520	N.D.	0.217 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081521\
Data File : PL069020.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2021 22:17
Operator : AR\AJ
Sample : M3371-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
JET-GROUT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 23:26:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

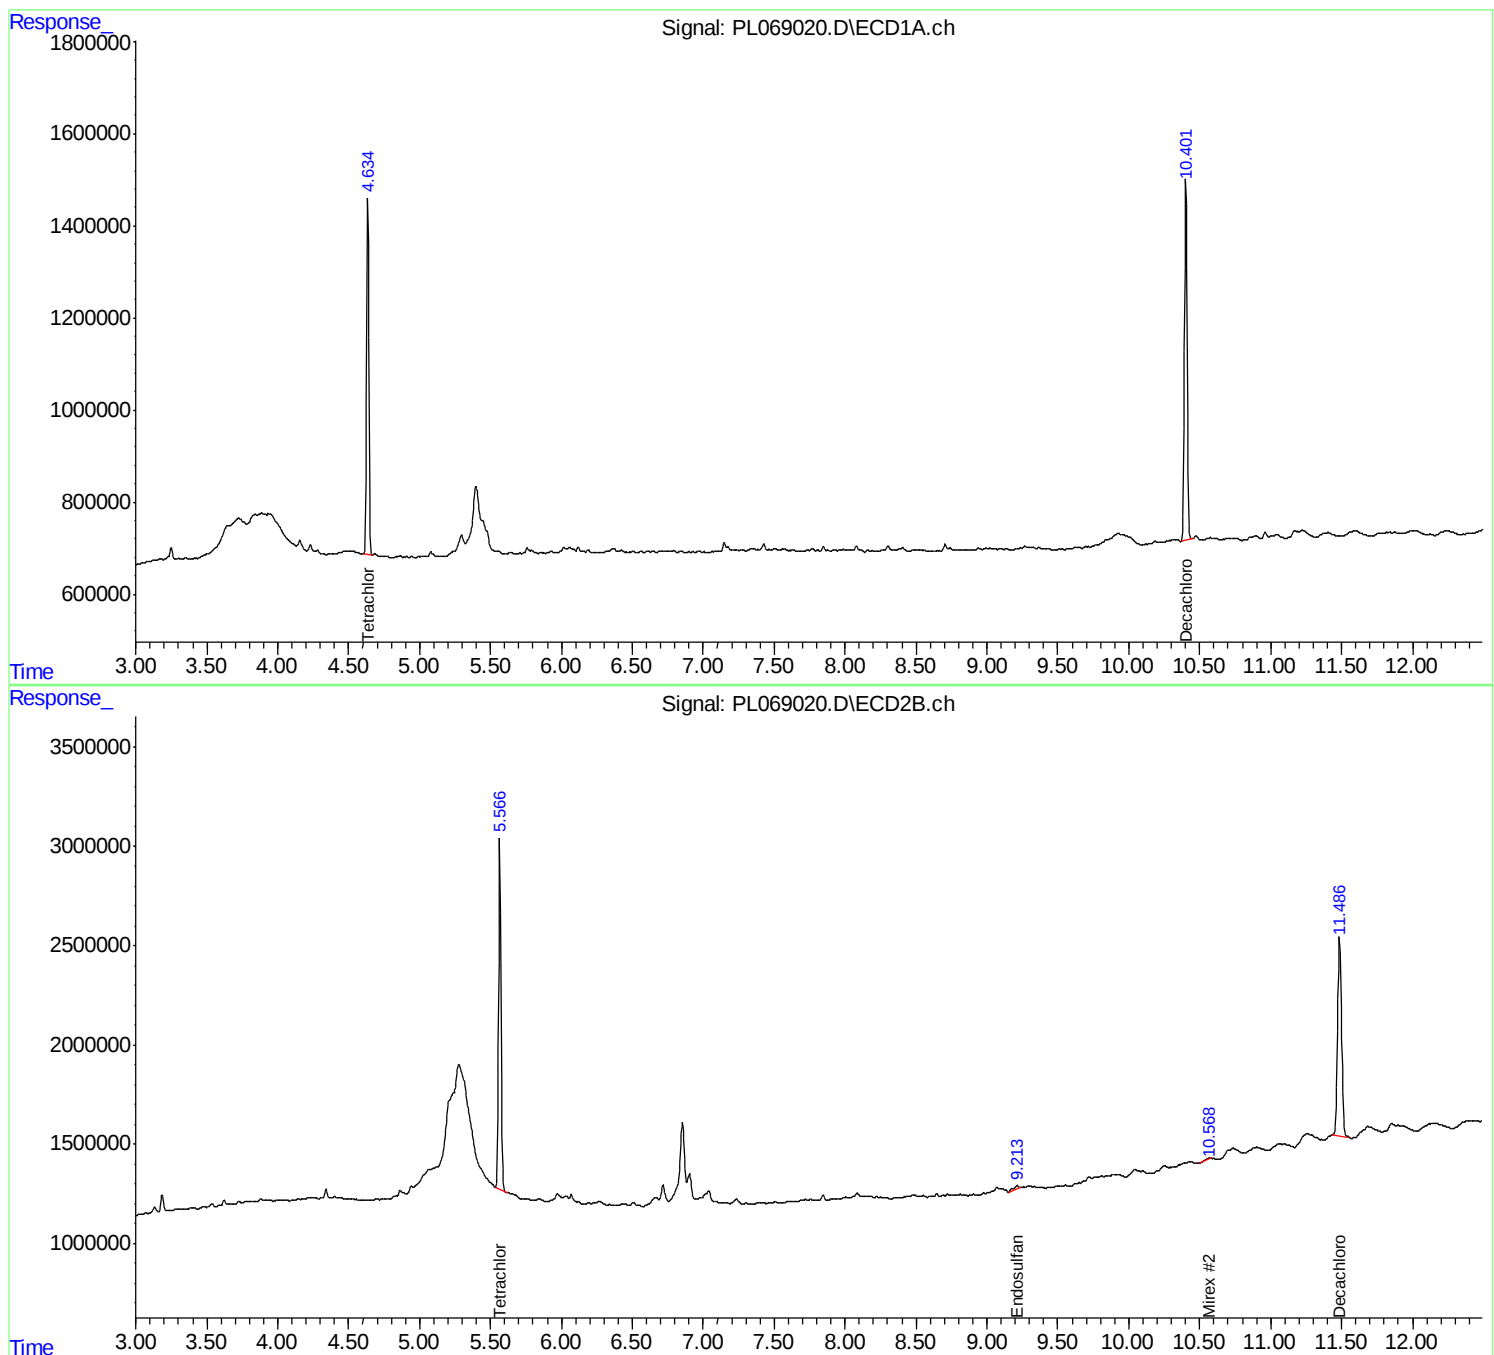


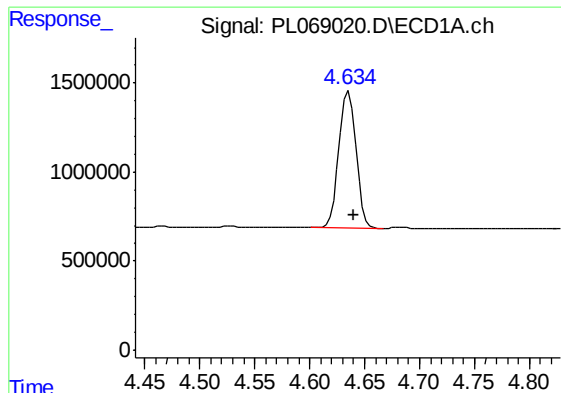

#1 Tetrachloro-m-xylene


R.T.: 4.636 min
Delta R.T.: -0.004 min
Response: 8375683
Conc: 20.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
JET-GROUT

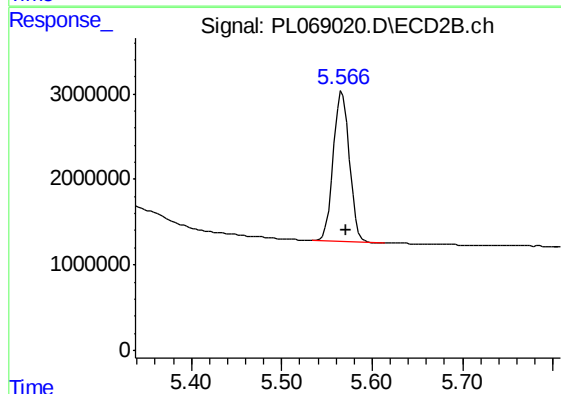


#1 Tetrachloro-m-xylene

R.T.: 5.567 min
Delta R.T.: -0.004 min
Response: 21727668
Conc: 21.40 ng/ml

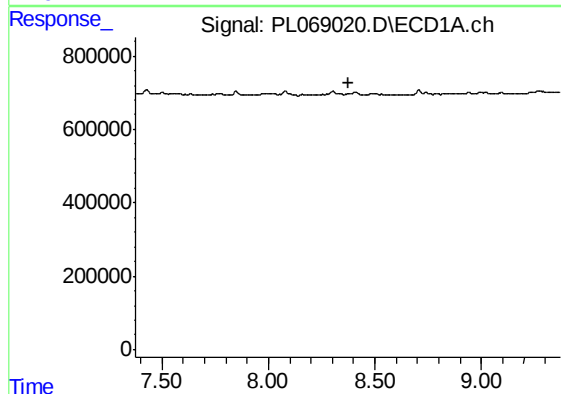


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

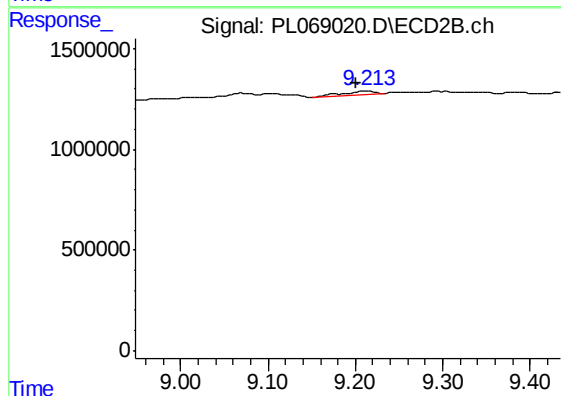

#15 Endosulfan II


R.T.: 9.213 min
Delta R.T.: 0.012 min
Response: 487352
Conc: 0.53 ng/ml

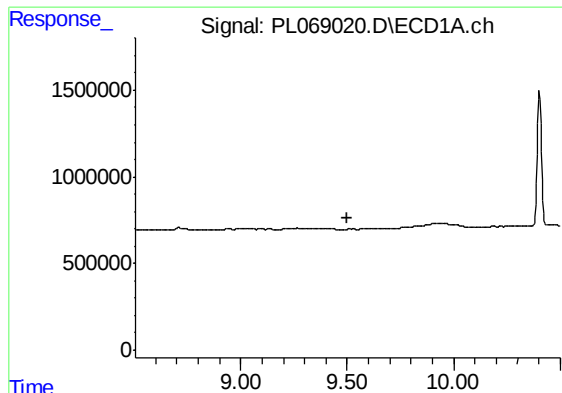

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.502 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
JET-GROUT

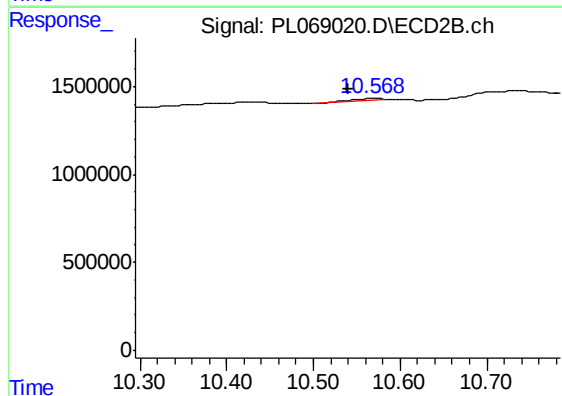


#22 Mirex

R.T.: 10.570 min
Delta R.T.: 0.030 min
Response: 171520
Conc: 0.22 ng/ml

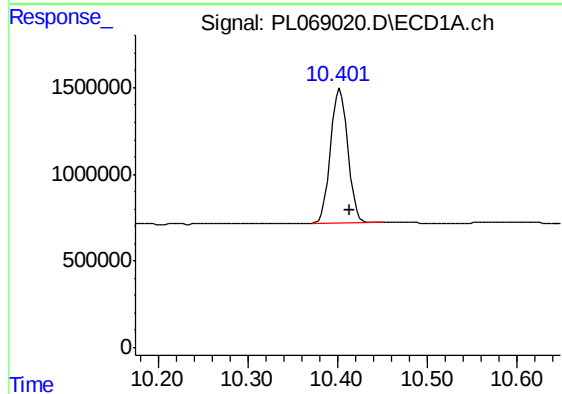

#28 Decachlorobiphenyl

R.T.: 10.403 min
Delta R.T.: -0.011 min
Response: 10495613
Conc: 18.26 ng/ml

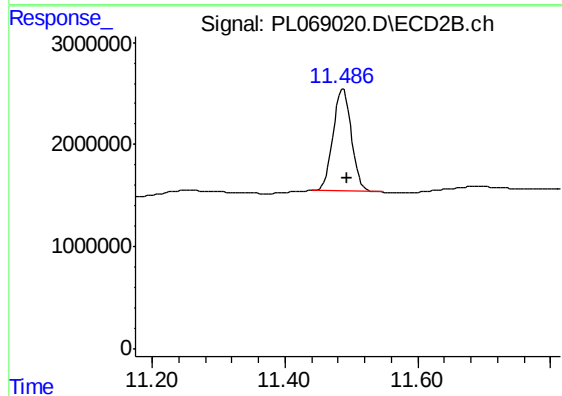

#28 Decachlorobiphenyl

R.T.: 11.488 min
Delta R.T.: -0.007 min
Response: 19336092
Conc: 19.93 ng/ml