

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081521\
 Data File : PL069024.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2021 23:23
 Operator : AR\AJ
 Sample : MM3407-06
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 25S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 23:52:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	4.636	5.568	9019553	24915158	21.805	24.539
28) SA	Decachlor...	10.403	11.487	10873092	19132786	18.920	19.720
Target Compounds							
9) A	Endosulfan I	0.000	8.455f	0	341646	N.D.	0.324 #
15) B	Endosulfa...	0.000	9.213	0	206150	N.D.	0.225 #
20) A	Methoxychlor	0.000	9.898f	0	521245	N.D.	1.002 #
21) B	Endrin ke...	0.000	10.078	0	322909	N.D.	0.317 #
24)	Chlordane-2	6.650	0.000	160123	0	7.627	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081521\
Data File : PL069024.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2021 23:23
Operator : AR\AJ
Sample : MM3407-06
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
25S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 23:52:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

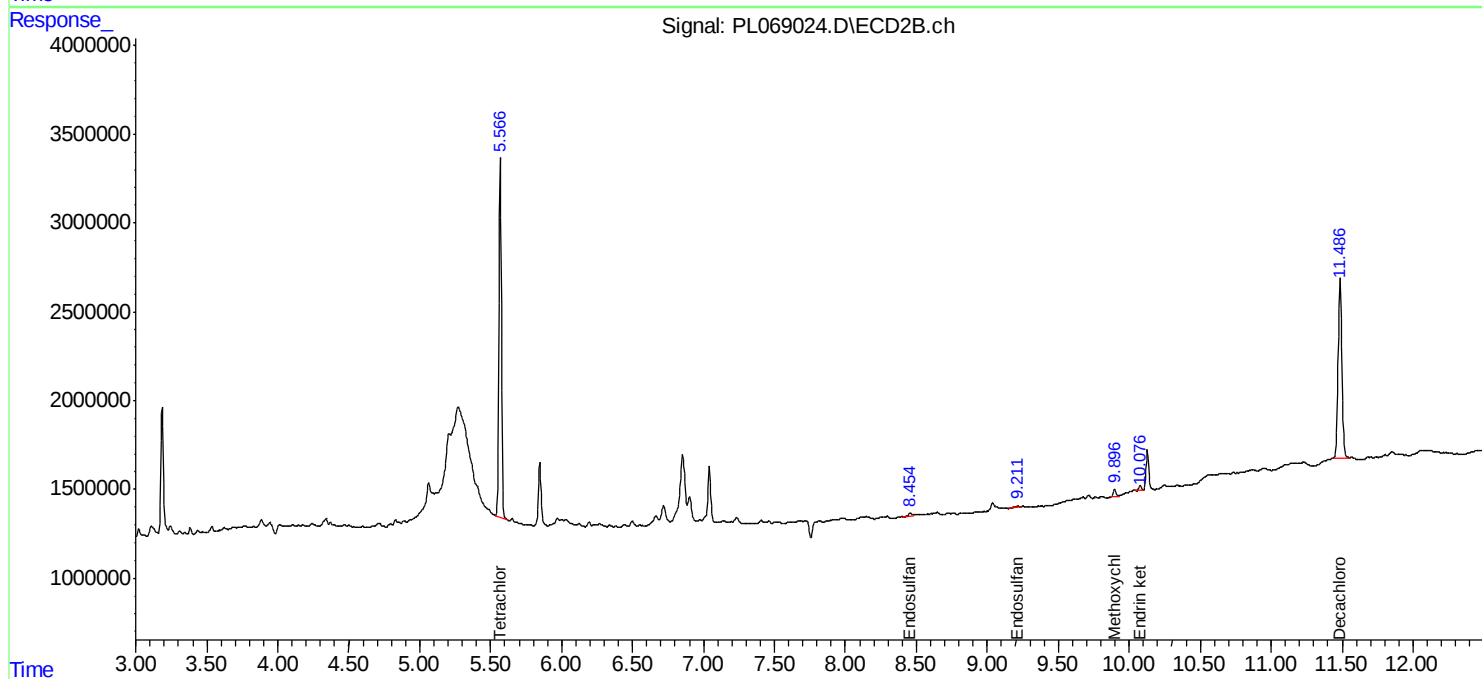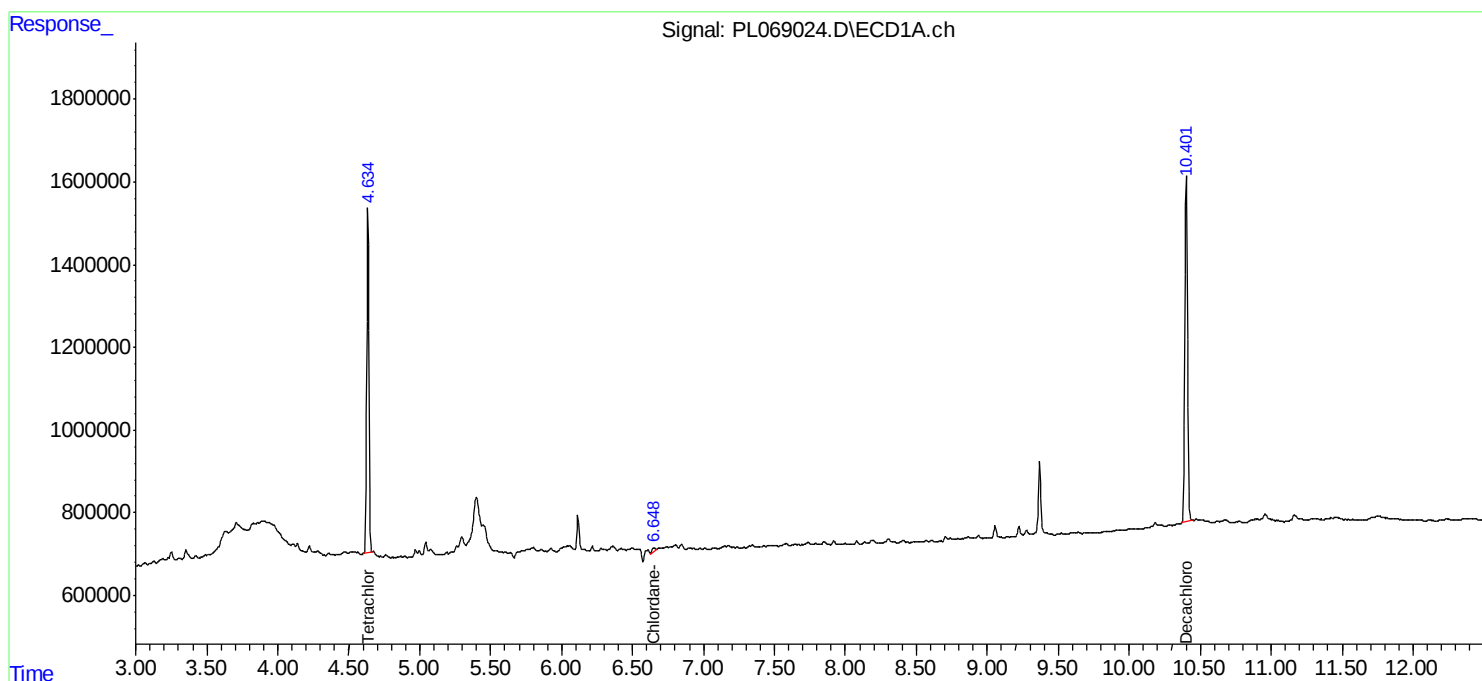


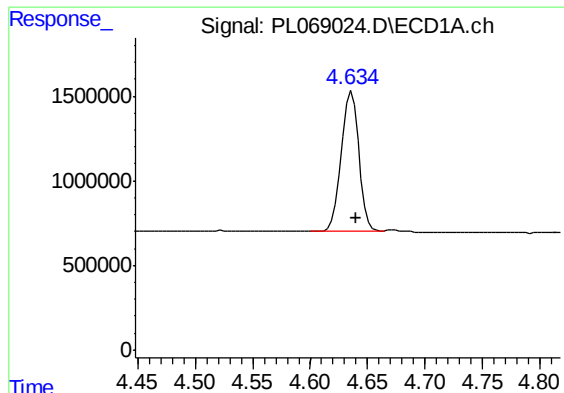

#1 Tetrachloro-m-xylene


R.T.: 4.636 min
Delta R.T.: -0.004 min
Response: 9019553
Conc: 21.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
25S

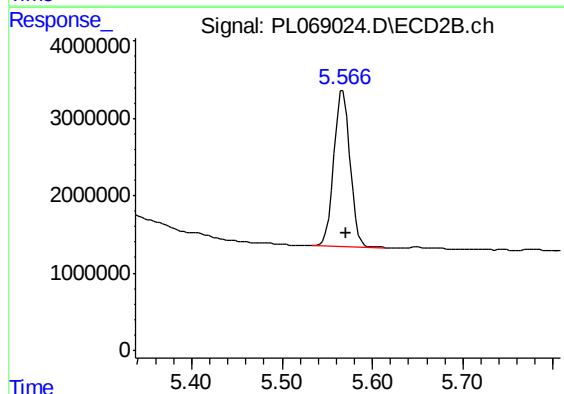


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 24915158
Conc: 24.54 ng/ml

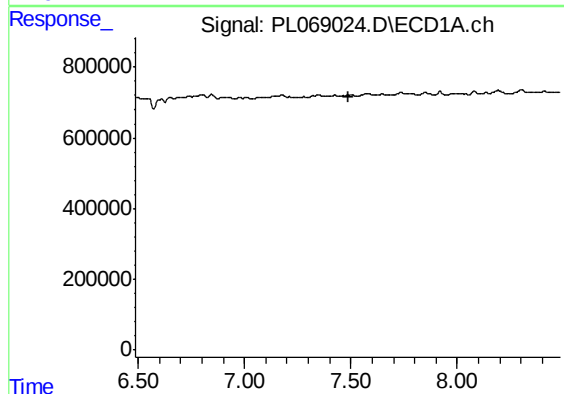


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.487 min
Response: 0
Conc: N.D.

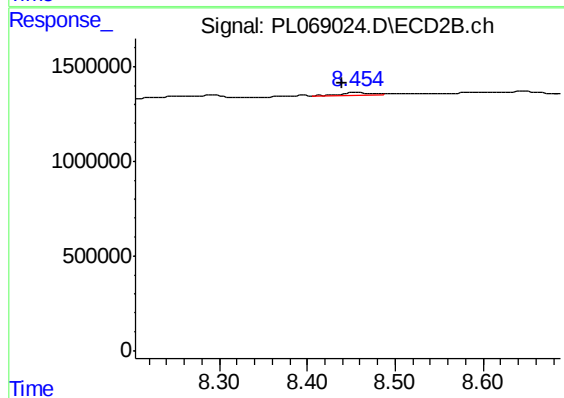

#9 Endosulfan I


R.T.: 8.455 min
Delta R.T.: 0.016 min
Response: 341646
Conc: 0.32 ng/ml

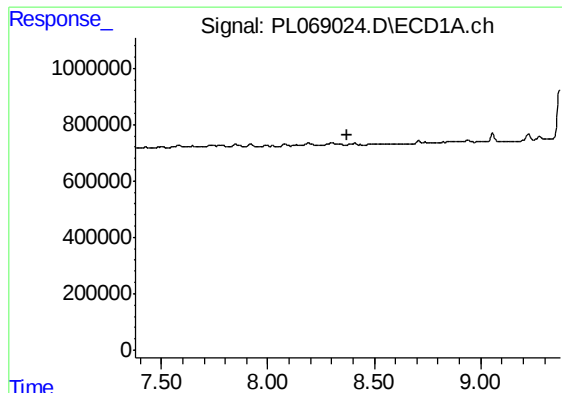

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
25S

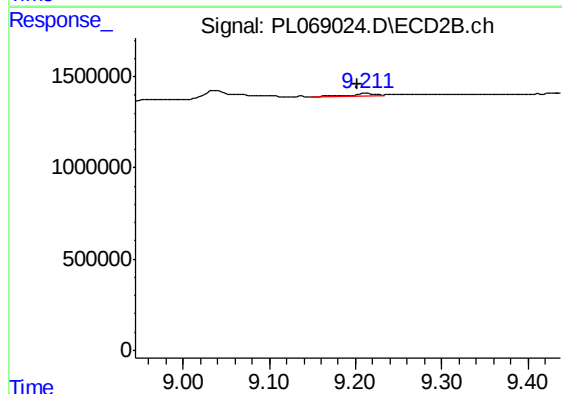


#15 Endosulfan II

R.T.: 9.213 min
Delta R.T.: 0.011 min
Response: 206150
Conc: 0.22 ng/ml

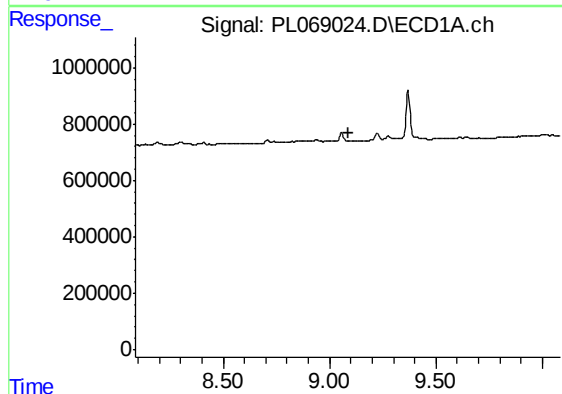


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.087 min
Response: 0
Conc: N.D.

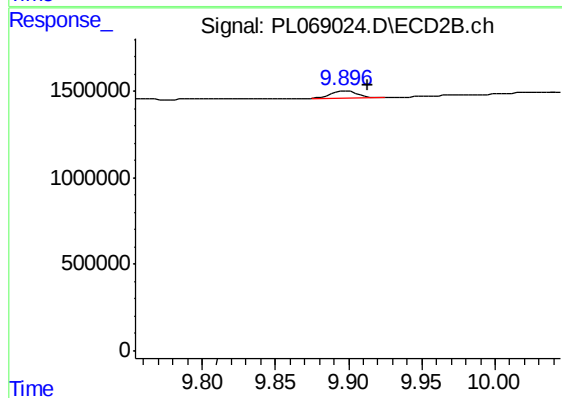

#20 Methoxychlor


R.T.: 9.898 min
Delta R.T.: -0.015 min
Response: 521245
Conc: 1.00 ng/ml

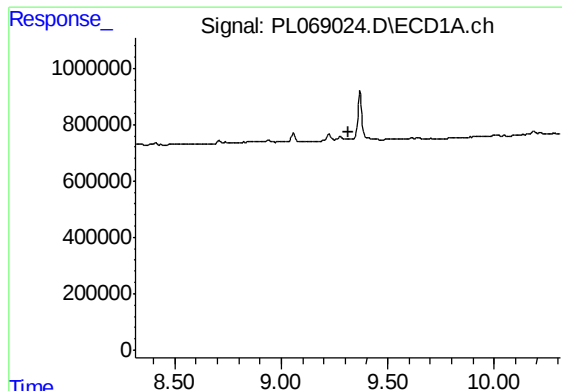

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.313 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
25S

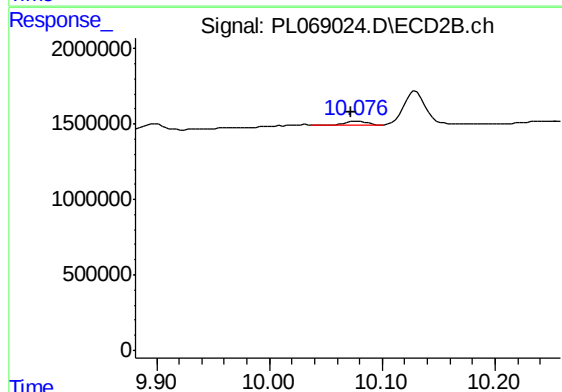


#21 Endrin ketone

R.T.: 10.078 min
Delta R.T.: 0.005 min
Response: 322909
Conc: 0.32 ng/ml

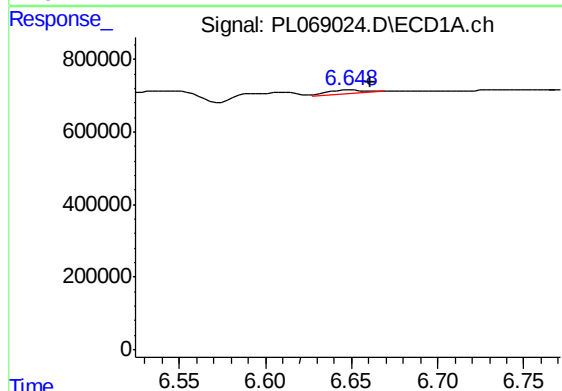


#24 Chlordane-2

R.T.: 6.650 min
Delta R.T.: -0.011 min
Response: 160123
Conc: 7.63 ng/ml

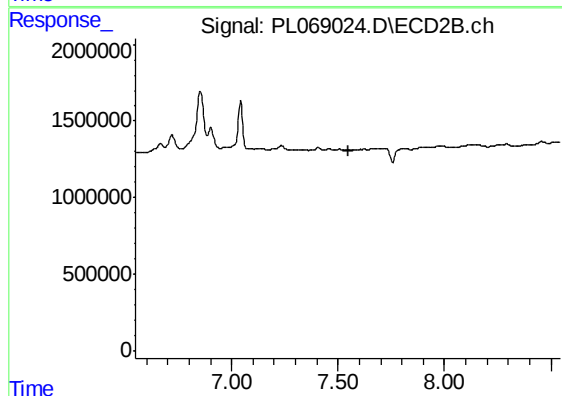

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 7.548 min
Response: 0
Conc: N.D.

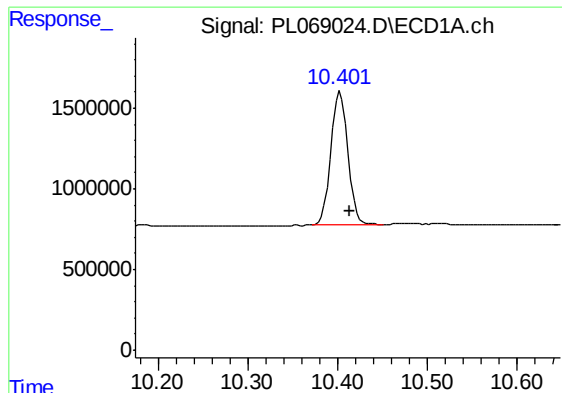

#28 Decachlorobiphenyl

R.T.: 10.403 min
Delta R.T.: -0.011 min
Response: 10873092
Conc: 18.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
25S

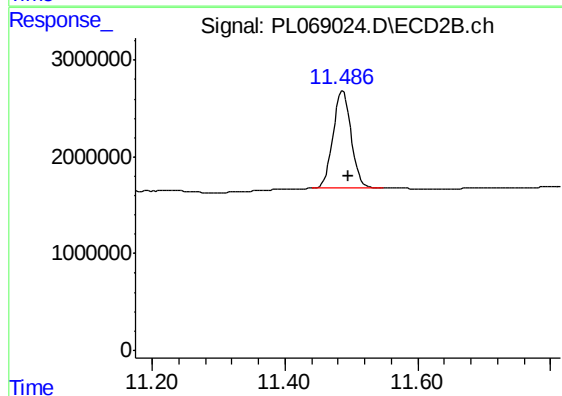

#28 Decachlorobiphenyl

R.T.: 11.487 min
Delta R.T.: -0.008 min
Response: 19132786
Conc: 19.72 ng/ml